

FIG. 1

S100

positioning the  
mouthguard into a desired  
position

S200

administering an  
electricity-based therapy to  
the target region

S300

isolating the electrically  
conductive material from  
the electricity-based  
therapy

FIG. 2

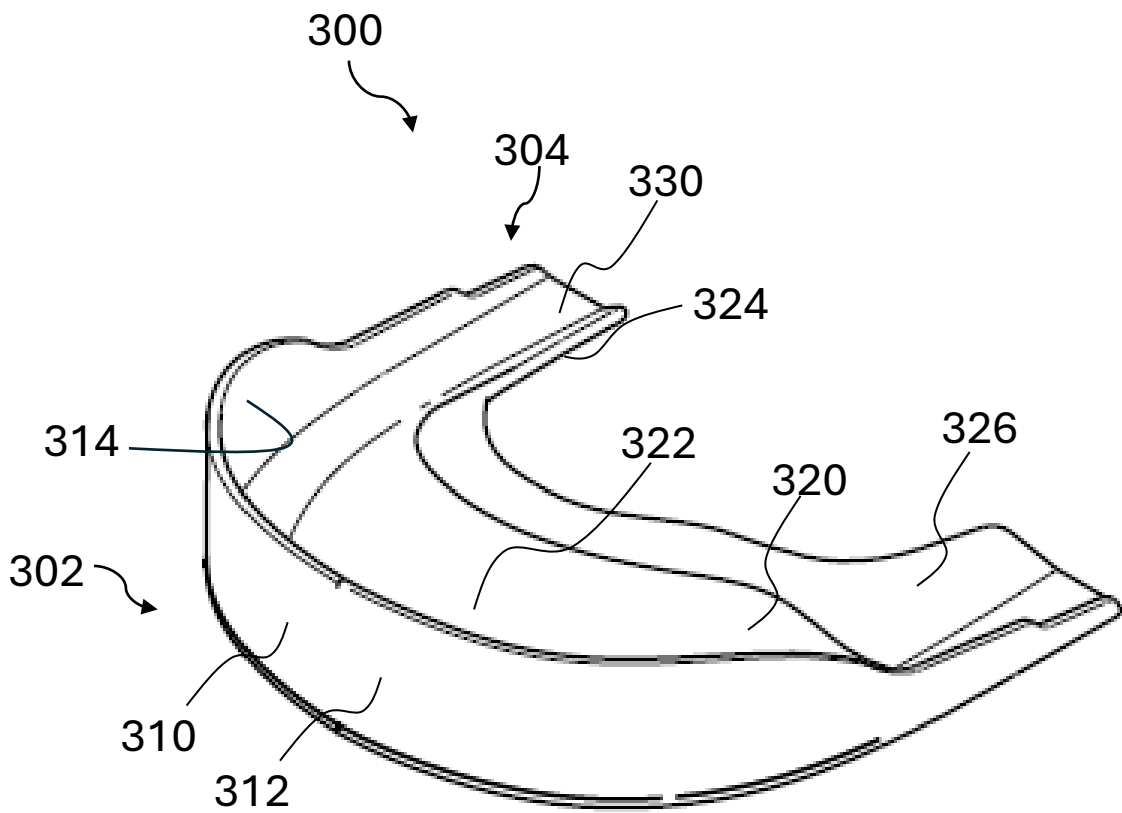


FIG. 3

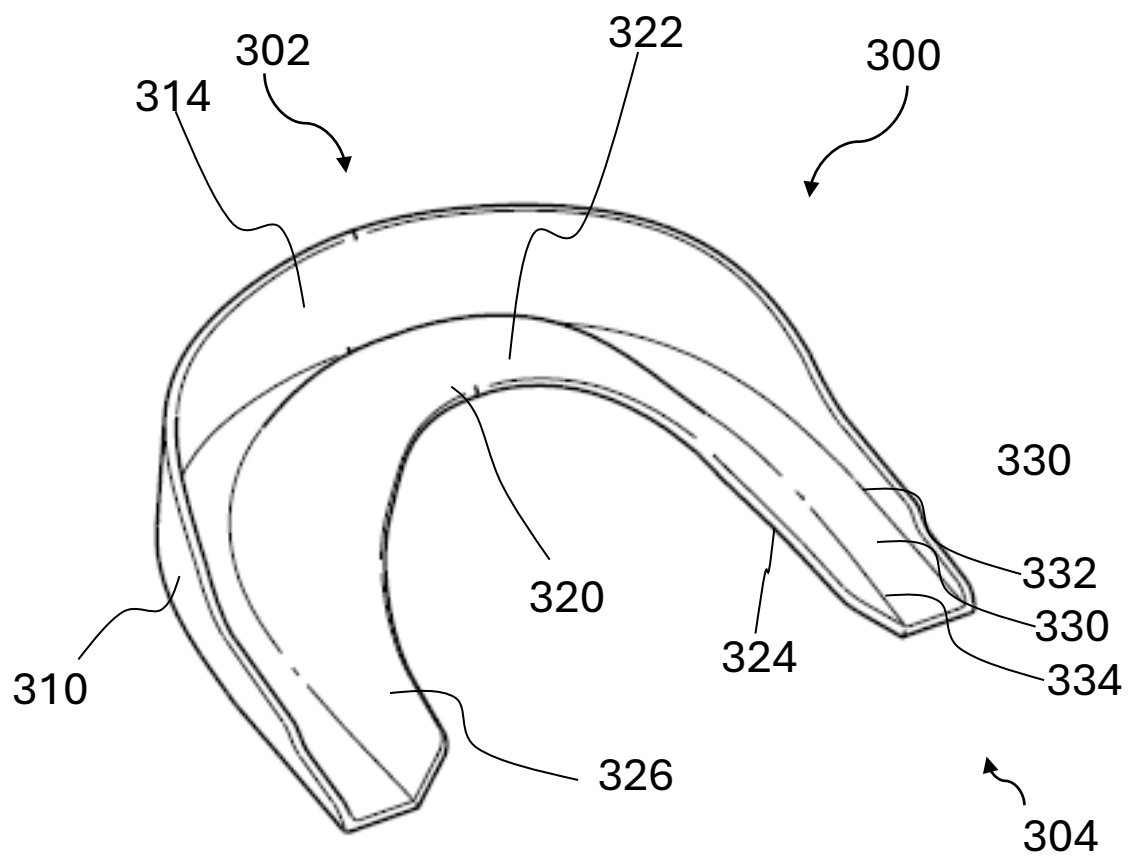


FIG. 4

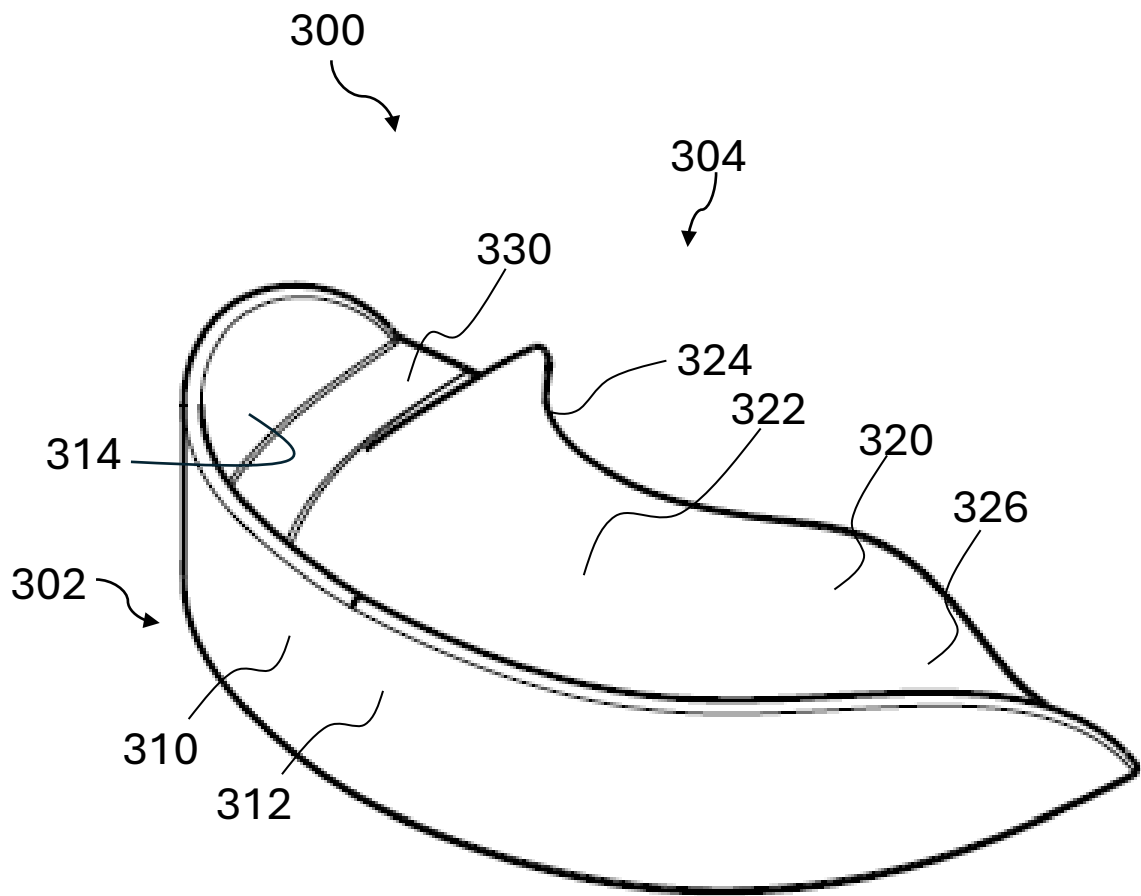


FIG. 5