



Frozen full HGB models: external transport is weak and uncertain

Patients with false alerts (444 negatives)

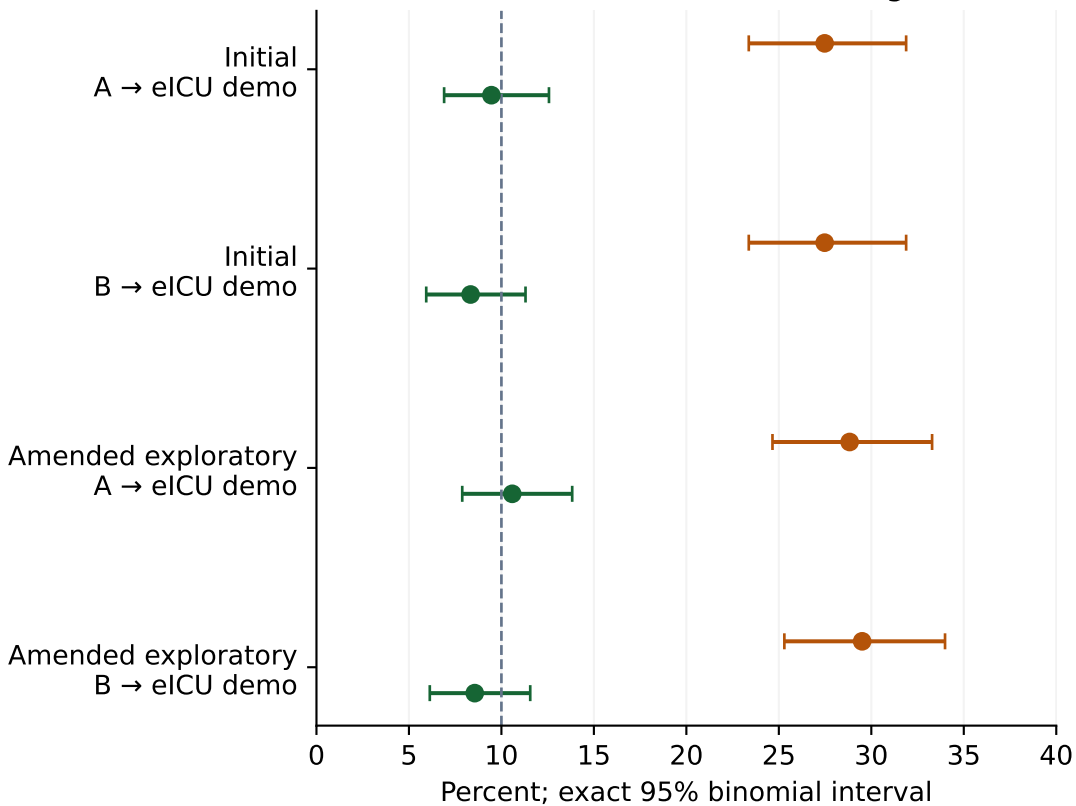

Any alert in 6 h before event (17 cases)

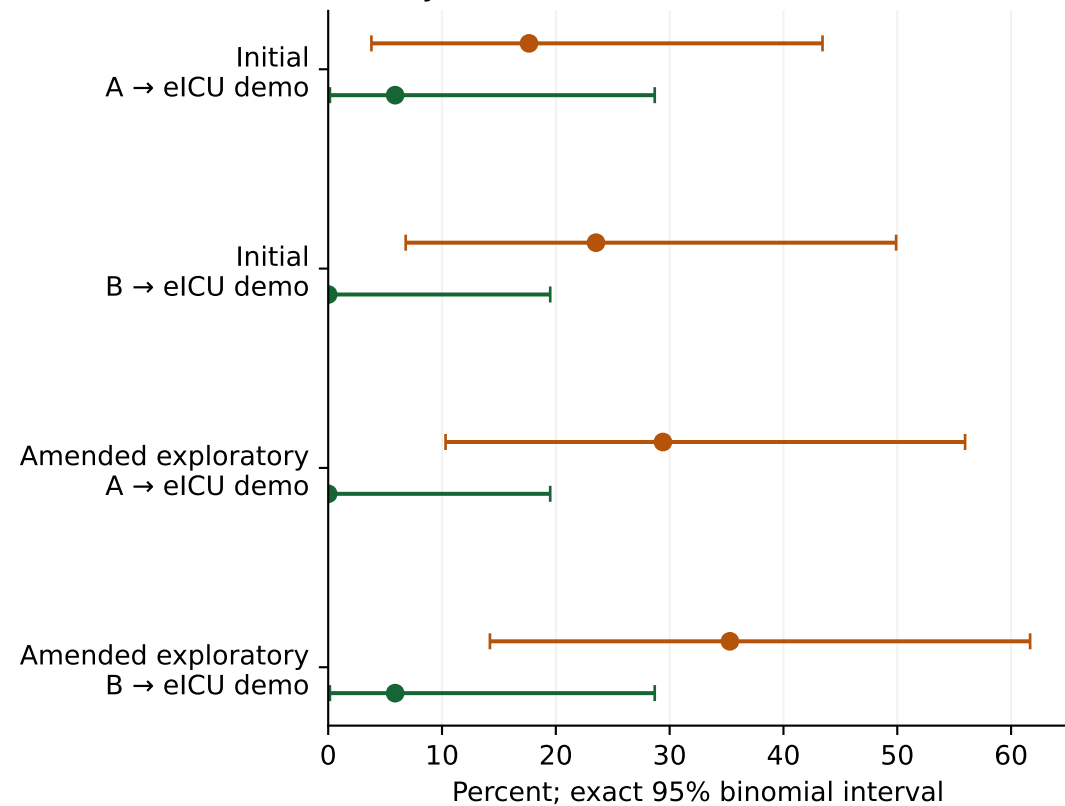

● Frozen source patient threshold
 ● External calibration threshold