


A Detection floor of the 3-IV wide-APOE-excluded scan



B Empirical-null calibration (wide panel)

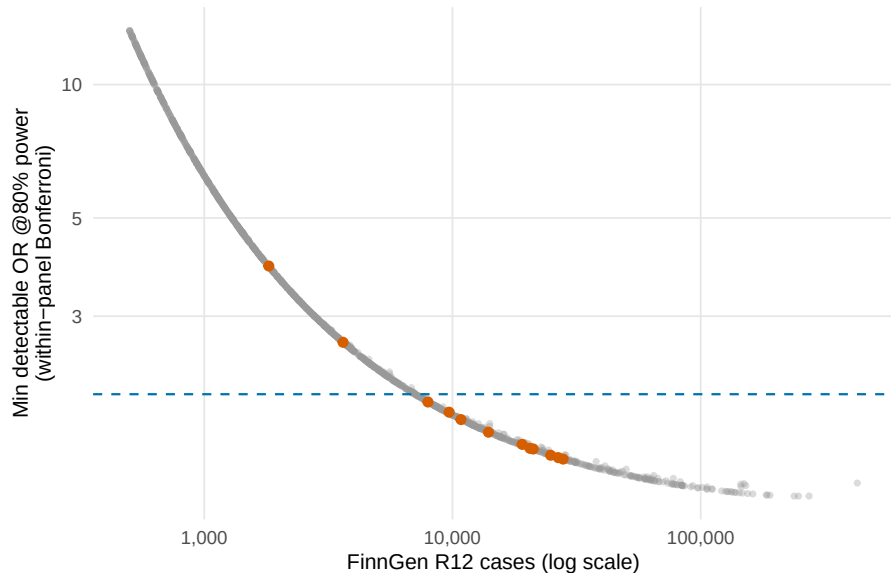