

Clinical Abdominal CT Volume (In Vivo Patient, 64^3 ROI, 4 Chunks):



(a) Conventional Clip
Continuous + Rounding
Phase Reset Error (D_0)
92.2% Error | Streaks

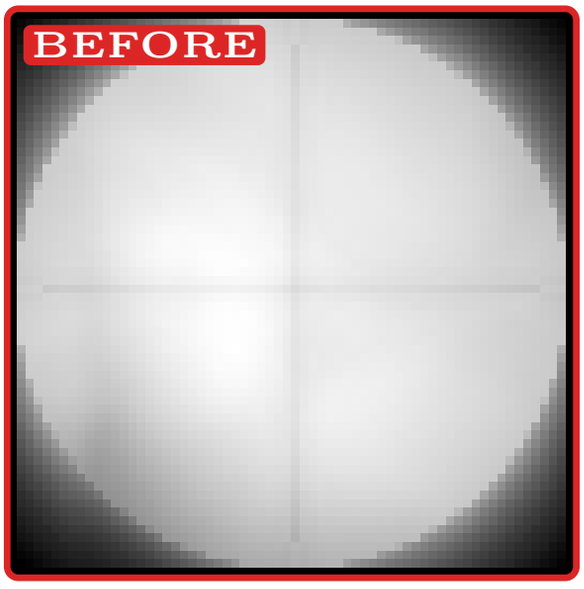


(b) AP-Bresenham
Exact Diophantine Entry
Phase Injection $D(k)$
0.0% Error | Bit-Exact

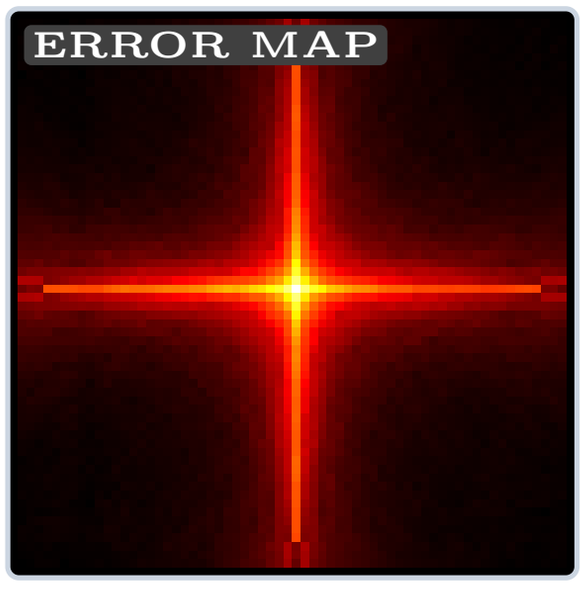


(c) Residual Error
Difference ($|\Delta I|$)
Boundary Streak Noise
Max Error = $15.94\,\mathrm{cm}^{-1}$


MNI-152 Human Brain MRI Volume (Isotropic $1\,\mathrm{mm}^3$, 4 Chunks):

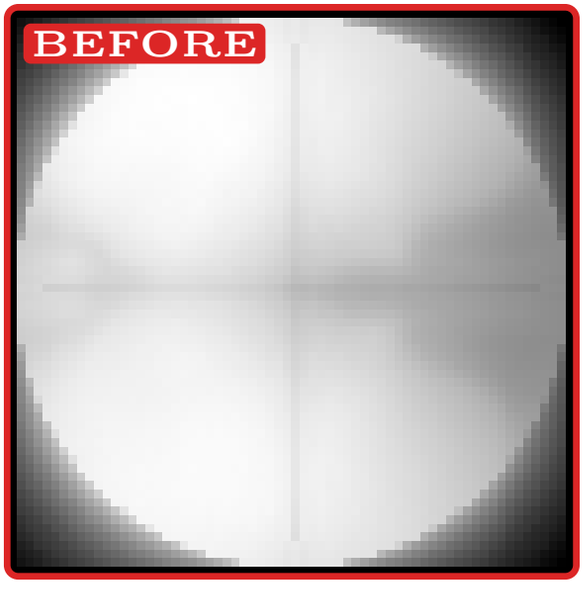

(d) Conventional Clip
Continuous + Rounding
Phase-Shift Seam Jump
90.2% Error | Step Shift

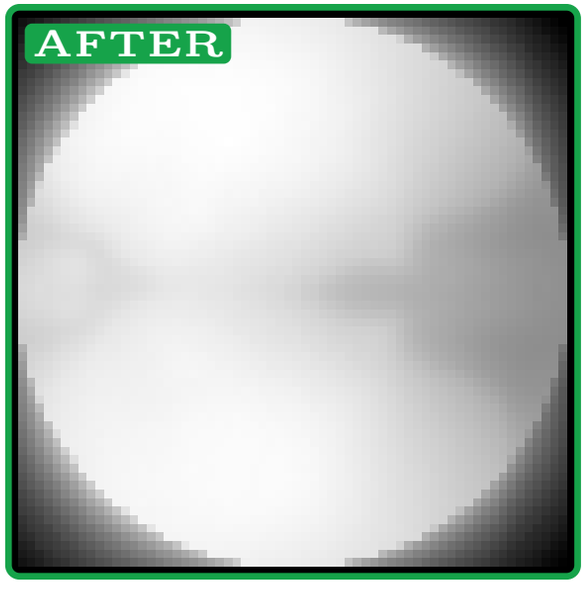

(e) AP-Bresenham
Exact Diophantine Entry
Phase Injection $D(k)$
0.0% Error | Seamless

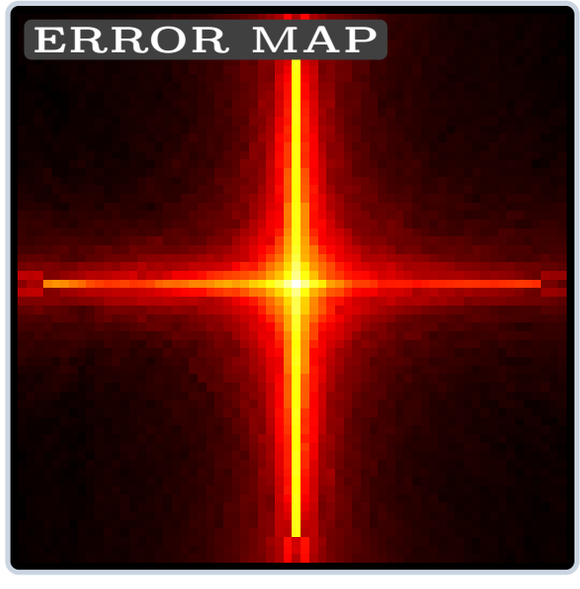

(f) Residual Error
Difference ($|\Delta I|$)
Boundary Step Error
Max Signal Diff = 41.61