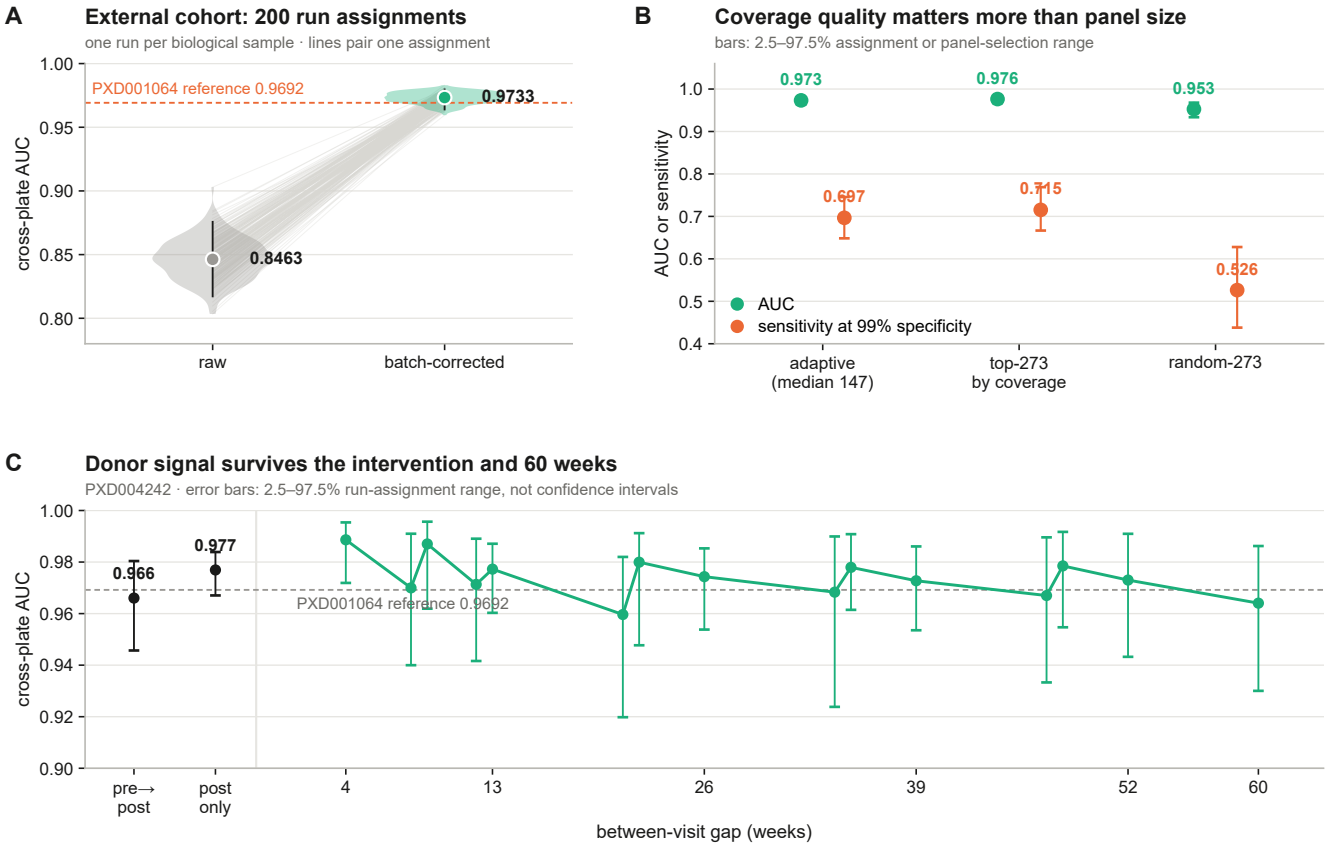

A
External cohort: 200 run assignments
one run per biological sample · lines pair one assignment
PXD001064 reference 0.9692
0.9733
0.8463
cross-plate AUC
raw
batch-corrected
B
Coverage quality matters more than panel size
bars: 2.5–97.5% assignment or panel-selection range
0.973
0.976
0.953
0.697
0.715
0.526
AUC or sensitivity
AUC
sensitivity at 99% specificity
adaptive (median 147)
top-273 by coverage
random-273
C
Donor signal survives the intervention and 60 weeks
PXD004242 · error bars: 2.5–97.5% run-assignment range, not confidence intervals
0.966
0.977
PXD001064 reference 0.9692
cross-plate AUC
pre→ post
post only
between-visit gap (weeks)