


BioLogic DuoFlow Run Report

Project: Runs
Method: S75 A=140ml 0.6ml/min QT
Run: 2019-01-17 CgPho4 post-Heparin 5ml

User: Bin He (Blue) Run Date: 04:26:30 PM 01-17-19

Printed: Friday, January 18, 2019

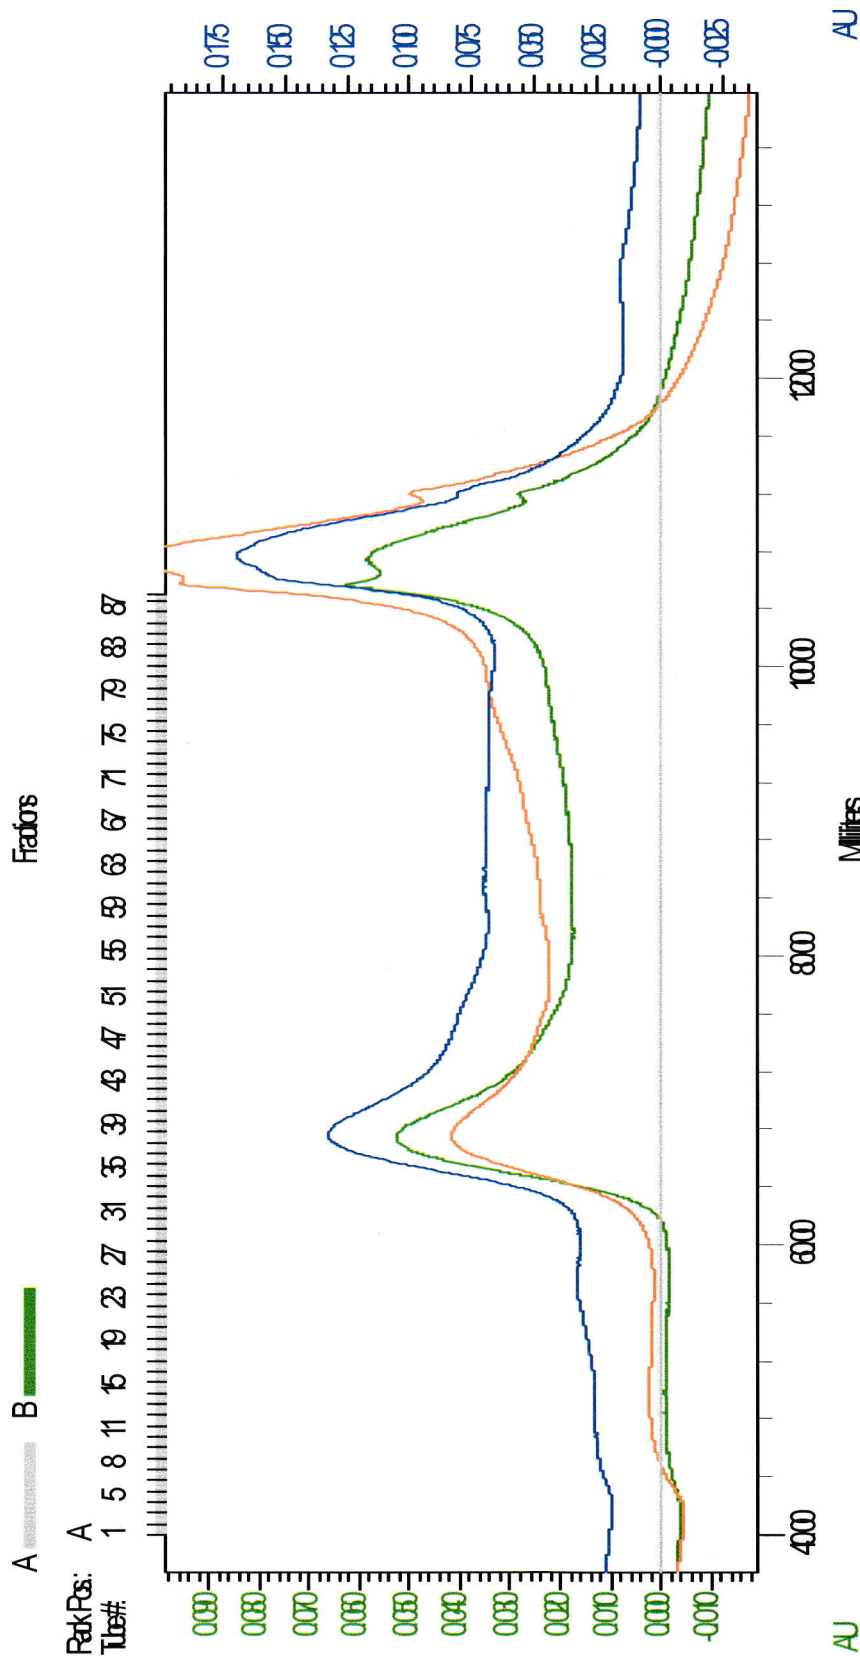

Line style	Detector	Base	Max	Units	Detector	Base	Max	Units
—	QuadTec-1 (280 nm)	0.000	0.100	AU	UV	0.000	0.200	AU
—	QuadTec-2 (240 nm)	0.00	2.00	AU	Conductivity	0.0	25.0	mS/cm
—	QuadTec-3 (214 nm)	0.00	2.00	AU	GP pressure	0.0	4000.0	psi
—	QuadTec-4 (260 nm)	0.000	0.100	AU	% Buffer B	0.0	105.0	% Buffer B