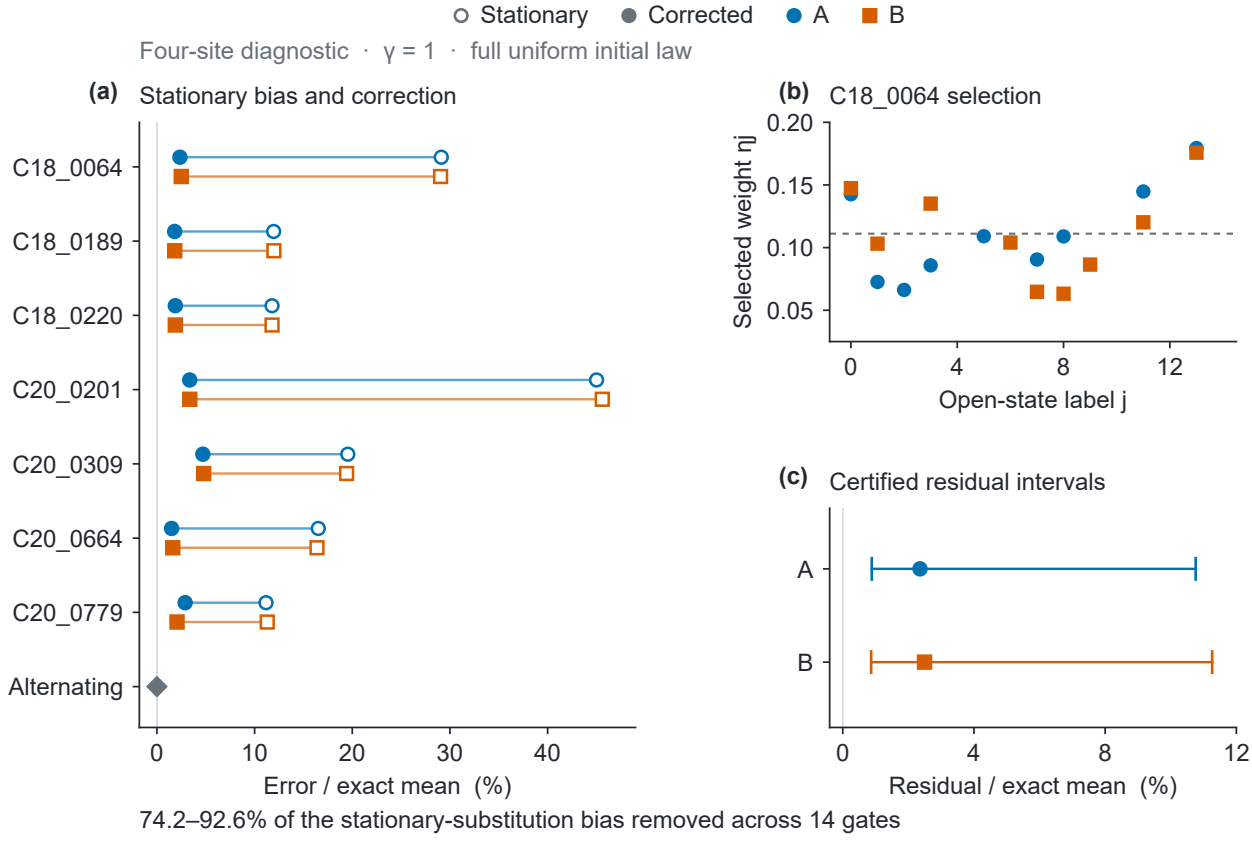

Stationary
Corrected
A
B
Four-site diagnostic · γ = 1 · full uniform initial law
(a)
Stationary bias and correction
C18_0064
C18_0189
C18_0220
C20_0201
C20_0309
C20_0664
C20_0779
Alternating
0
10
20
30
40
Error / exact mean (%)
(b)
C18_0064 selection
Selected weight πj
0.20
0.15
0.10
0.05
0
4
8
12
Open-state label j
(c)
Certified residual intervals
A
B
0
4
8
12
Residual / exact mean (%)
74.2–92.6% of the stationary-substitution bias removed across 14 gates