

1.

True Positives: 26


False Positives: 3

False Negatives: 21

True Negatives: 150

Precision: 0.90

Recall: 0.55

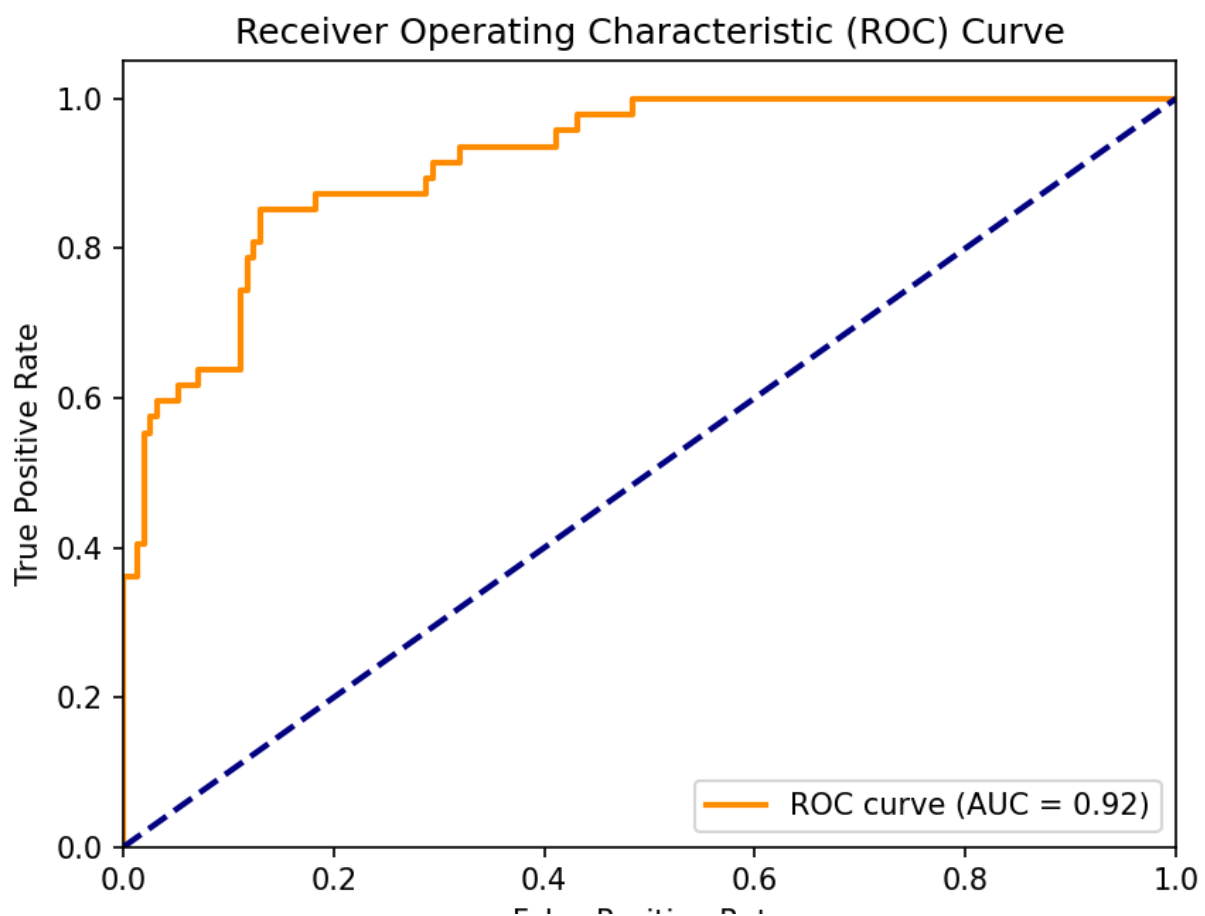

The minimum False Positive Rate at a True Positive Rate of at least 90% is: 0.29

2. Target class: Eggs

3. Parameter Count: 11169089

4. Training Accuracy: 100%      Test Accuracy: 50%

5. Number positive: 5      Number Negative: 5

