



0152GBO, couveuse, juin (active)
11 journées, plaque 200 W, 8 critères tenus sur 10

NRMSE 9,1 % $\leq$ 20,0	LDC 5,5 % $\leq$ 20,0	FFT 28,3 % $>$ 20,0	Énergie +0,1 % $\leq$ 12,5	Pointe −1,1 % $\leq$ 11,6
Fact. de charge 1,0 % $\leq$ 12,5	CORR_h 2,7 % $\leq$ 10,0	TVD_h 1,1 % $\leq$ 10,0	EXT_prof 18,4 % $\leq$ 50,0	Heure des pics 3,0 h $>$ 2,0
Forme 1 h 2,0 $\sigma \leq$ 3,7	Forme 2 h 0,9 $\sigma \leq$ 3,7	Pire écart 1 h 16,0 % $\leq$ 71,2	Verdict non vérifiable	Pointe jour. P95 200 / 177 W

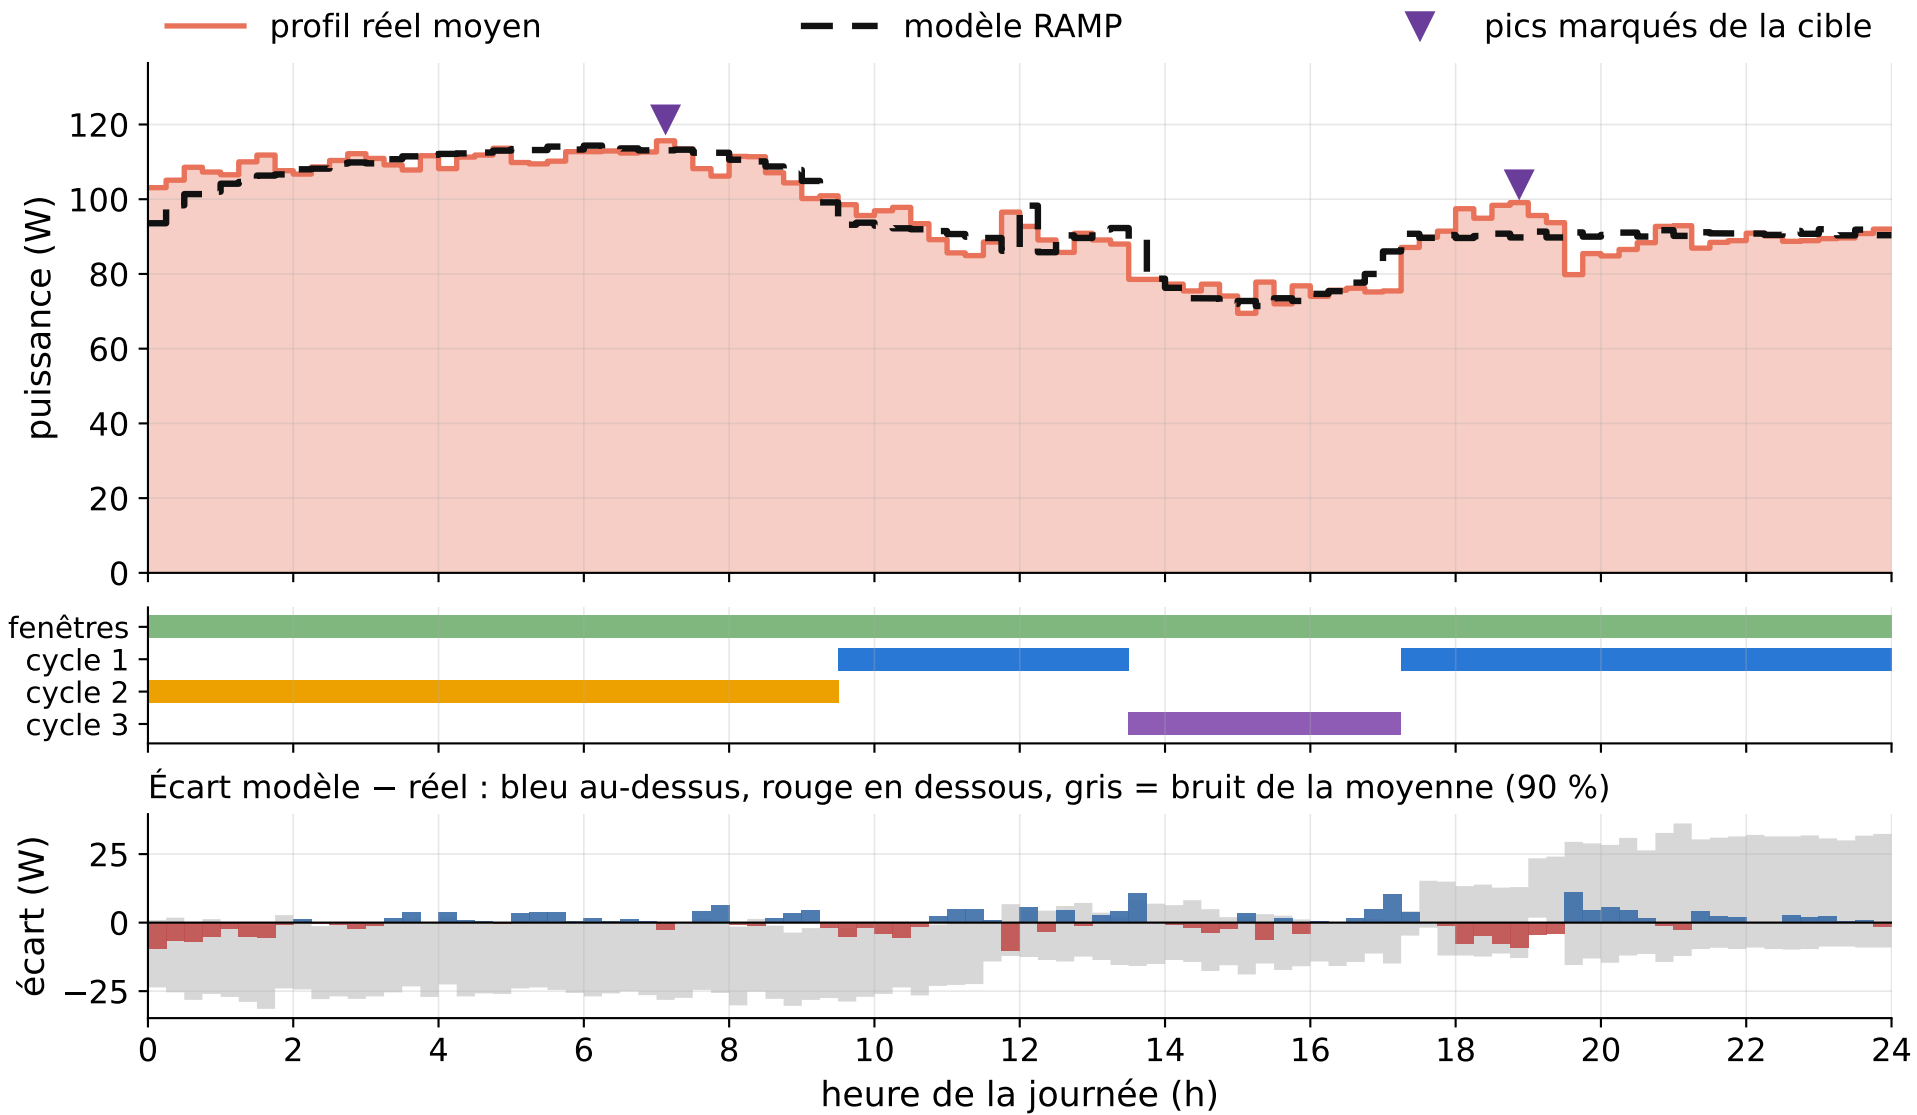

Courbe classée, LDC 5,5 %

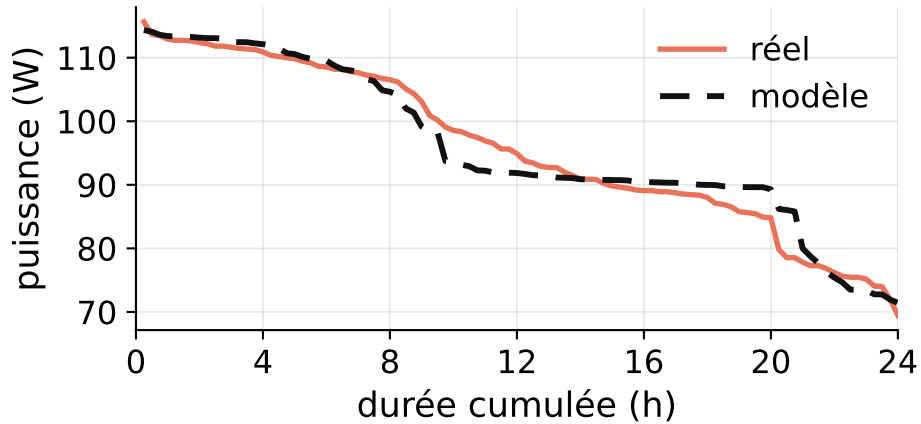

Harmoniques, FFT 28,3 %

