


Glaucoma progression: confirm, then reset the target

A reliable trend matters more than one printout or a population pressure limit.

Read quality before the grey scale

A | A suspicious field needs context

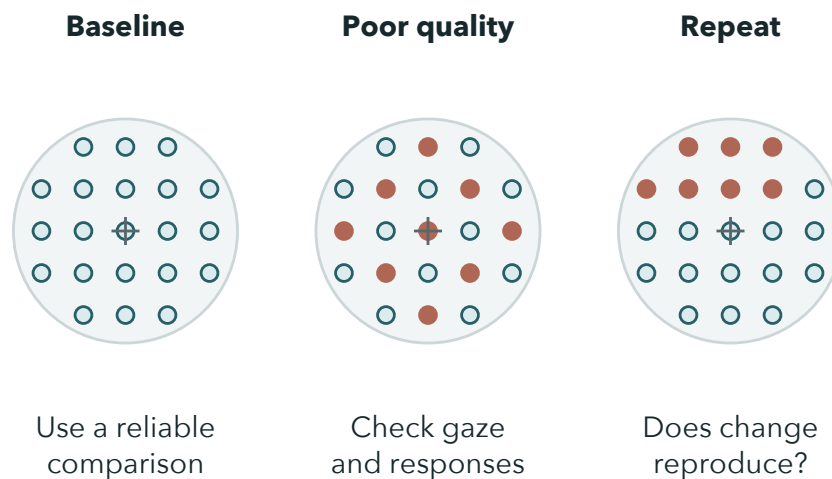

Correlate reliable fields with disc and OCT
An isolated poor test is not a progression trend


Original perimetry-style schematics, not patient tests. A repeatable pattern must be interpreted with quality and matching structural evidence.

Before declaring progression

Check	Reason
Identity and setup	Correct eye, refractive correction, test strategy and comparable previous tests.
Gaze and responses	Fixation, tracking, false responses, fatigue and technician observations influence interpretation.
OCT and disc	Review scan quality and segmentation; seek concordant structural change.
Uncertain isolated result	Repeat under better conditions; do not escalate solely from an unreliable printout.

The target belongs to this optic nerve

B | Normal pressure may still be insufficient

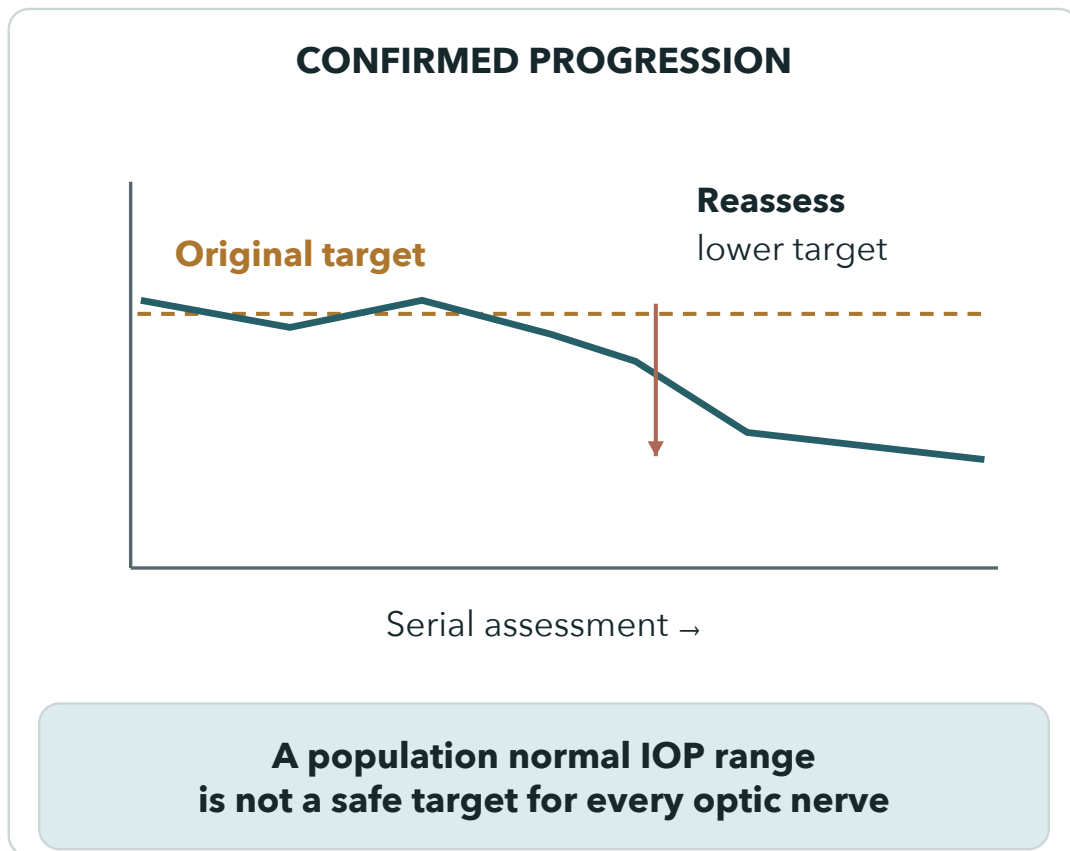

Original target-pressure timeline. Confirmed structural and functional progression prompts reassessment rather than reassurance from a normal-range reading.

Act on reproducible change

Assess adherence, delivery, pressure pattern and secondary causes. Confirmed progression at the previous target may justify a lower target and stronger medical, laser or surgical treatment. Severity, pace of loss, fixation threat and remaining lifetime shape the decision. Normal-tension glaucoma can benefit from pressure reduction. A disc haemorrhage supports closer assessment but is not a stand-alone guarantee of progression. Repeated measurements and clinical judgement avoid both delayed protection and unnecessary escalation. A new dark field plot after poor fixation does not have the same meaning as three reliable tests showing the same worsening defect with corresponding nerve loss. Confirmation resolves uncertainty; a reproducible trend then changes the target even when the pressure appears normal.

References AAO EyeWiki | Normal-tension glaucoma | NICE NG81 | Glaucoma recommendations | AAO EyeWiki | Standard automated perimetry