

Certificate of Analysis

Client:
H peptides

Amino acid sequence (Tesamorelin)

Tyr-Ala-Asp-Ala-Ile-Phe-Thr-Asn-Ser-Tyr-Arg-Lys-Val-Leu-Gly-Gln-Leu-Ser-Ala-Arg-Lys-Leu-Leu-Gln-Asp-Ile-Met-Ser-Arg-Gln-Gly-Gln-Ser-Gly-Gly-Ser-Ser-Ser-Gly-Gly-Gly-Ser-Ser-Gly-Gly-Gly

Sample Identification

Sample Name	Tesamorelin 10 mg	Batch Number	TS1020-01	Date Published	10-APR-2026
-------------	-------------------	--------------	-----------	----------------	-------------

Results for TS1020-01 TESAMORELIN

Analysis of Peptide Identity, Content and Purity	ResultUnit	Uncertainty	Reporting Limit
Tesamorelin Assay <i>Peptide Screening</i>	10.09 mg	[± 0.05]	
Tesamorelin Identification by RT <i>Peptide Screening</i>	0.991	[± 0.005]	
Tesamorelin Identification by spectrum <i>Peptide Screening</i>	5133	[± 20]	
Tesamorelin Purity <i>Peptide Screening</i>	99.1 %	[± 0.25]	

Bioburden	ResultUnit	Uncertainty	Reporting Limit
Total Aerobic Microbial Count <i>USP <61> Plate Count Method</i>	Not detected CFU/g		>= 1000 Δ
Total Yeast and Mold Count <i>USP <61> Plate Count Method</i>	Not detected CFU/g		>= 100 Δ

Endotoxin Analysis	ResultUnit	Uncertainty	Reporting Limit
Bacterial Endotoxin <i>USP<85> Bacterial Endotoxin Chromogenic Test</i>	< 0.001 EU/mg		> 0.5 Δ

Heavy Metals	ResultUnit	Uncertainty	Reporting Limit
--------------	------------	-------------	-----------------


Analysis Dashboard

Tesamorelin

• Batch: TS1020-01 • 10-APR-2026

HPLC Chromatogram


HIGH PERFORMANCE LIQUID CHROMATOGRAPHY • PURITY ANALYSIS

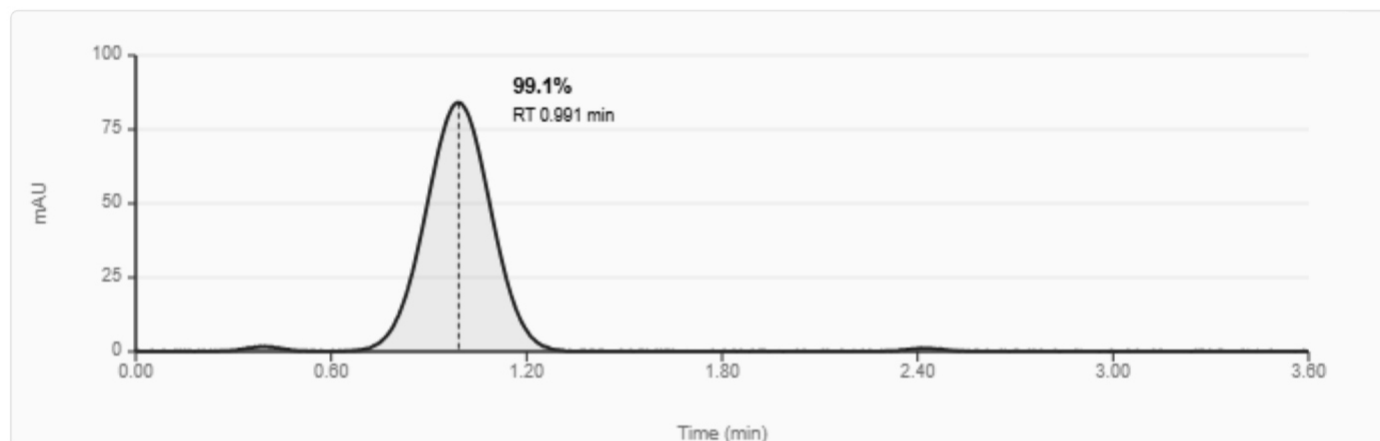

Column: C18, 250×4.6 mm, 5µm Mobile phase: H₂O/ACN + 0.1% TFA Detection: UV 220 nm RT: 0.991 min Purity: 99.1%

Mass Spectrum

ELECTROSPRAY IONIZATION MASS SPECTROMETRY • IDENTITY CONFIRMATION

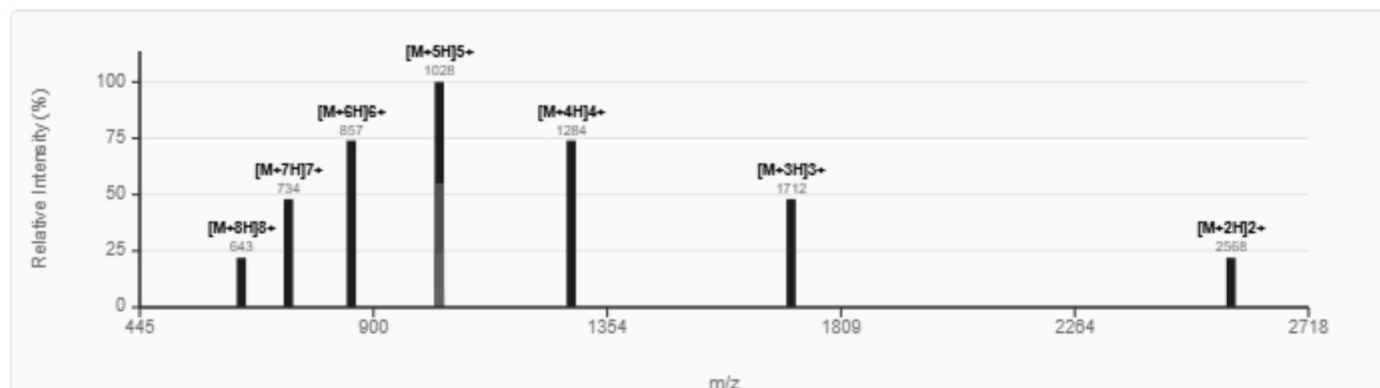

Ionization: ESI+, positive mode Instrument: LC-MS/MS Observed: 5133 m/z Identity: Confirmed ✓



Quality Assurance

SIGNED CERTIFICATION

Analysis results relate only to the samples tested.

This document shall not be reproduced except in full, without the written approval of H Peptides.

Edwin Hoag

Edwin Hoag, MD, PhD

Inspecting QA/QC Manager •