

An Extensible Induced Position Encoding Readout Method for Micro-pattern Gas Detectors

Shubin Liu, Siyuan Ma, Binxiang Qi, Zhongtao Shen, Guangyuan Yuan, Qi An

Abstract— The large number of electronics channels has become an issue to the further applications of Micro-pattern Gas Detectors (MPGDs), and poses a big challenge for the integration, power consumption, cooling and cost. Induced position encoding readout technique provides an attractive way to significantly reduce the number of readout channels. In this paper, we present an extensible induced position encoding readout method for MPGDs. The method is demonstrated by the Eulerian path of graph theory. A standard encoding rule is provided, and a general formula of encoding & decoding for n channels is derived. Under the premise of such method, a one-dimensional induced position encoding readout prototyping board is designed on a $5 \times 5 \text{ cm}^2$ Thick Gas Electron Multiplier (THGEM), where 47 anode strips are read out by 15 encoded multiplexing channels. Verification tests are carried out on an 8 keV Cu X-ray source with $100 \mu\text{m}$ slit. The test results show a robust feasibility of the method, and have a good spatial resolution and linearity in its position response. This method can dramatically reduce the number of readout channels, and has potential to build large area detectors and can be easily adapted to other detectors like MPGDs.

Index Terms—micro-pattern gas detector, position encoding, multiplexing readout, tracking

I. INTRODUCTION

OVER the past 20 years, Micro-pattern Gas Detectors (MPGDs) were widely used in high-energy physics, and had expanded to astrophysics, nuclear physics and medical imaging.[1][2] The conventional readout techniques employ a large number of electronic channels, which poses a big challenge to the further applications of MPGDs. By changing the readout electrodes' structure and multiplexing the readout channels, an induced position encoding technique for micro-channel plate detector was developed by D. Kataria et al. [3] in 2007. This technique was used for MPGDs by R. Hu et al. in 2011 [4], where a preliminary feasibility test was implemented with Micromegas. This technique could significantly reduce the number of readout channels, but the foregoing works didn't provide an extensible encoding method and the decoding was complicated. In this paper, an extensible induced position encoding readout method for MPGDs is

presented. This method is demonstrated by the Eulerian path of graph theory. A standard encoding rule is provided, and a general formula of encoding & decoding for n channels is derived. A prototyping design is implemented on a $5 \times 5 \text{ cm}^2$ Thick Gas Electron Multiplier (THGEM), and verification tests are carried out on a 8 keV Cu X-ray source with $100 \mu\text{m}$ slit.

II. PRINCIPLE AND METHOD

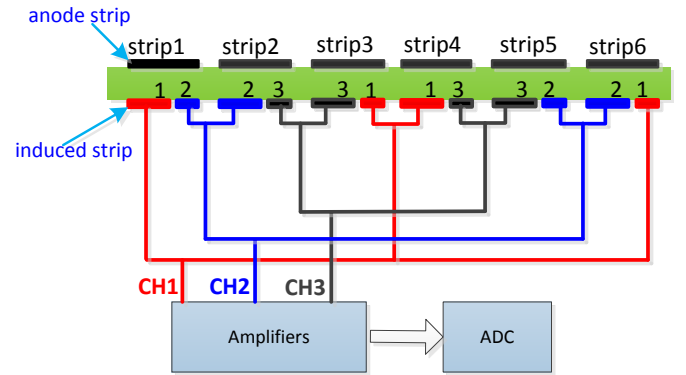


Fig. 1. Induced position encoding readout schematic

A. Principle

For ease of understanding, the simplified schematic is shown in Fig. 1, where 6 strips are readout by 3 encoded multiplexing channels. Charge from detectors is collected by an anode strip and split across two induced strips which correspond to the respective readout channels. Due to the different width, charge is split unequally between the two induced strips, thus the amplitude on one is always higher than the other. Based on the signals' amplitudes in corresponding channels, the hit position

TABLE I
DECODING TABLE OF 3 READOUT CHANNELS

Channel: comparsion	Strip: position
CH1>CH2	Strip 1
CH2>CH3	Strip 2
CH3>CH1	Strip 3
CH1>CH3	Strip 4
CH3>CH2	Strip 5
CH2>CH1	Strip 6

could be uniquely decoded as seen in Table I.

This paragraph of the first footnote will contain the date on which you submitted your paper for review.

This work was supported by National Natural Science Foundation of China (Grant No.11222552).

Shubin Liu is with State Key Laboratory of Particle Detection and Electronics, University of Science and Technology of China, No.96, Jinzhai Road, Hefei, Anhui, China (e-mail: liushb@ustc.edu.cn).




Fig. 2. An Eulerian Path

B. Eulerian Path Theorem

As shown in Fig. 1, 3 readout channels have P_3^2 ordered doublet combinations $\{12,23,31,13,32,21\}$ which correspond to 6 anode strips. This technique requires that any ordered doublet combination of channels appeared exactly once, and formed head to tail as an encoding list. Generally, the principle described above is a graph theory problem that whether there is an Eulerian path, where the doublet combinations represent the edges and the readout channels represent the vertices. Fig. 2 shows an Eulerian path of the 3 readout channels in Fig. 1. According to Eulerian path theorem [5], it can be proved that there is an Eulerian path for n channels induced position encoding readout, as all of its vertices have an even degree. In other words, n channels can encode readout a maximum P_n^2 anode strips.

C. Encoding and Decoding

It turns out that there are more than one construction of Eulerian path. We need to make appropriate constraints to construct a regular and extensible encoding method so as to easily decode and design. As shown in Table 2, it is an extensible encoding list for n channels, where the list is organized in rows. The encoding form XY means that the signal's amplitude of channel X is higher than channel Y .

According to the Table II, the encoding formula (1) and decoding formula (2) can be derived as follows:

$$i_{(x,y)} = \begin{cases} (y-1)(2n-y)+1 & \text{encoding form: } ny \\ (y-1)(2n-y)+2(x-y)+1 & \text{encoding form: } xy(x > y) \\ (x-1)(2n-x)+2(y-x) & \text{ending form: } xy(x < y) \end{cases} \quad (2)$$

D. Width Ratio of Two Induced Strips

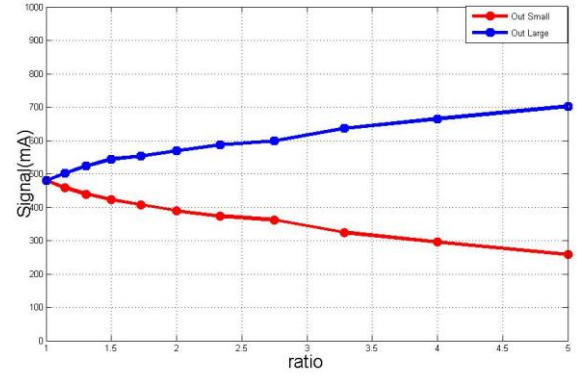


Fig. 3. The output signals of wide strip and narrow strip under different width ratio

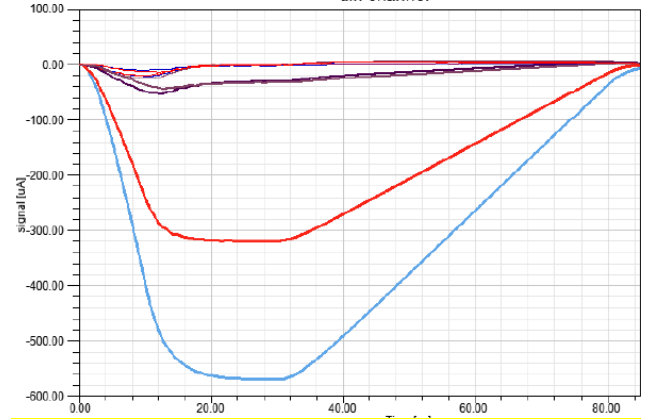


Fig. 4. Output signal of all electronic channels when ratio is 2:1

In order to study the relationship between the two induced strips, we used ANSYS's software Designer and SIwave to simulate magnitudes of induced signals. The relationship between the larger signal and the smaller signal at different width ratios have been shown in Fig. 3. It's necessary to ensure

TABLE II
THE ENCODING LIST OF N READOUT CHANNELS

Row	Encoding list									
1	12	21								
2	13	32	23	31						
3	14	42	24	43	34	41				
...				
k-1	1k	k2	2k	k3	3k	k4	...	k(k-1)	(k-1)k	k1
...
n-1	1n	n2	2n	n3	3n	n4	n(n-1)	(n-1)n
										n1

$$(xy)_i = \begin{cases} n, k & R = 1 \\ \left(k, \frac{R}{2} + k\right) & i = \text{even number} \\ \left(\frac{R-1}{2} + k, k\right) & i = \text{odd number} \end{cases} \quad (1)$$

that not only the signals from the two induced strips have enough difference, but also the smaller signal can be distinguished easily from crosstalk and noise. It's reasonable to take 2 as the ratio of the two strips, considering the production process of Printed Circuit Board (PCB). Fig. 4 shows the output signal of each channel when the width ratio is 2. It can be seen

from Fig. 4 that the smaller signal has enough recognition degree from crosstalk. And of course, it's also much larger than the noise.

E. Packet Coding Techniques

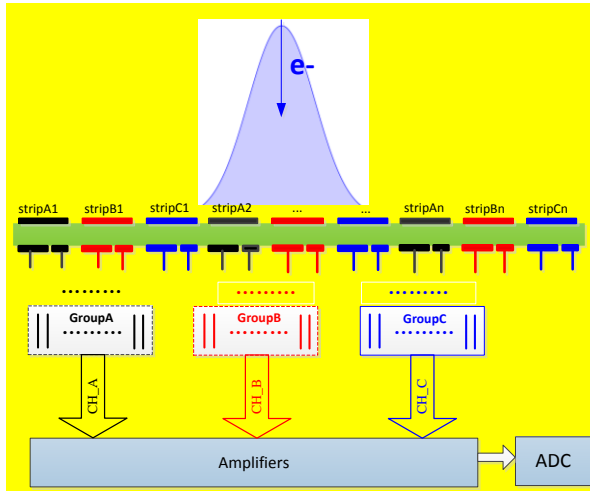


Fig. 5. Schematic of packet coding techniques

If two or more adjacent anode strips are directly encoded together, the decoding will have faults because the signal has a certain width and more than one strip is hit. To solve this problem, Packet Coding techniques are proposed. As shown in Fig. 5, the adjacent anode strips are assigned to different groups, which are encoded and decoded individually. In this way, an event with a certain width will not hit more than one strip of one group. The number of group is decided on the width of the signal and the width of the strip. Besides, by using Packet Coding method, higher position resolution can be obtained by applying finer strips.

III. VERIFICATION TEST

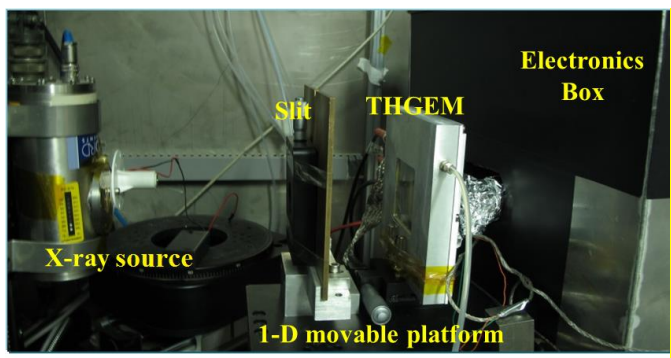


Fig. 6. Experimental setup

A. Experiment for verification

In order to verify this method, a prototyping readout board was manufactured and equipped for a 5×5 cm² THGEM detector[6]. To solve the case that each particle usually showers the signal on several neighboring strips, the neighboring strips are separated into three groups to encode respectively. Based

on the encoding list shown in TALBE II, the prototyping board has 47 one-dimensional 1.07mm strips which are readout by 15 channels. According to the decoding formula, the hit strip can be decoded by the fired channels.

As shown in Fig. 6, verification tests are carried out on the THGEM detector, which is filled with Ar/iC₄H₁₀(93:7) gas mixture. A 100 μ m slit in a thin brass sheet was used to produce a miniaturized X-ray beam. A manual movable platform was used for the position scanning test. The electronics are based on the VATA160 chip.[7]

B. Result of tests

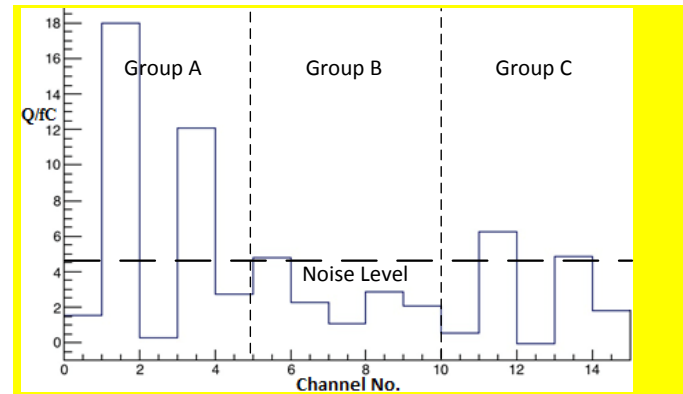


Fig. 7. The signal recorded on 15 channels when an event hit

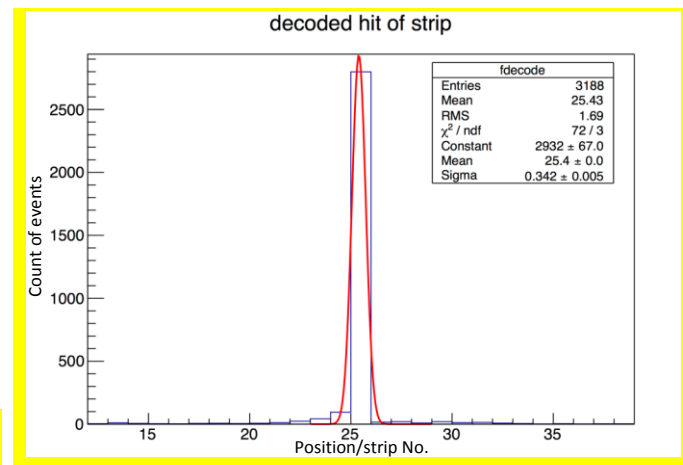


Fig. 8. Spatial resolution result of the detector

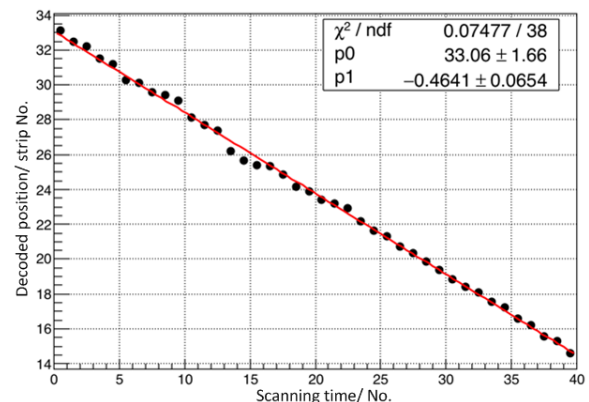


Fig. 9. Linear result of position scanning test

Fig. 7 shows the signals recorded on all 15 channels of one hit event. There are 47 anode strips, which are divided into 3 groups to be encoded and decoded individually, and the width of each strip is 1.07mm. The baseline noise is about 2.5fC. We take twice the noise of 5fC as the noise threshold to filter the valid signals. It can be inferred that the hit channels are channel 2, channel 4, channel 12 and channel 14. Channel 2 and channel 4 belong to group A, from which the hit strip of strip 25 can be decoded. The Channel 12 and channel 14 mean that strip 26 is hit, too. According to the distribution of charge on the two strips, the true hit point is strip 25.25, and the width of the event is about 2 strips, which means 2.14mm.

Fig. 8 shows the decoded spatial resolution result of the detector. The width of anode strip is 1.07mm. A large number of statistics have been made for a fixed X-ray incidence location. If the threshold is set to twice the noise, the correct rate of decoding can reach 94%. The root-mean-square (RMS) of the statistical histogram is 1.69 strips, which mean the resolution is 1.8mm.

Fig. 9 shows the results of linearity in the position scanning test. The test setup has been shown in Fig. 6. During the test, the detector was moved with a step of 0.5mm every time. The X-axis of Fig. 9 represents the No. of the scanning, and Y-axis means the decoded anode strip of each time. P0 shows the slope of the fitted red line, which means the step of every movement is 0.464 strips (0.496mm). It's very close to the ideal step of 0.5mm.

IV. CONCLUSION

A novel method of encoded multiplexing readout for micro-pattern gas detectors is presented in this work. The method is demonstrated by the Eulerian path of graph theory. A standard rule for encoding is provided, and general formulas of encoding & decoding for n channels are derived. Under the premise of such rules, a one-dimensional position encoding readout circuit board is designed based on a $5 \times 5 \text{ cm}^2$ THGEM, and a verification test is carried out on a 8 keV Cu X-ray source with 100 μm slit. The test results indicate that the method can decode the hit position. If the threshold is set to twice the noise, the correct rate of decoding can reach 94%. Concerning the correct rate of decoding, the RMS of the position resolution is 1.69 strips, which means 1.808 mm. This method provides an attractive way to significantly reduce the number of readout channels. Inevitably, the method has some disadvantages, such as lowering the signal to noise ratio (SNR) and lowering the detector's rate capability.

REFERENCES

Basic format for books:

- [1] Titov M. New developments and future perspectives of gaseous detectors[J]. Nuclear Instruments and Methods in Physics Research Section A: Accelerators, Spectrometers, Detectors and Associated Equipment, 2007, 581(1): 25-37.
- [2] Liu Q, Liu H B, Chen S, et al. A successful application of thinner-THGEMs[J]. Journal of Instrumentation, 2013, 8(11): C11008.
- [3] Kataria D O, Chaudery R, Rees K. High-speed position readout for microchannel plate-based space plasma instruments[J]. Nuclear

Instruments and Methods in Physics Research Section A: Accelerators, Spectrometers, Detectors and Associated Equipment, 2007, 573(1): 240-242.

- [4] R. Hu, et al., Nuclear Physics Review, 2011, 28(4):459-463
- [5] Gross J L, Yellen J. Graph theory and its applications[M]. CRC press, 2005.
- [6] Liu H B, Liu Q, Chen S, et al. A study of thinner-THGEM, with some applications[J]. Journal of Instrumentation, 2012, 7(06): C06001.
- [7] VATA160 datasheet, IDEAS, Nydalen, Oslo, Norway, 2013. <http://www.ideas.no>