


FEMTO Pulse Run Summary:**Filename and Data Path:** C:\Agilent Technologies\Data\2025 09 29\13-38-58\2025 09 29 13H 38M.raw**Created:** 9/29/2025 1:59 PM**# of Capillaries:** 2**Array Serial #:** 060222-25USFP**Effect Length:** 22 cm**Array Usage Count:** 629**FEMTO Pulse Version #:** 2.0.0.3**Device Serial #:** F12240**METHOD INFORMATION****Method Name:** FP-1003-22 - 55 Kb BAC.mthds**Gel Prime:** No**Full Conditioning:** Yes**Gel Prime to Buffer:** No**Gel Selection:** Gel 1**Perform Prerun:** -8.0 kV, 300 sec.**Rinse:** No**Marker 1:** No**Rinse:** Tray: 3, Row: A, # Dips: 1**Sample Injection:** -3.0 kV, 15 sec.**Separation:** 90.0 min.**Tray Name:** Tray-1**Analysis Mode:** NGS**NOTES**

Time Shift: Using configured: slope=0.00025, intercept=0.0

Gel Image

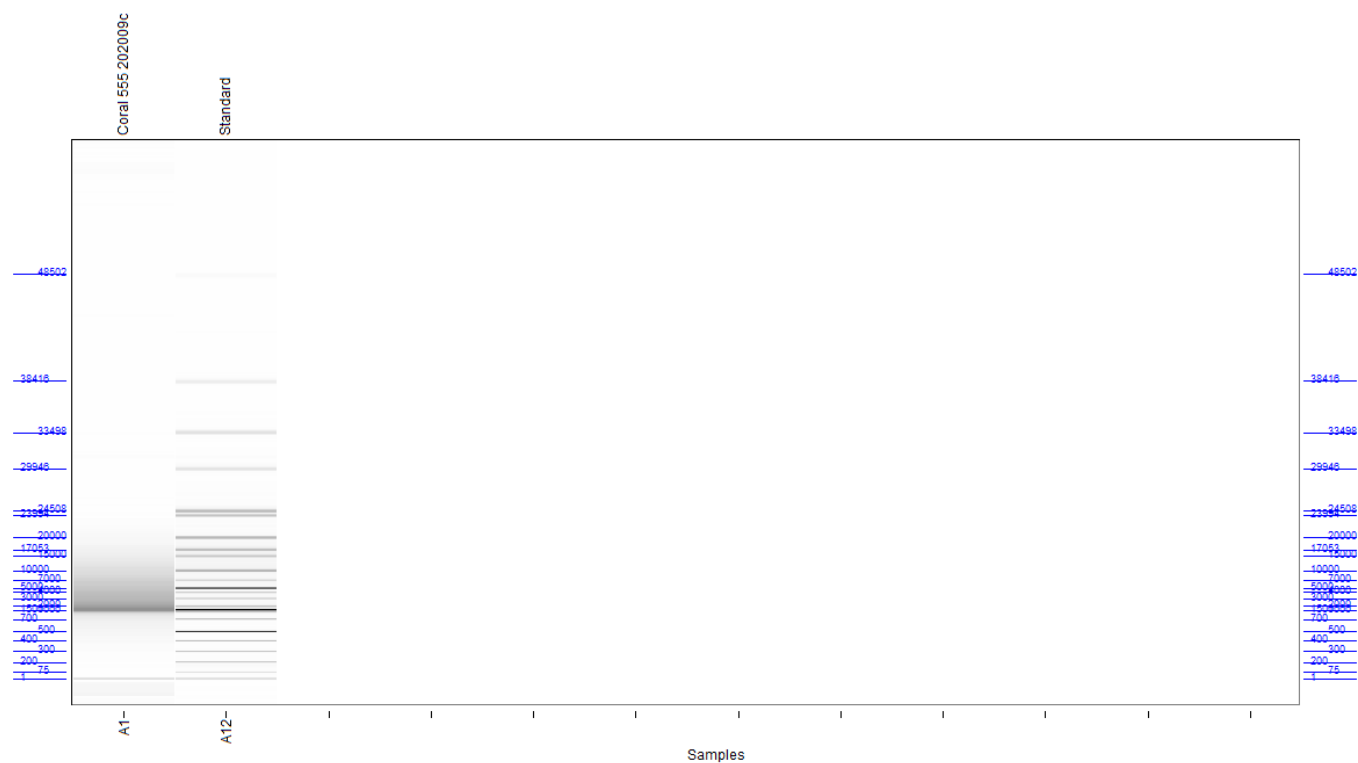



DQN Summary


Well	Sample ID	DQN	Size Threshold (bp)	Total Conc. (pg/uL)
A1 A12	Coral 555 202009c Post Extraction Standard	N/A	0	373.7380

Filename and Data Path: C:\Agilent Technologies\Data\2025 09 29\13-38-58\2025 09 29 13H 38M.raw

A1: Coral 555 202009c Post Extraction

DQN: N/A (Size threshold is less than lower marker end)

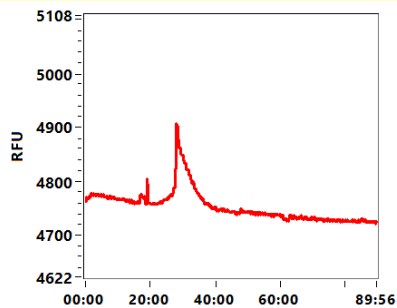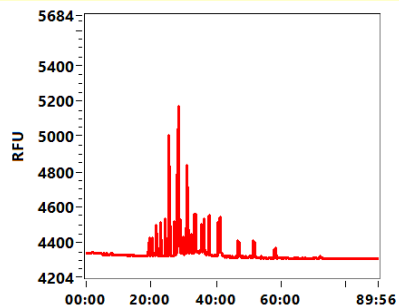**A12: Standard**

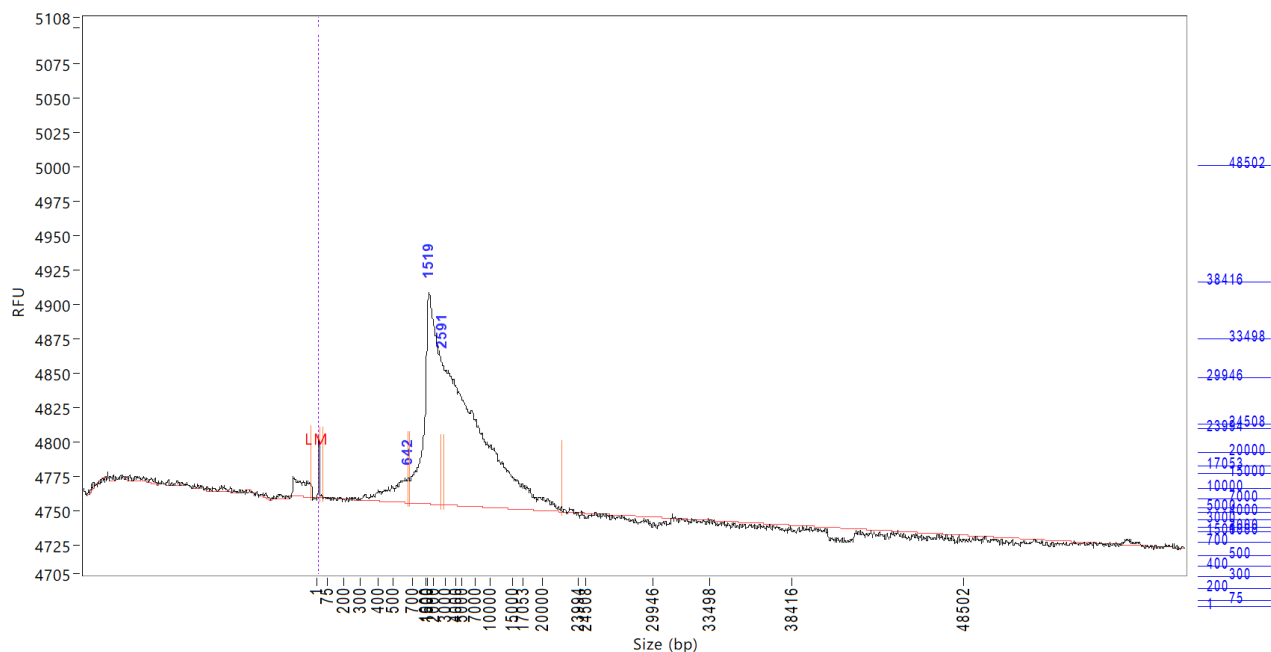Sample: Coral 555 202009c Post Extraction**Well Location:** A1**Created:** 9/29/2025 1:59 PM


Peak	Size (bp)	Conc. (pg/uL)	From (bp)	To (bp)	Avg. Size (bp)	CV%	RFU	Corr. Peak Area
1	1 (LM)	0.4675	0	15	0	-2552.39	44	0.255
2	642	20.2419	33	644	507	18.00	17	1.105
3	1519	146.8205	663	2836	1744	37.21	152	8.016
4	2591	220.7019	2591	22090	7168	62.18	102	12.049

TIC: 387.7643 pg/uL
TIM: 351.1907 pmole/L
Total Conc.: 373.7380 pg/uL

DQN: N/A (Size threshold is less than lower marker end point)
Threshold: 0

Sample Peak Width (sec): 10 Sample Min Peak Height: 50 Sample Baseline V to V?: Y Sample Baseline V to V pts: 3
Sample Filter: Binomial # of Pts for Filter: 3 Sample Start Region (min): 0 Sample End Region (min): 90
Manual Baseline Start (min): 17 Manual Baseline End (min): 90
Marker Peak Width (sec): 5 Marker Min Peak Height: 500 Marker Baseline V to V?: Y Marker Baseline V to V pts: 3
Lower Marker Selection: First Peak > 500 RFU Upper Marker Selection: Last Peak > 500 RFU
Ladder Size (bp): 1, 75, 200, 300, 400, 500, 700, 1000, 1500, 2000, 3000, 4000, 5000, 7000, 10000, 15000, 17053, 20000, 23994, 24508, 25000
Quantification Using: Ladder Final Concentration (ng/uL): 0.0200 Dilution Factor: 10.0
Min. RFU for Data Processing: 1 Size Threshold (b.p.): 0


Sample: Standard
Well Location: A12
Created: 9/29/2025 1:59 PM

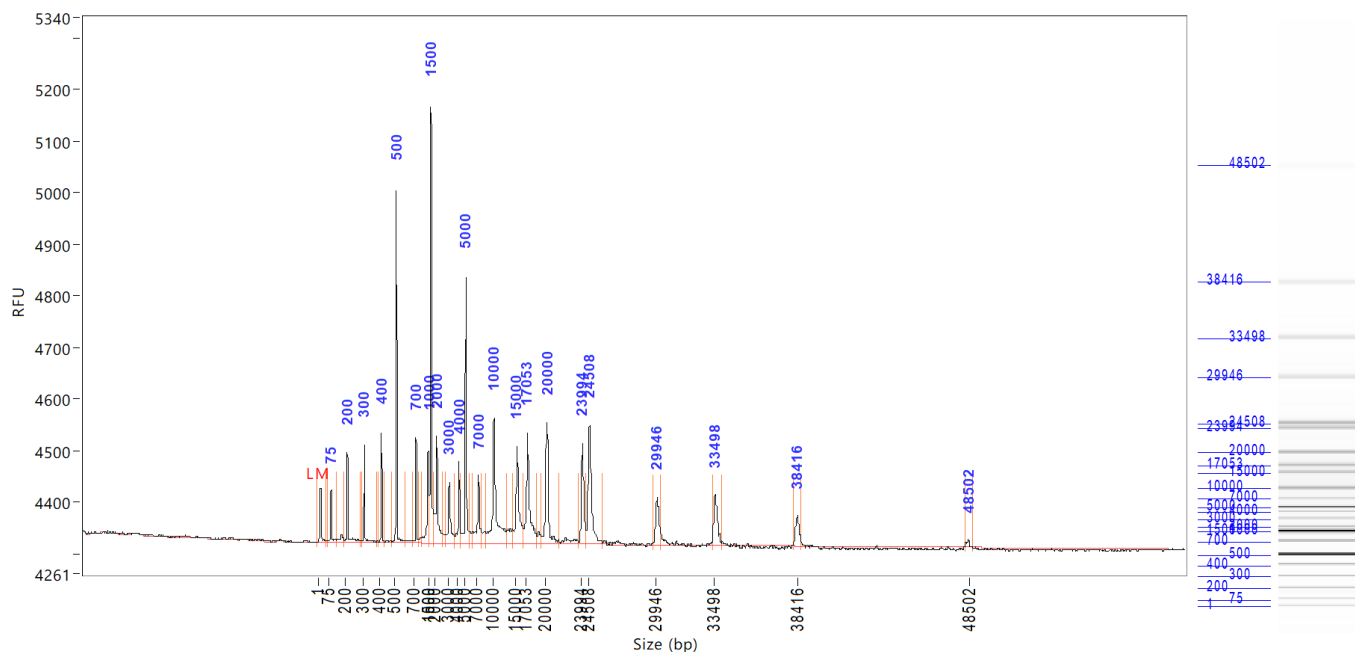

Peak	Size (bp)	Conc. (pg/uL)	From (bp)	To (bp)	Avg. Size (bp)	CV%	RFU	Corr. Peak Area
1	1 (LM)	0.4675	0	46	2	386.74	104	0.714
2	75	3.6110	61	122	77	15.86	99	0.552
3	200	6.0382	178	282	208	9.68	175	0.923
4	300	5.0486	287	376	303	4.38	188	0.771
5	400	4.6655	383	422	399	0.77	213	0.713
6	500	15.1516	478	600	501	2.58	683	2.315
7	700	4.4396	671	754	700	1.43	202	0.678
8	1000	10.7383	829	1001	964	3.79	204	1.641
9	1500	39.3760	754	2705	1429	31.04	846	6.016
10	2000	8.3024	1815	2476	2038	7.43	208	1.268
11	3000	6.0459	2705	3596	3042	6.20	117	0.924
12	4000	4.6564	3596	4323	3954	3.45	159	0.711
13	5000	13.4596	4323	5775	4999	4.34	514	2.056
14	7000	5.9169	6194	7771	6953	4.94	131	0.904
15	10000	17.0600	8541	13009	10422	9.50	241	2.606
16	15000	9.8797	14336	16273	15161	2.86	187	1.509
17	17053	12.0162	16273	18480	17184	2.63	214	1.836
18	20000	11.4709	19101	21464	19966	1.66	234	1.753
19	23994	7.3861	23599	24236	23983	0.46	193	1.128
20	24508	11.9239	24236	25511	24565	0.83	228	1.822
21	29946	4.2611	29634	30199	29941	0.38	92	0.651
22	33498	4.1634	33385	33938	33555	0.33	96	0.636
23	38416	2.4008	38172	38646	38398	0.27	57	0.367
24	48502	0.3340	48321	48803	48457	0.16	14	0.051

Sample Peak Width (sec): 10 Sample Min Peak Height: 100 Sample Baseline V to V?: Y Sample Baseline V to V pts: 3
Sample Filter: Binomial # of Pts for Filter: 3 Sample Start Region (min): 0 Sample End Region (min): 90
Manual Baseline Start (min): 17 Manual Baseline End (min): 90
Marker Peak Width (sec): 5 Marker Min Peak Height: 500 Marker Baseline V to V?: Y Marker Baseline V to V pts: 3
Lower Marker Selection: First Peak > 500 RFU Upper Marker Selection: Last Peak > 500 RFU
Ladder Size (bp): 1, 75, 200, 300, 400, 500, 700, 1000, 1500, 2000, 3000, 4000, 5000, 7000, 10000, 15000, 17053, 20000, 23994, 24508, 29946, 33498, 38416, 48502
Quantification Using: Ladder Final Concentration (ng/uL): 0.0200 Dilution Factor: 10.0
Min. RFU for Data Processing: 1 Size Threshold (b.p.): 0

Sample: Standard
Well Location: A12
Created: 9/29/2025 1:59 PM

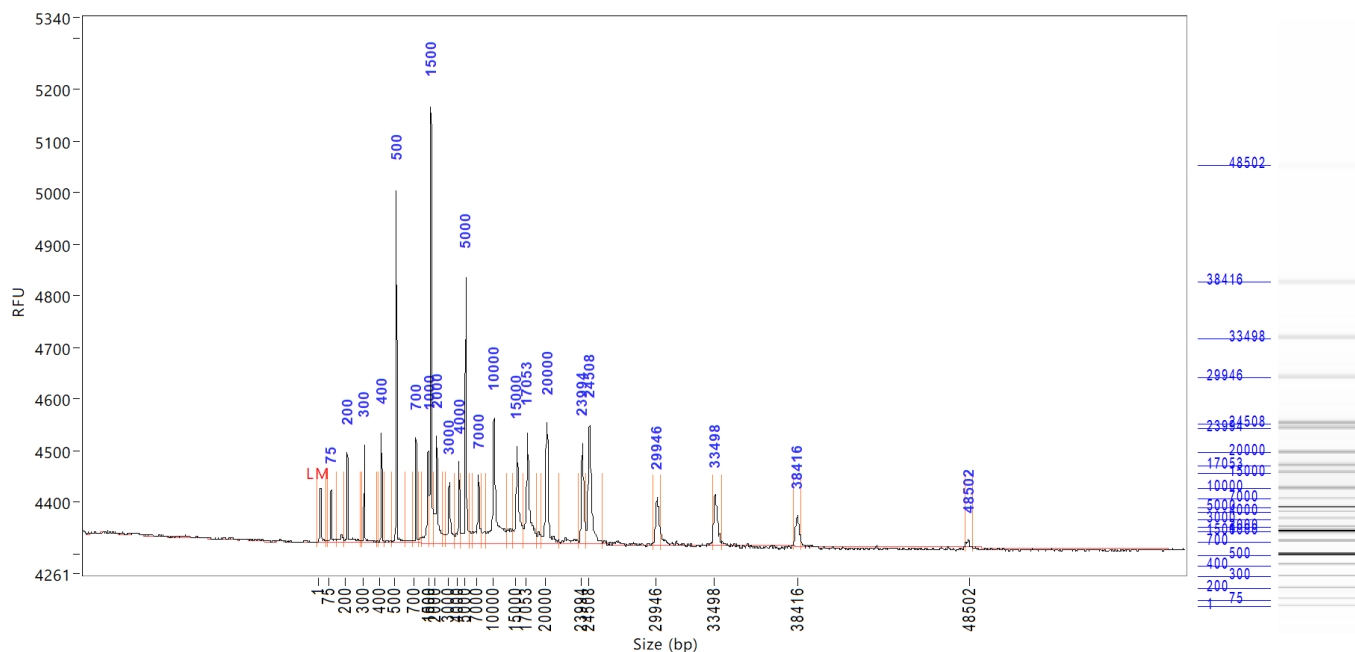

Peak	Size (bp)	Conc. (pg/uL)	From (bp)	To (bp)	Avg. Size (bp)	CV%	RFU	Corr. Peak Area
TIC: 208.3463 pg/uL								
TIM: 322.4428 pmole/L								
Total Conc.: 200.0000 pg/uL								

Sample Peak Width (sec): 10 Sample Min Peak Height: 100 Sample Baseline V to V?: Y Sample Baseline V to V pts: 3
Sample Filter: Binomial # of Pts for Filter: 3 Sample Start Region (min): 0 Sample End Region (min): 90
Manual Baseline Start (min): 17 Manual Baseline End (min): 90
Marker Peak Width (sec): 5 Marker Min Peak Height: 500 Marker Baseline V to V?: Y Marker Baseline V to V pts: 3
Lower Marker Selection: First Peak > 500 RFU Upper Marker Selection: Last Peak > 500 RFU
Ladder Size (bp): 1, 75, 200, 300, 400, 500, 700, 1000, 1500, 2000, 3000, 4000, 5000, 7000, 10000, 15000, 17053, 20000, 23994, 24508, 29946, 33498, 38416, 48502
Quantification Using: Ladder Final Concentration (ng/uL): 0.0200 Dilution Factor: 10.0
Min. RFU for Data Processing: 1 Size Threshold (b.p.): 0

Sample: Standard
Well Location: A12
Created: 9/29/2025 1:59 PM
Fit Type: Point to Point

Calibration Curve

