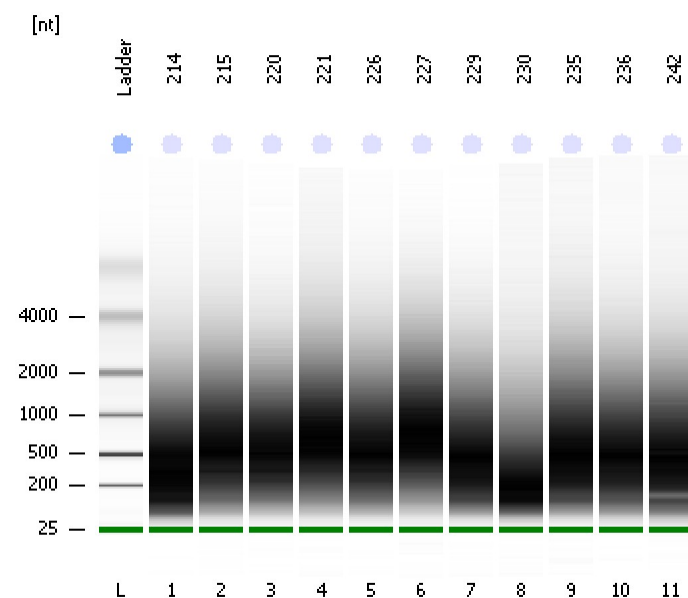


Assay Class: Eukaryote Total RNA Pico  
Data Path: C:\...Eukaryote Total RNA Pico\_DE72902486\_2016-12-12\_17-40-14.xad

Created: 12/12/2016 5:40:14 PM  
Modified: 12/12/2016 6:03:13 PM

**Electrophoresis File Run Summary**Instrument Information:

Instrument Name: DE72902486  
Serial#: DE72902486

Firmware: C.01.069  
Type: G2939A

Assay Information:

Assay Origin Path: C:\Program Files\Agilent\2100 bioanalyzer\2100 expert\assays\RNA\Eukaryote Total RNA Pico Series II.xsy

Assay Class: Eukaryote Total RNA Pico

Version: 2.6

Assay Comments: Total RNA Analysis pg sensitivity (Eukaryote)












© Copyright 2003 - 2009 Agilent Technologies, Inc.

Chip Information:

Chip Lot #:

Reagent Kit Lot #:

Chip Comments:

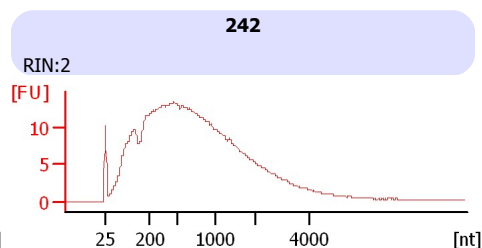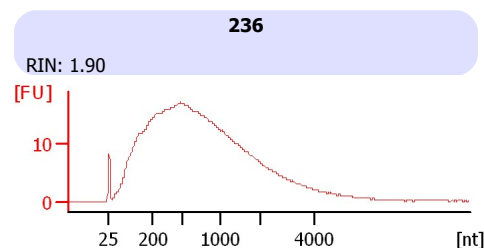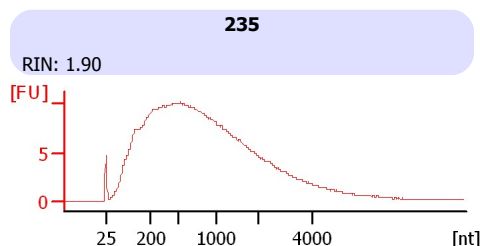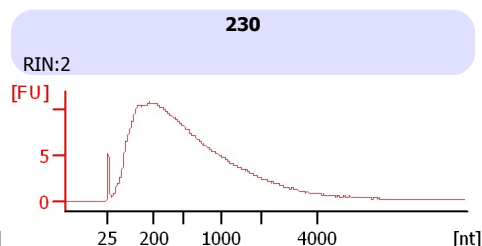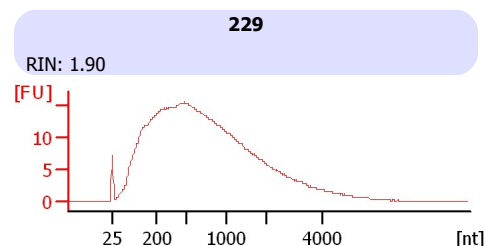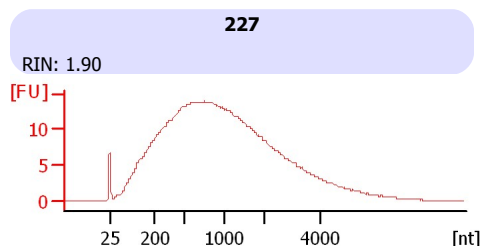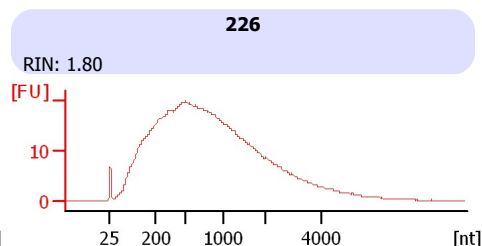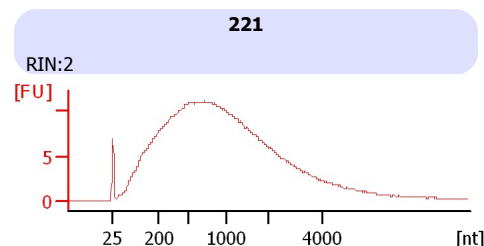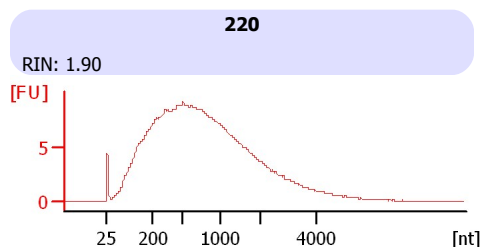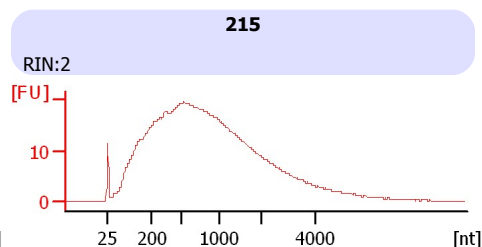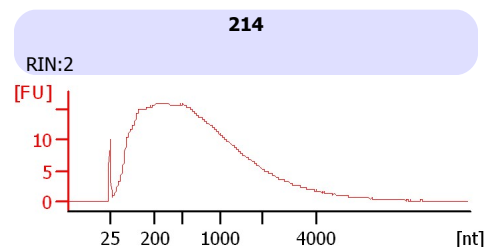

Assay Class: Eukaryote Total RNA Pico  
Data Path: C:\...Eukaryote Total RNA Pico\_DE72902486\_2016-12-12\_17-40-14.xad

Created: 12/12/2016 5:40:14 PM  
Modified: 12/12/2016 6:03:13 PM

**Electrophoresis File Run Summary (Chip Summary)**

Sample Name	Sample Comment	Stat Result Label	Result Color
		us	
214		✓ RIN:2	
215		✓ RIN:2	
220		✓ RIN: 1.90	
221		✓ RIN:2	
226		✓ RIN: 1.80	
227		✓ RIN: 1.90	
229		✓ RIN: 1.90	
230		✓ RIN:2	
235		✓ RIN: 1.90	
236		✓ RIN: 1.90	
242		✓ RIN:2	

**Chip Lot #****Reagent Kit Lot #****Chip Comments :**

Assay Class: Eukaryote Total RNA Pico  
Data Path: C:\...\Eukaryote Total RNA Pico\_DE72902486\_2016-12-12\_17-40-14.xad

Created: 12/12/2016 5:40:14 PM  
Modified: 12/12/2016 6:03:13 PM

## Electrophoresis Assay Details

### General Analysis Settings

Number of Available Sample and Ladder Wells (Max.) : 12

Minimum Visible Range [s] : 17

Maximum Visible Range [s] : 70

Start Analysis Time Range [s] : 18

End Analysis Time Range [s] : 69

Ladder Concentration [pg/μl] : 1000

Lower Marker Concentration [pg/μl] : 0

Upper Marker Concentration [pg/μl] : 0

Used Lower Marker for Quantitation

Standard Curve Fit is Logarithmic

Show Data Aligned to Lower Marker

### Integrator Settings

Integration Start Time [s] : 18

Integration End Time [s] : 69

Slope Threshold : 0.6

Height Threshold [FU] : 0.5

Area Threshold : 0.2

Width Threshold [s] : 0.3

Baseline Plateau [s] : 6

### Filter Settings

Filter Width [s] : 0.5

Polynomial Order : 4


### Ladder

Ladder Peak	Size
1	25
2	200
3	500
4	1000
5	2000
6	4000

Assay Class: Eukaryote Total RNA Pico  
Data Path: C:\...Eukaryote Total RNA Pico\_DE72902486\_2016-12-12\_17-40-14.xad

Created: 12/12/2016 5:40:14 PM  
Modified: 12/12/2016 6:03:13 PM

### Electropherogram Summary

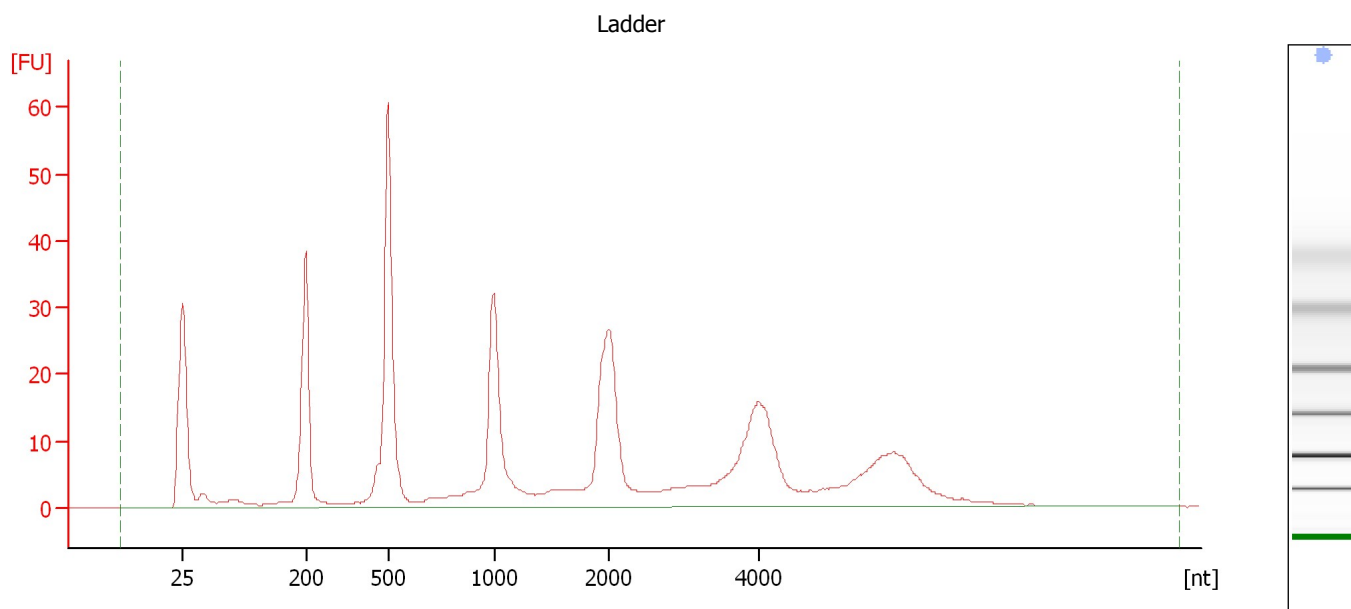

### Overall Results for Ladder

RNA Area: 467.2

Result Flagging Color:




RNA Concentration: 1,000 pg/μl

Result Flagging Label:

All Other Samples

Assay Class: Eukaryote Total RNA Pico  
Data Path: C:\...Eukaryote Total RNA Pico\_DE72902486\_2016-12-12\_17-40-14.xad

Created: 12/12/2016 5:40:14 PM  
Modified: 12/12/2016 6:03:13 PM

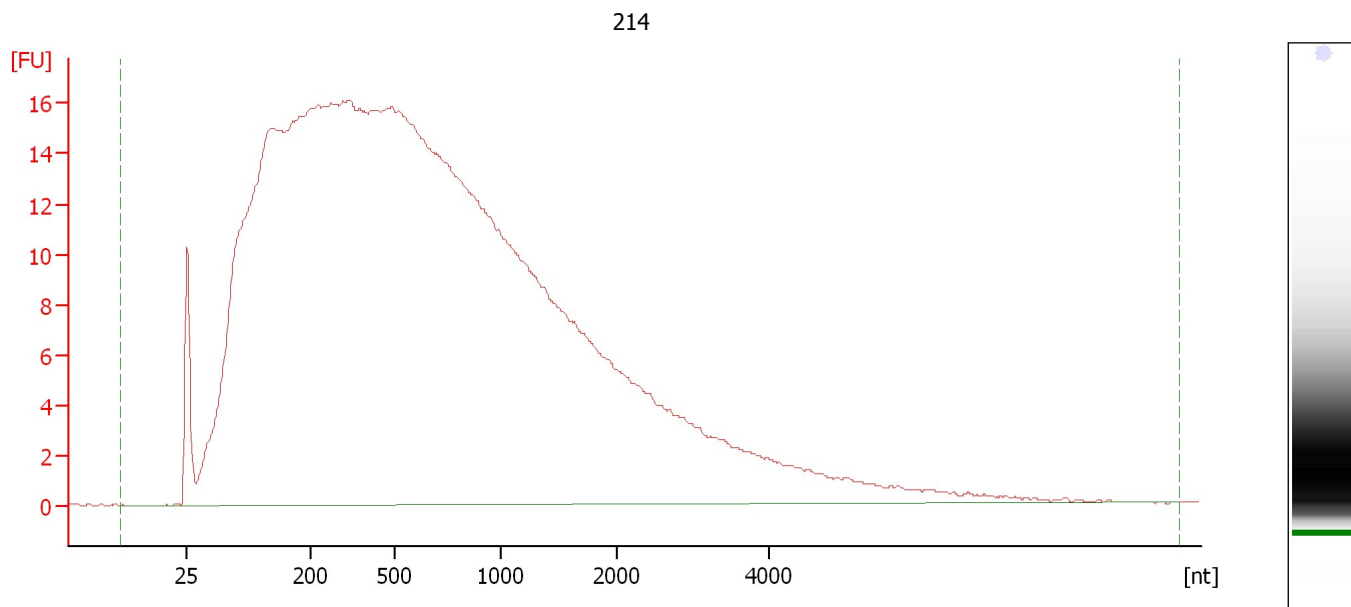
**Electropherogram Summary Continued ...****Overall Results for sample 1 : 214**

RNA Area: 792.0  
RNA Concentration: 1,695 pg/μl  
rRNA Ratio [28s / 18s]: 0.0

RNA Integrity Number (RIN): 2 (B.02.07)  
Result Flagging Color:   
Result Flagging Label: RIN:2

Assay Class: Eukaryote Total RNA Pico  
Data Path: C:\...Eukaryote Total RNA Pico\_DE72902486\_2016-12-12\_17-40-14.xad

Created: 12/12/2016 5:40:14 PM  
Modified: 12/12/2016 6:03:13 PM

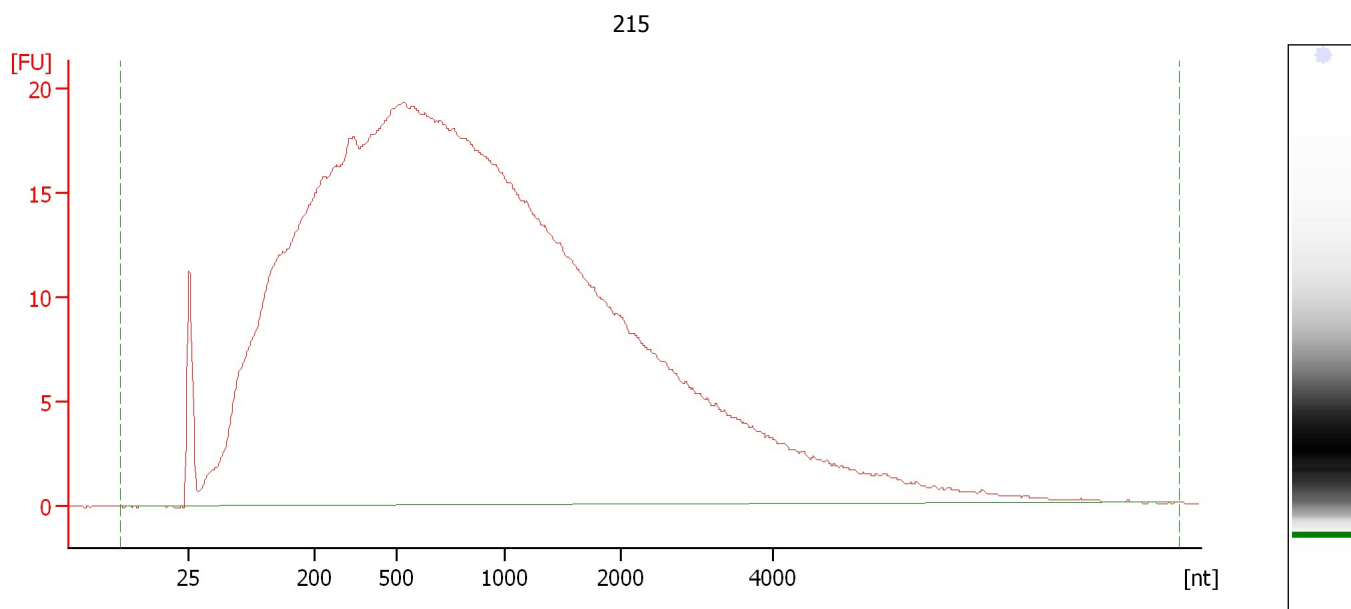
**Electropherogram Summary Continued ...****Overall Results for sample 2 : 215**

RNA Area: 924.0  
RNA Concentration: 1,978 pg/μl  
rRNA Ratio [28s / 18s]: 0.0

RNA Integrity Number (RIN): 2 (B.02.07)  
Result Flagging Color:   
Result Flagging Label: RIN:2

Assay Class: Eukaryote Total RNA Pico  
Data Path: C:\...Eukaryote Total RNA Pico\_DE72902486\_2016-12-12\_17-40-14.xad


Created: 12/12/2016 5:40:14 PM  
Modified: 12/12/2016 6:03:13 PM

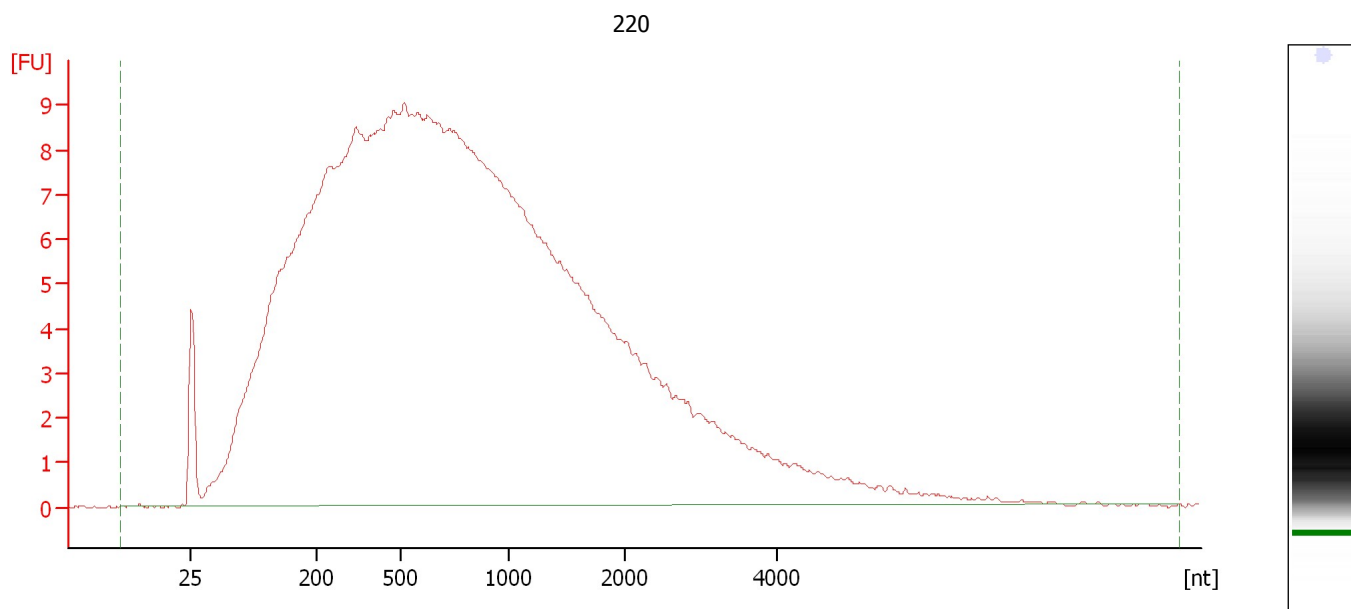**Electropherogram Summary Continued ...****Overall Results for sample 3 : 220**

RNA Area:	405.5	RNA Integrity Number (RIN):	1.9 (B.02.07)
RNA Concentration:	868 pg/μl	Result Flagging Color:	<div style="background-color: #ccccff; width: 30px; height: 15px; display: inline-block;"></div>
rRNA Ratio [28s / 18s]:	0.0	Result Flagging Label:	RIN: 1.90

Assay Class: Eukaryote Total RNA Pico  
Data Path: C:\...Eukaryote Total RNA Pico\_DE72902486\_2016-12-12\_17-40-14.xad

Created: 12/12/2016 5:40:14 PM  
Modified: 12/12/2016 6:03:13 PM

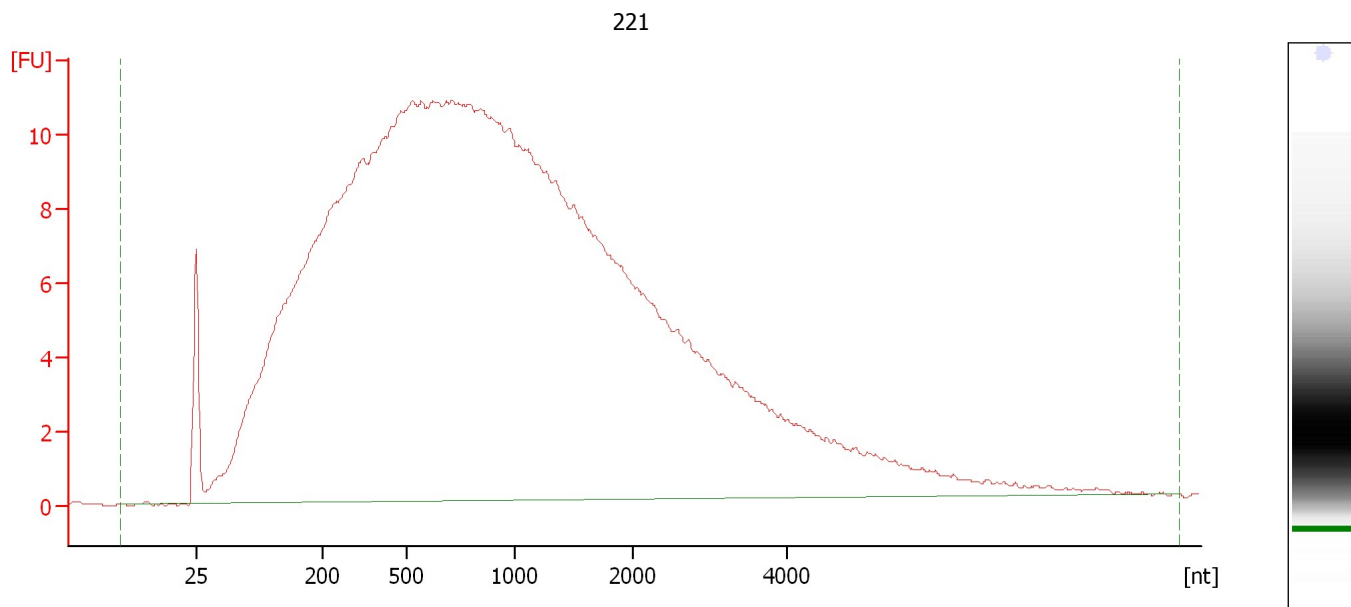**Electropherogram Summary Continued ...****Overall Results for sample 4 : 221**


RNA Area: 525.0  
RNA Concentration: 1,124 pg/μl  
rRNA Ratio [28s / 18s]: 0.0

RNA Integrity Number (RIN): 2 (B.02.07)  
Result Flagging Color:   
Result Flagging Label: RIN:2



Assay Class: Eukaryote Total RNA Pico  
Data Path: C:\...Eukaryote Total RNA Pico\_DE72902486\_2016-12-12\_17-40-14.xad


Created: 12/12/2016 5:40:14 PM  
Modified: 12/12/2016 6:03:13 PM

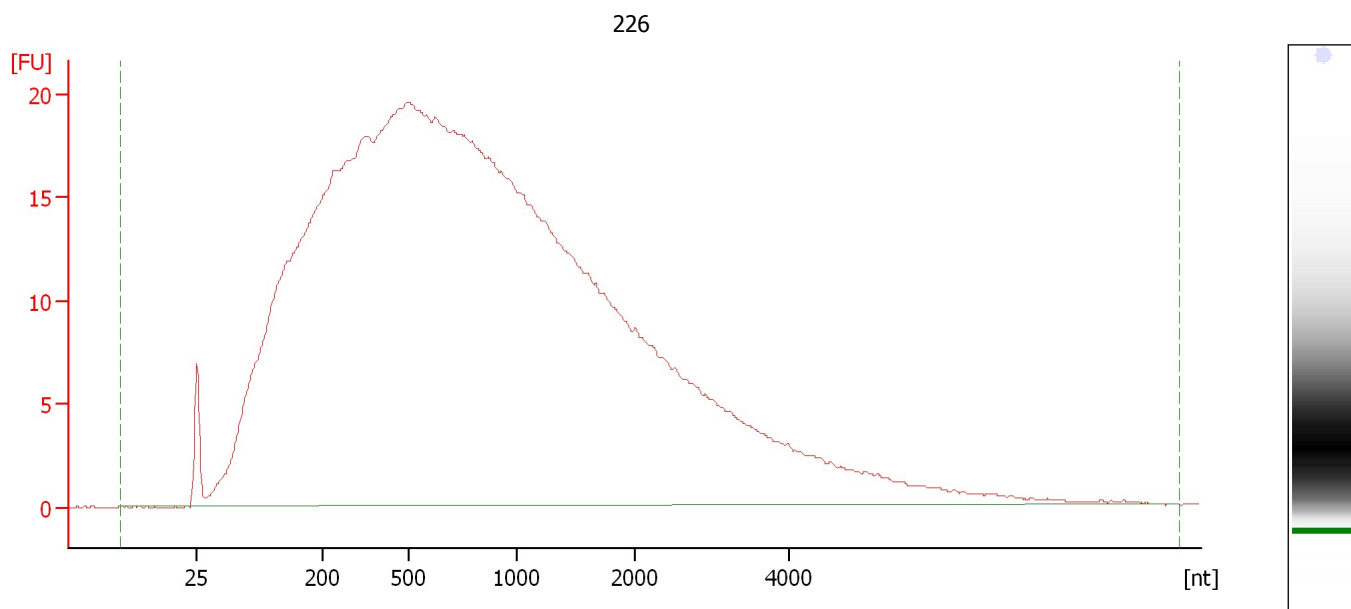**Electropherogram Summary Continued ...****Overall Results for sample 5 : 226**

RNA Area:	903.1	RNA Integrity Number (RIN):	1.8 (B.02.07)
RNA Concentration:	1,933 pg/ $\mu$ l	Result Flagging Color:	<div style="background-color: #ccccff; border: 1px solid black; width: 30px; height: 15px;"></div>
rRNA Ratio [28s / 18s]:	0.0	Result Flagging Label:	RIN: 1.80

Assay Class: Eukaryote Total RNA Pico  
Data Path: C:\...Eukaryote Total RNA Pico\_DE72902486\_2016-12-12\_17-40-14.xad

Created: 12/12/2016 5:40:14 PM  
Modified: 12/12/2016 6:03:13 PM

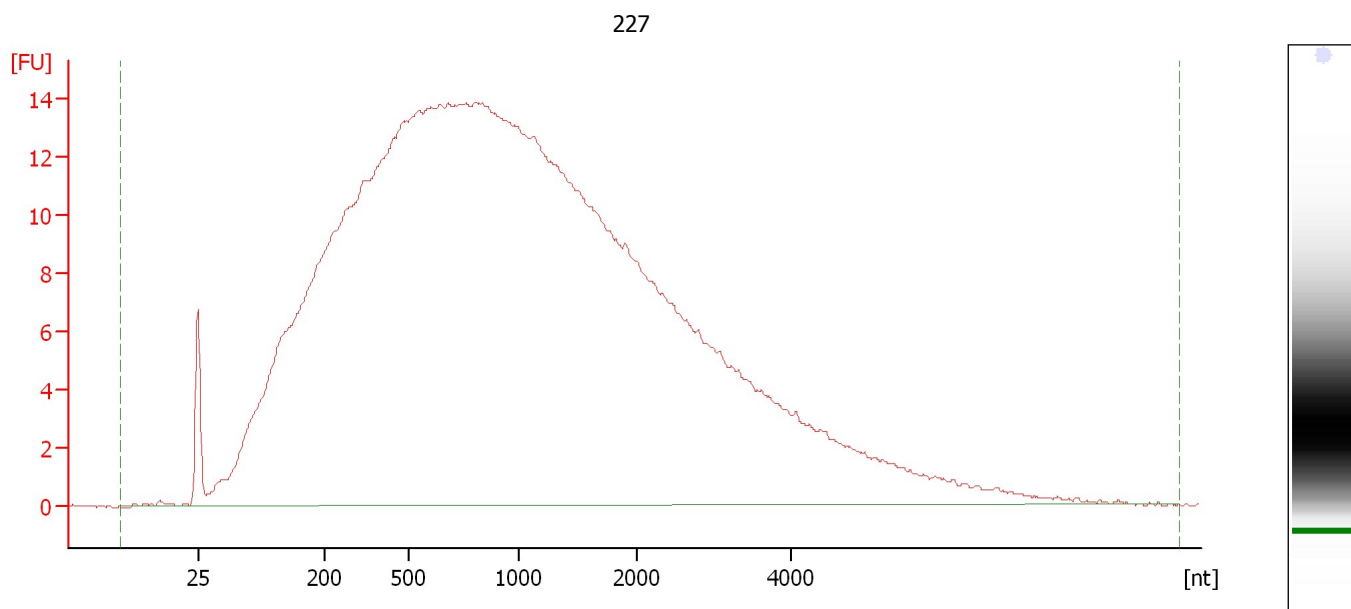
**Electropherogram Summary Continued ...****Overall Results for sample 6 : 227**

RNA Area: 684.0  
RNA Concentration: 1,464 pg/μl  
rRNA Ratio [28s / 18s]: 0.0

RNA Integrity Number (RIN): 1.9 (B.02.07)  
Result Flagging Color:   
Result Flagging Label: RIN: 1.90

Assay Class: Eukaryote Total RNA Pico  
Data Path: C:\...Eukaryote Total RNA Pico\_DE72902486\_2016-12-12\_17-40-14.xad


Created: 12/12/2016 5:40:14 PM  
Modified: 12/12/2016 6:03:13 PM

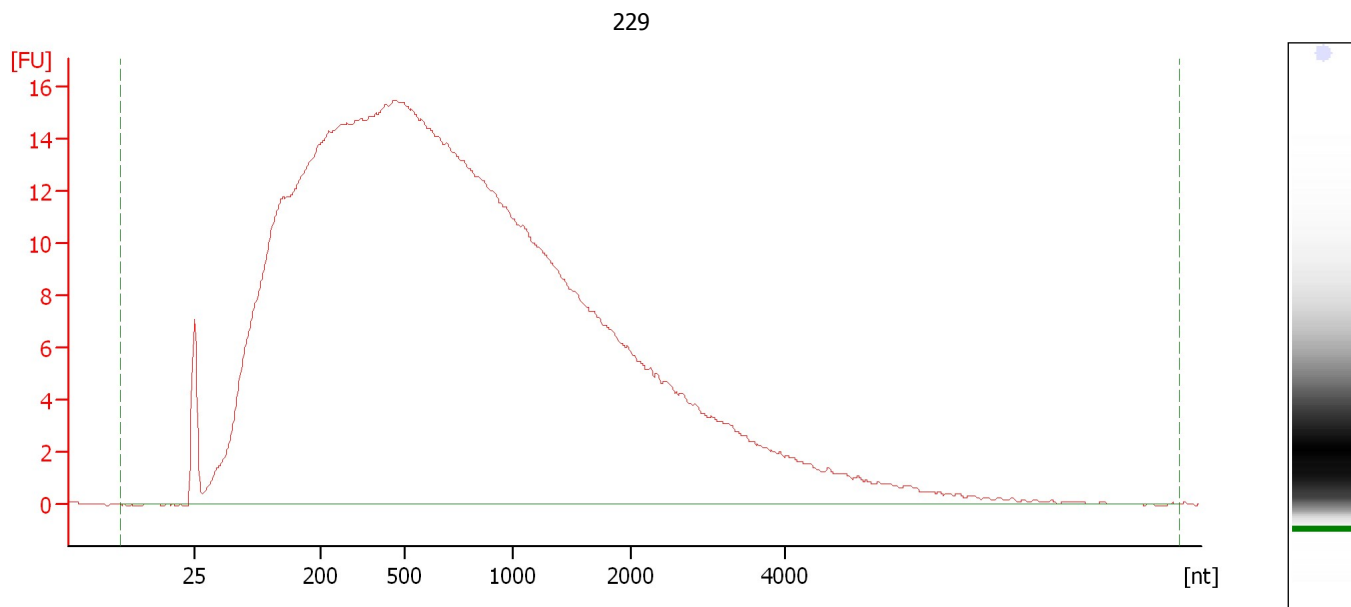**Electropherogram Summary Continued ...****Overall Results for sample 7 : 229**

RNA Area:	725.6	RNA Integrity Number (RIN):	1.9 (B.02.07)
RNA Concentration:	1,553 pg/μl	Result Flagging Color:	<span style="background-color: #ccccff; border: 1px solid black; display: inline-block; width: 20px; height: 10px;"></span>
rRNA Ratio [28s / 18s]:	0.0	Result Flagging Label:	RIN: 1.90

Assay Class: Eukaryote Total RNA Pico  
Data Path: C:\...Eukaryote Total RNA Pico\_DE72902486\_2016-12-12\_17-40-14.xad


Created: 12/12/2016 5:40:14 PM  
Modified: 12/12/2016 6:03:13 PM

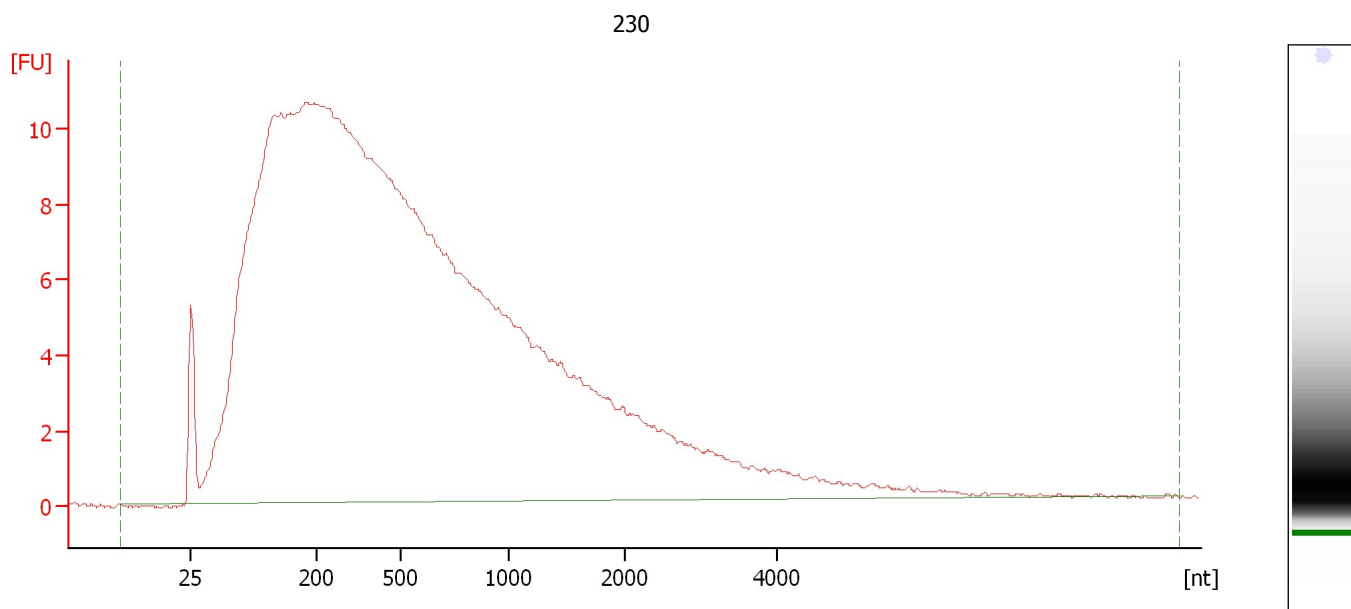**Electropherogram Summary Continued ...****Overall Results for sample 8 : 230**

RNA Area:	435.4	RNA Integrity Number (RIN):	2 (B.02.07)
RNA Concentration:	932 pg/μl	Result Flagging Color:	<div style="background-color: #ccccff; width: 30px; height: 15px; display: inline-block;"></div>
rRNA Ratio [28s / 18s]:	0.0	Result Flagging Label:	RIN:2

Assay Class: Eukaryote Total RNA Pico  
Data Path: C:\...Eukaryote Total RNA Pico\_DE72902486\_2016-12-12\_17-40-14.xad

Created: 12/12/2016 5:40:14 PM  
Modified: 12/12/2016 6:03:13 PM

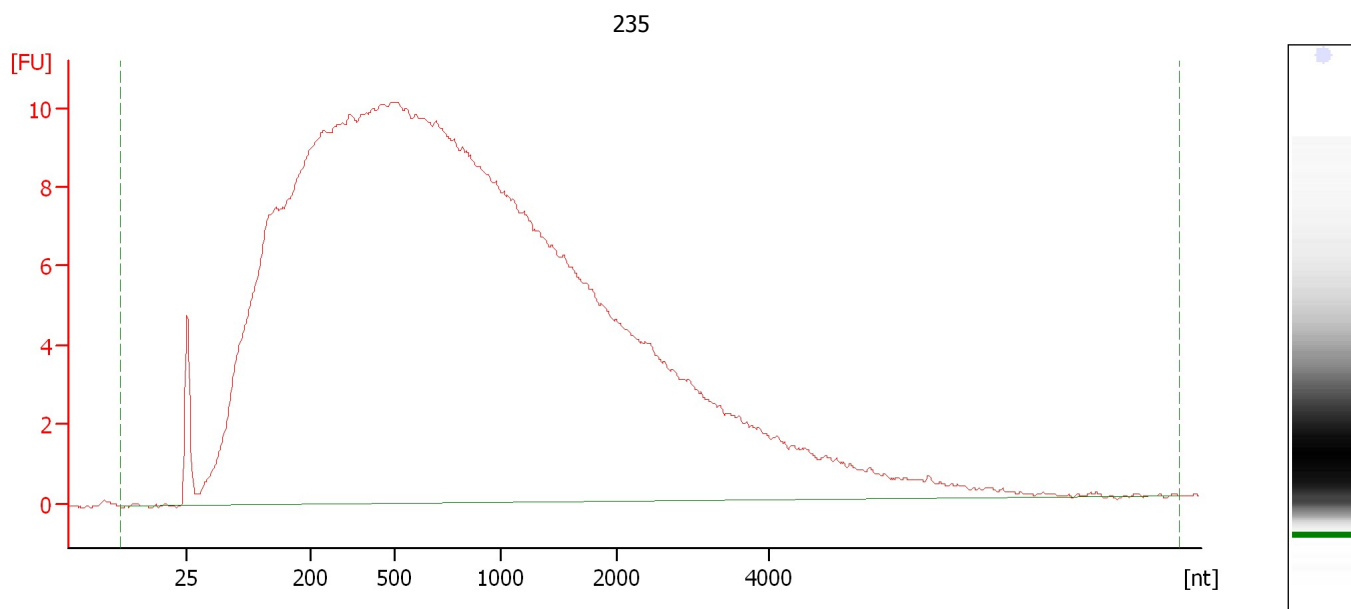
**Electropherogram Summary Continued ...****Overall Results for sample 9 : 235**

RNA Area: 502.4  
RNA Concentration: 1,075 pg/μl  
rRNA Ratio [28s / 18s]: 0.0

RNA Integrity Number (RIN): 1.9 (B.02.07)  
Result Flagging Color:   
Result Flagging Label: RIN: 1.90

Assay Class: Eukaryote Total RNA Pico  
Data Path: C:\...Eukaryote Total RNA Pico\_DE72902486\_2016-12-12\_17-40-14.xad


Created: 12/12/2016 5:40:14 PM  
Modified: 12/12/2016 6:03:13 PM

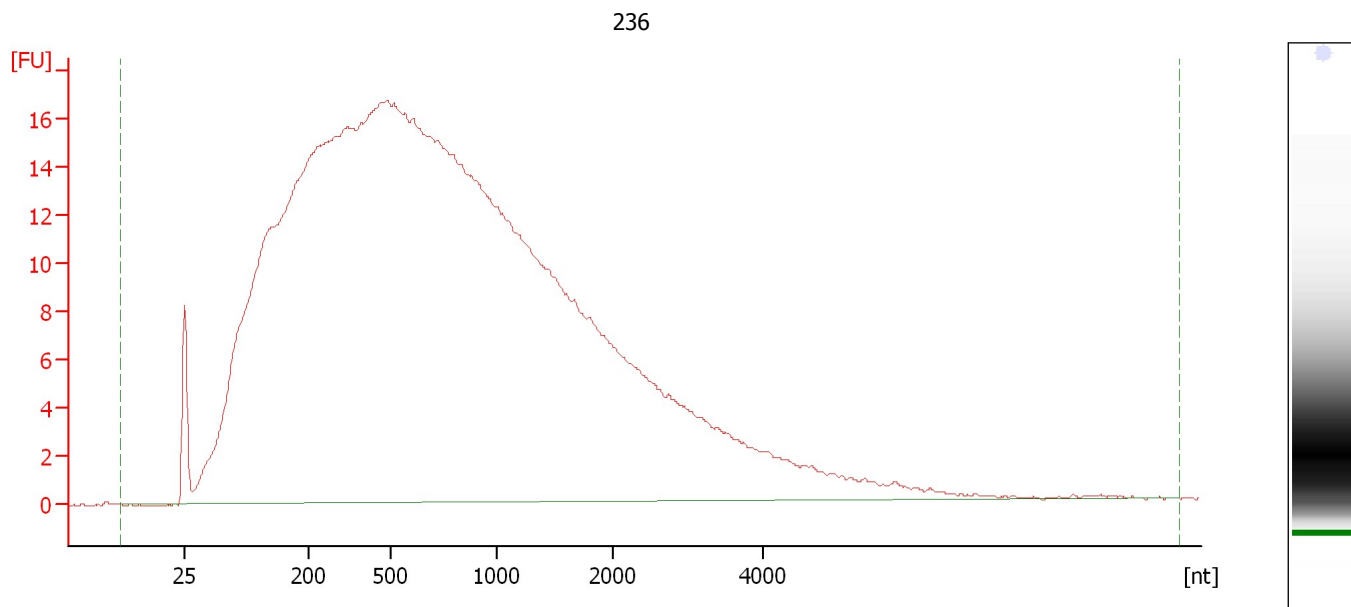**Electropherogram Summary Continued ...****Overall Results for sample 10 : 236**

RNA Area:	773.1	RNA Integrity Number (RIN):	1.9 (B.02.07)
RNA Concentration:	1,655 pg/μl	Result Flagging Color:	<div style="background-color: #ccccff; width: 30px; height: 15px; display: inline-block;"></div>
rRNA Ratio [28s / 18s]:	0.0	Result Flagging Label:	RIN: 1.90

Assay Class: Eukaryote Total RNA Pico  
Data Path: C:\...Eukaryote Total RNA Pico\_DE72902486\_2016-12-12\_17-40-14.xad


Created: 12/12/2016 5:40:14 PM  
Modified: 12/12/2016 6:03:13 PM

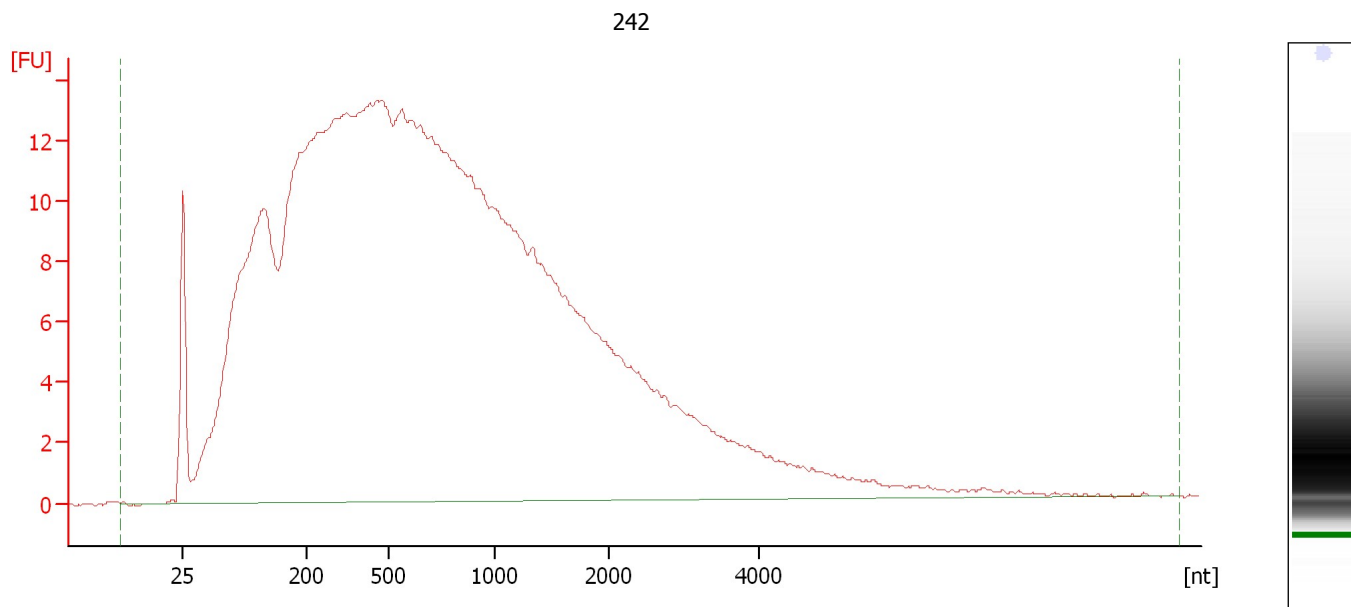**Electropherogram Summary Continued ...****Overall Results for sample 11 : 242**

RNA Area:	629.9	RNA Integrity Number (RIN):	2 (B.02.07)
RNA Concentration:	1,348 pg/μl	Result Flagging Color:	<div style="background-color: #ccccff; width: 30px; height: 15px; display: inline-block;"></div>
rRNA Ratio [28s / 18s]:	0.0	Result Flagging Label:	RIN:2

Assay Class: Eukaryote Total RNA Pico  
Data Path: C:\...Eukaryote Total RNA Pico\_DE72902486\_2016-12-12\_17-40-14.xad

Created: 12/12/2016 5:40:14 PM  
Modified: 12/12/2016 6:03:13 PM

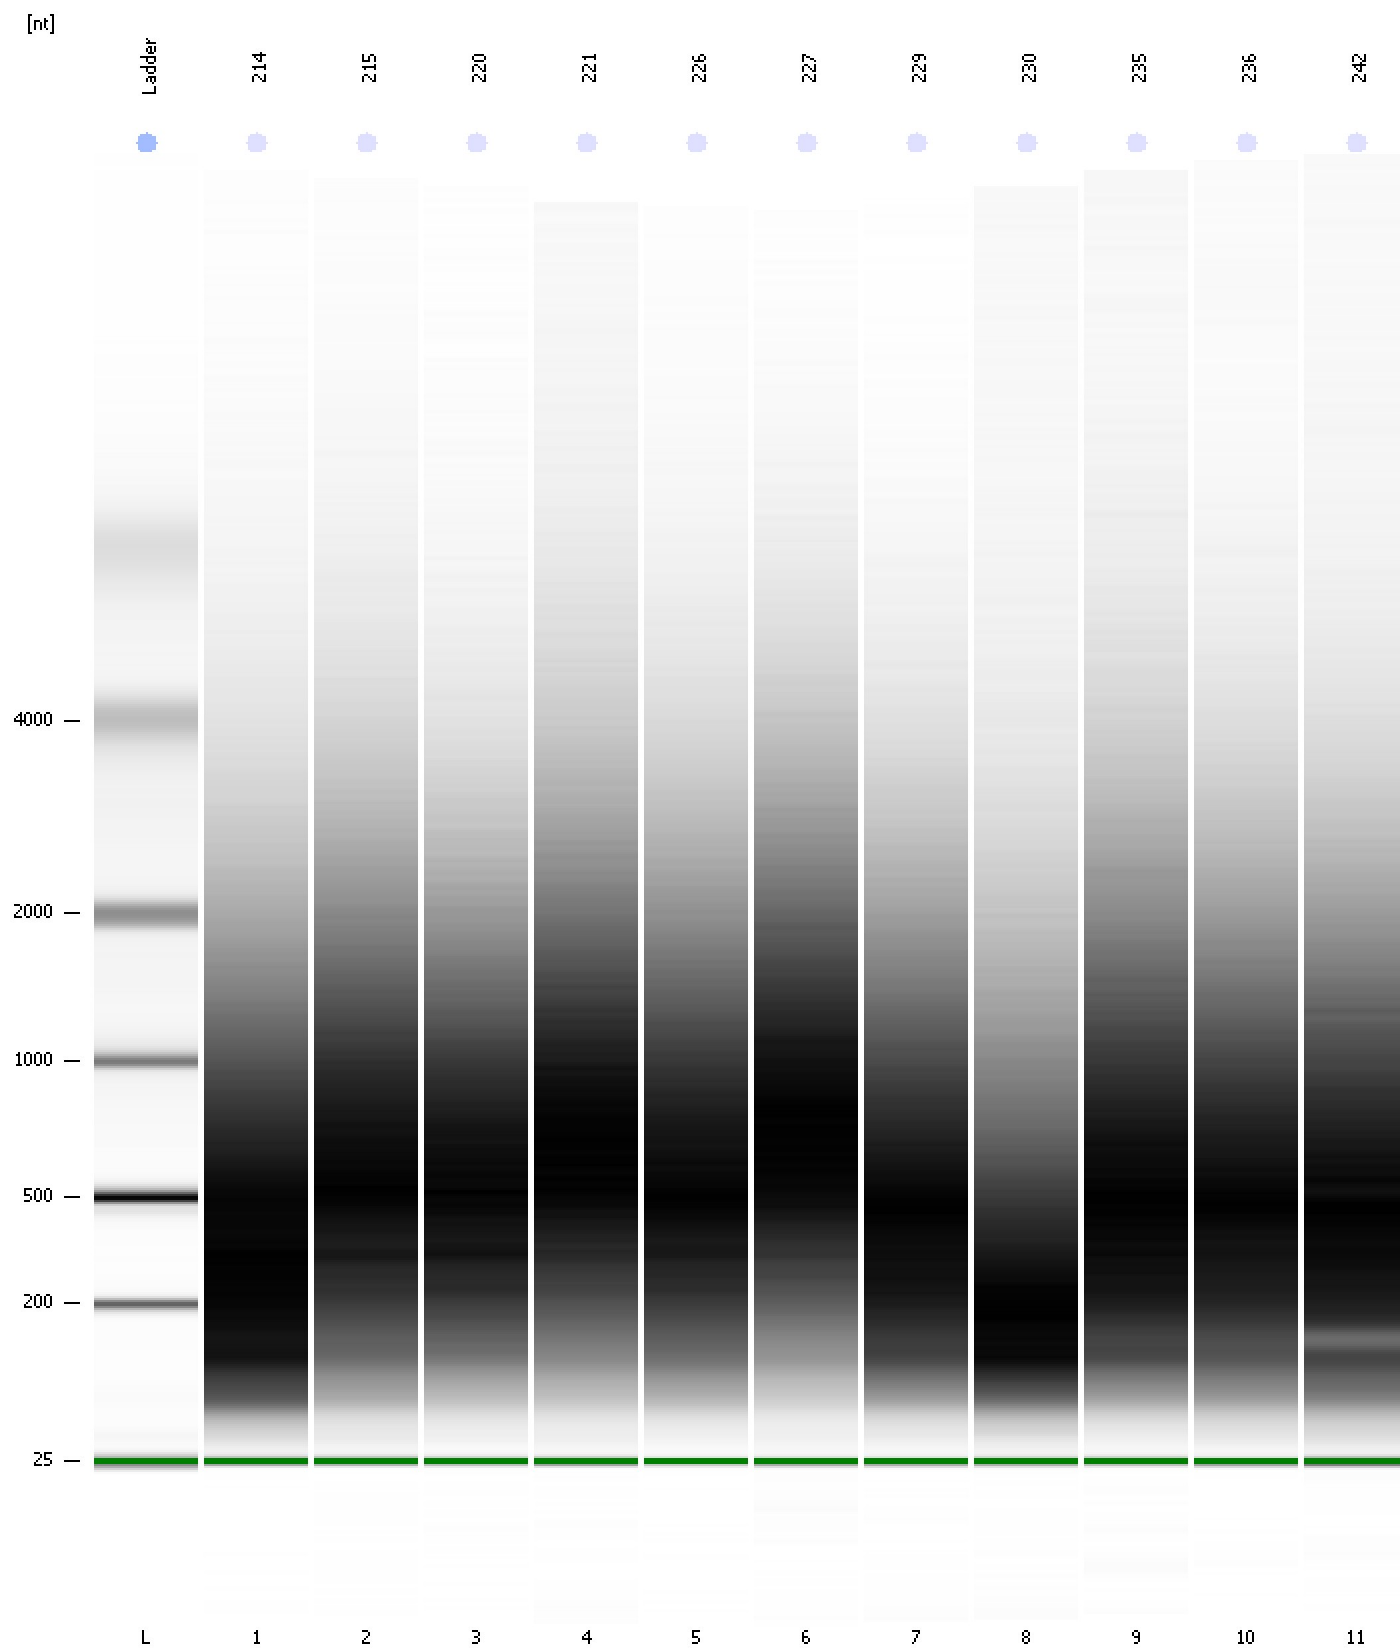**Gel Image**




Assay Class: Eukaryote Total RNA Pico  
Data Path: C:\...Eukaryote Total RNA Pico\_DE72902486\_2016-12-12\_17-40-14.xad

Created: 12/12/2016 5:40:14 PM  
Modified: 12/12/2016 6:03:13 PM

## Curves

### Standard Curve

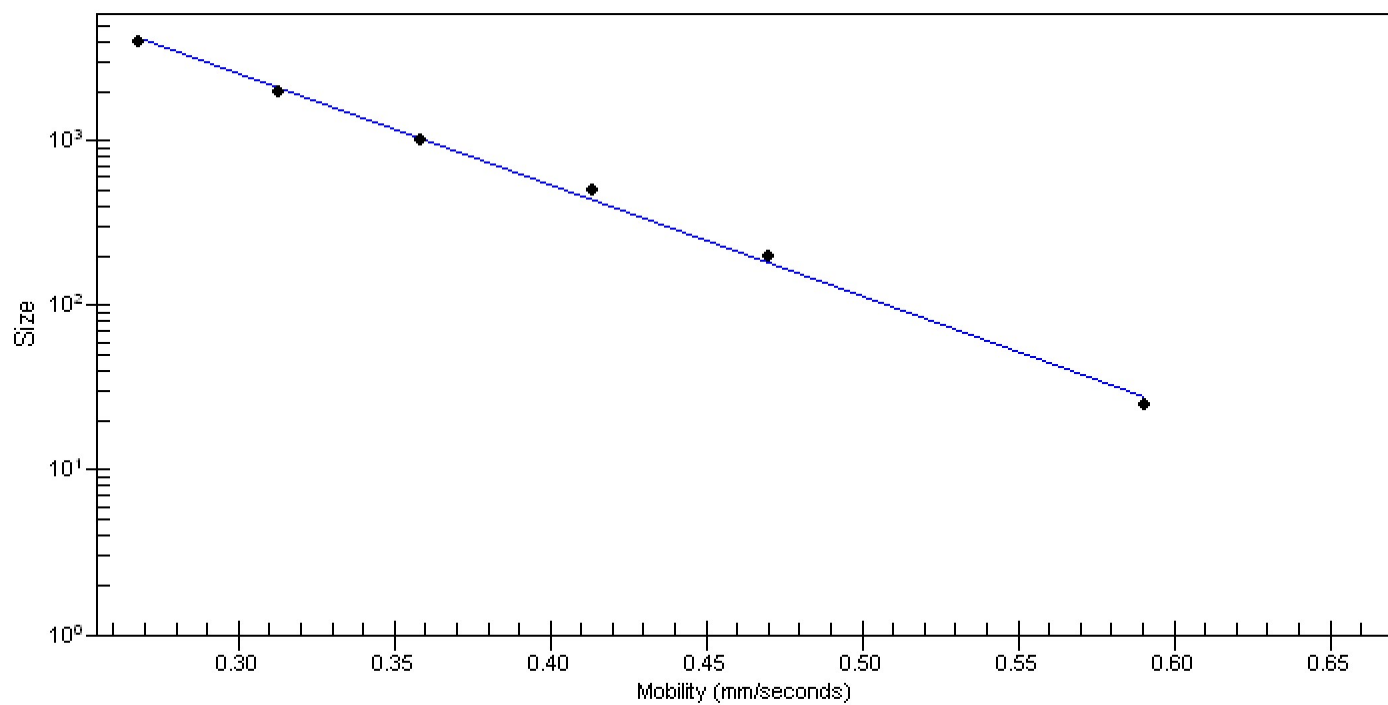

Assay Class: Eukaryote Total RNA Pico  
 Data Path: C:\...Eukaryote Total RNA Pico\_DE72902486\_2016-12-12\_17-40-14.xad

Created: 12/12/2016 5:40:14 PM  
 Modified: 12/12/2016 6:03:13 PM

**Run Logbook**

Description	Number	Source	Category	Sub Category	Time Stamp	Time Zone	User	Host
Run ended on port 1 (Number of wells acquired: 12)		Instrument	Run		12/12/2016 6:03:08 PM	(GMT --08:00) Pacific Standard Time	Administrator	DATASYSTEM01
Run started on port 1 (File: C:\Program Files\Agilent\2100 bioanalyzer\2100 expert\Data\2016-12-12\2100 expert_Eukaryote Total RNA Pico_DE72902486_2016-12-12_17-40-14.xad)		Instrument	Run		12/12/2016 5:40:20 PM	(GMT --08:00) Pacific Standard Time	Administrator	DATASYSTEM01
Product Number : G2939A		Instrument	Run		12/12/2016 5:40:20 PM	(GMT --08:00) Pacific Standard Time	Administrator	DATASYSTEM01
Name :		Instrument	Run		12/12/2016 5:40:20 PM	(GMT --08:00) Pacific Standard Time	Administrator	DATASYSTEM01
Vendor : Agilent Technologies		Instrument	Run		12/12/2016 5:40:20 PM	(GMT --08:00) Pacific Standard Time	Administrator	DATASYSTEM01
Serial# : DE72902486		Instrument	Run		12/12/2016 5:40:20 PM	(GMT --08:00) Pacific Standard Time	Administrator	DATASYSTEM01
Firmware : C.01.069		Instrument	Run		12/12/2016 5:40:20 PM	(GMT --08:00) Pacific Standard Time	Administrator	DATASYSTEM01
Cartridge : Electrode		Instrument	Run		12/12/2016 5:40:20 PM	(GMT --08:00) Pacific Standard Time	Administrator	DATASYSTEM01