
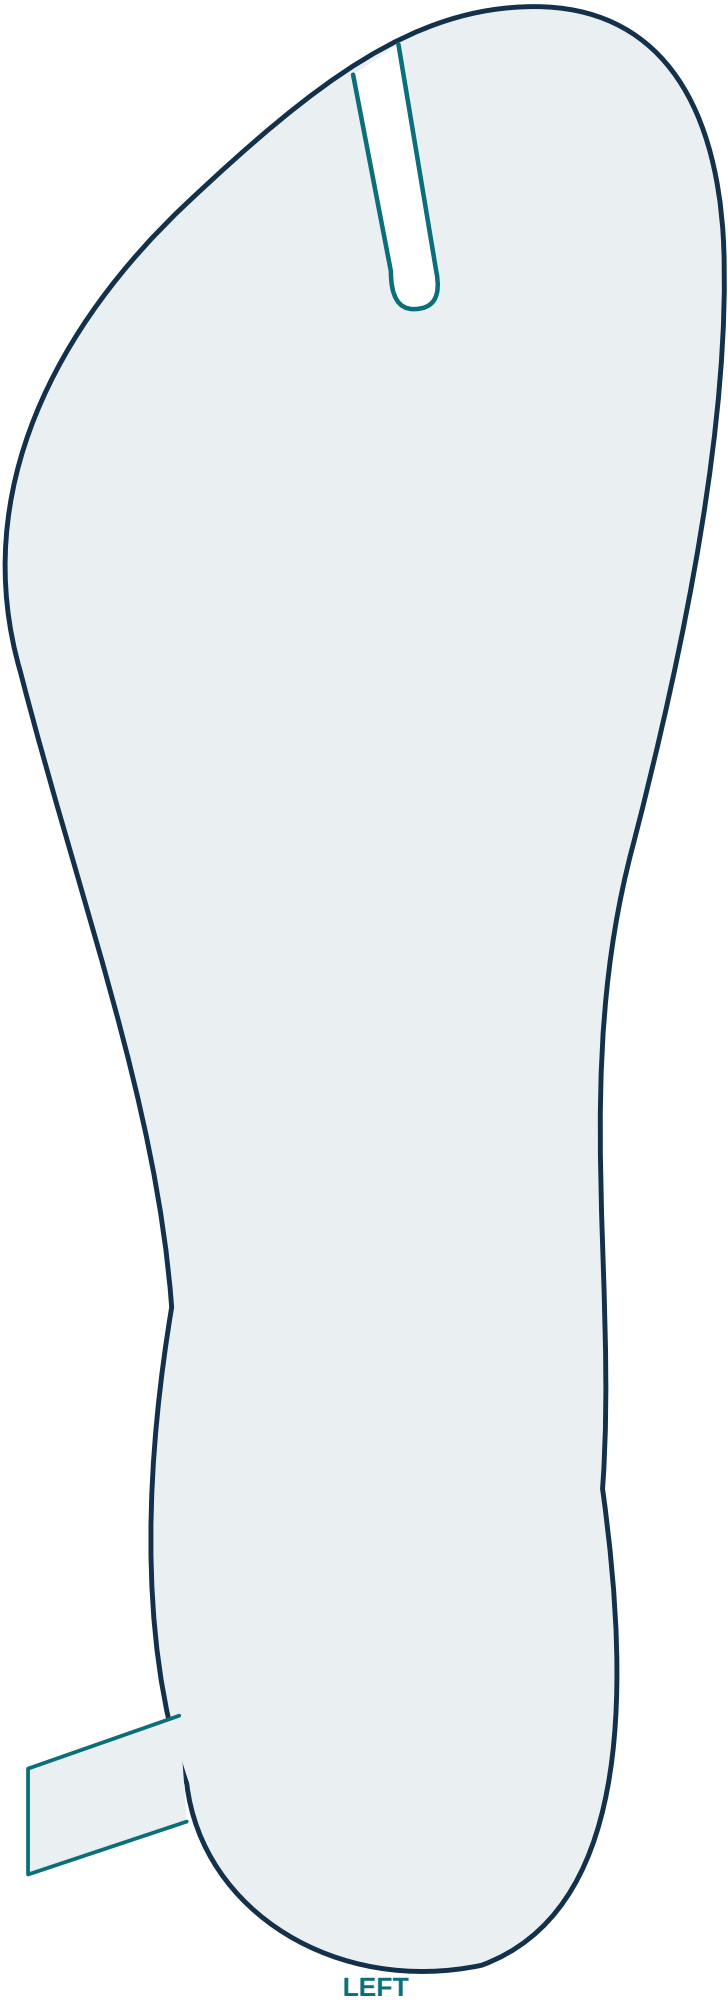


NIVA / MEDIUM FIT STUDY / 1:1

Print A3 at 100%. Measure the 100 mm check bar before use. Proposed outline; do not fabricate sensors from this file.

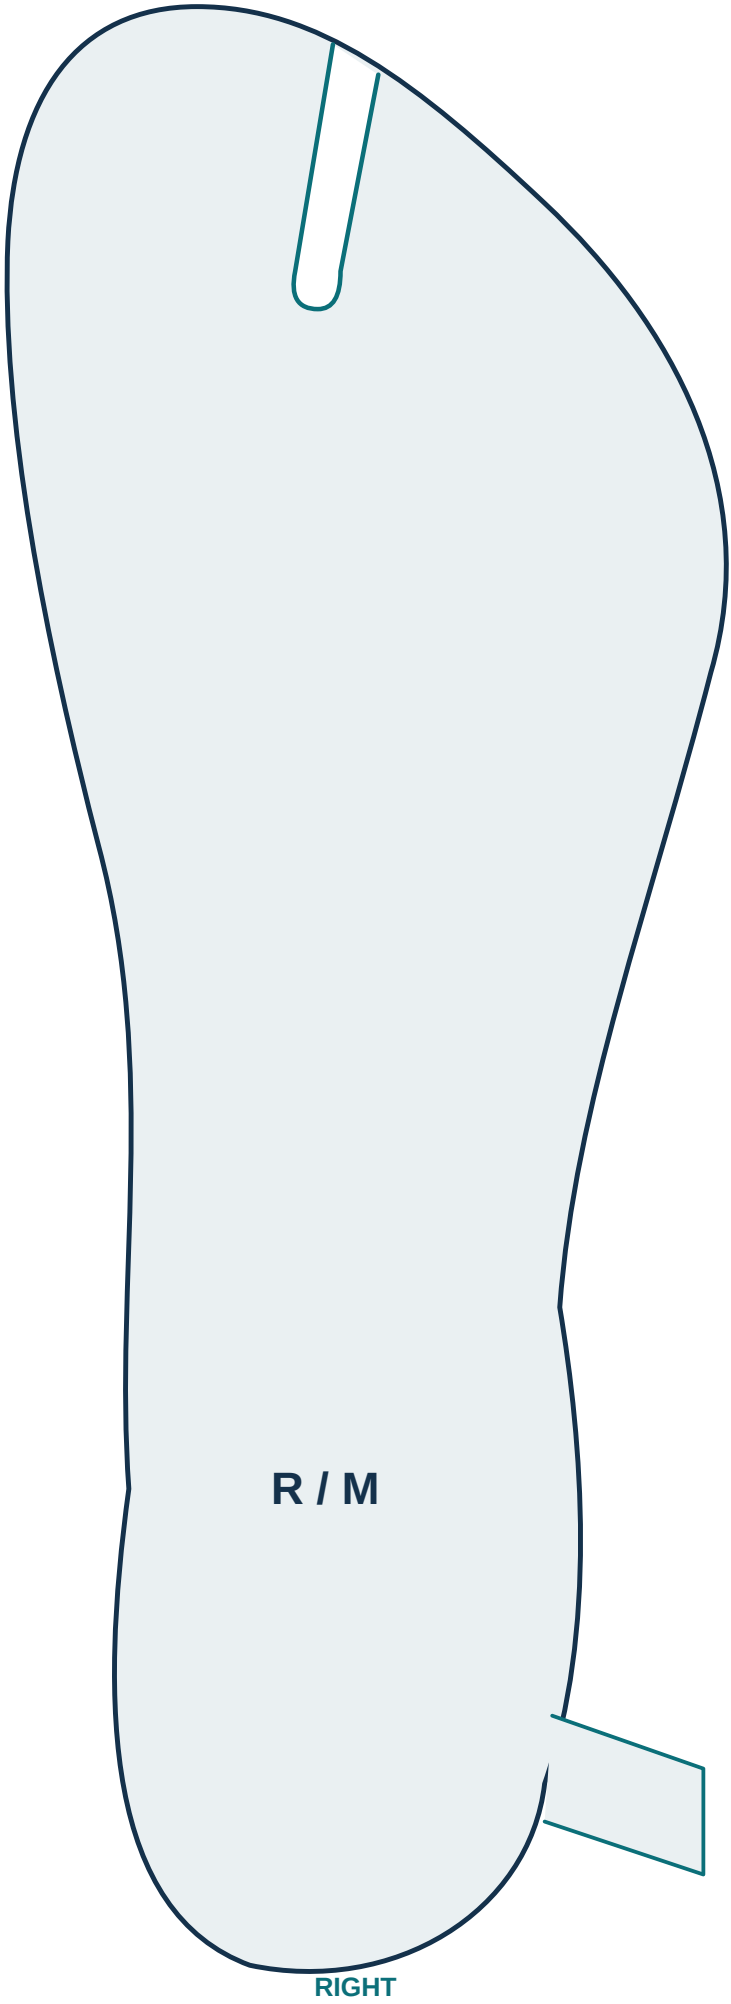

260 x 96 P

Foot outline only. Confirm heel, metatarsal heads, toe-web position and soft tissue clearance on measured users. This is not an approved size standard.

NO AUTOMATIC GRADING

Small and large outlines need anatomical fitting. Do not uniformly scale the sensor map and assume alignment.

