


Assay Class: High Sensitivity DNA Assay
Data Path: C:\...gh Sensitivity DNA Assay_DE13804677_2024-05-03_14-35-58.xad

Created: 5/3/2024 2:35:57 PM
Modified: 5/3/2024 3:19:48 PM

Electrophoresis File Run Summary

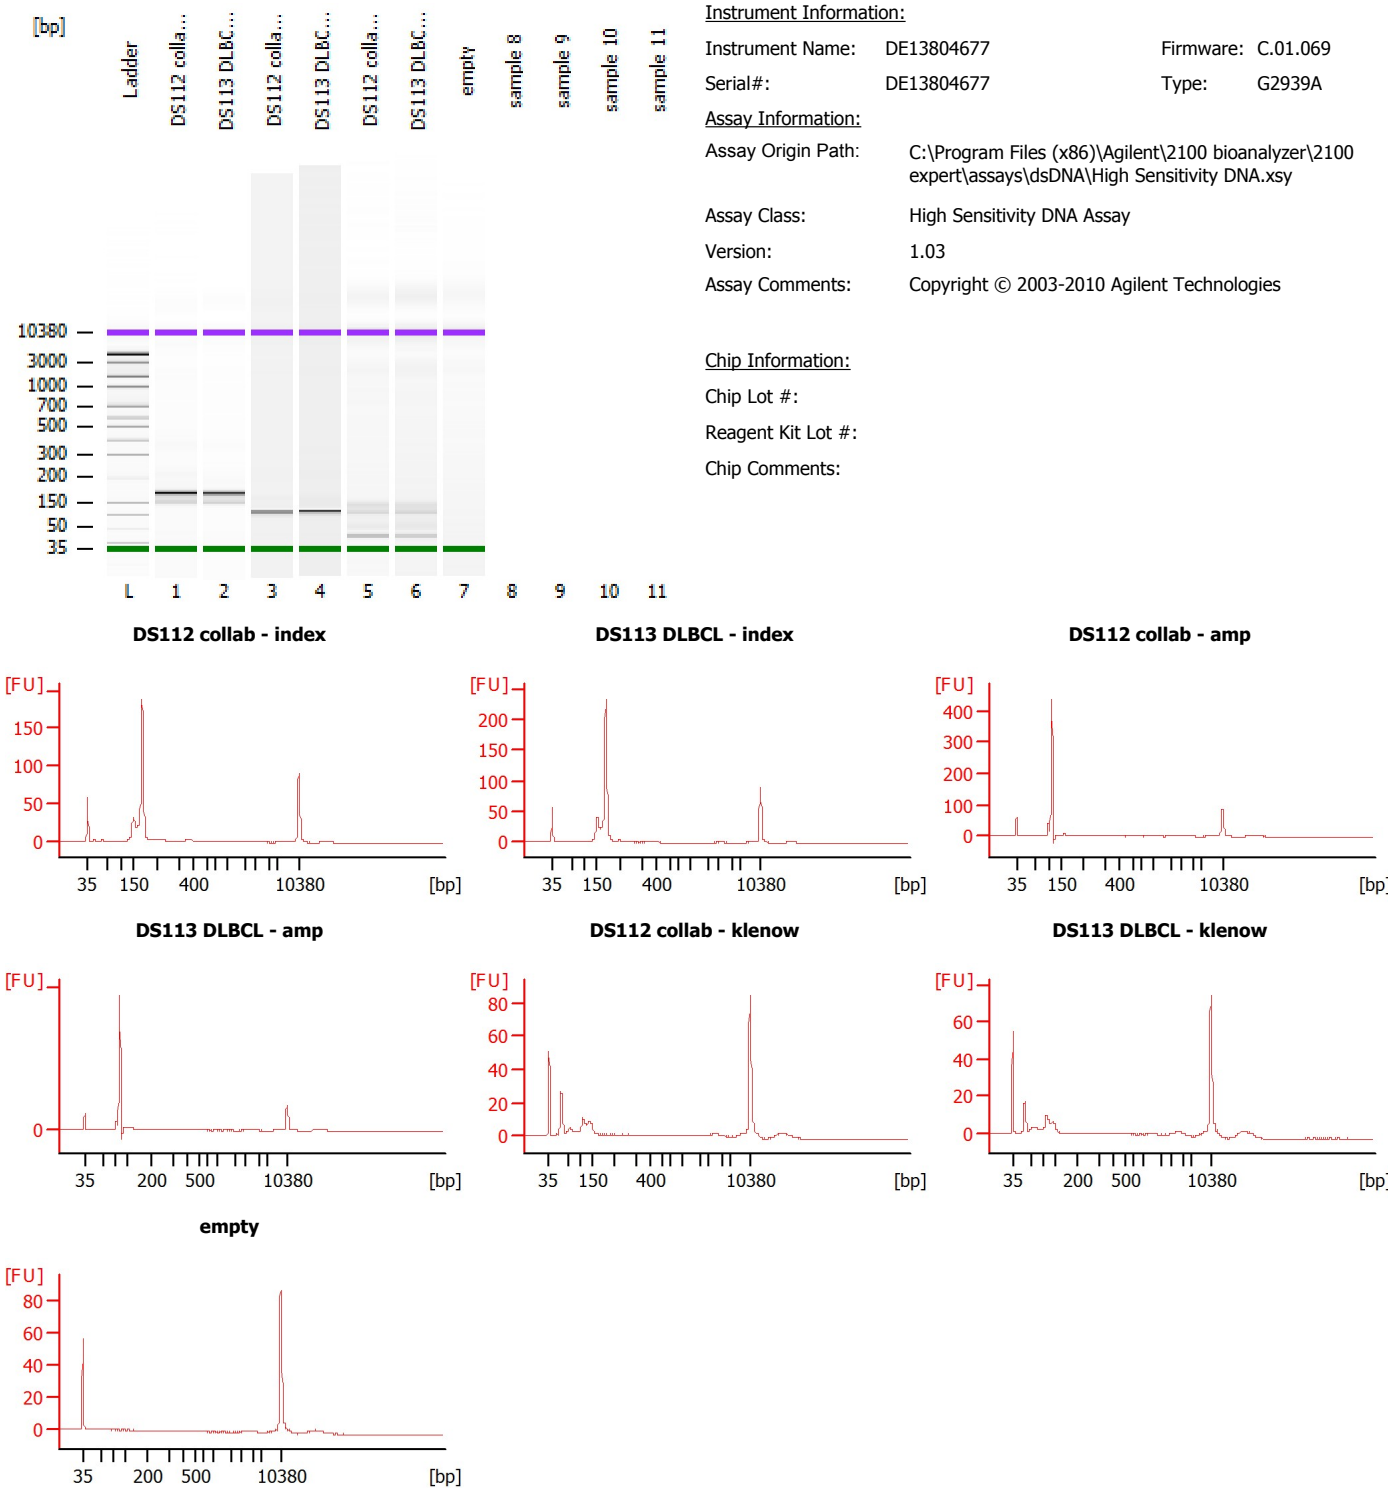

Assay Class: High Sensitivity DNA Assay
Data Path: C:\...gh Sensitivity DNA Assay_DE13804677_2024-05-03_14-35-58.xad

Created: 5/3/2024 2:35:57 PM
Modified: 5/3/2024 3:19:48 PM

Electrophoresis File Run Summary (Chip Summary)

Sample Name	Sample Comment	Rest. Digest	Status	Observation	Result Label	Result Color
DS112 collab - index		☐	✓			
DS113 DLBCL - index		☐	✓			
DS112 collab - amp		☐	✓			
DS113 DLBCL - amp		☐	✓			
DS112 collab - klenow		☐	✓			
DS113 DLBCL - klenow		☐	✓			
empty		☐	✓			
sample 8		☐				
sample 9		☐				
sample 10		☐				
sample 11		☐				
Ladder		☐	✓			

Chip Lot #

Reagent Kit Lot #

Chip Comments :

Assay Class: High Sensitivity DNA Assay
Data Path: C:\...gh Sensitivity DNA Assay_DE13804677_2024-05-03_14-35-58.xad

Created: 5/3/2024 2:35:57 PM
Modified: 5/3/2024 3:19:48 PM

Electrophoresis Assay Details

General Analysis Settings

Number of Available Sample and Ladder Wells (Max.) : 12
Minimum Visible Range [s] : 32
Maximum Visible Range [s] : 138
Start Analysis Time Range [s] : 33
End Analysis Time Range [s] : 137.5
Ladder Concentration [pg/μl] : 1950
Uses Standard Area for Ladder Fragments
Lower Marker Concentration [pg/μl] : 125
Upper Marker Concentration [pg/μl] : 75
Used Upper Marker for Quantitation
Standard Curve Fit is Point to Point
Show Data Aligned to Lower and Upper Marker

Integrator Settings

Integration Start Time [s] : 33.05
Integration End Time [s] : 137
Slope Threshold : 0.8
Height Threshold [FU] : 5
Area Threshold : 0.1
Width Threshold [s] : 0.6
Baseline Plateau [s] : 0.5

Filter Settings

Filter Width [s] : 0.5
Polynomial Order : 4


Ladder

Ladder Peak	Size	Area
1	35	160
2	50	210
3	100	208
4	150	221
5	200	242
6	300	270
7	400	305
8	500	306
9	600	336
10	700	321
11	1000	366
12	2000	413
13	3000	411
14	7000	400
15	10380	214

Assay Class: High Sensitivity DNA Assay
Data Path: C:\...gh Sensitivity DNA Assay_DE13804677_2024-05-03_14-35-58.xad

Created: 5/3/2024 2:35:57 PM
Modified: 5/3/2024 3:19:48 PM

Electropherogram Summary

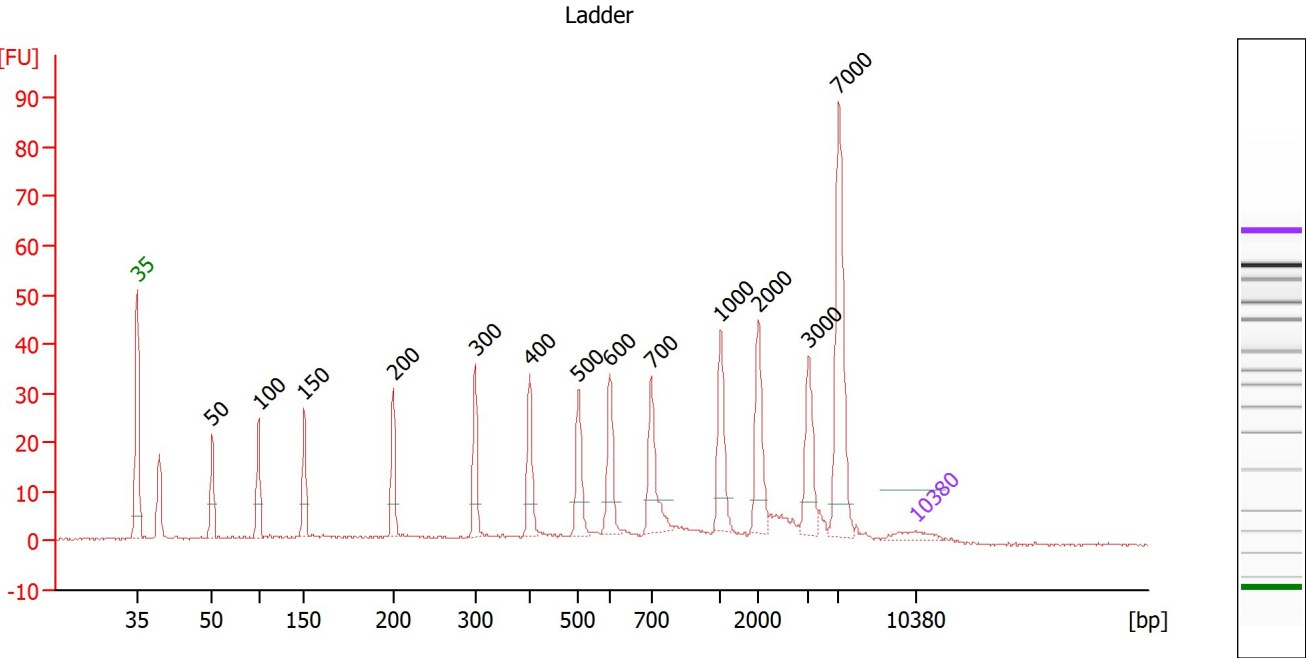

Overall Results for Ladder

Noise: 0.3


Peak table for Ladder

Peak		Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	◀	35	125.00	5,411.3	Lower Marker
2	└	50	150.00	4,545.5	Ladder Peak
3	└	100	150.00	2,272.7	Ladder Peak
4	└	150	150.00	1,515.2	Ladder Peak
5	└	200	150.00	1,136.4	Ladder Peak
6	└	300	150.00	757.6	Ladder Peak
7	└	400	150.00	568.2	Ladder Peak
8	└	500	150.00	454.5	Ladder Peak
9	└	600	150.00	378.8	Ladder Peak
10	└	700	150.00	324.7	Ladder Peak
11	└	1,000	150.00	227.3	Ladder Peak
12	└	2,000	150.00	113.6	Ladder Peak
13	└	3,000	150.00	75.8	Ladder Peak
14	└	7,000	150.00	32.5	Ladder Peak
15	▶	10,380	75.00	10.9	Upper Marker

Assay Class: High Sensitivity DNA Assay
Data Path: C:\...gh Sensitivity DNA Assay_DE13804677_2024-05-03_14-35-58.xad

Created: 5/3/2024 2:35:57 PM
Modified: 5/3/2024 3:19:48 PM

Electropherogram Summary Continued ...

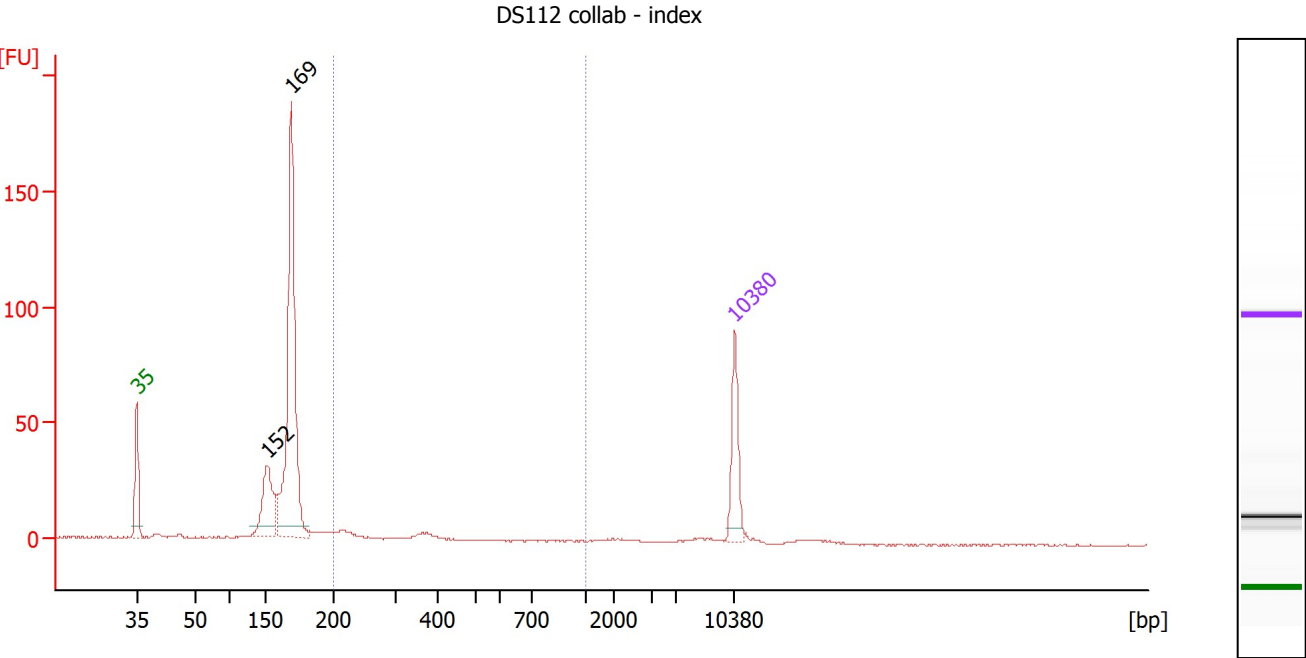

Overall Results for sample 1 : DS112 collab - index

Number of peaks found: 2

Corr. Area 1: 28.7

Noise: 0.3

Peak table for sample 1 : DS112 collab - index

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	35	125.00	5,411.3	Lower Marker
2	152	151.40	1,512.9	
3	169	567.29	5,084.3	
4	10,380	75.00	10.9	Upper Marker


Region table for sample 1 : DS112 collab - index

From [bp]	To [bp]	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Color
200	1,000	28.7	7	311	37.6	48.87	271.0	

Assay Class: High Sensitivity DNA Assay
Data Path: C:\...gh Sensitivity DNA Assay_DE13804677_2024-05-03_14-35-58.xad

Created: 5/3/2024 2:35:57 PM
Modified: 5/3/2024 3:19:48 PM

Electropherogram Summary Continued ...

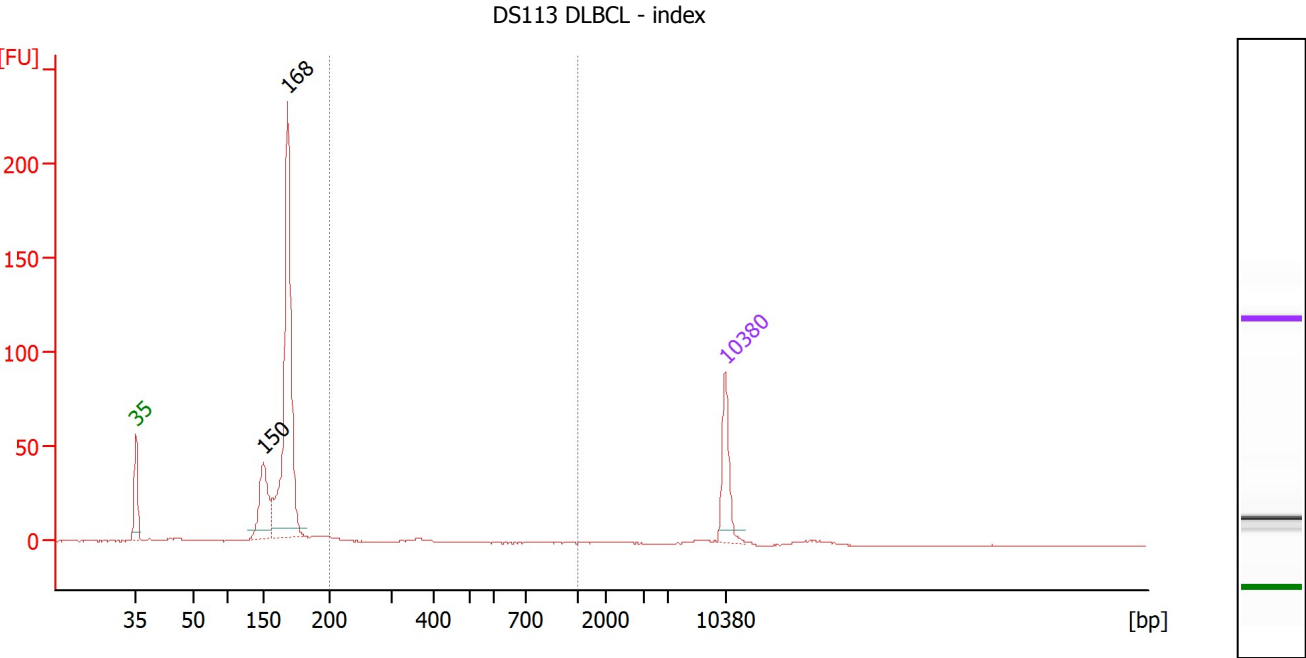

Overall Results for sample 2 : DS113 DLBCL - index

Number of peaks found: 2

Corr. Area 1: 19.0

Noise: 0.3

Peak table for sample 2 : DS113 DLBCL - index

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	35	125.00	5,411.3	Lower Marker
2	150	153.64	1,552.3	
3	168	660.86	5,944.5	
4	10,380	75.00	10.9	Upper Marker


Region table for sample 2 : DS113 DLBCL - index

From [bp]	To [bp]	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Color
200	1,000	19.0	4	372	50.1	30.17	154.5	

Assay Class: High Sensitivity DNA Assay
Data Path: C:\...gh Sensitivity DNA Assay_DE13804677_2024-05-03_14-35-58.xad

Created: 5/3/2024 2:35:57 PM
Modified: 5/3/2024 3:19:48 PM

Electropherogram Summary Continued ...

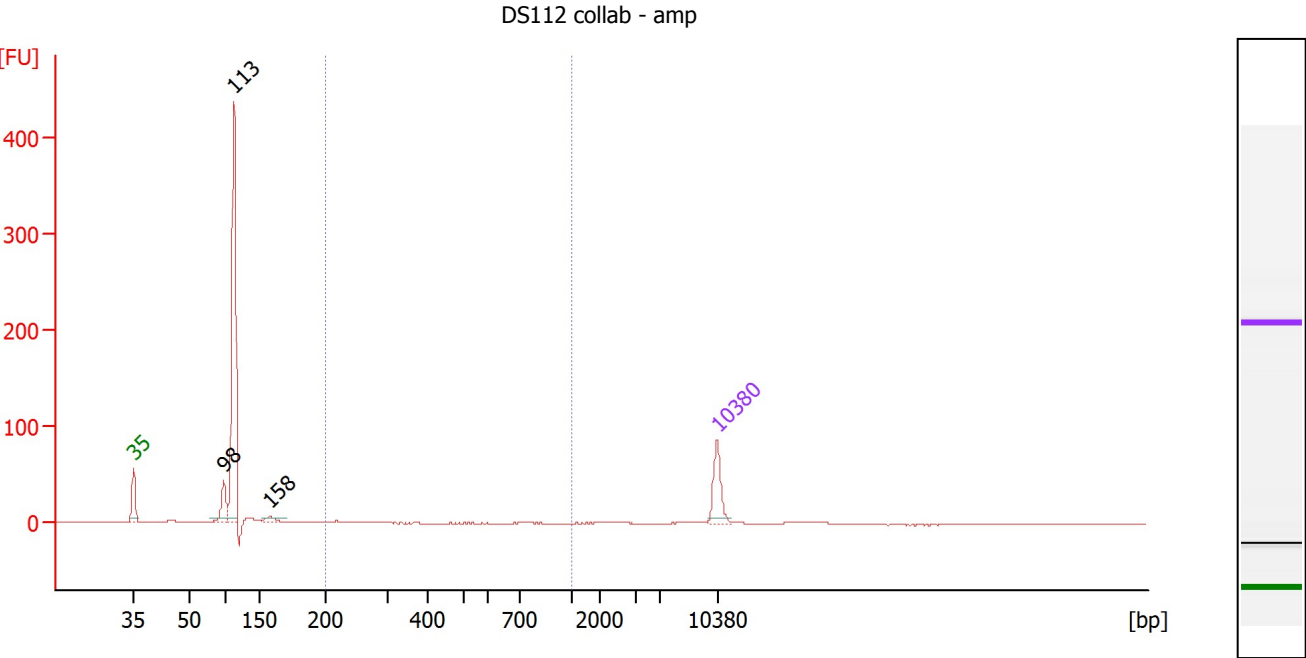

Overall Results for sample 3 : DS112 collab - amp

Number of peaks found: 3

Corr. Area 1: 17.7

Noise: 0.3

Peak table for sample 3 : DS112 collab - amp

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	35	125.00	5,411.3	Lower Marker
2	98	97.51	1,501.3	
3	113	824.50	11,014.6	
4	158	27.22	260.6	
5	10,380	75.00	10.9	Upper Marker


Region table for sample 3 : DS112 collab - amp

From [bp]	To [bp]	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Color
200	1,000	17.7	3	430	56.9	26.46	134.7	

Assay Class: High Sensitivity DNA Assay
Data Path: C:\...gh Sensitivity DNA Assay_DE13804677_2024-05-03_14-35-58.xad

Created: 5/3/2024 2:35:57 PM
Modified: 5/3/2024 3:19:48 PM

Electropherogram Summary Continued ...

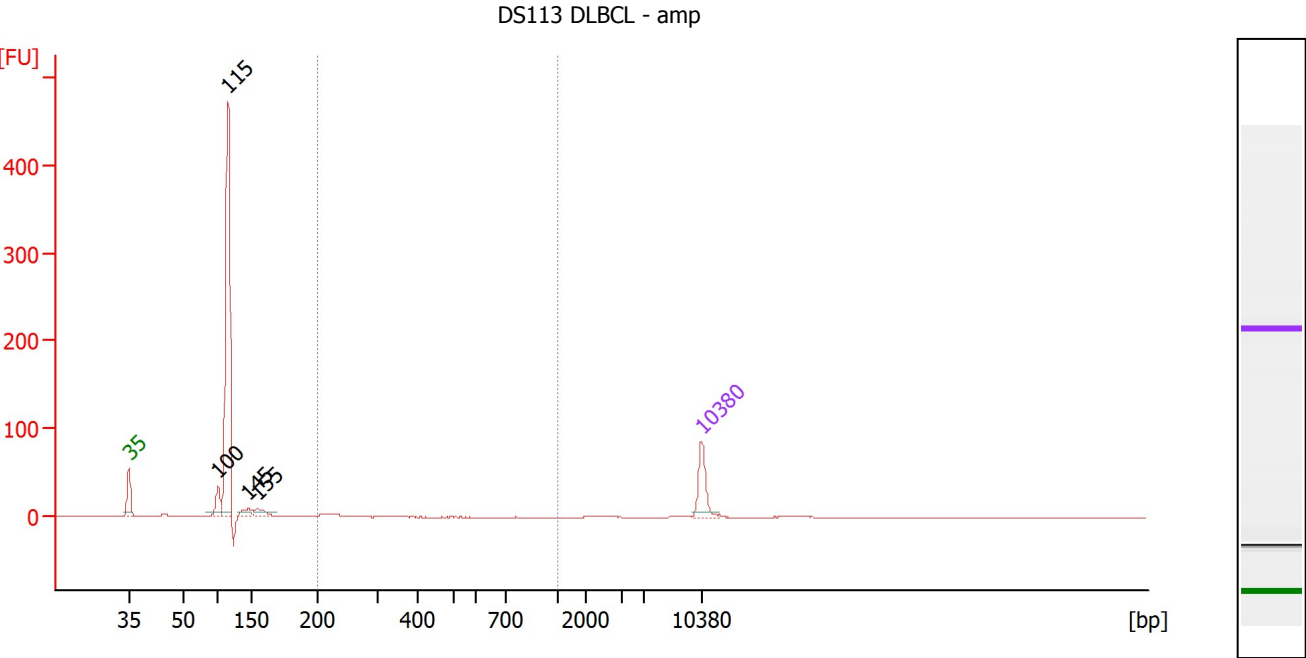

Overall Results for sample 4 : DS113 DLBCL - amp

Number of peaks found: 4

Corr. Area 1: 29.3

Noise: 0.3

Peak table for sample 4 : DS113 DLBCL - amp

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	35	125.00	5,411.3	Lower Marker
2	100	74.07	1,121.0	
3	115	873.33	11,540.8	
4	145	31.99	335.4	
5	155	39.10	383.0	
6	10,380	75.00	10.9	Upper Marker


Region table for sample 4 : DS113 DLBCL - amp

From [bp]	To [bp]	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Color
200	1,000	29.3	5	376	55.2	43.47	232.2	

Assay Class: High Sensitivity DNA Assay
Data Path: C:\...gh Sensitivity DNA Assay_DE13804677_2024-05-03_14-35-58.xad

Created: 5/3/2024 2:35:57 PM
Modified: 5/3/2024 3:19:48 PM

Electropherogram Summary Continued ...

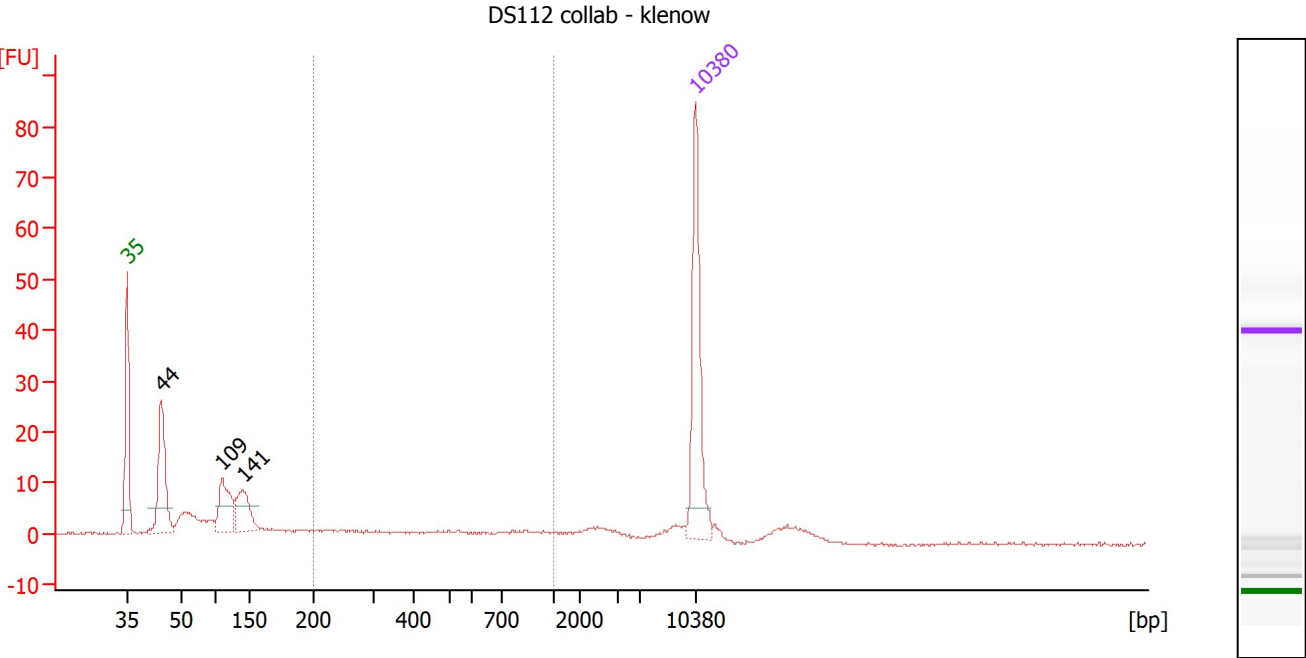

Overall Results for sample 5 : DS112 collab - klenow

Number of peaks found: 3

Corr. Area 1: 42.2

Noise: 0.3

Peak table for sample 5 : DS112 collab - klenow

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	35	125.00	5,411.3	Lower Marker
2	44	103.34	3,537.9	
3	109	53.28	742.0	
4	141	45.36	486.8	
5	10,380	75.00	10.9	Upper Marker


Region table for sample 5 : DS112 collab - klenow

From [bp]	To [bp]	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Color
200	1,000	42.2	17	517	45.3	59.40	235.8	

Assay Class: High Sensitivity DNA Assay
Data Path: C:\...gh Sensitivity DNA Assay_DE13804677_2024-05-03_14-35-58.xad

Created: 5/3/2024 2:35:57 PM
Modified: 5/3/2024 3:19:48 PM

Electropherogram Summary Continued ...

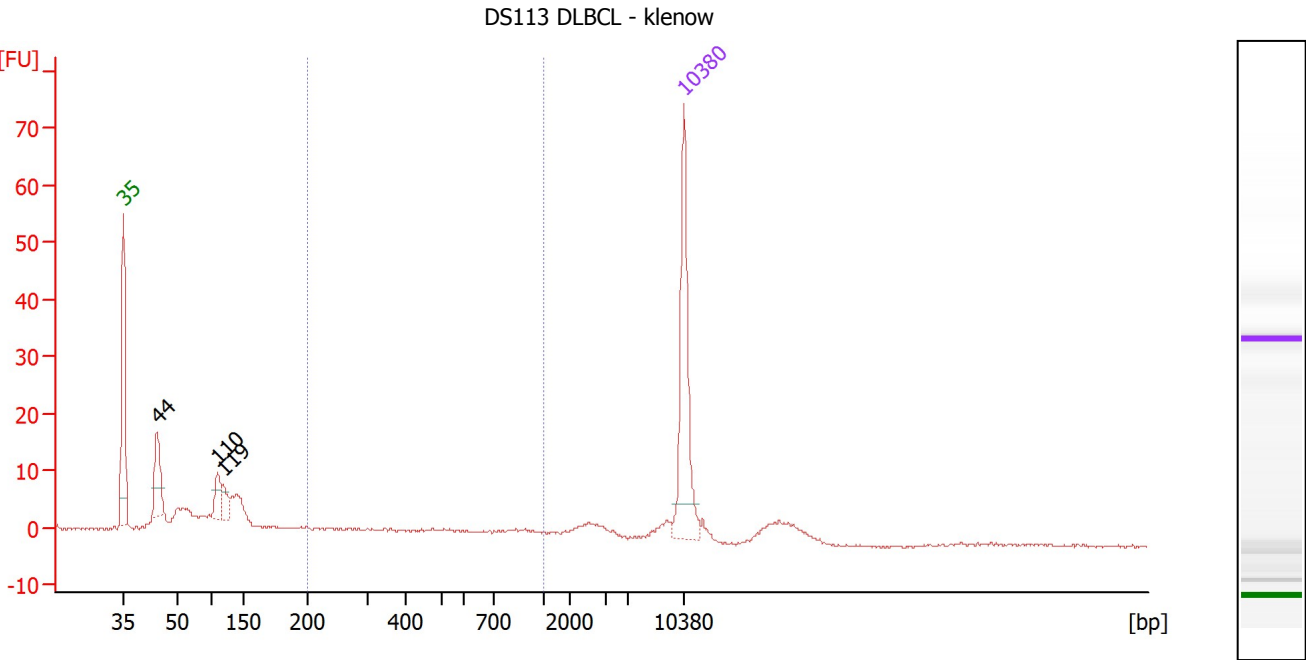

Overall Results for sample 6 : DS113 DLBCL - klenow

Number of peaks found: 3
Noise: 0.3

Corr. Area 1: 23.4

Peak table for sample 6 : DS113 DLBCL - klenow

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	35	125.00	5,411.3	Lower Marker
2	44	48.01	1,644.2	
3	110	24.21	333.6	
4	119	15.17	193.8	Upper Marker
5	10,380	75.00	10.9	


Region table for sample 6 : DS113 DLBCL - klenow

From [bp]	To [bp]	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Color
200	1,000	23.4	14	518	45.1	36.30	143.2	Blue

Assay Class: High Sensitivity DNA Assay
Data Path: C:\...gh Sensitivity DNA Assay_DE13804677_2024-05-03_14-35-58.xad

Created: 5/3/2024 2:35:57 PM
Modified: 5/3/2024 3:19:48 PM

Electropherogram Summary Continued ...

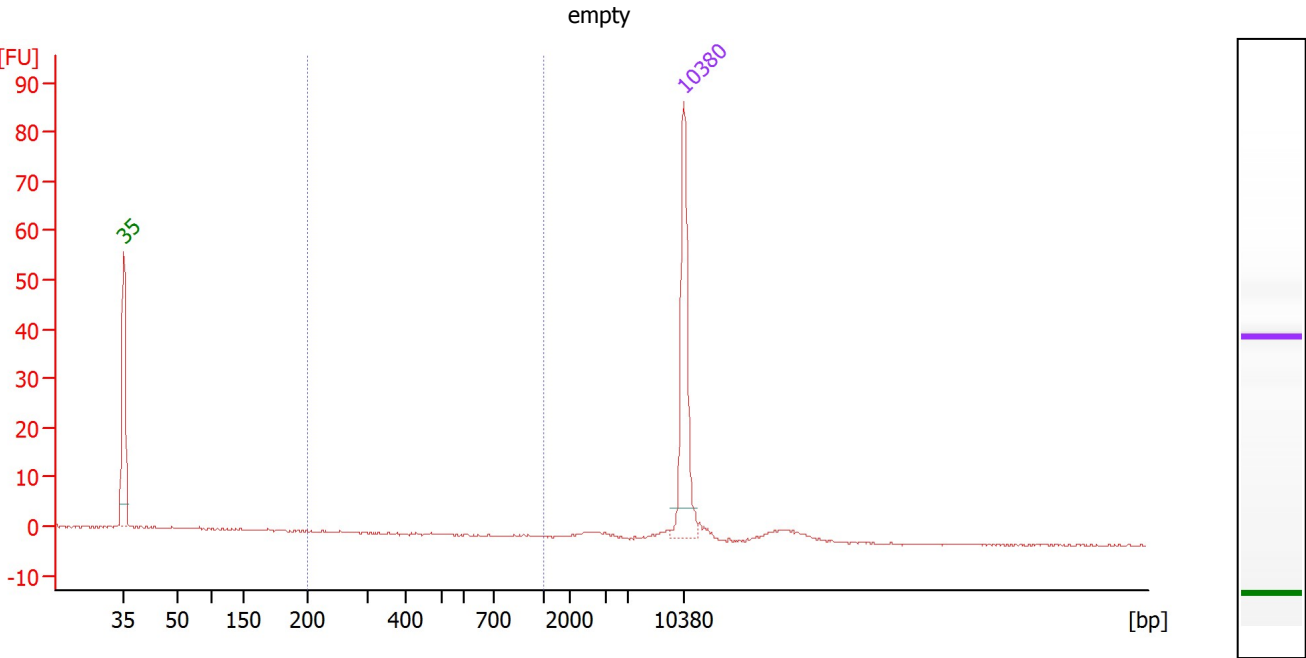

Overall Results for sample 7 : empty

Number of peaks found: 0
Noise: 0.2

Corr. Area 1: 0.1

Peak table for sample 7 : empty

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	35	125.00	5,411.3	Lower Marker
2	10,380	75.00	10.9	Upper Marker

Region table for sample 7 : empty

From [bp]	To [bp]	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Color
200	1,000	0.1	1	286	30.3	0.18	1.0	Blue


Assay Class: High Sensitivity DNA Assay

Data Path: C:\...gh Sensitivity DNA Assay_DE13804677_2024-05-03_14-35-58.xad

Created: 5/3/2024 2:35:57 PM

Modified: 5/3/2024 3:19:48 PM

Gel Image

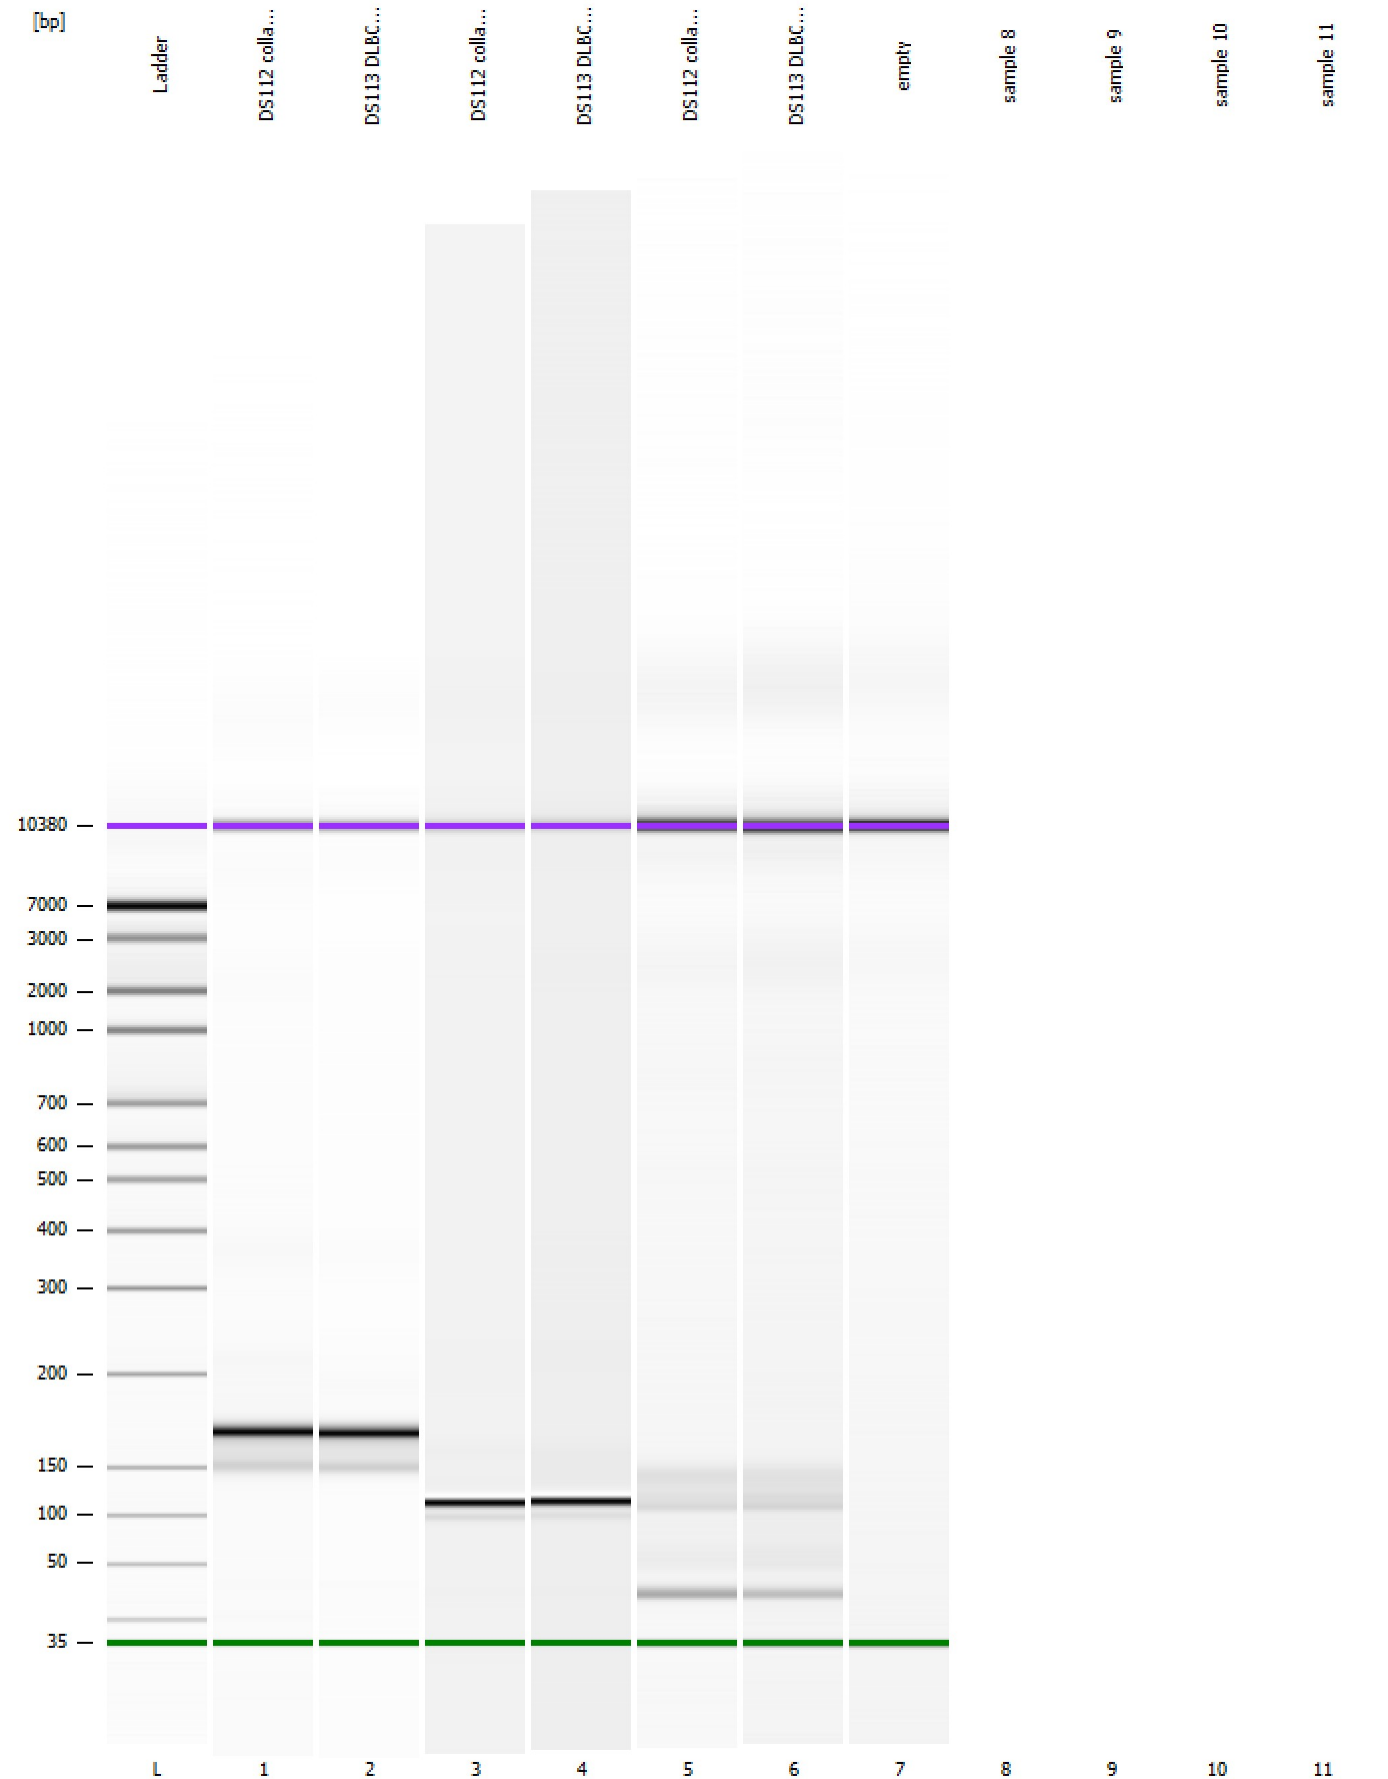


Assay Class: High Sensitivity DNA Assay
Data Path: C:\...gh Sensitivity DNA Assay_DE13804677_2024-05-03_14-35-58.xad

Created: 5/3/2024 2:35:57 PM
Modified: 5/3/2024 3:19:48 PM

Curves

Standard Curve

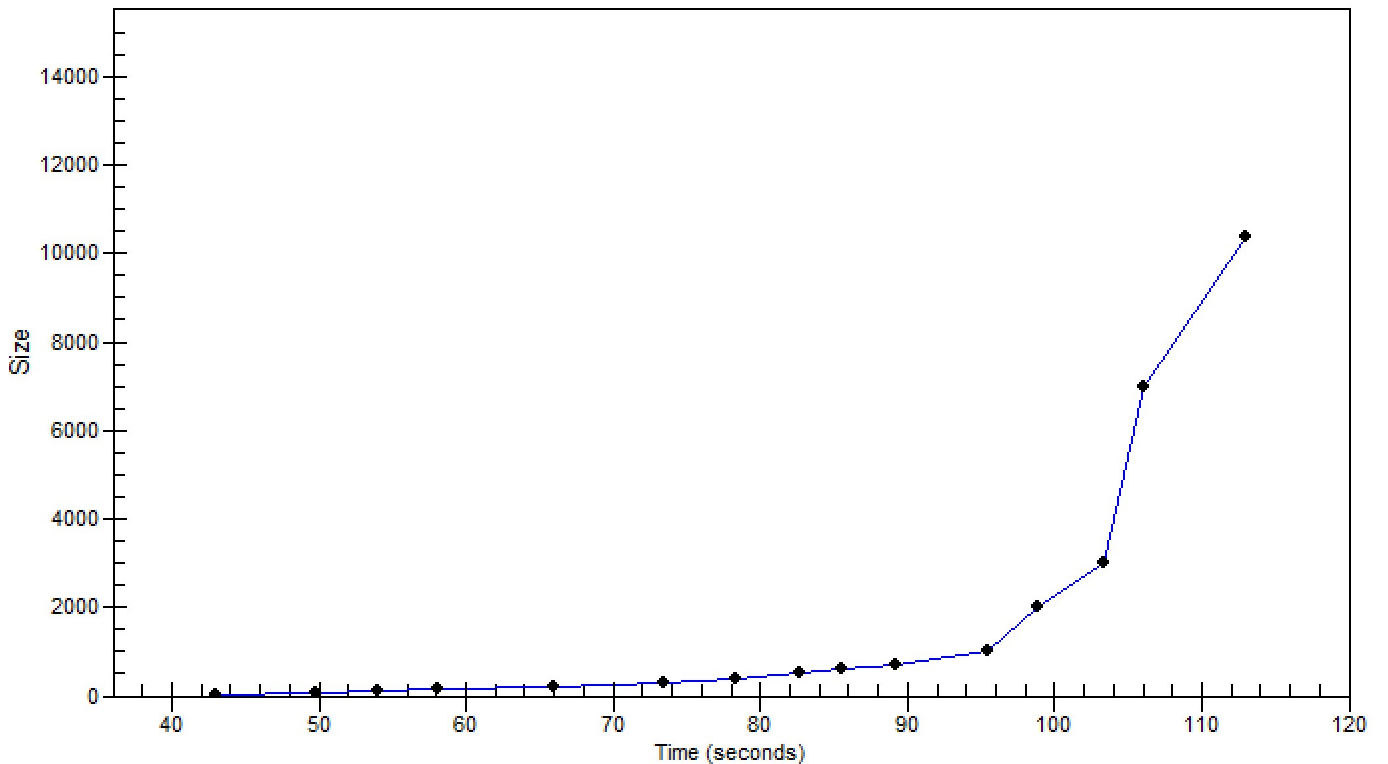

Assay Class: High Sensitivity DNA Assay
Data Path: C:\...gh Sensitivity DNA Assay_DE13804677_2024-05-03_14-35-58.xad

Created: 5/3/2024 2:35:57 PM
Modified: 5/3/2024 3:19:48 PM

Invalid Samples

Sample 8 has not been run, no results available.

Sample 9 has not been run, no results available.

Sample 10 has not been run, no results available.

Sample 11 has not been run, no results available.

Assay Class: High Sensitivity DNA Assay Created: 5/3/2024 2:35:57 PM
Data Path: C:\...gh Sensitivity DNA Assay_DE13804677_2024-05-03_14-35-58.xad Modified: 5/3/2024 3:19:48 PM

Run Logbook

Description	Number	Source	Category	Sub Category	Time	Time Zone	User	Host
Run ended on port 1 (Number of wells acquired: 8)		Instrument	Run		5/3/2024 3:05:49 PM	(GMT +02:00) W. Europe Standard Time	BioAnalyzer	BIOFPC-BIOANAL
Run started on port 1 (File: C:\Program Files (x86)\Agilent\2100 bioanalyzer\2100 expert\Data\2024-05-03\2100 expert_High Sensitivity DNA Assay_DE13804677_2024-05-03_14-35-58.xad)		Instrument	Run		5/3/2024 2:36:03 PM	(GMT +02:00) W. Europe Standard Time	BioAnalyzer	BIOFPC-BIOANAL
Product Number : G2939A		Instrument	Run		5/3/2024 2:36:03 PM	(GMT +02:00) W. Europe Standard Time	BioAnalyzer	BIOFPC-BIOANAL
Name :		Instrument	Run		5/3/2024 2:36:03 PM	(GMT +02:00) W. Europe Standard Time	BioAnalyzer	BIOFPC-BIOANAL
Vendor : Agilent Technologies		Instrument	Run		5/3/2024 2:36:03 PM	(GMT +02:00) W. Europe Standard Time	BioAnalyzer	BIOFPC-BIOANAL
Serial# : DE13804677		Instrument	Run		5/3/2024 2:36:03 PM	(GMT +02:00) W. Europe Standard Time	BioAnalyzer	BIOFPC-BIOANAL
Firmware : C.01.069		Instrument	Run		5/3/2024 2:36:03 PM	(GMT +02:00) W. Europe Standard Time	BioAnalyzer	BIOFPC-BIOANAL
Cartridge : Electrode		Instrument	Run		5/3/2024 2:36:03 PM	(GMT +02:00) W. Europe Standard Time	BioAnalyzer	BIOFPC-BIOANAL