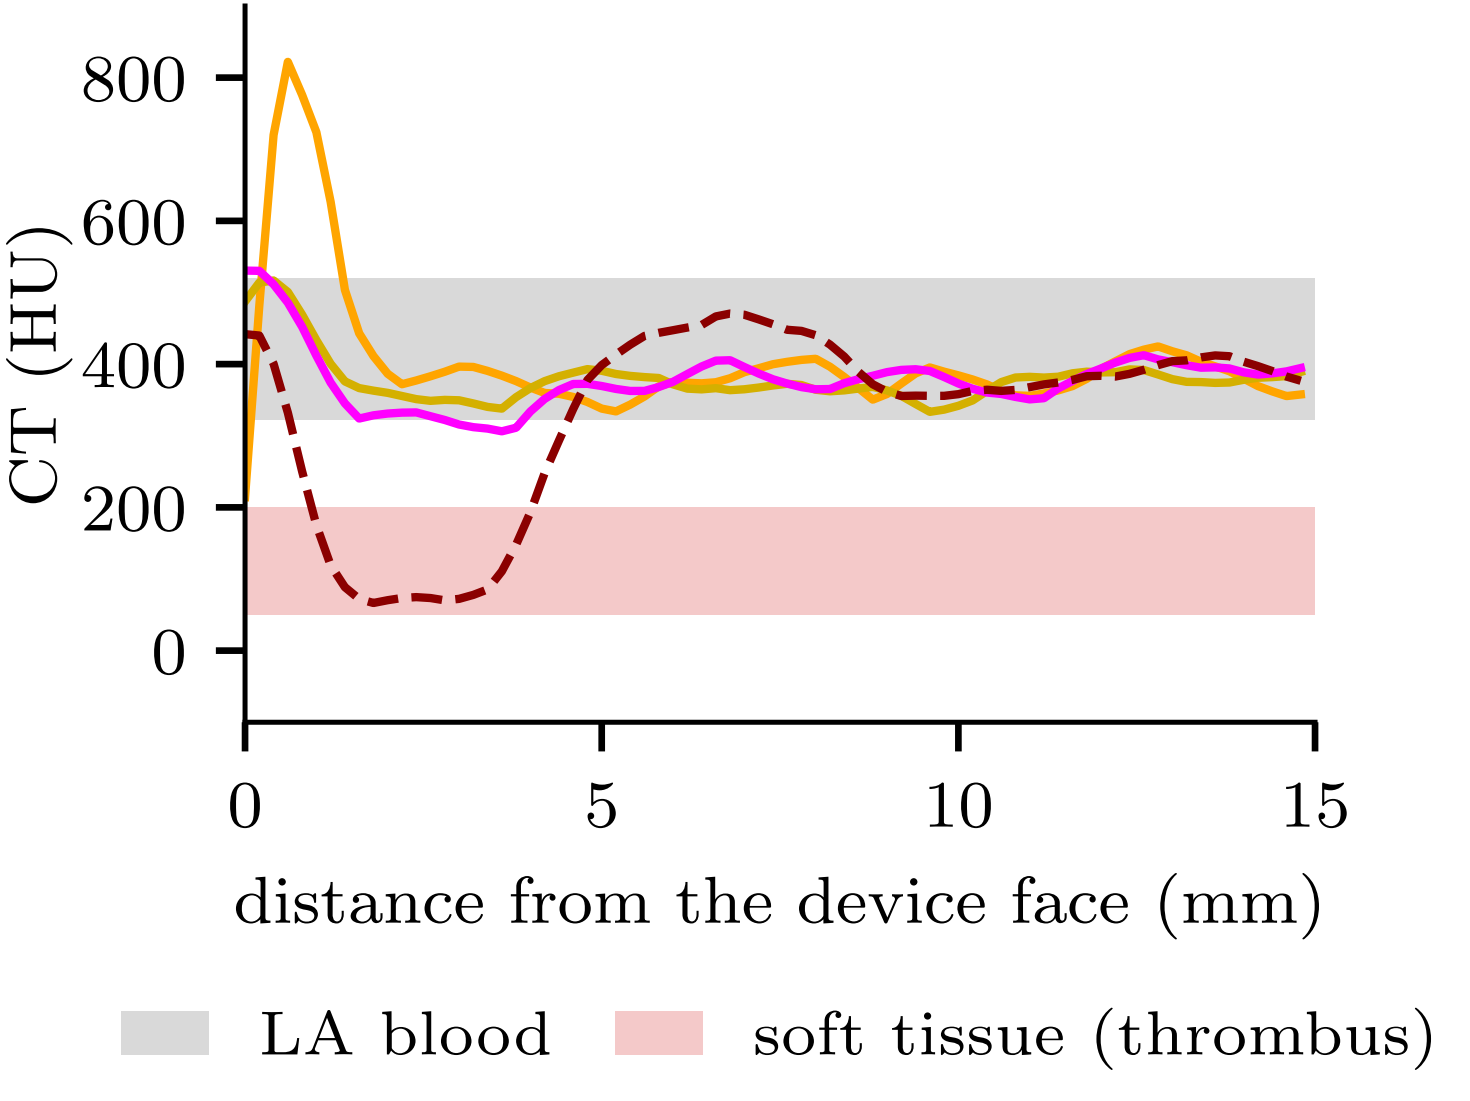
800
600
400
200
0
CT (HU)
0
5
10
15
distance from the device face (mm)
LA blood
soft tissue (thrombus)