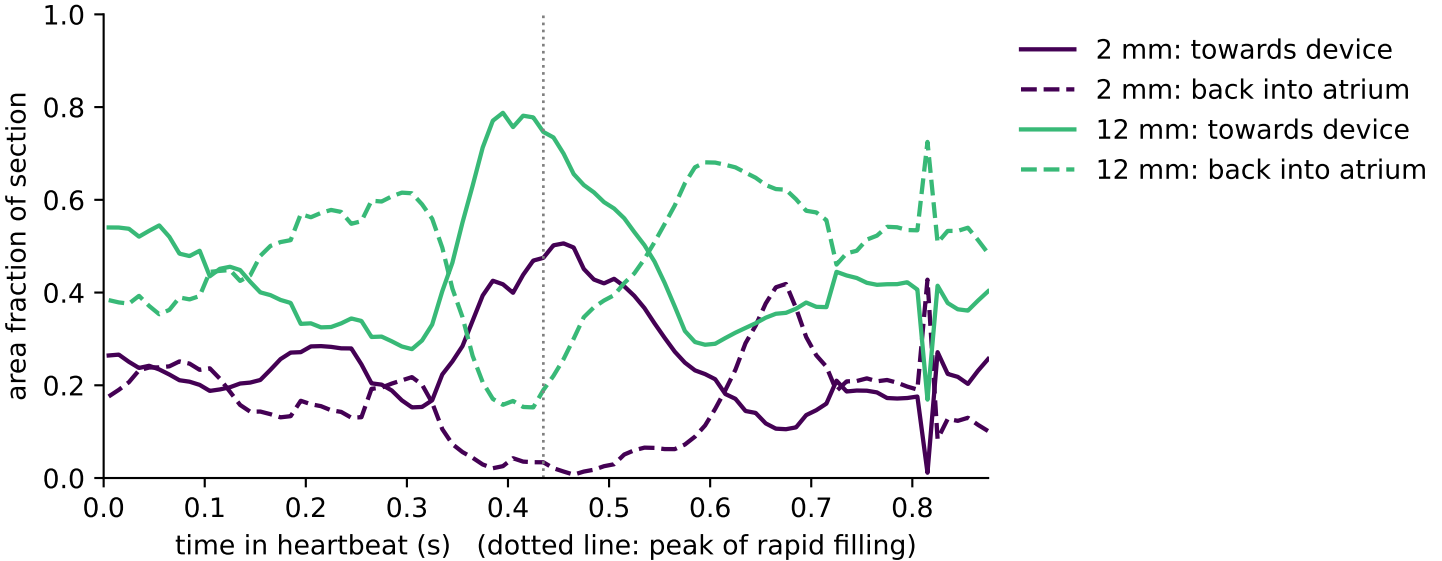
1.0
0.8
0.6
0.4
0.2
0.0
area fraction of section
0.0
0.1
0.2
0.3
0.4
0.5
0.6
0.7
0.8
time in heartbeat (s) (dotted line: peak of rapid filling)
2 mm: towards device
2 mm: back into atrium
12 mm: towards device
12 mm: back into atrium