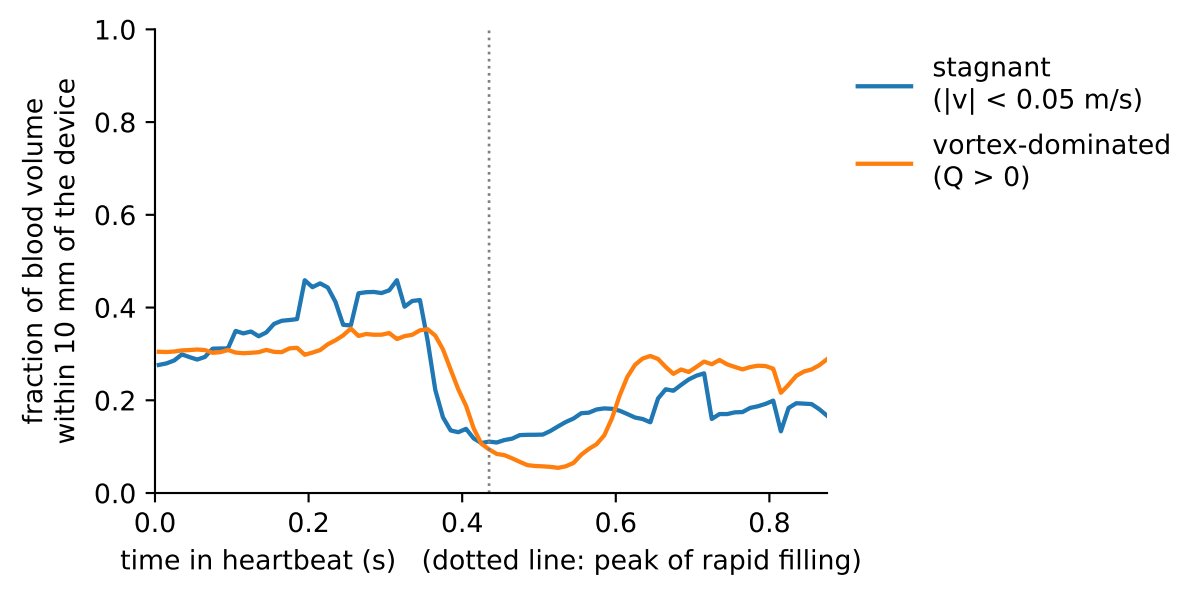
1.0
0.8
0.6
0.4
0.2
0.0
fraction of blood volume
within 10 mm of the device
0.0
0.2
0.4
0.6
0.8
time in heartbeat (s)
(dotted line: peak of rapid filling)
stagnant
(|v| < 0.05 m/s)
vortex-dominated
(Q > 0)