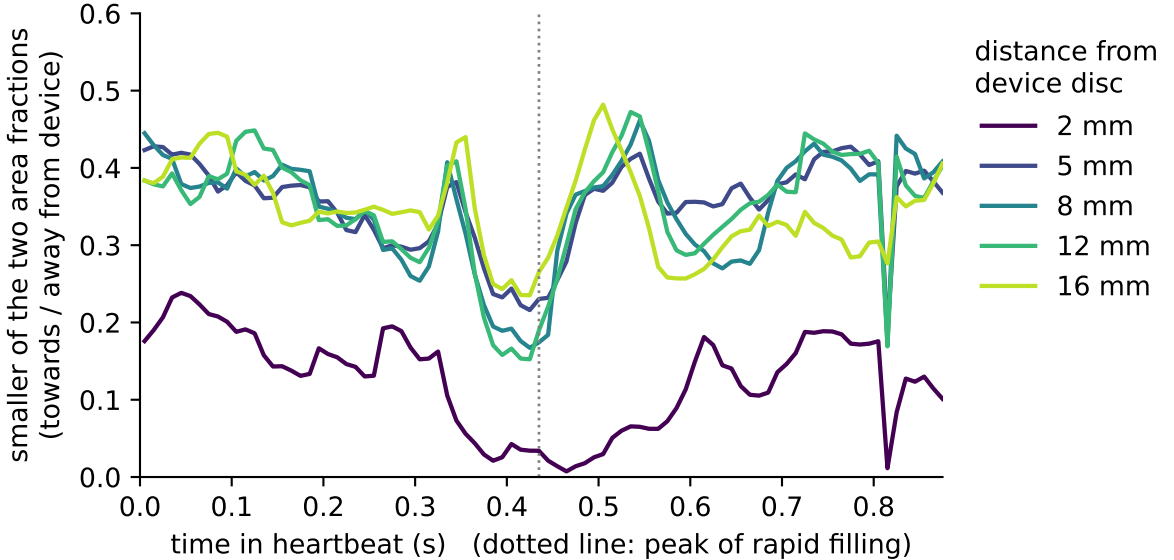
smaller of the two area fractions
(towards / away from device)
0.6
0.5
0.4
0.3
0.2
0.1
0.0
0.0
0.1
0.2
0.3
0.4
0.5
0.6
0.7
0.8
time in heartbeat (s)
(dotted line: peak of rapid filling)
distance from
device disc
2 mm
5 mm
8 mm
12 mm
16 mm