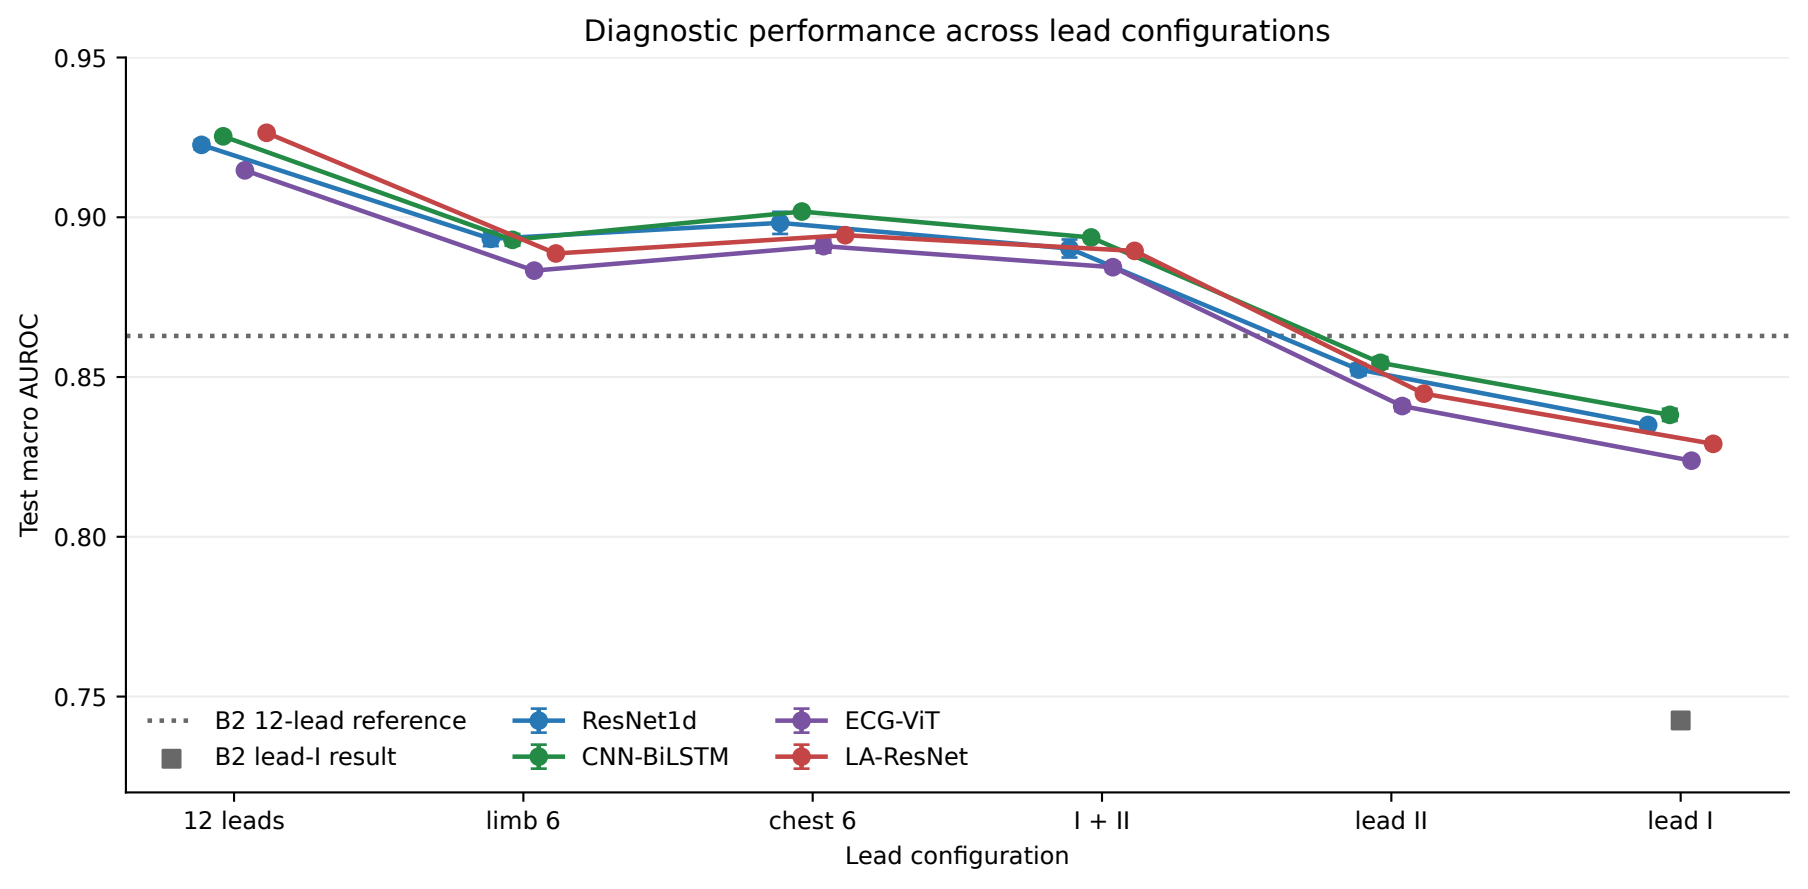
Diagnostic performance across lead configurations
Test macro AUROC
0.95
0.90
0.85
0.80
0.75
B2 12-lead reference
B2 lead-I result
ResNet1d
CNN-BiLSTM
ECG-ViT
LA-ResNet
12 leads
limb 6
chest 6
I + II
lead II
lead I
Lead configuration