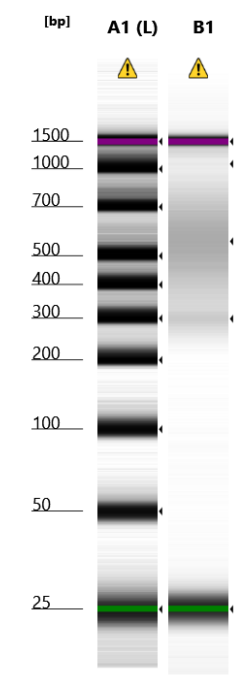


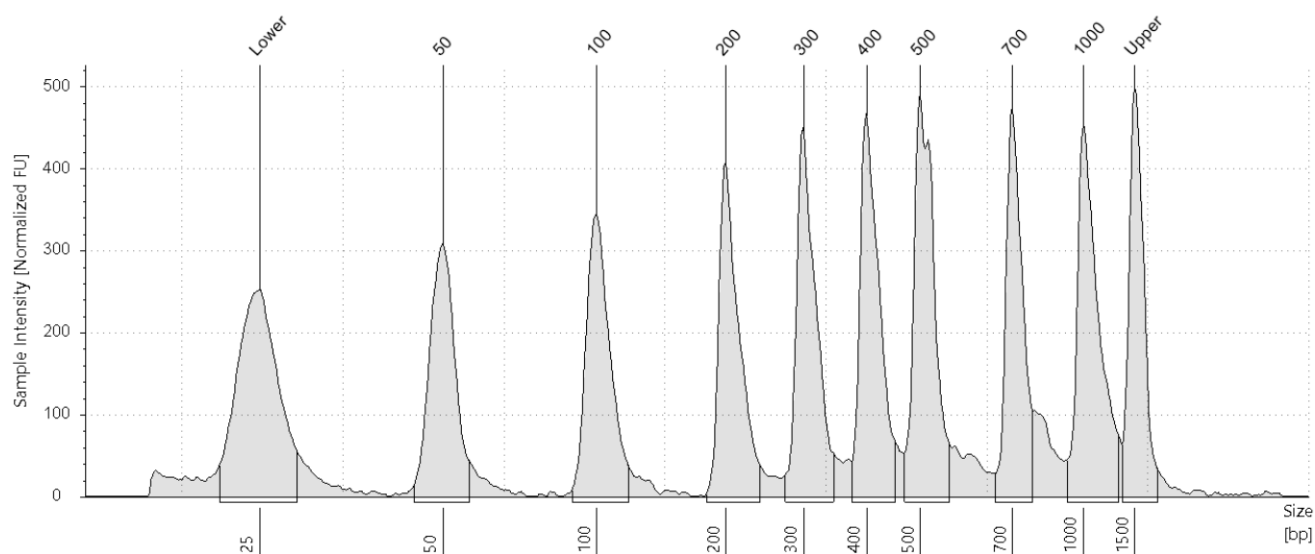
Filename: 2022-01-19 - 10.06.08.HSD1000



Default image (Contrast 100%)

Sample Info

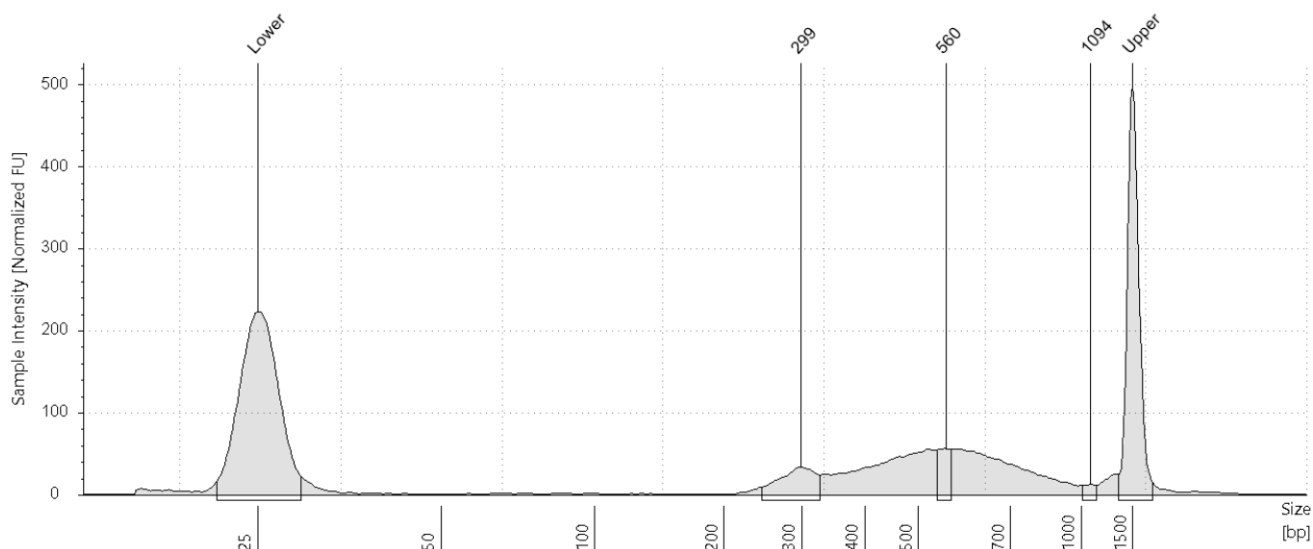
Well	Alert	Observations
A1		Caution! Expired ScreenTape device; Ladder
B1		Caution! Expired ScreenTape device

A1: Ladder**Sample Table**

Well	Alert	Observations
A1	⚠	Caution! Expired ScreenTape device; Ladder

Peak Table

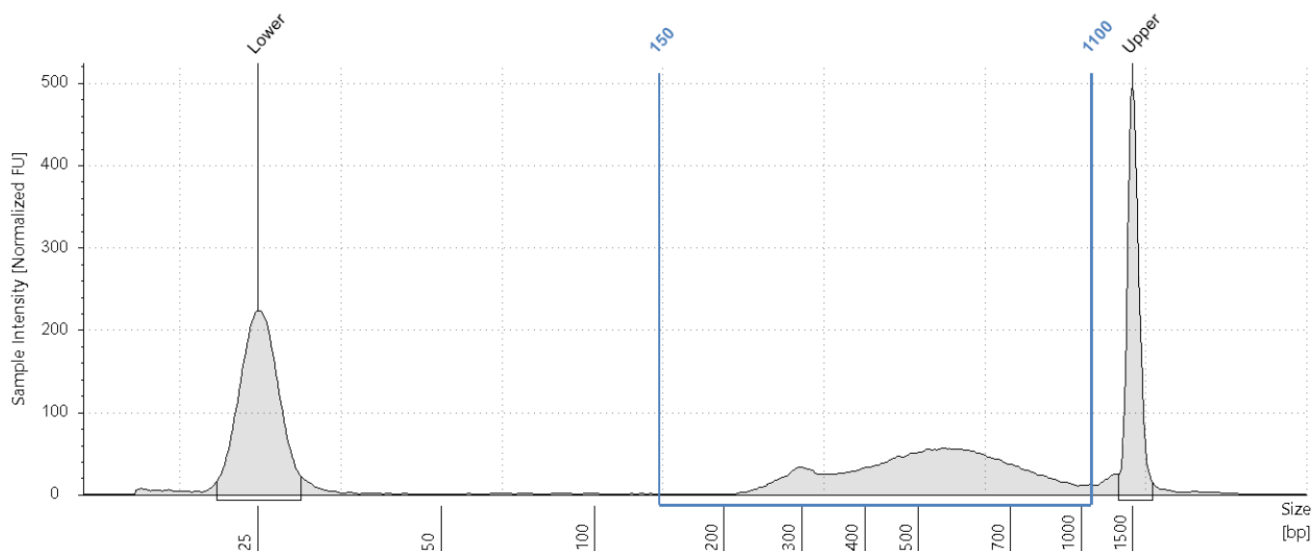
Size [bp]	Calibrated Conc. [pg/ul]	Assigned Conc. [pg/ul]	Peak Molarity [pmol/l]	% Integrated Area	Peak Comment	Observations
25	345	-	21200	-		Lower Marker
50	257	-	7900	11.13		
100	271	-	4170	11.75		
200	270	-	2070	11.69		
300	290	-	1490	12.59		
400	301	-	1160	13.07		
500	333	-	1020	14.43		
700	261	-	574	11.32		
1000	323	-	497	14.01		
1500	250	250	256	-		Upper Marker

B1: yan220120**Sample Table**

Well	Alert	Observations
B1		Caution! Expired ScreenTape device

Peak Table

Size [bp]	Calibrated Conc. [pg/ul]	Assigned Conc. [pg/ul]	Peak Molarity [pmol/l]	% Integrated Area	Peak Comment	Observations
25	376	-	23100	-		Lower Marker
299	51.3	-	264	57.01		
560	32.4	-	88.9	36.00		
1094	6.29	-	8.85	7.00		
1500	250	250	256	-		Upper Marker

**Region Table**

From [bp]	Average Size [bp]	Conc. [pg/ul]	Region Molarity [pmol/l]	% of Total	Region Comment	Color
150	539	414	1340	86.37		