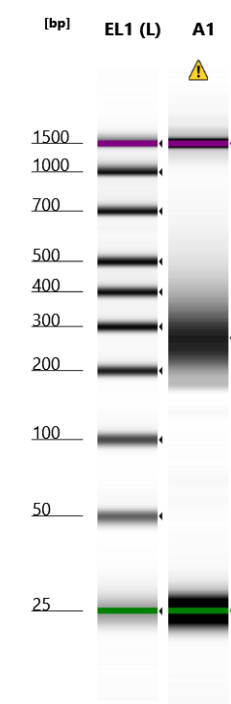


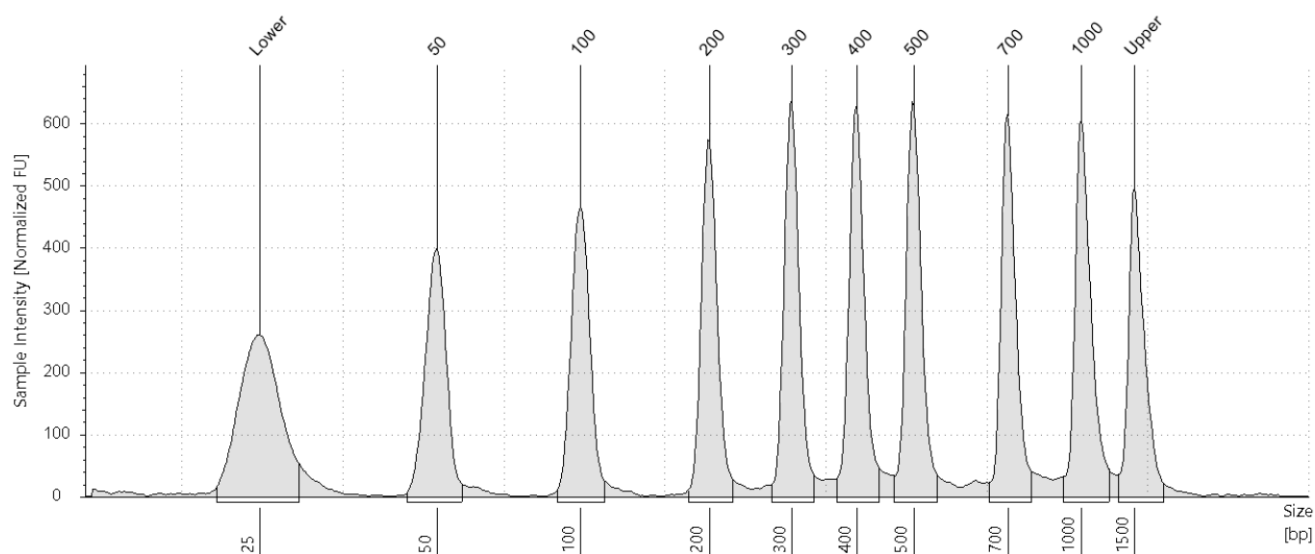
Filename: 2021-07-23 - 15.28.11.HSD1000



Default image (Contrast 50%), Image is Scaled to Sample

Sample Info

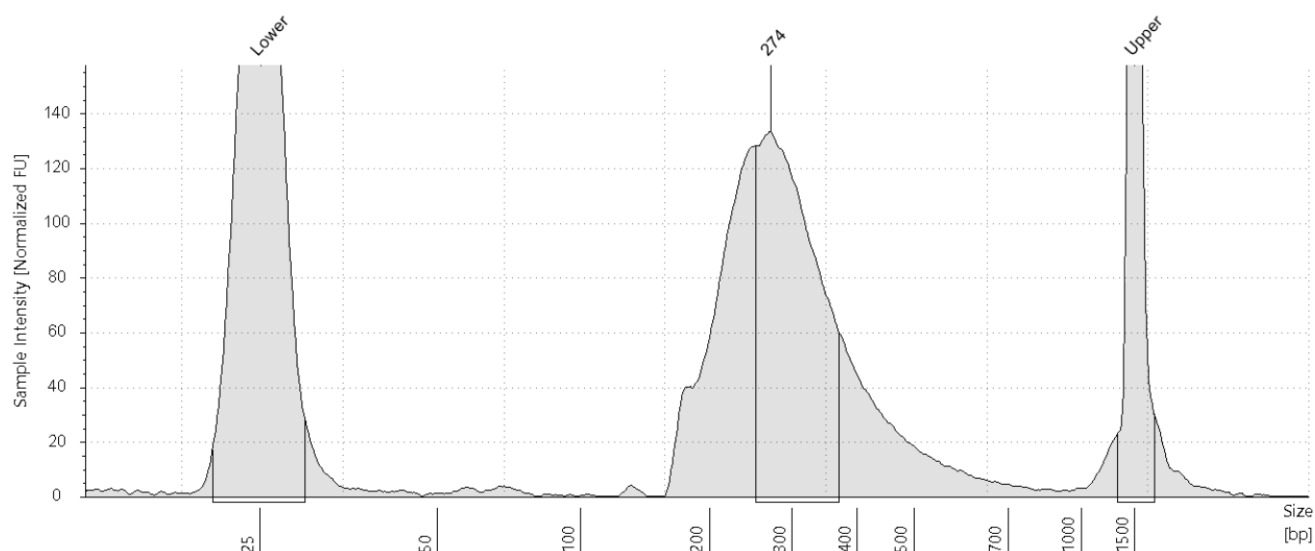
Well	Conc. [pg/ul]	Sample Description	Alert	Observations
EL1	2350	Electronic Ladder		Ladder
A1	333	pool		Caution! Expired ScreenTape device (used after two weeks of first use)

**EL1: Electronic Ladder****Sample Table**

Well	Conc. [pg/ul]	Sample Description	Alert	Observations
EL1	2350	Electronic Ladder		Ladder

**Peak Table**

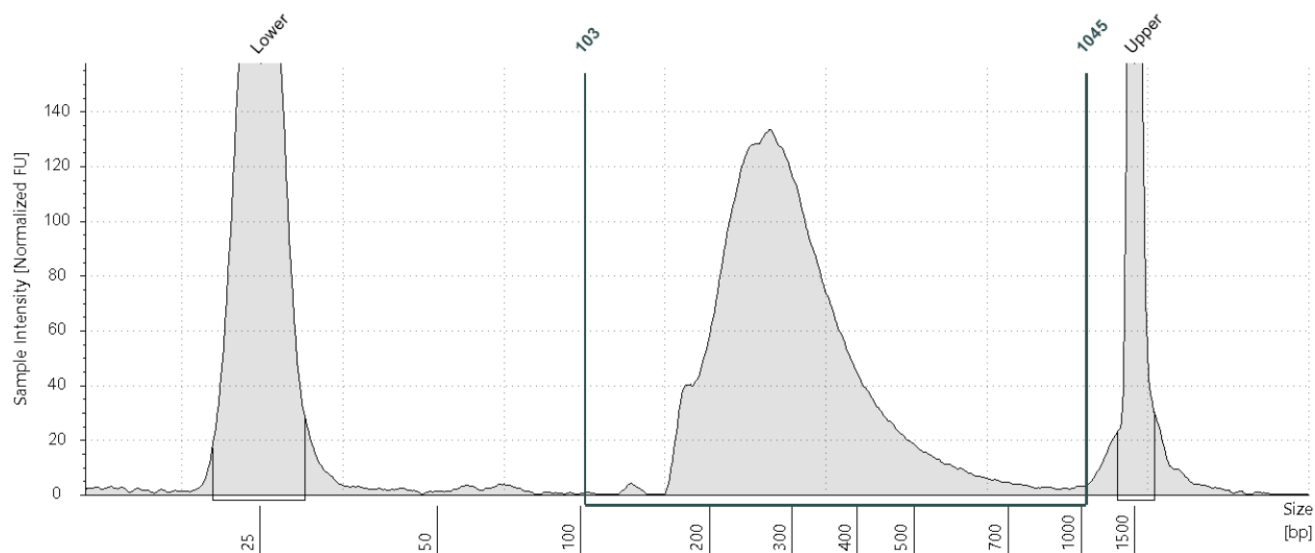
Size [bp]	Calibrated Conc. [pg/ul]	Assigned Conc. [pg/ul]	Peak Molarity [pmol/l]	% Integrated Area	Peak Comment	Observations
25	340	-	20900	-		Lower Marker
50	265	-	8160	11.28		
100	278	-	4270	11.82		
200	290	-	2230	12.32		
300	304	-	1560	12.95		
400	306	-	1180	13.00		
500	312	-	961	13.29		
700	286	-	629	12.19		
1000	309	-	476	13.15		
1500	250	250	256	-		Upper Marker

**A1: pool****Sample Table**

Well	Conc. [pg/μl]	Sample Description	Alert	Observations
A1	333	pool		Caution! Expired ScreenTape device (used after two weeks of first use)

**Peak Table**

Size [bp]	Calibrated Conc. [pg/μl]	Assigned Conc. [pg/μl]	Peak Molarity [pmol/l]	% Integrated Area	Peak Comment	Observations
25	507	-	31200	-		Lower Marker
274	333	-	1870	100.00		
1500	250	250	256	-		Upper Marker

**Region Table**

From [bp]	Average Size [bp]	Conc. [pg/μl]	Region Molarity [pmol/l]	% of Total	Region Comment	Color
103	312	698	3820	90.48		