

Instrument controller software run summary:

Filename and data path: C:\Agilent Technologies\Data\2026 04 07\13-40-07\2026 04 07 13H 40M.raw
Created: 7/4/2026 1:57 PM
Number of capillaries: 12
Array serial number: 050924-20USFP
Effective length: 22 cm
Array usage count: 64
Instrument type: Femto Pulse
Instrument controller software version: 2.0.0.3
Device serial number: MY2435AD41

Method Information

Method name: FP-1002-22 - gDNA 165Kb.mthds
Gel prime: No
Full conditioning: Yes
Gel prime to buffer: No
Gel selection: Gel 1
Prerun: -5.0 kV, 60 sec.
Rinse: No
Marker 1: No
Rinse: Tray: Marker, Row: G, Number of dips: 1
Sample injection: -5.0 kV, 30 sec.
Separation: 70.0 min.
Tray Name: Tray-1


Analysis mode: DNA

Report Generated on 07-Apr-2026 at 03:38:48 PM

Notes

Time Shift: Using configured: slope=0.00025, intercept=0.0


Gel Image

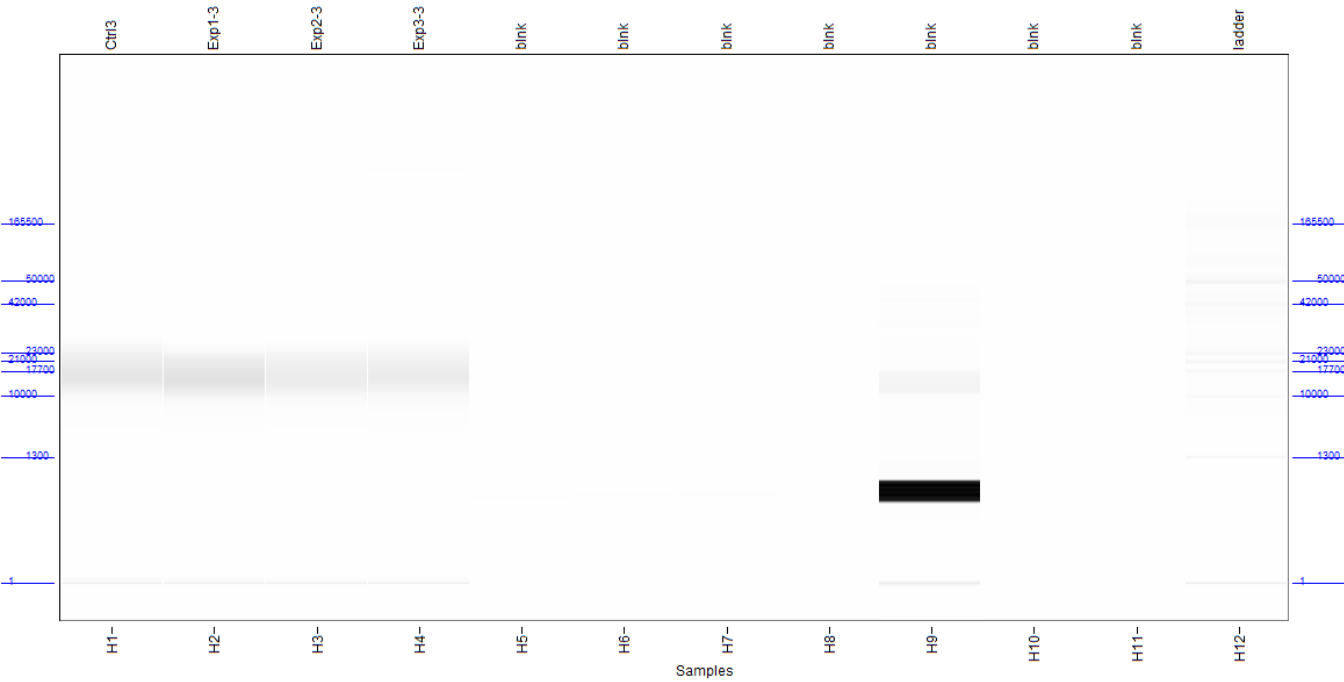


DQN Summary

Well	Sample ID	DQN	Size threshold (bp)	Total concentration (pg/ul)
H1	Ctrl3	9.1	10000	532.2341
H2	Exp1-3	9.0	10000	621.6293
H3	Exp2-3	8.9	10000	429.0400
H4	Exp3-3	8.9	10000	454.6769
H5	blnk	N/A	0	0.0000
H6	blnk	N/A	0	0.0000
H7	blnk	N/A	0	0.0000
H8	blnk	N/A	0	0.0000
H9	blnk	N/A	0	1767.0717
H10	blnk	N/A	0	0.0000
H11	blnk	N/A	0	0.0000
H12	ladder			

Filename and Data Path: C:\Agilent Technologies\Data\2026 04 07\13-40-07\2026 04 07 13H 40M.raw

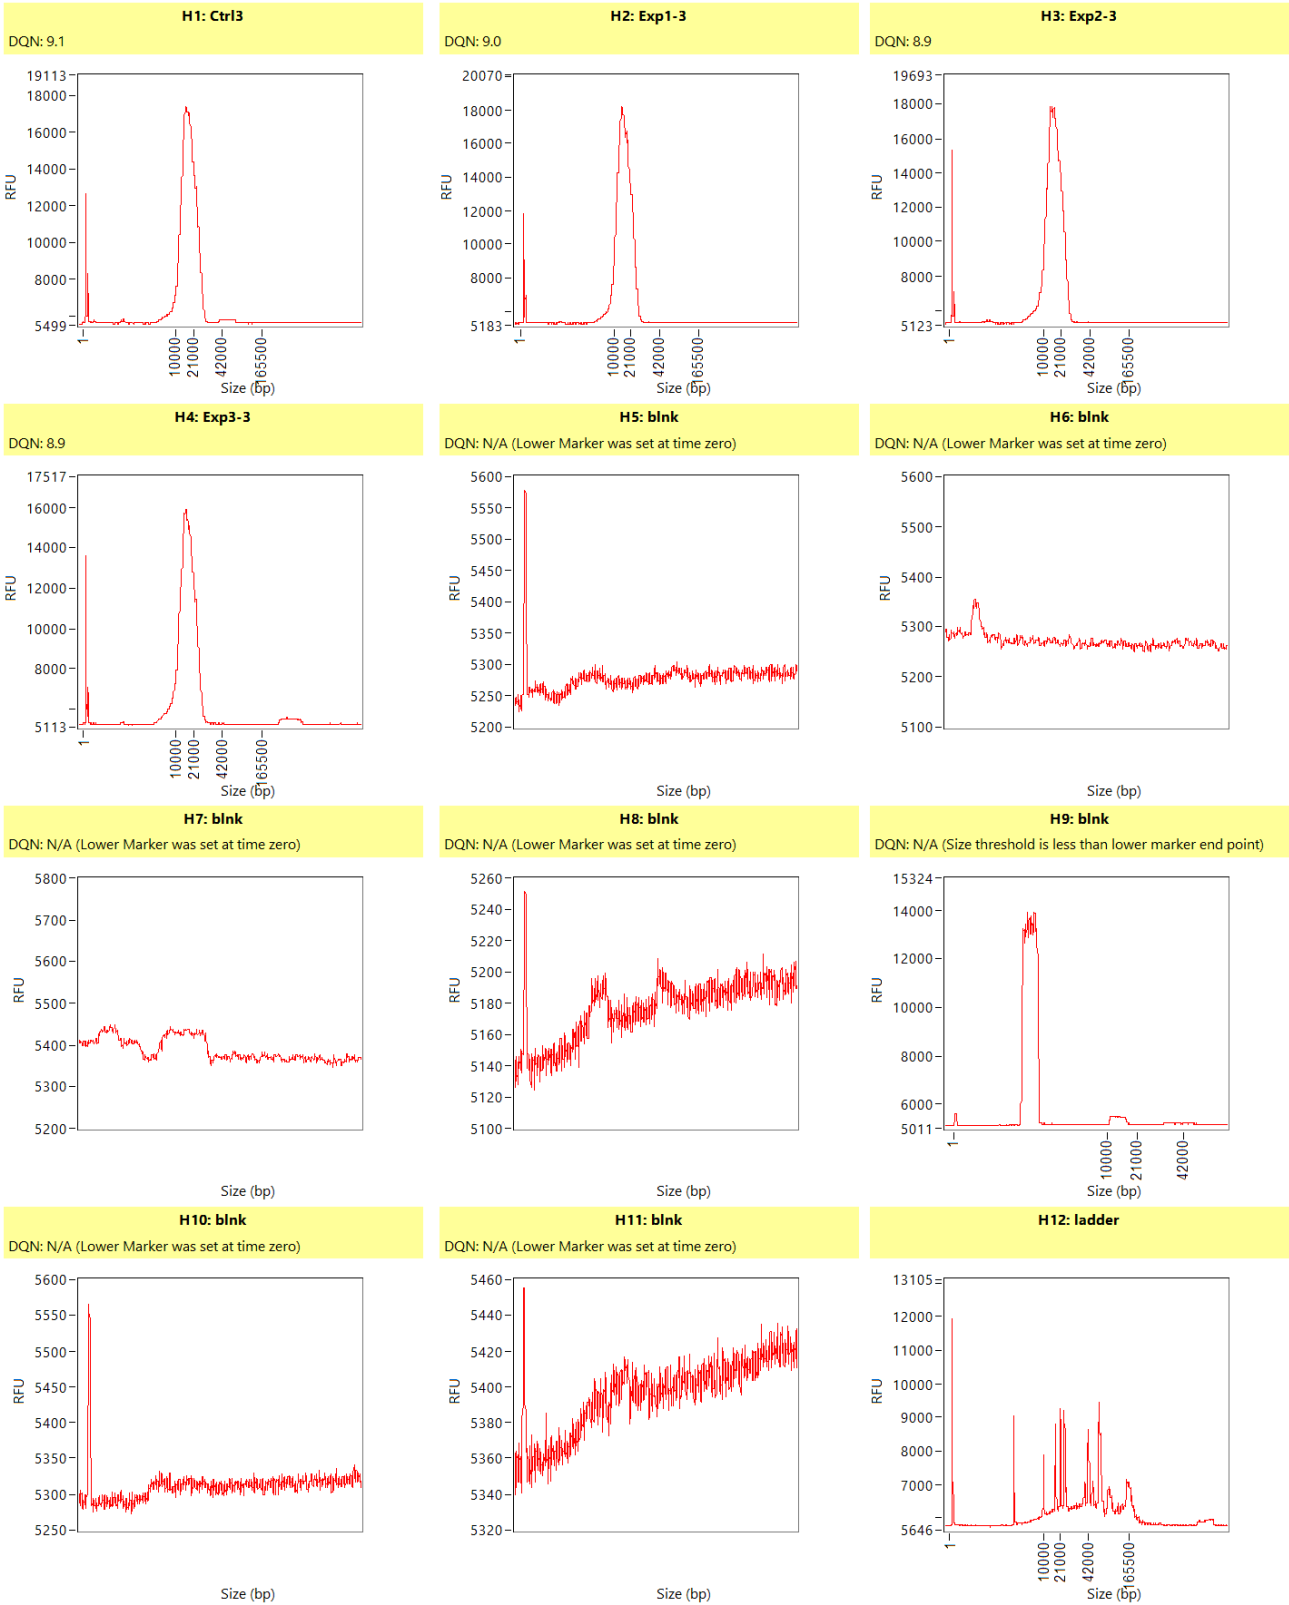

Sample: Ctrl3
Well location: H1
Created: 7/4/2026 1:57 PM

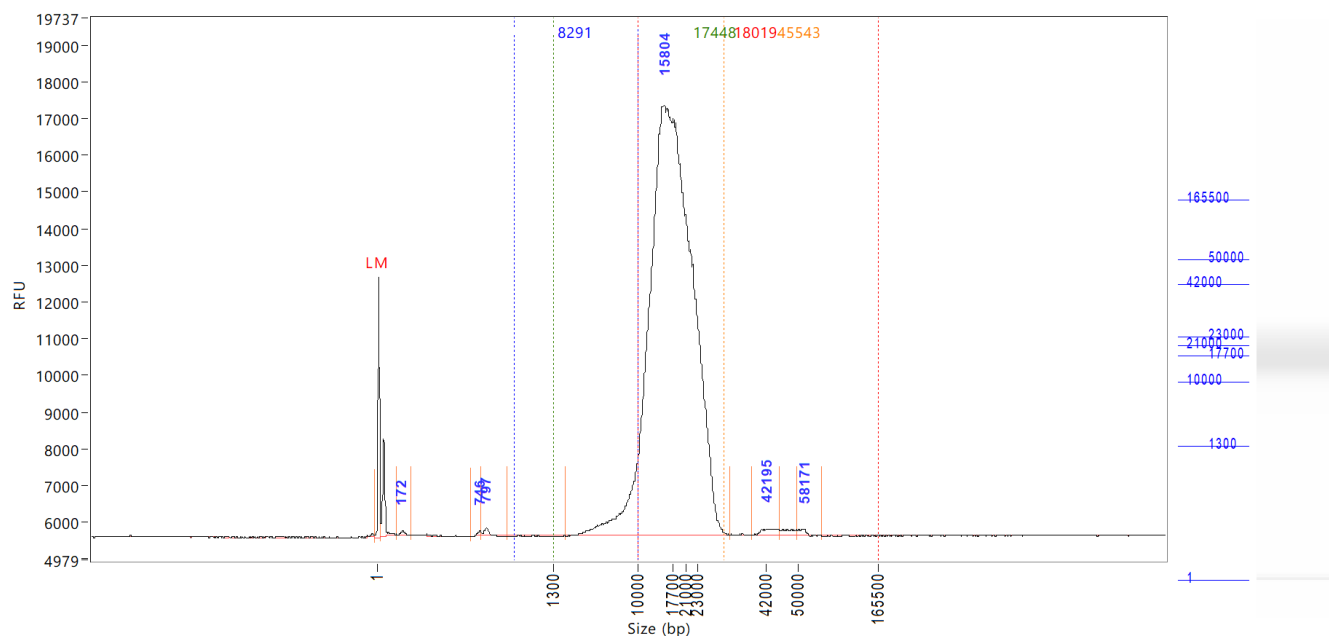

Sample Peak Width (sec): 20	Sample Min Peak Height: 50	Sample Baseline V to V?: Y	Sample Baseline V to V pts: 3
Sample filter: Binomial	Number of points for filter: 3	Sample start region (min): 0	Sample end region (min): 70
Manual baseline start (min): 25	Manual baseline end (min): 70	Marker peak width (sec): 8	Marker min peak height: 500
Marker baseline V to V?: N	Marker baseline V to V points: 3	Lower marker selection: First peak > 500 RFU	Upper marker selection: Last peak > 500 RFU
Ladder size (bp) 1, 1300, 10000, 17700, 21000, 23000, 42000, 50000, 165500	Quantification using: Ladder Final concentration (ng/uL): 0.0200 Dilution factor: 10.0	Minimum RFU for data processing: 1	Size threshold (b.p.): 10000

Sample: Ctrl3
 Well location: H1
 Created: 7/4/2026 1:57 PM


Table Information

Peak Table

Peak	Size	Concentration	From	To	Size	Percent CV	RFU	Corrected peak area					
	(bp)	(pg/ul)	(bp)	(bp)	(bp)								
1	1 (LM)	2.0345	0	15	1 (LM)	1494.92	7099	41.037					
2	172	0.8802	142	248	172	10.46	113	1.775					
3	746	0.6777	685	765	746	1.74	129	1.367					
4	797	1.3662	765	954	797	2.15	221	2.756					
5	15804	509.6877	2570	31853	15804	25.68	11733	1028.052					
6	42195	2.6234	37826	45484	42195	4.00	185	5.292					
7	58171	1.0051	49806	85282	58171	7.40	168	2.027					
	TIC:	516.2403	Pg/ul										
	TIM:	61.3001	Pmole/l										
	Total concentration:	532.2341	Pg/ul										
	DQN:	9.1											
	Threshold:	10000											

Smear Analysis	10000 bp to 165000 bp	485.1551 pg/ul	91.2 %Total	44.3261 pmole/L	18019 Avg. Size (bp)	27.61 %CV
	30000 bp to 165000 bp	5.8701 pg/ul	1.1 %Total	0.2122 pmole/L	45543 Avg. Size (bp)	14.76 %CV
	1300 bp to 165000 bp	515.3473 pg/ul	96.8 %Total	48.6268 pmole/L	17448 Avg. Size (bp)	30.69 %CV
	1000 bp to 10000 bp	30.6945 pg/ul	5.8 %Total	6.0952 pmole/L	8291 Avg. Size (bp)	18.17 %CV

Sample: Exp1-3
Well location: H2
Created: 7/4/2026 1:57 PM

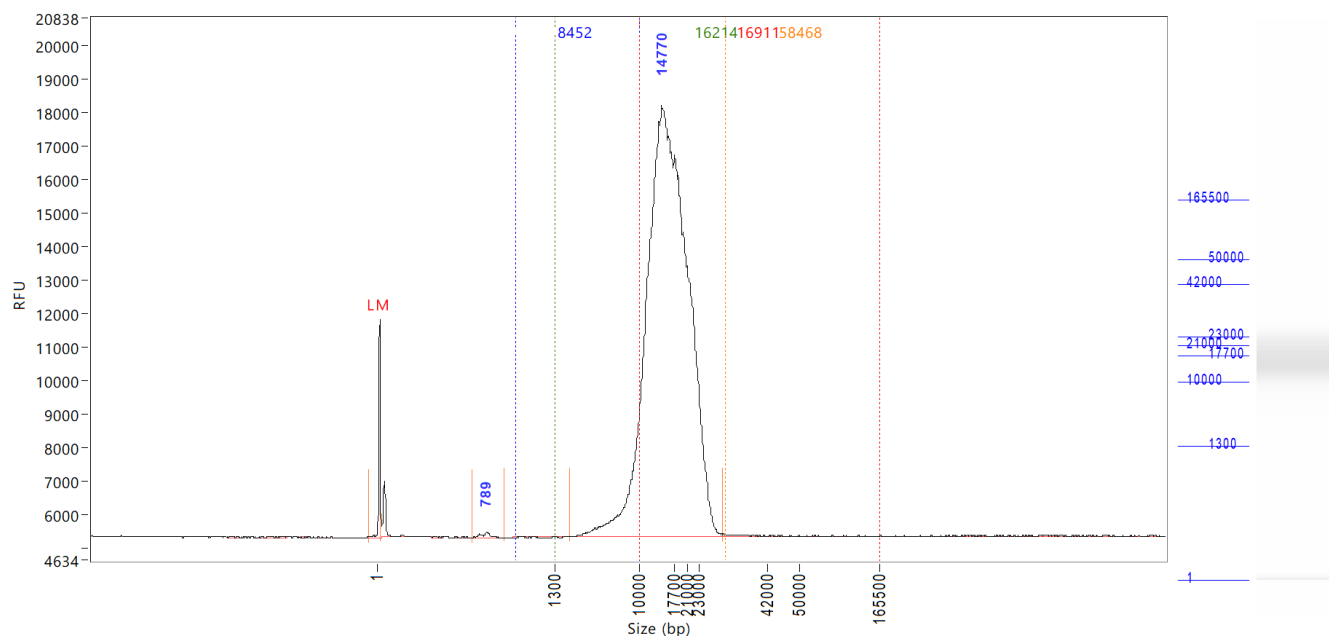

Sample Peak Width (sec): 20	Sample Min Peak Height: 50	Sample Baseline V to V?: Y	Sample Baseline V to V pts: 3
Sample filter: Binomial	Number of points for filter: 3	Sample start region (min): 0	Sample end region (min): 70
Manual baseline start (min): 25	Manual baseline end (min): 70	Marker peak width (sec): 8	Marker min peak height: 500
Marker baseline V to V?: N	Marker baseline V to V points: 3	Lower marker selection: First peak > 500 RFU	Upper marker selection: Last peak > 500 RFU
Ladder size (bp): 1, 1300, 10000, 17700, 21000, 23000, 42000, 50000, 165500	Quantification using: Ladder Final concentration (ng/uL): 0.0200 Dilution factor: 10.0	Minimum RFU for data processing: 1	Size threshold (b.p.): 10000

Sample: Exp1-3
Well location: H2
Created: 7/4/2026 1:57 PM


Table Information

Peak Table

Peak	Size	Concentration	From	To	Size	Percent CV	RFU	Corrected peak area					
	(bp)	(pg/ul)	(bp)	(bp)	(bp)								
1	1 (LM)	2.0345	0	17	1 (LM)	-2171.88	6501	36.527					
2	789	1.7980	687	929	789	4.46	145	3.228					
3	14770	604.2082	2808	29478	14770	26.27	12927	1084.775					
	TIC:	606.0062	Pg/ul										
	TIM:	65.9209	Pmole/l										
	Total concentration:	621.6293	Pg/ul										
	DQN:	9.0											
	Threshold:	10000											

Smear Analysis	10000 bp to 165000 bp	557.2099 pg/ul	89.6 %Total	54.2450 pmole/L	16911 Avg. Size (bp)	31.86 %CV
	30000 bp to 165000 bp	2.8482 pg/ul	0.5 %Total	0.0802 pmole/L	58468 Avg. Size (bp)	62.43 %CV
	1300 bp to 165000 bp	607.1798 pg/ul	97.7 %Total	61.6502 pmole/L	16214 Avg. Size (bp)	35.03 %CV
	1000 bp to 10000 bp	51.0851 pg/ul	8.2 %Total	9.9509 pmole/L	8452 Avg. Size (bp)	18.13 %CV

Sample: Exp2-3
Well location: H3
Created: 7/4/2026 1:57 PM

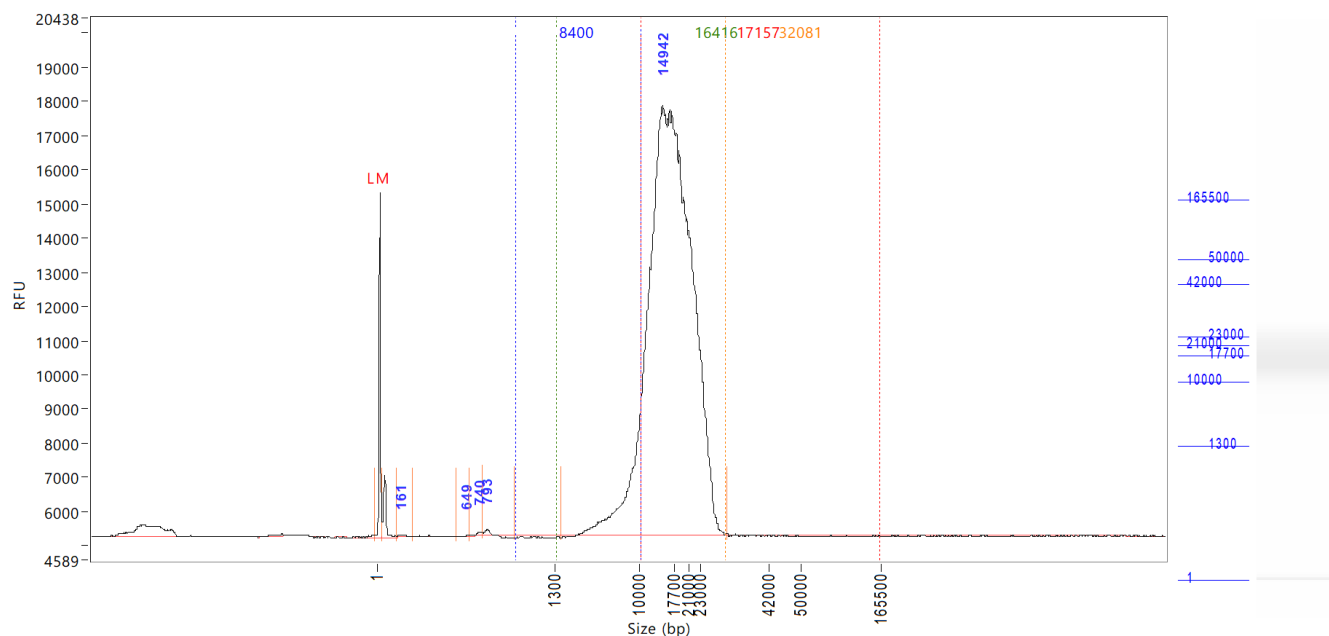

Sample Peak Width (sec): 20
Sample filter: Binomial
Manual baseline start (min): 25
Marker baseline V to V?: N

Ladder size (bp) 1, 1300, 10000,
17700, 21000, 23000, 42000,
50000, 165500

Sample Min Peak Height: 50
Number of points for filter: 3
Manual baseline end (min): 70
Marker baseline V to V points: 3

Quantification using: Ladder
Final concentration (ng/uL): 0.0200
Dilution factor: 10.0

Sample Baseline V to V?: Y
Sample start region (min): 0
Marker peak width (sec): 8

Lower marker selection: First peak
> 500 RFU
Minimum RFU for data processing:
1
Size threshold (b.p.): 10000

Sample Baseline V to V pts: 3
Sample end region (min): 70
Marker min peak height: 500
Upper marker selection: Last peak
> 500 RFU


Sample: Exp2-3
Well location: H3
Created: 7/4/2026 1:57 PM

Table Information

Peak Table

Peak	Size	Concentration	From	To	Size	Percent CV	RFU	Corrected peak area					
	(bp)	(pg/ul)	(bp)	(bp)	(bp)								
1	1 (LM)	2.0345	0	19	1 (LM)	872.12	10061	54.893					
2	161	0.8509	131	246	161	16.73	74	2.296					
3	649	0.3360	570	662	649	3.04	68	0.906					
4	740	0.7834	662	766	740	4.38	87	2.114					
5	793	0.6571	766	1005	793	1.66	145	1.773					
6	14942	418.8144	1830	30485	14942	26.88	12583	1129.992					
	TIC:	421.4417	Pg/ul										
	TIM:	53.8110	Pmole/l										
	Total concentration:	429.0400	Pg/ul										
	DQN:	8.9											
	Threshold:	10000											
Smear Analysis	10000 bp to 165000 bp	383.4042 pg/ul	89.4 %Total	36.7906 pmole/L	17157 Avg. Size (bp)	22.27 %CV							
	30000 bp to 165000 bp	0.0616 pg/ul	0.0 %Total	0.0032 pmole/L	32081 Avg. Size (bp)	11.96 %CV							
	1300 bp to 165000 bp	418.8374 pg/ul	97.6 %Total	42.0039 pmole/L	16416 Avg. Size (bp)	26.90 %CV							
	1000 bp to 10000 bp	36.0629 pg/ul	8.4 %Total	7.0681 pmole/L	8400 Avg. Size (bp)	17.10 %CV							

Sample: Exp3-3
Well location: H4
Created: 7/4/2026 1:57 PM

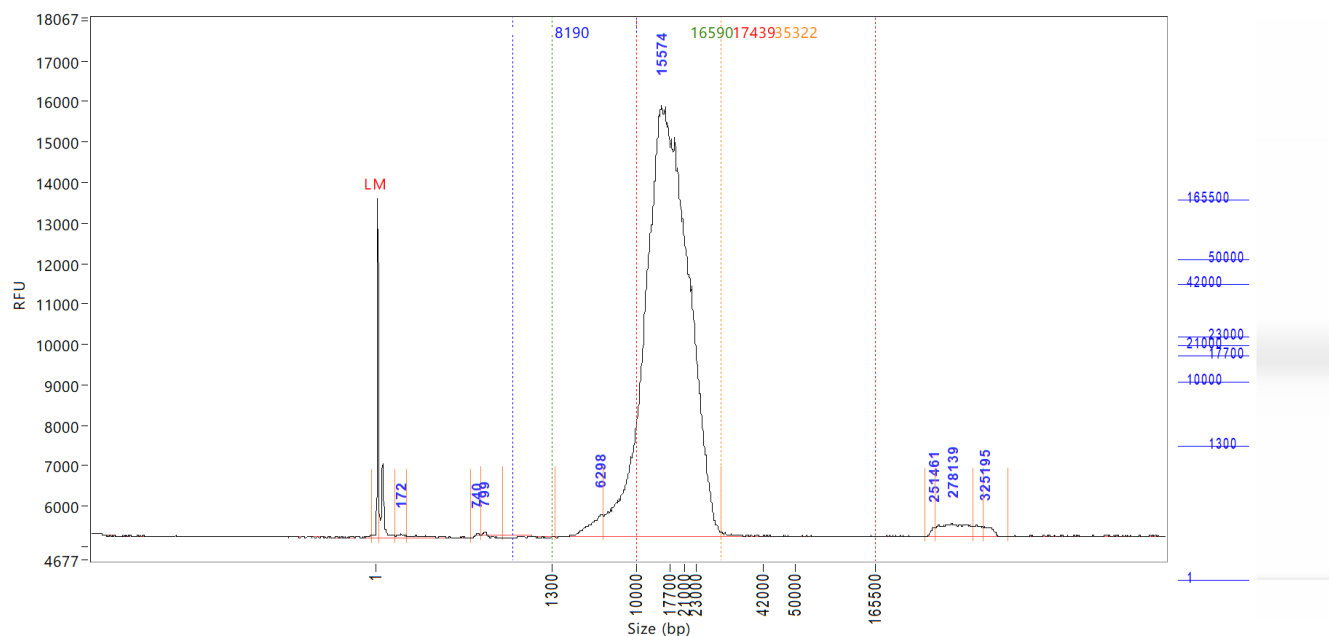

Sample Peak Width (sec): 20
Sample filter: Binomial
Manual baseline start (min): 25
Marker baseline V to V?: N

Ladder size (bp) 1, 1300, 10000,
17700, 21000, 23000, 42000,
50000, 165500

Sample Min Peak Height: 50
Number of points for filter: 3
Manual baseline end (min): 70
Marker baseline V to V points: 3

Quantification using: Ladder
Final concentration (ng/uL): 0.0200
Dilution factor: 10.0

Sample Baseline V to V?: Y
Sample start region (min): 0
Marker peak width (sec): 8

Lower marker selection: First peak
> 500 RFU
Minimum RFU for data processing:
1
Size threshold (b.p.): 10000

Sample Baseline V to V pts: 3
Sample end region (min): 70
Marker min peak height: 500
Upper marker selection: Last peak
> 500 RFU

Sample: Exp3-3
Well location: H4
Created: 7/4/2026 1:57 PM


Table Information

Peak Table

Peak	Size	Concentration	From	To	Size	Percent CV	RFU	Corrected peak area					
	(bp)	(pg/ul)	(bp)	(bp)	(bp)								
1	1 (LM)	2.0345	0	17	1 (LM)	441.06	8402	44.600					
2	172	0.8475	136	218	172	12.25	82	1.858					
3	740	0.2563	695	772	740	1.82	56	0.562					
4	799	0.4496	772	935	799	1.35	99	0.986					
5	6298	7.4879	1671	6616	6298	13.86	539	16.415					
6	15574	426.5444	6616	30126	15574	26.20	10655	935.051					
7	251461	0.4904	238863	252573	251461	0.93	208	1.075					
8	278139	5.3330	252573	308151	278139	5.62	300	11.691					
9	325195	1.2149	323343	359654	325195	1.56	224	2.663					
	TIC:	442.6240	Pg/ul										
	TIM:	53.6751	Pmole/l										
	Total concentration:	454.6769	Pg/ul										
	DQN:	8.9											
	Threshold:	10000											

Smear Analysis	10000 bp to 165000 bp	395.1461 pg/ul	86.9 %Total	37.3048 pmole/L	17439 Avg. Size (bp)	22.77 %CV
	30000 bp to 165000 bp	0.6330 pg/ul	0.1 %Total	0.0295 pmole/L	35322 Avg. Size (bp)	31.57 %CV
	1300 bp to 165000 bp	434.5224 pg/ul	95.6 %Total	43.1213 pmole/L	16590 Avg. Size (bp)	28.08 %CV
	1000 bp to 10000 bp	39.9501 pg/ul	8.8 %Total	8.0301 pmole/L	8190 Avg. Size (bp)	18.90 %CV

Sample: blnk
Well location: H5
Created: 7/4/2026 1:57 PM

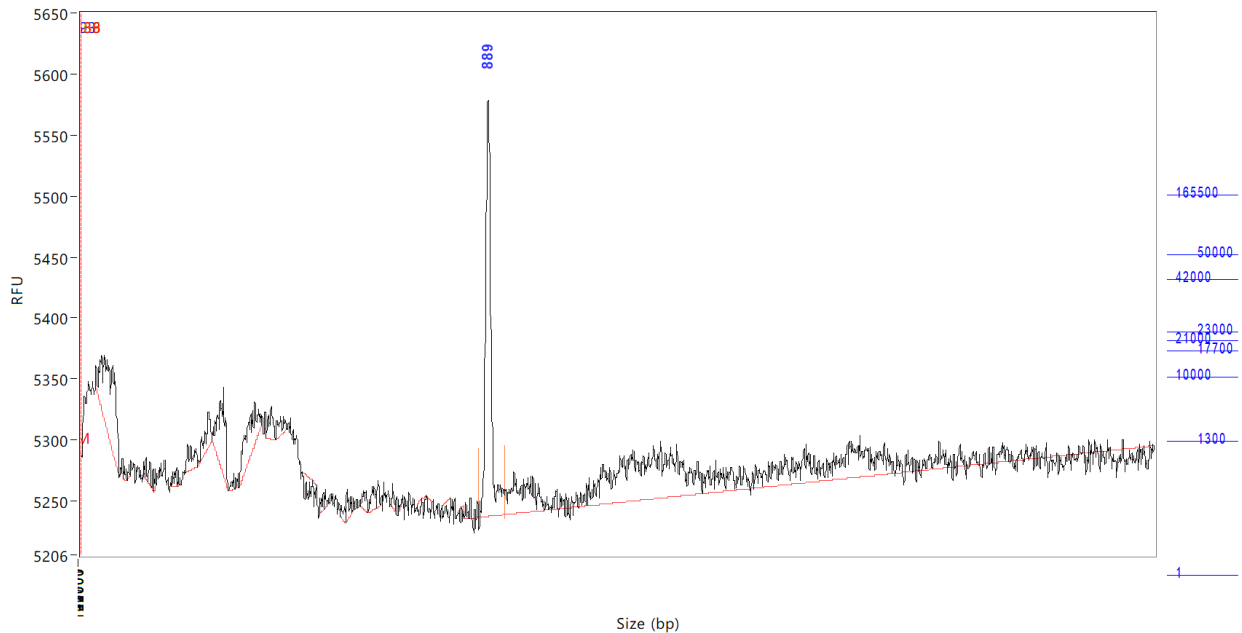


Sample Peak Width (sec): 20	Sample Min Peak Height: 50	Sample Baseline V to V?: Y	Sample Baseline V to V pts: 3
Sample filter: Binomial	Number of points for filter: 3	Sample start region (min): 0	Sample end region (min): 70
Manual baseline start (min): 25	Manual baseline end (min): 70	Marker peak width (sec): 8	Marker min peak height: 500
Marker baseline V to V?: N	Marker baseline V to V points: 3	Lower marker selection: First peak > 500 RFU	Upper marker selection: Last peak > 500 RFU
Ladder size (bp) 1, 1300, 10000, 17700, 21000, 23000, 42000, 50000, 165500	Quantification using: Ladder Final concentration (ng/uL): 0.0200 Dilution factor: 10.0	Minimum RFU for data processing: 1	Size threshold (b.p.): 0

Sample: blnk
Well location: H5
Created: 7/4/2026 1:57 PM

Table Information

Peak Table								
Peak	Size	Concentration	From	To	Size	Percent CV	RFU	Corrected peak area
	(bp)	(pg/ul)	(bp)	(bp)	(bp)			
1	1 (LM)	Inf	821	1022	1 (LM)	3.61	341	5.340
	TIC:	0.0000	Pg/ul					
	TIM:	0.0000	Pmole/l					
	Total concentration:	0.0000	Pg/ul					
	DQN:	N/a (lower marker was set at time zero)						
	Threshold:	0						
Smear Analysis	10000 bp to 165000 bp	NaN pg/ul	NaN %Total	NaN pmole/L	45638 Avg. Size (bp)	94.89 %CV		
	30000 bp to 165000 bp	NaN pg/ul	NaN %Total	NaN pmole/L	80889 Avg. Size (bp)	55.06 %CV		
	1300 bp to 165000 bp	NaN pg/ul	NaN %Total	NaN pmole/L	36666 Avg. Size (bp)	112.46 %CV		
	1000 bp to 10000 bp	NaN pg/ul	NaN %Total	NaN pmole/L	4593 Avg. Size (bp)	75.99 %CV		

Sample: blnk
Well location: H6
Created: 7/4/2026 1:57 PM

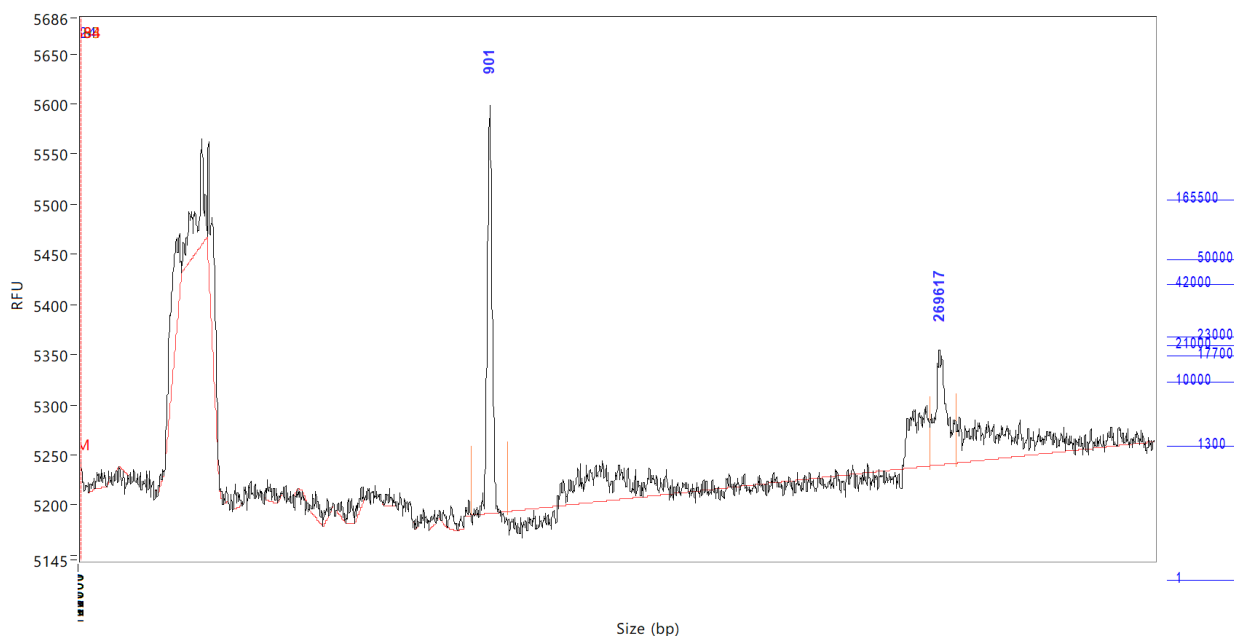

Sample Peak Width (sec): 20	Sample Min Peak Height: 50	Sample Baseline V to V?: Y	Sample Baseline V to V pts: 3
Sample filter: Binomial	Number of points for filter: 3	Sample start region (min): 0	Sample end region (min): 70
Manual baseline start (min): 25	Manual baseline end (min): 70	Marker peak width (sec): 8	Marker min peak height: 500
Marker baseline V to V?: N	Marker baseline V to V points: 3	Lower marker selection: First peak > 500 RFU	Upper marker selection: Last peak > 500 RFU
Ladder size (bp) 1, 1300, 10000, 17700, 21000, 23000, 42000, 50000, 165500	Quantification using: Ladder Final concentration (ng/uL): 0.0200 Dilution factor: 10.0	Minimum RFU for data processing: 1	Size threshold (b.p.): 0


Sample: blnk
Well location: H6
Created: 7/4/2026 1:57 PM

Table Information

Peak Table

Peak	Size	Concentration	From	To	Size	Percent CV	RFU	Corrected peak area
	(bp)	(pg/ul)	(bp)	(bp)	(bp)			
1	1 (LM)	Inf	772	1039	1 (LM)	2.13	407	5.487
2	269617	Inf	255537	294442	269617	3.56	113	1.818
	TIC:	Inf	Pg/ul					
	TIM:	Inf	Pmole/l					
	Total concentration:	0.0000	Pg/ul					
	DQN:	N/a (lower marker was set at time zero)						
	Threshold:	0						
Smear Analysis	10000 bp to 165000 bp	NaN pg/ul	NaN %Total	NaN pmole/L	21884 Avg. Size (bp)	90.65 %CV		
	30000 bp to 165000 bp	NaN pg/ul	NaN %Total	NaN pmole/L	55583 Avg. Size (bp)	63.62 %CV		
	1300 bp to 165000 bp	NaN pg/ul	NaN %Total	NaN pmole/L	10893 Avg. Size (bp)	117.20 %CV		
	1000 bp to 10000 bp	NaN pg/ul	NaN %Total	NaN pmole/L	6524 Avg. Size (bp)	29.36 %CV		

Sample: blnk
Well location: H7
Created: 7/4/2026 1:57 PM

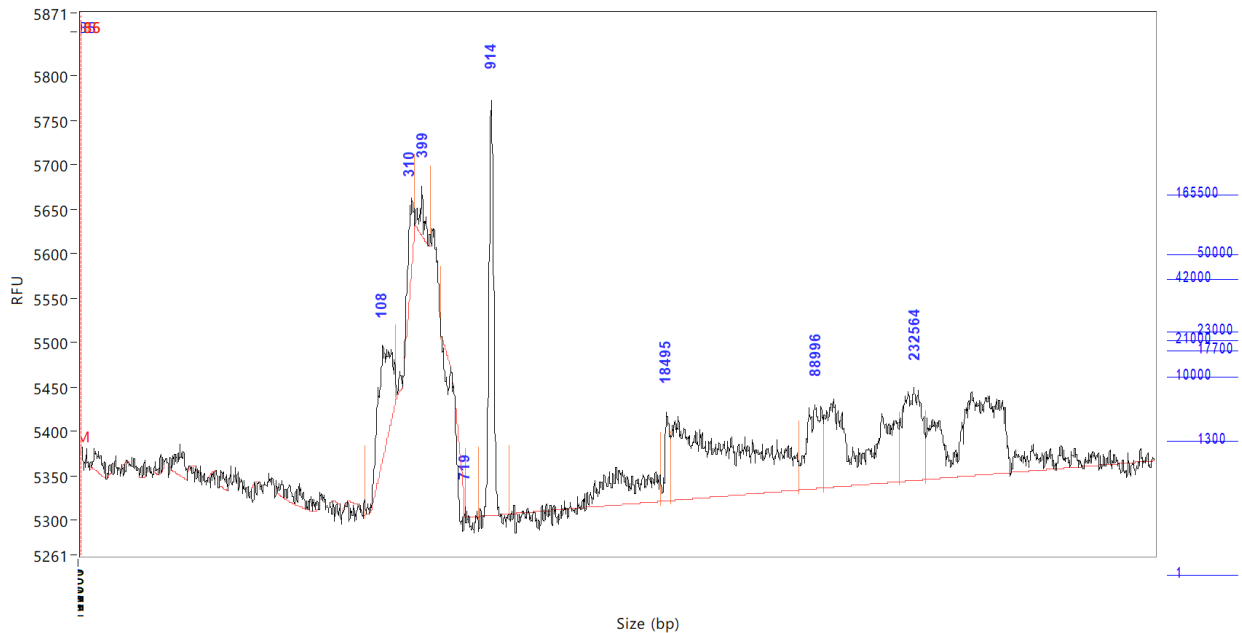

Sample Peak Width (sec): 20	Sample Min Peak Height: 50	Sample Baseline V to V?: Y	Sample Baseline V to V pts: 3
Sample filter: Binomial	Number of points for filter: 3	Sample start region (min): 0	Sample end region (min): 70
Manual baseline start (min): 25	Manual baseline end (min): 70	Marker peak width (sec): 8	Marker min peak height: 500
Marker baseline V to V?: N	Marker baseline V to V points: 3	Lower marker selection: First peak > 500 RFU	Upper marker selection: Last peak > 500 RFU
Ladder size (bp) 1, 1300, 10000, 17700, 21000, 23000, 42000, 50000, 165500	Quantification using: Ladder Final concentration (ng/uL): 0.0200 Dilution factor: 10.0	Minimum RFU for data processing: 1	Size threshold (b.p.): 0

Sample: blk
 Well location: H7
 Created: 7/4/2026 1:57 PM

Table Information

Peak Table

Peak	Size	Concentration	From	To	Size	Percent CV	RFU	Corrected peak area
	(bp)	(pg/ul)	(bp)	(bp)	(bp)			
1	1 (LM)	Inf	0	216	1 (LM)	37.25	127	6.179
2	310	Inf	216	348	310	9.25	95	2.004
3	399	Inf	348	473	399	7.01	54	0.752
4	719	Inf	547	723	719	0.25	11	0.022
5	914	Inf	819	1046	914	1.79	467	6.055
6	18495	Inf	17240	19717	18495	3.07	99	1.026
7	88996	Inf	66713	102737	88996	10.72	94	2.236
8	232564	Inf	211815	250349	232564	4.52	103	2.639


TIC: Inf Pg/ul
 TIM: Inf Pmole/l
 Total concentration: 0.0000 Pg/ul

DQN: N/a
 (lower marker was set at time zero)

Threshold: 0

Smear Analysis	10000 bp to 165000 bp	NaN pg/ul	NaN %Total	NaN pmole/L	53986 Avg. Size (bp)	73.64 %CV
	30000 bp to 165000 bp	NaN pg/ul	NaN %Total	NaN pmole/L	74115 Avg. Size (bp)	51.89 %CV
	1300 bp to 165000 bp	NaN pg/ul	NaN %Total	NaN pmole/L	49555 Avg. Size (bp)	81.05 %CV
	1000 bp to 10000 bp	NaN pg/ul	NaN %Total	NaN pmole/L	7835 Avg. Size (bp)	21.89 %CV

Sample: blnk
Well location: H8
Created: 7/4/2026 1:57 PM

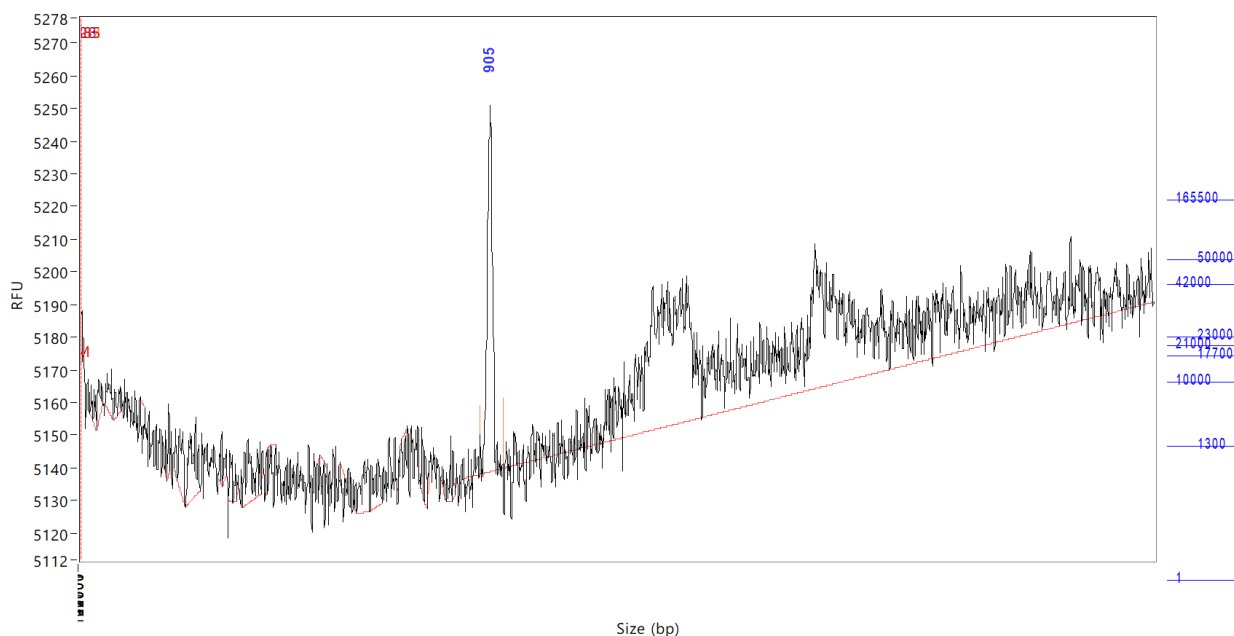


Sample Peak Width (sec): 20	Sample Min Peak Height: 50	Sample Baseline V to V?: Y	Sample Baseline V to V pts: 3
Sample filter: Binomial	Number of points for filter: 3	Sample start region (min): 0	Sample end region (min): 70
Manual baseline start (min): 25	Manual baseline end (min): 70	Marker peak width (sec): 8	Marker min peak height: 500
Marker baseline V to V?: N	Marker baseline V to V points: 3	Lower marker selection: First peak > 500 RFU	Upper marker selection: Last peak > 500 RFU
Ladder size (bp) 1, 1300, 10000, 17700, 21000, 23000, 42000, 50000, 165500	Quantification using: Ladder Final concentration (ng/uL): 0.0200 Dilution factor: 10.0	Minimum RFU for data processing: 1	Size threshold (b.p.): 0

Sample: blnk
Well location: H8
Created: 7/4/2026 1:57 PM

Table Information

Peak Table								
Peak	Size	Concentration	From	To	Size	Percent CV	RFU	Corrected peak area
	(bp)	(pg/ul)	(bp)	(bp)	(bp)			
1	1 (LM)	Inf	835	1007	1 (LM)	2.06	111	1.600
	TIC:	0.0000	Pg/ul					
	TIM:	0.0000	Pmole/l					
	Total concentration:	0.0000	Pg/ul					
	DQN:	N/a (lower marker was set at time zero)						
	Threshold:	0						
Smear Analysis	10000 bp to 165000 bp	NaN pg/ul	NaN %Total	NaN pmole/L	49885 Avg. Size (bp)	84.26 %CV		
	30000 bp to 165000 bp	NaN pg/ul	NaN %Total	NaN pmole/L	81502 Avg. Size (bp)	49.18 %CV		
	1300 bp to 165000 bp	NaN pg/ul	NaN %Total	NaN pmole/L	46235 Avg. Size (bp)	90.73 %CV		
	1000 bp to 10000 bp	NaN pg/ul	NaN %Total	NaN pmole/L	5728 Avg. Size (bp)	56.98 %CV		

Sample: blnk
Well location: H9
Created: 7/4/2026 1:57 PM

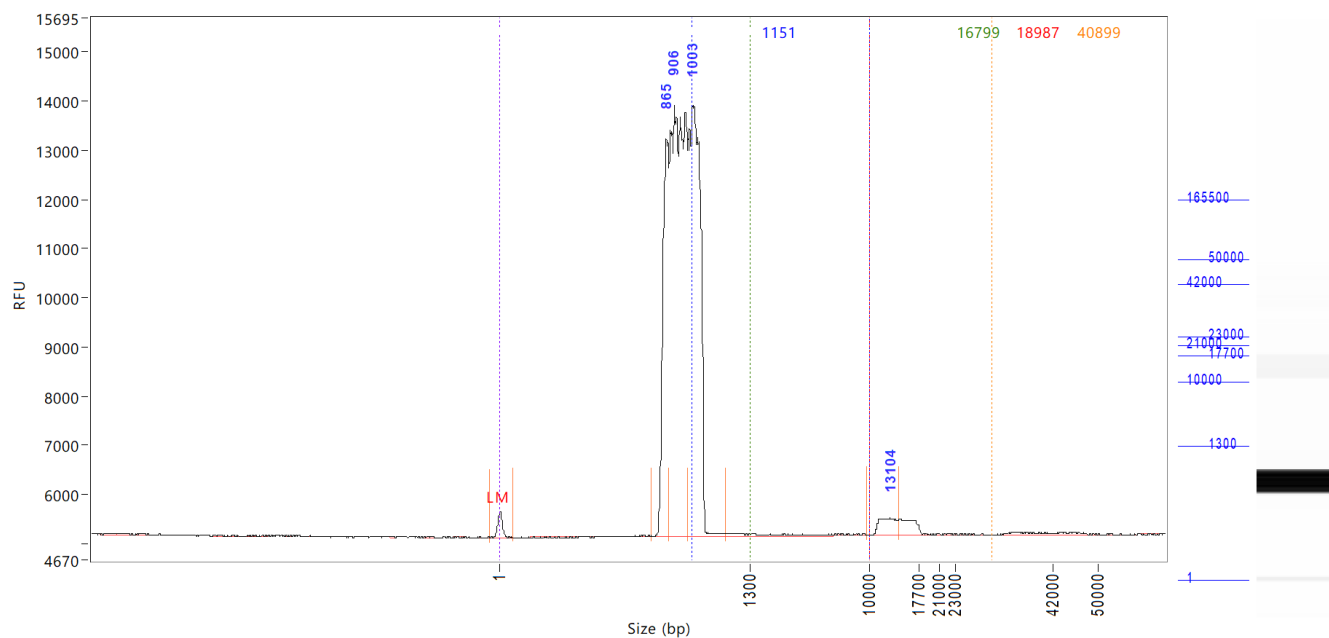

Sample Peak Width (sec): 20	Sample Min Peak Height: 50	Sample Baseline V to V?: Y	Sample Baseline V to V pts: 3
Sample filter: Binomial	Number of points for filter: 3	Sample start region (min): 0	Sample end region (min): 70
Manual baseline start (min): 25	Manual baseline end (min): 70	Marker peak width (sec): 8	Marker min peak height: 500
Marker baseline V to V?: N	Marker baseline V to V points: 3	Lower marker selection: First peak > 500 RFU	Upper marker selection: Last peak > 500 RFU
Ladder size (bp) 1, 1300, 10000, 17700, 21000, 23000, 42000, 50000, 165500	Quantification using: Ladder Final concentration (ng/uL): 0.0200 Dilution factor: 10.0	Minimum RFU for data processing: 1	Size threshold (b.p.): 0


Sample: blnk
Well location: H9
Created: 7/4/2026 1:57 PM

Table Information

Peak Table

Peak	Size	Concentration	From	To	Size	Percent CV	RFU	Corrected peak area					
	(bp)	(pg/ul)	(bp)	(bp)	(bp)								
1	1 (LM)	2.0345	0	70	1 (LM)	-6081.64	511	6.762					
2	865	286.0067	791	878	865	1.46	8098	95.062					
3	906	847.5758	878	982	906	3.27	8787	281.716					
4	1003	568.1600	982	1177	1003	2.34	8756	188.844					
5	13104	28.3274	9815	14483	13104	8.31	355	9.415					
TIC:		1730.0699	Pg/ul										
TIM:		2970.3259	Pmole/l										
Total concentration:		1767.0717	Pg/ul										
DQN:		N/a (size threshold is less than lower marker end point)											
Threshold:		0											
Smear Analysis	10000 bp to 165000 bp	65.1788 pg/ul	3.7 %Total	5.6515 pmole/L	18987 Avg. Size (bp)	55.51 %CV							
	30000 bp to 165000 bp	10.2894 pg/ul	0.6 %Total	0.4142 pmole/L	40899 Avg. Size (bp)	21.48 %CV							
	1300 bp to 165000 bp	77.3881 pg/ul	4.4 %Total	7.5843 pmole/L	16799 Avg. Size (bp)	65.10 %CV							
	1000 bp to 10000 bp	439.1665 pg/ul	24.9 %Total	627.7959 pmole/L	1151 Avg. Size (bp)	72.27 %CV							

Sample: blnk
Well location: H10
Created: 7/4/2026 1:57 PM

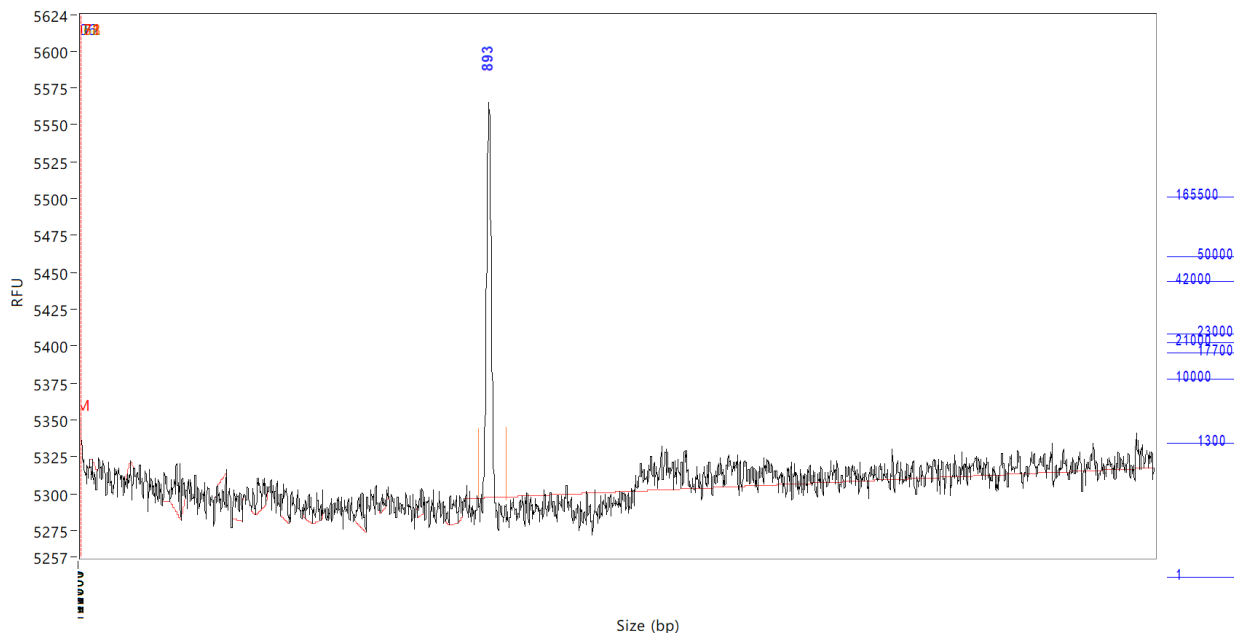


Sample Peak Width (sec): 20	Sample Min Peak Height: 50	Sample Baseline V to V?: Y	Sample Baseline V to V pts: 3
Sample filter: Binomial	Number of points for filter: 3	Sample start region (min): 0	Sample end region (min): 70
Manual baseline start (min): 25	Manual baseline end (min): 70	Marker peak width (sec): 8	Marker min peak height: 500
Marker baseline V to V?: N	Marker baseline V to V points: 3	Lower marker selection: First peak > 500 RFU	Upper marker selection: Last peak > 500 RFU
Ladder size (bp) 1, 1300, 10000, 17700, 21000, 23000, 42000, 50000, 165500	Quantification using: Ladder Final concentration (ng/uL): 0.0200 Dilution factor: 10.0	Minimum RFU for data processing: 1	Size threshold (b.p.): 0

Sample: blnk
Well location: H10
Created: 7/4/2026 1:57 PM

Table Information

Peak Table								
Peak	Size	Concentration	From	To	Size	Percent CV	RFU	Corrected peak area
	(bp)	(pg/ul)	(bp)	(bp)	(bp)			
1	1 (LM)	Inf	829	1026	1 (LM)	1.72	267	3.496
	TIC:	0.0000	Pg/ul					
	TIM:	0.0000	Pmole/l					
	Total concentration:	0.0000	Pg/ul					
	DQN:	N/a (lower marker was set at time zero)						
	Threshold:	0						
Smear Analysis	10000 bp to 165000 bp	NaN pg/ul	NaN %Total	NaN pmole/L	37971 Avg. Size (bp)	83.33 %CV		
	30000 bp to 165000 bp	NaN pg/ul	NaN %Total	NaN pmole/L	57838 Avg. Size (bp)	61.62 %CV		
	1300 bp to 165000 bp	NaN pg/ul	NaN %Total	NaN pmole/L	37862 Avg. Size (bp)	83.59 %CV		
	1000 bp to 10000 bp	NaN pg/ul	NaN %Total	NaN pmole/L	3306 Avg. Size (bp)	40.20 %CV		

Sample: blnk
Well location: H11
Created: 7/4/2026 1:57 PM

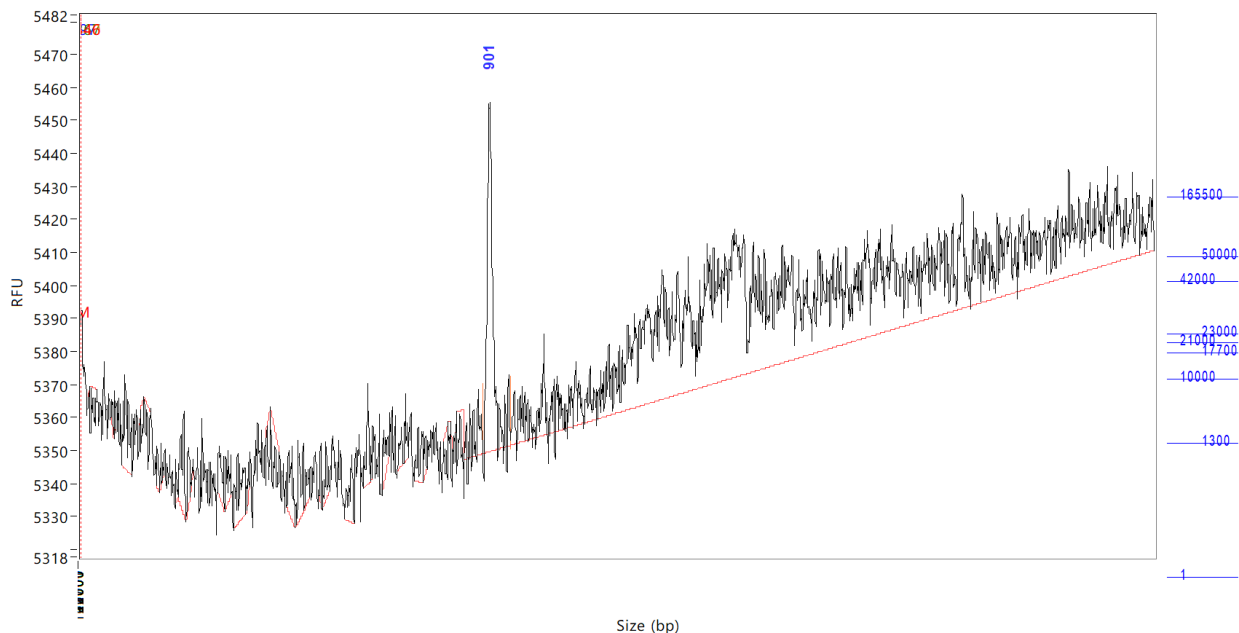

Sample Peak Width (sec): 20	Sample Min Peak Height: 50	Sample Baseline V to V?: Y	Sample Baseline V to V pts: 3
Sample filter: Binomial	Number of points for filter: 3	Sample start region (min): 0	Sample end region (min): 70
Manual baseline start (min): 25	Manual baseline end (min): 70	Marker peak width (sec): 8	Marker min peak height: 500
Marker baseline V to V?: N	Marker baseline V to V points: 3	Lower marker selection: First peak > 500 RFU	Upper marker selection: Last peak > 500 RFU
Ladder size (bp) 1, 1300, 10000, 17700, 21000, 23000, 42000, 50000, 165500	Quantification using: Ladder Final concentration (ng/uL): 0.0200 Dilution factor: 10.0	Minimum RFU for data processing: 1	Size threshold (b.p.): 0


Sample: blnk
Well location: H11
Created: 7/4/2026 1:57 PM

Table Information

Peak Table

Peak	Size	Concentration	From	To	Size	Percent CV	RFU	Corrected peak area
	(bp)	(pg/ul)	(bp)	(bp)	(bp)			
1	1 (LM)	Inf	855	1063	1 (LM)	4.20	105	1.736
	TIC:	0.0000	Pg/ul					
	TIM:	0.0000	Pmole/l					
	Total concentration:	0.0000	Pg/ul					
	DQN:	N/a (lower marker was set at time zero)						
	Threshold:	0						
Smear Analysis	10000 bp to 165000 bp	NaN pg/ul	NaN %Total	NaN pmole/L	46446 Avg. Size (bp)	80.71 %CV		
	30000 bp to 165000 bp	NaN pg/ul	NaN %Total	NaN pmole/L	64540 Avg. Size (bp)	60.47 %CV		
	1300 bp to 165000 bp	NaN pg/ul	NaN %Total	NaN pmole/L	40867 Avg. Size (bp)	91.80 %CV		
	1000 bp to 10000 bp	NaN pg/ul	NaN %Total	NaN pmole/L	4497 Avg. Size (bp)	70.99 %CV		

Sample: ladder
Well location: H12
Created: 7/4/2026 1:57 PM

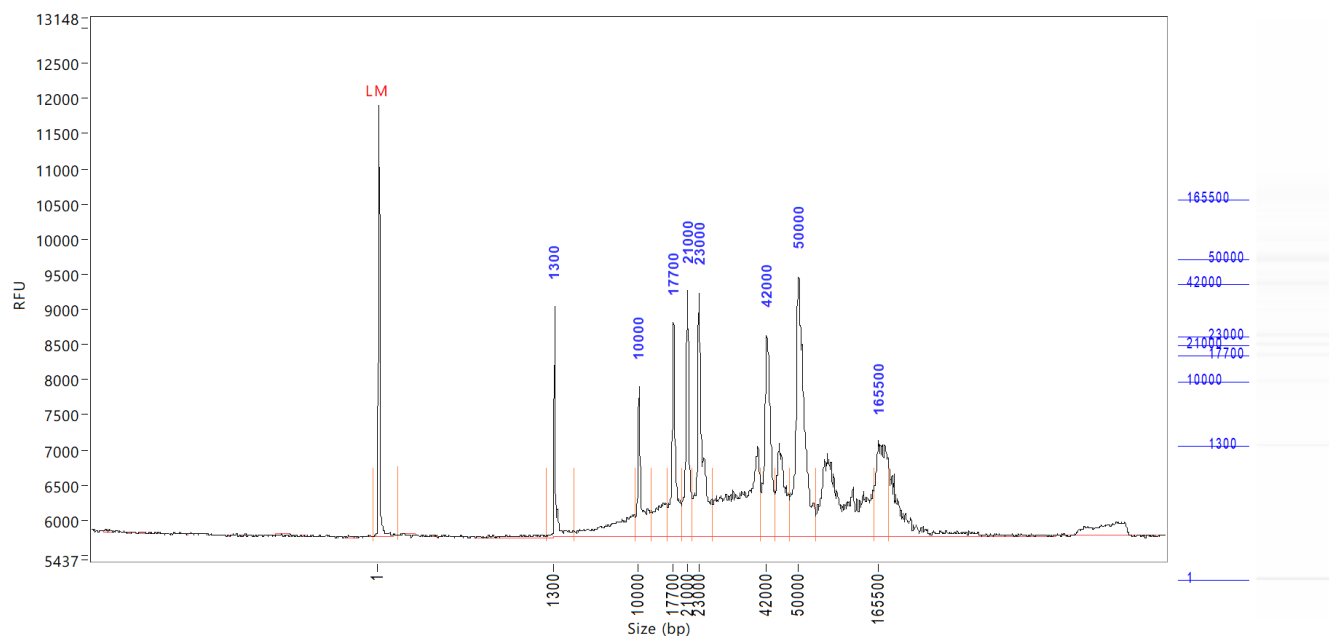

Sample Peak Width (sec): 20	Sample Min Peak Height: 1500	Sample Baseline V to V?: Y	Sample Baseline V to V pts: 3
Sample filter: Binomial	Number of points for filter: 3	Sample start region (min): 0	Sample end region (min): 70
Manual baseline start (min): 25	Manual baseline end (min): 70	Marker peak width (sec): 8	Marker min peak height: 500
Marker baseline V to V?: N	Marker baseline V to V points: 3	Lower marker selection: First peak > 500 RFU	Upper marker selection: Last peak > 500 RFU
Ladder size (bp) 1, 1300, 10000, 17700, 21000, 23000, 42000, 50000, 165500	Quantification using: Ladder Final concentration (ng/uL): 0.0200 Dilution factor: 10.0	Minimum RFU for data processing: 1	Size threshold (b.p.): 0

Sample: ladder
Well location: H12
Created: 7/4/2026 1:57 PM

Table Information

Peak Table

Peak	Size	Concentration	From	To	Size	Percent CV	RFU	Corrected peak area
	(bp)	(pg/ul)	(bp)	(bp)	(bp)			
1	1 (LM)	2.0345	0	151	1 (LM)	385.65	6147	36.690
2	1300	8.0464	1243	3284	1300	31.37	3275	14.511
3	10000	9.7556	9656	12931	10000	8.97	2131	17.593
4	17700	13.1608	16436	19595	17700	3.82	3048	23.734
5	21000	13.4367	19595	21864	21000	2.23	3505	24.231
6	23000	19.7868	21864	26815	23000	4.99	3464	35.683
7	42000	17.0887	40489	44130	42000	1.90	2870	30.817
8	50000	28.3636	47678	74141	50000	11.26	3693	51.150
9	165500	12.2090	158444	180691	165500	3.59	1357	22.017
TIC:		121.8477	Pg/ul					
TIM:		15.2736	Pmole/l					
Total concentration:		200.0000	Pg/ul					

Sample: ladder
Well location: H12
Created: 7/4/2026 1:57 PM
Fit type: Point to Point

Calibration Curve

