


discrete_dose — standard-error calibration

β correct; λ correct
 ω correct; m correct

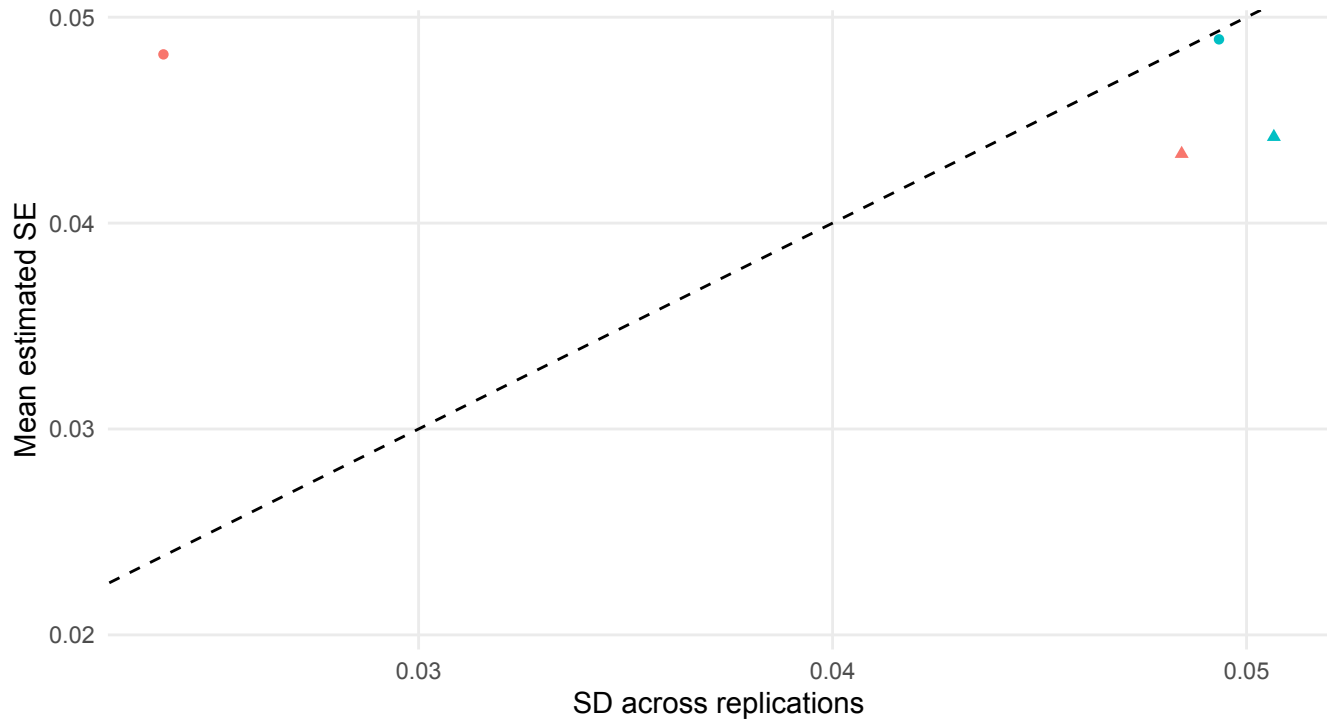

estimator ● sdr ● tmle n ● 500 ▲ 1000 ■ 4000