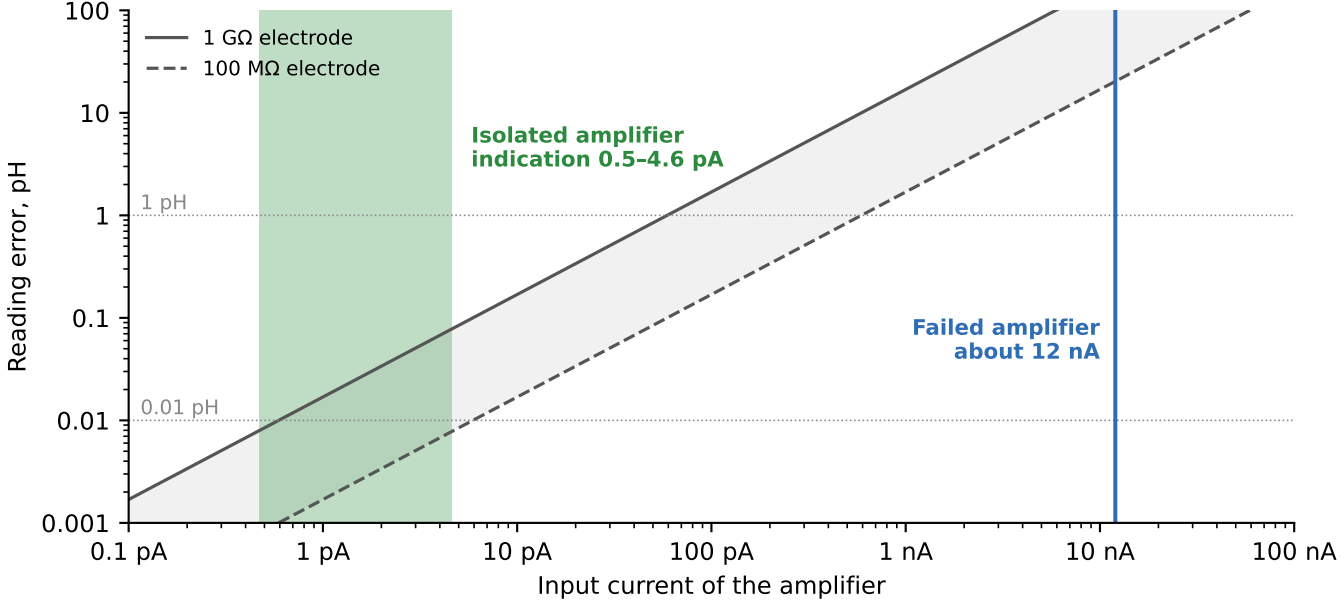
1 GΩ electrode
100 MΩ electrode
Isolated amplifier
indication 0.5–4.6 pA
Failed amplifier
about 12 nA
1 pH
0.01 pH
Reading error, pH
100
10
1
0.1
0.01
0.001
0.1 pA
1 pA
10 pA
100 pA
1 nA
10 nA
100 nA
Input current of the amplifier