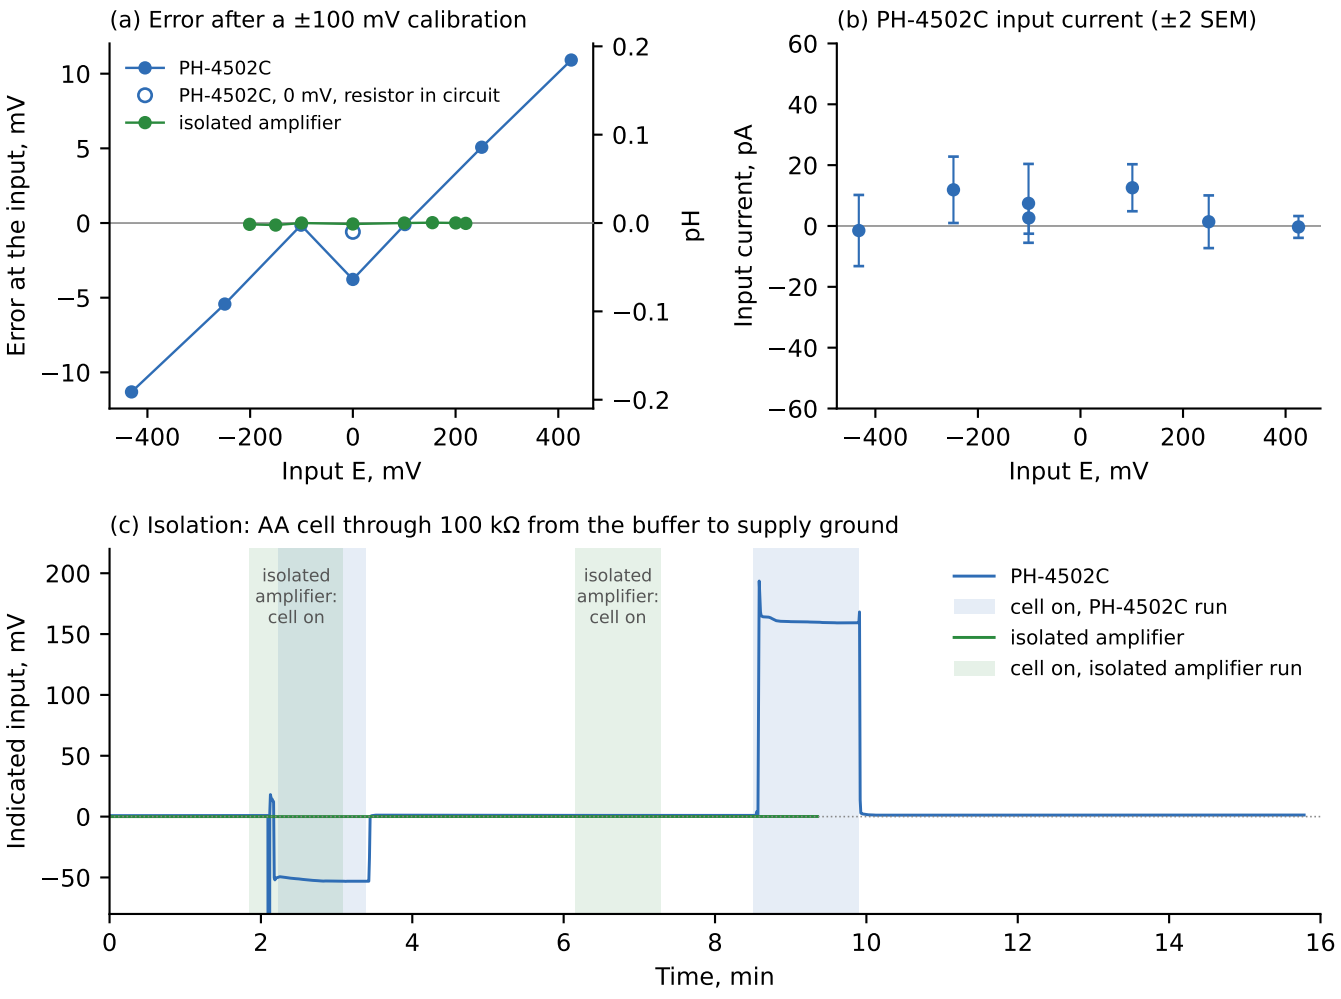
(a) Error after a ±100 mV calibration
PH-4502C
PH-4502C, 0 mV, resistor in circuit
isolated amplifier
Error at the input, mV
pH
Input E, mV
(b) PH-4502C input current (±2 SEM)
Input current, pA
Input E, mV
(c) Isolation: AA cell through 100 kΩ from the buffer to supply ground
isolated amplifier: cell on
isolated amplifier: cell on
PH-4502C
cell on, PH-4502C run
isolated amplifier
cell on, isolated amplifier run
Indicated input, mV
Time, min