

63X\_1\_4\_525

### Microscope info:

| Image  |             | Image4_bead7            |             |            |                       |                      |                     |  |
|--|-------------|-------------------------|-------------|------------|-----------------------|----------------------|---------------------|--|
| image's date 2024-10-17 10:22:18                   |             |                         |             |            |                       |                      |                     |  |
| creation   | method used | from file creation date |             |            |                       |                      |                     |  |
| Actual image depth                                 |             | 16                      |             |            |                       |                      |                     |  |
| Microscope type                                    |             | WideField               |             |            |                       |                      |                     |  |
|  | NA          | 1.4                     | 1.4         |            |                       |                      |                     |  |
| Objective im. refractive index 1.518               |             |                         |             |            |                       |                      |                     |  |
|  |             | Wavel                   | engths      |            | sampling (X,Y,Z)      |                      |                     |  |
| Chan   | nel(s)      | Ex.<br>(nm)             | Em.<br>(nm) | Saturation | Nyquist (µm)          | Found (µm)           | Nyquist/found ratio |  |
| Channel 0  |             |                         | 525.0       | none       | 0.094x0.094x0.<br>282 | 0.063x0.063x0.<br>06 | 0.7, 0.7, 0.2       |  |
| Bead original coordinates(in pixels) 1251.0, 691.0 |             |                         |             |            |                       |                      |                     |  |

# Warnings:

(No saturated pixels detected). (All channels sampled following Shannon-Nyquist criterion). (A subresolution bead is used for all channels).

#### Resolution table:

| Channel                    | Sig/Backgn<br>d ratio | Dimension | Measured<br>FWHM<br>(µm) | theory (µm) | Fit<br>Goodness | Mes./theory ratio |
|----------------------------|-----------------------|-----------|--------------------------|-------------|-----------------|-------------------|
|                            |                       | Х         | 0.225                    | 0.191       | 1.0             | 1.18              |
| Channel 0 (em.<br>525.0nm) |                       | Υ         | 0.234                    | 0.191       | 1.0             | 1.22              |
|                            |                       | Z         | 0.482                    | 0.72        | 0.99            | 0.67              |


Green: within specifications, red: outside specifications (ie. XY ratios above 1.5 or Z ratio above 2.0)

#### Lateral asymmetry ratios:

| Channel                 | Ratio |  |
|-------------------------|-------|--|
| Channel 0 (em. 525.0nm) | 0.96  |  |

# Detailed channel detection info:


# Channel #0







| Channel 0 (em. 525.0nm) |     |               |   |  |  |
|-------------------------|-----|---------------|---|--|--|
| Sig./Backgnd LAR        |     | FWHM          | Fit goodness                                |  |  |
|                         | X   | 0.225         | 1.0   |  |  |
| 0.96                    | Υ   | 0.234         | 1.0   |  |  |
|                         | Z   | 0.482         | 0.99  |  |  |
|                         | LAR | LAR Dimension | LAR Dimension FWHM   X 0.225   0.96 Y 0.234 |  |  |

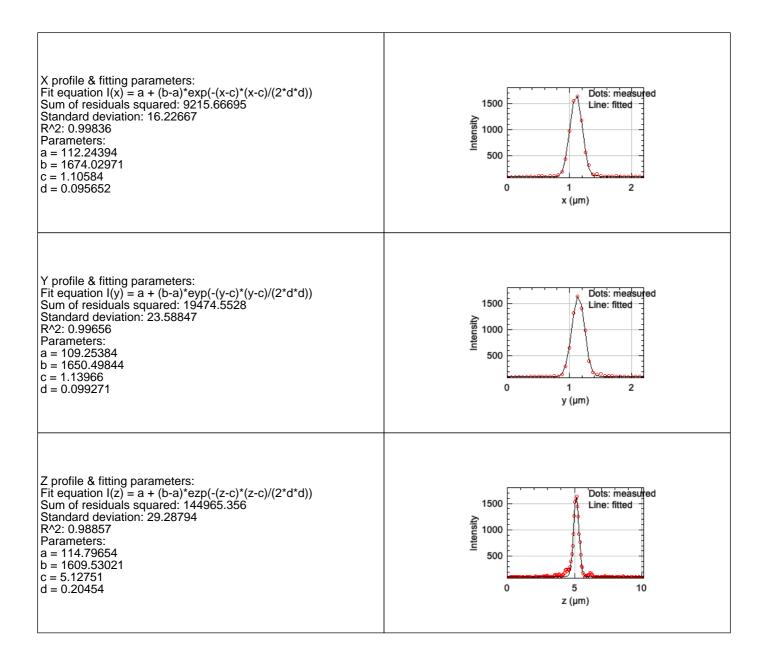

#### Analysis parameters

|                                 | Tool   | PSF Profiler (batch)  |  |  |  |  |
|---------------------------------|--|---|--|--|--|--|
| Tool &<br>Operator              | Versions   | MetroloJ_QC v1.3.1.1, ImageJ v2.14.0/1.54f, Java v1.8.0_322, OS Mac OS X  |  |  |  |  |
|                                 | Operator & date  | SO, October 25, 2024 2:35 PM  |  |  |  |  |
| data                            | result folder  | /Users/oggsc/Documents/OM/ImageAnalysis/QC/Elyra/PSFs/20241014/63X_1_4/525//Processed/63X_1_4_525/Image4/bead7/ |  |  |  |  |
| data                            | Type of saved data                                     | .pdf, .jpg, .xls  |  |  |  |  |
|                                 | Input data bit depth                                   | 16  |  |  |  |  |
| Dim                             | ension order   | XY-(C)Z   |  |  |  |  |
| Discard s                       | aturated samples                                       | false   |  |  |  |  |
|                                 | Bead detection threshold                               | Legacy  |  |  |  |  |
|                                 | Center detection method                                | Legacy Maximum Intensity  |  |  |  |  |
|                                 | Discard bead if more than one particle are thresholded | true  |  |  |  |  |
|                                 | Background annulus<br>thickness in µm                  | 0.5   |  |  |  |  |
| Beads                           | Background annulus<br>distance to bead edges<br>in µm  | 0.5   |  |  |  |  |
| Deads                           | Multiple beads in image                                | true  |  |  |  |  |
|                                 | Bead identification method                             | Using Find Maxima (prominence of 1000.0)  |  |  |  |  |
|                                 | Bead size (µm)   | 0.1   |  |  |  |  |
|                                 | Bead crop Factor                                       | 5.0   |  |  |  |  |
|                                 | Cropped ROI size in µm                                 | 2.31x2.31 (using bead size & background annulus parameters)   |  |  |  |  |
|                                 | Bead rejection distance to top/bottom                  | 2.0 μm  |  |  |  |  |
| Square Root PSF Image displayed |  | true  |  |  |  |  |
|                                 | Applied in this report                                 | true  |  |  |  |  |
| Tolerance                       | X & Y FWHM ratios valid if below                       | 1.5   |  |  |  |  |
|                                 | Z FWHM ratio valid if below                            | 2.0   |  |  |  |  |

# Analysis log

| image name    | creation<br>date       | saturation | sampling density | status   |
|---------------|------------------------|------------|------------------|----------|
| Image 4_bead7 | 2024-10-17<br>10:22:18 | none       | correct          | analysed |

#### Formulas used:

Lateral  $(res_{x,y}^o)$  and axial  $(res_z^o)$  theoretical resolution values used for widefield microscopes are calculated as defined in Wilhelm, S. Confocal Laser Scanning Microscopy, 2011:

$$res_{x,y}^o = \frac{0.51*\lambda_{em}}{NA}$$
  $res_z^o = \frac{1,77n*\lambda_{em}}{NA^2}$ 

NA: numerical aperture,  $\lambda_{em}$ : emission wavelength, n: refractive index of the lens immersion & mounting media.

Axis profiles are fitted using ImageJ Gaussian Curve Fitter and the following formula  $y = a + (b - a) * e^{\frac{-(x-c)^2}{2d^2}}$  (Gaussian fitting).

Measured lateral and axial resolution (Full Width at Half Maximum, FWHM) values are derived using FWHM =  $2d\sqrt{2ln(2)}$ 

Compliance with the Shannon-Nyquist criterion uses the following formulas for Shannon-Nyquist distances calculation:

$$\alpha = \arcsin(\frac{NA}{n})$$

$$\Delta_{x,y} = \frac{\lambda_{em}}{4.NA} \qquad \Delta_z = \frac{\lambda_{em}}{2.n. (1-\cos{(\alpha)})}$$