


Plan: BREAST^BOLUS/BreastBolus
Structure Set: BREAST^BOLUS/BreastBolus
Dose (Reference): BREAST^BOLUS/BreastBolus /RTDose
Dose (Comparison): BREAST^BOLUS/BreastBolus /RTDose
Report Generated: 2026/03/05 11:08:52
Reviewed by: _____

Dose Difference View

% Difference: 3% / Global Normalization (55.6725 Gy) / Lower TH = 10%
Distance Criterion: 2.0 mm Method: Gamma

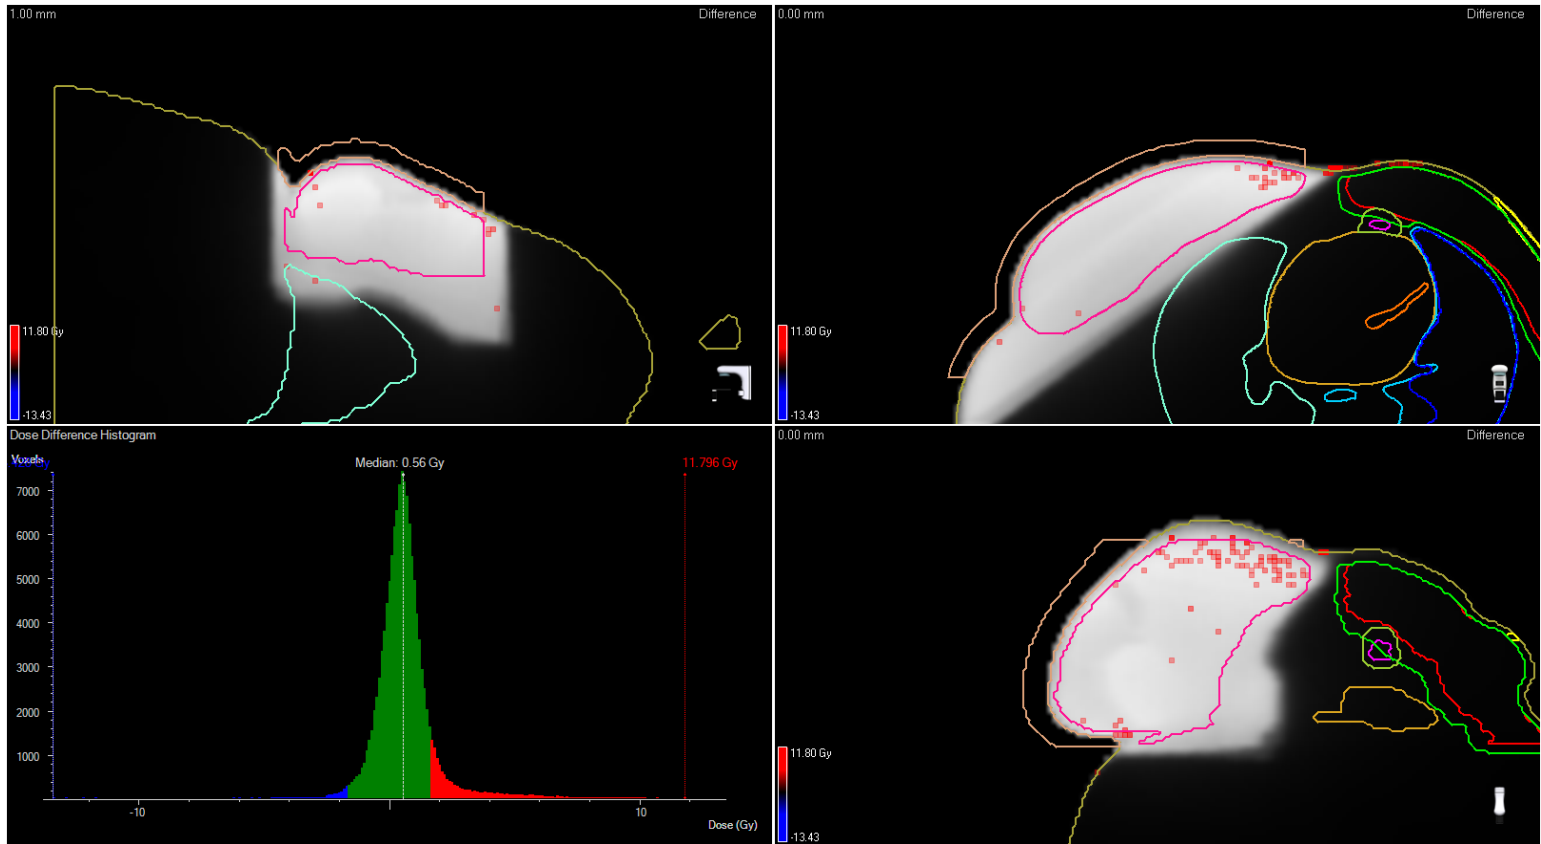

Dose Grid Info

REFERENCE (PRIMARY) DOSE...

Dose Grid Resolution & Size (IEC Couch Coordinate System*):


Grid Spacing (X):	3.000 mm	X Range (mm):	[-166.500-->442.500]	*X along width of couch
Grid Spacing (Y):	3.000 mm	Y Range (mm):	[-214.500-->226.500]	*Y along long axis of couch
Grid Spacing (Z):	3.000 mm	Z Range (mm):	[-232.500-->106.500]	*Z normal to couch surface
Dose Min --> Max:	0.0000 --> 55.6725 Gy			

COMPARISON (SECONDARY) DOSE...

Dose Grid Resolution & Size (IEC Couch Coordinate System*):

Grid Spacing (X):	3.000 mm	X Range (mm):	[-166.500-->442.500]	*X along width of couch
Grid Spacing (Y):	3.000 mm	Y Range (mm):	[-214.500-->226.500]	*Y along long axis of couch
Grid Spacing (Z):	3.000 mm	Z Range (mm):	[-232.500-->106.500]	*Z normal to couch surface
Dose Min --> Max:	0.0000 --> 57.8108 Gy			

Plan: BREAST^BOLUS/BreastBolus
Structure Set: BREAST^BOLUS/BreastBolus
Dose (Reference): BREAST^BOLUS/BreastBolus /RTDose
Dose (Comparison): BREAST^BOLUS/BreastBolus /RTDose
Report Generated: 2026/03/05 11:08:52
Reviewed by: _____

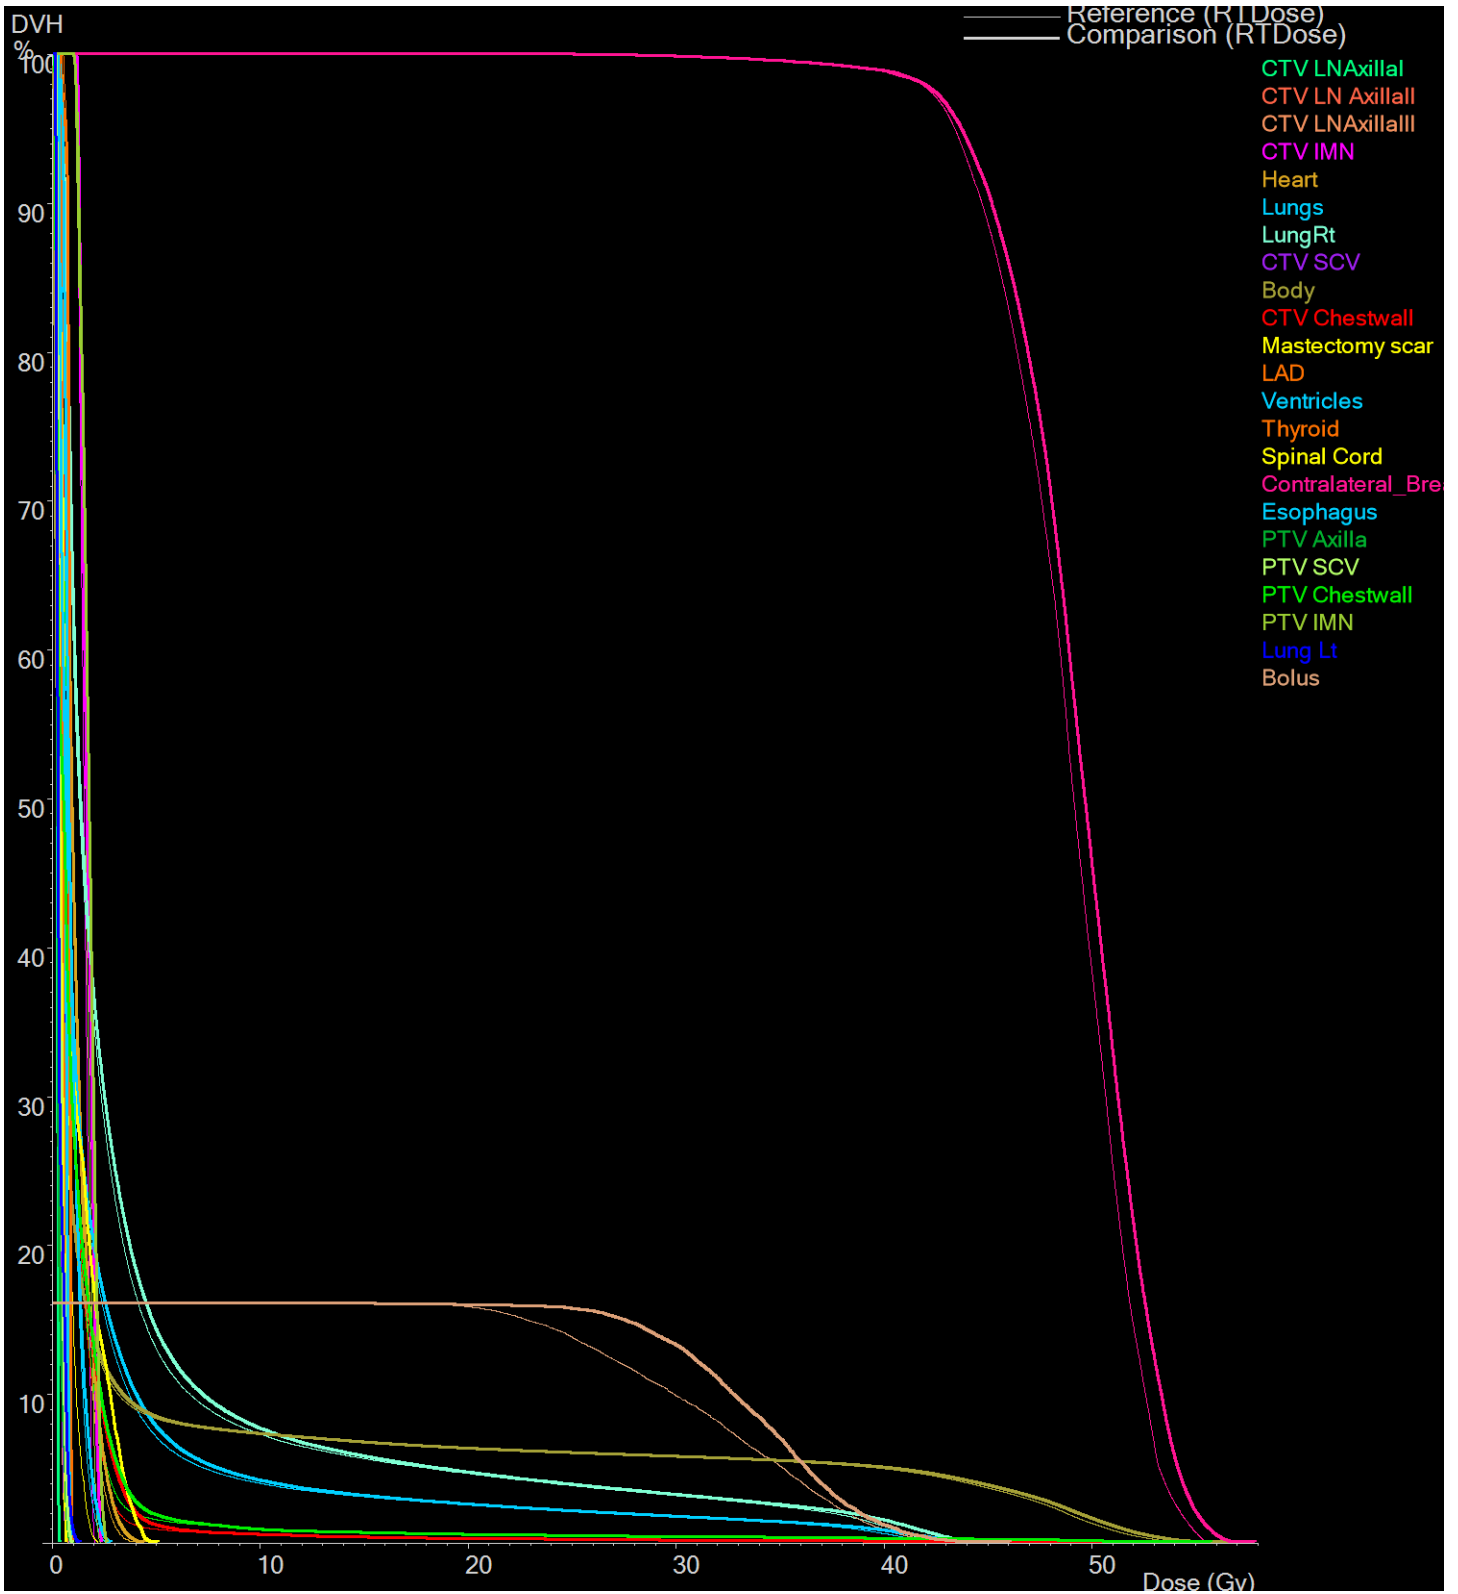

Plan: BREAST^BOLUS/BreastBolus
 Structure Set: BREAST^BOLUS/BreastBolus
 Dose (Reference): BREAST^BOLUS/BreastBolus /RTDose
 Dose (Comparison): BREAST^BOLUS/BreastBolus /RTDose
 Report Generated: 2026/03/05 11:08:52
 Reviewed by: _____

Comparison Parameters

% Difference: 3% / Global Normalization (55.6725 Gy) / Lower TH = 10%
 DTA Criterion: 2.0 mm
 Method: Gamma

Comparison Results: Main

Results: 97.6% Matching Rate (121 329 of 124 363 voxels, 3 012 high, 22 low)

Comparison Results: Per Anatomy ROI

ROI Name	Matching Rate (%)	Matching	High	Low	Total
CTV LNAxillaI		0	0	0	0
CTV LN AxillaII		0	0	0	0
CTV LNAxillaIII		0	0	0	0
CTV IMN		0	0	0	0
Heart		0	0	0	0
Lungs	97.8	6539	148	0	6687
LungRt	97.8	6539	148	0	6687
CTV SCV		0	0	0	0
Body	97.7	116307	2733	18	119058
CTV Chestwall	95.7	312	14	0	326
Mastectomy scar		0	0	0	0
LAD		0	0	0	0
Ventricles		0	0	0	0
Thyroid		0	0	0	0
Spinal Cord		0	0	0	0
Contralateral_Breast	97.7	38950	904	0	39854
Esophagus		0	0	0	0
PTV Axilla		0	0	0	0
PTV SCV		0	0	0	0
PTV Chestwall	94.1	665	42	0	707
PTV IMN		0	0	0	0
Lung Lt		0	0	0	0
Bolus	98.4	2649	43	0	2692

Plan: BREAST^BOLUS/BreastBolus
Structure Set: BREAST^BOLUS/BreastBolus
Dose (Reference): BREAST^BOLUS/BreastBolus /RTDose
Dose (Comparison): BREAST^BOLUS/BreastBolus /RTDose
Report Generated: 2026/03/05 11:08:52
Reviewed by: _____

----- Reference Data Sources -----

RTPlan

File: RTPLAN_2.16.840.1.114337.1.13408.1772674969.0.dcm

Dir: ~~C:\ProgramData\Sun Nuclear Patient Plans~~ BreastBolus_CCC

RTStructureSet

File: RTSTRUCT_2.16.840.1.114337.1.13408.1772674963.0.dcm

Dir: ~~C:\ProgramData\Sun Nuclear Patient Plans~~ BreastBolus_CCC

RTDose

File: RTDOSE_2.16.840.1.114337.1.13408.1772674969.1.dcm

Dir: ~~C:\ProgramData\Sun Nuclear Patient Plans~~ BreastBolus_CCC

Dose Grid Resolution & Size (IEC Couch Coordinate System*):

Grid Spacing (X):	3.000 mm	X Range (mm):	[-166.500-->442.500]	*X along width of couch
Grid Spacing (Y):	3.000 mm	Y Range (mm):	[-214.500-->226.500]	*Y along long axis of couch
Grid Spacing (Z):	3.000 mm	Z Range (mm):	[-232.500-->106.500]	*Z normal to couch surface
Dose Min --> Max:	0.0000 --> 55.6725 Gy			

----- Comparison Data Sources -----

RTDose

File: RTDOSE_2.16.840.1.114337.1.13408.1772675251.1.dcm

Dir: ~~C:\ProgramData\Sun Nuclear Patient Plans~~ BreastBolus_MC

Dose Grid Resolution & Size (IEC Couch Coordinate System*):

Grid Spacing (X):	3.000 mm	X Range (mm):	[-166.500-->442.500]	*X along width of couch
Grid Spacing (Y):	3.000 mm	Y Range (mm):	[-214.500-->226.500]	*Y along long axis of couch
Grid Spacing (Z):	3.000 mm	Z Range (mm):	[-232.500-->106.500]	*Z normal to couch surface
Dose Min --> Max:	0.0000 --> 57.8108 Gy			