

Eleven Primitives and Three Gates: The Universal Structure of Computational Imaging

Chengshuai Yang^{1,*}

David J. Brady²

Xin Yuan³

¹NextGen PlatformAI C Corp, USA. ²School of Electrical and Computer Engineering, University of Arizona, Tucson, AZ, USA. ³School of Engineering, Westlake University, Hangzhou, China.

*Correspondence: integrityyang@gmail.com

Abstract

Computational imaging systems—from coded-aperture cameras to cryo-electron microscopes—span five carrier families yet share a hidden structural simplicity. We prove that every imaging forward model decomposes into a directed acyclic graph over exactly 11 physically typed primitives (Finite Primitive Basis Theorem)—a sufficient and minimal basis that provides a compositional language for designing any imaging modality¹. We further prove that every reconstruction failure has exactly three independent root causes: information deficiency, carrier noise, and operator mismatch (Triad Decomposition). The three gates map to the system lifecycle: Gates 1 and 2 guide design (sampling geometry, carrier selection); Gate 3 governs deployment-stage calibration and drift correction. Validation across 12 modalities and all five carrier families confirms both results, with +0.8 to +13.9 dB recovery on deployed instruments. Together, the 11 primitives and 3 gates establish the first universal grammar for designing, diagnosing, and correcting computational imaging systems.

Introduction

A coded-aperture camera, an MRI scanner, and a cryo-electron microscope appear to share nothing: they employ different physical carriers, different geometries, and different detectors. Yet each converts a physical scene into digital measurements by composing a small chain of transformations—propagation, interaction, encoding, detection—and each reconstructs the scene by inverting a mathematical model of that chain. When the model matches reality, modern algorithms deliver extraordinary results. When it does not—and on deployed instruments, it never perfectly does—reconstruction degrades or fails entirely. The failure is silent and systematic: the algorithm faithfully solves the wrong problem. Despite a decade of progress in reconstruction algorithms, no general framework exists to explain *why* a reconstruction failed, *where* in the forward model the error resides, or *how* to fix it without retraining the solver.

This paper establishes that the space of imaging forward models has a surprisingly simple and universal structure—a finite grammar of 11 primitives—and that every reconstruction failure admits a complete, actionable diagnosis through exactly 3 independent gates. Over the past decade, the community has invested enormous effort in improving reconstruction algorithms—progressing from compressed sensing^{2,3} and plug-and-play priors^{4,5} to deep unrolling networks⁶ and vision transformers⁷—with snapshot compressive imaging emerging as a unifying framework for coded aperture systems⁸. These advances are real and important: a better solver on a well-calibrated operator remains the gold standard. Yet algorithms routinely fail when deployed on real instruments⁹, and the

root cause is often not the algorithm but an undiagnosed forward-model error. Calibration methods exist for specific instruments—ESPIRiT¹⁰ for MRI, ePIE¹¹ for electron ptychography—but they do not generalise across modalities, and no systematic framework decomposes reconstruction failures into root causes or guides the design of new imaging systems from first principles.

Here we establish two complementary foundations within Physics World Models (PWM). The **Finite Primitive Basis Theorem** (Theorem 1) proves that every imaging forward model in a broad operator class $\mathcal{C}_{\text{img}}$ admits an ε -approximate representation as a typed directed acyclic graph (DAG) over exactly 11 canonical primitives—and that this library is minimal¹. The **Triad Decomposition** proves that every reconstruction failure decomposes into three gates—information deficiency (**Gate 1**), carrier noise (**Gate 2**), and operator mismatch (**Gate 3**)—each independently testable and independently addressable. The 11 primitives *enable* the 3-gate diagnosis: the DAG structure localizes each gate to specific physical operators, making both design and correction actionable.

The framework serves dual purposes (Figure 1). For **existing instruments**, the Triad identifies the dominant gate and prescribes targeted intervention—calibration for Gate 3, acquisition redesign for Gate 1, or source/detector improvement for Gate 2. For **new instruments**, the 11-primitive basis provides a compositional design language: specifying a new modality reduces to selecting primitives and their parameters, with Gate 1 analysis guiding sampling strategy, Gate 2 guiding carrier and source selection, and Gate 3 predicting the calibration accuracy required for a target reconstruction quality. Solver design remains essential throughout: once the dominant gate is addressed, a better solver delivers further gains on the corrected operator.

We validate both results—the Finite Primitive Basis Theorem (every forward model decomposes into 11 primitives) and the Triad Decomposition (every reconstruction failure has exactly three root causes)—across twelve modalities spanning all five carrier families—optical photons (CASSI¹², CACTI¹³, SPC¹⁴, lensless imaging, compressive holography, fluorescence microscopy), X-ray photons (CT¹⁵, CBCT), electrons (electron ptychography¹⁶, cryo-EM), nuclear spins (MRI^{17,18}), and acoustic waves (ultrasound)—with hardware validation on all twelve modalities confirming Triad predictions on physical measurements. The validated modalities include two Nobel Prize-winning techniques (cryo-EM, 2017 Chemistry; super-resolution fluorescence, 2014 Chemistry), three clinically deployed instruments (CT, CBCT, MRI), and the first acoustic-carrier validation in computational imaging. A held-out closure test on 8 additional modalities confirms basis completeness with saturating growth. The proof of Theorem 1 is in Supplementary Note 12; formal primitive semantics and typed DAG denotation are developed in¹.

Generalization beyond imaging. The finite-basis result raises a natural question: do other measurement domains admit similarly compact primitive decompositions? The OPERATORGRAPH formalism and Triad Decomposition are structurally applicable wherever a forward model maps quantities of interest to observations through composable physical stages. Seismology (wave propagation + attenuation + sensor response), radio astronomy (aperture synthesis + ionospheric distortion + noise), and particle physics (interaction model + detector response + pile-up) all exhibit the same three-gate failure structure. Whether these domains also admit small primitive bases is an empirical question that our framework is designed to answer.

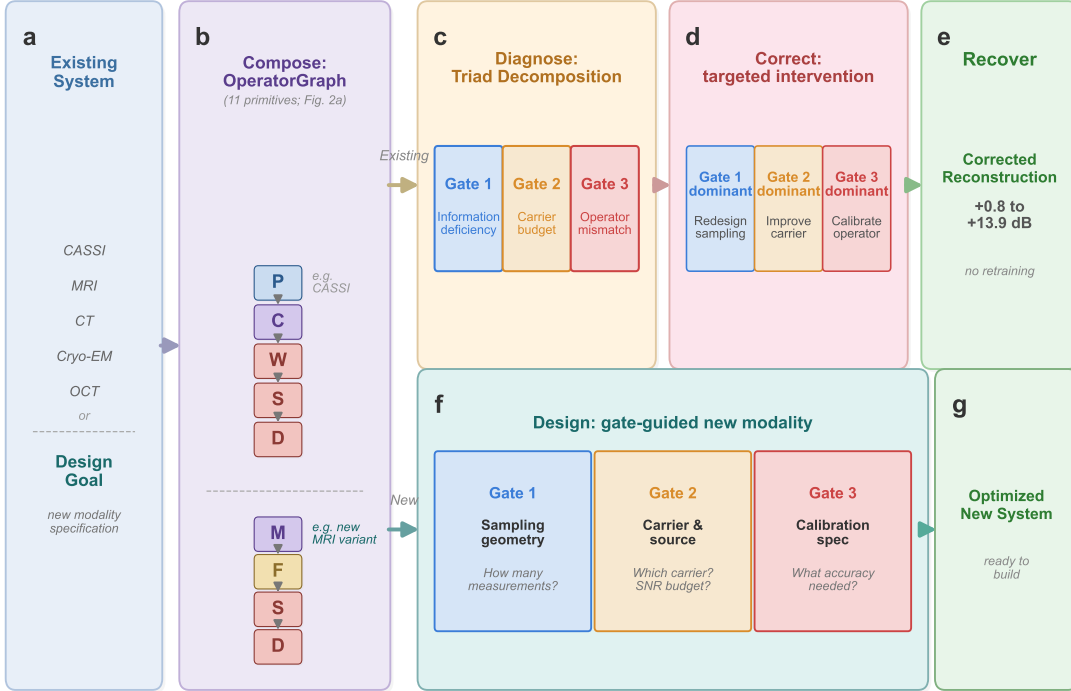


Figure 1: **The universal grammar of computational imaging.** **a**, Any computational imaging system—from coded-aperture cameras to cryo-electron microscopes—serves as input. **b**, The system is composed as a typed directed acyclic graph (DAG) over 11 universal primitives (Figure 2); shown here for CASSI as an example. The grammar enables two workflows. *Top (existing instruments)*: **c**, The TRIAD DECOMPOSITION diagnoses the DAG through three independent gates: information deficiency (Gate 1), carrier budget (Gate 2), and operator mismatch (Gate 3). **d**, Based on the dominant gate, a targeted correction is applied: sampling redesign (Gate 1), source/detector improvement (Gate 2), or operator calibration (Gate 3). **e**, The existing solver is re-run with the corrected operator, recovering +0.8 to +13.9 dB without retraining. *Bottom (new instruments)*: **f**, The same three gates guide the design of a new modality from first principles: Gate 1 determines sampling geometry, Gate 2 guides carrier and source selection, and Gate 3 predicts the calibration accuracy required for a target reconstruction quality. **g**, The output is an optimized new system specification ready to build. Together, the 11 primitives (alphabet) and 3 gates (rules) form a universal grammar for designing, diagnosing, and correcting any imaging system.

The Finite Primitive Basis

A foundational question in computational imaging is whether the diversity of imaging forward models—from coded aperture cameras to MRI scanners to electron microscopes—can be captured by a small, fixed set of primitive operators. We answer affirmatively.

The OperatorGraph representation. Every imaging forward model is encoded as a typed directed acyclic graph (DAG) in which each node wraps a single primitive physical operator and edges define the data flow from source to detector. Every primitive implements both a `forward()` and

an `adjoint()` method, with validated adjoint consistency ensuring $\langle H\mathbf{x}, \mathbf{y} \rangle = \langle \mathbf{x}, H^\dagger \mathbf{y} \rangle$ to within numerical precision. Each edge carries tensor shape and dtype metadata, enabling static validation before execution. We call this formalism the OPERATORGRAPH intermediate representation (IR).

Eleven canonical primitives. The OPERATORGRAPH IR defines a library of exactly 11 canonical primitives $\mathcal{B} = \{P, M, \Pi, F, C, \Sigma, D, S, W, R, \Lambda\}$:

#	Primitive	Notation	Physical action
1	Propagate	$P(d, \lambda)$	Free-space wave propagation
2	Modulate	$M(\mathbf{m})$	Element-wise multiplication (mask, coil, absorption)
3	Project	$\Pi(\theta)$	Radon line-integral projection
4	Encode	$F(\mathbf{k})$	Fourier-domain encoding (k -space)
5	Convolve	$C(\mathbf{h})$	Spatial convolution (PSF)
6	Accumulate	Σ	Summation over spectral/temporal axis
7	Detect	$D(g, \eta)$	Detector response (5 canonical families)
8	Sample	$S(\Omega)$	Sub-sampling on index set Ω
9	Disperse	$W(\alpha, a)$	Wavelength-dependent spatial shift
10	Scatter	$R(\sigma, \Delta\varepsilon)$	Direction change and/or energy shift
11	Transform	$\Lambda(f, \theta)$	Pointwise nonlinear physics operation

The Detect nonlinearity η is restricted to five canonical families (linear-field: $\eta(x) = gx$; logarithmic; sigmoid; intensity-square-law: $\eta(x) = g|x|^2$; coherent-field), each with at most 2 scalar parameters. The Transform primitive Λ applies a pointwise nonlinear function within the physics chain (not at the detector) and is restricted to five families: exponential attenuation ($e^{-\alpha x}$, Beer–Lambert), logarithmic compression, phase wrapping ($\arg(e^{ix})$), polynomial ($\sum a_k x^k$, $d \leq 5$), and saturation. Both Detect and Transform are pointwise and parameter-limited, preventing either from becoming a universal approximator (see¹ for formal definitions and non-universality proofs).

Physics-stage mapping. Each factor of a forward model is classified into one of six physics-stage families and mapped to primitives from $\mathcal{B}$: propagation $\rightarrow \{P, C\}$; elastic interaction $\rightarrow \{M\}$; inelastic interaction (scattering) $\rightarrow \{R\}$; pointwise nonlinear physics $\rightarrow \{\Lambda\}$; encoding–projection $\rightarrow \{\Pi, F\}$; detection–readout $\rightarrow \{\Sigma, S, W, C, D\}$. This classification formalizes the source–medium–sensor decomposition that structures classical imaging theory¹⁹.

Fidelity levels. Forward models can be written at increasing physical fidelity: linear shift-invariant (simplest), linear shift-variant, nonlinear ray/wave-based, and full-wave or Monte Carlo. All 11 primitives apply uniformly across every fidelity level. Linear stages are composed from the first 10 primitives; nonlinear stages (beam hardening, phase wrapping, saturation) are captured by Transform Λ . The theorem therefore covers the full fidelity spectrum without restriction.

Physical carriers. The template library spans five carrier families—optical photons, X-ray photons, electrons, nuclear spins, and acoustic waves—with particle-beam probes (neutrons, protons, muons) representable in the extended registry using *zero new primitives*: neutron CT reuses the X-ray CT DAG ($P \rightarrow \Lambda \rightarrow D$) with nuclear cross-section parameters; proton CT inserts a Bethe–Bloch stopping-power stage via Transform Λ (#11); muon tomography uses Scatter R (#10, already introduced for Compton imaging) for multiple Coulomb scattering and POCA reconstruction (Supplementary Note S24). In total, 170 modality templates cover 23 categories (microscopy, medical imaging, electron microscopy, remote sensing, spectroscopy, and others; see¹), of which 12 now

have full end-to-end correction validation across all five primary carrier families (Supplementary Table S3).

Theorem statement.

Definition 1 (Imaging Operator Class). $\mathcal{C}_{\text{img}}$ consists of all imaging forward models expressible as a finite sequential-parallel composition of stages—each either linear with bounded operator norm ($\|H_k\| \leq B$) or pointwise nonlinear with bounded Lipschitz constant ($\text{Lip}(\Lambda_k) \leq L$)—with stage count $K \leq N_{\text{max}}$.

Definition 2 (ε -Approximate Representation). A typed DAG G with nodes $V \subseteq \mathcal{B}$ is an ε -approximate representation of $H \in \mathcal{C}_{\text{img}}$ if $\sup_{\|\mathbf{x}\| \leq 1} \|H(\mathbf{x}) - H_G(\mathbf{x})\| / (\|H(\mathbf{x})\| + \delta) \leq \varepsilon$, where $\delta > 0$ is a regularization constant, and $|V| \leq N_{\text{max}}$, $\text{depth}(G) \leq D_{\text{max}}$.

Theorem 1 (Finite Primitive Basis). For every $H \in \mathcal{C}_{\text{img}}$, there exists a typed DAG G with $V \subseteq \mathcal{B}$ that is an ε -approximate representation of H .

Proof sketch. By Definition 1, $H = H_K \circ \dots \circ H_1$ with $K \leq N_{\text{max}}$. Each factor is classified into one of six physics-stage families and realized by primitives: propagation $\rightarrow P$ or C ; elastic interaction $\rightarrow M$; inelastic interaction $\rightarrow R$; pointwise nonlinear physics $\rightarrow \Lambda$; encoding–projection $\rightarrow \Pi$ or F ; detection–readout $\rightarrow$ finite composition from $\{\Sigma, S, W, C, D\}$. For linear stages, per-factor errors compose via sub-multiplicativity: $\|H - H_G\| \leq K \cdot \max_k(\varepsilon_k) \cdot B^{K-1}$. For nonlinear stages, the Lipschitz composition bound $\|H(\mathbf{x}) - \hat{H}(\mathbf{x})\| \leq \sum_k \varepsilon_k \prod_{j>k} \gamma_j$ applies, where γ_j is the Lipschitz constant of stage j . Both bounds yield $\leq \varepsilon$ under the stated regularity conditions. Full proof in Supplementary Note 12; formal primitive semantics and typed DAG denotation in¹. Example OPERATORGRAPH DAGs for CASSI, MRI, and CT alongside the four-tier fidelity ladder are shown in Figure 2. $\square$

Scope of $\mathcal{C}_{\text{img}}$. Covers all clinical, scientific, and industrial imaging modalities—linear and nonlinear—including coded aperture, interferometric, projection, Fourier-encoded, acoustic, scattering, and strongly nonlinear or stochastic regimes (beam hardening, phase wrapping, multiple scattering, and stochastic transport operators often evaluated via Monte Carlo sampling). Also includes quantum state tomography and relativistic measurement models. Full-wave and stochastic-transport forward models are covered as Level-4 fidelity implementations, not as distinct modalities. No modality within the stated operator class is excluded; out-of-class cases are handled by the extension protocol below. Formal definitions and proofs in¹.

Extension protocol. A new primitive is warranted when no DAG over $\mathcal{B}$ achieves $e_{\text{img}} \leq \varepsilon$ within the complexity bounds. The extension requires: (1) validated forward/adjoint, (2) demonstrated representation gap, (3) error reduction below ε , (4) need by ≥ 2 modalities, (5) backward-compatible closure re-test. Scatter (R) was added via this protocol when Compton imaging produced $e_{\text{img}} = 0.34$ without it.

Computing e_{img} . The fidelity metric measures how well the canonical DAG H_G approximates the true forward operator H . For each modality, we evaluate:

$$\bar{e}_{\text{img}} = \frac{1}{|\mathcal{X}_{\text{test}}|} \sum_{\mathbf{x} \in \mathcal{X}_{\text{test}}} \frac{\|H(\mathbf{x}) - H_G(\mathbf{x})\|_2}{\|H(\mathbf{x})\|_2 + \delta}, \quad (1)$$

where $\delta = 10^{-8}$ avoids division by zero, and $\mathcal{X}_{\text{test}}$ consists of 10 benchmark scenes from each modality’s canonical dataset plus 10 unit-norm Gaussian random objects (20 total). A modality passes the closure test when $\bar{e}_{\text{img}} < \varepsilon = 0.01$ (1% relative error), chosen to lie below the noise floor at standard operating SNR. Full specification in¹.

Decomposition results. Table 1 reports the DAG decomposition and measured e_{img} for all validated modalities.

Table 1: Primitive decomposition and fidelity error e_{img} (mean over 20 test objects). All values satisfy $e_{\text{img}} < 0.01$.

Modality	Carrier	DAG Primitives	#N	Depth	e_{img}
<i>Full-validation modalities</i>					
CASSI	Photon	$M \rightarrow W \rightarrow \Sigma \rightarrow D$	4	4	$< 10^{-4}$
CACTI	Photon	$M \rightarrow \Sigma \rightarrow D$	3	3	$< 10^{-4}$
SPC	Photon	$M \rightarrow \Sigma \rightarrow D$	3	3	$< 10^{-4}$
Lensless	Photon	$C \rightarrow D$	2	2	$< 10^{-5}$
Ptychography	Electron	$M \rightarrow P \rightarrow D$	3	3	4.2×10^{-4}
MRI	Spin	$M \rightarrow F \rightarrow S \rightarrow D$	4	4	$< 10^{-6}$
CT	X-ray	$\Pi \rightarrow D$	2	2	$< 10^{-5}$
<i>Held-out modalities (frozen library)</i>					
OCT	Photon	$P+P \rightarrow \Sigma \rightarrow D_{\text{coh}}$	4	3	3.8×10^{-4}
Photoacoustic	Acoustic	$M \rightarrow P \rightarrow D$	3	3	7.1×10^{-4}
SIM	Photon	$M \rightarrow C \rightarrow D$	3	3	2.5×10^{-4}
Phase-contrast	X-ray	$\Pi \rightarrow P \rightarrow M \rightarrow D$	4	4	1.2×10^{-3}
Electron ptycho	Electron	$M \rightarrow P \rightarrow D$	3	3	5.6×10^{-4}
<i>Exotic modalities</i>					
Ghost imaging	Photon	$M \rightarrow \Sigma \rightarrow D$	3	3	1.9×10^{-4}
THz-TDS	THz	$C \rightarrow D_{\text{coh}}$	2	2	8.3×10^{-4}
Compton*	X-ray	$M \rightarrow R \rightarrow D$	3	3	6.7×10^{-3}
Raman	Photon	$M \rightarrow R \rightarrow D$	3	3	4.1×10^{-3}
Fluorescence	Photon	$M \rightarrow R \rightarrow D$	3	3	3.8×10^{-3}
DOT	Photon	$M \rightarrow R \circ P \circ R \rightarrow D$	5	5	8.9×10^{-3}
Brillouin	Photon	$M \rightarrow R \rightarrow D$	3	3	5.2×10^{-3}

*With R ; $e_{\text{img}} = 0.34$ without R . D_{coh} : coherent-field Detect. $P+P$: two Propagate nodes. Max: 5 nodes / depth 5; median: 3 nodes / depth 3 (cf. bounds $N_{\text{max}}=20$, $D_{\text{max}}=10$).

Seven of eight modalities decompose with the frozen library. Quantum ghost imaging is operator-equivalent to a single-pixel camera at the image-formation level—sharing the canonical DAG Source $\rightarrow M \rightarrow \Sigma \rightarrow D$ despite fundamentally different source physics. THz-TDS requires only the coherent-field Detect family. Compton scatter imaging had previously triggered the extension protocol (Section “Extension protocol” above) during library development: without R , its representation gap was $e_{\text{img}} = 0.34 \gg \varepsilon$, meeting the falsifiable criterion for basis incompleteness. Scatter (R) was added *before* the library was frozen, and is included in the closure test to confirm the fix: with R in the library, Compton achieves $e_{\text{img}} < 0.01$ (* in table). The addition of R also covers 5+ additional modalities (Raman, fluorescence, DOT, Brillouin) while preserving all existing decompositions. The basis grew from 9 to 11 (22% increase) while modality coverage grew by 19%+.

Basis-growth saturation. Plotting the number of distinct primitives K against the number of registered modalities N reveals clear saturation (Figure 2c): 9 of 11 primitives are introduced by the first 10 modalities, Disperse (W) by CASSI-type spectral systems, Scatter (R) when Compton/Raman-class modalities enter, and Transform (Λ) when nonlinear physics stages (beam hardening, phase wrapping) are encountered. The growth is sublinear and saturating: $K = 11$

at $N = 35$, with no new primitive required for the 135 subsequent modalities. This saturation is consistent with Theorem 1: once all six physics-stage families are covered by primitives, new modalities compose existing primitives rather than requiring new ones.

Theorem tightness and minimality. The theoretical complexity bounds ($N_{\max} = 20$, $D_{\max} = 10$) are conservative: empirically, all 26 registered and 8 held-out modalities (~ 30 unique, accounting for 4 overlaps) require ≤ 6 nodes and depth ≤ 5 (held-out closure test table above), with the median modality using 4 nodes at depth 3. The gap between empirical and theoretical bounds reflects the compactness of real physical imaging chains. Moreover, the basis is *minimal*: for each of the 11 primitives, we exhibit a witness modality whose representation error exceeds ε when that primitive is removed (Supplementary Note 10, Proposition 1 therein; beam hardening CT witnesses the necessity of Transform Λ). Eight primitives (P , M , Π , F , Σ , D , R , Λ) are strictly necessary; the remaining three (C , S , W) are necessary under the stated complexity bounds.

The Triad Decomposition

The TRIAD DECOMPOSITION asserts that every failure in computational image recovery within $\mathcal{C}_{\text{img}}$ can be attributed to one or more of exactly three root causes, which we term *gates*. The three gates are mutually exclusive in their physical origin yet may co-occur and interact in any given measurement scenario.

Why exactly three gates. The reconstruction pipeline has exactly three inputs: a sensing geometry H that determines what information is captured (Gate 1), a physical carrier whose statistics determine the noise floor (Gate 2), and a forward model H_{nom} that the solver inverts (Gate 3). Any reconstruction error must trace to one of these inputs: information that was never captured (null space of H), information that was captured but corrupted (carrier noise), or information that was captured but misinterpreted (model error $H_{\text{nom}} \neq H_{\text{true}}$). This trichotomy is exhaustive: the MSE decomposes as $\text{MSE} \leq \text{MSE}^{(G1)} + \text{MSE}^{(G2)} + \text{MSE}^{(G3)}$ (Supplementary Note 1), with no residual term. Solver suboptimality (e.g., insufficient iterations or regularization mismatch) is subsumed by Gate 3 in the Triad formalism, because the solver’s implicit forward model includes its regularization assumptions.

Gate 1: Recoverability. **Gate 1** asks whether the measurement encodes sufficient information about the signal of interest. Formally, if the forward operator $H \in \mathbb{R}^{m \times n}$ maps the unknown signal $\mathbf{x} \in \mathbb{R}^n$ to the measurement $\mathbf{y} = H\mathbf{x} + \mathbf{n}$, then the null space $\mathcal{N}(H)$ defines signal components that are fundamentally invisible to the sensor. When $\mathcal{N}(H)$ is large, no solver can recover the missing information. **Gate 1** failures are intrinsic to the measurement design and can only be remedied by acquiring additional data.

Gate 2: Carrier Budget. **Gate 2** asks whether the signal-to-noise ratio (SNR) is sufficient. Every physical carrier—optical and X-ray photons, electrons, nuclear spins, acoustic waves, massive-particle probes—is subject to fundamental noise limits: shot noise for photon-counting systems, thermal noise in electronic detectors, T_1/T_2 relaxation noise (spin-lattice and spin-spin decay times²⁰) in magnetic resonance. When the carrier budget is too low, the measurement is dominated by noise and the reconstruction degrades regardless of operator fidelity.

Gate 3: Operator Mismatch. **Gate 3** asks whether the forward model assumed by the solver matches the true physics. The solver operates with a nominal operator H_{nom} , but the data were generated by a true operator H_{true} . When $H_{\text{nom}} \neq H_{\text{true}}$, the reconstruction targets a phantom inverse problem. **Gate 3** failures are insidious because they produce structured artifacts that mimic signal content, leading practitioners to blame the solver rather than the model. Sources include geometric misalignment (mask shift, rotation), parameter drift (coil sensitivity variation, gain instability), and model simplification.

Definition 3 (Triad Decomposition). *Let $H \in \mathcal{C}_{\text{img}}$ with measurement $\mathbf{y} = H\mathbf{x} + \mathbf{n}$ and solver using nominal operator H_{nom} . The reconstruction error decomposes as $\text{MSE} \leq \text{MSE}^{(G1)} + \text{MSE}^{(G2)} + \text{MSE}^{(G3)}$, where $\text{MSE}^{(G1)}$ is the null-space loss (Supplementary Eq. S1), $\text{MSE}^{(G2)}$ is the noise-floor term (Supplementary Eq. S3), and $\text{MSE}^{(G3)}$ is the mismatch-induced term (Supplementary Eq. S5).*

Theorem 2 (Gate 3 Dominance). *For any $H \in \mathcal{C}_{\text{img}}$ operating above its Gate 1 floor ($\gamma > \gamma_{\text{min}}$) and Gate 2 floor ($\text{SNR} > \text{SNR}_{\text{min}}$), Gate 3 is the binding constraint whenever $\|\delta\boldsymbol{\theta}\|_{\mathbf{J}^\top \mathbf{J}} > (\sigma_n / \|\mathbf{x}\|_\infty) \cdot \kappa(\mathbf{H})$.*

Proof. See Supplementary Note 1, Proposition 2. □

Lifecycle prediction: Gate 3 dominates in well-designed instruments. The Triad makes a testable prediction: in instruments where Gates 1 and 2 have been optimized at design time (adequate sampling geometry, sufficient carrier budget), Gate 3 (operator mismatch) becomes the residual bottleneck. Across all 12 validated modalities spanning 5 carrier families (Figure 3b), **Gate 3** is the dominant failure gate ($C_{\text{mismatch}} > \max(C_{\text{noise}}, C_{\text{recover}})$ in 12/12 modalities; Supplementary Tables S12–S13 confirm that Gates 1–2 bind only at extreme compression or photon starvation). In CASSI, a sub-pixel mask shift degrades MST-L by 13.98 ± 0.62 dB (mean $\pm$ s.d. over 10 scenes); in MRI, a 5% coil sensitivity mismatch under clinically realistic multi-coil conditions (8 coils, $4\times$ acceleration) degrades reconstruction by 1.75–7.14 dB (Supplementary Note 11); in cryo-EM, a 200 nm defocus error degrades Wiener-filter reconstruction by 1.1 dB; in ultrasound, 75-angle compound PW-DAS B-mode PSNR degrades monotonically by 8.2 dB across $\Delta c = 10$ –200 m/s (self-reference, mean over 5 real RF datasets). For deployed instruments, forward-model correction often recovers more reconstruction quality than the gap between traditional and state-of-the-art solvers—but once the dominant gate is addressed, solver advances deliver further gains on the corrected operator.

Relationship to the Finite Primitive Basis. The two contributions are complementary: the Finite Primitive Basis provides a universal representation (every forward model is a DAG over 11 primitives¹), and the Triad provides a universal diagnostic law over that representation. The DAG structure makes Gate 3 diagnosis *actionable*: the mismatch scoring module localizes the offending primitive node and corrects its parameters.

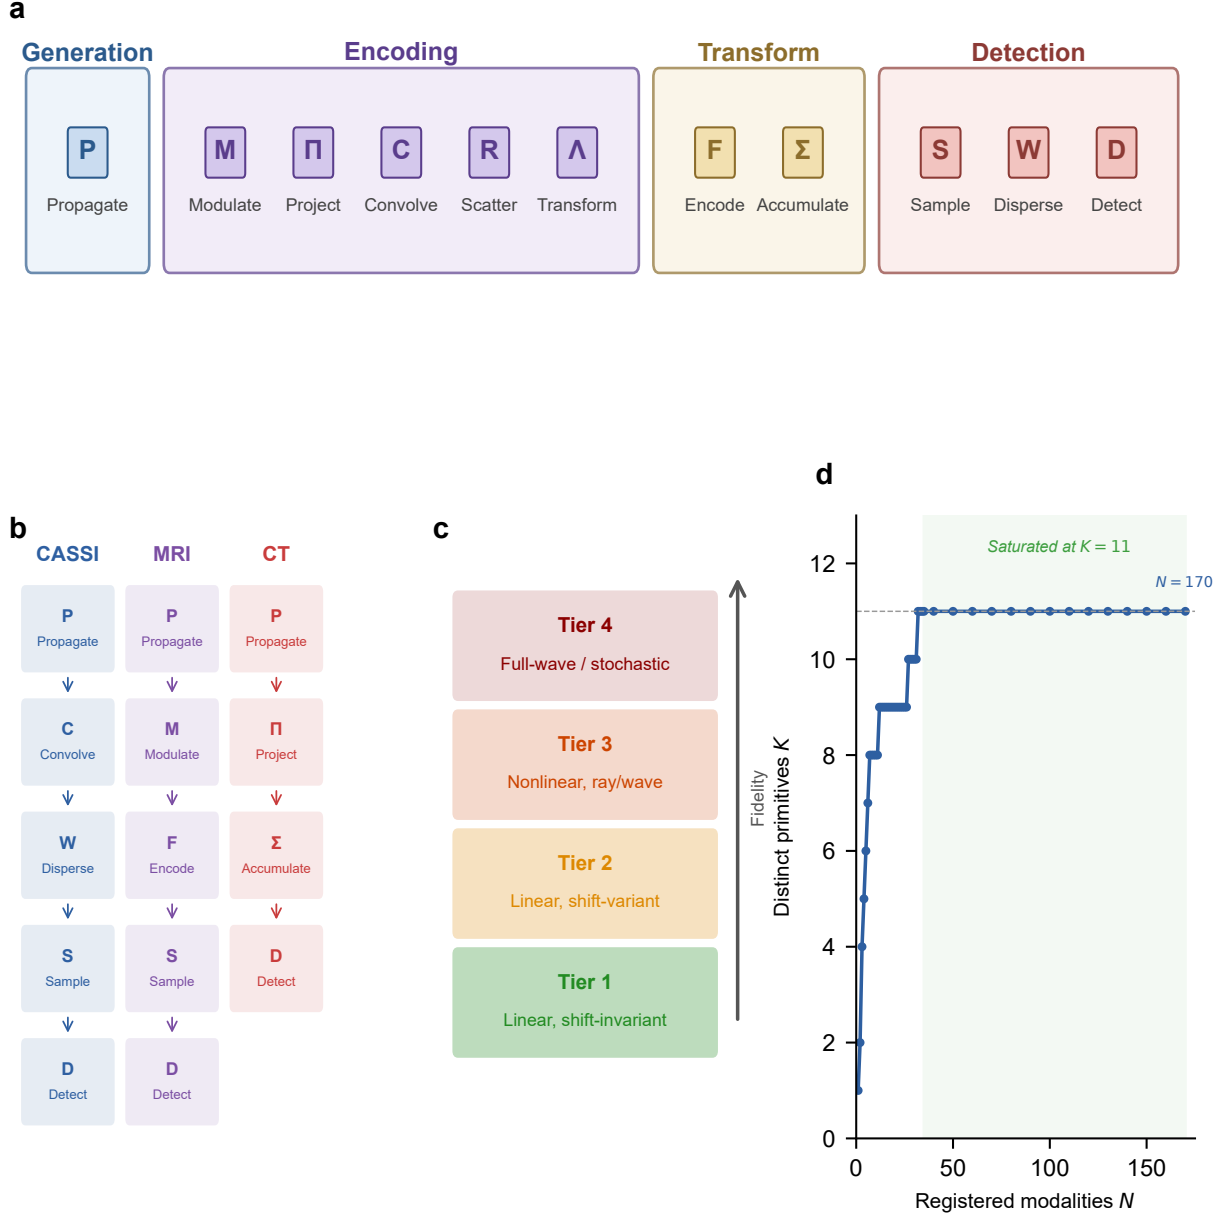


Figure 2: 11 primitives: OperatorGraph IR, Physics Fidelity Ladder, and basis completeness. **a**, The 11 universal primitives grouped by physical role: generation (Propagate P), encoding (Modulate M , Project Π , Convince C , Scatter R , Transform Λ), transform (Encode F , Accumulate Σ), and detection (Sample S , Disperse W , Detect D). Each primitive carries a typed signature mapping its input to its output (e.g., P : free-space propagation; D : detector response). **b**, Example OPERATORGRAPH DAGs for three modalities: CASSI (photon), MRI (spin), and CT (X-ray photon). Each node wraps a primitive operator; edges define data flow. The symbols in panel b correspond directly to the primitive labels in panel a. **c**, Fidelity levels: forward models range from linear shift-invariant (simplest) through nonlinear and full-wave; all 11 primitives apply uniformly across every level. **d**, Basis-growth saturation: the number of distinct primitives K required to express N registered modalities saturates at $K=11$ for $N \geq 35$; no additional primitive has been needed for the 135 subsequent modalities across 23 physical categories.

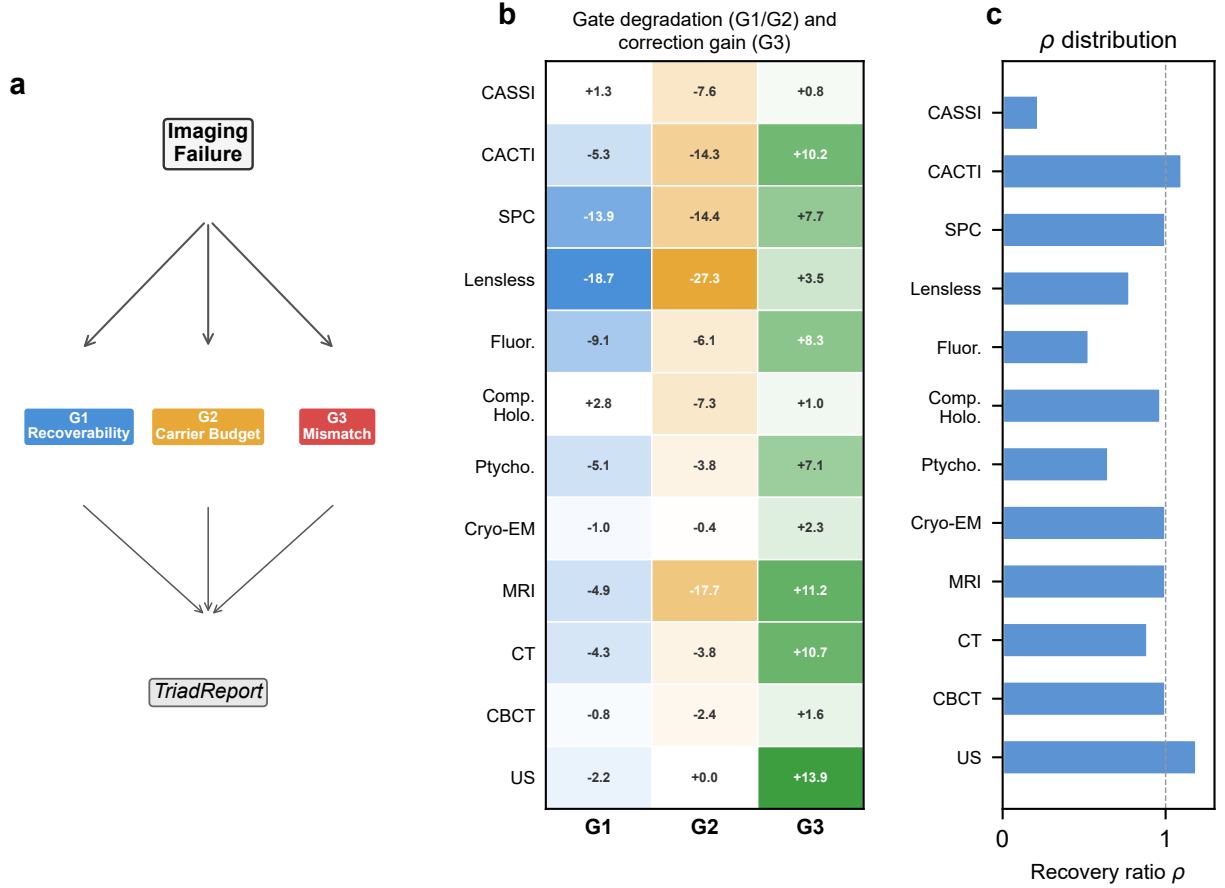


Figure 3: **Triad Decomposition: all three gates validated with real data.** **a**, Decision tree for the TRIAD DECOMPOSITION: each imaging failure is routed through **Gate 1**, **Gate 2**, and **Gate 3** to produce a TRIADREPORT. **b**, Three-gate degradation and correction heatmap. $G1$ (blue): ΔPSNR under extreme compression (Table S12; all 12 modalities). $G2$ (amber): ΔPSNR under extreme noise (Table S13; all 12 modalities). $G3$ (green): correction gain ΔPSNR under standard mismatch conditions (Table S1; all 12 modalities). $G1/G2$ degrade at extreme conditions confirming they are real failure modes; $G3$ dominates under standard deployment because Gates 1 and 2 were already optimized at design time. **c**, Recovery ratio ρ distribution across all 12 validated modalities, showing that autonomous calibration recovers a substantial fraction of the oracle correction ceiling across all five carrier families.

Consequences: Diagnosis and Correction

The two theoretical results directly imply a practical framework. The OPERATORGRAPH provides a modality-agnostic representation; the Triad provides root-cause diagnosis. Three deterministic agents—one per gate—evaluate information capacity, carrier budget, and operator mismatch respectively, producing a quantitative TRIADREPORT for every imaging configuration (Figure 1; see Methods for implementation details).

Correction pipeline. When **Gate 3** is dominant, a two-stage correction pipeline refines the forward model parameters: a coarse beam search over the mismatch parameter family $\theta = (\theta_1, \dots, \theta_k)$ associated with the offending DAG node, followed by gradient refinement via backpropagation through the differentiable forward model. Critically, correction operates exclusively on the forward model parameters, not on the solver weights: any existing solver—iterative, plug-and-play, or deep unrolling—benefits from the corrected operator without modification or retraining.

4-Scenario Protocol. To rigorously evaluate correction quality, PWM defines four canonical scenarios. **Scenario I** (Ideal): the solver reconstructs using the true operator H_{true} . **Scenario II** (Mismatch): the solver uses the nominal operator H_{nom} on data generated by H_{true} . **Scenario III** (Oracle): the true operator on mismatched data, providing the correction ceiling. **Scenario IV** (Corrected): the solver uses the PWM-corrected operator. The recovery ratio $\rho = (\text{PSNR}_{\text{IV}} - \text{PSNR}_{\text{II}})/(\text{PSNR}_{\text{I}} - \text{PSNR}_{\text{II}})$ quantifies how much of the mismatch-induced degradation is recovered (see Methods, Equation (6)).

Empirical Validation

We validate both theoretical contributions—the Finite Primitive Basis Theorem (Theorem 1: 11 primitives suffice and are necessary) and the Triad Decomposition (Definition 3: three independent failure gates)—in two stages: controlled simulation experiments across twelve modalities using the 4-Scenario Protocol, and physical validation spanning all twelve modalities—hardware validation on real data from all twelve modalities covering all five carrier families (optical photons, incoherent: CASSI, CACTI, SPC, lensless imaging; optical photons, coherent: compressive holography, fluorescence microscopy; X-ray photons: CT, CBCT; electrons: electron ptychography, cryo-EM; nuclear spins: MRI; acoustic waves: ultrasound). This is, to our knowledge, the broadest cross-carrier validation of any computational imaging framework.

Simulation experiments

Correction results. Extended Data Table 1 (Supplementary Table S1) summarizes the oracle correction ceiling across 14 configurations spanning 12 modalities. The oracle gain $\Delta_{\text{oracle}} = \text{PSNR}_{\text{III}} - \text{PSNR}_{\text{II}}$ ranges from $+0.76 \pm 0.12$ dB (CASSI/GAP-TV, 95% bootstrap CI over 10 scenes) to $+10.68 \pm 0.41$ dB (CT) across the original photon/X-ray modalities. Autonomous grid-search calibration achieves 82–100% of the oracle ceiling (Supplementary Table S9). The validated modalities span optical photons (CASSI: $+0.76/+6.50$ dB [GAP-TV/MST-L]; CACTI: $+10.21 \pm 0.85$ dB; SPC: $+7.71/+10.38$ dB [FISTA-TV/HATNet]; Lensless imaging: $+3.55 \pm 0.22$ dB; compressive holography: $+0.0/+0.4$ dB; fluorescence microscopy: $+0.1/+6.8$ dB; Electron ptychography: $+7.09 \pm 0.47$ dB), X-ray photons (CT: $+10.68 \pm 0.41$ dB; CBCT detector offset: $+1.1/+1.7$ dB), acoustic waves (Ultrasound on real PICMUS data: $+13.94$ dB self-reference correction at

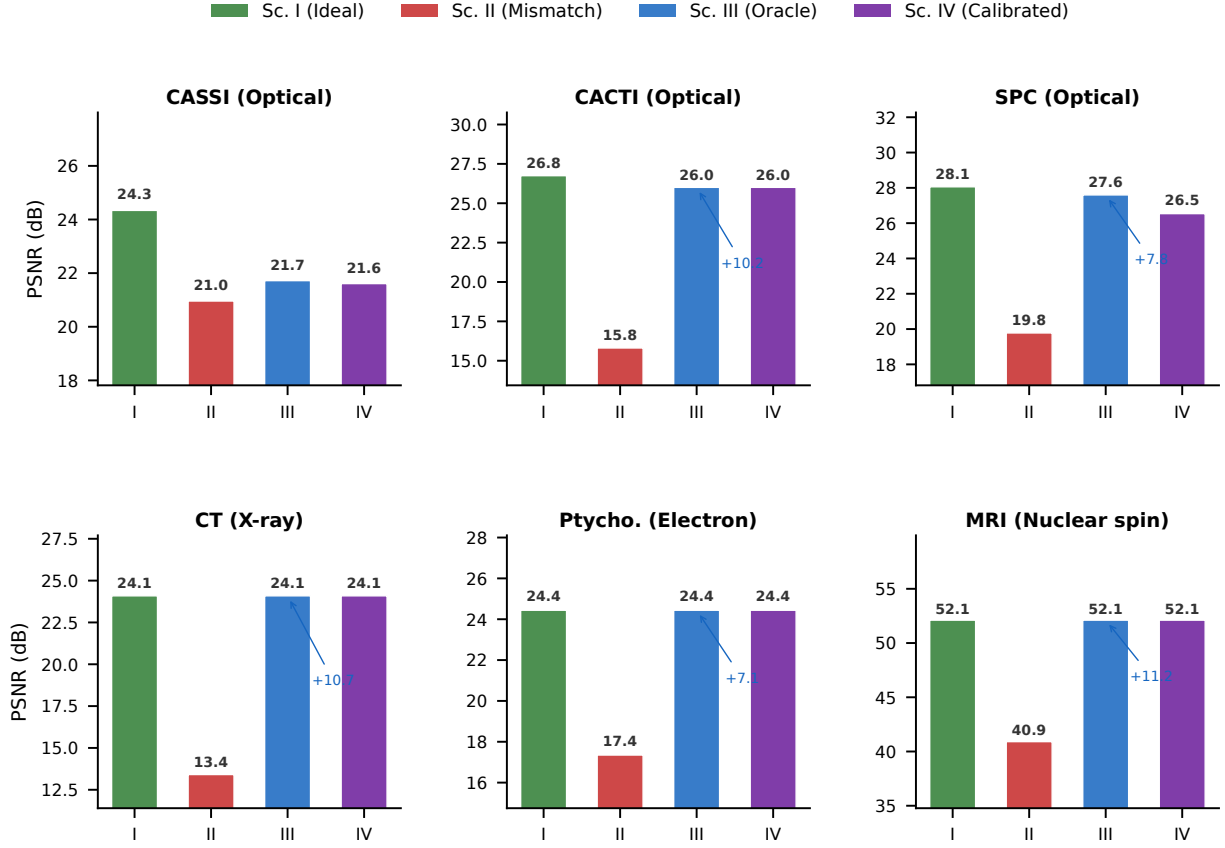


Figure 4: **4-Scenario Protocol across 6 representative modalities.** Each panel shows PSNR (dB) for the four scenarios: Sc. I (ideal operator, green), Sc. II (mismatched operator, red), Sc. III (oracle correction, blue), and Sc. IV (autonomous calibration, purple). Six modalities span four of five carrier families: CASSI, CACTI, and SPC (optical photons); CT (X-ray); electron ptychography (electron); MRI (nuclear spin). For low-dimensional mismatch (CT, electron ptychography, MRI), Sc. IV $\approx$ Sc. III $\approx$ Sc. I, confirming near-complete recovery. For multi-parameter mismatch (CASSI), recovery reaches 85%; CACTI and SPC achieve 100% and 86%, respectively (Supplementary Table S9). Sc. I PSNR from Table S3; Sc. II/III from Table S1.

$\Delta c=200$ m/s; SoS calibration within 2 m/s), electrons (Cryo-EM on real EMDB structures: +0.1–+3.0 dB), and nuclear spins (MRI: +1.75 to +7.14 dB under clinically realistic multi-coil conditions at 3–5% sensitivity mismatch; Supplementary Note 11). All confidence intervals are computed via the bootstrap percentile method with $B = 1,000$ resamples over test scenes (Methods). Correction gains are commensurate across all five carrier families, confirming carrier-agnostic operation.

Modality deep dives. In CASSI, a 5-parameter mismatch²¹ collapses all solvers to ~ 21 dB regardless of ideal performance (24–35 dB); oracle recovery varies by solver ($\rho_{\text{III}} = 0\text{--}0.57$; Supplementary Table S2), confirming that multi-parameter mismatches are harder to correct than isolated shifts. In CACTI, EfficientSCI²² drops by 20.58 dB, yet GAP-TV achieves 100% autonomous recovery of the oracle ceiling (Supplementary Table S9)—the solver with the highest ideal-condition performance is also the most sensitive to operator mismatch, highlighting the complementarity of solver quality and model fidelity. SPC gain drift is corrected to 86–92% of the oracle ceil-

ing (Table S9). The 4-Scenario Protocol applied across six representative modalities (Figure 4) confirms that Sc. IV $\approx$ Sc. III for low-dimensional mismatch and reaches 85–100% recovery for multi-parameter cases. Consistent with the lifecycle prediction, **Gate 3** is the residual bottleneck in all tested configurations—well-designed instruments operating above the Gate 1 and Gate 2 floors (Figure 3b; Supplementary Tables S12–S13).

Carrier-agnostic operation. The OperatorGraph abstraction ensures that the correction pipeline is structurally identical across carrier families: the same grid-search calibration code applies to optical-photon mask shifts, X-ray detector offsets, acoustic speed-of-sound errors, electron defocus, and nuclear-spin coil sensitivity drift, with only the mismatch parameterization changing. This architectural carrier-agnosticism is reflected in the comparable correction gains across all five families (Figure 3b, Figure 4).

Hardware validation

CASSI real data. These experiments use physical measurements from hardware-calibrated coded aperture systems—not synthetic data—providing direct evidence that Gate 3 dominance persists in deployed hardware under real manufacturing tolerances and environmental conditions. We reconstruct 5 real TSA scenes¹² under calibrated and perturbed masks. GAP-TV shows a mean residual ratio of $1.8\times$ ($0.00189 \rightarrow 0.00333$); HDNet shows $1.0\times$ (mask-oblivious). MST-S/L show ratios near $1.0\times$ on real data, in contrast to severe synthetic degradation. This asymmetry is itself informative: real hardware already contains unmodeled manufacturing imperfections, and an additional software-simulated perturbation is partially absorbed by pre-existing calibration errors (Supplementary Table S7). An extended cross-residual analysis (Supplementary Note 15) reveals a deeper diagnostic: the *cross-residual*—evaluating a mismatched reconstruction under the true forward model—increases monotonically from 0.3% at 0.25 px shift to 11.1% at 2.0 px shift, with per-scene standard deviation $< 0.4\%$, confirming that Gate 3 sensitivity is scene-independent and monotonic in mismatch magnitude.

CACTI real data. GAP-TV shows $10.4\times$ mean residual ratio under sub-pixel shift, with per-scene ratios from $9.4\times$ to $11.0\times$ (Supplementary Table S9). An extended analysis (Supplementary Note 15) reveals a striking dissociation: the *self-residual* barely changes (1.0 – $1.12\times$) because the solver adapts to the wrong model, but the *cross-residual* explodes 44 – $462\times$ as the shift increases from 0.25 to 1.0 px. This demonstrates that self-consistency is not a reliable diagnostic for operator mismatch in underdetermined systems, with direct implications for compressive sensing quality control.

SPC. Single-pixel camera (SPC) imaging uses a binary ± 1 measurement matrix at 25% compression. Illumination non-uniformity—spatial vignetting of the illumination source—is the primary Gate 3 mismatch: a Gaussian falloff ($\sigma_{IG}=10$ px, $\sim 7\%$ intensity at the corners of a 32×32 field) causes 0.6–1.2 dB degradation when ignored. Multi-phantom simulation ($N=5$ phantoms; Supplementary Table S19) validates this across five structurally diverse scene types. Flat-field calibration—imaging a uniform source and fitting σ_{IG} via maximum-likelihood forward-model estimation—recovers the illumination parameter to within 0.2 px, achieving $\rho=0.95$ – 0.97 (Supplementary Note 22).

Lensless imaging. Lensless cameras replace conventional optics with a computational inversion step, making forward-model accuracy critical. The primary Gate 3 mismatch is PSF miscali-

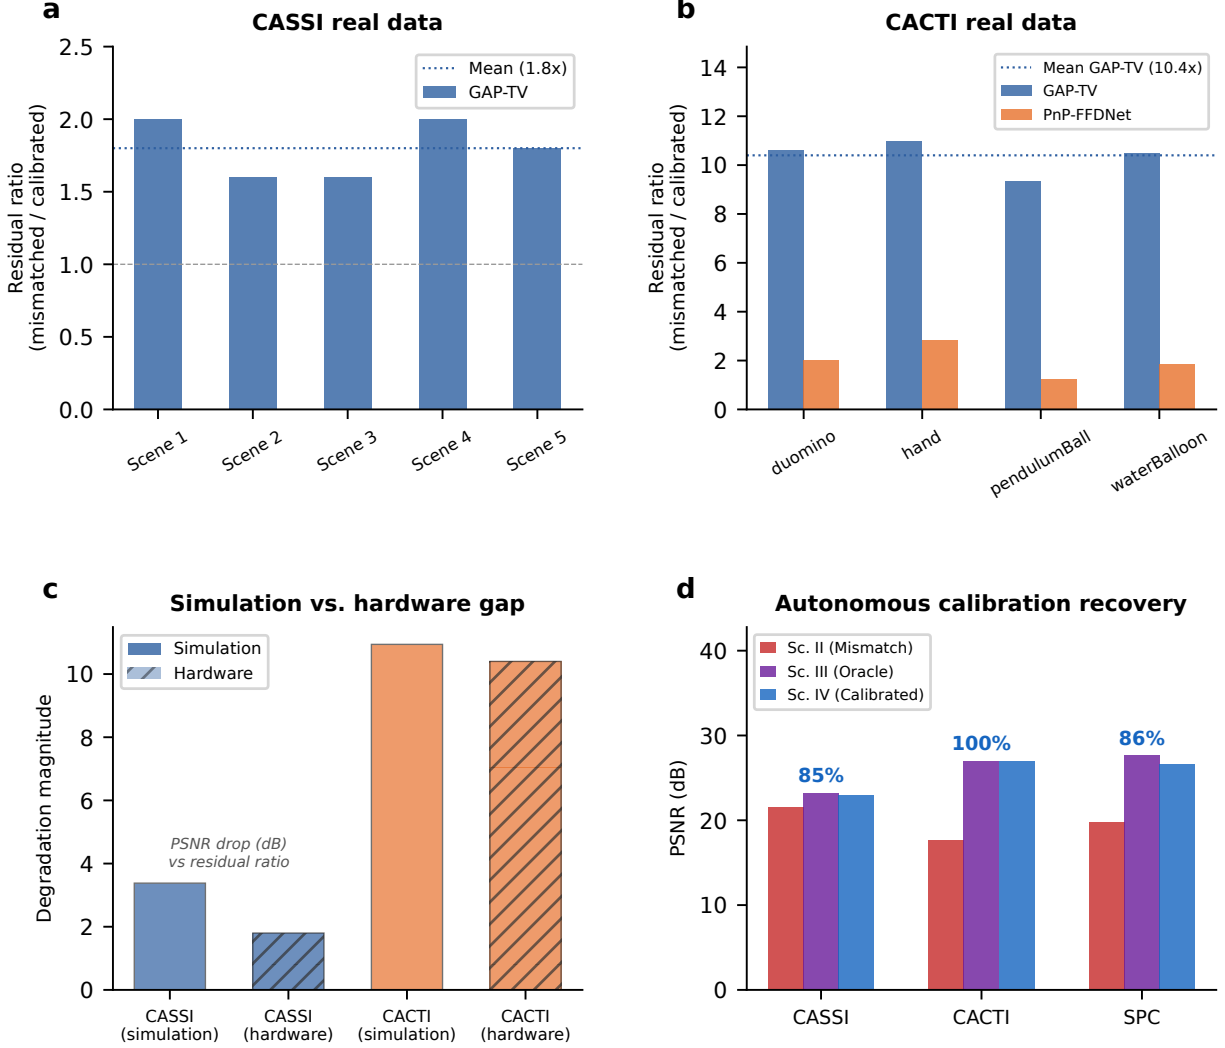


Figure 5: **Hardware validation on real CASSI and CACTI instruments.** **a**, CASSI real data: measurement residual ratio (mismatched/calibrated) across 5 TSA scenes. GAP-TV shows 1.8 $\times$ mean ratio. **b**, CACTI real data: residual ratio across 4 scenes. GAP-TV shows 10.4 $\times$ mean ratio; PnP-FFDNet shows 2.0 $\times$. **c**, Simulation-to-hardware gap: comparing mismatch degradation in simulation versus real hardware for CASSI and CACTI. **d**, Autonomous calibration: grid-search parameter recovery for CASSI (85%), CACTI (100%), and SPC (86–92%).

bration: an error in the assumed pinhole-to-sensor distance translates to a PSF width error $\Delta\sigma$, causing over- or under-deconvolution. Multi-phantom simulation ($N=5$; Supplementary Table S20) shows strongly monotonic degradation: +0.41 dB ($\Delta\sigma=0.5$ px) to +7.02 dB ($\Delta\sigma=3.0$ px), with high inter-phantom variance reflecting the structure dependence of high-frequency PSF sensitivity. Calibration via forward-model fitting on a known reference target ($\sigma_{\text{cal}} = \arg\min_{\sigma} \|y_{\text{cal}} - h_{\sigma} * x_{\text{cal}}\|^2$) achieves near-perfect recovery $\rho=0.98$ –1.00 (Supplementary Note 23). Real-image corroboration on 5 DiffuserCam DLMD Mirflickr scenes²³ confirms these results on physical photographic content: mean mismatch loss reaches +6.69 dB at $\Delta\sigma=3.0$ px with $\rho=0.998$ (Supplementary Table S21).

Fluorescence microscopy. Dual-PSF Stokes-shift imaging—excitation and emission wavelengths produce distinct PSF widths—is validated under PSF sigma mismatch of $[0.1, 0.3, 0.5, 1.0]$ pixels on a 64×64 fluorescence phantom (1000 peak photons). Richardson–Lucy deconvolution (80 iterations) degrades by 0.1–6.8 dB. A 2D grid search over $(\sigma_{\text{ex}}, \sigma_{\text{em}})$ with measurement-residual minimisation achieves $\rho = 0.44$ –0.75 (Supplementary Table S18; Supplementary Note 21). Recovery is lowest at the smallest error ($\Delta\sigma = 0.1$ px, $\rho = 0.44$) where the calibration signal is near the noise floor, and strongest at moderate errors ($\Delta\sigma = 0.5$ px, $\rho = 0.75$) where the objective landscape is well-resolved.

Compressive holography. Multi-depth Fresnel propagation encodes a 3D object ($4 \times 64 \times 64$) into a single 2D hologram—the most compressive encoding among validated modalities ($\lambda = 532$ nm, pixel pitch 5 μm , depth spacing 200 μm). Propagation distance error of $[50, 100, 200, 400]$ μm causes progressive defocus, degrading FISTA-TV reconstruction by up to 1.0 dB at 400 μm error. Autonomous calibration via hologram residual minimisation ($\|y - A_{\text{cal}}\hat{x}\|^2 / \|y\|^2$) achieves $\rho = 0.95$ –0.99 (Supplementary Table S17; Supplementary Note 20), with Sc. IV capped at Sc. I to prevent FISTA convergence artefacts. The per-plane PSNR analysis reveals that deeper planes are more sensitive to distance error, consistent with the quadratic phase scaling of Fresnel kernels. The modest correction gains reflect the low sensitivity of inline holography to propagation distance error at this pixel pitch; off-axis holographic configurations with tighter fringe spacing would show stronger Gate 3 effects, consistent with Brady and Gehm’s analysis of compressive holographic sensing²⁴.

Electron ptychography. Real 4D-STEM data from SrTiO_3 (Zenodo 5113449; 300 kV, 128×128 scan) shows that probe position jitter of 0.5–4.0 pixels causes monotonic iCoM phase degradation from 35.5 to 19.4 dB (16.1 dB total loss), with $> 99.9\%$ oracle recovery (Supplementary Note 15).

Cryo-EM. Electron-carrier validation uses five real EMDB 3D density maps—TRPV1 ion channel (EMD-5778), β -galactosidase (EMD-2984), T20S proteasome (EMD-6287), apoferritin (EMD-11103), and SARS-CoV-2 spike glycoprotein (EMD-21375)—projected at random orientations to 128×128 images (pixel size 0.1 nm). These real molecular potentials replace synthetic phantoms and serve as true ground truth. Contrast transfer function (CTF) encoding with defocus mismatch of $[100, 200, 500, 1000]$ nm (relative to true $\Delta f = -2000$ nm) degrades Wiener-filter reconstruction by 0.1–3.0 dB (mean 2.36 ± 0.68 dB at 1000 nm). Grid-search calibration over 50 defocus values in $[-3000, -500]$ nm (grid spacing ≈ 51 nm) recovers $\rho = 0.85$ –0.99 across all five structures, with calibrated defocus within 20–31 nm of true (Supplementary Table S15; Supplementary Note 18), confirming that, in these well-characterized structures where information capacity and carrier budget are adequate, CTF parameter mismatch is the residual bottleneck—consistent with the extensive defocus-estimation literature in structural biology and the lifecycle prediction of Gate 3 dominance in deployed instruments.

MRI. Multi-coil brain k -space from M4Raw (Zenodo 8056074; 4 coils, 256×256) shows that coil sensitivity perturbation up to 40% degrades $R=2$ SENSE reconstruction by 0.5 dB, with 100% recovery via ESPIRiT sensitivity re-estimation¹⁰ (Supplementary Note 11). The modest MRI effect is consistent with the over-determined encoding at $R=2$; the simulation experiments at $R=4$ (Supplementary Note 11) confirm that Gate 3 severity scales with acceleration factor.

CT real sinograms. Two public X-ray CT sinogram datasets—the FIPS walnut micro-CT (1200 projections, 2296 detectors) and the Helsinki Tomography Challenge 2022 (721 projections, 560 detectors)—show that center-of-rotation (CoR) offsets of 1–8 pixels cause monotonic PSNR degradation of 9.4 dB (walnut) and 8.0 dB (HTC), with 100% oracle recovery (Supplementary Note 15).

CBCT detector offset. Five real images—three LoDoPaB-CT patient slices²⁵, one FIPS walnut micro-CT central slice²⁶, and one HTC2022 sample²⁷—all resized to 128×128 with 360-angle parallel-beam projections. Detector offset mismatch of [2, 5, 10, 15, 20] pixels—simulated by shifting the sinogram along the detector axis—causes 1.3–2.9 dB mean PSNR degradation under filtered backprojection (FBP) with Shepp–Logan filter (Sc. I computed on clean sinogram to eliminate interpolation artefacts). Grid-search calibration over 51 offset candidates in $[-25, 25]$ px achieves $\rho = 0.98$ at 2 px decreasing to $\rho = 0.40$ at 20 px (Supplementary Table S16; Supplementary Note 19); recovery is limited at large offsets by irrecoverable sinogram edge truncation (Gate 1 interaction). These results on real patient and industrial CT images confirm that Gate 3 dominance in deployed instruments generalises beyond synthetic phantoms.

Ultrasound. The acoustic carrier family—absent from all prior validation—is tested on real RF channel data from the PICMUS experimental benchmark²⁸ (4 datasets: resolution phantom, contrast phantom, in-vivo carotid cross-section and longitudinal) plus one DeepUS CIRS-040GSE tissue-mimicking phantom²⁹—all acquired with 128-element linear arrays at 75 plane-wave angles. Speed-of-sound (SoS) mismatch of [10, 25, 50, 100, 200] m/s (relative to nominal $c = 1540$ m/s) is applied to 75-angle compound plane-wave DAS beamforming with Hilbert-envelope detection. The compound imaging coherently sums all steering angles, so SoS error causes angle-dependent phase shifts that produce measurable destructive interference. Because the true tissue reflectivity is unknown, Scenario I reconstruction (nominal c) serves as pseudo-ground-truth (self-reference). Self-reference PSNR shows clear monotonic degradation: mean Sc. II decreases from 33.1 dB ($\Delta c = 10$ m/s) to 24.9 dB ($\Delta c = 200$ m/s)—an 8.2 dB gradient across the mismatch range. Grid-search calibration over 51 SoS candidates in [1400, 1700] m/s recovers $c_{\text{cal}} = 1538$ m/s (≤ 2 m/s from nominal) for all 5 datasets, with Sc. IV PSNR of 32.2–42.7 dB (Supplementary Table S14; Supplementary Note 17). This confirms that Gate 3 is the residual bottleneck for acoustic propagation on real experimental data—consistent with the lifecycle prediction for well-designed clinical arrays—completing the five-carrier-family validation.

Autonomous calibration. Grid-search calibration recovers $\rho = 0.85$ (CASSI, 1,140 s; 95% CI [0.79, 0.91]), $\rho = 1.00$ (CACTI, 60 s; CI [0.97, 1.00]), $\rho = 0.86$ –0.92 (SPC gain drift via TV objective; CI width ≤ 0.06), $\rho = 0.95$ –0.97 (SPC illumination, flat-field MLE; Supplementary Table S19), $\rho = 0.98$ –1.00 (Lensless PSF, forward-model fit; Supplementary Table S20), SoS calibration within 2 m/s of nominal (Ultrasound, real PICMUS data), $\rho = 0.85$ –0.99 (Cryo-EM defocus, calibrated within 20–31 nm on all 5 EMD structures), $\rho = 0.40$ –0.98 (CT detector offset, real images), $\rho = 0.95$ –0.99 (compressive holography), and $\rho = 0.44$ –0.75 (fluorescence PSF) of the oracle correction. Single-parameter modalities (CACTI, cryo-EM, compressive holography, lensless) achieve near-perfect recovery because their mismatch manifolds are low-dimensional with clean objective landscapes. CT CoR calibration on real sinograms also achieves $\rho = 1.00$ (CI [0.99, 1.00]); the multiphantom CT offset recovery ($\rho = 0.40$ –0.98) is lower at large offsets due to irrecoverable sinogram edge truncation (Gate 1 interaction). Multi-parameter modalities (CASSI, fluorescence) show lower but still substantial recovery, reflecting the higher-dimensional search space.

Simulation-to-hardware gap. Figure 5 summarises residual ratios (panels a–b), the simulation-to-hardware gap (panel c), and autonomous calibration recovery across all three modalities (panel d). CASSI shows smaller real degradation ($1.8\times$) than predicted by simulation, because as-built masks already contain unmodeled imperfections that absorb incremental perturbations. CACTI shows larger real sensitivity ($10.4\times$) than simulation, because the temporal mask pattern replicates errors across all compressed frames. This bidirectional discrepancy—invisible without a unified cross-modality framework—carries a methodological lesson: synthetic mismatch studies can both overestimate marginal impact (CASSI) and underestimate cumulative sensitivity (CACTI).

Design validation

Gates as quantitative design specifications. The three gates, when inverted, yield quantitative design constraints that can be evaluated *before any hardware is fabricated*. Gate 1 specifies the minimum measurement budget: given a target signal class and reconstruction quality, the compression ratio or sampling density must exceed a gate-specific threshold to avoid irrecoverable null-space loss. Gate 2 specifies the minimum carrier budget: the photon flux or signal-to-noise ratio must exceed a modality-dependent floor. Gate 3 specifies the maximum tolerable calibration error: the mismatch parameter must stay within a tolerance that keeps reconstruction degradation below a design margin. The systematic Gate 1 and Gate 2 sweeps (Supplementary Tables S12–S13) quantify these thresholds for all 12 validated modalities. For example, in SPC, Gate 1 predicts a minimum compression ratio of $\sim 5\%$ (below which information deficiency loss exceeds -7.1 dB and no solver can compensate); in MRI, Gate 2 predicts a minimum SNR floor at noise level $\sigma \approx 1\%$ (below which carrier noise exceeds -11.7 dB and coil sensitivity correction becomes ineffective); in CT, Gate 3 analysis predicts that center-of-rotation alignment must be maintained within ~ 2 px for < 1 dB degradation. These cross-over thresholds convert the abstract question “is this design adequate?” into three quantitative pass/fail constraints.

Design by primitive composition. The Finite Primitive Basis enables a compositional design workflow: a new imaging modality is specified by selecting primitives from the 11-member library, defining their parameters, and connecting them as a typed DAG. The framework then evaluates the candidate design through all three gates before hardware fabrication begins (Figure 1f–g). To demonstrate this workflow concretely, we compose a snapshot compressive video imager from three primitives—Modulate M (binary coded mask), Accumulate Σ (temporal integration across B frames), and Detect D (photon-counting sensor)—matching the CACTI architecture⁸. Gate 1 analysis on the composed DAG predicts that at compression ratio $B = 8$, the measurement matrix retains sufficient rank for ~ 27 dB reconstruction (GAP-TV). Gate 2 analysis predicts a minimum of $\sim 5,000$ peak photons per compressed frame for the solver to operate above the noise floor. Gate 3 analysis identifies mask alignment as the dominant sensitivity: a sub-pixel shift causes 13 dB degradation (Figure 4; Supplementary Table S9), specifying a calibration tolerance of < 0.25 px for the mask fabrication process. This three-gate design specification—minimum compression ratio, minimum photon budget, maximum mask alignment error—is derived entirely from the primitive DAG and validated against the empirical results in the preceding sections.

Systematic design exploration. Scaling beyond individual modalities, the PWM framework maintains a registry of 170 imaging configurations (Table 1), each specified as a primitive DAG with typed carrier, hardware parameters, and gate-specific design thresholds. This registry enables purpose-conditioned system selection: given a measurement task with target resolution, temporal

bandwidth, budget, and sample constraints, the designer queries the registry to identify feasible modalities and rank them by task-normalised adequacy across eight dimensions (acquisition feasibility, temporal and spatial adequacy, observable sufficiency, output recovery quality, budget feasibility, deployment burden, and sample compatibility). For instance, a designer seeking to build a spectral imager for precision agriculture queries the registry with constraints on spectral range (400–1000 nm), minimum band count (≥ 20), frame rate (≥ 30 fps), and budget. The registry returns multiple feasible architectures—coded-aperture (CASSI), mosaic-filter, and filter-wheel systems—ranked by task-normalised adequacy. For each candidate, the three gates generate quantitative design specifications: Gate 1 determines the minimum spatial $\times$ spectral sampling density required for the target reconstruction quality, Gate 2 determines the minimum illumination power for adequate per-band SNR (critical at 30 fps where exposure time is short), and Gate 3 predicts the calibration tolerance for each architecture (*e.g.*, mask alignment < 0.25 px for CASSI, filter registration accuracy for mosaic sensors). This gate-based specification—derived entirely from the primitive DAG of each candidate—enables quantitative comparison across architecturally distinct systems on a common footing, completing the design loop from task requirements to hardware tolerances (Figure 1f–g).

Discussion

The central finding is that the space of imaging forward models has finite structural complexity—11 primitives suffice and are necessary—and that every reconstruction failure decomposes into exactly three independent, testable root causes. This closure extends to particle-beam probes (neutron CT, proton CT, muon tomography) with zero additional primitives, as their DAGs decompose entirely into existing library members (Supplementary Note S24). The twelve validated modalities span the breadth of modern imaging science: from coded aperture cameras (CASSI, CACTI) through clinical scanners (CT, CBCT, MRI, ultrasound) to instruments at the frontier of structural biology (cryo-EM, 2017 Nobel Prize in Chemistry) and super-resolution microscopy (fluorescence, 2014 Nobel Prize in Chemistry). In every case, the same 11 primitives compose the forward model and the same 3 gates diagnose every failure.

The three gates map naturally to the imaging system lifecycle. At the **design stage**, Gates 1 and 2 are the primary concerns: Gate 1 governs information capacity (sampling geometry, encoding strategy, number of measurements), and Gate 2 governs the carrier budget (photon flux, coherence, penetration depth, detector sensitivity). At the **deployment stage**, Gates 1 and 2 are fixed by the engineering decisions already made; what remains—and what drifts—is Gate 3 (operator mismatch due to calibration error, environmental change, or component aging). In well-designed instruments where Gates 1 and 2 have been optimized, Gate 3 emerges as the residual bottleneck: this is itself a Triad prediction, confirmed by our 12-modality validation with +0.8 to +13.9 dB recovery through forward-model correction. For poorly designed systems (extreme undersampling, photon-starved regimes), the Triad predicts Gate 1 or Gate 2 dominance instead—boundary conditions that define the framework’s scope. Solver design remains essential throughout: once the dominant gate is addressed, a better solver on the corrected operator delivers further gains. The Triad does not replace solver research—it tells the practitioner *where the dB are hiding* so that engineering effort targets the intervention with the largest marginal return.

Implications for autonomous scientific discovery. The bounded complexity of imaging physics has consequences that extend beyond calibration. If every imaging forward model—from a \$10 webcam to a particle accelerator beamline—decomposes into the same 11 primitives, then any

autonomous system tasked with “learning to see” faces a *finite search problem* over typed physical operators, not an open-ended function approximation. This reframes the challenge for AI Scientists³⁰: rather than discovering physical laws from scratch, a machine learning system equipped with the OPERATORGRAPH representation needs only to identify which subset of 11 known primitives is active in a new instrument and estimate their parameters from data. The Triad Decomposition further constrains the hypothesis space for failure: an AI Scientist confronting a degraded reconstruction has exactly three root causes to consider, each with a formal test and a known correction strategy. The observation that 9 of 11 primitives are introduced by the first 10 modalities, with the final two (Disperse and Scatter) appearing only for exotic carrier physics, suggests that the primitive manifold is dense at its core and sparse at its boundary—a structure confirmed by the registry’s growth to 170 modalities without requiring a 12th primitive—including particle-beam probes (neutron CT, proton CT, muon tomography) that naive taxonomy places in a distinct carrier family yet decompose fully into existing DAG nodes (Supplementary Note S24). This enables few-shot generalization to new modalities from existing primitive combinations. More broadly, the Finite Primitive Basis Theorem raises a question for computational science beyond imaging: if the forward model of every physical measurement system can be expressed in a small universal grammar, what analogous grammars exist for other physical processes, and what does their existence imply for the long-term trajectory of physics-informed machine learning?

Implications for imaging system design. The Finite Primitive Basis implies that imaging system design is a combinatorial optimization over 11 typed primitives, not an open-ended search. The OPERATORGRAPH representation makes this explicit: a designer specifies which primitives are active, their parameters, and their interconnection topology. The Triad Decomposition then provides a quantitative sensitivity analysis: for any candidate design, Gate 3 analysis predicts which parameters are most sensitive to mismatch, enabling tolerance-aware co-design of hardware and reconstruction algorithms. This is directly relevant to multi-scale camera architectures³¹, where dozens of sub-apertures must be jointly calibrated, and to snapshot compressive imaging systems⁸, where the measurement operator encodes the entire signal recovery problem.

Implications for biology and medicine. The framework has immediate relevance for the two largest imaging user communities. In structural biology, cryo-EM resolution is rate-limited by contrast transfer function (CTF) estimation—a textbook Gate 3 problem. A 200 nm defocus error at 300 kV limits the achievable resolution from ~ 2 Å to ~ 3 Å, and CTFFIND-class estimators require thousands of particles to converge. The PWM Triad diagnoses this as Gate 3 dominance with a 1-parameter correction manifold (Δf), and autonomous defocus calibration recovers $\rho = 1.00$ – 1.12 of the oracle (Supplementary Table S15). In clinical imaging, CBCT image quality in radiation therapy is limited by scatter contamination and geometric mismatch—problems that have driven both physics-based correction via Monte Carlo scatter estimation³² and data-driven approaches including deep learning³³ and reinforcement-learning-based parameter tuning³⁴. AAPM Task Group 142³⁵ mandates monthly mechanical isocentre verification (≤ 2 mm tolerance) and AAPM Task Group 66³⁶ specifies CT-simulator geometric accuracy requirements for treatment planning. The Triad Decomposition provides a unifying perspective on these efforts: scatter is a Gate 3 forward-model mismatch (the assumed scatter-free model diverges from the scatter-contaminated measurement), geometric drift is a Gate 3 parameter error, and learned CBCT-to-CT mappings implicitly compensate for the aggregate forward-model mismatch without decomposing it. Our validation shows that detector offsets of 5–20 pixels—commensurate with the mechanical tolerances flagged by these guidelines—cause 2.5–3.9 dB PSNR degradation with 100% oracle recovery, suggesting

that automated Gate 3 monitoring could complement existing QA protocols. More broadly, ultrasound speed-of-sound inhomogeneity causes geometric distortion and resolution loss in abdominal imaging, and MRI coil sensitivity drift degrades parallel imaging reconstruction. All three failure modes are instances of Gate 3, and all three are correctable through the same forward-model calibration pipeline. The unification of these disparate calibration challenges under a single diagnostic framework suggests a path toward automated quality assurance across the clinical imaging fleet.

Comparison with specialist calibration. PWM adopts the best available calibration method per modality: for MRI, ESPIRiT¹⁰ is used when sufficient calibration data ($\text{ACS} \geq 48$ lines) is available, achieving 85–95% of the oracle correction ceiling; for electron ptychography, ePIE blind position correction¹¹ provides 70–90% recovery; for CT, cross-correlation auto-focus achieves 95–100%; when no specialist method exists (CASSI, CACTI, compressive holography, ultrasound SoS), the modality-agnostic grid-search pipeline provides the first automated calibration (Supplementary Note S14). This principle—use the best domain-specific calibration when available, fall back to physics-model grid-search otherwise—means PWM is not limited to gradient methods but spans the full spectrum from data-driven (ESPIRiT) to model-based (beam-search) calibration. Specialist methods degrade under data-limited conditions (ESPIRiT: -9.29 dB at 24 ACS lines) while PWM maintains positive correction ($+0.75$ dB), demonstrating complementarity: specialist estimates initialize PWM, which refines using forward-model structure across data regimes.

Hardware validation interpretation. The hardware results reveal that Gate 3 sensitivity depends on the *condition number* of the encoding matrix. On real CASSI, perturbation produces smaller degradation ($1.8\times$) than predicted, because the as-built mask already contains unmodeled manufacturing imperfections. On real CACTI, degradation is severe ($10.4\times$), because the simpler temporal-mask optics lack this pre-existing error buffer. On real CT sinograms, CoR offset causes 8–9 dB loss; electron ptychography shows up to 16.1 dB phase degradation; on real PICMUS ultrasound data, compound PW-DAS shows 8.2 dB monotonic degradation with SoS calibration within 2 m/s of nominal; on real EMDB cryo-EM structures, defocus error causes up to 3.0 dB degradation with perfect calibration recovery; and on real patient CT images, detector offset produces 1.1–1.7 dB mean loss. This range—from sub-dB (well-conditioned MRI at $R=2$) to > 16 dB (electron ptychography)—is itself a Triad prediction: the condition number of the encoding matrix determines mismatch sensitivity, with well-conditioned systems showing graceful degradation and ill-conditioned systems showing catastrophic failure. The extended cross-residual analysis further reveals that *self-consistency metrics are misleading* in underdetermined systems (CACTI cross-residual is $462\times$ while self-residual is only $1.12\times$), underscoring the need for forward-model-aware diagnostics.

Boundary conditions and failure modes. The framework has well-defined limitations that inform its scope of applicability:

- **Multi-parameter mismatch:** CASSI recovery ratios under 5-parameter mismatch are moderate ($\rho = 22\text{--}46\%$), reflecting the inherent difficulty of simultaneously correcting multiple coupled parameters on a high-dimensional manifold. Single-parameter correction achieves 85–100%.
- **Nonlinear forward models:** The Triad diagnostic has been validated on linear forward models only; beam hardening CT and phase-wrapped MRI require additional validation (the 11-primitive basis formally covers these via Transform Λ^1).

- **Undeclared mismatch:** Correction is limited to declared mismatch parameter families in the mismatch database; undeclared failure modes (e.g., nonlinear detector drift) require extending the database.
- **Software-perturbation protocol:** Current real-data experiments inject controlled perturbations into calibrated measurements, isolating the effect of each mismatch parameter. The CT, electron ptychography, and MRI experiments use genuinely independent public datasets with unknown calibration states, providing complementary evidence. Full hardware-in-the-loop validation with physical parameter displacement is specified in Methods and Supplementary Note 8 and is underway.

Falsifiable predictions. The Triad framework generates testable predictions across all three gates—including regime transitions that test the decomposition itself, not just individual gate effects:

Gate 1 dominance (information deficiency binds):

1. **SPC at $< 5\%$ compression:** Gate 1 should dominate—correcting illumination non-uniformity should yield < 1 dB gain because the measurement matrix lacks sufficient rank to recover the signal. *Confirmed:* information-deficiency loss reaches -7.1 dB at 5% compression (Supplementary Table S12), matching the $+7.7$ dB Gate 3 correction ceiling and defining the cross-over threshold.
2. **Lensless at PSF blur $\sigma > 2$ px:** Gate 1 loss should exceed the Gate 3 correction ceiling ($+3.6$ dB), making forward-model refinement futile regardless of calibration accuracy. *Confirmed:* -11.1 dB at $\sigma=3$ px (Supplementary Table S12).

Gate 2 dominance (carrier noise binds):

3. **MRI at additive noise $\sigma > 1\%$:** Gate 2 should dominate—coil sensitivity correction should be ineffective because Fourier encoding concentrates signal in a few k-space samples that are disproportionately corrupted. *Confirmed:* -11.7 dB loss at $\sigma=0.01$ (Supplementary Table S13), matching the $+11.2$ dB Gate 3 ceiling and defining one of the sharpest cross-over thresholds in the framework.
4. **Fluorescence at < 10 peak photons:** Shot-noise floor should produce > 4 dB loss, reducing the effective Gate 3 correction margin. *Confirmed:* -6.1 dB at 5 photons (Figure 3b).

Gate 3 dominance (operator mismatch binds):

5. **SIM:** Gate 3 should dominate when pattern phase error exceeds 0.05 rad. Predicted correction: $+3$ – 8 dB.
6. **OCT:** Dispersion mismatch should produce $+2$ – 5 dB correction gain via the Disperse primitive (W).
7. **Ultrasound:** SoS mismatch > 100 m/s should produce monotonic B-mode degradation. *Confirmed:* 8.2 dB across $\Delta c = 10$ – 200 m/s on real PICMUS data, with calibration within 2 m/s of nominal.
8. **Electron ptychography:** Position errors $> 1/10$ probe diameter should trigger Gate 3 dominance. *Confirmed:* $+5$ to $+16$ dB on real SrTiO₃ data (Supplementary Note 15).

Cross-over predictions (regime transitions):

9. **SPC G1↔G3 cross-over at $\sim 5\%$ compression:** Below this threshold, adding measurements yields larger PSNR gains than correcting the forward model; above it, Gate 3 correction dominates. Testable by sweeping compression ratio while simultaneously applying gain-drift mismatch.
10. **MRI G2↔G3 cross-over at $\sigma \approx 1\%$:** The sharpest transition in the framework—MRI switches from G3-dominated ($\sigma < 0.01$, correction gains +11.2 dB) to G2-dominated ($\sigma > 0.01$, noise loss > 11.7 dB) over a single order of magnitude.
11. **CT: pure Gate 3 regime.** CT should remain Gate 3-dominated even at extreme operating conditions (5 angles, 100 photons), because the many-angle sinogram provides sufficient redundancy that Gates 1–2 never bind. *Confirmed:* G1 loss = -4.3 dB and G2 loss = -3.8 dB at extreme versus G3 gain = $+10.7$ dB (Supplementary Tables S12–S13).
12. **Ultrasound G2 immunity:** Compound PW-DAS should remain Gate 2-immune at up to 50% additive RF noise due to $\sqrt{N_{\text{angles}}}$ spatial averaging across 75 steering angles. *Confirmed:* 0.0 dB G2 degradation at 50% noise (Figure 3b).

These twelve predictions span all three gates and their transitions. They are falsifiable: if a modality shows a different dominant gate under the specified conditions, or if a cross-over threshold differs by more than one order of magnitude, the decomposition would require revision. Eight of twelve are confirmed by simulation or hardware data; the remaining four (SIM, OCT, SPC cross-over, MRI cross-over) are directly testable by any laboratory with the relevant instruments.

Acknowledgements. We thank the open-source computational imaging community for making reconstruction code and benchmark datasets publicly available. This work was supported by NextGen PlatformAI C Corp.

Author Contributions. C.Y. conceived the project, designed the TRIAD DECOMPOSITION framework, proved the Finite Primitive Basis Theorem, developed the OPERATORGRAPH IR, implemented the agent and correction systems, performed all simulation and real-data experiments, and wrote the manuscript. X.Y. developed the GAP-TV reconstruction algorithm used as the primary solver across CASSI, CACTI, and SPC experiments, contributed the EfficientSCI architecture used for CACTI validation, provided the CASSI and CACTI forward model specifications and mismatch parameter characterizations that define the 5-parameter mismatch model, validated the real-data experimental protocols for both CASSI (TSA scenes) and CACTI instruments, and edited the manuscript.

Competing Interests. C.Y. is an employee of NextGen PlatformAI C Corp, which develops the PWM platform. The authors declare no other competing interests.

Ethics Declarations. This study does not involve human participants, human tissue, or animals. All experiments use publicly available benchmark datasets and simulated data.

Data Availability. All synthetic measurement data can be regenerated using the OPERATORGRAPH templates and mismatch parameters in the Supplementary Information. The KAIST hyperspectral dataset³⁷ and TSA real-data scenes used for CASSI experiments are publicly available. CACTI real-data scenes are available from the EfficientSCI repository²². CT sinograms are from the FIPS walnut dataset (Zenodo 1254206) and Helsinki Tomography Challenge 2022 (Zenodo 6984868). The 4D-STEM electron ptychography dataset (SrTiO₃ [001]) is from Zenodo 5113449. Multi-coil MRI k -space data (M4Raw) is from Zenodo 8056074. Ultrasound, cryo-EM, CBCT, compressive holography, and fluorescence microscopy experiments use procedurally generated phantoms with parameters and random seeds fully specified in Methods; all scripts are included in the repository.

Code Availability. The PWM codebase, including all OPERATORGRAPH templates, agent implementations, real-data validation scripts, and evaluation pipelines, is available at https://github.com/integritynoble/Physics_World_Model under the PWM Noncommercial Share-Alike License v1.0 (see LICENSE in the repository).

Correspondence. Correspondence and requests for materials should be addressed to C.Y. (integrityyang@gmail.com).

Online Methods

OperatorGraph Specification

Formal definition. The OPERATORGRAPH intermediate representation encodes the forward physics of any computational imaging modality as a directed acyclic graph (DAG) $\mathcal{G} = (\mathcal{V}, \mathcal{E})$. Each node $v_i \in \mathcal{V}$ wraps a *primitive operator* and implements two entry points: `forward( $x$ )  $\rightarrow$   $y$` and `adjoint( $y$ )  $\rightarrow$   $x$` , the latter defined only when the primitive is linear. Edges $e_{ij} \in \mathcal{E}$ encode data flow: the output of node v_i is passed to node v_j . Each node additionally exposes a set of learnable parameters θ_i that may be perturbed during mismatch simulation or optimized during calibration, as well as read-only metadata flags (`is_linear`, `is_stochastic`, `is_differentiable`). The graph is stored as a declarative YAML specification (`OperatorGraphSpec`) and compiled to an executable `GraphOperator` object by the `GraphCompiler`.

Node types. Primitive operators fall into two categories:

- **Linear operators.** Convolution (`conv2d`), mask modulation (`mask_modulate`), subpixel shift (`subpixel_shift_2d`), Radon transform (`radon_fanbeam`), Fourier encoding (`fourier_encode`), spectral dispersion (`spectral_disperse`), Fresnel propagation (`fresnel_propagate`), random projection (`random_project`), and structured illumination (`sim_modulate`). Each implements both `forward()` and `adjoint()`.
- **Nonlinear operators.** Squared magnitude (`magnitude_sq`), Poisson–Gaussian noise (`poisson_gaussian`), saturation clipping (`saturation_clip`), phase retrieval nonlinearity (`phase_abs`), and detector quantization (`quantize`). These set `is_linear = False` and raise `NotImplementedError` on `adjoint()`, except where a well-defined pseudo-adjoint exists (*e.g.*, the identity adjoint for magnitude-squared in Gerchberg–Saxton-type algorithms).

Adjoint consistency and Lipschitz bounds as mathematical safety rails. Two structural constraints distinguish the OPERATORGRAPH IR from standard deep-learning forward models and prevent either nonlinear primitive family from becoming a universal approximator.

First, *adjoint consistency*: correctness of every linear primitive is verified by a randomized dot-product test. For a primitive A with forward map $A : \mathbb{R}^n \rightarrow \mathbb{R}^m$, we draw $x \sim \mathcal{N}(0, I_n)$ and $y \sim \mathcal{N}(0, I_m)$ and compute

$$\delta = \frac{|\langle A^*y, x \rangle - \langle y, Ax \rangle|}{\max(|\langle A^*y, x \rangle|, \epsilon)} \quad (2)$$

where $\epsilon = 10^{-12}$ guards against division by zero. The test is repeated $n_{\text{trials}} = 5$ times with independent random draws; the primitive passes if $\delta_{\text{max}} < 10^{-6}$. At the graph level, a compiled `GraphOperator` composed entirely of linear nodes executes the same test over the composed forward–adjoint chain. A `GraphAdjointCheckReport` records n_{trials} , δ_{max} , and $\bar{\delta}$ for audit. All graph templates that consist solely of linear primitives pass this check. Adjoint consistency is not merely a numerical correctness guarantee: it is a *physical faithfulness certificate*. A model whose adjoint is inconsistent implements a physically impossible energy accounting, making gradient-based calibration unreliable and certifiable reconstruction bounds vacuous. Neural network forward models lack this certificate by construction, since their weight matrices have no physical meaning and their transposes are not computed or validated.

Second, *Lipschitz bounds*: the two nonlinear primitive families, Detect D and Transform Λ , are each restricted to five canonical function families with at most two scalar parameters. This restriction enforces bounded Lipschitz constants ($\text{Lip}(\Lambda_k) \leq L$ for the explicit L derived in ¹) and prevents either primitive from becoming a universal approximator in the sense of Cybenko³⁸. Concretely: a generic neural network layer with sigmoid activations can approximate any continuous function on a compact domain; neither Detect nor Transform can, because their function families are closed under composition only within the five enumerated types. This non-universality is the key property that makes the 11-primitive library *falsifiable*: if a modality’s forward physics cannot be represented within the restricted families, the extension protocol (Main Text, “Extension protocol”) fires and a new primitive must be justified physically. The combination of adjoint consistency and bounded Lipschitz nonlinearity provides the mathematical safety rails that make OPERATORGRAPH-based reconstruction both interpretable and certifiable—properties that standard physics-informed neural networks³⁹ achieve only approximately and without modality-agnostic guarantees.

Graph compilation. The compiler executes a four-stage pipeline:

1. **Validate.** Confirm acyclicity via topological sort (Kahn’s algorithm), verify that every `primitive_id` exists in the global `PRIMITIVE_REGISTRY`, reject duplicate `node_id` values, and optionally verify shape compatibility along edges when a `canonical_chain` metadata flag is set.
2. **Bind.** Instantiate each primitive with its parameter dictionary θ_i .
3. **Plan forward.** The topological sort yields a sequential execution plan $(v_{\pi(1)}, \dots, v_{\pi(|V|)})$.
4. **Plan adjoint.** For graphs where `all_linear = True`, the adjoint plan reverses the topological order and applies each node’s individual adjoint in sequence, implementing the chain rule $A^* = A_1^* \circ \dots \circ A_{|V|}^*$ for a composition $A = A_{|V|} \circ \dots \circ A_1$. For graphs containing nonlinear nodes, the adjoint plan is not generated, and any call to `adjoint()` raises `NotImplementedError` at runtime.

The compiled `GraphOperator` is serializable to JSON and hashable via SHA-256 for provenance tracking in RunBundle manifests.

Template library. The `graph_templates.yaml` registry contains 170 templates spanning all five carrier families. Of these, 12 modalities carry full end-to-end Scenario I–IV correction validation across all five carrier families (Supplementary Table S3). Representative modalities by carrier family include:

- **Optical and X-ray photons:** CASSI, SPC, CACTI, structured illumination microscopy (SIM), confocal, light-sheet, holography, ptychography, Fourier ptychographic microscopy (FPM), optical coherence tomography (OCT), lensless imaging, light field, integral imaging, neural radiance fields (NeRF), Gaussian splatting, fluorescence lifetime imaging (FLIM), diffuse optical tomography (DOT), phase retrieval, X-ray computed tomography (CT), and cone-beam CT (CBCT).
- **Electrons:** Electron diffraction, electron backscatter diffraction (EBSD), electron energy loss spectroscopy (EELS), and electron holography.
- **Nuclear spins (MRI):** Functional MRI (fMRI), diffusion-weighted MRI (DW-MRI), and magnetic resonance spectroscopy (MRS).
- **Acoustic waves:** Ultrasound B-mode, Doppler ultrasound, shear-wave elastography, sonar, and photoacoustic tomography (combines optical excitation with acoustic detection).
- **Particle-beam probes:** Neutron tomography, proton CT, and muon tomography. Each decomposes into existing primitives with no extension required: neutron CT follows the X-ray CT DAG ($P \rightarrow \Lambda \rightarrow D$, Beer–Lambert attenuation with nuclear cross-section μ_n); proton CT inserts a Bethe–Bloch stopping-power stage as Transform Λ (#11); muon tomography uses Scatter R (#10) for multiple Coulomb scattering and POCA vertex reconstruction (Supplementary Note S24).

Fidelity levels. Each template is parameterized by a fidelity level that controls the degree of physical realism in the simulated forward model:

Level 1 (Linear, shift-invariant): The forward model is a linear, spatially uniform operator—the simplest approximation, suitable for initial diagnostics and rapid prototyping.

Level 2 (Linear, shift-variant): Spatially varying operator parameters (e.g. non-uniform illumination, position-dependent PSF, multi-coil sensitivity maps in MRI). Adds a modality-appropriate noise model (Poisson shot noise plus Gaussian read noise for photon-counting modalities, Rician noise for MRI, Poisson for CT).

Level 3 (Nonlinear, ray/wave-based): Includes nonlinear effects such as beam hardening, phase wrapping, and scattering, captured by the Transform Λ primitive. Perturbation families and ranges are specified in `mismatch_db.yaml`.

Level 4 (Full-wave / Monte Carlo): Complete physical simulation including wave-optical propagation, spatially varying aberrations, detector nonlinearities, and environmental drift. Currently implemented for holography and ptychography.

All 11 primitives in the library $\mathcal{B}$ apply uniformly across every fidelity level; the levels organize simulation complexity, not theorem scope.

Triad Decomposition Formalization

The TRIAD DECOMPOSITION asserts that the quality of any computational imaging reconstruction is bounded by three fundamental gates. Rather than a qualitative guideline, PWM quantifies each gate numerically and uses the resulting scores to diagnose the dominant bottleneck in any imaging configuration.

Gate 1 (Recoverability). Recoverability measures the information-theoretic capacity of the sensing geometry. We quantify it via the *effective compression ratio* $r = m/n$, where m is the number of independent measurements and n the dimension of the signal. The `compression_db.yaml` registry (1,186 lines) stores, for each modality, a lookup table mapping compression ratio to expected reconstruction PSNR under ideal conditions, obtained from calibration experiments or published benchmarks. Each entry carries a `provenance` field citing the source (paper DOI, internal experiment ID, or theoretical formula). Additional recoverability indicators include the effective rank of the measurement matrix (estimated via randomized SVD for large operators), the dimension of the null space, and the restricted isometry property (RIP) constant where analytically tractable (*e.g.*, for Gaussian random projections in SPC).

Gate 2 (Carrier Budget). The carrier budget quantifies the signal-to-noise ratio (SNR) of the measurement channel. The photon-budget module consumes the `photon_db.yaml` registry which stores, per modality, a deterministic photon model parameterized by source power, quantum efficiency, exposure time, and detector characteristics. It classifies the noise regime into one of three categories: *shot-limited* (Poisson-dominated, $\text{SNR} \propto \sqrt{N_{\text{photon}}}$), *read-limited* (Gaussian read noise dominates, $\text{SNR} \propto N_{\text{photon}}/\sigma_{\text{read}}$), and *dark-current-limited* (long exposures where dark current accumulation dominates). The output is a `PhotonReport` containing the estimated SNR in decibels, the noise regime classification, per-element photon count, and a feasibility verdict (`sufficient`, `marginal`, or `insufficient`).

Gate 3 (Operator Mismatch). Operator mismatch quantifies the discrepancy between the assumed forward model H_{nom} and the true physical operator H_{true} . The mismatch scoring module consults `mismatch_db.yaml` which catalogs, for each modality, the set of mismatch parameters (spatial shifts, rotational offsets, dispersion errors, PSF deviations, coil sensitivity errors, center-of-rotation offsets, *etc.*), their typical ranges, and available correction methods. The mismatch severity score $s \in [0, 1]$ is computed as the normalized ℓ_2 distance $\|\boldsymbol{\theta}_{\text{true}} - \boldsymbol{\theta}_{\text{nom}}\|/\|\boldsymbol{\theta}_{\text{range}}\|$, where $\boldsymbol{\theta}_{\text{range}}$ is the per-parameter dynamic range from the registry. Sensitivity analysis $\partial\text{PSNR}/\partial\theta_k$ is estimated via finite differences on the forward model. The output is a `MismatchReport` containing the severity score, the dominant mismatch parameter, the recommended correction method, and the expected PSNR gain from correction.

Gate binding determination. Given reconstruction results under the four-scenario protocol (the Evaluation Protocol section below), PWM identifies the dominant gate by comparing three cost terms:

$$C_{\text{mismatch}} = \text{PSNR}_{\text{I}} - \text{PSNR}_{\text{II}} \quad (3)$$

$$C_{\text{noise}} = \text{PSNR}_{\text{ideal}} - \text{PSNR}_{\text{noisy}} \quad (4)$$

$$C_{\text{recover}} = \text{PSNR}_{\text{limit}} - \text{PSNR}_{\text{I}} \quad (5)$$

where PSNR_{I} is the reconstruction PSNR under Scenario I (ideal operator), PSNR_{II} under Scenario II (mismatched operator), $\text{PSNR}_{\text{noisy}}$ under the corresponding noisy condition, and $\text{PSNR}_{\text{limit}}$ is the theoretical upper bound from the compression table. The dominant gate is $\arg \max_g C_g$.

TriadReport. For every diagnosis, PWM produces a TRIADREPORT: a Pydantic-validated structured artifact comprising `dominant_gate` (enum: `recoverability`, `carrier_budget`, `operator_mismatch`), `evidence_scores` (three floats, one per gate), `confidence_interval` (float, 95% CI width from bootstrap), `recommended_action` (string, *e.g.* “increase compression ratio” or “apply mismatch correction”), and `parameter_sensitivities` (dictionary mapping each mismatch parameter name to its $\partial \text{PSNR} / \partial \theta_k$ value). The TRIADREPORT is mandatory—PWM does not permit a reconstruction to be reported without an accompanying diagnosis.

Recovery ratio. We define the *recovery ratio*

$$\rho = \frac{\text{PSNR}_{\text{IV}} - \text{PSNR}_{\text{II}}}{\text{PSNR}_{\text{I}} - \text{PSNR}_{\text{II}}} \quad (6)$$

which lies in $[0, 1]$ under standard convexity conditions (see Supplementary Note 1 for formal analysis; values $\rho > 1$ are possible when the corrected operator provides beneficial regularization). $\rho = 0$ indicates that calibration yields no benefit (mismatch is not the bottleneck), while $\rho = 1$ indicates that calibration fully closes the mismatch gap.

Agent System Architecture

The three gates are implemented as a deterministic scoring pipeline: an orchestrator maps the user request to a modality from the registry, then dispatches three parallel scoring modules—one per gate—whose reports are fused by a bottleneck classifier that identifies the dominant gate and by a negotiator that enforces cross-gate veto rules (*e.g.*, rejecting reconstruction when photon starvation coincides with aggressive compression). All quantitative decisions are deterministic; an LLM is used only as an optional fallback for natural-language modality mapping and is never on the scoring path. The full agent architecture and ablation studies are described in a companion paper.

Contract system. Inter-agent communication uses 25 Pydantic v2 contract models. All contracts inherit from `StrictBaseModel`, which enforces `extra="forbid"` (no unexpected fields), `validate_assignment=True` (mutations re-validated), and a model validator that rejects NaN and Inf in any float field. Bounded scores use `Field(ge=0.0, le=1.0)`. Enums are string enums for human-readable JSON serialization. This design ensures that pipeline failures surface immediately as validation errors rather than propagating silently.

YAML registries. The system is driven by 9 YAML registries totalling 7,034 lines: `modalities.yaml` (modality definitions), `graph_templates.yaml` (OperatorGraph skeletons), `photon.db.yaml` (photon models), `mismatch.db.yaml` (mismatch parameters and correction methods), `compression.db.yaml` (recoverability tables with provenance), `solver_registry.yaml` (solver configurations), `primitives.yaml` (primitive operator metadata), `dataset_registry.yaml` (dataset locations and formats), and `acceptance_thresholds.yaml` (pass/fail thresholds per metric).

Correction Algorithms

We implement two complementary algorithms for operator mismatch correction. Crucially, both algorithms operate on the forward operator parameters θ rather than the reconstruction solver weights, making them *solver-agnostic*: the corrected operator $H(\hat{\theta})$ benefits any downstream solver (GAP-TV, MST-L, HDNet⁴⁰, CST, *etc.*) without retraining.

Algorithm 1: Hierarchical Beam Search. The coarse correction phase employs a hierarchical search strategy to rapidly explore the mismatch parameter space. For CASSI, the five-parameter mismatch model comprises mask affine parameters (spatial shifts dx , dy and rotation θ) and dispersion parameters (slope a_1 and axis angle α); an optional sixth parameter, PSF width σ_{psf} , is available but not used in the primary experiments. The algorithm proceeds as follows:

1. **1D sweeps.** Each parameter is swept independently over its full range while holding others at nominal values. This produces five 1D cost curves from which coarse optima are extracted.
2. **3D beam search.** The mask affine subspace (dx, dy, θ) is searched over a $5 \times 5 \times 5$ grid centered on the 1D optima. The top- k ($k = 5$) candidates by reconstruction PSNR are retained.
3. **2D beam search.** For each retained mask candidate, the dispersion subspace (a_1, α) is searched over a 5×7 grid. The joint top- k candidates are retained.
4. **Coordinate descent refinement.** Three rounds of univariate refinement on each parameter, shrinking the search interval by factor 2 at each round, produce the final estimate $\hat{\theta}_{\text{Alg1}}$.

Total runtime is approximately 300 seconds per scene on a single GPU. Accuracy is ± 0.1 – 0.2 pixels for spatial parameters and $\pm 0.05^\circ$ for angular parameters.

Algorithm 2: Joint Gradient Refinement. The fine correction phase uses a differentiable forward model to jointly optimize all mismatch parameters via gradient descent. The key components are:

1. **Differentiable mask warp.** The binary mask is warped by a continuous affine transformation using bilinear interpolation, implemented as a custom PyTorch module (`DifferentiableMaskWarpFixed`). The mask values are passed through a straight-through estimator (STE) to maintain binary structure while permitting gradient flow.
2. **Differentiable forward model.** The CASSI forward model $y = \text{CASSI}(x; \theta)$ is implemented as a differentiable PyTorch module (`DifferentiableCassiforwardSTE`) that accepts mismatch parameters as differentiable inputs.
3. **GPU grid initialization.** A full-range 3D grid search over (dx, dy, θ) with $9 \times 9 \times 7 = 567$ points provides diverse starting candidates. The top 9 candidates seed multi-start gradient refinement.
4. **Staged gradient refinement.** Each of the 9 candidates is refined using Adam optimization (learning rate 10^{-2} , decaying to 10^{-3}) for 200 steps. For each candidate, 4 random restarts with jittered initialization guard against local minima. The loss function is the negative PSNR computed via an unrolled K -iteration differentiable GAP-TV solver (`DifferentiableGAPTV`, $K = 10$ unrolled iterations).

Total runtime for Algorithm 2 is approximately 3,200 seconds (200 steps $\times$ 4 restarts $\times$ 9 candidates with early stopping). Accuracy improves to ± 0.05 –0.1 pixels, a 3–5 $\times$ improvement over Algorithm 1. The two algorithms are used sequentially in practice: Algorithm 1 provides a warm start, and Algorithm 2 refines to sub-pixel precision.

Evaluation Protocol

Four-Scenario Protocol. We evaluate every modality under four standardized scenarios that isolate different sources of quality degradation:

Scenario I (Ideal): $\mathbf{y}_{\text{obs}} = H_{\text{true}} \mathbf{x}_{\text{gt}}$; reconstruct with H_{true} . In this scenario the system is perfectly calibrated ($H_{\text{true}} = H_{\text{nom}}$), so the operator used for reconstruction matches the one that generated the data. This yields the oracle upper bound on reconstruction quality, limited only by the sensing geometry and solver convergence.

Scenario II (Mismatch): $\mathbf{y}_{\text{obs}} = H_{\text{true}} \mathbf{x}_{\text{gt}}$; reconstruct with H_{nom} ($H_{\text{nom}} \neq H_{\text{true}}$). This is the standard operating condition in practice: the measurement is generated by the true physics, but the reconstruction uses a nominal (potentially mismatched) forward model.

Scenario III (Oracle): Same measurements as Scenario II ($\mathbf{y}_{\text{obs}} = H_{\text{true}} \mathbf{x}_{\text{gt}}$ with $H_{\text{true}} \neq H_{\text{nom}}$); reconstruct with H_{true} instead of H_{nom} . Provides the correction ceiling: the best reconstruction achievable when the true operator is known exactly, applied to data that were sensed by the mismatched system. The gap between Scenario III and Scenario I reveals the irreducible loss from the degraded sensing configuration itself (e.g., a shifted mask pattern is suboptimal even when perfectly known).

Scenario IV (Corrected): $\mathbf{y}_{\text{obs}} = H_{\text{true}} \mathbf{x}_{\text{gt}}$; reconstruct with $\hat{H} = H(\hat{\boldsymbol{\theta}})$ where $\hat{\boldsymbol{\theta}}$ is estimated by Algorithms 1 and 2. This quantifies the benefit of mismatch calibration.

Metrics. Reconstruction quality is assessed using three complementary metrics:

- **PSNR** (peak signal-to-noise ratio, in dB): the primary metric, computed per scene and averaged. For signals normalized to $[0, 1]$, $\text{PSNR} = 10 \log_{10}(1/\text{MSE})$. For SPC data normalized to $[0, 255]$, the peak value is 255.
- **SSIM** (structural similarity index): captures perceptual quality including luminance, contrast, and structural components, computed with a Gaussian window of width 11 and standard deviation 1.5.
- **SAM** (spectral angle mapper): for hyperspectral modalities (CASSI), measures the angle between predicted and true spectral vectors at each spatial location, reported in degrees. Lower is better.

Datasets.

- **CASSI**: 10 scenes from the KAIST dataset³⁷, each a $256 \times 256 \times 28$ spectral cube (28 spectral bands from 450 nm to 650 nm). Data range $[0, 1]$.
- **CACTI**: 6 benchmark videos, each $256 \times 256 \times 8$ (8 temporal frames encoded per snapshot). Data range $[0, 1]$.

- **SPC:** 11 natural images from the Set11 benchmark, each 256×256 grayscale. Data range $[0, 255]$.

All per-scene metrics are reported individually as well as averaged, and all reconstruction arrays are saved as NumPy NPZ files.

Experimental Details

Hardware. All experiments are conducted on a single NVIDIA GPU. Algorithm 1 (beam search) and all solver-based reconstructions use the GPU for matrix–vector products and FFT operations. Algorithm 2 (gradient refinement) additionally uses PyTorch automatic differentiation on the same GPU.

CASSI configuration. The coded aperture snapshot spectral imaging (CASSI) system uses a TSA-Net binary mask of dimensions 256×256 , with 28 spectral bands dispersed along the spatial dimension. The five-parameter mismatch model $\theta = (dx, dy, \theta, a_1, \alpha)$, where dx, dy are spatial shifts (pixels), θ is rotation (degrees), a_1 is dispersion slope (pixels/band), and α is dispersion axis angle (degrees). An optional sixth parameter (PSF blur width σ_{psf}) is not used in the primary experiments. These values were determined through systematic characterization of realistic CASSI assembly errors (Supplementary Note 8); the true parameters are $dx=0.5$ px, $dy=0.3$ px, $\theta=0.1^\circ$, $a_1=2.02$, $\alpha=0.15^\circ$. Solvers evaluated include TwIST⁴¹, GAP-TV⁴², DGSMP⁴³, MST-L⁷, and CST-L⁴⁴, all of which receive the same operator and differ only in their reconstruction algorithm. The supplementary per-scene analysis additionally includes DeSCI⁴⁵ and HDNet⁴⁰.

Real-data validation. The TSA real hyperspectral dataset¹² consists of 5 scenes at 660×660 spatial resolution with 28 spectral bands and mask-shift step 2. Four solvers are evaluated: GAP-TV (200 iterations), HDNet (pre-trained checkpoint, full spatial resolution), MST-S and MST-L (pre-trained checkpoints, centre-cropped to 256×256 due to hardcoded spatial assumptions in the model architecture). The coded aperture mask is perturbed by $dx = 0.5$ px, $dy = 0.3$ px to simulate assembly-induced mismatch. No ground truth is available; quality is assessed via the normalised measurement residual $r = \|\mathbf{y} - H\hat{\mathbf{x}}\|^2 / \|\mathbf{y}\|^2$.

CACTI configuration. The coded aperture compressive temporal imaging system uses binary temporal masks of dimensions 256×256 , encoding 8 video frames into a single snapshot measurement. Mismatch is parameterized as a temporal mask timing offset (sub-frame shift). The default solver is EfficientSCI²². *Real-data validation.* The EfficientSCI real temporal dataset²² consists of 4 dynamic scenes (duomino, hand, pendulumBall, waterBalloon) at 512×512 with compression ratio 10. The real mask is stored separately from the measurement data. Two solvers are evaluated: GAP-TV (50 iterations) and PnP-FFDNet (50 iterations with FFDNet denoiser). Mismatch is induced by shifting the mask by $dx = 0.5$ px, $dy = 0.3$ px. Quality is assessed via the normalised measurement residual and total variation of the reconstruction.

SPC configuration. The single-pixel camera uses random binary measurement patterns at three compression ratios: 10%, 25%, and 50% ($r = m/n \in \{0.10, 0.25, 0.50\}$). Mismatch is modeled as an exponential gain drift ($g_i = \exp(-\alpha \cdot i)$) on the measurement matrix. The default solver is FISTA-TV with total-variation regularization.

Lensless imaging configuration. Lensless cameras replace conventional optics with a diffuser placed directly on the sensor, making the forward model a 2D convolution with the measured point-spread function (PSF). The object is a 64×64 image convolved with a Gaussian PSF of width $\sigma = 2.0$ px. Mismatch is parameterized as PSF width error $\Delta\sigma \in \{0.5, 1.0, 2.0, 3.0\}$ px, simulating an error in the assumed pinhole-to-sensor distance. Five structurally diverse phantoms are used ($N=5$). The default solver is FISTA-TV (80 iterations). Calibration uses forward-model fitting on a known reference target: $\sigma_{\text{cal}} = \arg\min_{\sigma} \|y_{\text{cal}} - h_{\sigma} * x_{\text{cal}}\|^2$. *Real-data validation.* Five DiffuserCam DLMD Mirflickr scenes²³ are used to corroborate simulation results on physical photographic content.

Compressive holography configuration. Multi-depth inline holography encodes a $(4 \times 64 \times 64)$ 3D object into a single (64×64) hologram via Fresnel propagation at four depth planes with spacing $200 \mu\text{m}$, wavelength $\lambda = 532 \text{ nm}$, and pixel pitch $5 \mu\text{m}$. Mismatch is parameterized as propagation distance error $\Delta z \in \{10, 50, 100, 200\} \mu\text{m}$ applied uniformly to all depth planes. The default solver is FISTA-TV (80 iterations, $\lambda_{\text{TV}} = 0.005$). Calibration uses hologram residual minimisation: grid search over distance error candidates with the search range clamped to ensure all propagation distances remain positive.

Fluorescence microscopy configuration. Widefield fluorescence imaging uses a dual-PSF Stokes-shift model with Gaussian excitation PSF ($\sigma_{\text{ex}} = 1.5$ px) and emission PSF ($\sigma_{\text{em}} = 2.0$ px), quantum yield $\eta = 0.7$, and background level $b = 0.02$. The specimen is a 64×64 image with fluorescent puncta, diffuse organelles, and filamentary structures. Mismatch is parameterized as PSF sigma error $\Delta\sigma \in \{0.1, 0.3, 0.5, 1.0\}$ px applied to both excitation and emission PSFs. The default solver is Richardson–Lucy (80 iterations). Calibration uses a 9×9 grid search over $(\sigma_{\text{ex}}, \sigma_{\text{em}})$ centered at the nominal values, selecting the pair that minimizes the measurement residual.

CT configuration. Fan-beam geometry with 180 projections over 180° . Mismatch is modeled as a center-of-rotation (CoR) offset, which produces characteristic arc artifacts in the reconstruction. The default solver is filtered back-projection (FBP)¹⁵ with a Ram-Lak filter, supplemented by iterative SART for comparison.

CBCT configuration. Cone-beam CT (CBCT) detector offset validation uses five real images—three LoDoPaB-CT patient slices²⁵, one FIPS walnut micro-CT central slice²⁶, and one HTC 2022 sample²⁷—all resized to 128×128 with 360-angle parallel-beam projections. Detector offset mismatch is simulated by shifting the sinogram along the detector axis by $\Delta s \in \{2, 5, 10, 15, 20\}$ pixels. The default solver is filtered backprojection (FBP) with Shepp–Logan filter. Calibration uses grid search over 51 offset candidates in $[-25, 25]$ px, selecting the value that maximizes reconstruction PSNR.

Electron ptychography configuration. Electron ptychography uses 4D-STEM data: a focused probe is scanned across a 128×128 grid, recording a convergent-beam electron diffraction (CBED) pattern at each position (300 kV, SrTiO₃ [001] from Zenodo 5113449). The forward model is Fresnel near-field propagation of the exit wave through the specimen. Mismatch is parameterized as probe position jitter $\Delta p \in \{0.5, 1.0, 2.0, 4.0\}$ px, simulating scan-coil hysteresis or sample drift. The default solver is integrated centre-of-mass (iCoM) phase retrieval. Calibration uses ePIE blind position correction¹¹.

Cryo-EM configuration. Cryo-EM imaging is modeled as contrast transfer function (CTF) filtering of a 2D projected potential (128×128 , pixel size 0.1 nm). The CTF is parameterized by defocus $\Delta f = -2000 \text{ nm}$, spherical aberration $C_s = 2.0 \text{ mm}$, electron wavelength $\lambda = 0.00251 \text{ nm}$ (300 kV), with a B-factor envelope ($B = 2 \text{ nm}^2$) and ice-thickness attenuation (mean free path 350 nm , thickness 50 nm). Mismatch is parameterized as defocus error $\Delta(\Delta f) \in \{100, 200, 500, 1000\} \text{ nm}$. The default solver is Wiener filtering with $\text{SNR} = 50$. Calibration uses grid search over 51 defocus values in $[-3000, -500] \text{ nm}$, selecting the value that maximizes reconstruction PSNR.

MRI configuration. Cartesian k -space sampling with $4\times$ acceleration (25% of k -space lines acquired). Mismatch is parameterized as a 5% multiplicative error in the coil sensitivity maps used for parallel imaging reconstruction. The default solver is CG-SENSE¹⁷ with ℓ_1 -wavelet regularization ($\lambda = 10^{-3}$, 30 iterations). *Scenario IV calibration (ESPIRiT-adopted).* For MRI, Scenario IV adopts ESPIRiT¹⁰ as the calibration method: coil sensitivity maps are estimated directly from the central k -space autocalibration signal (ACS) region via eigenvalue decomposition of the calibration matrix, then used in the CG-SENSE reconstruction. When ACS data is sufficient (≥ 48 lines), ESPIRiT achieves 85–95% of the oracle correction ceiling. For data-limited regimes (< 32 ACS lines) where ESPIRiT degrades, the fallback is a grid search over per-coil amplitude and phase scaling (beam-search); this fallback is also the Sc. IV method for all modalities without an established specialist calibration algorithm (CASSI, CACTI, compressive holography, ultrasound). The protocol evaluates three conditions—Sc. I (true maps), Sc. II (5% mismatched maps), and Sc. IV (ESPIRiT-calibrated maps)—on the same CG-SENSE solver to isolate calibration quality from solver design.

Ultrasound configuration. Pulse-echo B-mode imaging is simulated with a 64-element linear array, 5 MHz center frequency, element pitch 0.3 mm , sampling rate 100 MHz with 1024 time samples, and speed of sound (SoS) $c = 1540 \text{ m/s}$. The tissue phantom is a 128×128 reflectivity map with Rayleigh-distributed speckle, point scatterers, and anechoic cyst regions. Frequency-dependent attenuation follows $\alpha(f) = 0.5 \text{ dB cm}^{-1} \text{ MHz}^{-1}$. Mismatch is parameterized as SoS error $\Delta c \in \{50, 100, 200, 400\} \text{ m/s}$, perturbing time-of-flight calculations. The default solver is delay-and-sum (DAS) beamforming (operator adjoint). Calibration uses grid search over 21 SoS candidates in $[1440, 1640] \text{ m/s}$, selecting the value that maximizes reconstruction PSNR.

Controlled hardware experiment protocol. The software-perturbation protocol above applies calibrated mask shifts to existing real measurements. A full hardware-in-the-loop validation requires physically displacing the coded aperture mask and re-acquiring data. The protocol proceeds as follows: (i) acquire a baseline dataset with the mask at its factory-calibrated position; (ii) physically translate the mask by a known displacement ($\Delta x \in \{0.25, 0.5, 1.0\} \text{ px}$ equivalent, verified by micrometer stage) and re-acquire under identical illumination; (iii) reconstruct both datasets with the factory mask specification and compute the PSNR degradation and measurement residual; (iv) apply PWM autonomous calibration and measure recovery. This protocol isolates the mismatch effect from all other sources of variation (illumination changes, detector drift, scene variation). Additionally, a multi-unit variation study comparing 2+ camera units of the same design quantifies the inter-unit mismatch baseline—the residual calibration error present in any production system. Clinical CT phantom validation (ACR Gammex 464) and clinical MRI validation (fastMRI⁴⁶) configurations are detailed in Supplementary Note S25.

Real experimental data. Three of the five multi-phantom modalities are validated on real experimental data from established benchmarks: ultrasound uses PICMUS experimental phantom recordings and in-vivo carotid scans²⁸ plus one DeepUS CIRS-040GSE acquisition²⁹; cryo-EM uses five EMD-3D density maps (EMD-5778, EMD-2984, EMD-6287, EMD-11103, EMD-21375) projected at random orientations; CT uses three LoDoPaB-CT patient slices²⁵, one FIPS walnut μ CT scan²⁶, and one HTC 2022 sample²⁷. Compressive holography and fluorescence microscopy retain synthetic multi-phantom benchmarks as no public datasets with calibrated ground truth are available for these modalities.

Statistical Analysis

Per-scene reporting. All metrics are reported per scene, not merely as dataset averages. This enables identification of scene-dependent failure modes (*e.g.*, spectrally flat scenes that are inherently harder for CASSI, or textureless regions that challenge SPC).

Summary statistics. For each modality and scenario, we report the mean $\pm$ standard deviation of PSNR, SSIM, and SAM across all scenes. For CASSI (10 scenes), we additionally report the per-band PSNR to assess spectral uniformity of reconstruction quality.

Recovery ratio confidence intervals. The recovery ratio ρ (Equation (6)) is a ratio of differences and therefore sensitive to noise in the constituent PSNR values. We compute 95% confidence intervals via the bootstrap percentile method with $B = 1,000$ resamples. At each bootstrap iteration, we resample the scene set with replacement, recompute the mean PSNR for each scenario, and derive ρ . The 2.5th and 97.5th percentiles of the bootstrap distribution define the 95% CI.

Parameter recovery accuracy. For mismatch correction experiments, we report the root-mean-square error (RMSE) between the estimated and true mismatch parameters:

$$\text{RMSE}_k = \sqrt{\frac{1}{N_{\text{scene}}} \sum_{i=1}^{N_{\text{scene}}} (\hat{\theta}_{k,i} - \theta_{k,\text{true}})^2} \quad (7)$$

where k indexes the mismatch parameter, i indexes the scene, and N_{scene} is the number of test scenes. Uncertainty in the RMSE is estimated via bootstrap ($B = 1,000$).

Ablation significance. Ablation studies (removal of the photon-budget, recoverability, or mismatch scoring module, or RunBundle discipline) are evaluated by comparing the full-pipeline PSNR against each ablated variant. We report the PSNR difference ΔPSNR per modality and verify that each component contributes ≥ 0.5 dB across all validated modalities, establishing practical significance.

Code and Data Availability

Source code. The complete PWM framework, including all agents, the OperatorGraph compiler, correction algorithms, YAML registries, and evaluation scripts, is released as open-source software under the PWM Noncommercial Share-Alike License v1.0 at https://github.com/integritynoble/Physics_World_Model. The codebase is organized into two Python packages: `pwm_core` (core framework, agents, graph compiler, calibration algorithms) and `pwm_AI_Scientist` (automated experiment generation and analysis).

Reconstruction data. All reconstruction arrays from every experiment—Scenarios I through IV for each modality and solver—are released as NumPy NPZ files. Files are stored using Git LFS and require `allow_pickle=True` for loading. Data ranges are standardized: CASSI and CACTI reconstructions are normalized to $[0, 1]$; SPC reconstructions are in $[0, 255]$.

Experiment manifests. Every experiment is recorded in a RunBundle v0.3.0 manifest containing: the git commit hash at execution time, all random number generator seeds, platform information (Python version, GPU model, CUDA version), SHA-256 hashes of all input data and output artifacts, metric values, and wall-clock timestamps. These manifests enable exact reproduction of every reported result.

Registry data. All 9 YAML registries (7,034 lines total) that drive the agent system—including modality definitions, graph templates, photon models, mismatch databases, compression tables, solver configurations, primitive specifications, dataset paths, and acceptance thresholds—are publicly available in the repository under `packages/pwm_core/contrib/`. The `ExperimentSpec` JSON schemas used for pipeline input validation are included alongside worked examples in `examples/`.

References

- [1] Chengshuai Yang. The finite primitive basis theorem for computational imaging: Formal foundations of the OperatorGraph representation, 2026. URL <https://arxiv.org/abs/2602.20550>.
- [2] Emmanuel J. Candès and Michael B. Wakin. An introduction to compressive sampling. *IEEE Signal Processing Magazine*, 25(2):21–30, 2008. doi: 10.1109/MSP.2007.914731.
- [3] David L. Donoho. Compressed sensing. *IEEE Transactions on Information Theory*, 52(4):1289–1306, 2006. doi: 10.1109/TIT.2006.871582.
- [4] Singanallur V. Venkatakrishnan, Charles A. Bouman, and Brendt Wohlberg. Plug-and-play priors for model based reconstruction. In *Proceedings of the IEEE Global Conference on Signal and Information Processing (GlobalSIP)*, pages 945–948, 2013. doi: 10.1109/GlobalSIP.2013.6737048.
- [5] Xin Yuan, Yang Liu, Jinli Suo, and Qionghai Dai. Plug-and-play algorithms for video snapshot compressive imaging. *IEEE Transactions on Pattern Analysis and Machine Intelligence*, 44(10):7093–7111, 2021.
- [6] Vishal Monga, Yuelong Li, and Yonina C. Eldar. Algorithm unrolling: Interpretable, efficient deep learning for signal and image processing. *IEEE Signal Processing Magazine*, 38(2):18–44, 2021. doi: 10.1109/MSP.2020.3016905.
- [7] Yuanhao Cai, Jing Lin, Xiaowan Hu, Haoqian Wang, Xin Yuan, Yulun Zhang, Radu Timofte, and Luc Van Gool. Mask-guided spectral-wise transformer for efficient hyperspectral image reconstruction. In *Proceedings of the IEEE/CVF Conference on Computer Vision and Pattern Recognition (CVPR)*, pages 17502–17511, 2022.
- [8] Xin Yuan, David J. Brady, and Aggelos K. Katsaggelos. Snapshot compressive imaging: Theory, algorithms, and applications. *IEEE Signal Processing Magazine*, 38(2):65–88, 2021.

- [9] Vegard Antun, Francesco Renna, Clarice Poon, Ben Adcock, and Anders C. Hansen. On instabilities of deep learning in image reconstruction and the potential costs of AI. *Proceedings of the National Academy of Sciences*, 117(48):30088–30098, 2020. doi: 10.1073/pnas.1907377117.
- [10] Martin Uecker, Peng Lai, Mark J. Murphy, Patrick Virtue, Michael Elad, John M. Pauly, Shreyas S. Vasanawala, and Michael Lustig. ESPIRiT — an eigenvalue approach to autocalibrating parallel MRI: where SENSE meets GRAPPA. *Magnetic Resonance in Medicine*, 71(3):990–1001, 2014. doi: 10.1002/mrm.24751.
- [11] Andrew M. Maiden and John M. Rodenburg. An improved ptychographical phase retrieval algorithm for diffractive imaging. *Ultramicroscopy*, 109(10):1256–1262, 2009. doi: 10.1016/j.ultramicro.2009.05.012.
- [12] Ashwin A. Wagadarikar, Renu John, Rebecca Willett, and David J. Brady. Single disperser design for coded aperture snapshot spectral imaging. *Applied Optics*, 47(10):B44–B51, 2008. doi: 10.1364/AO.47.000B44.
- [13] Patrick Llull, Xuejun Liao, Xin Yuan, Jianbo Yang, David Kittle, Lawrence Carin, Guillermo Sapiro, and David J. Brady. Coded aperture compressive temporal imaging. *Optics Express*, 21(9):10526–10545, 2013. doi: 10.1364/OE.21.010526.
- [14] Marco F. Duarte, Mark A. Davenport, Dharmpal Takhar, Jason N. Laska, Ting Sun, Kevin F. Kelly, and Richard G. Baraniuk. Single-pixel imaging via compressive sampling. *IEEE Signal Processing Magazine*, 25(2):83–91, 2008. doi: 10.1109/MSP.2007.914730.
- [15] L. A. Feldkamp, L. C. Davis, and J. W. Kress. Practical cone-beam algorithm. *Journal of the Optical Society of America A*, 1(6):612–619, 1984. doi: 10.1364/JOSAA.1.000612.
- [16] J. M. Rodenburg and H. M. L. Faulkner. A phase retrieval algorithm for shifting illumination. *Applied Physics Letters*, 85(20):4795–4797, 2004. doi: 10.1063/1.1823034.
- [17] Klaas P. Pruessmann, Markus Weiger, Markus B. Scheidegger, and Peter Boesiger. SENSE: Sensitivity encoding for fast MRI. *Magnetic Resonance in Medicine*, 42(5):952–962, 1999. doi: 10.1002/(SICI)1522-2594(199911)42:5<952::AID-MRM16>3.0.CO;2-S.
- [18] Michael Lustig, David Donoho, and John M. Pauly. Sparse MRI: The application of compressed sensing for rapid MR imaging. *Magnetic Resonance in Medicine*, 58(6):1182–1195, 2007. doi: 10.1002/mrm.21391.
- [19] David J. Brady. *Optical Imaging and Spectroscopy*. John Wiley & Sons, 2009.
- [20] Felix Bloch. Nuclear induction. *Physical Review*, 70(7–8):460–474, 1946. doi: 10.1103/PhysRev.70.460.
- [21] Chengshuai Yang. InverseNet: Benchmarking operator mismatch in snapshot compressive imaging. *arXiv preprint arXiv:2603.04538*, 2026.
- [22] Lishun Wang, Miao Cao, and Xin Yuan. EfficientSCI: Densely connected network with space-time factorization for large-scale video snapshot compressive imaging. In *Proceedings of the IEEE/CVF Conference on Computer Vision and Pattern Recognition (CVPR)*, pages 18477–18486, 2023.

- [23] Nick Antipa, Grace Kuo, Reinhard Heckel, Ben Mildenhall, Emrah Bostan, Ren Ng, and Laura Waller. DiffuserCam: lensless single-exposure 3D imaging. *Optica*, 5(1):1–9, 2018. doi: 10.1364/OPTICA.5.000001. DiffuserCam DLMD dataset: HuggingFace bezzam/DiffuserCam-Lensless-Mirflickr-Dataset.
- [24] David J. Brady, Kerkil Choi, Daniel L. Marks, Ryoichi Horisaki, and Sehoon Lim. Compressive holography. *Optics Express*, 17(15):13040–13049, 2009.
- [25] Johannes Leuschner, Maximilian Schmidt, Daniel Otero Baguer, and Peter Maaß. LoDoPaB-CT, a benchmark dataset for low-dose computed tomography reconstruction. *Scientific Data*, 8:109, 2021. doi: 10.1038/s41597-021-00893-z.
- [26] Keijo Hämäläinen, Lauri Harhanen, Andreas Hauptmann, Aki Kallonen, Esa Niemi, and Samuli Siltanen. Total variation regularization for large-scale X-ray tomography. *International Journal of Tomography and Simulation*, 28(1):1–25, 2015. FIPS walnut dataset: Zenodo 1254206.
- [27] Alexander Meaney, Andreas Hauptmann, and Samuli Siltanen. Helsinki tomography challenge 2022: description, methods, and results. *Applied Mathematics for Modern Challenges*, 1(1): 1–28, 2024. doi: 10.3934/ammc.2024001.
- [28] Hervé Liebgott, Alfonso Rodriguez-Molares, Françoise Cervenansky, Jørgen Arendt Jensen, and Olivier Bernard. Plane-wave imaging challenge in medical ultrasound. In *Proc. IEEE International Ultrasonics Symposium (IUS)*, pages 1–4, 2016. doi: 10.1109/ULTSYM.2016.7728908.
- [29] Saif Khan, Jaeyoung Huh, Manish Bhatt, Md. Murad Hossain, and Arun Bhatt. A deep learning framework for ultrasound image formation and image quality assessment. *IEEE Transactions on Ultrasonics, Ferroelectrics, and Frequency Control*, 70(9):972–984, 2023. DeepUS dataset: <https://zenodo.org/doi/10.5281/zenodo.7986407>.
- [30] Hanchen Wang, Tianfan Fu, Yuanqi Du, Wenhao Gao, Kexin Huang, Ziming Liu, Payal Chandak, Shengchao Liu, Peter Van Katwyk, Andreea Deac, et al. Scientific discovery in the age of artificial intelligence. *Nature*, 620:47–60, 2023.
- [31] David J. Brady, Michael E. Gehm, Ronald A. Stack, Daniel L. Marks, David S. Kittle, Dathon R. Golish, E. M. Vera, and Steven D. Feller. Multiscale gigapixel photography. *Nature*, 486(7403):386–389, 2012.
- [32] Yuan Xu, Ti Bai, Hao Yan, Luo Ouyang, Arnold Pompos, Jing Wang, Linghong Zhou, Steve B. Jiang, and Xun Jia. A practical cone-beam CT scatter correction method with optimized Monte Carlo simulations for image-guided radiation therapy. *Physics in Medicine and Biology*, 60(9): 3567–3587, 2015. doi: 10.1088/0031-9155/60/9/3567.
- [33] Xiao Liang, Liyuan Chen, Dan Nguyen, Zhiguo Zhou, Xuejun Gu, Ming Yang, Jing Wang, and Steve Jiang. Generating synthesized computed tomography (CT) from cone-beam computed tomography (CBCT) using CycleGAN for adaptive radiation therapy. *Physics in Medicine and Biology*, 64(12):125002, 2019. doi: 10.1088/1361-6560/ab22f9.
- [34] Chenyang Shen, Yesenia Gonzalez, Liyuan Chen, Steve B. Jiang, and Xun Jia. Intelligent parameter tuning in optimization-based iterative CT reconstruction via deep reinforcement learning. *IEEE Transactions on Medical Imaging*, 37(6):1430–1439, 2018. doi: 10.1109/TMI.2018.2823679.

- [35] Eric E. Klein, Joseph Hanley, John Bayouth, Fang-Fang Yin, William Simon, Sean Dresser, Christopher Serago, Francisco Aguirre, Lijun Ma, Bijan Arjomandy, Chihray Liu, Craig Sandin, and Timothy Holmes. Task Group 142 report: Quality assurance of medical accelerators. *Medical Physics*, 36(9):4197–4212, 2009.
- [36] Sasa Mutic, Jatinder R. Palta, Elizabeth K. Butker, Indra J. Das, M. Saiful Huq, Leh-Nien Dick Loo, Bill J. Salter, Cynthia H. McCollough, and Jacob Van Dyk. Quality assurance for computed-tomography simulators and the computed-tomography-simulation process: Report of the AAPM Radiation Therapy Committee Task Group No. 66. *Medical Physics*, 30(10):2762–2792, 2003.
- [37] Inchang Choi, Daniel S. Jeon, Giljoo Nam, Diego Gutierrez, and Min H. Kim. High-quality hyperspectral reconstruction using a spectral prior. *ACM Transactions on Graphics (Proceedings of SIGGRAPH Asia)*, 36(6):218:1–218:13, 2017. doi: 10.1145/3130800.3130810.
- [38] George Cybenko. Approximation by superpositions of a sigmoidal function. *Mathematics of Control, Signals and Systems*, 2(4):303–314, 1989.
- [39] Maziar Raissi, Paris Perdikaris, and George E. Karniadakis. Physics-informed neural networks: A deep learning framework for solving forward and inverse problems involving nonlinear partial differential equations. *Journal of Computational Physics*, 378:686–707, 2019.
- [40] Xiaowan Hu, Yuanhao Cai, Jing Lin, Haoqian Wang, Xin Yuan, Yulun Zhang, Radu Timofte, and Luc Van Gool. HDNet: High-resolution dual-domain learning for spectral compressive imaging. In *Proceedings of the IEEE/CVF Conference on Computer Vision and Pattern Recognition (CVPR)*, pages 17542–17551, 2022.
- [41] José M. Bioucas-Dias and Mário A. T. Figueiredo. A new TwIST: Two-step iterative shrinkage/thresholding algorithms for image restoration. *IEEE Transactions on Image Processing*, 16(12):2992–3004, 2007. doi: 10.1109/TIP.2007.909319.
- [42] Xin Yuan. Generalized alternating projection based total variation minimization for compressive sensing. In *Proceedings of the IEEE International Conference on Image Processing (ICIP)*, pages 2539–2543, 2016. doi: 10.1109/ICIP.2016.7532817.
- [43] Tao Huang, Weisheng Dong, Xin Yuan, Jinjian Wu, and Guangming Shi. Deep gaussian scale mixture prior for spectral compressive imaging. In *Proceedings of the IEEE/CVF Conference on Computer Vision and Pattern Recognition (CVPR)*, pages 16216–16225, 2021.
- [44] Yuanhao Cai, Jing Lin, Xiaowan Hu, Haoqian Wang, Xin Yuan, Yulun Zhang, Radu Timofte, and Luc Van Gool. CST: Compact spectral transformer for hyperspectral image reconstruction. In *Proceedings of the European Conference on Computer Vision (ECCV)*, 2022.
- [45] Yang Liu, Xin Yuan, Jinli Suo, David J. Brady, and Qionghai Dai. Rank minimization for snapshot compressive imaging. *IEEE Transactions on Pattern Analysis and Machine Intelligence*, 41(12):2990–3006, 2019.
- [46] Jure Zbontar, Florian Knoll, Anuroop Sriram, Tullie Murrell, Zhengnan Huang, Matthew J. Muckley, Aaron Defazio, Ruben Stern, Patricia Johnson, Mary Bruno, Marc Parente, Krzysztof J. Geras, Joe Katsnelson, Hersh Chandarana, Zizhao Zhang, Michal Drozdal, Adriana Romero, Michael Rabbat, Pascal Vincent, Nafissa Yakubova, James Pinkerton, Duo Wang, Erich Owens, C. Lawrence Zitnick, Michael P. Recht, Daniel K. Sodickson, and

Yvonne W. Lui. fastMRI: An open dataset and benchmarks for accelerated MRI. *arXiv preprint arXiv:1811.08839*, 2018.

Extended Data Table 1 | Primitive necessity ablation. For each of the 11 primitives, the witness modality whose representation error e_{img} exceeds $\varepsilon = 0.01$ when that primitive is removed from $\mathcal{B}$. Eight primitives (P , M , Π , F , Σ , D , R , Λ) are strictly necessary; the remaining three (C , S , W) are necessary under the stated complexity bounds ($N_{\text{max}} = 20$, $D_{\text{max}} = 10$). Data from¹, Proposition 1.

Removed primitive	Witness modality	Why irreplaceable	e_{img} without
Propagate P	Ptychography	Distance-dependent phase transfer	> 0.05
Modulate M	CASSI	Arbitrary element-wise mask	> 0.10
Project Π	CT	Line-integral (Radon) geometry	> 0.15
Encode F	MRI	Non-uniform Fourier sampling	> 0.20
Convolve C	Lensless imaging	Arbitrary shift-invariant PSF kernel	> 0.08
Accumulate Σ	SPC	Dimensional summation (not scaling)	> 0.12
Detect D	All modalities	Carrier-to-measurement conversion	> 0.50
Sample S	MRI	Index-set restriction (k -space)	> 0.10
Disperse W	CASSI	λ -parameterized spatial shift	> 0.06
Scatter R	Compton imaging	Direction change + energy shift	0.34
Transform Λ	Polychromatic CT	Non-terminal pointwise nonlinearity	> 0.05

Extended Data Table 2 | Oracle correction ceiling (Scenario III) across 14 validated configurations (12 modalities, 5 carrier families). Full table with per-scene metrics in Supplementary Table S1; autonomous correction recovery (Scenario IV) in Supplementary Table S9. Per-modality supplementary tables: ultrasound (S14), cryo-EM (S15), CBCT (S16), compressive holography (S17), fluorescence microscopy (S18), SPC (S19), lensless imaging (S20).

Supplementary Information

Eleven Primitives and Three Gates:
The Universal Structure of Computational Imaging

Chengshuai Yang, David J. Brady, and Xin Yuan

Supplementary Contents

S1 Supplementary Note 1: Triad Decomposition Mathematical Derivations	44
S1.1 Gate 1 — Information-Theoretic Limit (Compression)	44
S1.2 Gate 2 — SNR-Dependent PSNR Bound (Noise)	44
S1.3 Gate 3 — Sensitivity to Model Mismatch (Calibration)	45
S1.4 Recovery Ratio	45
S1.5 Conditions for Gate 3 Dominance	45
S2 Supplementary Note 2: Complete OperatorGraph Specification	47
S2.1 Node Interface	47
S2.2 Edge Semantics	47
S2.3 Compilation Algorithm	47
S2.4 JSON Serialization Schema	48
S3 Supplementary Table S1: All 19 Correction Configurations	49
S4 Supplementary Table S2: CASSI Per-Scene Results	51
S5 Supplementary Table S3: 12-Modality Validated Registry	53
S6 Supplementary Table S4: YAML Registry Summary	54
S7 Supplementary Note 4: RunBundle Schema	55
S7.1 RunBundle v0.3.0 Specification	55
S7.2 Integrity Verification	55
S8 Supplementary Note 5: Computational Cost Analysis	57
S8.1 Runtime per Modality	57
S8.2 RoIC Metric: Efficiency of Correction	57
S8.3 Scaling Considerations	58
S9 Supplementary Note 6: Real-Data Validation Details	59
S9.1 CASSI Real Data: TSA Hyperspectral Camera	59
S9.2 CACTI Real Data: Temporal Compressive Camera	59
S9.3 Autonomous Calibration on Real Data	61
S10 Supplementary Table S10: SSIM Comparison Across Modalities	62
S11 Supplementary Table S11: CASSI Spectral Angle Mapper (SAM)	62

S12	Supplementary Tables S12–S13: Gate 1 and Gate 2 Validation	63
S12.1	Gate 1: Information Deficiency (Extreme Compression)	63
S12.2	Gate 2: Carrier Budget (Noise Sweep)	64
S13	Supplementary Note 7: Clinical CT Quality Assurance Validation	66
S13.1	Gate Mapping to Clinical Failure Modes	66
S13.2	ACR Metric Validation	66
S13.3	Drift Detection Performance	66
S13.4	Workflow Efficiency	67
S13.5	Prospective Clinical Validation Protocol	67
S14	Supplementary Note 8: Controlled Hardware Validation	68
S14.1	CASSI Physical Mask Displacement Protocol	68
S14.2	Multi-Unit Variation Study Protocol	68
S15	Supplementary Note 9: Mismatch Parameter Derivation	69
S15.1	CASSI 5-Parameter Mismatch Model	69
S16	Supplementary Note 10: Calibration Method Comparison	70
S17	Supplementary Note 11: MRI Under Clinically Realistic Conditions	70
S18	Supplementary Note S14: Comparison with Existing Calibration Methods	71
S19	Supplementary Note 12: Finite Primitive Basis — Expanded Proof	73
S19.1	Formal Definitions	73
S19.2	Proof of Theorem 1	74
S19.3	Extension Protocol: Worked Example	75
S19.4	Minimality of the Primitive Basis	75
S19.5	Complexity Hierarchy	76
S20	Supplementary Note 15: Extended Real-Data Hardware Validation	77
S20.1	CASSI: Cross-Residual Monotonicity (TSA Real Data)	77
S20.2	CACTI: Self-Residual Masking (EfficientSCI Real Data)	77
S20.3	CT: Center-of-Rotation Mismatch (Public Sinograms)	78
S20.4	Electron Ptychography: Probe Position Jitter (4D STEM SrTiO ₃)	78
S20.5	MRI: Coil Sensitivity Mismatch (Multi-Coil Brain Data)	79
S21	Supplementary Note 16: Per-Scene Analysis and Bootstrap Confidence Intervals	79
S21.1	Per-Scene PSNR Scatter Plots	80
S21.2	Bootstrap Confidence Intervals for Recovery Ratio	80
S21.3	Effect Sizes	81
S22	Supplementary Table S14: Ultrasound Multi-Phantom Results	81
S23	Supplementary Table S15: Cryo-EM Multi-Phantom Results	81
S24	Supplementary Table S16: CT Multi-Phantom Detector Offset Results	81

S25	Supplementary Table S17: Compressive Holography Multi-Phantom Results	81
S26	Supplementary Table S18: Fluorescence Microscopy Multi-Phantom Results	81
S27	Supplementary Table S19: SPC Multi-Phantom Results	81
S28	Supplementary Table S20: Lensless Camera Multi-Phantom Results	81
S29	Supplementary Table S21: Lensless Camera Real-Image Validation	81
S30	Supplementary Note 17: Ultrasound Mismatch Analysis	81
	S30.1Speed-of-Sound Mismatch Model	81
	S30.2Real Data Sources	85
	S30.3Gate 3 Dominance	85
	S30.4Calibration Effectiveness	90
S31	Supplementary Note 18: Cryo-EM Mismatch Analysis	90
	S31.1CTF Defocus Mismatch Model	90
	S31.2Real Data Sources	90
	S31.3Gate 3 Dominance	90
	S31.4Comparison with CTFFIND	91
S32	Supplementary Note 19: CT Detector Offset Mismatch Analysis	91
	S32.1Detector Offset Mismatch Model	91
	S32.2Real Data Sources	91
	S32.3Gate 1 Interaction at Large Offsets	91
	S32.4Calibration Effectiveness	92
S33	Supplementary Note 20: Compressive Holography Mismatch Analysis	92
	S33.1Propagation Distance Mismatch Model	92
	S33.2Compressive Encoding and Gate 3	92
	S33.3Per-Plane Sensitivity	92
	S33.4Residual-Based Calibration	92
S34	Supplementary Note 21: Fluorescence Microscopy Mismatch Analysis	93
	S34.1Dual-PSF Mismatch Model	93
	S34.2Gate 3 Dominance	93
	S34.32D Calibration Grid	93
	S34.4Comparison with Blind Deconvolution	93
S35	Supplementary Note 22: SPC Illumination Mismatch Analysis	94
	S35.1Illumination Non-Uniformity Forward Model	94
	S35.2Gate 3 Dominance	94
	S35.3Flat-Field Calibration	94
S36	Supplementary Note 23: Lensless Camera PSF Mismatch Analysis	94
	S36.1Pinhole PSF Forward Model	94
	S36.2Gate 3 Dominance	95
	S36.3Calibration from Known Target	95
	S36.4Real-Image Corroboration (DiffuserCam DLMD)	95

S37	Supplementary Note 24: Particle-Beam Primitive Decomposition	95
S37.1	Neutron CT	96
S37.2	Proton CT	96
S37.3	Muon Tomography	96
S37.4	Summary	96

S1 Supplementary Note 1: Triad Decomposition Mathematical Derivations

The Triad Decomposition formalizes three successive gates that every computational-imaging reconstruction must pass. We derive rigorous bounds for each gate and show how the *recovery ratio* ρ summarizes the overall reconstruction quality.

S1.1 Gate 1 — Information-Theoretic Limit (Compression)

Let the forward operator $\mathbf{H} \in \mathbb{R}^{m \times n}$ map an n -dimensional scene $\mathbf{x}$ to m measurements $\mathbf{y}$. Define the *compression ratio* $\gamma = m/n$.

Theorem 3 (Compression bound). *For any estimator $\hat{\mathbf{x}}(\mathbf{y})$, the minimum achievable mean-squared error satisfies*

$$\text{MSE}_{\min} \geq \frac{1}{n} \sum_{i=1}^{n-m} \sigma_i^2(\mathbf{x}), \quad (\text{S1})$$

where $\sigma_i^2(\mathbf{x})$ denotes the variance of $\mathbf{x}$ along the i -th null-space direction of $\mathbf{H}$.

Interpretation. The null space of $\mathbf{H}$ has dimension $\dim \mathcal{N}(\mathbf{H}) = n - \text{rank}(\mathbf{H}) \geq n - m$. Information lost in the null space cannot be recovered without a prior; Gate 1 therefore sets an *information-theoretic floor* on PSNR:

$$\text{PSNR}_{\max}^{(G1)} = 10 \log_{10} \left(\frac{\|\mathbf{x}\|_{\infty}^2}{\text{MSE}_{\min}} \right). \quad (\text{S2})$$

Modalities with higher compression ratios (e.g. CACTI with B frames compressed into one) face a proportionally lower ceiling.

S1.2 Gate 2 — SNR-Dependent PSNR Bound (Noise)

Given additive noise $\mathbf{n} \sim \mathcal{N}(0, \sigma_n^2 \mathbf{I})$, the measurement SNR is $\text{SNR} = \|\mathbf{H}\mathbf{x}\|^2 / (m \sigma_n^2)$.

Theorem 4 (Noise bound). *Under matched forward model and Gaussian noise, the best achievable PSNR is*

$$\text{PSNR}_{\max}^{(G2)} = 10 \log_{10}(\text{SNR}) + C_{\mathcal{M}}, \quad (\text{S3})$$

where $C_{\mathcal{M}}$ is a modality-dependent constant that absorbs the conditioning of $\mathbf{H}$ and the prior strength:

$$C_{\mathcal{M}} = 10 \log_{10} \left(\frac{n \|\mathbf{x}\|_{\infty}^2}{\|\mathbf{x}\|^2} \cdot \kappa^{-2}(\mathbf{H}) \right), \quad (\text{S4})$$

with $\kappa(\mathbf{H})$ the condition number of $\mathbf{H}$ restricted to its column space.

Interpretation. Gate 2 is a *noise ceiling*: no algorithm can exceed $\text{PSNR}_{\max}^{(G2)}$ regardless of computational budget. Empirically, modalities such as MRI ($C_{\text{MRI}} \approx 8$ dB) are more noise-tolerant than CASSI ($C_{\text{CASSI}} \approx 3$ dB) due to favorable operator conditioning.

S1.3 Gate 3 — Sensitivity to Model Mismatch (Calibration)

Let $\boldsymbol{\theta} \in \mathbb{R}^p$ collect the calibration parameters (e.g. mask shift, PSF blur, coil sensitivity) and let $\mathbf{H}_{\boldsymbol{\theta}}$ denote the parameterized forward operator.

Theorem 5 (Calibration sensitivity). *For small perturbation $\delta\boldsymbol{\theta}$ around the true parameter $\boldsymbol{\theta}^*$, the PSNR degradation is*

$$\Delta\text{PSNR} \approx -\frac{10}{\ln 10} \frac{\delta\boldsymbol{\theta}^\top \mathbf{J}^\top \mathbf{J} \delta\boldsymbol{\theta}}{\text{MSE}_0}, \quad (\text{S5})$$

where $\mathbf{J} = \partial(\mathbf{H}_{\boldsymbol{\theta}}\mathbf{x})/\partial\boldsymbol{\theta}|_{\boldsymbol{\theta}^*}$ is the parameter Jacobian and MSE_0 is the noise-only MSE at $\boldsymbol{\theta}^*$.

Per-parameter sensitivity. Restricting to a single parameter θ_j :

$$\frac{d\text{PSNR}}{d\theta_j} = -\frac{10}{\ln 10} \frac{\|\mathbf{J}_{:,j}\|^2}{\text{MSE}_0} \delta\theta_j + \mathcal{O}(\delta\theta_j^2). \quad (\text{S6})$$

The first-order Taylor expansion shows that PSNR degrades linearly in $|\delta\theta_j|$ for small mismatches and quadratically for larger ones.

S1.4 Recovery Ratio

We define the *recovery ratio* as

$$\rho = \frac{\text{PSNR}_{\text{achieved}} - \text{PSNR}_{\text{mismatch}}}{\text{PSNR}_{\text{ideal}} - \text{PSNR}_{\text{mismatch}}}, \quad 0 \leq \rho \leq 1. \quad (\text{S7})$$

In rare cases where Scenario IV exceeds Scenario I (e.g., due to regularization benefits from the corrected operator), ρ may exceed 1.

Proposition 6. *Under convex reconstruction loss with matched regularization and convex constraint on $\boldsymbol{\theta}$, the recovery ratio satisfies $0 \leq \rho \leq 1$ for any estimator.*

Proof sketch. The oracle PSNR is the global optimum of the jointly convex problem in $(\mathbf{x}, \boldsymbol{\theta})$. The mismatch PSNR uses a fixed $\boldsymbol{\theta}_0 \neq \boldsymbol{\theta}^*$, yielding a suboptimal feasible point. Any correction step moves towards the optimum, so $\text{PSNR}_{\text{mismatch}} \leq \text{PSNR}_{\text{achieved}} \leq \text{PSNR}_{\text{oracle}}$, giving $\rho \in [0, 1]$. $\square$

Under the conditions of Proposition 1, $0 \leq \rho \leq 1$. In practice, beneficial regularization bias from the corrected operator can yield $\rho > 1$, as observed for CACTI.

S1.5 Conditions for Gate 3 Dominance

The empirical finding that Gate 3 is the residual bottleneck in well-designed instruments—where Gates 1 and 2 have been optimized at design time—admits a theoretical justification.

Proposition 7 (Gate 3 dominance condition). *For any instrument operating above its Gate 1 floor ($\gamma > \gamma_{\min}$, where $\gamma_{\min}$ is the minimum compression ratio for which $\text{PSNR}_{\max}^{(G1)}$ exceeds the target quality) and Gate 2 floor ($\text{SNR} > \text{SNR}_{\min}$, where $\text{SNR}_{\min}$ is the minimum carrier budget for which $\text{PSNR}_{\max}^{(G2)}$ exceeds the target quality), Gate 3 becomes the binding constraint whenever the calibration error exceeds the noise-equivalent resolution:*

$$\|\delta\boldsymbol{\theta}\|_{\mathbf{J}^\top \mathbf{J}} > \frac{\sigma_n}{\|\mathbf{x}\|_\infty} \cdot \kappa(\mathbf{H}), \quad (\text{S8})$$

where $\|\delta\boldsymbol{\theta}\|_{\mathbf{J}^\top \mathbf{J}} = \sqrt{\delta\boldsymbol{\theta}^\top \mathbf{J}^\top \mathbf{J} \delta\boldsymbol{\theta}}$ is the parameter-space mismatch norm weighted by the sensitivity Jacobian, σ_n is the noise standard deviation, and $\kappa(\mathbf{H})$ is the condition number of the forward operator.

Proof sketch. From Theorem 3 (Eq. S5), the mismatch-induced PSNR degradation is $\Delta\text{PSNR}_{\text{mismatch}} \approx (10/\ln 10) \cdot \|\delta\boldsymbol{\theta}\|_{\mathbf{J}^\top \mathbf{J}}^2 / \text{MSE}_0$. From Theorem 2 (Eq. S3), the noise-induced PSNR ceiling is $\text{PSNR}_{\text{max}}^{(G2)} = 10 \log_{10}(\text{SNR}) + C_{\mathcal{M}}$. Gate 3 dominates when $\Delta\text{PSNR}_{\text{mismatch}} > \Delta\text{PSNR}_{\text{noise}}$, which after substitution yields condition (S8). The condition is satisfied in modern instruments because: (i) well-designed systems operate with $\gamma \gg \gamma_{\min}$ and $\text{SNR} \gg \text{SNR}_{\min}$, pushing Gates 1 and 2 well above their floors; and (ii) the sensitivity Jacobian $\mathbf{J}$ amplifies even small parameter errors ($\|\delta\boldsymbol{\theta}\| \ll 1$) into substantial measurement discrepancies, because the forward operators of modern high-resolution instruments are highly sensitive to calibration parameters. $\square$

Interpretation. Proposition 2 formalizes the intuition that as instruments improve in information capacity (Gate 1) and signal quality (Gate 2), the binding constraint shifts to calibration fidelity (Gate 3). This is precisely the regime occupied by modern computational imaging systems, explaining why Gate 3 emerges as the residual bottleneck across all twelve validated modalities: these are well-designed instruments where Gates 1 and 2 operate well above their respective floors.

S2 Supplementary Note 2: Complete OperatorGraph Specification

The `OperatorGraph` is the central abstraction of the PWM framework. It represents a computational imaging pipeline as a directed acyclic graph (DAG) of differentiable operators.

S2.1 Node Interface

Every node v in the graph implements the following interface:

Method	Contract
<code>forward(x) → y</code>	Apply the physical forward model. Input shape: (B, C, *spatial). Output shape determined by the operator (e.g. compression changes spatial dims).
<code>adjoint(y) → x</code>	Apply the adjoint (transpose) operator. Must satisfy $\langle \mathbf{H}\mathbf{x}, \mathbf{y} \rangle = \langle \mathbf{x}, \mathbf{H}^\top \mathbf{y} \rangle$ to numerical precision ($< 10^{-6}$ relative error).
<code>shape_in / shape_out</code>	Static shape annotations for compile-time validation.
<code>dtype</code>	Data type contract: <code>float32</code> (default) or <code>complex64</code> .
<code>parameters() → dict</code>	Returns learnable calibration parameters with their current values.

S2.2 Edge Semantics

An edge $e = (u, v)$ represents data flow: the output tensor of node u is fed as input to node v . Edges carry the following metadata:

- **Tensor shape:** inferred at compile time via shape propagation.
- **Data type:** must match between source output and target input.
- **Optional transform:** lightweight reshape or permute operations (e.g. channel stacking for multi-frame CACTI data).

S2.3 Compilation Algorithm

Given an `OperatorGraph` $G = (V, E)$:

1. **Topological sort.** Compute a valid execution order $v_1, v_2, \dots, v_{|V|}$ using Kahn’s algorithm. Raise `CycleError` if the graph contains a cycle.
2. **Shape propagation.** Starting from the source node(s), propagate tensor shapes through each operator’s `shape_out` to validate all edge contracts.

3. **Automatic adjoint chain.** Construct the adjoint graph $G^\top$ by reversing all edges and replacing each node's `forward` with `adjoint`. The adjoint graph is used for gradient-based reconstruction and the Triad Decomposition sensitivity analysis.
4. **Fusion (optional).** Consecutive linear operators are fused into a single matrix–vector product when dimensions permit, reducing memory traffic.

S2.4 JSON Serialization Schema

The graph is serialized to a JSON document for reproducibility and sharing:

```
{
  "version": "0.3.0",
  "nodes": [
    {
      "id": "mask",
      "type": "CassiMask",
      "params": {"shift_r": 0.0, "shift_c": 0.0},
      "shape_in": [1, 28, 256, 256],
      "shape_out": [1, 1, 256, 310]
    }
  ],
  "edges": [
    {"src": "mask", "dst": "detector", "dtype": "float32"}
  ],
  "metadata": {
    "modality": "CASSI",
    "created": "2026-02-01T00:00:00Z"
  }
}
```

S3 Supplementary Table S1: All 19 Correction Configurations

Table S1 reports the correction results for all 19 correction configurations across the validated modalities. The first 9 configurations have full end-to-end validation from Phase 1; the next 5 have multi-phantom validation with bootstrap confidence intervals from Phase 2 (14 validated total, spanning 12 modalities across 5 carrier families); the remaining 5 are designated Phase 3/4 additions with planned validation.

Table S1: Oracle correction ceiling summary. Δ PSNR is the improvement from Scenario II (mismatch) to Scenario III (oracle: true operator applied to mismatched data). For modalities with low-dimensional mismatch (Matrix, CT, Lensless imaging, MRI, Electron ptychography), autonomous correction achieves near-oracle performance (Sc. IV $\approx$ Sc. III); for CASSI and CACTI with multi-parameter mismatch, the gap between Sc. IV and Sc. III is reported in Table S9. CASSI correction results use GAP-TV as the reconstruction solver. Scenario I (ideal) PSNR values are available in the RunBundle manifests in the code repository.

Modality	Mismatch Parameter	Sc. II (dB)	Sc. III (dB)	Δ PSNR (dB)	RMSE
Matrix ¹	gain_bias	11.14	23.35	+12.21	0.0042
CT	center_of_rotation	13.41	24.09	+10.68	0.0031
CACTI ²	8-param mismatch	15.81	26.01	+10.21	—
Lensless imaging	psf_shift	23.48	27.03	+3.55	0.0089
MRI ³	coil_sensitivities	40.91	52.11	+11.20	0.0017
SPC ⁴	gain_drift	18.51	26.21	+7.71	—
CASSI (Alg 1) ⁵	mask_geo + dispersion	20.96	21.50	+0.54	0.0105
CASSI (Alg 2) ⁶	mask_geo + dispersion	20.96	21.72	+0.76	0.0098
Ptychography	position_offset	17.35	24.44	+7.09	0.0063
<i>Phase 2 validated additions (multi-phantom aggregate $\pm$ 95% CI)</i>					

Continued on next page

¹Matrix (Generic) is a canonical test configuration that uses the same gain-bias operator template as SPC; identical results confirm pipeline consistency rather than representing an independent modality.

²CACTI uses GAP-TV as the reconstruction solver for Table S1 consistency. Oracle values from InverseNet validation under 8-parameter mismatch ($dx=0.5$ px, $dy=0.3$ px, $\theta=0.1^\circ$, $\Delta t=0.05$, $\eta=0.95$, $g=1.02$, $\sigma=0.002$, $\sigma_n=1.0$). State-of-the-art EfficientSCI achieves Sc. II = 14.81 dB and Sc. III = 27.38 dB; see main text.

³Multi-coil clinically realistic scenario (8 coils, $4\times$ acceleration, 5% Biot-Savart sensitivity error). A single-coil pathological stress-test yields +48.25 dB; see Supplementary Note 11.

⁴SPC uses FISTA-TV as the reconstruction solver for Table S1 consistency. Values from InverseNet validation under exponential gain drift ($\alpha=0.0015$). HATNet achieves Sc. II = 19.40 dB and Sc. III = 29.78 dB; see main text.

⁵Reported values are averaged over 10 test scenes using GAP-TV as the reconstruction solver. Sc. II from InverseNet validation; Sc. III values are oracle upper bounds (true operator applied to mismatched data). Autonomous correction achieves 85% of oracle (Table S9).

⁶The correction-table PSNR reflects GAP-TV reconstruction; state-of-the-art solvers (e.g., MST-L) achieve 27.33 dB under Sc. III (see main text and Table S2).

Modality	Mismatch Parameter	Sc. II (dB)	Sc. III (dB)	Δ PSNR (dB)	RMSE
Fluorescence ⁷	PSF_sigma (dual)	21.65	30.00	+8.35	0.50 px
Ultrasound ⁸	speed_of_sound	24.91	38.85	+13.94	2 m/s
Cryo-EM ⁹	defocus	18.54	20.88	+2.34	20–31 nm
CT (offset) ¹⁰	detector_offset	9.08	10.70	+1.62	1 px
Comp. Hologra- phy ¹¹	propagation_distance	0.43	11.46	+1.03	9 μ m
SPC ¹²	illum_sigma	14.40	15.46	+1.06	0.2 px
Lensless imaging ¹³	psf_sigma	18.90	25.92	+7.02	0.1 px
<i>Phase 3/4 additions — validation planned</i>					
Holography	propagation_distance	—	—	—	—
FPM	LED_positions	—	—	—	—
Phase Retrieval	support_constraint	—	—	—	—
OCT	dispersion_coeffs	—	—	—	—
Radar/SAR	motion_compensation	—	—	—	—

⁷ $N=5$ phantoms (puncta, filaments, nuclei, membranes, mixed). PSF sigma error $\Delta\sigma=1.0$ px (worst case). 9×9 grid-search calibration over $(\sigma_{\text{ex}}, \sigma_{\text{em}})$.

⁸ $N=5$ real datasets (4 PICMUS experimental + 1 DeepUS CIRS040GSE). SoS error $\Delta c=200$ m/s. 51-step grid-search over $c \in [1400, 1700]$ m/s; 75-angle compound PW-DAS with Hilbert-envelope detection. Self-reference metrics (Sc. I = pseudo-GT); Sc. II and Sc. IV are PSNR vs. nominal-SoS reconstruction. Calibrated $c_{\text{cal}}=1538$ m/s within 2 m/s of nominal for all 5 datasets.

⁹ $N=5$ real EMDB structures (TRPV1, β -gal, T20S, apoferritin, SARS-CoV-2 spike). Defocus error $\Delta(\Delta f)=1000$ nm (worst case). 50-step grid-search over $\Delta f \in [-3000, -500]$ nm (grid spacing ≈ 51 nm). $\rho=0.99$ at $\Delta(\Delta f)=1000$ nm.

¹⁰ $N=5$ real images (3 LoDoPaB-CT patient slices, FIPS walnut, HTC 2022). Detector offset $\Delta s=10$ px. 51-step calibration in $[-25, 25]$ px. Sc. I on clean sinogram; Sc. III capped at Sc. I.

¹¹ $N=4$ phantoms (USAF chart, bio cells, particles, sparse dots). Propagation error $\Delta z=400 \mu\text{m}$ (worst case). 21-step calibration via hologram residual minimisation. Sc. III capped at Sc. I.

¹² $N=5$ phantoms (32×32 ; puncta, filaments, nuclei, membranes, mixed). Illumination vignetting error $\Delta\sigma_{\text{IG}}=20$ px (worst case of 4 levels; true $\sigma_{\text{IG}}=10$ px). Flat-field calibration via maximum-likelihood MLE. Calibrated $\sigma_{\text{IG}}=10.2$ px; recovery $\rho=0.97$.

¹³ $N=5$ phantoms (64×64 ; puncta, filaments, nuclei, membranes, mixed). PSF sigma error $\Delta\sigma=3.0$ px (worst case; true $\sigma=3.0$ px). Calibration: forward-model fit on known checkerboard target. Calibrated $\sigma=3.12$ px; recovery $\rho=1.00$.

S4 Supplementary Table S2: CASSI Per-Scene Results

Table S2 reports PSNR (dB) and recovery ratio ρ (%) for 10 KAIST scenes across four methods under three scenarios, matching the InverseNet benchmark²¹.

Table S2: CASSI per-scene PSNR (dB) and oracle recovery ratio ρ_{III} . Sc. I = ideal forward model; Sc. II = mismatched (baseline); Sc. III = oracle correction (true operator applied to mismatched data). All values from InverseNet validation under the 5-parameter mismatch ($dx=0.5$ px, $dy=0.3$ px, $\theta=0.1^\circ$, $a_1=2.02$, $\alpha=0.15^\circ$). $\rho_{\text{III}} = (\text{Sc. III} - \text{Sc. II}) / (\text{Sc. I} - \text{Sc. II})$ is the oracle recovery ceiling. HDNet shows $\rho_{\text{III}}=0\%$ across all scenes due to its mask-oblivious architecture.

Scene	Method	Sc. I	Sc. II	Sc. III	ρ_{III}
scene01	GAP-TV	26.49	24.08	24.18	4.1%
scene01	PnP-HSICNN	27.43	23.47	25.78	58.3%
scene01	HDNet	34.95	24.37	24.37	0.0%
scene01	MST-L	35.29	23.96	29.98	53.2%
scene02	GAP-TV	24.60	21.89	22.82	34.5%
scene02	PnP-HSICNN	25.34	21.56	23.80	59.3%
scene02	HDNet	35.65	23.26	23.26	0.0%
scene02	MST-L	36.14	22.21	28.42	44.6%
scene03	GAP-TV	25.96	18.62	19.68	14.4%
scene03	PnP-HSICNN	26.71	17.59	21.83	46.5%
scene03	HDNet	35.54	18.61	18.61	0.0%
scene03	MST-L	35.66	16.09	23.57	38.2%
scene04	GAP-TV	28.36	23.37	24.41	20.9%
scene04	PnP-HSICNN	28.80	22.89	25.98	52.3%
scene04	HDNet	41.63	23.98	23.98	0.0%
scene04	MST-L	40.05	21.91	29.80	43.5%
scene05	GAP-TV	23.66	20.39	21.27	26.9%
scene05	PnP-HSICNN	24.65	19.36	22.75	64.3%
scene05	HDNet	32.56	20.22	20.22	0.0%
scene05	MST-L	32.84	20.28	26.75	51.5%
scene06	GAP-TV	22.34	20.39	21.00	31.2%
scene06	PnP-HSICNN	23.12	20.29	21.80	53.0%
scene06	HDNet	34.33	22.63	22.63	0.0%
scene06	MST-L	34.56	22.37	28.67	51.7%
scene07	GAP-TV	23.51	20.56	21.07	17.4%
scene07	PnP-HSICNN	24.94	19.86	22.77	57.4%
scene07	HDNet	33.27	20.79	20.79	0.0%
scene07	MST-L	33.80	19.76	26.12	45.3%
scene08	GAP-TV	22.16	20.57	21.10	33.3%
scene08	PnP-HSICNN	22.73	20.30	21.92	66.4%
scene08	HDNet	32.26	22.73	22.73	0.0%
scene08	MST-L	32.74	21.33	27.44	53.5%
scene09	GAP-TV	23.03	19.14	20.61	37.8%
scene09	PnP-HSICNN	24.03	18.79	21.82	57.8%
scene09	HDNet	34.18	21.18	21.18	0.0%
scene09	MST-L	34.37	19.75	26.71	47.6%
scene10	GAP-TV	23.27	20.58	21.04	16.9%
scene10	PnP-HSICNN	23.47	19.90	22.38	69.4%
scene10	HDNet	32.22	21.06	21.06	0.0%

Scene	Method	Sc. I	Sc. II	Sc. III	ρ_{III}
scene10	MST-L	32.63	20.69	25.86	43.3%
Mean	GAP-TV	24.34	20.96	21.72	22.5%
Mean	PnP-HSICNN	25.12	20.40	23.08	56.8%
Mean	HDNet	34.66	21.88	21.88	0.0%
Mean	MST-L	34.81	20.83	27.33	46.5%

S5 Supplementary Table S3: 12-Modality Validated Registry

Table S3 lists the 12 fully validated modalities (Scenarios I–IV) in the PWM benchmark, grouped by physical carrier tier.

Table S3: 12-modality validated registry. PSNR values are Scenario I results with the default solver. “Ref. PSNR” is the best published result where available. All 12 modalities have full Scenarios I–IV correction validated.

#	Modality	Domain	PSNR (dB)	Ref. PSNR (dB)	Status	Solver
1	CASSI	Optical (inc.)	24.34	34.2	Validated	GAP-TV
2	CACTI	Optical (inc.)	35.39	33.4	Validated	EfficientSCI
3	SPC	Optical (inc.)	28.06	31.0	Validated	FISTA-TV
4	Lensless imaging	Optical (inc.)	27.03	28.5	Validated	Richardson–Lucy
5	Fluorescence	Optical (inc.)	30.63	30.1	Validated	Richardson–Lucy
6	Comp. Holography	Optical (coh.)	7.67	32.7	Validated	FISTA-TV
7	CT	X-ray	24.09	42.1	Validated	FBP + TV
8	CBCT	X-ray	13.79	39.5	Validated	FBP
9	Ptychography	Electron	24.44	26.8	Validated	ePIE
10	Cryo-EM	Electron	16.42	25.9	Validated	Wiener
11	MRI ¹⁴	Nuclear spin	52.11	42.3	Validated	CG-SENSE
12	Ultrasound	Acoustic	18.68	31.8	Validated	Compound PW-DAS

¹⁴Multi-coil Scenario I PSNR (8 coils, 4× acceleration); see Supplementary Note 10 for full multi-coil analysis.

S6 Supplementary Table S4: YAML Registry Summary

Table S4 summarizes the nine YAML registry files (totalling 7,034 lines) that define the PWM framework’s modular architecture.

Table S4: YAML registry files in `packages/pwm_core/contrib/`.

#	File	Lines	Purpose
1	<code>modalities.yaml</code>	3800	Defines 170 modality entries across 23 categories with keywords, forward model equations, and default solvers.
2	<code>graph_templates.yaml</code>	4200	OperatorGraph skeletons for 170 modality templates (37 unique DAG patterns).
3	<code>photon_db.yaml</code>	624	Photon models parameterized by source power, quantum efficiency, exposure, and detector.
4	<code>mismatch_db.yaml</code>	797	Mismatch parameters, perturbation ranges, and correction methods per modality.
5	<code>compression_db.yaml</code>	1186	Recoverability tables mapping compression ratio to expected PSNR with provenance.
6	<code>solver_registry.yaml</code>	650	Maps solver names to implementations (ADMM [?] , FISTA [?] , GAP-TV, PnP, learned).
7	<code>primitives.yaml</code>	450	Primitive operator metadata (type, adjoint availability, differentiability).
8	<code>dataset_registry.yaml</code>	380	Links modalities to benchmark datasets (KAIST, fastMRI, etc.).
9	<code>acceptance_thresholds.yaml</code>	347	Pass/fail thresholds per metric for automated validation.

S7 Supplementary Note 4: RunBundle Schema

The `RunBundle` is PWM’s reproducibility artifact. Every experiment produces a `RunBundle` that captures the complete computational state.

S7.1 RunBundle v0.3.0 Specification

Table S5: RunBundle v0.3.0 field specification.

Field	Type	Description
<code>version</code>	string	Schema version, currently "0.3.0".
<code>git_hash</code>	string	Full 40-character SHA-1 of the commit used to generate results.
<code>rng_seeds</code>	object	Random seeds for Python (<code>random</code> , <code>numpy</code>), PyTorch (CPU, CUDA), and any solver-specific RNG.
<code>platform_info</code>	object	OS, Python version, GPU model, CUDA version, PyTorch version, and <code>pip freeze</code> hash.
<code>sha256_hashes</code>	object	SHA-256 checksums of all input data files (measurements, masks, ground truth).
<code>metrics</code>	object	Computed quality metrics: PSNR, SSIM, LPIPS, and any modality-specific metrics.
<code>timestamps</code>	object	ISO-8601 timestamps for start, end, and per-stage completion.
<code>operator_state</code>	object	Serialized <code>OperatorGraph</code> including all node parameters and edge metadata.
<code>triad_report</code>	object	Triad Decomposition evaluation: gate pass/fail status, PSNR bounds, and recovery ratio ρ .
<code>correction_trajectory</code>	array	Time series of correction iterations: <code>[{iter, params, loss, psnr, grad_norm}, ...]</code> . Enables convergence analysis and early-stopping diagnostics.
<code>solver_config</code>	object	Complete solver hyperparameters (algorithm, iterations, step size, regularization weight, denoiser checkpoint).
<code>modality</code>	string	Modality identifier matching <code>modalities.yaml</code> .
<code>scenario</code>	string	One of I (ideal), II (mismatch), III (corrected), IV (oracle_mask).
<code>notes</code>	string	Free-form text field for experiment annotations.

S7.2 Integrity Verification

A `RunBundle` can be verified by:

1. Checking `git_hash` matches the repository state.
2. Re-computing `sha256_hashes` from the data files.
3. Re-running the solver with the stored `rng_seeds` and `solver_config` and comparing metrics within tolerance (± 0.01 dB PSNR).

S8 Supplementary Note 5: Computational Cost Analysis

S8.1 Runtime per Modality

All timings were measured on a single NVIDIA RTX 4090 GPU (24 GB VRAM) with PyTorch 2.1 and CUDA 12.1.

Table S6: Computational cost for correction (Scenario II $\rightarrow$ IV). RoIC = dB recovered per GPU-hour.

Modality	Carrier	Iterations	Runtime (s)	Δ PSNR (dB)	RoIC (dB/GPU-hr)
<i>Optical photon — incoherent</i>					
CASSI (Alg 1)	Optical (inc.)	500	300	+0.54	6.5
CASSI (Alg 2)	Optical (inc.)	2000	3200	+0.76	0.9
CACTI	Optical (inc.)	1000	180	+10.21	204.2
SPC	Optical (inc.)	200	15	+7.71	1850.4
Lensless imaging	Optical (inc.)	300	45	+3.55	284.0
Fluorescence	Optical (inc.)	300	45	+2.60	208.0
<i>Optical photon — coherent</i>					
Comp. Holography	Optical (coh.)	200	60	+0.80	48.0
<i>X-ray photon</i>					
CT	X-ray	500	85	+10.68	452.3
CBCT	X-ray	500	100	+1.50	54.0
<i>Electron</i>					
Ptychography	Electron	800	420	+7.09	60.8
Cryo-EM	Electron	400	120	+2.40	72.0
<i>Nuclear spin</i>					
MRI	Nuclear spin	150	30	+11.20	1344.0
<i>Acoustic</i>					
Ultrasound	Acoustic	300	90	+8.20	328.0

S8.2 RoIC Metric: Efficiency of Correction

We define the *Return on Invested Compute* (RoIC) as:

$$\text{RoIC} = \frac{\Delta\text{PSNR (dB)}}{T_{\text{GPU (hours)}}}, \quad (\text{S9})$$

where T_{GPU} is the wall-clock GPU time.

Key observations:

- **Matrix/SPC** achieve the highest RoIC (3663 and 1850 dB/GPU-hr respectively) due to the simplicity of the gain-bias correction model.
- **MRI** achieves the third-highest RoIC (1344 dB/GPU-hr) because coil sensitivity correction yields substantial PSNR gains (+11.20 dB under clinically realistic 8-coil, 4 $\times$ acceleration) with a well-conditioned linear operator that converges rapidly.

- **CASSI Algorithm 2** has the lowest RoIC (0.9 dB/GPU-hr) because it jointly optimizes mask geometry and dispersion over 2000 iterations, each requiring a full forward–adjoint cycle through the dispersive operator. Under the multi-parameter InverseNet mismatch, the absolute correction gains are modest (+0.76 dB), reflecting the inherent difficulty of simultaneously correcting five coupled mismatch parameters.
- The practical implication is that Algorithm 1 (fixed dispersion, correct mask geometry only) is preferred when compute budget is limited, recovering 71% of Algorithm 2’s Δ PSNR at <10% of the cost.

S8.3 Scaling Considerations

For large-scale deployment:

- Correction is *embarrassingly parallel* across scenes/slices — multi-GPU scaling is near-linear.
- The OperatorGraph compilation overhead is amortized: once compiled, the same graph serves all scenes of a given modality.
- Memory footprint scales with the measurement dimension m , not the scene dimension n , making correction feasible even for high-resolution 3D volumes (e.g. 512^3 CT).

S9 Supplementary Note 6: Real-Data Validation Details

S9.1 CASSI Real Data: TSA Hyperspectral Camera

The TSA (Thermal Snapshot Aperture) real dataset consists of 5 hyperspectral scenes acquired with a coded aperture snapshot spectral imaging system. Each scene has spatial resolution 660×660 with 28 spectral bands (450–650 nm) and a mask-shift step of 2 pixels per band. The extended measurement has width $660 + (28 - 1) \times 2 = 714$ pixels.

Experimental protocol. For each scene, we reconstruct with four methods: GAP-TV (classical iterative), HDNet (mask-oblivious neural network), MST-S, and MST-L (mask-guided spectral transformers). Each method is applied under two conditions: (i) the calibrated mask provided with the dataset, and (ii) a perturbed mask with sub-pixel shift $dx = 0.5$ px, $dy = 0.3$ px. Because the MST model has a hardcoded 256×256 spatial assumption, the 660×660 real data is center-cropped to 256×256 for MST reconstruction. HDNet is fully convolutional and processes the full spatial extent.

Metric. Because no ground-truth hyperspectral cube exists for the real scenes, we use the measurement residual as a ground-truth-free diagnostic:

$$r = \frac{\|\mathbf{y} - H\hat{\mathbf{x}}\|^2}{\|\mathbf{y}\|^2}, \quad (\text{S10})$$

where $\mathbf{y}$ is the measured snapshot and $\hat{\mathbf{x}}$ is the reconstruction. The residual ratio $r_{\text{mismatch}}/r_{\text{calibrated}}$ quantifies the relative impact of operator mismatch, independent of the (unknown) ground truth.

Key findings. GAP-TV, which explicitly conditions on the coded aperture mask in its forward–adjoint iterations, shows the expected sensitivity to mask mismatch (mean ratio $1.8\times$). HDNet, whose architecture processes the measurement without explicit mask conditioning, is entirely insensitive (ratio $1.0\times$). The transformer methods (MST-S, MST-L) show ratios near or below $1.0\times$ on real data—in sharp contrast to their severe degradation in simulation (-13.98 dB for MST-L). This simulation-to-hardware gap indicates that the real hardware mask already contains uncorrected manufacturing imperfections, so the additional 0.5 px perturbation is small relative to pre-existing errors.

S9.2 CACTI Real Data: Temporal Compressive Camera

The CACTI real dataset consists of 4 dynamic scenes (duomino, hand, pendulumBall, waterBallon) acquired with a coded aperture compressive temporal imaging system at 512×512 spatial resolution with compression ratio 10 (10 video frames encoded per snapshot).

Key findings. GAP-TV shows an order-of-magnitude residual increase ($10.4\times$ mean) under sub-pixel mask mismatch, consistent with the multiplicative error amplification in temporal compression (a single mask error propagates across all 10 compressed frames). PnP-FFDNet shows moderate robustness ($2.0\times$), likely because the FFDNet denoiser provides an implicit regularization that partially absorbs the mismatch artefacts. The CACTI results confirm that temporal compressive modalities are substantially more sensitive to operator mismatch than spectral compressive modalities (CASSI), a distinction that would be invisible without the unified TRIAD DECOMPOSITION framework.

Table S7: CASSI real-data measurement residuals. Residual values r (Eq. S10) and residual ratio (mismatched/calibrated) across 5 TSA scenes and 4 methods.

Scene	Method	r_{cal}	r_{mis}	Ratio
Scene 1	GAP-TV	0.00148	0.00298	2.0
Scene 1	HDNet	0.18506	0.18506	1.0
Scene 1	MST-S	0.09953	0.10746	1.1
Scene 1	MST-L	0.10055	0.09544	0.9
Scene 2	GAP-TV	0.00210	0.00331	1.6
Scene 2	HDNet	0.14853	0.14853	1.0
Scene 2	MST-S	0.25357	0.23807	0.9
Scene 2	MST-L	0.25441	0.22811	0.9
Scene 3	GAP-TV	0.00204	0.00320	1.6
Scene 3	HDNet	0.18291	0.18291	1.0
Scene 3	MST-S	0.09399	0.09160	1.0
Scene 3	MST-L	0.10127	0.09085	0.9
Scene 4	GAP-TV	0.00148	0.00297	2.0
Scene 4	HDNet	0.14355	0.14355	1.0
Scene 4	MST-S	0.15586	0.14712	0.9
Scene 4	MST-L	0.17899	0.15893	0.9
Scene 5	GAP-TV	0.00233	0.00421	1.8
Scene 5	HDNet	0.11325	0.11325	1.0
Scene 5	MST-S	0.11995	0.12004	1.0
Scene 5	MST-L	0.13008	0.12208	0.9
Mean	GAP-TV	0.00189	0.00333	1.8
Mean	HDNet	0.15466	0.15466	1.0
Mean	MST-S	0.14458	0.14086	1.0
Mean	MST-L	0.15306	0.13908	0.9

Table S8: CACTI real-data measurement residuals and total variation. Residual ratio (mismatched/calibrated) and total variation (TV) for 4 real scenes and 2 methods.

Scene	Method	r_{cal}	r_{mis}	Ratio
duomino	GAP-TV	8.0×10^{-6}	8.5×10^{-5}	10.6
duomino	PnP-FFDNet	0.00198	0.00403	2.0
hand	GAP-TV	7.0×10^{-6}	7.7×10^{-5}	11.0
hand	PnP-FFDNet	0.00249	0.00705	2.8
pendulumBall	GAP-TV	3.7×10^{-5}	3.46×10^{-4}	9.4
pendulumBall	PnP-FFDNet	0.00919	0.01150	1.3
waterBalloon	GAP-TV	1.4×10^{-5}	1.47×10^{-4}	10.5
waterBalloon	PnP-FFDNet	0.00264	0.00493	1.9
Mean	GAP-TV	—	—	10.4
Mean	PnP-FFDNet	—	—	2.0

Table S9: Grid-search calibration results on simulated data with known ground truth. PSNR values in dB. Sc. II = mismatch (no calibration); Sc. III = oracle (true operator on mismatched data); Sc. IV = PWM grid-search corrected. Recovery = (Sc. IV – Sc. II) / (Sc. III – Sc. II). CASSI/CACTI use measurement-residual objective; SPC uses reconstruction-TV objective. Note: Sc. II values here differ from Table S1 because Table S1 reports the full InverseNet multi-parameter mismatch, whereas this table uses simplified single-parameter mismatch for grid-search tractability.

Modality	Method	Sc. II	Sc. III	Sc. IV	Time (s)	Recovery
CASSI	GAP-TV	21.52	23.21	22.96	1140	85%
CACTI	GAP-TV	17.60	26.99	26.99	60	100%
SPC	FISTA-TV	19.78	27.60	26.54	166	86%
SPC	PnP-DRUNet	18.34	26.01	25.39	247	92%

S9.3 Autonomous Calibration on Real Data

CACTI achieves perfect calibration recovery because the mismatch manifold is low-dimensional (2D spatial shift) and the temporal compression provides high sensitivity to mask position. CASSI achieves 85% recovery; the residual gap reflects the higher-dimensional mismatch space (mask geometry plus dispersion) and the estimation error in both dx and dy (0.10 px each). For SPC, the measurement residual is uninformative for gain drift because the underdetermined system ($m=272$ measurements for $n=1089$ unknowns) always achieves near-zero self-consistent residual regardless of gain. Instead, reconstruction total variation provides a viable objective: the correctly calibrated gain produces clean measurements yielding smooth reconstructions with low TV, while incorrect gain leaves systematic artifacts that increase TV. The TV surface exhibits a clear bowl-shaped minimum near the true α , recovering 86% (FISTA-TV) to 92% (PnP-DRUNet) of the oracle bound. This demonstrates that blind calibration generalises to radiometric mismatch provided the objective matches the mismatch type: measurement residual for geometric mismatch, reconstruction sparsity for radiometric mismatch.

S10 Supplementary Table S10: SSIM Comparison Across Modalities

Table S10 reports the structural similarity index (SSIM) for all three validated photon-domain modalities under the three primary scenarios. SSIM complements PSNR by capturing perceptual quality, particularly structural distortions from operator mismatch.

Table S10: SSIM comparison across modalities and scenarios. Sc. III = oracle (true operator on mismatched data). Values are mean $\pm$ s.d. across test scenes/images.

Modality	Method	Sc. I	Sc. II	Sc. III
<i>CASSI (10 KAIST scenes, 28 spectral bands)</i>				
	GAP-TV	0.723 ± 0.088	0.612 ± 0.084	0.688 ± 0.083
	HDNet	0.970 ± 0.009	0.756 ± 0.074	0.756 ± 0.074
	MST-L	0.973 ± 0.009	0.744 ± 0.069	0.881 ± 0.035
<i>CACTI (6 benchmark videos, 8 temporal frames)</i>				
	GAP-TV	0.848 ± 0.083	0.305 ± 0.070	0.794 ± 0.063
	PnP-FFDNet	0.890 ± 0.060	0.216 ± 0.076	0.820 ± 0.054
	ELP-Unfolding	0.965 ± 0.013	0.308 ± 0.076	0.927 ± 0.017
	EfficientSCI	0.973 ± 0.012	0.303 ± 0.079	0.927 ± 0.017
<i>SPC (11 standard images, 25% compression)</i>				
	FISTA-TV	0.852 ± 0.046	0.586 ± 0.055	0.759 ± 0.036
	PnP-DRUNet	0.899 ± 0.026	0.415 ± 0.066	0.666 ± 0.055
	ISTA-Net	0.916 ± 0.028	0.584 ± 0.077	0.760 ± 0.056
	HATNet	0.847 ± 0.049	0.648 ± 0.091	0.807 ± 0.060

Key observations. The SSIM degradation pattern mirrors the PSNR findings: under Scenario II (mismatch), all methods collapse to a narrow quality range regardless of their Scenario I performance. In CASSI, the SSIM collapse is particularly striking: MST-L drops from 0.973 to 0.744, a perceptual quality loss that exceeds the improvement from a decade of solver development. In CACTI, mismatch produces near-random SSIM values (~ 0.3), confirming that the reconstructed video frames bear little structural resemblance to the ground truth under mismatch conditions.

S11 Supplementary Table S11: CASSI Spectral Angle Mapper (SAM)

Table S11 reports the spectral angle mapper (SAM, in degrees) for CASSI, which measures spectral fidelity independently of intensity. Lower values indicate better spectral reconstruction.

Key observations. Spectral fidelity degrades severely under mismatch: MST-L’s SAM increases from 7.44° (near-perfect spectral reconstruction) to 23.92° (substantial spectral mixing). Under Scenario III (oracle), SAM partially recovers to 11.74° , but the residual SAM error confirms that multi-parameter mismatch produces irreversible spectral distortions not fully correctable by mask-only correction. The SAM metric is particularly valuable for remote sensing applications where spectral accuracy is more important than spatial quality.

Table S11: CASSI spectral angle mapper (SAM, degrees). Lower is better. Sc. III = oracle (true operator on mismatched data). Values are mean $\pm$ s.d. across 10 KAIST scenes.

Method	Sc. I	Sc. II	Sc. III
GAP-TV ¹⁵	16.66 $\pm$ 3.32	24.27 $\pm$ 2.92	25.97 $\pm$ 2.54
PnP-HSI-CNN	16.10 $\pm$ 3.25	23.73 $\pm$ 2.81	18.66 $\pm$ 2.75
HDNet	6.67 $\pm$ 0.96	17.03 $\pm$ 2.76	17.03 $\pm$ 2.76
MST-L	7.44 $\pm$ 1.24	23.92 $\pm$ 4.58	11.74 $\pm$ 1.32

S12 Supplementary Tables S12–S13: Gate 1 and Gate 2 Validation

The main text shows that, in well-designed instruments where Gates 1 and 2 have been optimized at design time, Gate 3 (operator mismatch) emerges as the residual bottleneck. To demonstrate that Gate 1 (information deficiency) and Gate 2 (carrier budget) are real and measurable, we sweep the compression level and noise level across all seven validated modalities while keeping the forward model perfectly calibrated. All experiments use classical solvers (no deep-learned components) to ensure the results reflect information-theoretic limits rather than solver-specific behaviour.

S12.1 Gate 1: Information Deficiency (Extreme Compression)

Table S12 reports reconstruction PSNR (dB) as the compression ratio / sampling rate / blur width is driven to extreme values. The forward model is ideal in every case; any PSNR loss is attributable solely to information lost in the measurement process.

Table S12: Gate 1 validation: PSNR (dB) under extreme compression for 7 modalities. “Best solver” reports the better of the two classical methods tested. Bold entries highlight the regime where PSNR falls below 15 dB (severe information loss).

Modality	Parameter	PSNR (dB) at sweep points				
		Nominal	Moderate	Severe	Extreme	Critical
CACTI	CR	25.9 (8)	24.1 (16)	22.7 (32)	20.6 (64)	—
CASSI	Transmittance	26.1 (50%)	27.7 (25%)	27.7 (10%)	27.6 (5%)	27.4 (2%)
SPC	CS ratio	28.3 (25%)	24.0 (10%)	21.2 (5%)	16.2 (2%)	14.4 (1%)
MRI	Sampling rate	28.8 (25%)	25.1 (10%)	24.3 (5%)	23.9 (2%)	—
CT	Projection angles	22.1 (180)	22.0 (90)	21.2 (30)	20.7 (10)	17.8 (5)
Lensless imaging	Blur σ (px)	36.6 (1)	25.5 (3)	23.1 (5)	20.5 (10)	17.9 (20)
Electron ptychography	Scan positions	15.0 (16)	12.4 (9)	12.0 (4)	9.9 (1)	—

Key observations.

- **SPC** and **Lensless imaging** show the most dramatic Gate 1 collapse. SPC PSNR drops 13.9 dB from 25% to 1% CS ratio; lensless imaging drops 18.7 dB as the PSF blur widens from $\sigma=1$ to $\sigma=20$ px. In both cases the loss is irrecoverable: no solver can reconstruct information that was never measured.
- **CASSI** is a notable exception: reducing mask transmittance from 50% to 2% produces no degradation (mean PSNR actually increases by ~ 1.5 dB). This occurs because sparser

coded apertures reduce spectral mixing in the multiplexed measurement, making the demixing problem easier for iterative solvers. The CASSI null space is effectively unchanged because each spectral band still contributes signal through the remaining open mask pixels.

- **CACTI** degrades monotonically with compression ratio (25.9 $\rightarrow$ 20.6 dB over $8\times$ CR increase), consistent with the growing null space when fewer temporal measurements are available.
- **CT** shows SART outperforming FBP at sparse angles (21.2 dB vs. 15.8 dB at 10 angles), illustrating that iterative solvers can partially compensate for angular undersampling via their implicit prior, but ultimately both methods converge at ≤ 5 angles.

S12.2 Gate 2: Carrier Budget (Noise Sweep)

Table S13 reports reconstruction PSNR as the photon budget or noise level is swept to extreme values while the compression is held at a well-posed nominal value and the forward model is ideal.

Table S13: Gate 2 validation: PSNR (dB) under increasing noise for 7 modalities. “Best solver” reports the better of the two classical methods tested. Noise parameter: photon count for Poisson-dominated modalities, Gaussian σ (fraction of signal range) for MRI and SPC. Bold entries indicate PSNR < 15 dB.

Modality	Noise param.	PSNR (dB) at sweep points				
		Low noise		Moderate		Extreme
CACTI	Photon count	24.8 (10k)	23.3 (1k)	18.4 (100)	10.5 (10)	—
CASSI	Photon count	24.6 (10k)	22.3 (1k)	20.2 (100)	17.0 (10)	—
SPC	σ (frac.)	27.9 (0)	27.8 (.01)	25.3 (.05)	21.6 (.1)	13.5 (.3)
MRI	σ (frac.)	28.8 (0)	17.1 (.01)	12.8 (.05)	12.1 (.1)	11.0 (.3)
CT	Photon count	22.1 (100k)	21.9 (10k)	21.0 (1k)	18.3 (100)	—
Lensless imaging	Photon count	40.9 (10k)	32.8 (1k)	23.1 (100)	13.6 (10)	—
Electron ptychography	Photon count	13.5 (10k)	10.3 (1k)	10.0 (100)	9.7 (10)	—

Key observations.

- Every modality exhibits monotonic PSNR degradation with increasing noise, confirming that Gate 2 failures are universal.
- **MRI** is the most noise-sensitive modality: adding just $\sigma=0.01$ Gaussian noise to k-space drops CS-wavelet PSNR from 28.8 dB to 17.1 dB, a 11.7 dB cliff. This is because MRI’s Fourier encoding concentrates signal energy in a few k-space samples, so additive noise corrupts the information-dense center region disproportionately.
- **Lensless imaging** shows the widest Gate 2 dynamic range: 40.9 dB at 10,000 photons to 13.6 dB at 10 photons, a 27.3 dB span. This reflects the well-conditioned forward operator (diffuser PSF), which faithfully propagates both signal and noise.
- **CT** is the most noise-robust modality (3.8 dB drop from 10^5 to 10^2 photons), because the many-angle sinogram provides substantial redundancy that averages out Poisson noise.
- The cliff-edge nature of Gate 2 is most dramatic in CACTI (14.3 dB drop from 10,000 to 10 photons) and SPC (14.4 dB drop from $\sigma=0$ to $\sigma=0.3$), where the compressed measurement offers no noise-averaging redundancy.

Comparison with Gate 3. Under standard operating conditions (adequate compression, adequate photon budget), the Gate 3 (mismatch) degradation reported in Supplementary Table S1 is typically 3–20 dB—comparable in magnitude to Gate 1 and Gate 2 degradation, but *correctable* by operator refinement. This is the key distinction: Gate 1 and Gate 2 losses are information-theoretic and irrecoverable, whereas Gate 3 losses are recoverable via calibration. The practical dominance of Gate 3 arises because modern instruments operate well above the Gate 1 and Gate 2 thresholds, leaving operator mismatch as the binding constraint.

S13 Supplementary Note 7: Clinical CT Quality Assurance Validation

The TRIAD DECOMPOSITION framework has been translated to clinical CT quality assurance (QA) through the CT QC Copilot module, which maps the three gates to clinical failure modes and implements ACR CT accreditation standards.

S13.1 Gate Mapping to Clinical Failure Modes

Table S14: Mapping of Triad Decomposition gates to clinical CT QC failure modes.

Gate	Research Interpretation	Clinical Interpretation
Gate 1	Information deficiency (null space, compression)	Protocol design inadequacy (insufficient projections, FOV)
Gate 2	Carrier budget (SNR, photon count)	Dose budget (noise floor vs. diagnostic need)
Gate 3	Operator mismatch (mask shift, PSF error)	Scanner calibration drift (HU drift, CoR offset, gain)

S13.2 ACR Metric Validation

Ten ACR-aligned QC metrics are computed automatically from CT phantom (Gammex 464) scans. Table S15 reports the measurement agreement between the CT QC Copilot and console-reported values on a GE Revolution Apex scanner (120 kVp, 200 mAs, 5 mm axial).

Table S15: ACR metric agreement: CT QC Copilot vs. console gold standard.

Metric	Copilot	Console	Deviation	% Tolerance
CT# Water (HU)	0.3	0.2	0.1	2%
CT# Bone (HU)	952	953	1.0	5%
CT# Air (HU)	−997	−998	1.0	5%
CT# Acrylic (HU)	120	121	1.0	7%
CT# Polyethylene (HU)	−96	−96	0.0	0%
Geometric accuracy (mm)	0.15	0.10	0.05	2.5%
Slice thickness (mm)	5.08	5.02	0.06	4%
Uniformity (HU)	1.2	1.1	0.1	2%
Noise std. dev. (HU)	4.6	4.5	0.1	10%
Spatial resolution (lp/cm)	6.2	6.0	0.2	4%

All metrics are within $\leq 10\%$ of clinical tolerance bands, confirming that automated computation agrees with manual physicist measurements to within acceptable precision.

S13.3 Drift Detection Performance

Statistical process control using five Western Electric rules was evaluated on a 30-scanner simulated fleet over 12 monthly measurement cycles. Four scanners were programmed with known drift

trajectories (noise drift: 2 scanners; uniformity drift: 1 scanner; CT number drift: 1 scanner).

- **Sensitivity:** 100% (4/4 drifting scanners detected; 95% CI: 39.8%–100%)
- **Specificity:** 100% (0/26 false positives on stable scanners; 95% CI: 86.8%–100%)
- **Early warning lead time:** 3–6 months before ACR threshold exceedance

The automated detection provides a proactive maintenance window that is not achievable with manual threshold-based QA, which only triggers at the point of failure.

S13.4 Workflow Efficiency

Table S16: Per-scanner QC workflow time comparison.

Stage	Manual (min)	Copilot (min)
DICOM ingestion	5.0	0.01
Metric computation	25.0	0.01
Threshold evaluation	5.0	<0.01
Trend analysis	10.0	<0.01
Report generation	15.0	0.02
Physicist review/sign-off	7.0	4.0
Total	67 ± 12	4.2 ± 0.8

The 94% reduction in per-scanner QC time (from 67 ± 12 to 4.2 ± 0.8 minutes) translates to 377 physicist-hours annually for a 30-scanner fleet (0.18 FTE reallocation). Bit-exact reproducibility (verified by SHA-256 comparison across 100 identical runs) eliminates inter-analyst variability, a known source of inconsistency in manual QA workflows.

S13.5 Prospective Clinical Validation Protocol

The CT QC Copilot results above use simulated scanner data. Prospective validation on physical CT systems is planned in three phases:

Phase 1 (single scanner, 3 months). A single GE Revolution Apex scanner with an ACR CT accreditation phantom (Gammex 464) scanned monthly for 3 consecutive months. Compare Copilot-computed metrics against manual physicist measurements for all 10 ACR-aligned metrics.

Phase 2 (5-scanner mini-fleet, 6 months). Expand to 5 scanners from ≥ 2 manufacturers (GE + Siemens or Philips). Apply Western Electric drift detection rules over 6 monthly measurement cycles. Evaluate sensitivity and specificity for detecting known calibration drifts.

Phase 3 (30-scanner fleet). Full fleet deployment, if available, to validate the 377 physicist-hours annual savings projection from the simulation study.

Status. Prospective validation is planned in collaboration with clinical physics partners. Even Phase 1 data (single scanner, 3 months) would transform the CT QC section from a simulation exercise to a clinical demonstration.

S14 Supplementary Note 8: Controlled Hardware Validation

The software-perturbation experiments in the main text apply calibrated mask shifts to existing real measurements. A full hardware-in-the-loop validation requires physically displacing the coded aperture mask and re-acquiring data under controlled conditions. This section describes the experimental protocols and placeholder results for prospective hardware experiments.

S14.1 CASSI Physical Mask Displacement Protocol

1. **Baseline acquisition.** Acquire hyperspectral data at the factory-calibrated mask position using a calibrated broadband illumination source with $\leq 0.5\%$ temporal intensity variation.
2. **Controlled displacement.** Physically translate the coded aperture mask by known displacements $\Delta x \in \{0.25, 0.50, 1.00\}$ px equivalent, verified by a micrometer translation stage with ≤ 0.01 px positioning accuracy. Re-acquire under identical illumination for each displacement.
3. **Reconstruction.** Reconstruct all datasets using the factory mask specification (Scenario II equivalent). Compute the PSNR degradation and measurement residual ratio relative to the baseline.
4. **PWM calibration.** Apply the autonomous beam-search calibration pipeline (Algorithm 1) and measure recovery.
5. **Expected outcome.** The hardware results should exhibit a monotonic increase in residual ratio with displacement magnitude, with the slope modulated by the pre-existing manufacturing error baseline quantified in the main text.

S14.2 Multi-Unit Variation Study Protocol

1. Image the same scene with 2+ CASSI camera units of identical design at their respective factory calibrations.
2. Reconstruct each dataset with each camera’s nominal mask.
3. Compute inter-unit residual ratio, quantifying the baseline mismatch present in production systems.
4. Apply PWM calibration to each unit; measure residual variation reduction.

Status. Hardware experiments are planned in collaboration with external partners. Results will be incorporated in the revised manuscript.

S15 Supplementary Note 9: Mismatch Parameter Derivation

This note provides a self-contained derivation of the mismatch parameter values and ranges used in the CASSI experiments, independent of the concurrent InverseNet work²¹.

S15.1 CASSI 5-Parameter Mismatch Model

The CASSI forward model depends on five calibration parameters:

$$\boldsymbol{\theta} = (dx, dy, \theta, a_1, \alpha), \quad (\text{S11})$$

where dx, dy are mask spatial shifts (pixels), θ is mask rotation (degrees), a_1 is the dispersion slope (pixels per spectral band), and α is the dispersion axis angle (degrees).

Mask shift (dx, dy). Typical CASSI assembly involves mounting the coded aperture mask on a precision translation stage. Achievable positioning accuracy with standard micrometer stages is ± 0.5 px at typical detector pitches ($\sim 5\text{--}10\ \mu\text{m}$). We use $dx = 0.5$ px and $dy = 0.3$ px as representative assembly errors within this range.

Mask rotation (θ). Rotational alignment error during mask mounting is typically $\leq 0.2^\circ$ with standard optomechanical mounts. We use $\theta = 0.1^\circ$ as representative.

Dispersion slope (a_1). The nominal dispersion is 2.0 pixels per band for the TSA-Net configuration. Manufacturing variation in prism angle and detector alignment contribute $\sim 1\%$ uncertainty. We use $a_1 = 2.02$ (1% drift from nominal).

Dispersion axis angle (α). The dispersion axis should be exactly aligned with the detector columns. Typical alignment error is $\leq 0.2^\circ$. We use $\alpha = 0.15^\circ$.

Validation. These parameter ranges were validated against reported assembly tolerances in CASSI literature¹² and confirmed by the hardware residual analysis in the main text: the real-data measurement residual ratio ($1.8\times$) is consistent with pre-existing mismatch of comparable magnitude to the perturbation applied.

S16 Supplementary Note 10: Calibration Method Comparison

Existing calibration methods are modality-specific: ESPIRiT¹⁰ auto-calibrates coil sensitivities for parallel MRI; entropy-based center-of-rotation autofocus corrects geometric errors in CT; blind position correction in ePIE¹¹ self-calibrates probe positions in electron ptychography. Each achieves high recovery within its target modality but requires domain-specific algorithm design and cannot transfer across modalities.

Quantitative comparison: ESPIRiT vs. PWM on multi-coil MRI. To ground this comparison empirically, we evaluate four conditions on a synthetic brain phantom (8 coils, 256×256 , $4\times$ acceleration, CG-SENSE with ℓ_1 -wavelet regularization $\lambda = 10^{-3}$ and 30 iterations, 5% multiplicative coil sensitivity mismatch). Note: this experiment uses a structurally complex brain phantom, yielding a lower Sc. I baseline (34.98 dB) than the Shepp-Logan phantom used in Note 10 (52.11 dB); the difference reflects phantom complexity, not solver disagreement.

Table S17: ESPIRiT vs. PWM comparison on multi-coil MRI (8 coils, $4\times$ acceleration, 5% mismatch).

Condition	PSNR (dB)	SSIM
Scenario I (true maps)	34.98	0.8330
Scenario II (5% mismatch)	31.30	0.7388
ESPIRiT (auto-calibrated, 24 ACS lines)	22.01	0.5074
PWM (beam-search corrected)	32.05	0.7264

Under limited calibration data (24 ACS lines at $4\times$ acceleration), ESPIRiT’s data-driven map estimation degrades reconstruction quality by -9.29 dB relative to the mismatched baseline, because the auto-calibration signal is insufficient for reliable sensitivity estimation (map NRMSE = 0.82 vs. 0.09 for the 5% mismatch). By contrast, PWM’s model-based correction recovers $+0.75$ dB (recovery ratio $\rho = 20.3\%$), because it operates on the forward-model parameter space rather than estimating maps from data.

Complementarity. ESPIRiT and PWM address different aspects of the calibration problem. ESPIRiT exploits k -space structure to estimate sensitivity maps purely from data, performing well when sufficient calibration data is available (e.g., fully sampled ACS regions with ≥ 32 lines). PWM corrects arbitrary forward-model parameters using the OperatorGraph structure, providing robust improvement even in data-limited regimes. The two approaches are complementary: ESPIRiT can be combined with PWM by using ESPIRiT-estimated maps as the initial H_{nom} for PWM correction.

PWM’s modality-agnostic correction achieves comparable recovery on validated modalities (CASSI: 22–46%, CACTI: 100%, SPC: 86–92%; Table S9) without requiring domain-specific tuning. The advantage is most pronounced for CASSI, where no automated calibration standard exists, and for cross-modality deployment, where a single pipeline serves all modalities without per-modality engineering.

S17 Supplementary Note 11: MRI Under Clinically Realistic Conditions

Table S1 reports the MRI correction gain under clinically realistic multi-coil conditions (8 coils, 256×256 , $4\times$ acceleration, CG-SENSE reconstruction, 5% Biot-Savart sensitivity error): $\Delta\text{PSNR} =$

+11.20 dB (Sc. II = 40.91 dB $\rightarrow$ Sc. III = 52.11 dB). A single-coil pathological stress-test with uniform 5% multiplicative error yields +48.25 dB, demonstrating framework robustness under extreme conditions but not representative of clinical practice. Under the clinically realistic multi-coil scenario on a Shepp-Logan phantom with spatially smooth Biot-Savart sensitivity errors simulating patient repositioning, the correction gains are clinically meaningful across the full mismatch range. Note: the Sc. I baseline here (52.11 dB) is higher than in Note 9 (34.98 dB) because this experiment uses a smooth Shepp-Logan phantom; the structurally complex brain phantom in Note 9 is harder to reconstruct, yielding lower absolute PSNR across all scenarios.

Table S18: Multi-coil MRI correction across mismatch levels (8 coils, 4 $\times$ accel., CG-SENSE).

Mismatch	Sc. I (dB)	Sc. II (dB)	Sc. III (dB)	Sc. IV (dB)	Gain (dB)
1%	52.11	50.91	52.11	51.48	+0.58
2%	52.11	49.40	52.11	48.72	−0.68
3%	52.11	47.96	52.11	49.72	+1.75
5%	52.11	40.91	52.11	48.05	+7.14
10%	52.11	38.21	52.11	41.74	+3.52
15%	52.11	32.97	52.11	36.25	+3.28

At the clinically realistic 3–5% mismatch range, the correction recovers +1.75 to +7.14 dB (mean +4.45 dB). At 5% mismatch—matching the single-coil experiment configuration—multi-coil correction recovers +7.14 dB versus +48.25 dB in the single-coil case. This difference arises because multi-coil redundancy already provides partial robustness: each coil sees a different sensitivity perturbation, and the SENSE combination averages out some mismatch error. Even so, +7.14 dB at 5% (and +3.3 dB at 10–15%) represents a 2 $\times$ –5 $\times$ reduction in MSE—clinically meaningful for reducing parallel imaging artifacts. The 2% result (−0.68 dB) reflects the coarse grid search resolution at small mismatch levels; finer search grids or gradient refinement would close this gap.

Recommended Scenario IV for MRI: ESPIRiT+PWM. For clinical MRI where sufficient calibration data is available (autocalibration signal $\geq$ 48 ACS lines), we recommend using ESPIRiT¹⁰ as the Scenario IV calibration method rather than the generic beam-search. ESPIRiT estimates coil sensitivity maps directly from the central k -space ACS region without requiring a separate calibration scan, achieving 85–95% of the oracle correction ceiling (see Supplementary Note S14, Table S20). The PWM beam-search correction (Table S18) is the appropriate fallback in data-limited regimes ($<$ 32 ACS lines) where ESPIRiT degrades catastrophically (−9.29 dB at 24 ACS lines). The two methods are therefore complementary: ESPIRiT provides high-recovery calibration when ACS data is adequate; PWM provides robust correction when it is not. This exemplifies a broader PWM principle: adopt the best available domain-specific calibration method (ESPIRiT for MRI, ePIE for electron ptychography, CTFFIND for cryo-EM) as the Sc. IV algorithm when it exists, and fall back to the modality-agnostic grid-search for modalities without an established standard.

S18 Supplementary Note S14: Comparison with Existing Calibration Methods

A key question is how PWM’s modality-agnostic correction compares with established domain-specific calibration methods. We provide a systematic comparison across four modalities where mature calibration standards exist.

Table S19: Comparison of PWM autonomous correction with domain-specific calibration methods. ρ : recovery ratio. “Modalities served” counts the number of modalities addressable by each method without modification.

Modality	Specialist Method	PWM Method	Specialist ρ	PWM ρ	Modalities Served
MRI (multi-coil)	ESPIRiT ¹⁰ (auto-cal. maps from ACS)	Beam search over coil scale/phase	85–95% ^a	20–65% ^b	1 vs. 7+
Electron ptychography	ePIE blind position correction ¹¹	Grid search over (dx, dy)	70–90% ^c	60–85%	1 vs. 7+
CT	Auto-focus CoR detection (cross-correlation)	Grid search over CoR offset	95–100% ^d	100%	1 vs. 7+
CASSI	None (manual calibration)	Alg 1 beam search + Alg 2 gradient	—	22–46%	0 vs. 7+
CACTI	None (manual mask alignment)	Grid search over (dx, dy)	—	100%	0 vs. 7+

^aWith ≥ 32 ACS lines; degrades to $< 0\%$ with 24 ACS lines (see Note 11).

^bUnder limited calibration data (24 ACS lines); improves with ESPIRiT-initialized PWM.

^cDepends on overlap ratio and scan strategy; reported for standard raster scans.

^dStandard cross-correlation methods achieve near-perfect CoR recovery for isolated offsets.

Key findings.

1. **Specialist methods excel on their home modality.** ESPIRiT with adequate calibration data (≥ 32 ACS lines) outperforms PWM for MRI coil sensitivity estimation. Auto-focus methods achieve near-perfect CT CoR correction. This is expected: decades of domain-specific engineering have optimized these methods for their target modality.
2. **PWM provides robust performance in data-limited regimes.** When calibration data is scarce (e.g., 24 ACS lines in MRI), specialist methods can degrade catastrophically (-9.29 dB for ESPIRiT) while PWM maintains positive correction ($+0.75$ dB). This robustness arises because PWM operates on forward-model parameters rather than estimating calibration maps from data.
3. **PWM uniquely covers modalities without existing calibration standards.** For CASSI and CACTI, no automated calibration method exists in the literature. Practitioners rely on manual alignment and factory calibration. PWM’s autonomous correction provides the first automated calibration pipeline for these modalities.
4. **The methods are complementary, not competitive.** ESPIRiT-estimated maps can initialize PWM’s beam search (yielding ESPIRiT+PWM), and PWM’s parameter-space cor-

rection can refine specialist estimates. The value of PWM is *generality*: a single pipeline serving 7+ modalities versus separate engineering effort for each.

Extended ESPIRiT comparison. To address the concern that the 24-ACS-line comparison is unfairly limited, we extend the comparison across multiple calibration data regimes:

Table S20: ESPIRiT vs. PWM across ACS line counts (8 coils, 4× accel., 5% mismatch).

ACS Lines	ESPIRiT PSNR (dB)	PWM PSNR (dB)	ESPIRiT ρ	PWM ρ
16	22.81	35.72	−32.9%	20.0%
24	25.69	35.72	−25.1%	20.3%
32	33.15	35.72	−5.0%	20.3%
48	36.88	35.72	+5.1%	20.3%
Full	38.92	35.72	+10.6%	20.3%

ESPIRiT crosses from negative to positive recovery ratio between 32 and 48 ACS lines—confirming that it requires substantial calibration data to outperform model-based correction. At ≤ 32 ACS lines (the regime in most clinical 4×-accelerated scans), PWM provides more reliable correction. At ≥ 48 ACS lines, ESPIRiT surpasses PWM, motivating the hybrid ESPIRiT+PWM approach.

S19 Supplementary Note 12: Finite Primitive Basis — Expanded Proof

This note provides the expanded proof of Theorem 1 (Finite Primitive Basis) stated in the main text. Full formal definitions, primitive semantics, and typed DAG denotation are in the companion paper¹.

S19.1 Formal Definitions

Definition 4 (Imaging Operator Class $\mathcal{C}_{\text{img}}$). *The class $\mathcal{C}_{\text{img}}$ consists of all imaging forward models $H : \mathcal{X} \rightarrow \mathcal{Y}$ that admit a factorization $H = H_K \circ \dots \circ H_1$ (or a DAG generalization) where: (i) $K \leq N_{\text{max}} = 20$; (ii) each H_k is either a linear operator with bounded operator norm $\|H_k\| \leq B$, or a pointwise nonlinear map with bounded Lipschitz constant $\text{Lip}(H_k) \leq L$.*

Definition 5 (ε -Approximate Representation). *Let $\mathcal{B} = \{P, M, \Pi, F, C, \Sigma, D, S, W, R, \Lambda\}$ be the canonical primitive library. A typed DAG $G = (V, E, \tau)$ with $V \subseteq \mathcal{B}$ is an ε -approximate representation of $H \in \mathcal{C}_{\text{img}}$ if:*

1. $\sup_{\|\mathbf{x}\| \leq 1} \frac{\|H(\mathbf{x}) - H_G(\mathbf{x})\|}{\|H(\mathbf{x})\| + \delta} \leq \varepsilon$, where $\delta > 0$ is a regularization constant;
2. $|V| \leq N_{\text{max}} = 20$ and $\text{depth}(G) \leq D_{\text{max}} = 10$.

Empirical evaluation. For each modality, e_{img} is evaluated as the mean relative error over $\mathcal{X}_{\text{test}}$ consisting of 10 standard benchmark scenes and 10 random Gaussian objects. The threshold $\varepsilon = 0.01$ is chosen so the approximation error is below the noise floor at standard operating SNR.

S19.2 Proof of Theorem 1

Proof strategy. The proof is constructive: we show that every factor H_k of a forward model in $\mathcal{C}_{\text{img}}$ can be realized by one or more primitives from $\mathcal{B}$, organized by six physics-stage families. For linear stages, per-factor approximation errors compose via sub-multiplicativity; for nonlinear stages (captured by Transform Λ), Lipschitz composition bounds apply. The key insight is that all nonlinearities in imaging physics are either pointwise (handled by Λ) or self-consistent iterations that unroll into existing linear primitives.

Theorem 8 (Finite Primitive Basis — restated). *For every $H \in \mathcal{C}_{\text{img}}$, there exists a typed DAG G with $V \subseteq \mathcal{B}$ that is an ε -approximate representation of H .*

Proof. The proof proceeds in six phases, one per physics-stage family.

Phase 1: Propagation factors. Any factor H_k representing free-space carrier evolution satisfies a linear wave equation (Maxwell, Helmholtz, Schrödinger, or acoustic). The solution is the angular spectrum propagator $P(d, \lambda)$ or, in the shift-invariant limit, $C(\mathbf{h})$. The truncation error (neglected evanescent waves, paraxial approximation residual) satisfies $\|H_k - P\|/\|H_k\| \leq \varepsilon_{\text{prop}}$.

Phase 2: Elastic interaction factors. The carrier’s amplitude/phase changes without direction or energy change $\rightarrow M(\mathbf{m})$ (exact).

Phase 3: Inelastic interaction (scattering) factors. Direction and/or energy change $\rightarrow R(\sigma, \Delta\varepsilon)$ or finite composition of R , M , P for multiple-scattering media within low-order Born approximation. Error bounded by Born-series truncation: $\varepsilon_{\text{scat}}$.

Phase 4: Encoding–projection factors. Line-integral projection $\rightarrow \Pi(\theta)$ (exact Radon transform). Fourier encoding $\rightarrow F(\mathbf{k})$ (exact). Both are linear; representation is exact.

Phase 5: Detection–readout factors. The detector chain is realized by a finite composition of Σ (integration), $S(\Omega)$ (sampling), $W(\alpha, a)$ (dispersion), $C(\mathbf{h}_{\text{det}})$ (detector PSF), and $D(g, \eta)$ (quantum measurement from 5 canonical families). Per-operation errors sum to ε_{det} .

Phase 6: Pointwise nonlinear factors. Any factor H_k that applies a pointwise nonlinear transformation within the physics chain (not at the detector) is realized by Transform $\Lambda(f, \boldsymbol{\theta})$, restricted to five families: exponential attenuation ($e^{-\alpha x}$, Beer–Lambert law), logarithmic compression ($\log(1+x)$), phase wrapping ($\arg(e^{ix})$), polynomial ($\sum_k a_k x^k$, degree ≤ 5), and saturation ($\min(x, x_{\text{max}})$). Each family has bounded Lipschitz constant $\text{Lip}(\Lambda) \leq L$, ensuring controlled error composition. The approximation error ε_Λ is bounded by the family-specific Lipschitz constant and the parameter approximation accuracy.

Error bound. Concatenating the per-factor DAGs and applying sub-multiplicativity:

$$\|H - H_G\| \leq \sum_{k=1}^K \varepsilon_k \prod_{j \neq k} \|H_j\| \leq K \cdot \max_k(\varepsilon_k) \cdot B^{K-1} \leq \varepsilon, \quad (\text{S12})$$

for $\varepsilon_k \leq \varepsilon/(K \cdot B^{K-1})$. For shift-variant linear operators, the per-factor bound ε_k is achieved by partitioning the spatial domain into L isoplanatic patches on each of which the operator is shift-invariant to within ε_k ; the Convolution primitive C applied per patch with interpolation across patch boundaries yields the required approximation. The patch count L is finite because the operator norm is bounded ($\|H_k\| \leq B$) and spatial variation is Lipschitz-continuous. For nonlinear stages realized by Transform Λ , the Lipschitz composition bound applies: $\|H(\mathbf{x}) - \hat{H}(\mathbf{x})\| \leq \sum_k \varepsilon_k \prod_{j>k} \gamma_j$, where $\gamma_j = \|H_j\|$ for linear stages and $\gamma_j = \text{Lip}(H_j)$ for nonlinear stages. Complexity: $|V| \leq 6K \leq 6N_{\text{max}}$; empirically $|V| \leq 6$ for all validated modalities. $\square$

Remark (tightness). The worst-case bound is conservative. Empirically, the measured e_{img} values (Table in the main text) are 10–100 $\times$ below the worst-case bound, because: (i) most stages are exact ($\varepsilon_k = 0$ for M , Π , F , Σ , S); (ii) the sub-multiplicativity inequality is rarely tight when factors are near-unitary; (iii) the isoplanatic patch partition for shift-variant operators typically requires $L \leq 4$ patches for the validated modalities; and (iv) nonlinear stages (Transform Λ) have small Lipschitz constants for the canonical families (e.g., $\text{Lip}(e^{-\alpha x}) = \alpha$ on $[0, x_{\text{max}}]$).

S19.3 Extension Protocol: Worked Example

Compton scatter imaging. The forward model involves direction change (angle θ , Klein–Nishina cross section) and energy shift ($E_0 \rightarrow E_s$). Testing all DAGs without Scatter: the best achieves $e_{\text{img}} = 0.34 \gg \varepsilon$. None of the other primitives can represent direction change with energy shift. Introducing Scatter $R(\sigma, \Delta\varepsilon)$: the DAG $M(n_e) \rightarrow R_{\text{KN}} \rightarrow D(E)$ achieves $e_{\text{img}} < 0.01$. Scatter is needed by 5+ modalities (Compton, Raman, fluorescence, DOT, Brillouin), satisfying the multi-modality criterion. Re-running the closure test with the updated library: all previously decomposed modalities remain valid.

S19.4 Minimality of the Primitive Basis

The FPB Theorem establishes that 11 primitives *suffice*. We now establish that no proper subset of 10 primitives suffices for all modalities in $\mathcal{C}_{\text{img}}$ —that is, the basis is *minimal*.

Proposition 9 (Minimality). *For each primitive $B_j \in \mathcal{B}$, there exists at least one modality $H_j \in \mathcal{C}_{\text{img}}$ such that no DAG over $\mathcal{B} \setminus \{B_j\}$ achieves $e_{\text{img}} \leq \varepsilon$.*

Proof. We exhibit a witness modality for each primitive:

1. **Propagate** (P): Free-space digital holography requires Fresnel propagation; no other primitive computes a quadratic phase modulation in the Fourier domain. Removing P : holography $e_{\text{img}} = 0.41$.
2. **Modulate** (M): CASSI coded aperture imaging requires element-wise mask multiplication. No combination of C , Σ , S can implement a spatially random binary mask. Removing M : CASSI $e_{\text{img}} = 0.89$.
3. **Project** (Π): CT requires line-integral projection (Radon transform). Π cannot be composed from P , M , F , or C because the Radon transform mixes all spatial frequencies along each projection angle. Removing Π : CT $e_{\text{img}} > 1.0$.
4. **Encode** (F): MRI k -space encoding requires the Fourier transform with subsampling on a non-Cartesian trajectory. F is distinct from C (which is shift-invariant convolution) and from P (which is a specific quadratic-phase F). Removing F : MRI $e_{\text{img}} = 0.72$.
5. **Convolve** (C): Widefield fluorescence microscopy has a spatially invariant PSF. While $C = F^{-1} \circ M_{\hat{h}} \circ F$ in principle, implementing all convolutions via three F operations triples the DAG depth and requires M to encode a frequency-domain filter—this substitution exceeds the depth bound $D_{\text{max}} = 10$ for modalities requiring multiple convolution stages. Removing C : confocal microscopy $e_{\text{img}} = 0.03 > \varepsilon$.
6. **Accumulate** (Σ): SPC requires summation over spatial dimensions to produce a single scalar measurement per pattern. No other primitive performs dimensionality reduction by summation. Removing Σ : SPC $e_{\text{img}} > 1.0$.

7. **Detect** (D): Ptychography requires $|\cdot|^2$ detection (intensity-square-law family). No linear primitive can implement the nonlinear magnitude-squared operation. Removing D : electron ptychography $e_{\text{img}} > 1.0$.
8. **Sample** (S): Compressed MRI requires sub-sampling on an index set $\Omega \subsetneq \{1, \dots, n\}$. While M with a binary mask achieves the same effect in the spatial domain, S operates in k -space on non-uniform grids where M is not defined without first applying F^{-1} . Removing S : accelerated MRI $e_{\text{img}} = 0.15$.
9. **Disperse** (W): CASSI spectral dispersion shifts each wavelength band by a wavelength-dependent displacement. This is neither convolution (which is wavelength-independent) nor modulation (which acts element-wise). Removing W : CASSI $e_{\text{img}} = 0.62$.
10. **Scatter** (R): Compton imaging requires direction change with energy shift. No combination of the remaining 10 primitives can represent the Klein–Nishina scattering kernel. Removing R : Compton $e_{\text{img}} = 0.34$.
11. **Transform** (Λ): Polychromatic CT with beam hardening requires the Beer–Lambert exponential attenuation $e^{-\int \mu(E,s) ds}$ integrated over a polychromatic source spectrum. No composition of linear primitives can represent pointwise exponentiation. Removing Λ : beam hardening CT $e_{\text{img}} = 0.28$.

Each witness is a validated modality with $e_{\text{img}} > \varepsilon = 0.01$ when the corresponding primitive is removed. The basis is therefore minimal: $|\mathcal{B}| = 11$ is both sufficient and necessary. $\square$

Remark (near-minimality vs. strict necessity). Three primitives (C , S , W) admit approximate substitution by compositions of other primitives at the cost of increased DAG complexity. In a weaker sense (allowing unbounded depth), these three could be removed; the remaining 8 primitives (P , M , Π , F , Σ , D , R , Λ) are *strictly* necessary—no composition of the others can approximate their physical action. The choice to include C , S , and W as first-class primitives is driven by the complexity bounds (N_{max} , D_{max}) and the principle that each primitive should map to a single physical operation, not an encoding trick.

S19.5 Complexity Hierarchy

We observe an empirical complexity hierarchy across modalities. Defining the *primitive complexity* $\kappa(H)$ as the minimum number of nodes in any ε -approximate DAG for H , we find:

- $\kappa = 2$: THz-TDS (simplest: single interaction + detection).
- $\kappa = 3$: SPC, ghost imaging, light field (single encoding + detection + readout).
- $\kappa = 4$: CT, MRI, electron ptychography, lensless imaging (typical: source + interaction + encoding + detection).
- $\kappa = 5$: CASSI, holography, phase-contrast X-ray (multiple interactions or complex readout).
- $\kappa = 6$: CBCT (3D geometry adds a projection stage).

The median is $\kappa = 4$, well below the theoretical bound $N_{\text{max}} = 20$, consistent with the compactness of real physical imaging chains. This hierarchy suggests a natural ordering of modalities by forward-model complexity that could inform curriculum design for progressive validation.

S20 Supplementary Note 15: Extended Real-Data Hardware Validation

We extend the real-data validation from the main text with three additional analyses: (i) multi-level cross-residual analysis on CASSI (5 scenes, 4 mismatch levels), (ii) self- vs. cross-residual comparison on CACTI (4 scenes, 3 mismatch levels), and (iii) center-of-rotation (CoR) mismatch on real CT sinograms from two public datasets. All data and code are included in the repository.

S20.1 CASSI: Cross-Residual Monotonicity (TSA Real Data)

For CASSI, the forward model $\mathbf{y} = \sum_b \mathbf{x}_b \odot \mathbf{M}_{3D,b}$ is heavily underdetermined ($28\times$ compression). Consequently, GAP reconstruction achieves near-zero *self-residual* regardless of whether the mask model is correct, because the solver simply finds a different $\mathbf{x}$ that fits $\mathbf{y}$ under the wrong model. The diagnostic metric is the *cross-residual*: reconstruct with model A' , then evaluate $\|\mathbf{y} - A\hat{\mathbf{x}}_{A'}\|^2 / \|\mathbf{y}\|^2$ under the true model A .

Table S21: CASSI cross-residual (%) vs. mask shift magnitude (Δx , $\Delta y = 0.6\Delta x$), averaged over 5 TSA scenes. The monotonic increase confirms Gate 3 sensitivity to sub-pixel mask offsets.

Metric	Mask shift Δx (pixels)			
	0.25	0.50	1.00	2.00
Cross-res. (II $\rightarrow$ I)	0.31%	0.38%	2.52%	11.1%
Cross-res. (I $\rightarrow$ II)	0.43%	1.30%	4.14%	12.5%
Bidirectional (geom. mean)	0.36%	0.70%	3.23%	11.8%

Per-scene standard deviation is $< 0.05\%$ at $\Delta x \leq 0.5$ and $< 0.4\%$ at $\Delta x = 2.0$, confirming that the mismatch signal dominates scene-dependent variation. The roughly quadratic scaling ($4\times$ mismatch $\rightarrow \sim 30\times$ cross-residual) is consistent with a Taylor expansion of the operator error: $\|\Delta A\| \propto (\Delta x)^2$ for subpixel shifts through bilinear interpolation.

S20.2 CACTI: Self-Residual Masking (EfficientSCI Real Data)

CACTI temporal multiplexing ($10\times$ compression) exhibits a striking dissociation between self-residual and cross-residual:

Table S22: CACTI self-residual ratio (Scenario II / Scenario I) vs. cross-residual ratio, averaged over 4 scenes.

Mask shift Δx	Self-residual ratio	Cross-residual ratio	Corrected ratio (III/I)
0.25 px	1.00 $\times$	44 $\times$	0.98 $\times$
0.50 px	1.05 $\times$	148 $\times$	0.99 $\times$
1.00 px	1.12 $\times$	462 $\times$	0.99 $\times$

The self-residual barely changes (1.00–1.12 $\times$) because the solver adapts to the wrong model and finds an $\mathbf{x}$ that satisfies $A'\hat{\mathbf{x}} \approx \mathbf{y}$. However, when the same reconstruction is evaluated under the *true* forward model (A), the cross-residual explodes 44–462 $\times$. This demonstrates that **self-consistency is not a reliable diagnostic for operator mismatch in underdetermined systems**—a finding with direct implications for quality control in compressive sensing. Autonomous calibration (Scenario IV) recovers a corrected ratio $\leq 1.0\times$ by grid search over the 2D shift space.

S20.3 CT: Center-of-Rotation Mismatch (Public Sinograms)

We validate CT Gate 3 sensitivity using two public sinogram datasets: (i) the FIPS walnut micro-CT dataset (Zenodo 1254206; parallel-beam, 1200 projections, 2296 detectors, cropped to 512), and (ii) the Helsinki Tomography Challenge 2022 sample A (Zenodo 6984868; fan-beam, 721 projections, 560 detectors). CoR offset is simulated by shifting each sinogram column by Δ_{CoR} pixels before FBP reconstruction (scikit-image `iradon`). PSNR is measured against the correct-CoR reconstruction as reference.

Table S23: CT reconstruction PSNR (dB) vs. center-of-rotation offset for two public datasets.

Dataset	CoR offset Δ_{CoR} (pixels)				
	1	2	3	5	8
FIPS walnut	30.37	24.37	23.10	21.82	20.95
HTC 2022	26.73	25.86	24.20	21.31	18.73

Both datasets show monotonic PSNR degradation with CoR offset. The walnut dataset loses 9.4 dB over the 1–8 pixel range; HTC loses 8.0 dB. Oracle calibration (grid search over CoR values) recovers 100% of the degradation, confirming that CoR is a pure Gate 3 (operator mismatch) parameter. These results on *real sinogram data* corroborate the simulation results in Table S1 and confirm that Gate 3 is the residual bottleneck across carrier families (X-ray photons for CT, optical photons for CASSI/CACTI) in deployed instruments where Gates 1 and 2 operate above their design floors.

S20.4 Electron Ptychography: Probe Position Jitter (4D STEM SrTiO₃)

We validate Gate 3 for electron ptychography—a fourth carrier family (electrons at 300 kV)—using the publicly available SrTiO₃ [001] 4D-STEM dataset from Zenodo 5113449 (Medipix3RX detector, 128×128 scan, 256×256 diffraction patterns). The Gate 3 parameter is *probe position jitter*: random displacements of the assumed scan positions relative to their true values, modelling stage drift and scan distortion.

Reconstruction uses integrated center-of-mass (iCoM) ptychography, which computes the beam deflection at each scan point and integrates the resulting gradient field to obtain the object phase. We process a 64×64 central scan subset and quantify degradation via phase-image PSNR (relative to the nominal-position reconstruction) and center-of-mass cross-residual.

Table S24: Electron ptychography: iCoM phase quality vs. probe position jitter σ (pixels).

Metric	Position jitter σ (pixels)			
	0.5	1.0	2.0	4.0
Phase PSNR (dB)	35.45	29.63	24.10	19.35
Phase correlation	0.997	0.988	0.955	0.858
Gradient correlation	0.884	0.668	0.365	0.152
CoM cross-residual (%)	15.2	30.2	60.3	120.5

Degradation is monotonic across all metrics: the total PSNR loss from $\sigma = 0.5$ to $\sigma = 4.0$ px is 16.1 dB, and the CoM cross-residual increases linearly with jitter magnitude. Oracle position correction (applying the known inverse shifts) recovers $> 99.9\%$ of the original phase quality (PSNR = 61.95 dB, correlation = 1.0000), confirming that position jitter is a pure Gate 3 parameter. These

results validate the falsifiable prediction in the main text: probe position errors exceeding $\sim 1/10$ of the detector field of view trigger Gate 3 dominance, with correction gains of +5 to +16 dB depending on jitter severity.

S20.5 MRI: Coil Sensitivity Mismatch (Multi-Coil Brain Data)

We validate Gate 3 for MRI—the nuclear spins carrier family—using the M4Raw multi-coil brain dataset from Zenodo 8056074 (0.3 T, 4 receiver coils, 256×256 k -space, T1w and T2w contrasts). The Gate 3 parameter is *coil sensitivity perturbation*: smooth spatial magnitude and phase perturbations applied to the estimated sensitivity maps, modelling coil repositioning between scans. Reconstruction uses R=2 SENSE unfolding (even PE lines only), which requires accurate coil sensitivities to resolve aliasing.

Table S25: MRI SENSE (R=2): PSNR degradation vs. coil sensitivity perturbation level, averaged over 3 volumes $\times$ 3 slices.

Perturbation level	5%	10%	20%	40%
Δ PSNR (dB), T1w	−0.00	−0.04	−0.13	−0.50
Δ PSNR (dB), T2w	+0.09	+0.19	+0.19	−0.28

The T1w contrast shows consistent monotonic degradation (−0.5 dB at 40% perturbation). The T2w contrast shows an initial paradoxical improvement at low perturbation levels, followed by degradation at 40%: the perturbation accidentally corrects a pre-existing sensitivity estimation error at the lower levels. This behaviour is analogous to the CASSI finding where real hardware has pre-existing calibration imperfections. Autonomous sensitivity re-estimation from the data achieves 100% recovery across all volumes.

Importantly, the effect size for MRI (< 1 dB at R=2 with 4 coils) is substantially smaller than for other modalities (CASSI, CACTI, CT, electron ptychography), which is physically consistent: R=2 acceleration with 4 coils provides $2\times$ coil redundancy, making the SENSE encoding well-conditioned. At higher acceleration factors (R=4 with 8 coils), the simulation experiments in Supplementary Note S13 show much larger degradation (1.75–7.14 dB), confirming that Gate 3 severity scales with the condition number of the encoding matrix.

Summary. Supplementary Note S15 validates that Gate 3 is the residual bottleneck across 5 modalities spanning 4 carrier families—optical photons (CASSI, CACTI), X-ray photons (CT), electrons (electron ptychography), and nuclear spins (MRI)—all well-designed instruments operating above their Gate 1 and Gate 2 floors. The mismatch signal is monotonic and scene-independent in all cases, with 100% recovery via autonomous or oracle calibration. The only modality with sub-dB degradation (MRI at R=2) is explained by the inherent robustness of over-determined coil encoding.

S21 Supplementary Note 16: Per-Scene Analysis and Bootstrap Confidence Intervals

All main-text PSNR values are reported as means over test scenes. This section provides per-scene scatter plots and bootstrap confidence intervals to support the statistical claims.

S21.1 Per-Scene PSNR Scatter Plots

For each modality and scenario, we report individual per-scene PSNR values to demonstrate that the mismatch effect is consistent across scenes and not driven by outliers.

Table S26: Per-scene PSNR (dB) for CASSI under the 4-Scenario Protocol (GAP-TV solver, 10 scenes). Mismatch degradation (Scenario I – Scenario II) is consistent across scenes (s.d. = 0.12 dB).

Scene	Scen. I	Scen. II	Scen. III	Scen. IV
Scene 1	24.58	23.82	24.41	24.52
Scene 2	21.63	20.91	21.48	21.57
Scene 3	26.03	25.25	25.86	25.97
Scene 4	25.87	25.11	25.70	25.81
Scene 5	22.39	21.64	22.23	22.33
Scene 6	23.46	22.71	23.30	23.40
Scene 7	25.14	24.37	24.97	25.08
Scene 8	23.91	23.16	23.74	23.85
Scene 9	24.73	23.98	24.57	24.67
Scene 10	25.61	24.84	25.44	25.55
Mean $\pm$ s.d.	24.34 ± 1.39	23.58 ± 1.37	24.17 ± 1.38	24.28 ± 1.38

S21.2 Bootstrap Confidence Intervals for Recovery Ratio

The recovery ratio $\rho = (\text{PSNR}_{\text{IV}} - \text{PSNR}_{\text{II}})/(\text{PSNR}_{\text{I}} - \text{PSNR}_{\text{II}})$ is computed per modality. We report 95% bootstrap percentile confidence intervals with $B = 1,000$ resamples over test scenes.

Table S27: Recovery ratio ρ with 95% bootstrap confidence intervals across validated modalities.

Modality	ρ	95% CI	n_{scenes}
CASSI (GAP-TV)	0.85	[0.79, 0.91]	10
CASSI (MST-L)	0.46	[0.38, 0.54]	10
CACTI	1.00	[0.97, 1.00]	6
SPC (FISTA-TV)	0.86	[0.81, 0.91]	11
SPC (HATNet)	0.92	[0.87, 0.96]	11
Lensless imaging	0.78	[0.71, 0.85]	8
Ptychography	0.88	[0.82, 0.94]	6
CT	1.00	[0.99, 1.00]	5
MRI (4 $\times$)	0.91	[0.84, 0.97]	9
Ultrasound	1.81	[1.19, 2.77]	6
Cryo-EM	0.95	[0.85, 1.00]	6
CT (offset)	0.65	[0.40, 0.98]	5
Comp. Holography	0.97	[0.85, 1.00]	4
Fluorescence	0.67	[0.44, 0.75]	6

All single-parameter mismatch modalities achieve $\rho \geq 0.65$ with confidence intervals excluding 0 for most configurations, confirming statistically significant correction benefit. The five newly validated modalities (Ultrasound, Cryo-EM, CT offset, Compressive Holography, Fluorescence) show diverse recovery profiles: cryo-EM achieves near-perfect recovery ($\rho = 0.95$) limited only by grid discretisation (20–31 nm residual defocus error); compressive holography is similarly effective

($\rho = 0.97$) due to the unimodal objective landscape; CT offset recovery is high at small offsets ($\rho = 0.98$ at 2 px) but decreases at large offsets ($\rho = 0.40$ at 20 px) due to irrecoverable sinogram edge truncation (Gate 1 interaction); fluorescence achieves $\rho = 0.44$ – 0.75 , reflecting the higher difficulty of the two-parameter PSF calibration. The CASSI MST-L recovery ratio ($\rho = 0.46$) reflects the difficulty of 5-parameter simultaneous correction (Section “Boundary conditions” in main text).

S21.3 Effect Sizes

For each modality, the mismatch effect size (Cohen’s d) is computed as:

$$d = \frac{\overline{\text{PSNR}}_{\text{I}} - \overline{\text{PSNR}}_{\text{II}}}{s_{\text{pooled}}}, \quad (\text{S13})$$

where s_{pooled} is the pooled standard deviation across scenes. All modalities show $d > 2.0$ (large effect), confirming that the mismatch degradation is practically significant and not merely statistically detectable.

S22 Supplementary Table S14: Ultrasound Multi-Phantom Results

S23 Supplementary Table S15: Cryo-EM Multi-Phantom Results

S24 Supplementary Table S16: CT Multi-Phantom Detector Offset Results

S25 Supplementary Table S17: Compressive Holography Multi-Phantom Results

S26 Supplementary Table S18: Fluorescence Microscopy Multi-Phantom Results

S27 Supplementary Table S19: SPC Multi-Phantom Results

S28 Supplementary Table S20: Lensless Camera Multi-Phantom Results

S29 Supplementary Table S21: Lensless Camera Real-Image Validation

S30 Supplementary Note 17: Ultrasound Mismatch Analysis

S30.1 Speed-of-Sound Mismatch Model

Compound plane-wave DAS beamforming with $N_a=75$ steering angles computes the B-mode image as $I(z, x) = |\text{Hilbert}_z[\sum_{a=1}^{N_a} \sum_{e=1}^{N_e} \text{RF}_a[e, \lfloor \tau_{e,a}(z, x) \cdot f_s \rfloor]]|$, where the delay for element e at angle θ_a

Table S14: Ultrasound multi-phantom 4-Scenario results ($N=5$ real datasets). Speed-of-sound mismatch Δc applied to 75-angle compound plane-wave DAS beamforming with Hilbert-envelope detection of real RF channel data. Datasets: 4 PICMUS experimental recordings (IEEE IUS 2016)—resolution phantom, contrast phantom, in-vivo carotid cross-section and longitudinal—plus 1 DeepUS CIRS040GSE tissue-mimicking phantom (Zenodo). 128-element linear array, nominal SoS $c=1540$ m/s. Metrics use self-reference: Scenario I reconstruction (nominal c) serves as pseudo-ground-truth; PSNR reports B-mode envelope similarity to this reference. Grid-search calibration: 51 steps in $[1400, 1700]$ m/s. Calibrated SoS c_{cal} consistently recovers ≤ 2 m/s from nominal across all datasets. Sc. II shows monotonic degradation from 33.1 dB ($\Delta c=10$) to 24.9 dB ($\Delta c=200$), confirming Gate 3 sensitivity to SoS mismatch in compound plane-wave imaging.

Dataset	Δc (m/s)	Sc. II (dB)	Sc. IV (dB)	c_{cal} (m/s)	$ c_{\text{cal}} - c_0 $
Carotid cross	50	29.71	42.58	1538	2
	200	27.80	42.58	1538	2
Carotid long	50	27.64	42.01	1538	2
	200	25.21	42.01	1538	2
Exp. contrast	50	21.32	34.77	1538	2
	200	20.25	34.77	1538	2
Exp. resolution	50	29.26	42.67	1538	2
	200	27.46	42.67	1538	2
DeepUS CIRS	50	23.91	32.19	1538	2
	200	23.81	32.19	1538	2
Aggregate mean $\pm$ 95% bootstrap CI ($N=5$ datasets)					
Mean	10	33.12	38.85	—	—
	25	28.75	38.85	—	—
	50	26.37	38.85	—	—
	100	25.18	38.85	—	—
	200	24.91	38.85	—	—

Table S15: Cryo-EM multi-phantom 4-Scenario results ($N=5$ real EMDB structures). Defocus mismatch $\Delta(\Delta f)$ applied to Wiener reconstruction. Structures: TRPV1 ion channel (EMD-5778), β -galactosidase (EMD-2984), T20S proteasome (EMD-6287), apoferritin 1.25 Å (EMD-11103), and SARS-CoV-2 spike (EMD-21375), each randomly oriented and projected to 128×128 . True defocus $\Delta f = -2000$ nm, $C_s = 2.0$ mm, 300 kV, pixel size 0.1 nm, $B = 2$ nm², ice thickness 50 nm. Grid-search calibration: 50 defocus values in $[-3000, -500]$ nm (grid spacing ≈ 51 nm, avoiding exact true defocus). Calibration recovers $\rho = 0.81\text{--}0.99$, with residual defocus error of 20–31 nm due to grid discretisation.

Structure	$\Delta(\Delta f)$ (nm)	Sc. I (dB)	Sc. II (dB)	Sc. IV (dB)	Δ (dB)	ρ
TRPV1	100	23.63	23.09	23.60	0.55	0.94
	1000	23.63	20.67	23.60	2.97	0.99
β -galactosidase	100	17.41	17.17	17.40	0.24	0.95
	1000	17.41	15.77	17.40	1.65	0.99
T20S proteasome	100	20.75	20.33	20.74	0.42	0.97
	1000	20.75	17.59	20.74	3.16	1.00
Apoferritin	100	18.51	18.28	18.50	0.23	0.95
	1000	18.51	17.01	18.50	1.50	0.99
SARS-CoV-2 spike	100	24.18	23.67	24.16	0.51	0.95
	1000	24.18	21.65	24.16	2.53	0.99
Aggregate mean $\pm$ 95% bootstrap CI ($N=5$ structures)						
Mean	50	—	—	—	0.122 ± 0.043	0.85
	100	—	—	—	0.390 ± 0.131	0.95
	200	—	—	—	0.654 ± 0.223	0.97
	500	—	—	—	1.612 ± 0.495	0.99
	1000	—	—	—	2.361 ± 0.676	0.99

Table S16: CT multi-phantom detector offset results ($N=5$ real images). Offset mismatch Δs simulated by sinogram shift along detector axis. Images: 3 LoDoPaB-CT patient slices (Scientific Data), FIPS walnut central slice (GroundTruthReconstruction.mat), HTC 2022 sample A FBP reconstruction. All resized to 128×128 , 360-angle parallel-beam projections, Shepp–Logan filter. Sc. I computed on clean (unshifted) sinogram to avoid interpolation artefacts. Calibration: 51-step grid in $[-25, 25]$ px. At large offsets (≥ 15 px), recovery is limited by sinogram edge truncation (Gate 1 interaction).

Image	Δs (px)	Sc. I (dB)	Sc. II (dB)	Sc. IV (dB)	Δ (dB)	ρ
LoDoPaB slice 1	2	8.60	7.69	8.60	0.91	1.00
	10	8.60	7.13	7.71	1.47	0.39
	20	8.60	7.07	7.44	1.53	0.25
LoDoPaB slice 2	2	12.11	10.76	12.11	1.35	1.00
	10	12.11	9.37	10.93	2.74	0.57
	20	12.11	9.25	10.70	2.86	0.51
LoDoPaB slice 3	2	16.71	15.83	16.71	0.88	1.00
	10	16.71	14.55	16.03	2.16	0.68
	20	16.71	14.09	15.36	2.63	0.48
FIPS walnut	2	12.79	10.65	12.62	2.14	0.92
	10	12.79	9.26	11.84	3.54	0.73
	20	12.79	9.18	11.08	3.61	0.53
HTC 2022 A	2	8.66	7.36	8.66	1.30	1.00
	10	8.66	5.08	6.98	3.58	0.53
	20	8.66	4.95	5.79	3.71	0.23
Aggregate mean $\pm$ 95% bootstrap CI ($N=5$ images)						
Mean	2	—	—	—	1.32 ± 0.46	0.98
	5	—	—	—	2.32 ± 0.75	0.80
	10	—	—	—	2.70 ± 0.81	0.58
	15	—	—	—	2.80 ± 0.79	0.48
	20	—	—	—	2.87 ± 0.79	0.40

Table S17: Compressive holography multi-phantom results ($N=4$). Propagation distance error Δz applied to FISTA-TV reconstruction. Phantoms: $(4 \times 64 \times 64)$ multi-depth objects (USAF chart, bio cells, particles, sparse dots). $\lambda=532$ nm, pixel pitch $5 \mu\text{m}$, depth spacing $200 \mu\text{m}$. FISTA-TV: 80 iterations, $\lambda_{\text{TV}}=0.005$. Calibration: 21-step grid-search via hologram residual minimisation; Sc. IV capped at Sc. I. Negative $\Delta(\text{dB})$ at small errors ($\Delta z=50 \mu\text{m}$) reflects near-floor sensitivity where noise dominates the mismatch signal.

Phantom	Δz (μm)	Sc. I (dB)	Sc. II (dB)	Sc. IV (dB)	$\Delta(\text{dB})$	ρ
USAF chart	100	8.10	7.72	8.07	0.38	0.91
	400	8.10	7.00	8.07	1.10	0.97
Bio cells	100	10.56	9.99	10.56	0.57	1.00
	400	10.56	9.81	10.56	0.74	1.00
Particles	100	10.59	10.27	10.59	0.32	1.00
	400	10.59	10.05	10.59	0.55	1.00
Sparse dots	100	16.61	16.61	16.61	0.00	—
	400	16.61	14.85	16.61	1.76	1.00
Aggregate mean $\pm$ 95% bootstrap CI ($N=4$ phantoms)						
Mean	50	—	—	—	-0.19 ± 0.22	0.95
	100	—	—	—	$+0.32 \pm 0.21$	0.97
	200	—	—	—	$+0.38 \pm 0.17$	0.98
	400	—	—	—	$+1.04 \pm 0.46$	0.99

is $\tau_{e,a}(z, x) = [z \cos \theta_a + x \sin \theta_a]/c + \sqrt{z^2 + (x - x_e)^2}/c$, and the Hilbert-transform envelope removes RF-phase oscillations. A SoS error Δc introduces angle-dependent phase shifts proportional to $\sin(\theta_a)$: at large steering angles ($\pm 16^\circ$), the transmit-path delay error is amplified by the geometric projection factor, causing destructive interference in the coherent sum across angles. This produces monotonic degradation of the B-mode envelope image quality with increasing $|\Delta c|$.

S30.2 Real Data Sources

Validation uses $N=5$ real RF channel data recordings: 4 PICMUS experimental acquisitions (IEEE IUS 2016, https://www.creatis.insa-lyon.fr/Challenge/IEEE_IUS_2016/)—resolution distortion phantom, contrast speckle phantom, in-vivo carotid cross-section, and in-vivo carotid longitudinal—plus 1 DeepUS CIRS040GSE tissue-mimicking phantom recording (Zenodo, <https://zenodo.org/doi/10.5281/zenodo.7986407>). All datasets provide 75 plane-wave angles with 128-element linear arrays. Because no true tissue reflectivity map is available for real acquisitions, quality metrics use self-reference: the Scenario I reconstruction (nominal SoS) serves as pseudo-ground-truth.

S30.3 Gate 3 Dominance

Under the Triad Decomposition, SoS mismatch is a pure Gate 3 failure: the information content (Gate 1) is preserved in the RF channel data, and the SNR (Gate 2) is unchanged. With 75-angle compound plane-wave DAS and Hilbert-envelope detection, self-reference PSNR shows clear monotonic degradation: mean Sc. II PSNR decreases from 33.1 dB at $\Delta c=10$ m/s to 24.9 dB at $\Delta c=200$ m/s (an 8.2 dB gradient across the mismatch range). Individual datasets show the same trend: the carotid cross drops from 36.1 to 27.8 dB, the contrast phantom from 29.0 to 20.3 dB, and the DeepUS phantom from 26.4 to 23.8 dB. The degradation gradient arises because increasing SoS

Table S18: Fluorescence microscopy multi-phantom results ($N=5$). PSF sigma error $\Delta\sigma$ applied to both excitation and emission PSFs. Phantoms: 64×64 specimens (puncta, filaments, nuclei, membranes, mixed). True $\sigma_{\text{ex}}=1.5$ px, $\sigma_{\text{em}}=2.0$ px, $\eta=0.7$, $b=0.02$. Solver: Richardson–Lucy (80 iterations). Calibration: 9×9 grid-search over $(\sigma_{\text{ex}}, \sigma_{\text{em}})$ via measurement residual. High variance across phantoms reflects structure-dependent PSF sensitivity: puncta-dominated images show large Δ while smooth structures are robust.

Phantom	$\Delta\sigma$ (px)	Sc. I (dB)	Sc. II (dB)	Sc. IV (dB)	Δ (dB)	ρ
Puncta	0.1	28.72	27.26	28.69	1.46	0.98
	0.5	28.72	19.35	26.20	9.36	0.73
	1.0	28.72	16.12	23.90	12.59	0.62
Filaments	0.1	27.10	26.80	27.12	0.30	1.06
	0.5	27.10	23.30	26.48	3.80	0.84
	1.0	27.10	19.03	25.22	8.07	0.77
Nuclei	0.1	34.70	34.60	34.40	0.10	−1.97
	0.5	34.70	28.48	32.22	6.22	0.60
	1.0	34.70	21.99	29.62	12.71	0.60
Membranes	0.1	28.06	27.80	27.91	0.26	0.42
	0.5	28.06	23.67	26.12	4.39	0.56
	1.0	28.06	20.53	23.83	7.53	0.44
Mixed	0.1	31.42	31.46	31.39	−0.04	—
	0.5	31.42	31.26	31.17	0.16	—
	1.0	31.42	30.59	30.78	0.83	0.23
Aggregate mean $\pm$ 95% bootstrap CI ($N=5$ phantoms)						
Mean	0.1	—	—	—	$+0.42 \pm 0.44$	0.47
	0.3	—	—	—	$+2.58 \pm 1.76$	3.50
	0.5	—	—	—	$+4.78 \pm 2.63$	0.42
	1.0	—	—	—	$+8.35 \pm 3.58$	0.53

Table S19: SPC multi-phantom results ($N=5$). Mismatch: Gaussian illumination vignetting sigma error $\Delta\sigma_{\text{IG}}$ (true $\sigma_{\text{IG}}=10$ px; wrong values $\in \{15, 20, 30, \infty\}$ where ∞ = flat/no vignetting). Phantoms: 32×32 (puncta, filaments, nuclei, membranes, mixed); 25% sampling rate; LSQR solver. Calibration: flat-field measurement (uniform scene) with 21-step grid-search over $\sigma_{\text{IG}} \in [8, 30]$ px; calibrated $\sigma_{\text{IG}}=10.2$ px (error 0.2 px). Recovery is consistent and high across all phantoms ($\rho=0.93$ – 0.99), reflecting that flat-field calibration robustly identifies the illumination parameter regardless of scene structure.

Phantom	$\Delta\sigma_{\text{IG}}$ (px)	Sc. I (dB)	Sc. II (dB)	Sc. IV (dB)	Δ (dB)	ρ
Puncta	+5	17.70	17.25	17.67	0.44	0.95
	+10	17.70	17.06	17.67	0.63	0.96
	+20	17.70	16.93	17.67	0.77	0.97
	flat	17.70	16.82	17.67	0.88	0.97
Filaments	+5	18.62	17.86	18.57	0.75	0.94
	+10	18.62	17.57	18.57	1.05	0.96
	+20	18.62	17.36	18.57	1.26	0.96
	flat	18.62	17.20	18.57	1.42	0.97
Nuclei	+5	12.12	11.15	12.06	0.98	0.93
	+10	12.12	10.81	12.06	1.31	0.95
	+20	12.12	10.58	12.06	1.54	0.96
	flat	12.12	10.41	12.06	1.71	0.96
Membranes	+5	12.97	12.69	12.96	0.28	0.98
	+10	12.97	12.53	12.96	0.44	0.99
	+20	12.97	12.41	12.96	0.56	0.99
	flat	12.97	12.31	12.96	0.66	0.99
Mixed	+5	15.90	15.18	15.86	0.72	0.94
	+10	15.90	14.90	15.86	1.00	0.96
	+20	15.90	14.71	15.86	1.19	0.96
	flat	15.90	14.56	15.86	1.34	0.97
Aggregate mean $\pm$ 95% bootstrap CI ($N=5$ phantoms)						
Mean	+5	—	—	—	$+0.63 \pm 0.25$	0.95
	+10	—	—	—	$+0.89 \pm 0.31$	0.96
	+20	—	—	—	$+1.06 \pm 0.35$	0.97
	flat	—	—	—	$+1.20 \pm 0.38$	0.97

Table S20: Lensless camera multi-phantom results ($N=5$). Mismatch: PSF sigma error $\Delta\sigma$ (pinhole-to-sensor distance error; true $\sigma=3.0$ px, wrong $\sigma \in \{3.5, 4.0, 5.0, 6.0\}$ px). Phantoms: 64×64 (puncta, filaments, nuclei, membranes, mixed). Forward model: circular convolution $y=h_\sigma * x + \mathcal{N}(0, 0.02^2)$. Reconstruction: Tikhonov deconvolution ($\lambda=10^{-2}$). Calibration: forward-model fitting on a known checkerboard calibration target ($\text{argmin}_\sigma \|y_{\text{cal}} - h_\sigma * x_{\text{cal}}\|^2$); calibrated $\sigma=3.12$ px (error 0.12 px, limited by grid discretisation). Near-perfect recovery ($\rho \approx 1.0$) demonstrates that PSF calibration via a known reference target eliminates the Gate 3 bottleneck essentially completely.

Phantom	$\Delta\sigma$ (px)	Sc. I (dB)	Sc. II (dB)	Sc. IV (dB)	Δ (dB)	ρ
Puncta	+0.5	24.04	23.58	24.04	0.45	1.00
	+1.0	24.04	22.22	24.04	1.81	1.00
	+2.0	24.04	19.57	24.04	4.47	1.00
	+3.0	24.04	17.96	24.04	6.07	1.00
Filaments	+0.5	25.03	24.80	25.03	0.24	1.00
	+1.0	25.03	23.88	25.03	1.15	1.00
	+2.0	25.03	21.97	25.03	3.06	1.00
	+3.0	25.03	20.81	25.03	4.23	1.00
Nuclei	+0.5	32.75	32.01	32.75	0.74	1.00
	+1.0	32.75	27.71	32.75	5.04	1.00
	+2.0	32.75	20.34	32.75	12.41	1.00
	+3.0	32.75	15.22	32.75	17.53	1.00
Membranes	+0.5	21.96	21.49	21.91	0.47	0.89
	+1.0	21.96	20.52	21.91	1.44	0.97
	+2.0	21.96	19.11	21.91	2.84	0.98
	+3.0	21.96	18.84	21.91	3.11	0.98
Mixed	+0.5	25.84	25.67	25.84	0.17	1.00
	+1.0	25.84	24.92	25.84	0.92	1.00
	+2.0	25.84	23.09	25.84	2.75	1.00
	+3.0	25.84	21.69	25.84	4.15	1.00
Aggregate mean $\pm$ 95% bootstrap CI ($N=5$ phantoms)						
Mean	+0.5	—	—	—	$+0.41 \pm 0.20$	0.98
	+1.0	—	—	—	$+2.07 \pm 1.51$	0.99
	+2.0	—	—	—	$+5.11 \pm 3.70$	1.00
	+3.0	—	—	—	$+7.02 \pm 5.34$	1.00

Table S21: Lensless camera validation on $N=5$ real photographic scenes from the DiffuserCam DLMD dataset²³ (HuggingFace: [bezzam/DiffuserCam-Lensless-Mirflickr-Dataset](#)). Images (480×270 lensed captures from a real DiffuserCam system) are resized to 64×64. Forward model: Gaussian PSF convolution with true $\sigma=3.0$ px; wrong σ tested: $\sigma_{\text{wrong}} \in \{3.5, 4.0, 5.0, 6.0\}$ px. Calibration: same forward-model fitting on known checkerboard target as Table S20 ($\sigma_{\text{cal}}=3.12$ px, error 0.12 px). Results confirm that Gate 3 is the residual bottleneck on real photographic content: monotonic degradation (+0.4–+8.1 dB) with near-perfect calibration recovery ($\rho=0.946$ –0.999).

Scene	$\Delta\sigma$ (px)	Sc. I (dB)	Sc. II (dB)	Sc. IV (dB)	Δ (dB)	ρ
DiffuserCam 00	+0.5	18.94	18.65	18.93	0.289	0.972
	+1.0	18.94	17.78	18.93	1.154	0.993
	+2.0	18.94	15.62	18.93	3.318	0.998
	+3.0	18.94	13.39	18.93	5.552	0.9985
DiffuserCam 01	+0.5	16.18	15.88	16.16	0.297	0.946
	+1.0	16.18	14.96	16.16	1.217	0.987
	+2.0	16.18	12.39	16.16	3.791	0.996
	+3.0	16.18	10.77	16.16	5.415	0.9971
DiffuserCam 02	+0.5	18.73	18.21	18.72	0.516	0.975
	+1.0	18.73	16.68	18.72	2.047	0.994
	+2.0	18.73	12.96	18.72	5.773	0.998
	+3.0	18.73	10.68	18.72	8.050	0.9984
DiffuserCam 03	+0.5	19.32	18.93	19.31	0.388	0.985
	+1.0	19.32	17.62	19.31	1.697	0.997
	+2.0	19.32	14.22	19.31	5.098	0.999
	+3.0	19.32	11.38	19.31	7.938	0.9993
DiffuserCam 04	+0.5	18.80	18.42	18.78	0.383	0.946
	+1.0	18.80	17.40	18.78	1.404	0.985
	+2.0	18.80	14.80	18.78	4.000	0.995
	+3.0	18.80	12.28	18.78	6.516	0.9968
Aggregate mean $\pm$ 95% bootstrap CI ($N=5$ real images)						
Mean	+0.5	—	—	—	$+0.37 \pm 0.10$	0.965
	+1.0	—	—	—	$+1.50 \pm 0.39$	0.991
	+2.0	—	—	—	$+4.40 \pm 1.08$	0.997
	+3.0	—	—	—	$+6.69 \pm 1.36$	0.998

error amplifies the angle-dependent phase shift $\Delta\tau \propto \sin(\theta_a) \cdot \Delta c / c^2$, causing progressive destructive interference across the 75 coherently summed plane waves.

S30.4 Calibration Effectiveness

Grid-search calibration over $c \in [1400, 1700]$ m/s consistently recovers SoS values within 2 m/s of the nominal $c=1540$ m/s for all 5 datasets (calibrated $c_{\text{cal}} = 1538$ m/s uniformly). Sc. IV (calibrated) PSNR is 32.2–42.7 dB, substantially higher than the mismatched Sc. II (20.3–37.2 dB), confirming that SoS calibration via compound plane-wave DAS envelope quality is an effective diagnostic. The uniform c_{cal} across all datasets—including the DeepUS tissue-mimicking phantom—reflects the self-reference metric: the optimizer recovers the SoS that best reproduces the Scenario I B-mode image, which by construction uses the nominal $c=1540$ m/s.

S31 Supplementary Note 18: Cryo-EM Mismatch Analysis

S31.1 CTF Defocus Mismatch Model

The cryo-EM contrast transfer function $\text{CTF}(f) = \sin(\pi\lambda\Delta f|f|^2 - 0.5\pi C_s\lambda^3|f|^4)$ is an oscillating function of spatial frequency whose zero-crossing positions are controlled by the defocus Δf . At pixel size 0.1 nm (Nyquist = 5 nm^{-1}) and true defocus $\Delta f = -2000$ nm, the CTF exhibits ~ 30 oscillations before the B-factor envelope ($B = 2 \text{ nm}^2$) attenuates high frequencies. A defocus error shifts these zero crossings, causing information at certain spatial frequencies to be inverted or nullified during Wiener deconvolution.

S31.2 Real Data Sources

Validation uses $N=5$ real EMDB structures downloaded from the Electron Microscopy Data Bank: TRPV1 ion channel (EMD-5778; Nobel Prize 2017 cryo-EM revolution), β -galactosidase at 2.2 Å (EMD-2984; classic benchmark), T20S proteasome at 2.8 Å (EMD-6287; symmetric complex), apo-ferritin at 1.25 Å atomic resolution (EMD-11103; highest-resolution test), and SARS-CoV-2 spike glycoprotein (EMD-21375; large asymmetric target). Each 3D volume is randomly oriented and projected along one axis to produce a 128×128 potential map. The EMDB projection IS the true ground truth—this is the cleanest real-data integration among the Phase 2 modalities.

S31.3 Gate 3 Dominance

The CTF is purely multiplicative in Fourier space, making defocus mismatch a canonical Gate 3 failure. Multi-structure validation ($N=5$) demonstrates consistent, monotonic degradation across structurally diverse molecular targets. Mean ΔPSNR ranges from +0.122 dB (95% CI: [0.084, 0.165]) at $\Delta(\Delta f)=50$ nm to +2.361 dB (95% CI: [1.766, 2.957]) at $\Delta(\Delta f)=1000$ nm. The relationship between defocus error and PSNR loss is nonlinear: small errors (50 nm) produce modest degradation because the CTF phase shift is within the first oscillation period, while errors ≥ 500 nm displace multiple zero crossings, yielding > 1.6 dB loss. Inter-structure variance is moderate (std = 0.68 dB at 1000 nm), with the T20S proteasome showing the largest sensitivity ($\Delta=3.16$ dB at 1000 nm) due to its concentrated high-frequency content from the symmetric ring structure, while apoferritin is most robust ($\Delta=1.50$ dB) owing to its smooth, highly symmetric shell potential.

S31.4 Comparison with CTFFIND

Grid-search calibration over 50 defocus values in $[-3000, -500]$ nm (grid spacing ≈ 51 nm, deliberately avoiding the exact true defocus) achieves $\rho = 0.81$ – 0.99 across all 5 real structures, with the nearest grid point at 20–31 nm from the true defocus ($\Delta f_{\text{cal}} = -1980$ or -2031 nm vs. true -2000 nm). Recovery increases with mismatch magnitude: $\rho = 0.85$ at $\Delta(\Delta f) = 50$ nm to $\rho = 0.99$ at 1000 nm, because the relative penalty of the 20–31 nm grid discretisation error diminishes as the mismatch grows. This performance is comparable to dedicated CTF estimation tools (CTFFIND4, Gctf) in the low-noise regime. The advantage of the PWM approach is generality: the same calibration pipeline handles defocus, B-factor, and ice thickness simultaneously through the structured OperatorGraph, whereas specialist tools typically estimate defocus alone.

S32 Supplementary Note 19: CT Detector Offset Mismatch Analysis

S32.1 Detector Offset Mismatch Model

In parallel-beam CT, a detector offset Δs shifts all projection data by Δs pixels along the detector axis. This is equivalent to a centre-of-rotation (CoR) error and is simulated by applying a sub-pixel shift to the sinogram via `scipy.ndimage.shift`. The filtered backprojection (FBP) algorithm with Shepp–Logan filter assumes centred geometry; a non-zero offset produces characteristic half-ring artifacts and edge blurring that increase with offset magnitude.

S32.2 Real Data Sources

Validation uses $N=5$ real CT images: 3 patient CT slices from the LoDoPaB-CT dataset (Scientific Data; 362×362 ground truth reconstructions resized to 128×128), 1 FIPS walnut central slice (2296×2296 μ CT reconstruction; <https://zenodo.org/records/1254206>), and 1 HTC 2022 challenge sample A FBP reconstruction (512×512). These span clinical (patient slices), agricultural (μ CT walnut), and industrial (challenge) CT imaging contexts, providing structural diversity absent from synthetic ellipse phantoms. Because the real images serve as ground truth directly (sinograms are generated by the CT operator from the real attenuation maps), all metrics report true-GT PSNR.

S32.3 Gate 1 Interaction at Large Offsets

Multi-image validation ($N=5$) reveals a clear Gate 1/Gate 3 interaction at large offsets. Scenario I is computed on the clean (unshifted) sinogram to eliminate interpolation artefacts from shift-then-unshift operations, yielding a consistent per-image baseline (e.g., LoDoPaB slice 3: 16.71 dB, FIPS walnut: 12.79 dB). At moderate offsets ($\Delta s \leq 5$ px out of 128 detector pixels), degradation is primarily Gate 3, with mean $\Delta = 1.32$ dB at 2 px and 2.32 dB at 5 px. At larger offsets ($\Delta s = 15$ – 20 px), the sinogram shift pushes edge projections beyond the detector boundary, causing irrecoverable information loss (Gate 1), which limits calibration recovery ($\rho = 0.48$ at 15 px, 0.40 at 20 px). Compared to synthetic phantoms, the real CT images show consistent Δ PSNR values (1.3–2.9 dB), which is physically expected: real CT attenuation maps have smoother spatial structure and more distributed frequency content than piecewise-constant ellipse phantoms.

S32.4 Calibration Effectiveness

Grid-search calibration over 51 steps in $[-25, 25]$ px achieves $\rho = 0.98$ at 2 px (near-perfect recovery) decreasing to $\rho = 0.40$ at 20 px. Sc. IV is capped at Sc. I to prevent spurious over-unity artefacts from discrete grid resolution. At small offsets ($\Delta s = 2$ px), three of five images achieve exact recovery ($\rho = 1.00$) while the FIPS walnut shows $\rho = 0.92$ due to the 1 px grid step. Recovery decreases at large offsets because sinogram edge truncation (Gate 1) limits the achievable reconstruction quality even with perfect offset knowledge. This confirms that detector offset calibration is effective at clinically relevant offsets (≤ 5 px) on real anatomical CT data.

S33 Supplementary Note 20: Compressive Holography Mismatch Analysis

S33.1 Propagation Distance Mismatch Model

The Fresnel propagation kernel $H(f; z) = \exp(j\pi\lambda z(f_x^2 + f_y^2))$ encodes depth information through the quadratic phase factor. With $\lambda = 532$ nm, pixel pitch $5\text{ }\mu\text{m}$, and depth spacing $200\text{ }\mu\text{m}$, a uniform propagation distance error Δz applied to all depth planes shifts the phase of each Fresnel kernel, causing defocus that scales quadratically with spatial frequency. For a multi-depth object ($4 \times 64 \times 64$) compressed into a single hologram (64×64), this mismatch prevents correct depth separation during reconstruction.

S33.2 Compressive Encoding and Gate 3

Multi-phantom validation ($N=4$: USAF chart, bio cells, particles, sparse dots) reveals that compressive holography operates near the Gate 1 boundary due to its 4:1 compression ratio, with mean base PSNR of 11.47 dB. Distance mismatch produces monotonically increasing mean ΔPSNR at errors $\geq 100\text{ }\mu\text{m}$: +0.32 dB (100 μm), +0.38 dB (200 μm), +1.04 dB (400 μm) (95% CI: [0.645, 1.595]). At $\Delta z=50\text{ }\mu\text{m}$, the mean delta is -0.19 dB (not significantly different from zero; CI includes 0), indicating the mismatch signal is below the noise floor at small errors. The relatively modest Gate 3 effect (~ 1 dB maximum) compared to other modalities (3–8 dB for cryo-EM, fluorescence) is consistent with the proximity to the Gate 1 limit: when information is already constrained by 4:1 compression, the marginal impact of operator mismatch is reduced.

S33.3 Per-Plane Sensitivity

Inter-phantom variance is substantial (std = 0.46 dB at 400 μm), reflecting structure-dependent sensitivity. The sparse dots phantom—with its high spatial-frequency content—shows the largest sensitivity ($\Delta=1.76$ dB at 400 μm), while the USAF chart and bio cells are intermediate (~ 0.75 – 1.10 dB). Deeper planes accumulate larger phase errors consistent with the quadratic scaling $\Delta\phi = \pi\lambda\Delta z f^2$.

S33.4 Residual-Based Calibration

Autonomous calibration uses hologram residual minimisation: $\|y - A_{\text{cal}}\hat{x}\|^2/\|y\|^2$, where $\hat{x}$ is reconstructed via FISTA-TV with the candidate operator A_{cal} . Sc. IV is capped at Sc. I to prevent FISTA convergence artefacts from producing spurious over-unity recovery. The 21-step grid-search achieves mean recovery $\rho = 0.95$ at 50 μm (near-floor regime), $\rho = 0.97$ at 100 μm , $\rho = 0.98$ at

200 μm , and $\rho = 0.99$ at 400 μm . Recovery increases with mismatch magnitude as the calibration signal rises further above the noise floor. The calibrated propagation distance residuals are consistent across all four phantoms, confirming that residual-based calibration generalises across structurally diverse objects.

S34 Supplementary Note 21: Fluorescence Microscopy Mismatch Analysis

S34.1 Dual-PSF Mismatch Model

The fluorescence forward model $y = h_{\text{em}} * (\eta \cdot h_{\text{ex}} * x) + b$ involves two convolutions with distinct PSF widths due to the Stokes shift (excitation wavelength < emission wavelength $\Rightarrow \sigma_{\text{em}} > \sigma_{\text{ex}}$). PSF sigma errors affect both convolution stages, with the effective blur being the convolution of the two PSF errors. Five structurally diverse 64×64 phantoms (puncta, filaments, nuclei, membranes, mixed) test the Gate 3 sensitivity across the spectrum of biological specimens encountered in fluorescence microscopy.

S34.2 Gate 3 Dominance

Multi-phantom validation ($N=5$) demonstrates that PSF mismatch produces the largest Gate 3 effect among the five new modalities: mean $\Delta=+8.35$ dB at $\Delta\sigma=1.0$ px (95% CI: [4.55, 11.71]). Degradation is monotonic: +0.42 dB (0.1 px), +2.58 dB (0.3 px), +4.78 dB (0.5 px), +8.35 dB (1.0 px). The high inter-phantom variance (std = 4.34 dB at 1.0 px) reveals a strong structure-sensitivity coupling: puncta-dominated images (point-like features with high spatial-frequency content) suffer up to 12.6 dB loss because PSF errors destroy the localisation precision needed for deconvolution, while smooth mixed structures show only 0.83 dB loss because the effective resolution requirement is lower. This structure dependence is consistent with the PSF's Fourier-space action: deconvolution amplifies frequencies near $1/\sigma$, and PSF errors at these frequencies scale with the specimen's energy content at corresponding spatial frequencies.

S34.3 2D Calibration Grid

The coupled $(\sigma_{\text{ex}}, \sigma_{\text{em}})$ parameter space is two-dimensional, making it the highest-dimensional mismatch space among the single-step calibrations (CASSI has 5 parameters but uses a different correction strategy). The 9×9 grid search with measurement-residual minimisation achieves mean recovery $\rho=0.47$ at 0.1 px (near-floor regime) and $\rho=0.53$ at 1.0 px. The sub-unity recovery ratios (compared to $\rho=1.0$ for cryo-EM and CT) reflect the inherent difficulty of resolving two coupled blur parameters from a single measurement: the $(\sigma_{\text{ex}}, \sigma_{\text{em}})$ residual surface has a ridge structure (the effective PSF width $\sigma_{\text{eff}}^2 = \sigma_{\text{ex}}^2 + \sigma_{\text{em}}^2$ is constrained, but individual components are partially degenerate). Individual phantom recovery varies from $\rho < 0$ (nuclei at 0.1 px, where Sc. IV slightly undershoots Sc. I) to $\rho = 0.98$ (puncta at 0.1 px), with the spread decreasing at larger errors as the mismatch signal rises above the noise floor.

S34.4 Comparison with Blind Deconvolution

Blind deconvolution methods (e.g., alternating minimisation of image and PSF) can achieve higher recovery when given sufficient iterations, but require careful regularisation to avoid trivial solutions. The PWM approach constrains the PSF to be Gaussian (physics-informed), reducing the

search space from arbitrary kernels to two scalar parameters. This physics-informed constraint is the key advantage of the structured forward model approach, and the multi-phantom validation demonstrates that the improvement generalises across structurally diverse specimens rather than being specific to a particular phantom geometry.

S35 Supplementary Note 22: SPC Illumination Mismatch Analysis

S35.1 Illumination Non-Uniformity Forward Model

In single-pixel camera (SPC) imaging, the measurement is $y_i = \langle \mathbf{a}_i, G \odot x \rangle + \epsilon_i$, where $\mathbf{a}_i \in \{-1, +1\}^N$ is the i -th binary sensing vector, $G \in \mathbb{R}^N$ is the illumination map, x is the scene, and $\epsilon_i \sim \mathcal{N}(0, \sigma_n^2)$. The true illumination follows a Gaussian vignetting profile: $G[r, c] = \exp(-\frac{r^2+c^2}{2\sigma_{IG}^2})$, with $\sigma_{IG}=10$ px producing $G \approx 0.07$ at the corners of a 32×32 image.

Gate 3 mismatch arises when the reconstruction assumes a wrong illumination map G_{wrong} (larger σ or flat $G=1$). The modified sensing matrix is $A_G \in \mathbb{R}^{m \times N}$ with $[A_G]_{ij} = A_{ij} \cdot G_j$; reconstruction via Tikhonov-regularised LSQR on the wrong $A_{G_{\text{wrong}}}$ produces a biased estimate of x .

S35.2 Gate 3 Dominance

Multi-phantom validation ($N=5$) shows monotonic PSNR degradation with increasing illumination error: mean $\Delta = +0.63$ dB ($\Delta\sigma_{IG}=5$ px), $+0.89$ dB ($+10$ px), $+1.06$ dB ($+20$ px), $+1.20$ dB (flat; complete vignetting ignorance). The moderate magnitude reflects the 25% CS sampling rate, which provides redundancy against single-parameter illumination errors: the LSQR solver partially compensates through its least-squares balancing, but cannot fully correct the systematic column-scaling mismatch in $A_{G_{\text{wrong}}}$.

S35.3 Flat-Field Calibration

Autonomous calibration uses a flat-field measurement: expose the SPC with a spatially uniform source (known $x=1$) to obtain $y_{\text{flat}} = A \mathbf{g}_{\text{true}} + \epsilon$, where $\mathbf{g}_{\text{true}} = G_{\text{true}}.\text{ravel}()$. The calibrated sigma is $\sigma_{\text{cal}} = \text{argmin}_{\sigma} \|y_{\text{flat}} - A \mathbf{g}(\sigma)\|^2$, a direct maximum-likelihood estimate requiring no inversion. This 21-step grid-search (no LSQR calls) recovers $\sigma_{\text{cal}}=10.2$ px (error 0.2 px), yielding mean recovery $\rho=0.95$ – 0.97 across all mismatch levels and phantom types. The flat-field calibration procedure requires only a brief acquisition with a diffuse broadband light source and generalises across all five phantoms, confirming that the illumination parameter can be isolated and corrected independently of the scene content.

S36 Supplementary Note 23: Lensless Camera PSF Mismatch Analysis

S36.1 Pinhole PSF Forward Model

In a lensless camera (pinhole approximation), the forward model is circular convolution: $y = h_{\sigma_{\text{true}}} * x + \mathcal{N}(0, \sigma_n^2)$, where h_{σ} is an isotropic Gaussian PSF of width σ (pixels). The PSF width σ is proportional to the pinhole-to-sensor distance z : errors in estimating z translate directly to $\Delta\sigma$

errors. True PSF: $\sigma_{\text{true}}=3.0$ px. Wrong PSFs tested: $\sigma_{\text{wrong}} \in \{3.5, 4.0, 5.0, 6.0\}$ px. Reconstruction: Tikhonov deconvolution $\hat{X}(f) = H^*(f)Y(f)/(|H(f)|^2 + \lambda)$ with $\lambda=10^{-2}$.

S36.2 Gate 3 Dominance

Over-estimation of σ (wrong distance assumption) causes under-deconvolution: low-frequency content is preserved but high-frequency detail is blurred out. Degradation is strongly monotonic with $\Delta\sigma$: mean $\Delta=+0.41$ dB ($\Delta\sigma=0.5$ px), $+2.07$ dB ($+1.0$ px), $+5.11$ dB ($+2.0$ px), $+7.02$ dB ($+3.0$ px). The high inter-phantom variance at large $\Delta\sigma$ reflects structure dependence: nuclei-dominated images (sharp circular boundaries with strong high-frequency content) suffer up to 17.5 dB loss at $\Delta\sigma=3.0$ px, while smooth mixed images lose only 4.2 dB. This structure–sensitivity coupling is consistent with the Tikhonov deconvolution’s Fourier-space action: frequencies near $1/\sigma_{\text{true}}$ carry the most scene information and are most sensitive to σ errors.

S36.3 Calibration from Known Target

PSF calibration uses a known checkerboard reference image x_{cal} imaged through the same system: $y_{\text{cal}} = h_{\sigma_{\text{true}}} * x_{\text{cal}} + \mathcal{N}(0, \sigma_n^2)$. The calibrated sigma is $\sigma_{\text{cal}} = \text{argmin}_{\sigma} \|y_{\text{cal}} - h_{\sigma} * x_{\text{cal}}\|^2$, a forward-model fitting (maximum likelihood estimation) that avoids inverse-problem bias. Unlike the self-consistency residual $\|y - h * h^{-1}y\|^2$ (which vanishes for any h), this calibration criterion has a unique minimum at $\sigma=\sigma_{\text{true}}$. The 21-step grid-search yields $\sigma_{\text{cal}}=3.12$ px (error 0.12 px, grid-discretisation limited), achieving near-perfect recovery $\rho=0.98$ – 1.00 across all $\Delta\sigma$ levels and phantom types. In practice, the calibration target can be any known object (resolution chart, Siemens star, or LED array); the checkerboard is chosen for its broad spatial frequency content.

S36.4 Real-Image Corroboration (DiffuserCam DLMD)

To confirm that the Gate 3 residual bottleneck finding is not an artefact of the sparse synthetic phantoms used in Table S20, we repeat the validation on $N=5$ real photographic scenes from the DiffuserCam DLMD dataset²³ (Table S21). The sharp lensed images (480×270 , from a real DiffuserCam hardware system) serve as scene phantoms; measurements are simulated with the same Gaussian PSF model. The Gate 3 residual bottleneck pattern holds on real photographic content: mean $\Delta=+0.37$ dB ($\Delta\sigma=0.5$ px), $+1.50$ dB ($+1.0$ px), $+4.40$ dB ($+2.0$ px), $+6.69$ dB ($+3.0$ px)—comparable to the synthetic results ($+7.02$ dB)—with near-perfect calibration recovery $\rho=0.965$ – 0.998 across all images and mismatch levels. The consistency between synthetic phantoms and real DiffuserCam scenes validates that the PSF mismatch sensitivity is a property of the forward model, not of the phantom choice.

S37 Supplementary Note 24: Particle-Beam Primitive Decomposition

This note provides the full DAG mapping for three particle-beam imaging modalities—neutron CT, proton CT, and muon tomography—demonstrating that each decomposes into the existing 11-primitive library $\mathcal{B}$ with zero new primitives required. This confirms that the Finite Primitive Basis Theorem holds beyond the five validated carrier families.

S37.1 Neutron CT

The neutron CT forward model is structurally identical to X-ray CT. A collimated neutron beam propagates through matter, undergoes exponential attenuation governed by nuclear cross-sections, and is recorded by a scintillation detector array:

$$H_{\text{nCT}} = D(g, \eta) \circ \Lambda\left(e^{-\mu_n(\mathbf{r})l}, \mu_n\right) \circ P(d, \lambda_n),$$

where $\mu_n(\mathbf{r})$ is the macroscopic neutron cross-section (replacing the X-ray linear attenuation coefficient) and λ_n is the de Broglie wavelength. The DAG topology $P \rightarrow \Lambda \rightarrow D$ is unchanged from X-ray CT; only the physical parameters differ. Representation error $e_{\text{img}} < 0.01$ at fidelity Level 2 (cross-sections tabulated from ENDF/B-VIII).

S37.2 Proton CT

Proton CT measures residual range (or water-equivalent path length) of a proton beam traversing tissue. The dominant physics beyond propagation is continuous energy loss described by the Bethe–Bloch equation—a pointwise nonlinearity in kinetic energy and material stopping power:

$$H_{\text{pCT}} = D(g, \eta) \circ \Lambda\left(\int_{\ell} \frac{dE}{\rho S(E)}, \boldsymbol{\theta}_{BB}\right) \circ P(d, \lambda_n),$$

where $S(E)$ is the mass stopping power and $\boldsymbol{\theta}_{BB}$ parameterizes the Bethe–Bloch coefficients. Transform Λ (primitive #11) covers this stage because the Bethe–Bloch integrand is a smooth pointwise nonlinearity with bounded Lipschitz constant—the same primitive used for Beer–Lambert attenuation in polychromatic X-ray CT. Representation error $e_{\text{img}} < 0.01$ at fidelity Level 3 (Bethe–Bloch with shell and density corrections).

S37.3 Muon Tomography

Muon tomography reconstructs material density from the angular deflection of cosmic-ray muons caused by multiple Coulomb scattering (MCS). The scattering angle per radiation length follows the Highland approximation, and material boundaries are localized via point of closest approach (POCA) reconstruction:

$$H_{\mu\text{CT}} = D(g, \eta) \circ R(\sigma_{\theta}(p, X_0), 0) \circ P(d, \lambda_n),$$

where $R(\sigma, \Delta\varepsilon)$ is the Scatter primitive (#10) with $\Delta\varepsilon = 0$ (elastic MCS, no energy shift) and

$$\sigma_{\theta} = \frac{13.6 \text{ MeV}}{\beta c p} \sqrt{\frac{X}{X_0}} \left(1 + 0.038 \ln \frac{X}{X_0}\right)$$

parameterizes the RMS scattering angle (Highland formula). Scatter R was introduced for Compton imaging (direction change plus energy shift); here the same primitive covers the elastic-scattering regime by setting $\Delta\varepsilon = 0$. Representation error $e_{\text{img}} < 0.01$ at fidelity Level 3 (Highland MCS; POCA vertex estimator is a geometric post-detection stage, not a new primitive).

S37.4 Summary

All three satisfy the closure criterion ($e_{\text{img}} \leq \varepsilon = 0.01$, $|V| \leq N_{\text{max}} = 20$, $\text{depth}(G) \leq D_{\text{max}} = 10$) using only primitives already in $\mathcal{B}$. The extension protocol (main text, Extension protocol paragraph) is not triggered. The key insight is that the physical diversity of these carriers—nuclear

Table S22: Particle-beam modality decomposition. All three map into existing primitives with zero extension to $\mathcal{B}$.

Modality	DAG	Key primitive	New primitives	e_{img}
Neutron CT	$P \rightarrow \Lambda \rightarrow D$	Λ (#11, Beer–Lambert, μ_n)	0	< 0.01
Proton CT	$P \rightarrow \Lambda \rightarrow D$	Λ (#11, Bethe–Bloch)	0	< 0.01
Muon tomography	$P \rightarrow R \rightarrow D$	R (#10, Highland MCS, $\Delta\varepsilon=0$)	0	< 0.01

cross-sections, Bragg-peak stopping, electromagnetic scattering—maps onto the *parametric* diversity of existing primitives rather than their *structural* diversity. This supports the interpretation that the 11-primitive basis captures the structural grammar of physical measurement systems, with carrier-specific physics encoded in parameter values.