



Source Preprocessing Quality Control


(A) CoronaCases
coronacases_003 | z = 81 | Selection

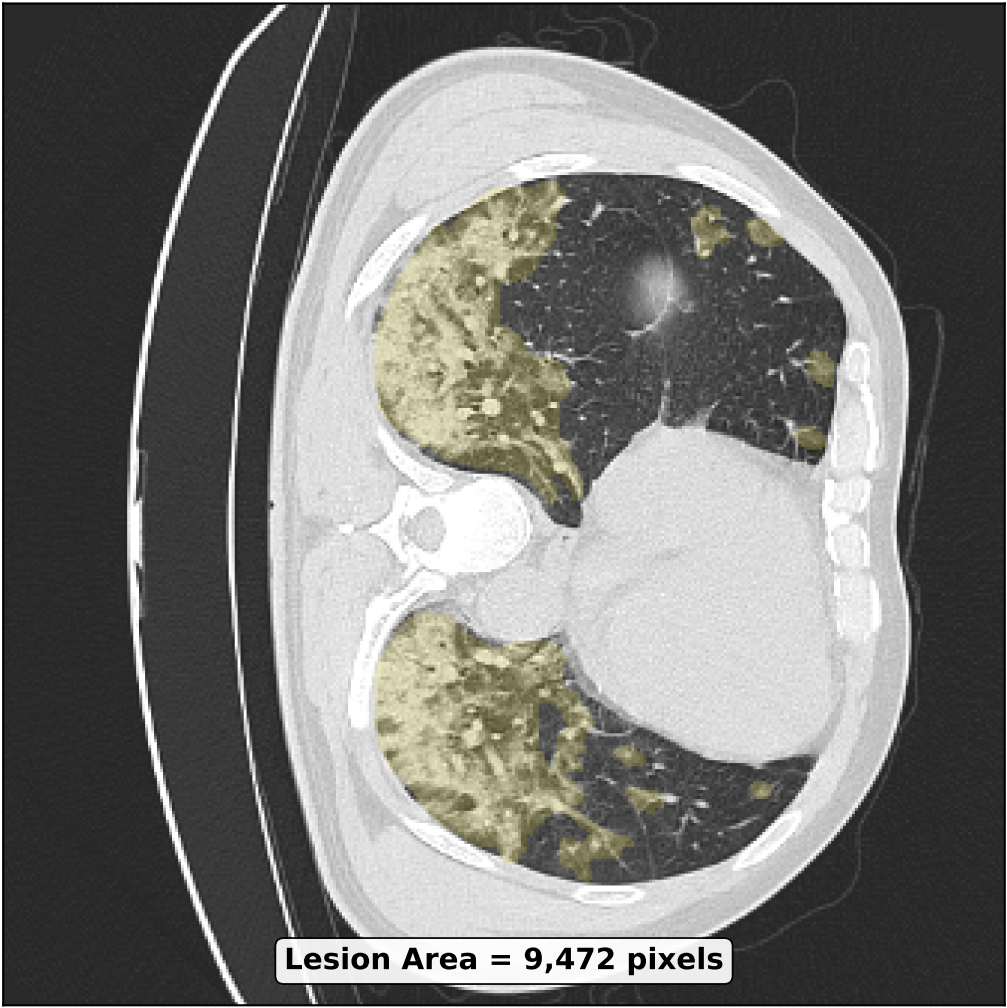

(B) CoronaCases
coronacases_010 | z = 121 | Selection

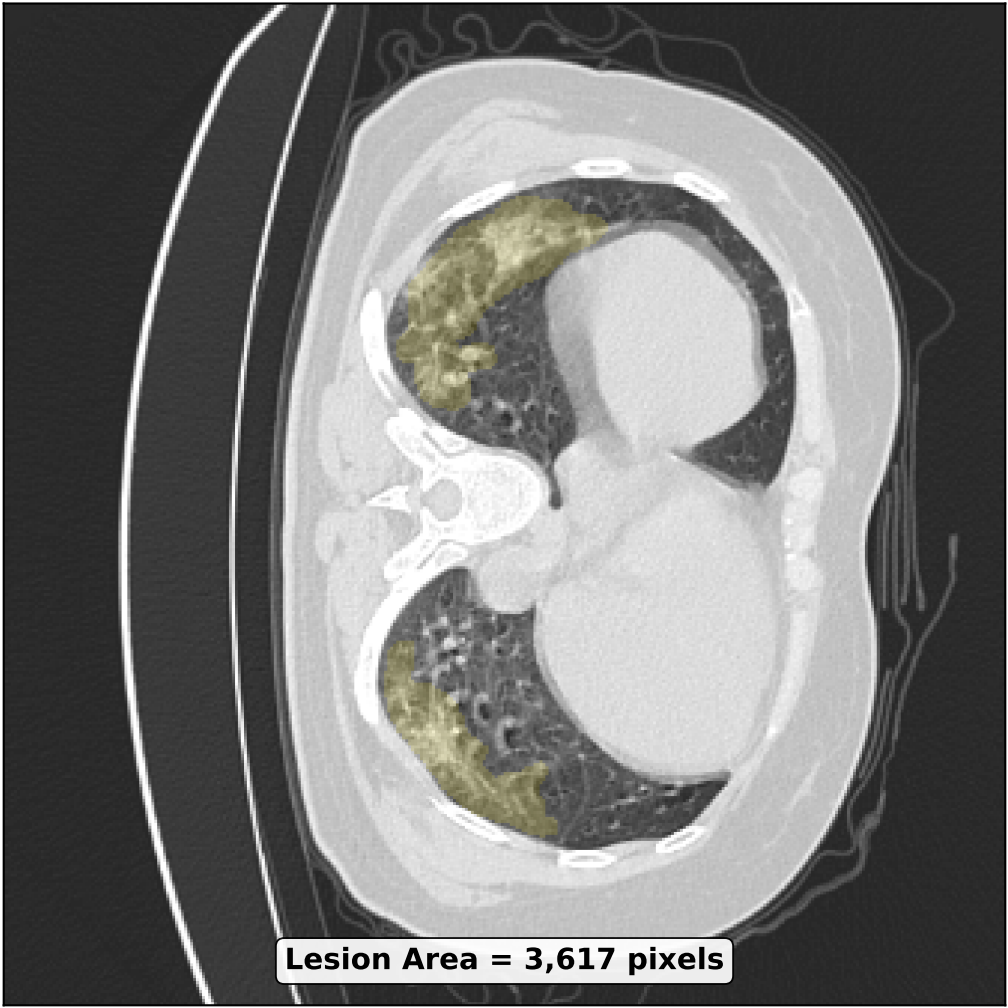


(C) CoronaCases
coronacases_006 | z = 71 | Calibration

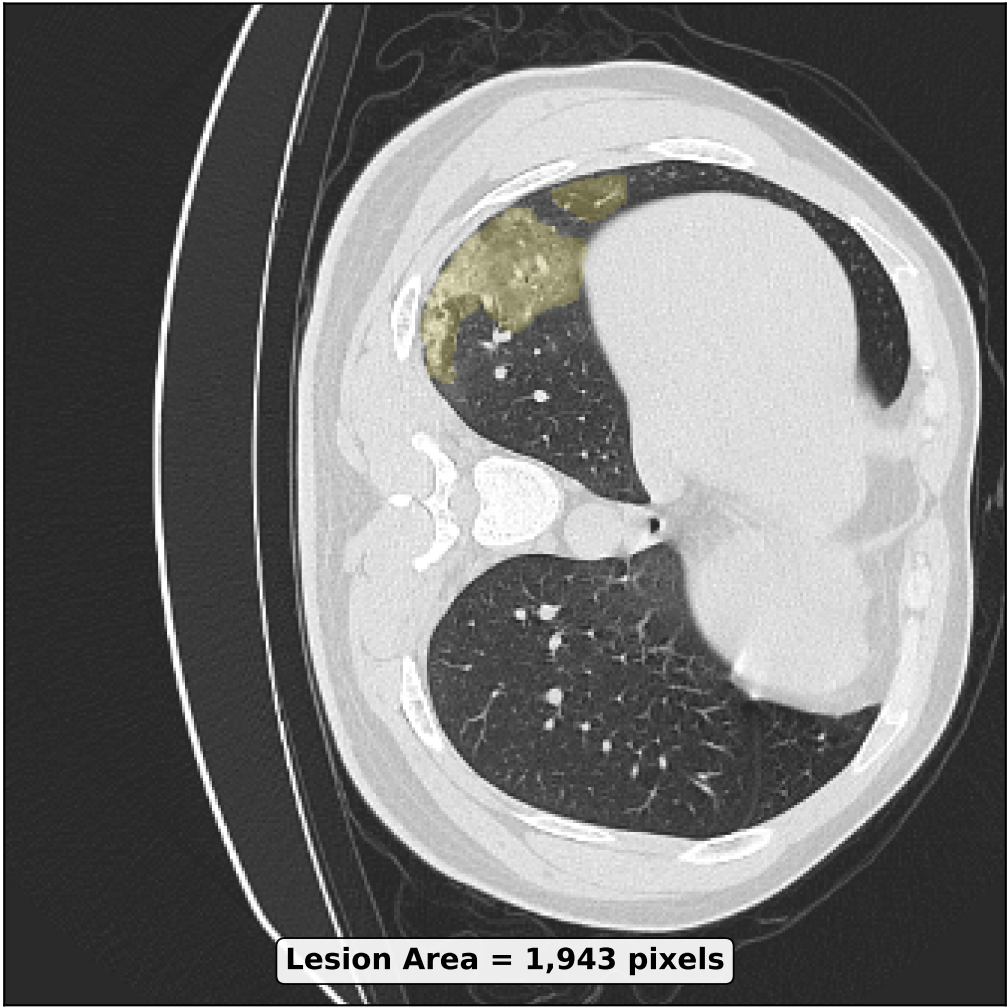


(D) Radiopaedia
radiopaedia_40_86625_0 | z = 32 | Calibration



(E) Radiopaedia
radiopaedia_4_85506_1 | z = 13 | Selection

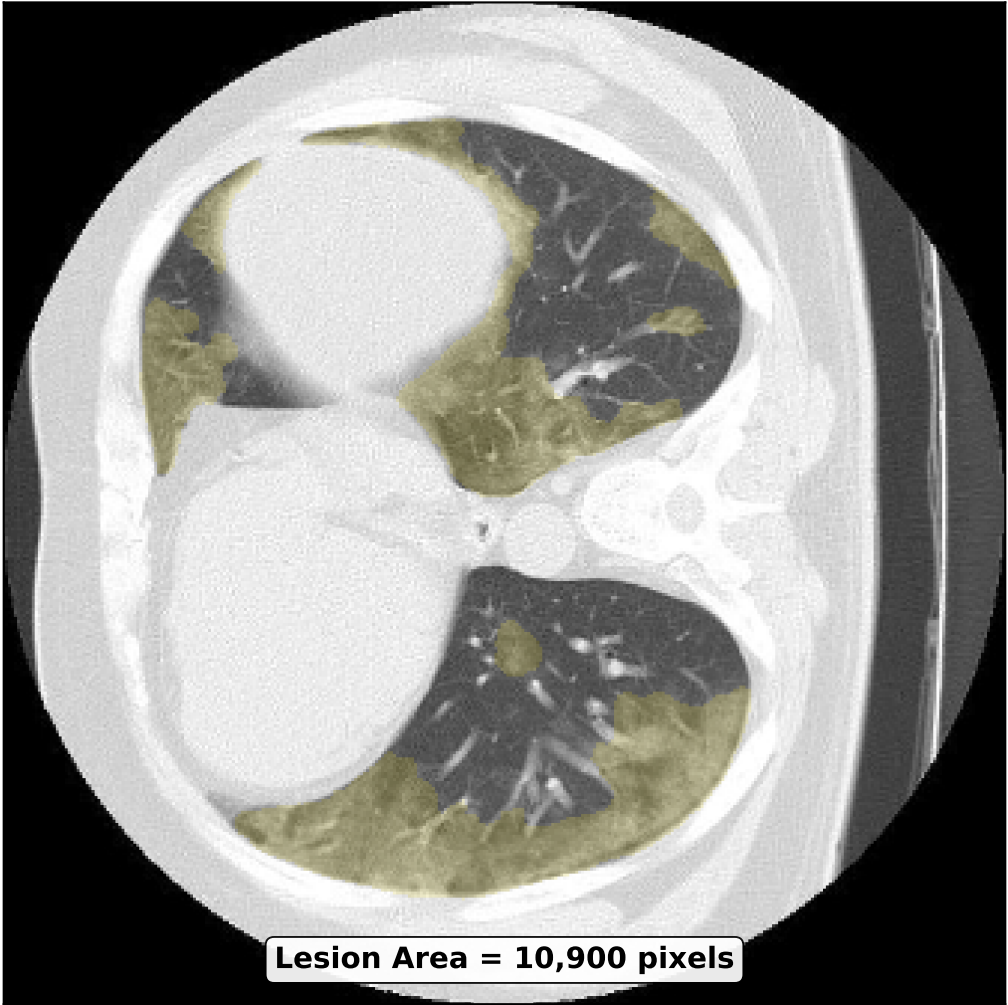

(F) Radiopaedia
radiopaedia_10_85902_1 | z = 12 | Selection

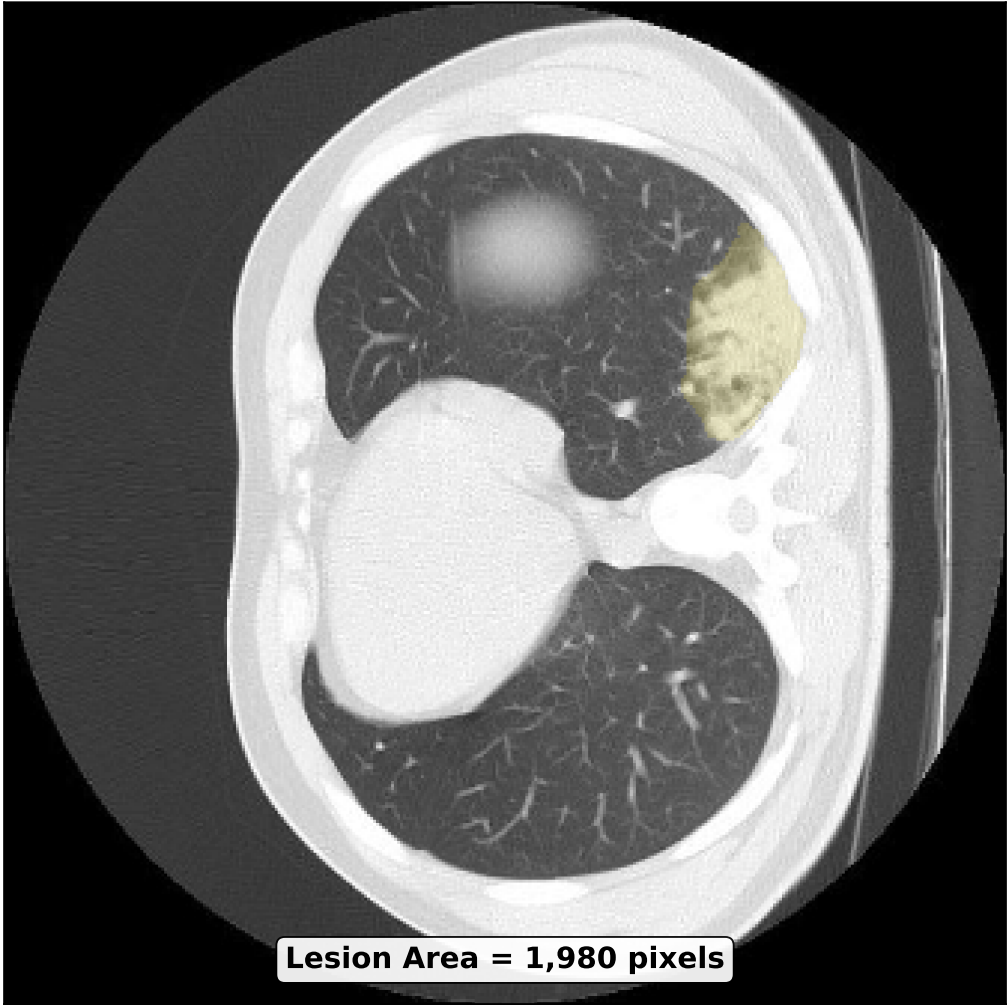

Each panel shows one representative lesion-positive held-out source slice after preprocessing. Top row: three different CoronaCases volumes. Bottom row: three different Radiopaedia volumes. Yellow overlay indicates the reference infection annotation used only for source-side quality control.