


Filename: 2020-02-19 - 11.48.47.GDNA

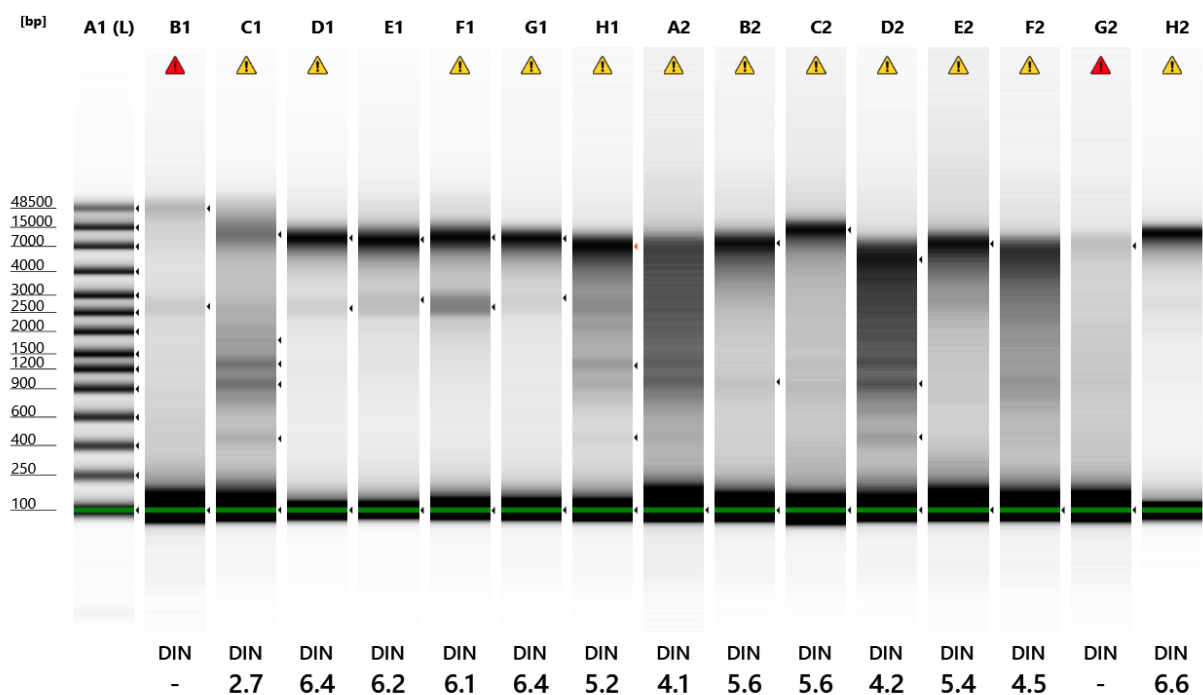


Default image (Contrast 50%), Image is Scaled to Sample

Sample Info

Well	DIN	Conc. [ng/ul]	Sample Description	Alert	Observations
A1	-	68.3	Ladder		Ladder
B1	-	2.52	3	▲	Sample concentration outside functional range for DIN and the assay
C1	2.7	6.91	16	▲	Sample concentration outside recommended range
D1	6.4	6.62	22	▲	Sample concentration outside recommended range
E1	6.2	12.0	25		
F1	6.1	8.12	31	▲	Sample concentration outside recommended range
G1	6.4	5.25	37	▲	Sample concentration outside recommended range
H1	5.2	7.96	42	▲	Sample concentration outside recommended range
A2	4.1	6.96	45	▲	Sample concentration outside recommended range
B2	5.6	5.57	51	▲	Sample concentration outside recommended range
C2	5.6	4.70	55	▲	Sample concentration outside functional range for DIN and the assay
D2	4.2	7.88	65	▲	Sample concentration outside recommended range
E2	5.4	6.32	72	▲	Sample concentration outside recommended range
F2	4.5	7.53	78	▲	Sample concentration outside recommended range
G2	-	2.84	84	▲	Sample concentration outside functional range for DIN and the assay
H2	6.6	8.29	89	▲	Sample concentration outside recommended range

A1: Ladder

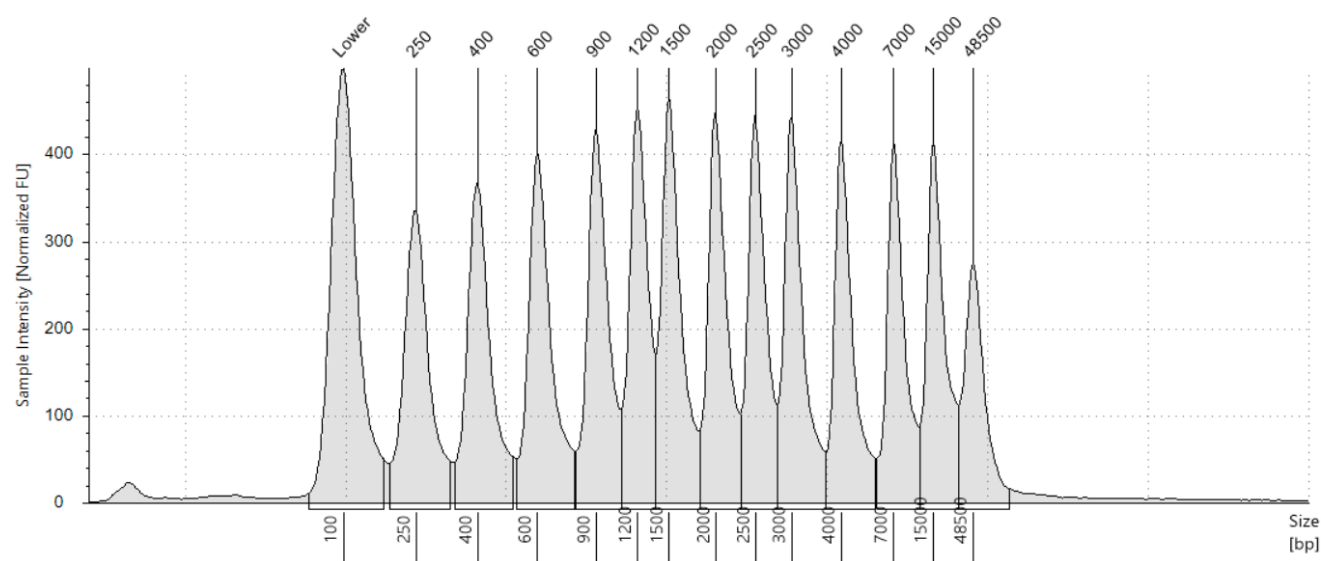


Sample Table

Well	DIN	Conc. [ng/ul]	Sample Description	Alert	Observations
A1	-	68.3	Ladder		Ladder

Peak Table

Size [bp]	Calibrated Conc. [ng/ul]	Assigned Conc. [ng/ul]	% Integrated Area	From [bp]	To [bp]	Peak Comment	Observations
100	8.50	8.50	-	65	165		Lower Marker
250	5.30	-	7.81	180	325		
400	5.43	-	8.01	335	506		
600	5.81	-	8.56	521	774		
900	5.67	-	8.35	781	1070		
1200	5.48	-	8.08	1070	1361		
1500	6.06	-	8.94	1361	1807		
2000	5.44	-	8.02	1807	2297		
2500	5.20	-	7.67	2297	2797		
3000	5.48	-	8.07	2797	3663		
4000	4.92	-	7.25	3663	5780		
7000	4.63	-	6.83	5866	11533		
15000	4.84	-	7.13	11533	24112		
48500	3.58	-	5.28	24112	78534		

B1: 3

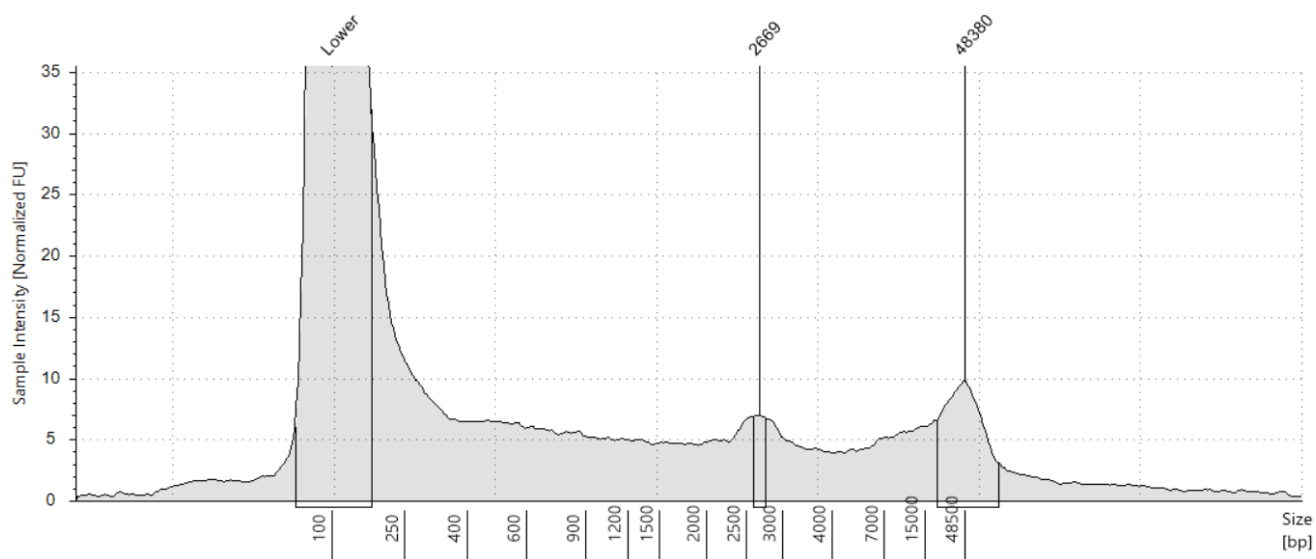


Sample Table

Well	DIN	Conc. [ng/ul]	Sample Description	Alert	Observations
B1	-	2.52	3	▲	Sample concentration outside functional range for DIN and the assay

Peak Table

Size [bp]	Calibrated Conc. [ng/ul]	Assigned Conc. [ng/ul]	% Integrated Area	From [bp]	To [bp]	Peak Comment	Observations
100	8.50	8.50	-	64	165		Lower Marker
2669	0.0541	-	17.19	2595	2765		
48380	0.261	-	82.81	18952	>60000		

C1: 16

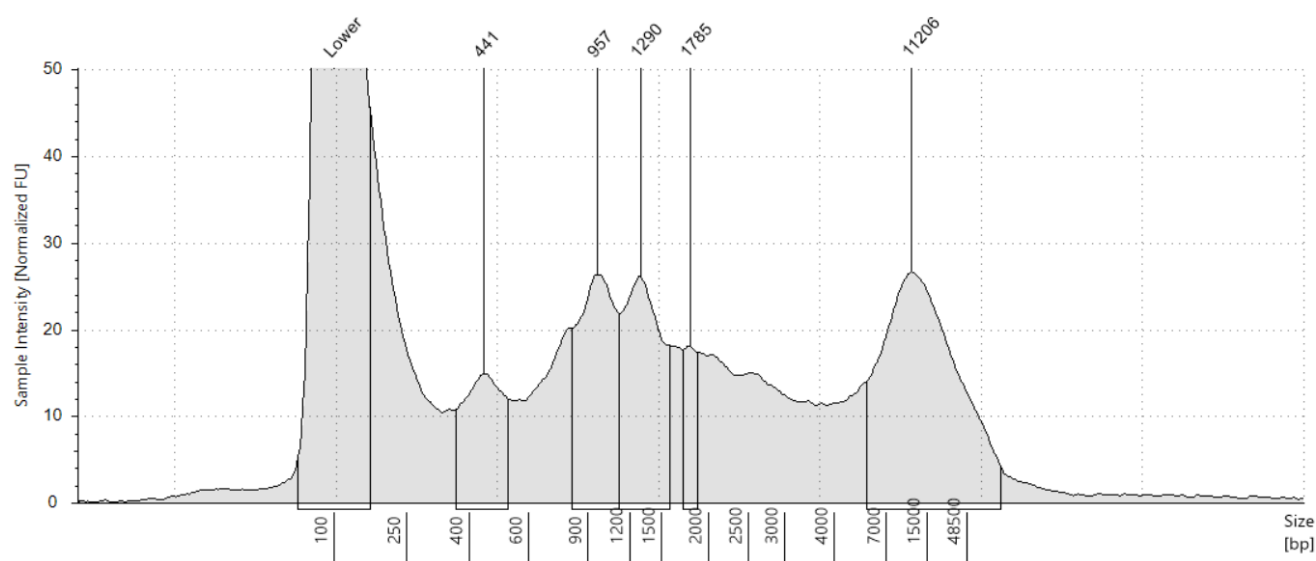


Sample Table

Well	DIN	Conc. [ng/ul]	Sample Description	Alert	Observations
C1	2.7	6.91	16	⚠	Sample concentration outside recommended range

Peak Table

Size [bp]	Calibrated Conc. [ng/ul]	Assigned Conc. [ng/ul]	% Integrated Area	From [bp]	To [bp]	Peak Comment	Observations
100	8.50	8.50	-	64	157		Lower Marker
441	0.429	-	12.16	361	517		
957	0.717	-	20.34	807	1116		
1290	0.726	-	20.60	1116	1572		
1785	0.170	-	4.82	1711	1862		
11206	1.48	-	42.07	5599	>60000		

D1: 22

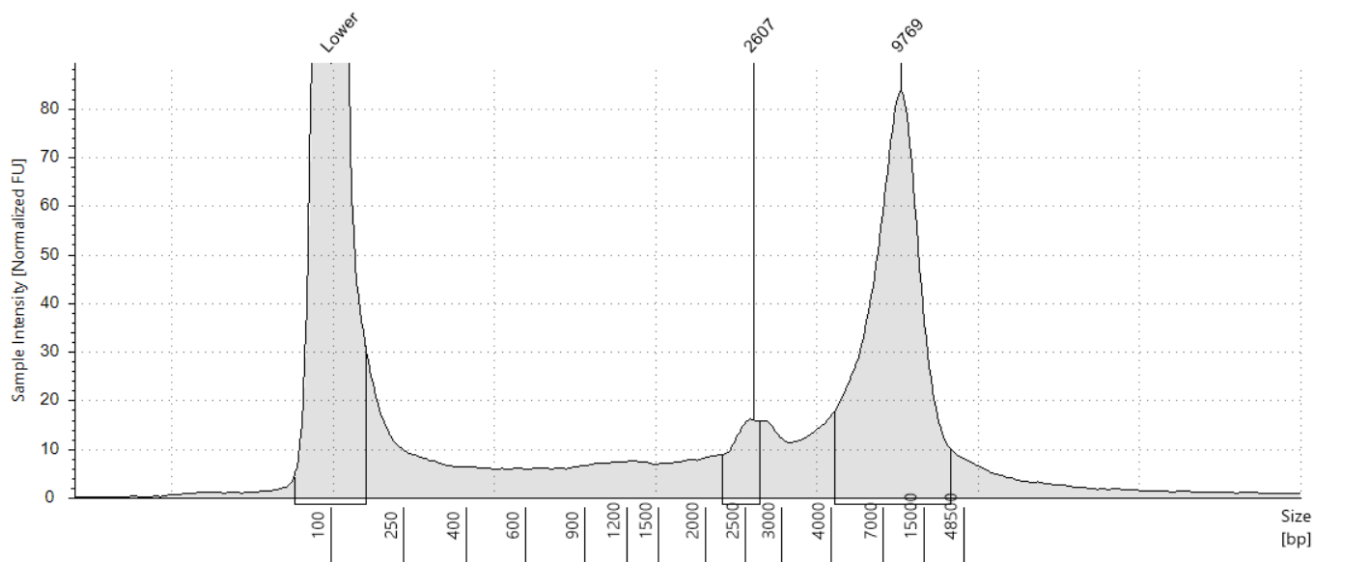


Sample Table

Well	DIN	Conc. [ng/ul]	Sample Description	Alert	Observations
D1	6.4	6.62	22		Sample concentration outside recommended range

Peak Table

Size [bp]	Calibrated Conc. [ng/ul]	Assigned Conc. [ng/ul]	% Integrated Area	From [bp]	To [bp]	Peak Comment	Observations
100	8.50	8.50	-	64	155		Lower Marker
2607	0.330	-	9.14	2191	2682		
9769	3.28	-	90.86	4142	24729		

E1: 25

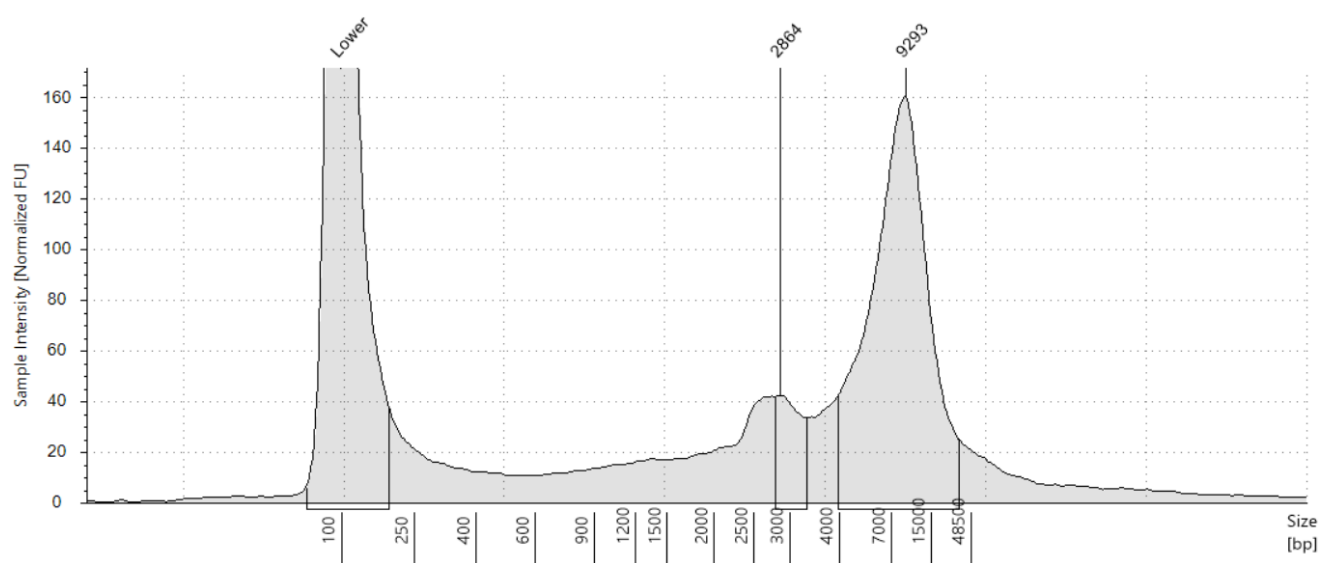


Sample Table

Well	DIN	Conc. [ng/ul]	Sample Description	Alert	Observations
E1	6.2	12.0	25		

Peak Table

Size [bp]	Calibrated Conc. [ng/ul]	Assigned Conc. [ng/ul]	% Integrated Area	From [bp]	To [bp]	Peak Comment	Observations
100	8.50	8.50	-	65	184		Lower Marker
2864	0.691	-	10.67	2784	3314		
9293	5.78	-	89.33	3986	25479		

F1: 31

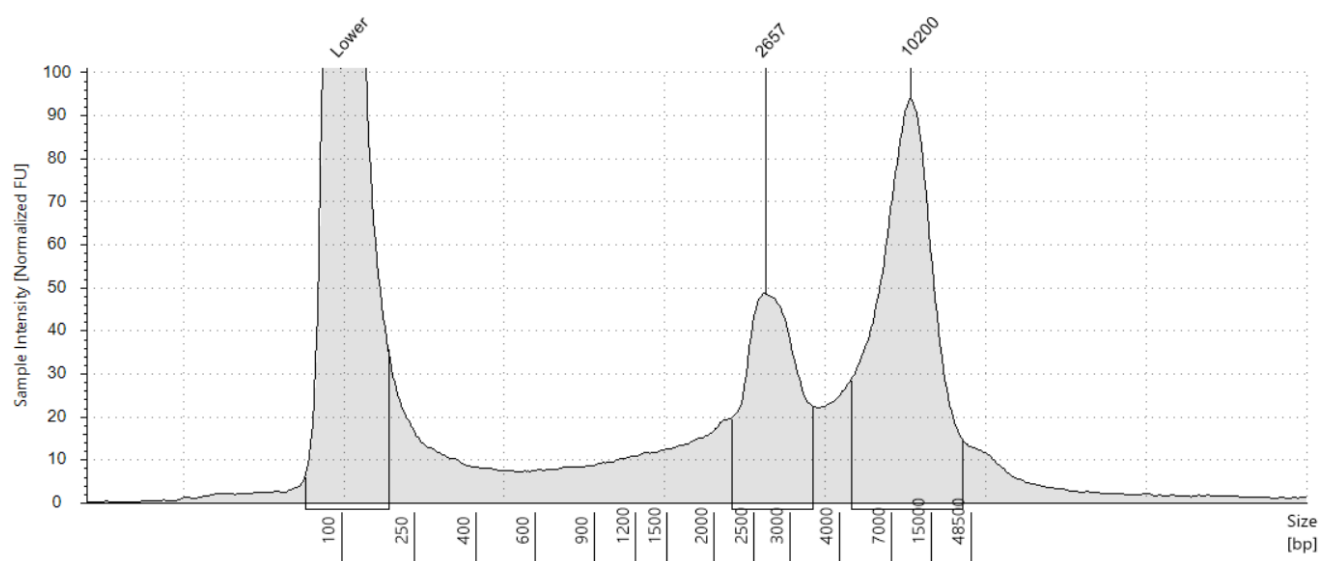


Sample Table

Well	DIN	Conc. [ng/ul]	Sample Description	Alert	Observations
F1	6.1	8.12	31	⚠	Sample concentration outside recommended range

Peak Table

Size [bp]	Calibrated Conc. [ng/ul]	Assigned Conc. [ng/ul]	% Integrated Area	From [bp]	To [bp]	Peak Comment	Observations
100	8.50	8.50	-	64	183		Lower Marker
2657	1.60	-	32.82	2212	3452		
10200	3.28	-	67.18	4584	28663		

G1: 37

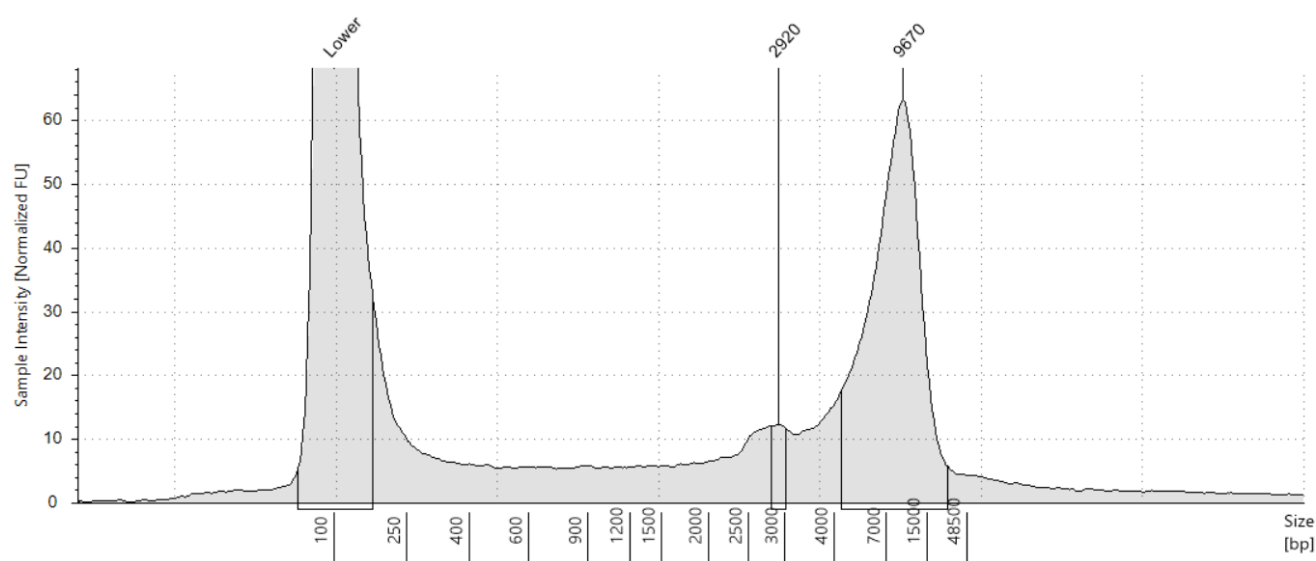


Sample Table

Well	DIN	Conc. [ng/ul]	Sample Description	Alert	Observations
G1	6.4	5.25	37	⚠	Sample concentration outside recommended range

Peak Table

Size [bp]	Calibrated Conc. [ng/ul]	Assigned Conc. [ng/ul]	% Integrated Area	From [bp]	To [bp]	Peak Comment	Observations
100	8.50	8.50	-	64	162		Lower Marker
2920	0.117	-	4.87	2816	3033		
9670	2.29	-	95.13	4353	22493		

H1: 42

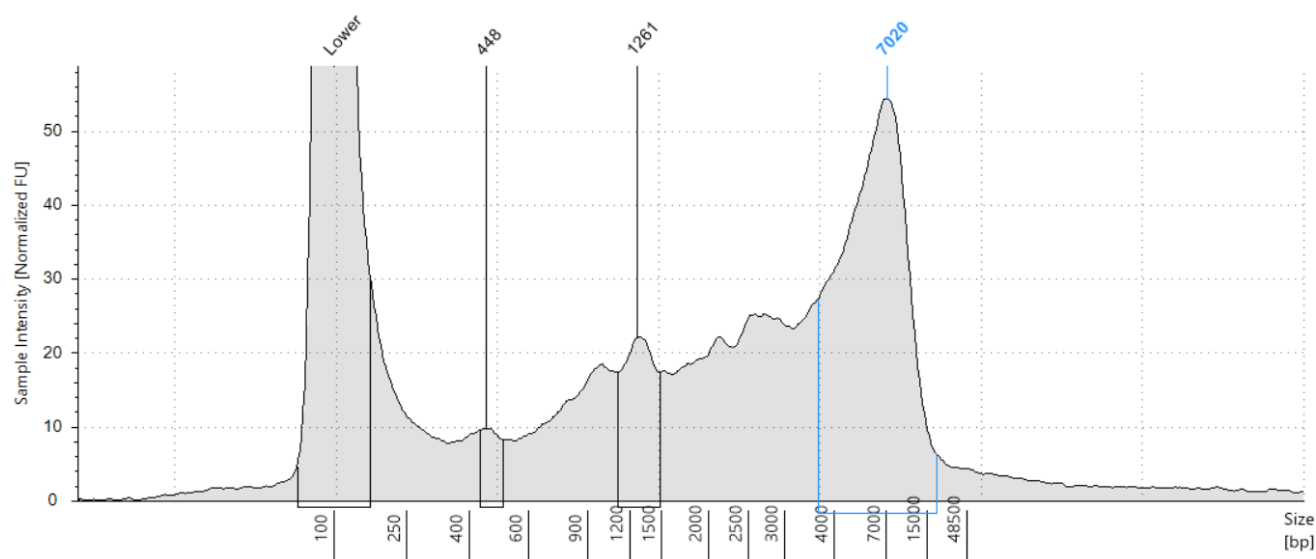


Sample Table

Well	DIN	Conc. [ng/μl]	Sample Description	Alert	Observations
H1	5.2	7.96	42	⚠	Sample concentration outside recommended range

Peak Table

Size [bp]	Calibrated Conc. [ng/μl]	Assigned Conc. [ng/μl]	% Integrated Area	From [bp]	To [bp]	Peak Comment	Observations
100	8.50	8.50	-	63	158		Lower Marker
448	0.143	-	4.18	431	505		
1261	0.555	-	16.22	1104	1486		
7020	2.72	-	79.60	3645	18075		

A2: 45

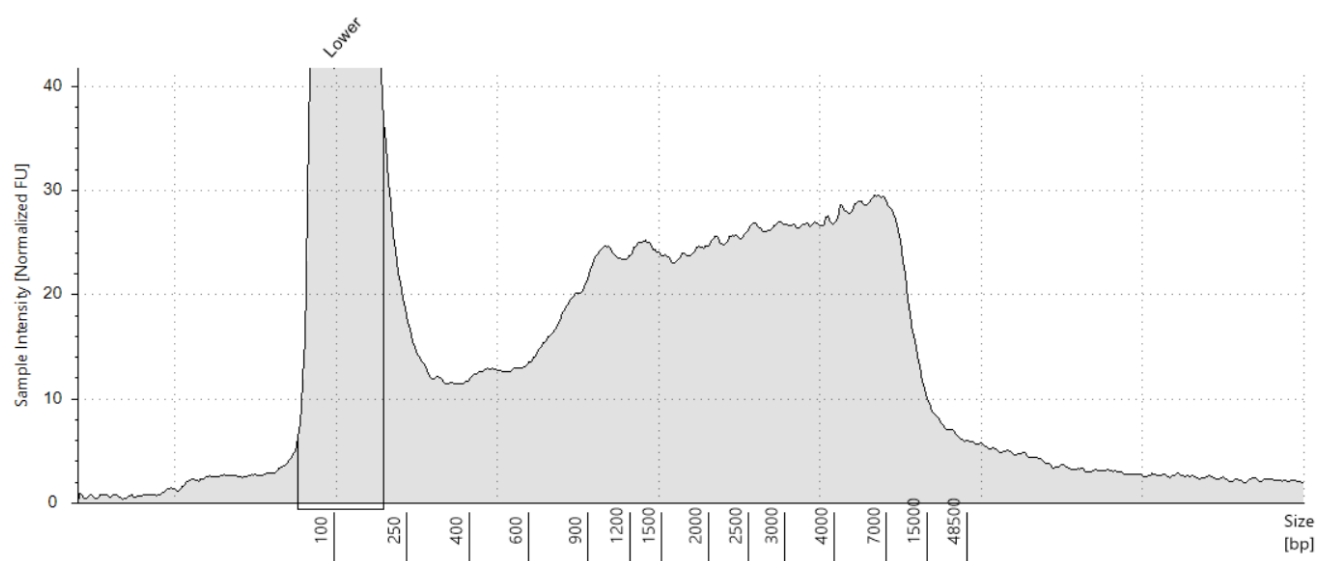


Sample Table

Well	DIN	Conc. [ng/ul]	Sample Description	Alert	Observations
A2	4.1	6.96	45	⚠	Sample concentration outside recommended range

Peak Table

Size [bp]	Calibrated Conc. [ng/ul]	Assigned Conc. [ng/ul]	% Integrated Area	From [bp]	To [bp]	Peak Comment	Observations
100	8.50	8.50	-	64	187		Lower Marker

B2: 51

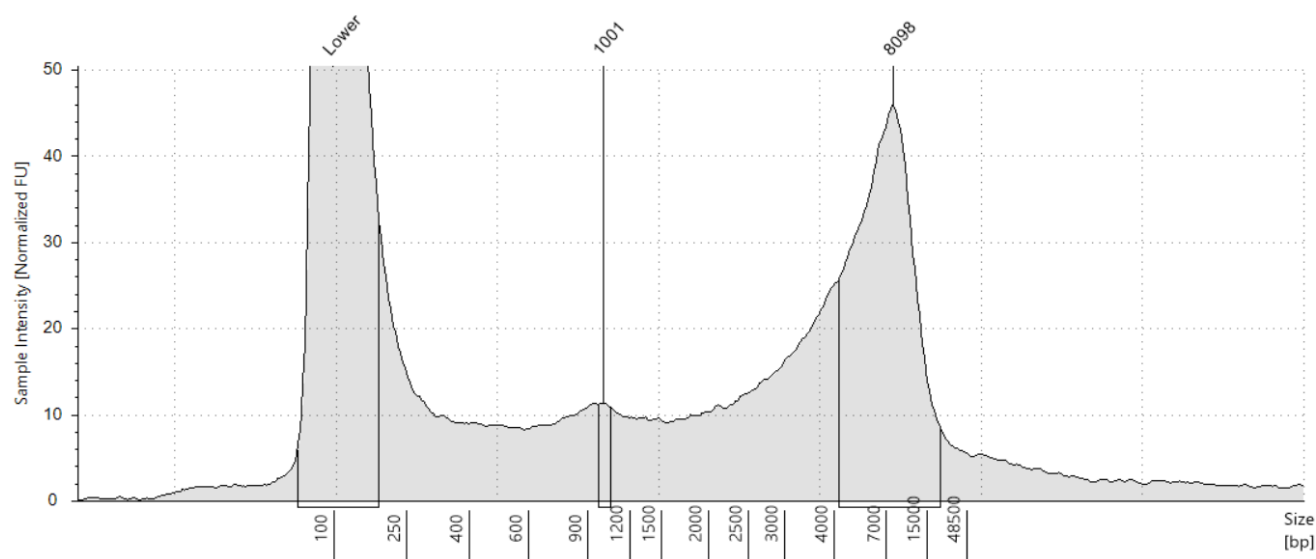


Sample Table

Well	DIN	Conc. [ng/μl]	Sample Description	Alert	Observations
B2	5.6	5.57	51	⚠	Sample concentration outside recommended range

Peak Table

Size [bp]	Calibrated Conc. [ng/μl]	Assigned Conc. [ng/μl]	% Integrated Area	From [bp]	To [bp]	Peak Comment	Observations
100	8.50	8.50	-	64	176		Lower Marker
1001	0.0778	-	4.18	972	1051		
8098	1.79	-	95.82	4212	19728		

C2: 55

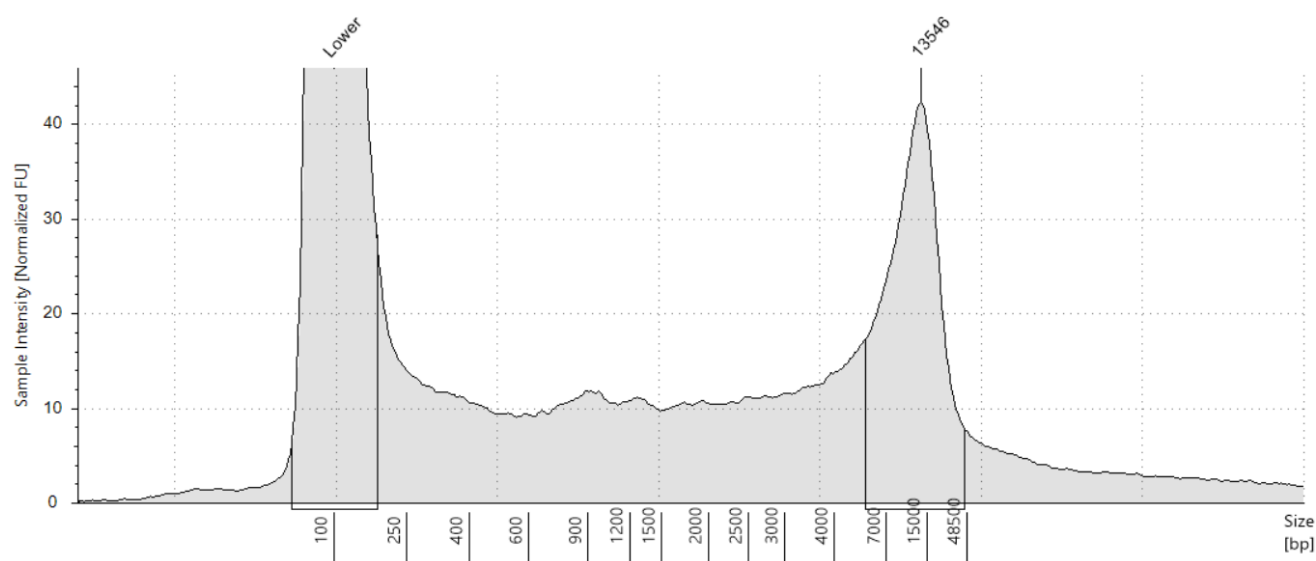


Sample Table

Well	DIN	Conc. [ng/ul]	Sample Description	Alert	Observations
C2	5.6	4.70	55	⚠	Sample concentration outside functional range for DIN and the assay

Peak Table

Size [bp]	Calibrated Conc. [ng/ul]	Assigned Conc. [ng/ul]	% Integrated Area	From [bp]	To [bp]	Peak Comment	Observations
100	8.50	8.50	-	59	171		Lower Marker
13546	1.32	-	98.25	5578	38403		
-	-	-	-	-	-		Sample Well

D2: 65

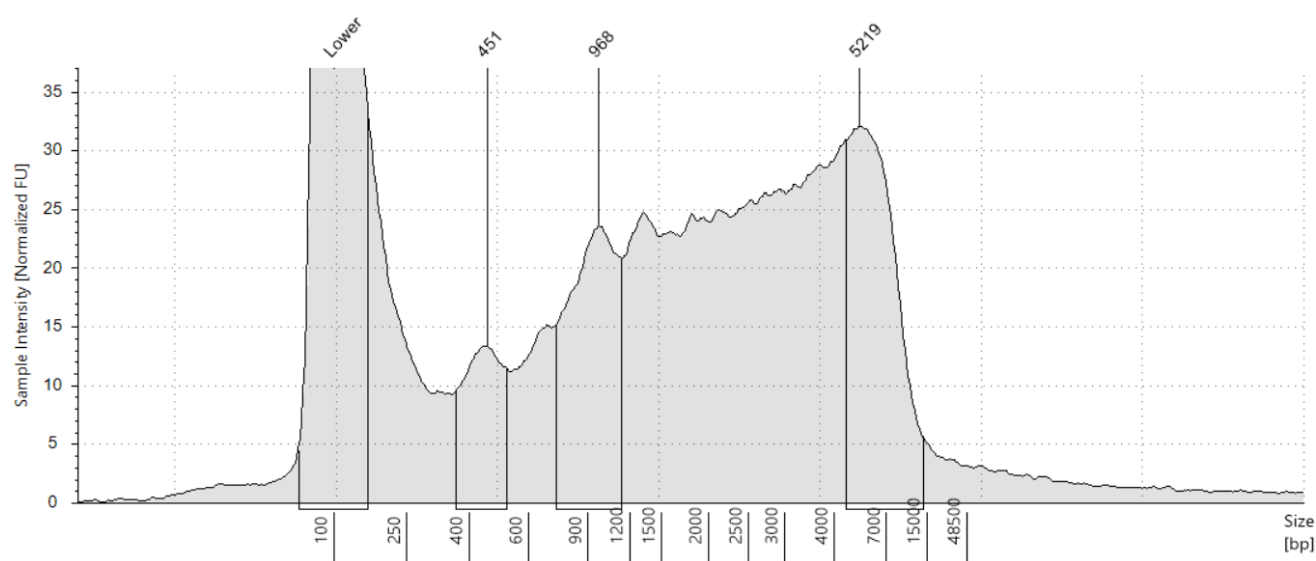


Sample Table

Well	DIN	Conc. [ng/ul]	Sample Description	Alert	Observations
D2	4.2	7.88	65	⚠	Sample concentration outside recommended range

Peak Table

Size [bp]	Calibrated Conc. [ng/ul]	Assigned Conc. [ng/ul]	% Integrated Area	From [bp]	To [bp]	Peak Comment	Observations
100	8.50	8.50	-	64	153		Lower Marker
451	0.402	-	16.21	361	516		
968	0.887	-	35.76	723	1132		
5219	1.19	-	48.03	4556	13920		

E2: 72

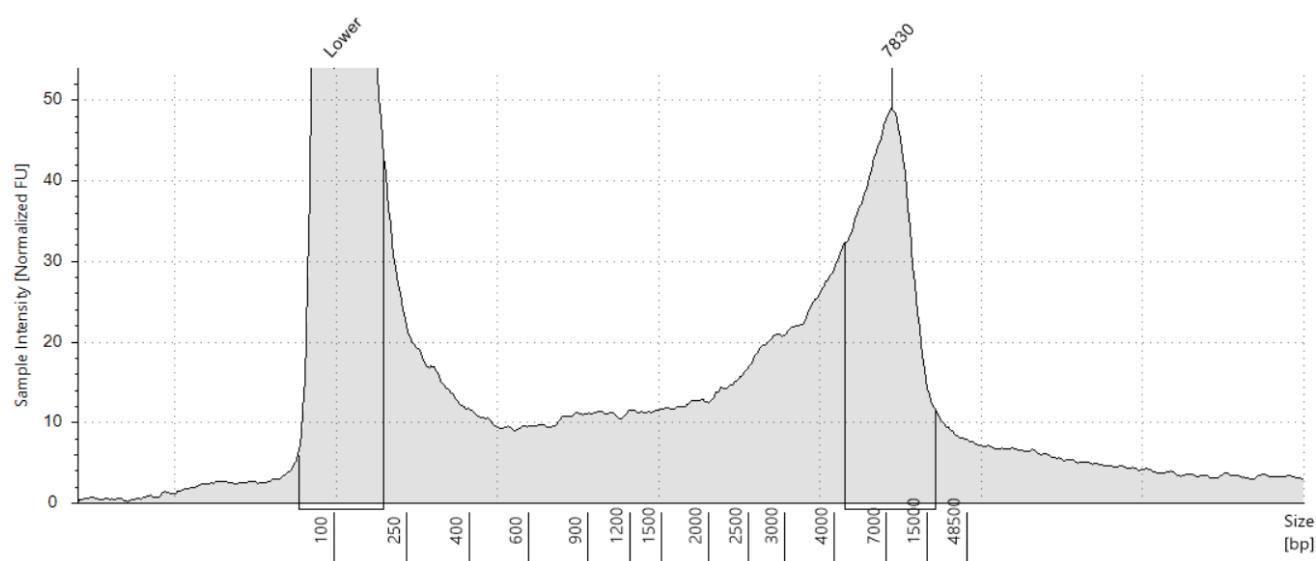


Sample Table

Well	DIN	Conc. [ng/ul]	Sample Description	Alert	Observations
E2	5.4	6.32	72	⚠	Sample concentration outside recommended range

Peak Table

Size [bp]	Calibrated Conc. [ng/ul]	Assigned Conc. [ng/ul]	% Integrated Area	From [bp]	To [bp]	Peak Comment	Observations
100	8.50	8.50	-	64	187		Lower Marker
7830	1.62	-	100.00	4515	17656		

F2: 78

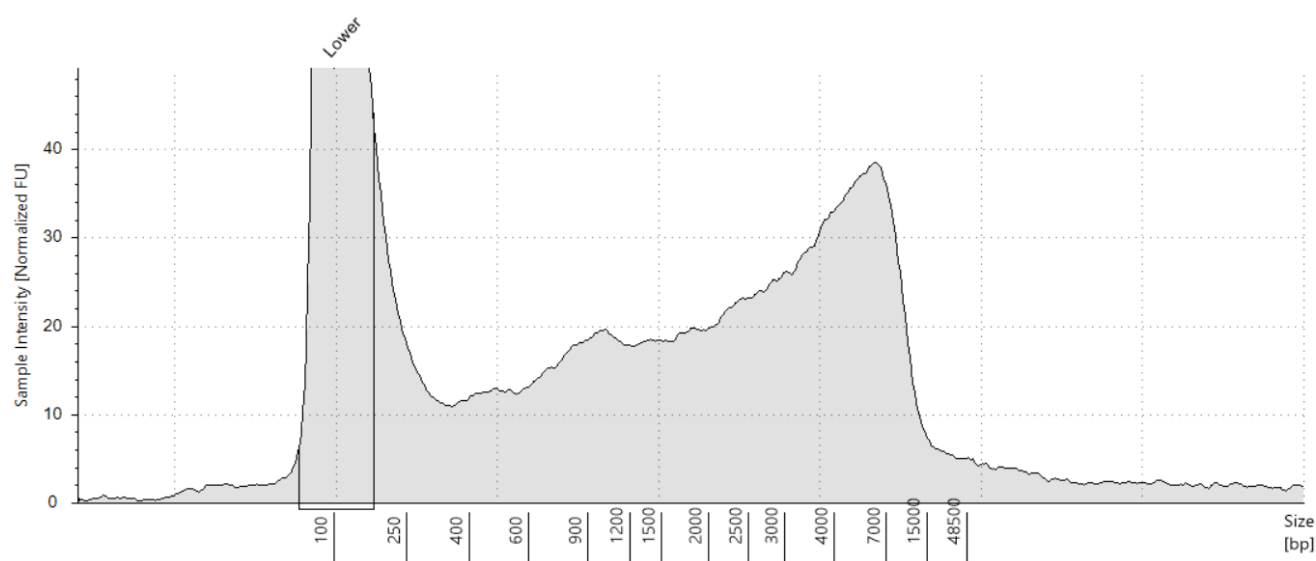


Sample Table

Well	DIN	Conc. [ng/ul]	Sample Description	Alert	Observations
F2	4.5	7.53	78	⚠	Sample concentration outside recommended range

Peak Table

Size [bp]	Calibrated Conc. [ng/ul]	Assigned Conc. [ng/ul]	% Integrated Area	From [bp]	To [bp]	Peak Comment	Observations
100	8.50	8.50	-	65	164		Lower Marker

G2: 84

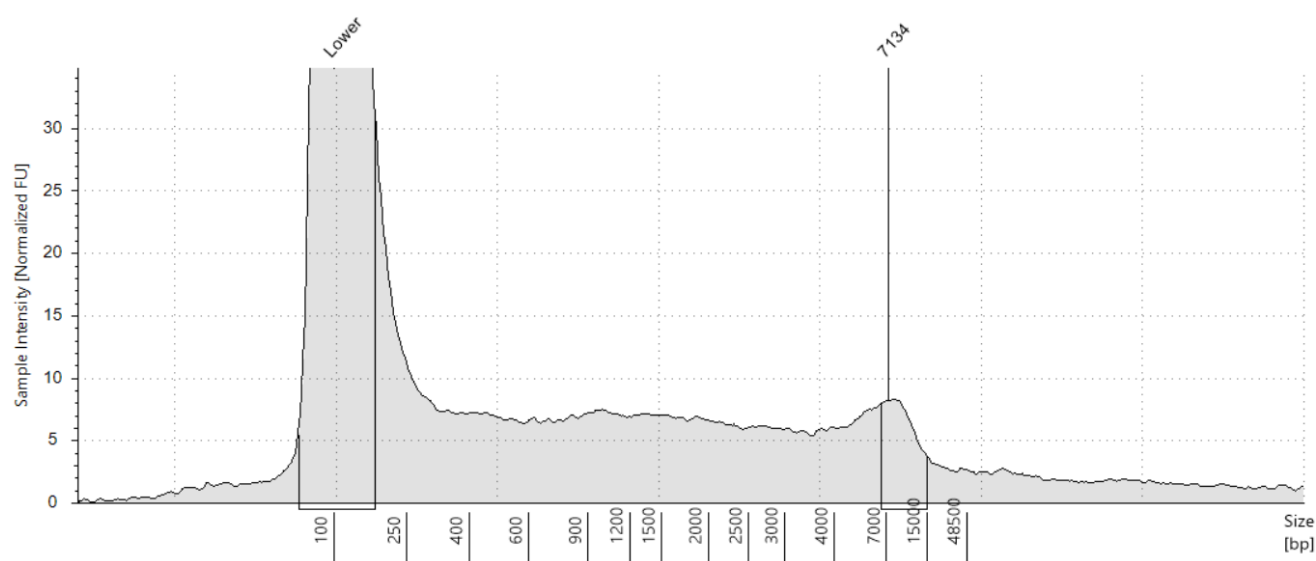


Sample Table

Well	DIN	Conc. [ng/μl]	Sample Description	Alert	Observations
G2	-	2.84	84	▲	Sample concentration outside functional range for DIN and the assay

Peak Table

Size [bp]	Calibrated Conc. [ng/μl]	Assigned Conc. [ng/μl]	% Integrated Area	From [bp]	To [bp]	Peak Comment	Observations
100	8.50	8.50	-	64	168		Lower Marker
7134	0.185	-	100.00	6558	14818		

H2: 89

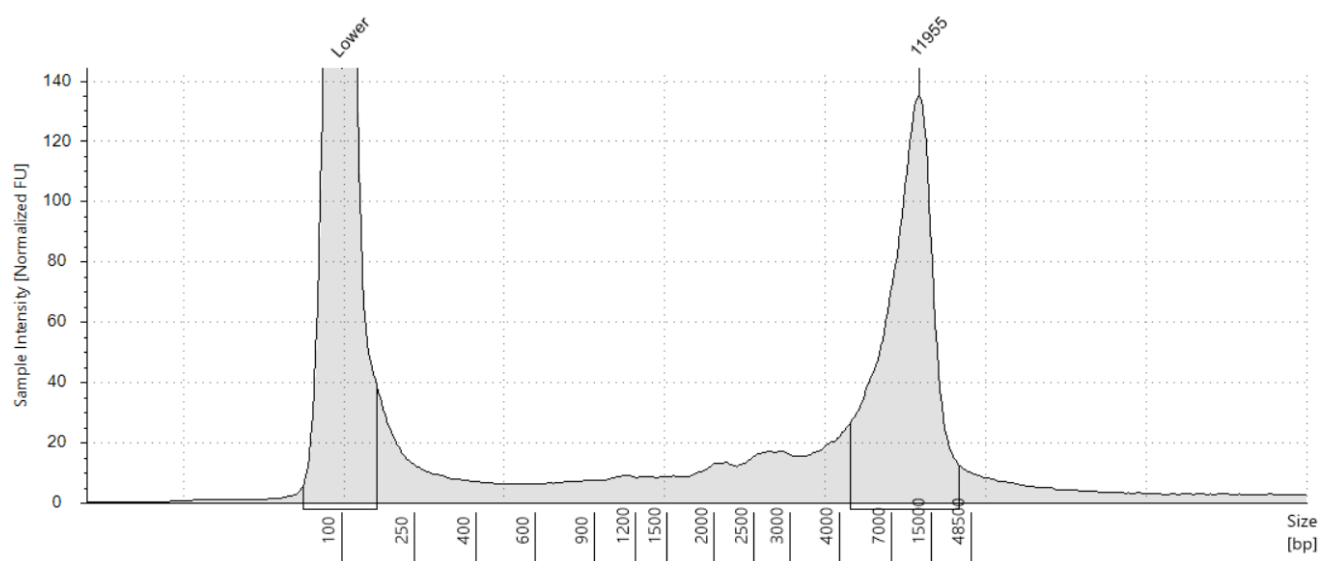



Sample Table

Well	DIN	Conc. [ng/ul]	Sample Description	Alert	Observations
H2	6.6	8.29	89	⚠	Sample concentration outside recommended range

Peak Table

Size [bp]	Calibrated Conc. [ng/ul]	Assigned Conc. [ng/ul]	% Integrated Area	From [bp]	To [bp]	Peak Comment	Observations
100	8.50	8.50	-	62	154		Lower Marker
11955	4.27	-	98.93	4514	25879		
-	-	-	-	-	-		Sample Well

Profile Comparison

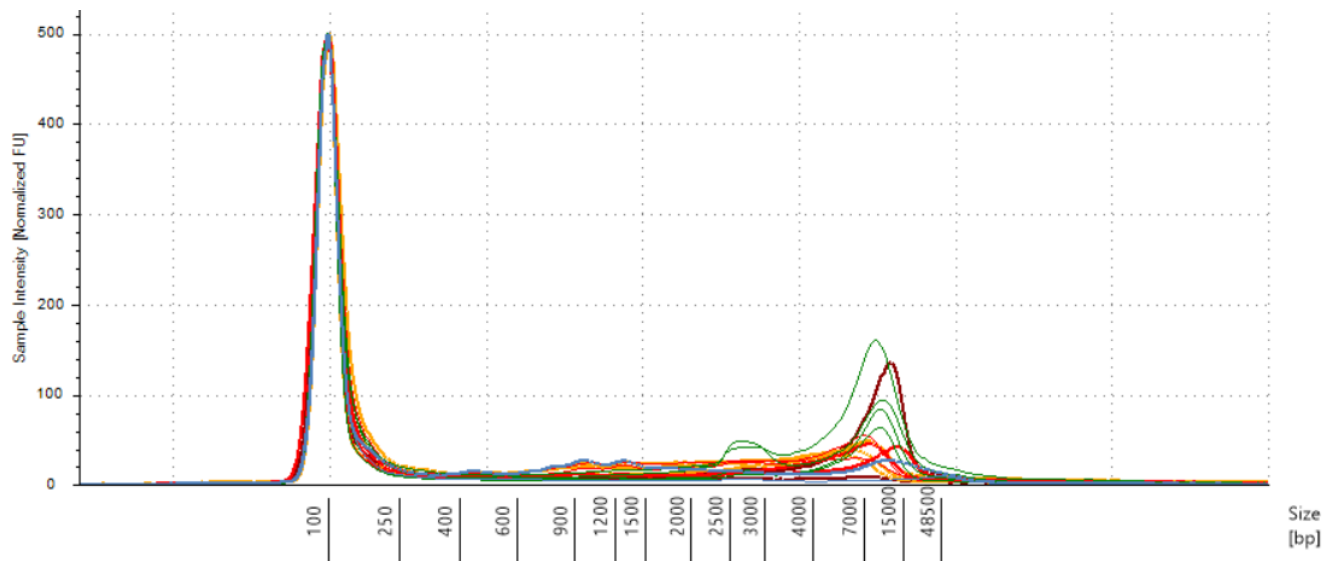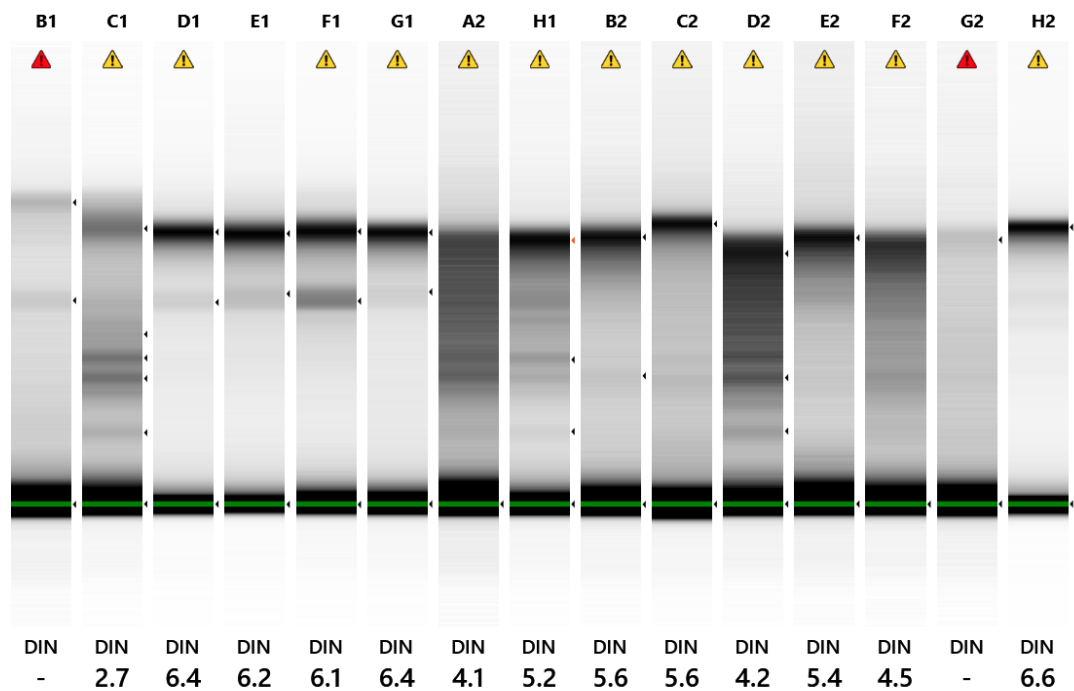

Samples

File	Indicator	Well ID	Comment
File 1		B1	3
File 1		C1	16
File 1		D1	22
File 1		E1	25
File 1		F1	31
File 1		G1	37
File 1		A2	45
File 1		H1	42
File 1		B2	51
File 1		C2	55
File 1		D2	65
File 1		E2	72
File 1		F2	78
File 1		G2	84
File 1		H2	89

Files used in the Profile Comparison

File	Comments	Filename
------	----------	----------

File 1	C:\Users\4150 TapeStation\Documents\Agilent\TapeStation Data\2020-02-19\2020-02-19 - 11.48.47.GDNA
--------	--