


C1: 5026473

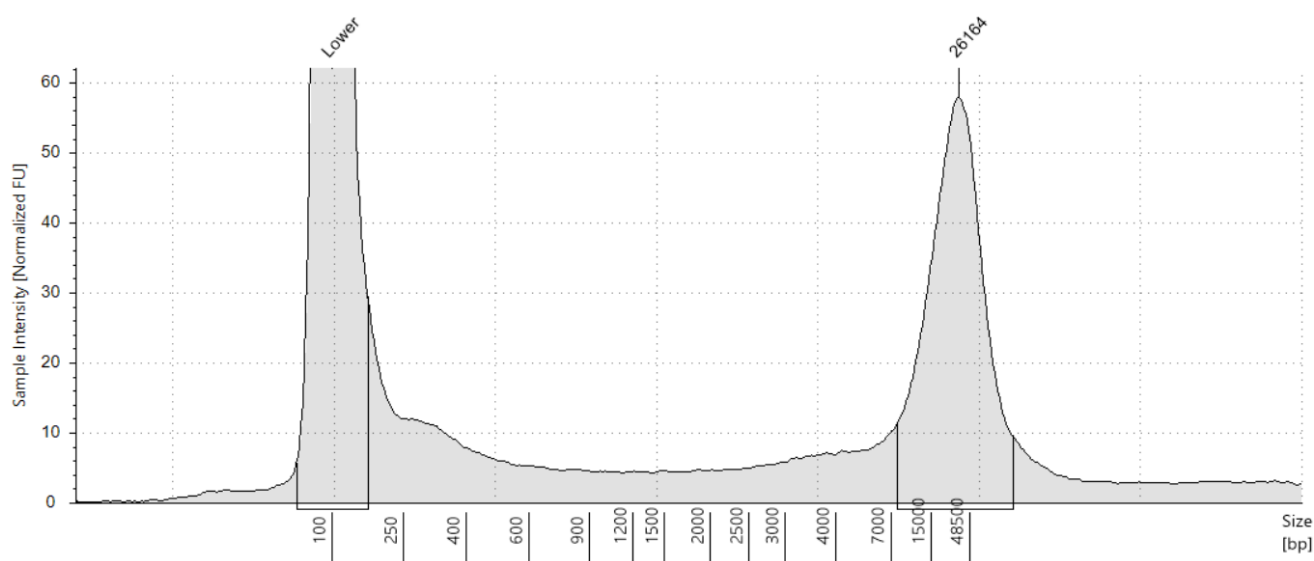


Sample Table

Well	DIN	Conc. [ng/ul]	Sample Description	Alert	Observations
C1	7.2	5.66	5026473	⚠	Sample concentration outside recommended range

Peak Table

Size [bp]	Calibrated Conc. [ng/ul]	Assigned Conc. [ng/ul]	% Integrated Area	From [bp]	To [bp]	Peak Comment	Observations
100	8.50	8.50	-	64	159		Lower Marker
26164	2.42	-	82.27	7942	>60000		
-	-	-	-	-	-		Sample Well

D1: 5024381

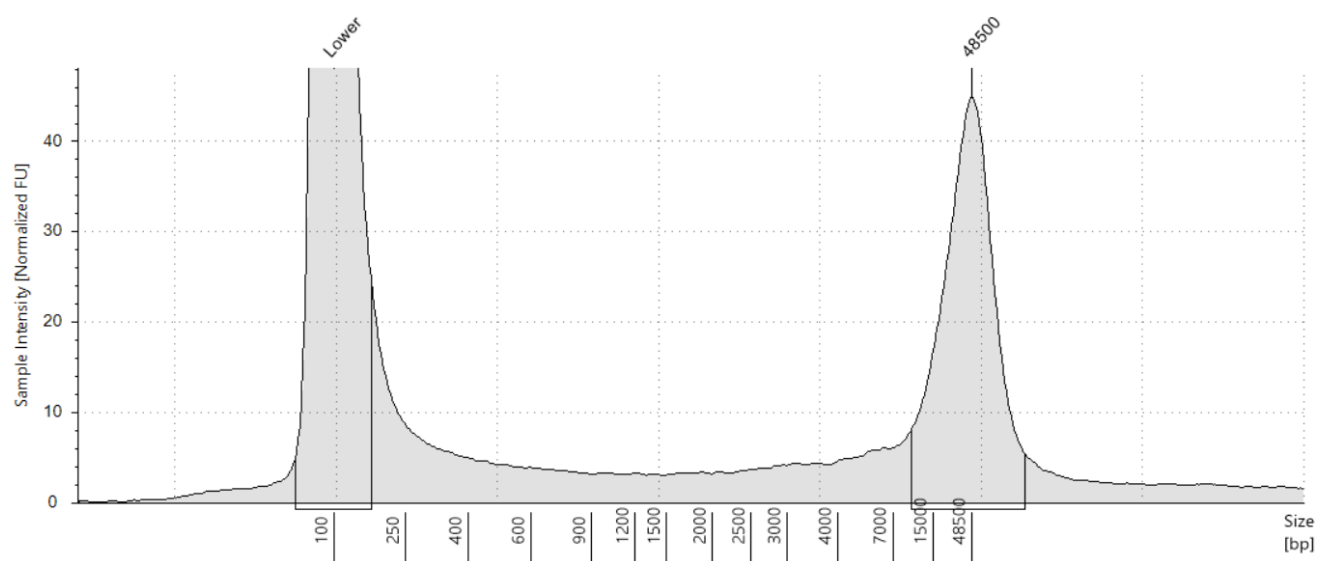

Sample Table

Well	DIN	Conc. [ng/ul]	Sample Description	Alert	Observations
D1	8.7	3.51	5024381	⚠	Sample concentration outside functional range for DIN and the assay

Peak Table

Size [bp]	Calibrated Conc. [ng/ul]	Assigned Conc. [ng/ul]	% Integrated Area	From [bp]	To [bp]	Peak Comment	Observations
100	8.50	8.50	-	61	163		Lower Marker
48500	1.65	-	86.11	9861	>60000		
-	-	-	-	-	-		Sample Well