


Assay Class: High Sensitivity DNA Assay
Data Path: C:\...gh Sensitivity DNA Assay_DE13805677_2019-06-20_09-10-48.xad

Created: 20/06/2019 09:10:48
Modified: 20/06/2019 10:26:04

Electrophoresis File Run Summary

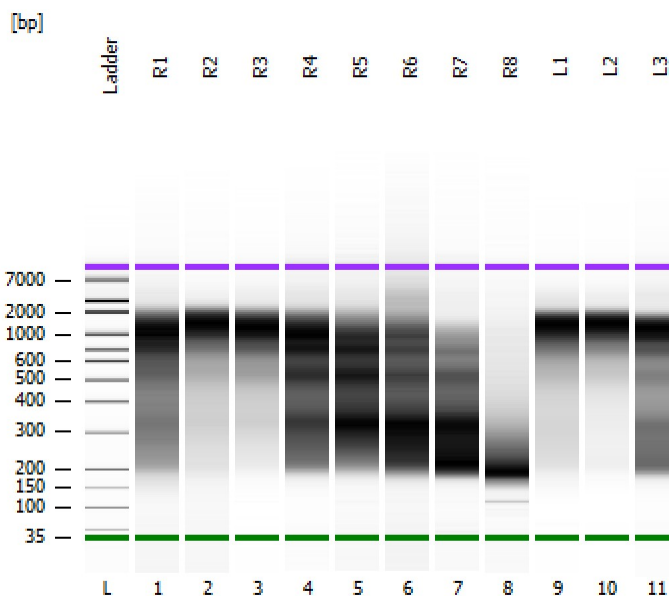

Instrument Information:

Instrument Name: DE13805677
Serial#: DE13805677

Firmware: C.01.069
Type: G2939A

Assay Information:

Assay Origin Path: C:\Program Files (x86)\Agilent\2100 bioanalyzer\2100 expert\assays\dsDNA\High Sensitivity DNA.xsy

Assay Class: High Sensitivity DNA Assay

Version: 1.03


Assay Comments: Copyright © 2003-2010 Agilent Technologies

Chip Information:

Chip Lot #:

Reagent Kit Lot #:

Chip Comments:

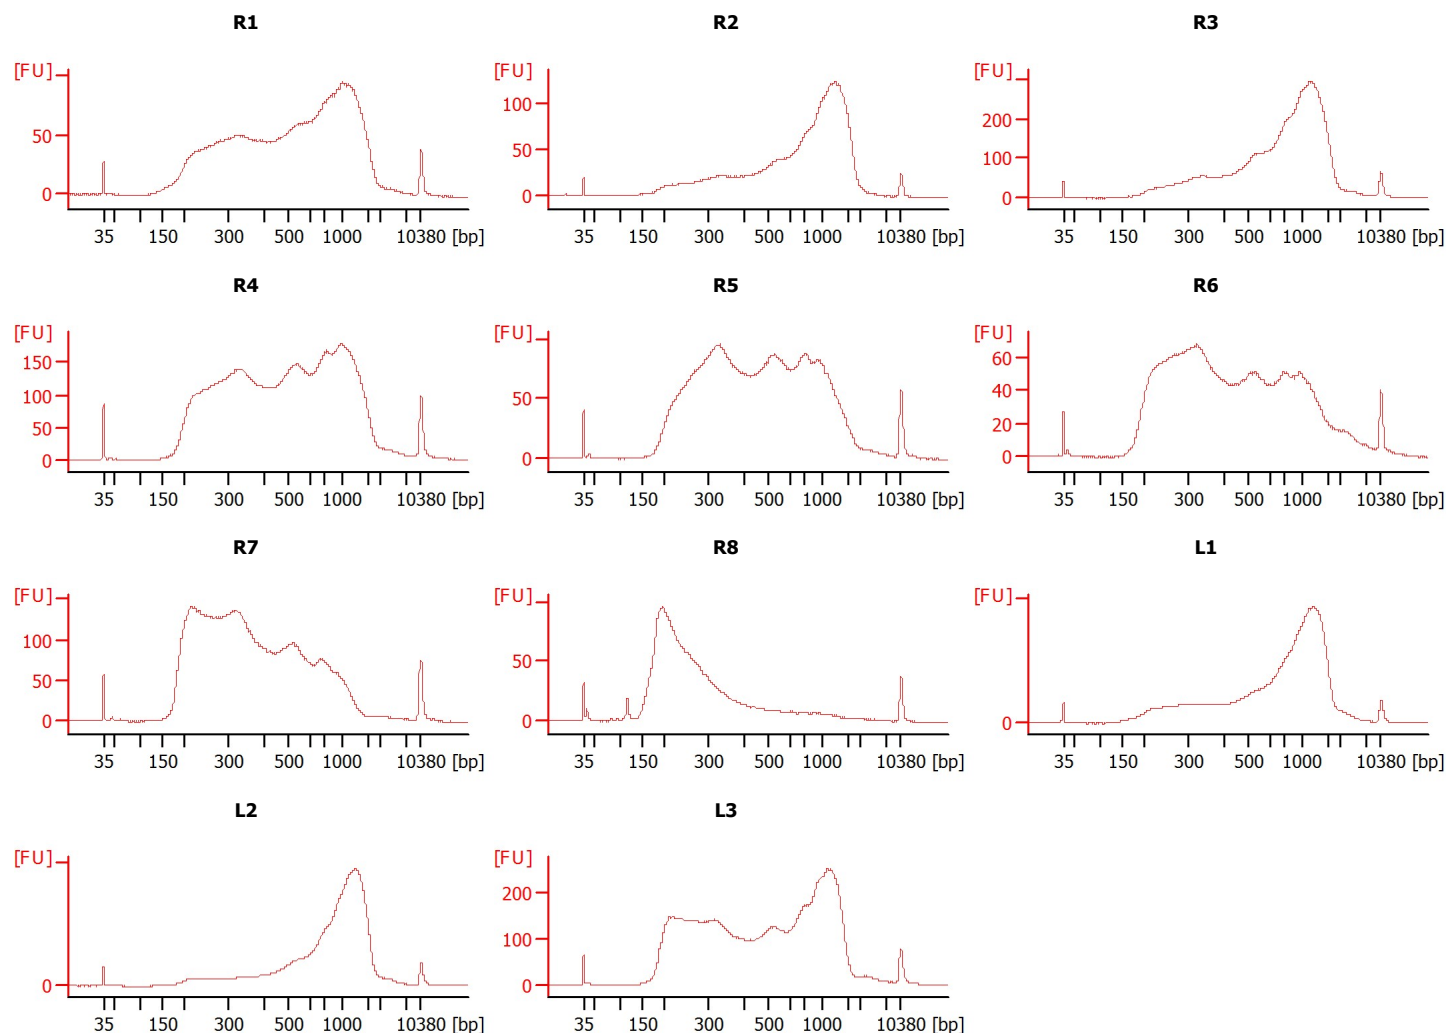

Assay Class: High Sensitivity DNA Assay
Data Path: C:\...gh Sensitivity DNA Assay_DE13805677_2019-06-20_09-10-48.xad

Created: 20/06/2019 09:10:48
Modified: 20/06/2019 10:26:04

Electrophoresis File Run Summary (Chip Summary)

Sample Name	Sample Comment	Rest. Digest	Status	Observation	Result Label	Result Color
R1		☐	✓			
R2		☐	✓			
R3		☐	✓			
R4		☐	✓			
R5		☐	✓			
R6		☐	✓			
R7		☐	✓			
R8		☐	✓			
L1		☐	✓			
L2		☐	✓			
L3		☐	✓			
Ladder		☐	✓			
Chip Lot #			Reagent Kit Lot #			

Chip Comments :

Assay Class: High Sensitivity DNA Assay
Data Path: C:\...gh Sensitivity DNA Assay_DE13805677_2019-06-20_09-10-48.xad

Created: 20/06/2019 09:10:48
Modified: 20/06/2019 10:26:04

Electrophoresis Assay Details

General Analysis Settings

Number of Available Sample and Ladder Wells (Max.) : 12
Minimum Visible Range [s] : 32
Maximum Visible Range [s] : 138
Start Analysis Time Range [s] : 33
End Analysis Time Range [s] : 137,5
Ladder Concentration [pg/ μ l] : 1950
Uses Standard Area for Ladder Fragments
Lower Marker Concentration [pg/ μ l] : 125
Upper Marker Concentration [pg/ μ l] : 75
Used Upper Marker for Quantitation
Standard Curve Fit is Point to Point
Show Data Aligned to Lower and Upper Marker

Integrator Settings

Integration Start Time [s] : 33,05
Integration End Time [s] : 137
Slope Threshold : 0,8
Height Threshold [FU] : 5
Area Threshold : 0,1
Width Threshold [s] : 0,6
Baseline Plateau [s] : 0,5

Filter Settings

Filter Width [s] : 0,5
Polynomial Order : 4


Ladder

Ladder Peak	Size	Area
1	35	160
2	50	210
3	100	208
4	150	221
5	200	242
6	300	270
7	400	305
8	500	306
9	600	336
10	700	321
11	1000	366
12	2000	413
13	3000	411
14	7000	400
15	10380	214

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...gh Sensitivity DNA Assay_DE13805677_2019-06-20_09-10-48.xad

Created: 20/06/2019 09:10:48
 Modified: 20/06/2019 10:26:04

Electropherogram Summary

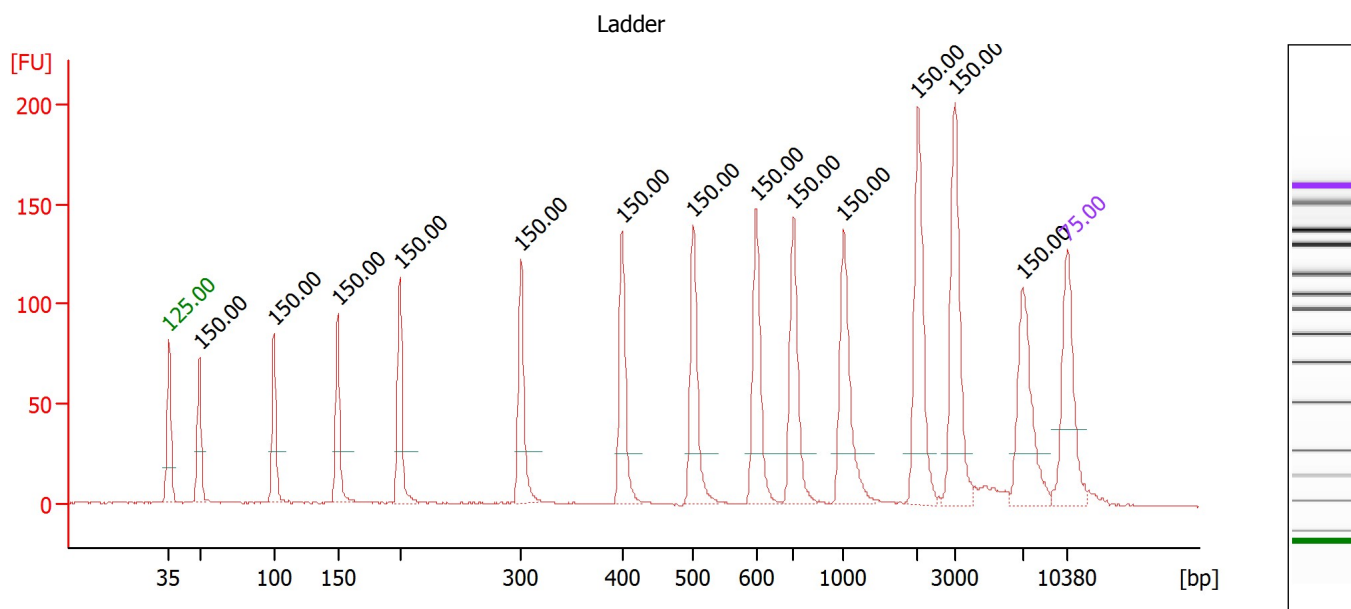

Overall Results for Ladder

Noise: 0,3


Peak table for Ladder

Peak		Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	◀	35	125,00	5 411,3	Lower Marker
2	█	50	150,00	4 545,5	Ladder Peak
3	█	100	150,00	2 272,7	Ladder Peak
4	█	150	150,00	1 515,2	Ladder Peak
5	█	200	150,00	1 136,4	Ladder Peak
6	█	300	150,00	757,6	Ladder Peak
7	█	400	150,00	568,2	Ladder Peak
8	█	500	150,00	454,5	Ladder Peak
9	█	600	150,00	378,8	Ladder Peak
10	█	700	150,00	324,7	Ladder Peak
11	█	1 000	150,00	227,3	Ladder Peak
12	█	2 000	150,00	113,6	Ladder Peak
13	█	3 000	150,00	75,8	Ladder Peak
14	█	7 000	150,00	32,5	Ladder Peak
15	▶	10 380	75,00	10,9	Upper Marker

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...gh Sensitivity DNA Assay_DE13805677_2019-06-20_09-10-48.xad

Created: 20/06/2019 09:10:48
 Modified: 20/06/2019 10:26:04

Electropherogram Summary Continued ...

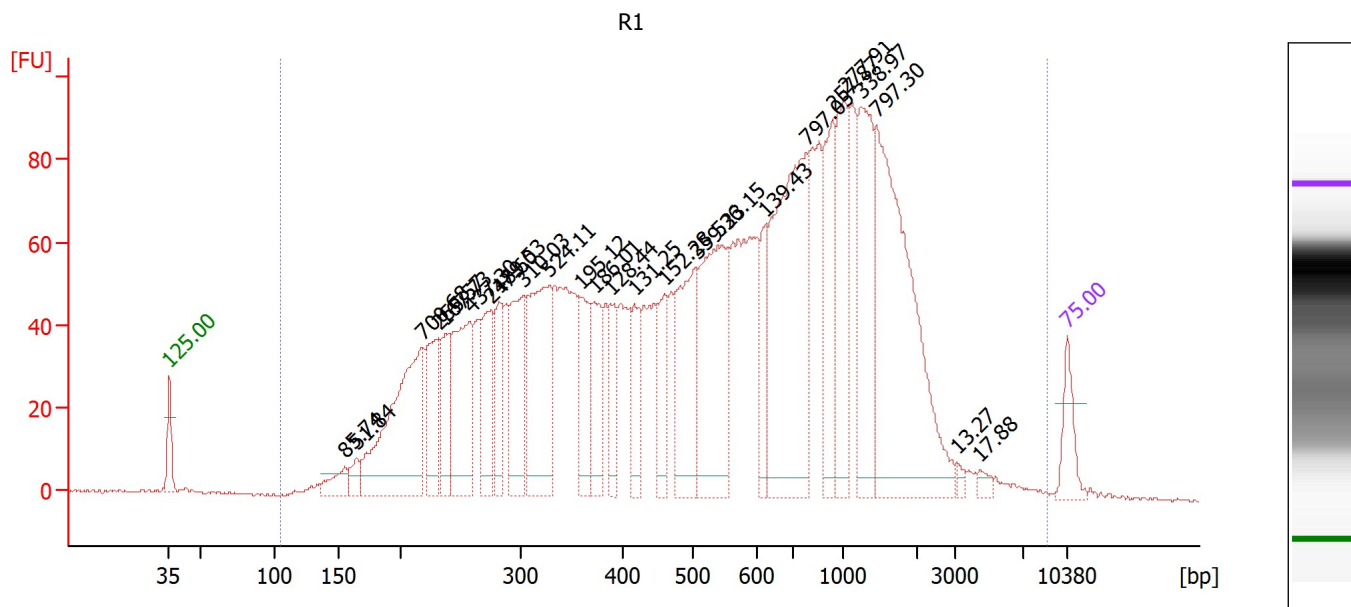

Overall Results for sample 1 : R1

Number of peaks found: 25 Corr. Area 1: 3 154,9
 Noise: 0,4

Peak table for sample 1 : R1

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	35	125,00	5 411,3	Lower Marker
2	156	85,74	833,2	
3	165	51,84	476,3	
4	219	700,68	4 849,8	
5	232	255,57	1 667,4	
6	237	167,73	1 070,6	
7	258	437,30	2 569,3	
8	274	247,60	1 367,7	
9	282	189,53	1 018,4	
10	302	310,03	1 556,6	
11	328	524,11	2 419,1	
12	359	195,12	823,4	
13	372	186,01	757,6	
14	389	128,44	500,7	
15	418	131,25	475,9	
16	459	152,28	502,8	
17	504	359,36	1 080,9	
18	539	523,15	1 469,5	
19	623	139,43	339,0	
20	776	797,05	1 557,2	
21	934	257,87	418,1	
22	1 002	277,91	420,1	
23	1 221	338,97	420,6	
24	1 440	797,30	838,8	
25	3 114	13,27	6,5	
26	4 461	17,88	6,1	

Assay Class: High Sensitivity DNA Assay
Data Path: C:\...gh Sensitivity DNA Assay_DE13805677_2019-06-20_09-10-48.xad

Created: 20/06/2019 09:10:48
Modified: 20/06/2019 10:26:04


Electropherogram Summary Continued ...**... Peak table for sample 1 : R1**

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
27	 10 380	75,00	10,9	Upper Marker

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...gh Sensitivity DNA Assay_DE13805677_2019-06-20_09-10-48.xad

Created: 20/06/2019 09:10:48
 Modified: 20/06/2019 10:26:04

Electropherogram Summary Continued ...

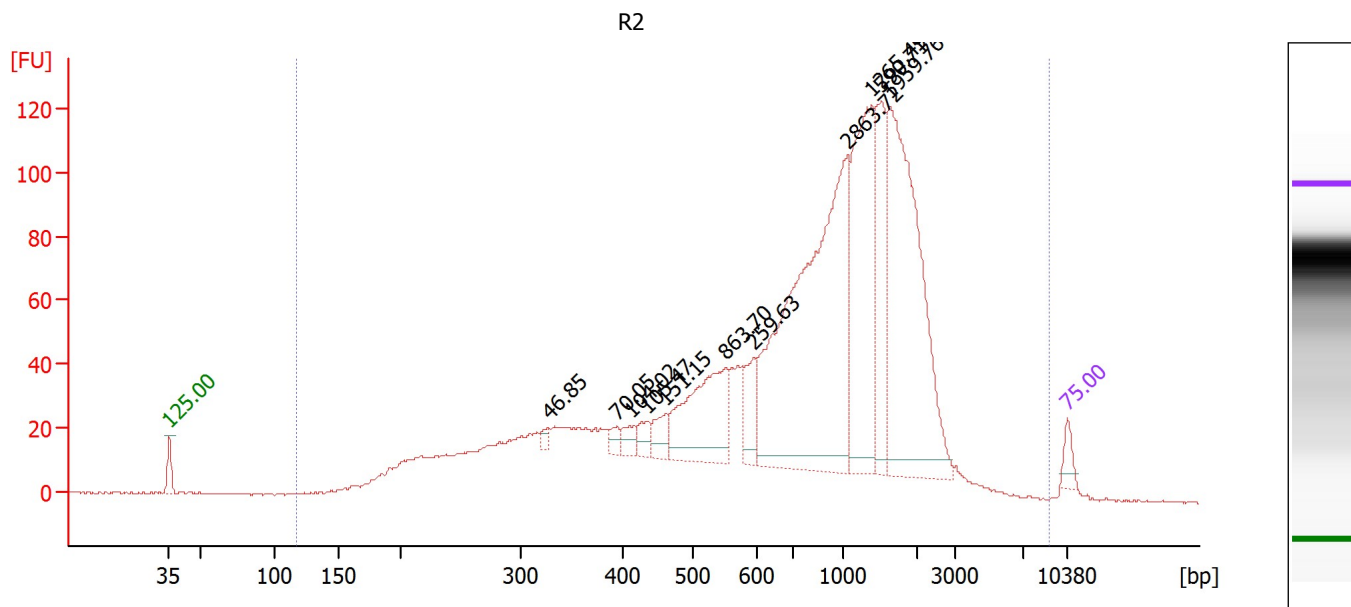

Overall Results for sample 2 : R2

Number of peaks found: 11 Corr. Area 1: 2 251,4
 Noise: 0,4


Peak table for sample 2 : R2

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	35	125,00	5 411,3	Lower Marker
2	327	46,85	217,4	
3	394	70,05	269,1	
4	411	104,02	383,7	
5	435	105,47	367,1	
6	461	151,15	496,9	
7	551	863,70	2 375,8	
8	595	259,63	661,2	
9	1 043	2 863,72	4 160,0	
10	1 367	1 265,49	1 402,8	
11	1 503	590,71	595,4	
12	1 614	1 959,76	1 839,9	
13	10 380	75,00	10,9	Upper Marker

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...gh Sensitivity DNA Assay_DE13805677_2019-06-20_09-10-48.xad

Created: 20/06/2019 09:10:48
 Modified: 20/06/2019 10:26:04

Electropherogram Summary Continued ...

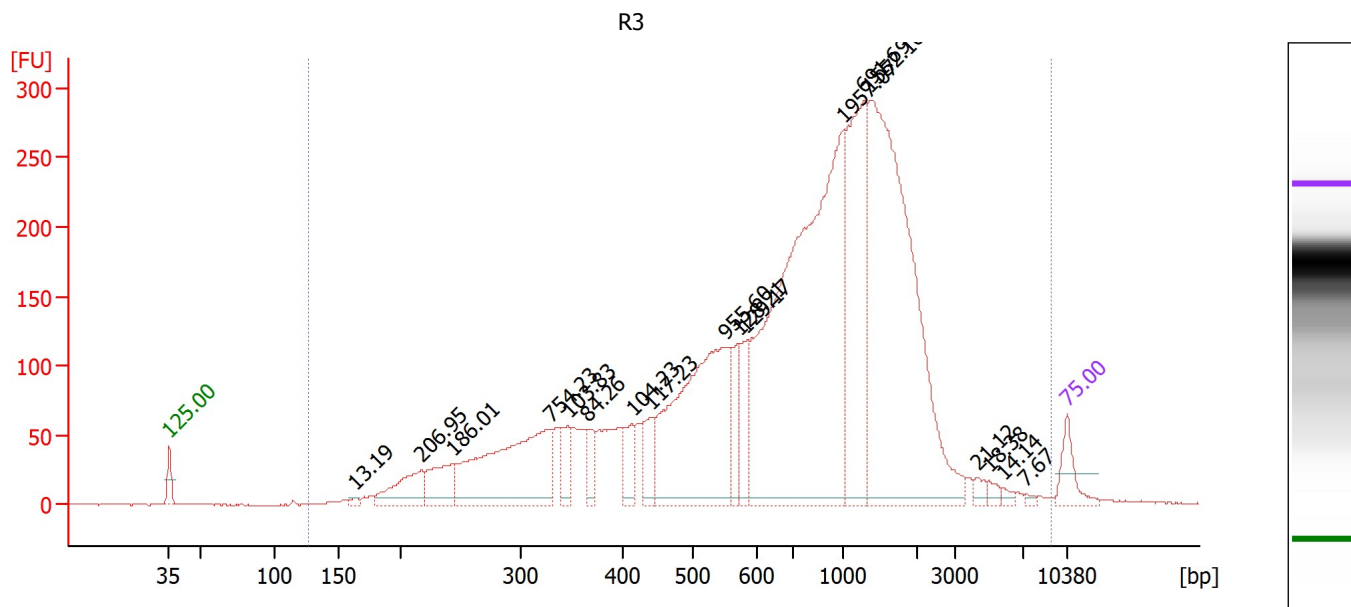

Overall Results for sample 3 : R3

Number of peaks found: 18 Corr. Area 1: 5 546,2
 Noise: 0,4


Peak table for sample 3 : R3

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	35	125,00	5 411,3	Lower Marker
2	164	13,19	122,1	
3	218	206,95	1 439,2	
4	244	186,01	1 154,6	
5	329	754,23	3 477,5	
6	346	103,83	454,3	
7	365	84,26	349,6	
8	414	104,23	381,5	
9	441	117,23	403,0	
10	551	955,60	2 627,2	
11	571	128,21	340,0	
12	580	129,17	337,1	
13	994	1 957,07	2 984,2	
14	1 270	691,69	825,4	
15	1 347	1 552,16	1 745,6	
16	4 345	21,12	7,4	
17	5 016	18,38	5,6	
18	5 835	14,14	3,7	
19	7 133	7,67	1,6	
20	10 380	75,00	10,9	Upper Marker

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...gh Sensitivity DNA Assay_DE13805677_2019-06-20_09-10-48.xad

Created: 20/06/2019 09:10:48
 Modified: 20/06/2019 10:26:04

Electropherogram Summary Continued ...

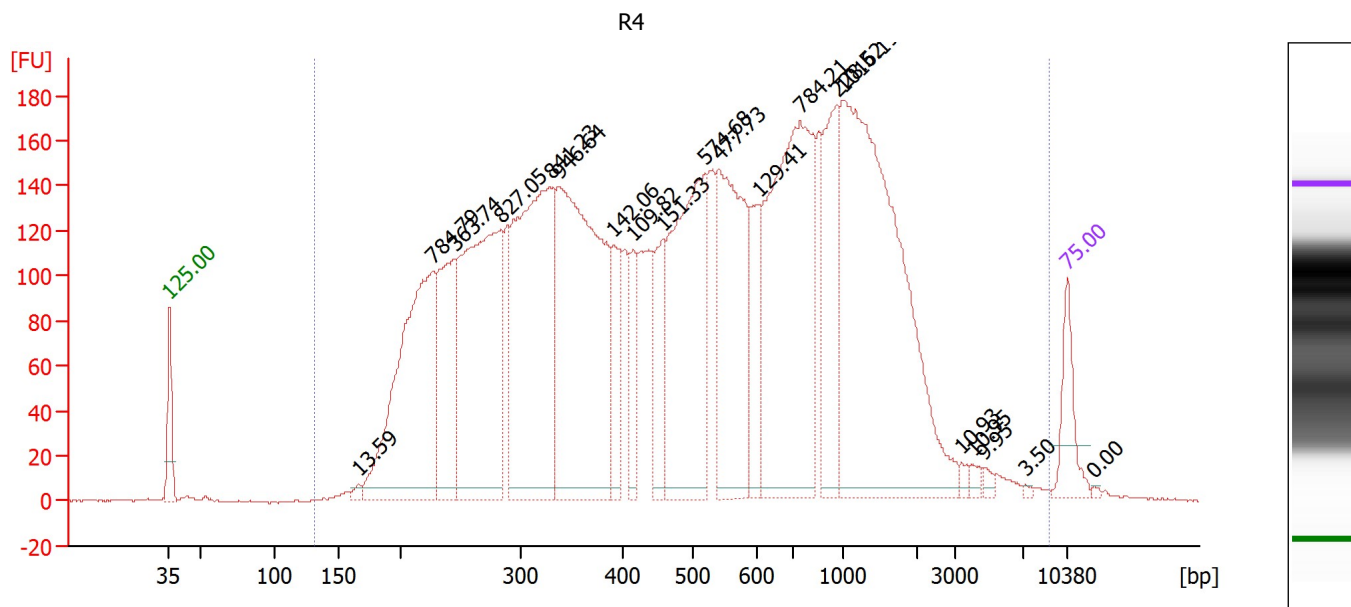

Overall Results for sample 4 : R4

Number of peaks found: 20 Corr. Area 1: 7 085,3
 Noise: 0,5


Peak table for sample 4 : R4

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	35	125,00	5 411,3	Lower Marker
2	167	13,59	123,1	
3	228	784,79	5 222,6	
4	245	363,74	2 250,7	
5	283	827,05	4 427,9	
6	329	841,23	3 878,6	
7	338	946,64	4 247,9	
8	391	142,06	550,2	
9	416	109,82	400,2	
10	458	151,33	500,9	
11	518	574,68	1 679,7	
12	540	477,73	1 340,0	
13	606	129,41	323,6	
14	741	784,21	1 603,2	
15	958	228,52	361,5	
16	993	1 016,19	1 551,0	
17	3 382	10,93	4,9	
18	4 068	10,95	4,1	
19	4 678	9,95	3,2	
20	7 156	3,50	0,7	
21	10 380	75,00	10,9	Upper Marker
22	12 445	0,00	0,0	

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...gh Sensitivity DNA Assay_DE13805677_2019-06-20_09-10-48.xad

Created: 20/06/2019 09:10:48
 Modified: 20/06/2019 10:26:04

Electropherogram Summary Continued ...

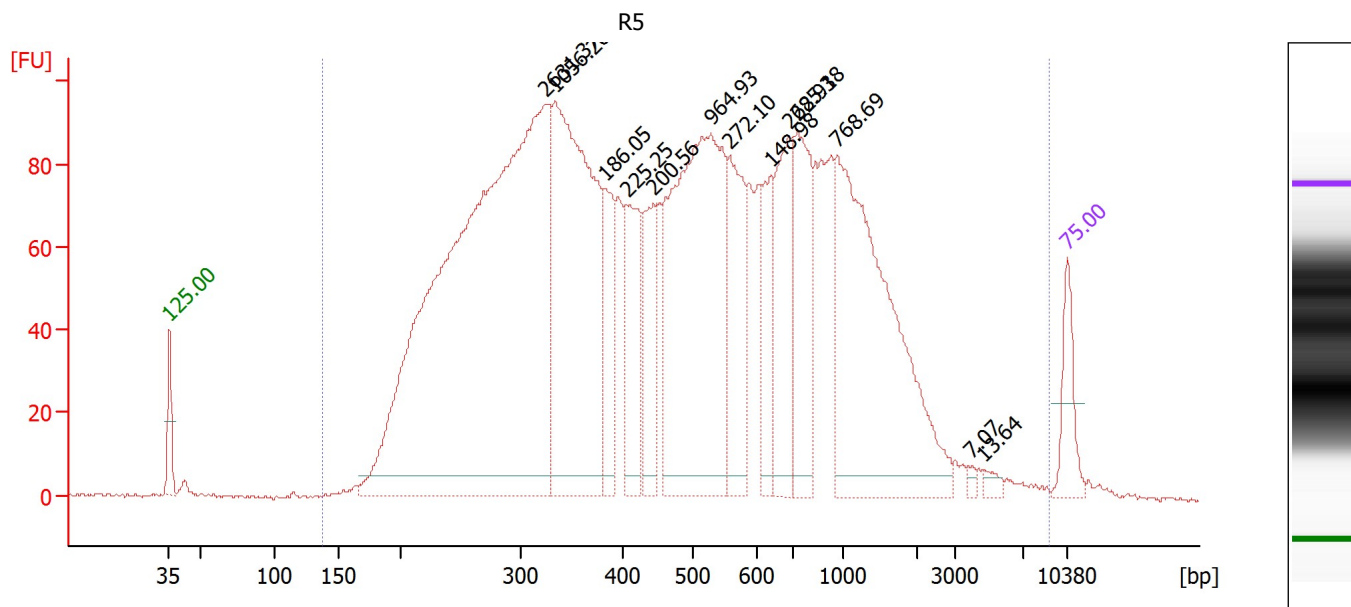

Overall Results for sample 5 : R5

Number of peaks found: 13 Corr. Area 1: 3 985,9
 Noise: 0,5


Peak table for sample 5 : R5

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	35	125,00	5 411,3	Lower Marker
2	323	2 631,37	12 330,1	
3	333	1 056,26	4 805,4	
4	382	186,05	737,7	
5	407	225,25	839,1	
6	444	200,56	684,1	
7	527	964,93	2 774,7	
8	556	272,10	741,5	
9	638	148,98	353,7	
10	688	262,91	579,3	
11	723	285,38	597,8	
12	960	768,69	1 213,5	
13	3 984	7,07	2,7	
14	4 671	13,64	4,4	
15	10 380	75,00	10,9	Upper Marker

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...gh Sensitivity DNA Assay_DE13805677_2019-06-20_09-10-48.xad

Created: 20/06/2019 09:10:48
 Modified: 20/06/2019 10:26:04

Electropherogram Summary Continued ...

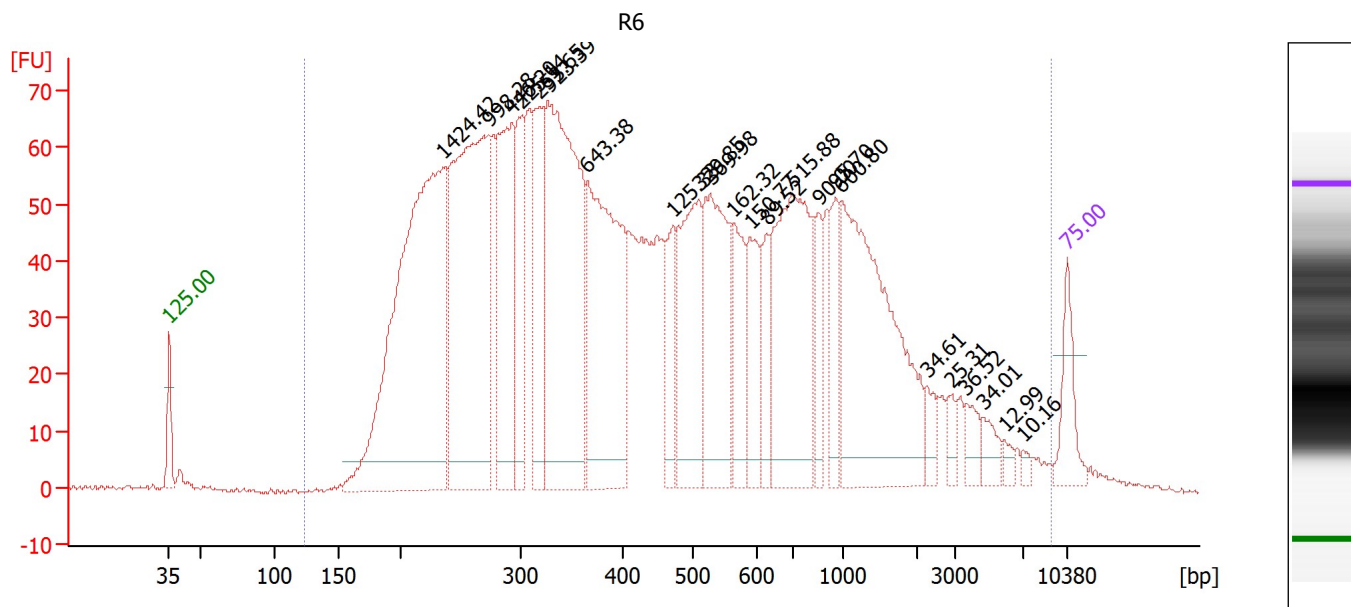

Overall Results for sample 6 : R6

Number of peaks found: 23 Corr. Area 1: 2 976,1
 Noise: 0,5


Peak table for sample 6 : R6

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	35	125,00	5 411,3	Lower Marker
2	236	1 424,42	9 161,6	
3	273	998,28	5 537,6	
4	292	446,20	2 315,8	
5	300	225,14	1 137,1	
6	318	253,65	1 208,4	
7	326	923,39	4 286,3	
8	366	643,38	2 665,4	
9	471	125,33	403,2	
10	508	329,85	982,9	
11	526	369,98	1 065,6	
12	562	162,32	437,3	
13	590	150,77	387,0	
14	626	89,52	216,7	
15	698	515,88	1 119,6	
16	847	90,00	161,1	
17	951	95,70	152,4	
18	982	600,80	926,9	
19	2 245	34,61	23,4	
20	2 879	25,31	13,3	
21	3 615	36,52	15,3	
22	4 643	34,01	11,1	
23	5 901	12,99	3,3	
24	6 968	10,16	2,2	
25	10 380	75,00	10,9	Upper Marker

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...gh Sensitivity DNA Assay_DE13805677_2019-06-20_09-10-48.xad

Created: 20/06/2019 09:10:48
 Modified: 20/06/2019 10:26:04

Electropherogram Summary Continued ...

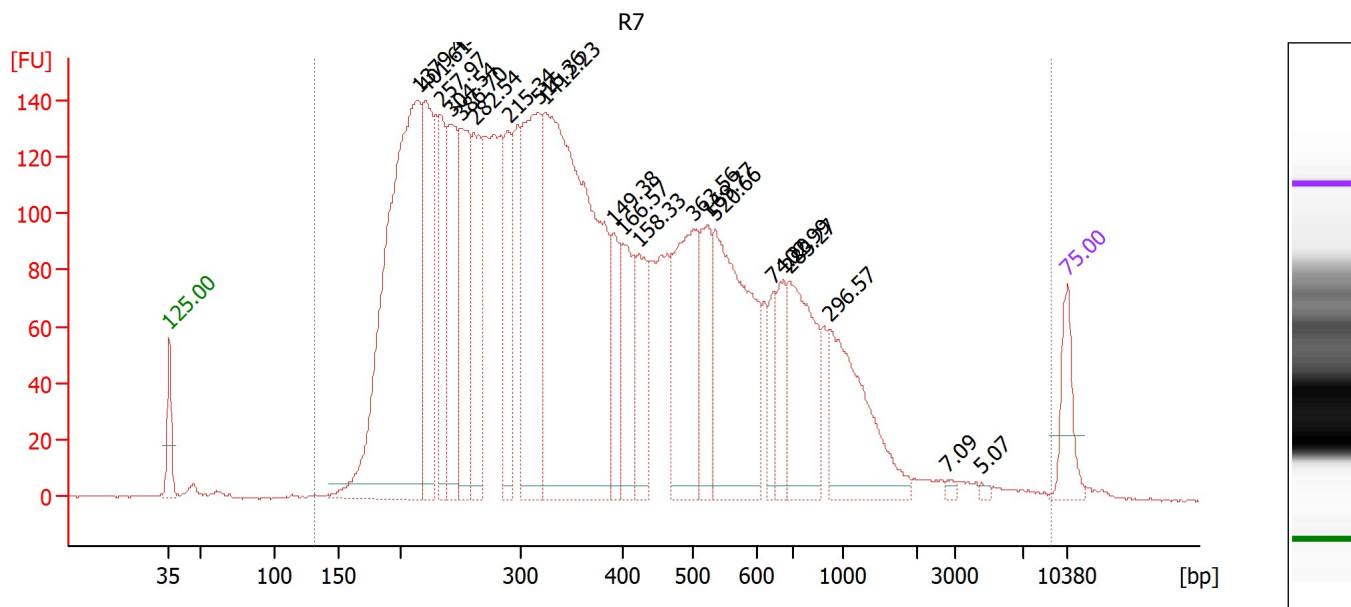

Overall Results for sample 7 : R7

Number of peaks found: 21 Corr. Area 1: 5 511,4
 Noise: 0,5


Peak table for sample 7 : R7

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	35	125,00	5 411,3	Lower Marker
2	215	1 379,45	9 717,3	
3	221	401,61	2 753,3	
4	233	257,97	1 674,8	
5	243	304,54	1 902,6	
6	251	386,70	2 338,1	
7	261	282,54	1 638,0	
8	289	215,34	1 127,8	
9	318	516,36	2 463,9	
10	324	1 412,23	6 604,3	
11	391	149,38	578,6	
12	402	166,57	627,6	
13	422	158,33	568,1	
14	500	363,56	1 101,9	
15	523	169,77	492,1	
16	534	520,66	1 476,8	
17	647	74,20	173,8	
18	672	102,99	232,3	
19	688	283,27	624,1	
20	909	296,57	494,1	
21	2 784	7,09	3,9	
22	4 556	5,07	1,7	
23	10 380	75,00	10,9	Upper Marker

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...gh Sensitivity DNA Assay_DE13805677_2019-06-20_09-10-48.xad

Created: 20/06/2019 09:10:48
 Modified: 20/06/2019 10:26:04

Electropherogram Summary Continued ...

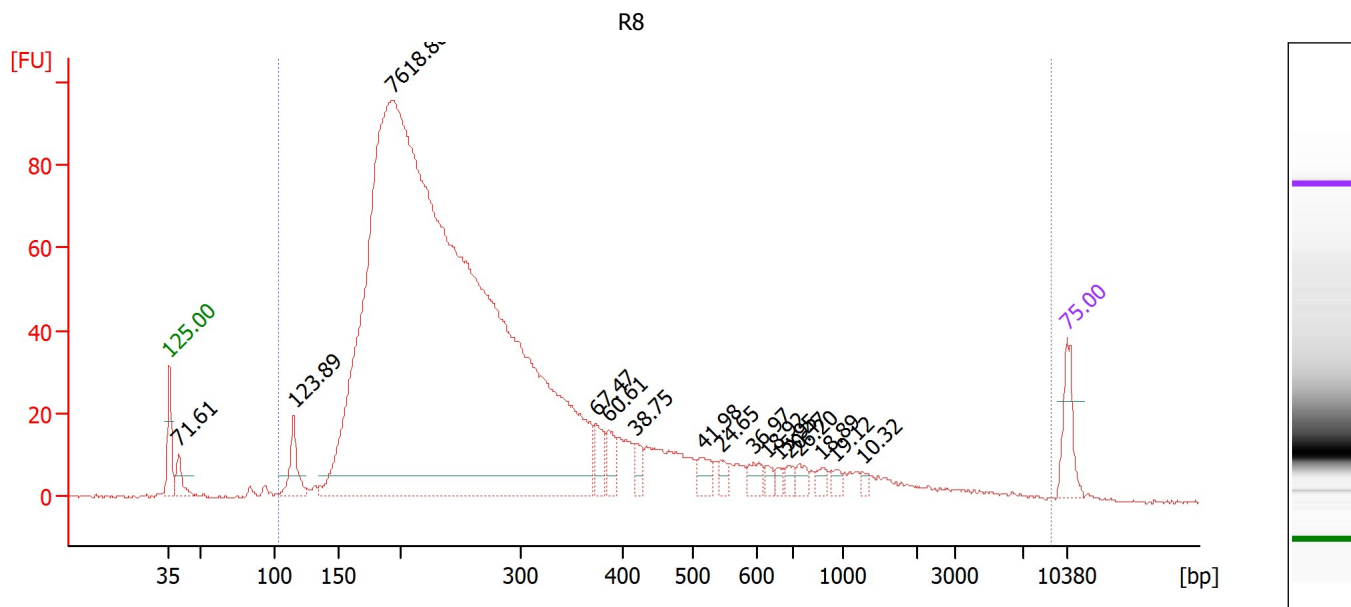

Overall Results for sample 8 : R8

Number of peaks found: 16 Corr. Area 1: 1 980,0
 Noise: 0,5


Peak table for sample 8 : R8

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	35	125,00	5 411,3	Lower Marker
2	39	71,61	2 747,2	
3	116	123,89	1 622,7	
4	194	7 618,86	59 382,8	
5	374	67,47	273,1	
6	387	60,61	237,3	
7	418	38,75	140,5	
8	515	41,98	123,6	
9	542	24,65	68,9	
10	596	36,97	94,0	
11	628	18,92	45,7	
12	659	15,95	36,7	
13	685	20,47	45,3	
14	733	26,20	54,2	
15	867	18,89	33,0	
16	948	19,12	30,6	
17	1 248	10,32	12,5	
18	10 380	75,00	10,9	Upper Marker

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...gh Sensitivity DNA Assay_DE13805677_2019-06-20_09-10-48.xad

Created: 20/06/2019 09:10:48
 Modified: 20/06/2019 10:26:04

Electropherogram Summary Continued ...

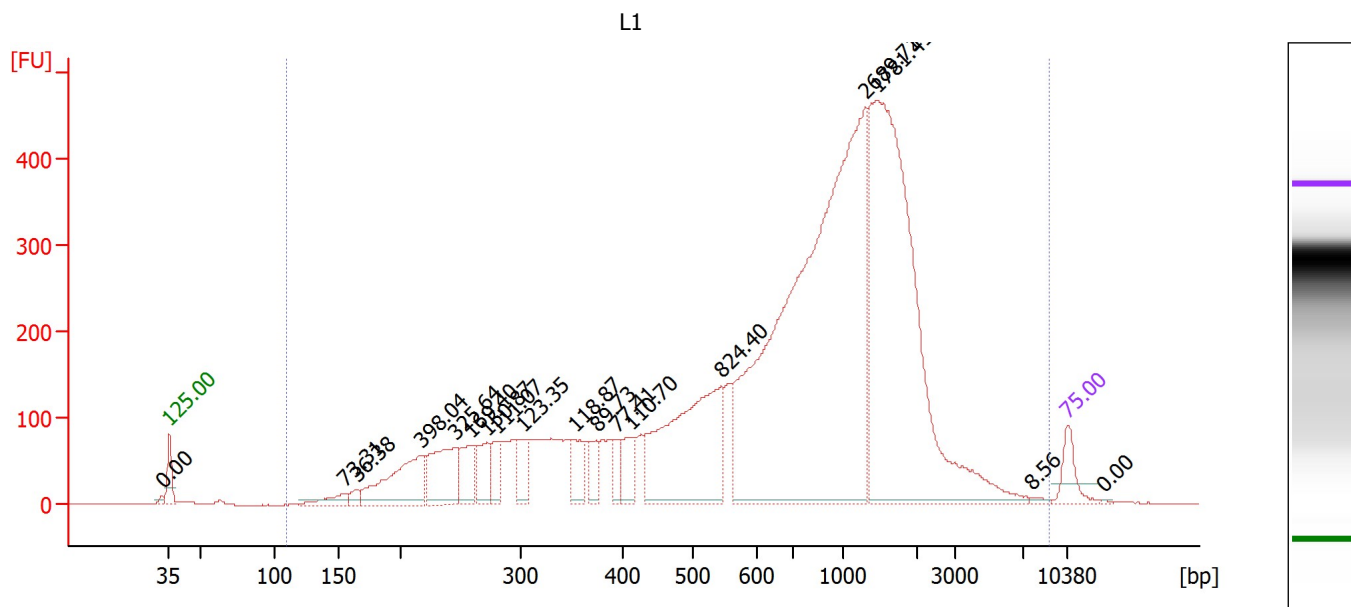

Overall Results for sample 9 : L1


Number of peaks found: 18 Corr. Area 1: 8 381,2
 Noise: 0,4

Peak table for sample 9 : L1

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	33	0,00	0,0	
2	35	125,00	5 411,3	Lower Marker
3	156	73,31	712,6	
4	165	36,38	333,5	
5	218	398,04	2 767,2	
6	245	325,64	2 011,7	
7	259	169,40	990,3	
8	272	150,87	842,0	
9	281	111,07	599,7	
10	302	123,35	619,3	
11	353	118,87	510,8	
12	374	89,73	363,0	
13	394	77,41	297,9	
14	413	110,70	406,1	
15	545	824,40	2 292,4	
16	1 282	2 689,71	3 177,9	
17	1 441	1 781,41	1 873,6	
18	7 668	8,56	1,7	
19	10 380	75,00	10,9	Upper Marker
20	13 243	0,00	0,0	

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...gh Sensitivity DNA Assay_DE13805677_2019-06-20_09-10-48.xad

Created: 20/06/2019 09:10:48
 Modified: 20/06/2019 10:26:04

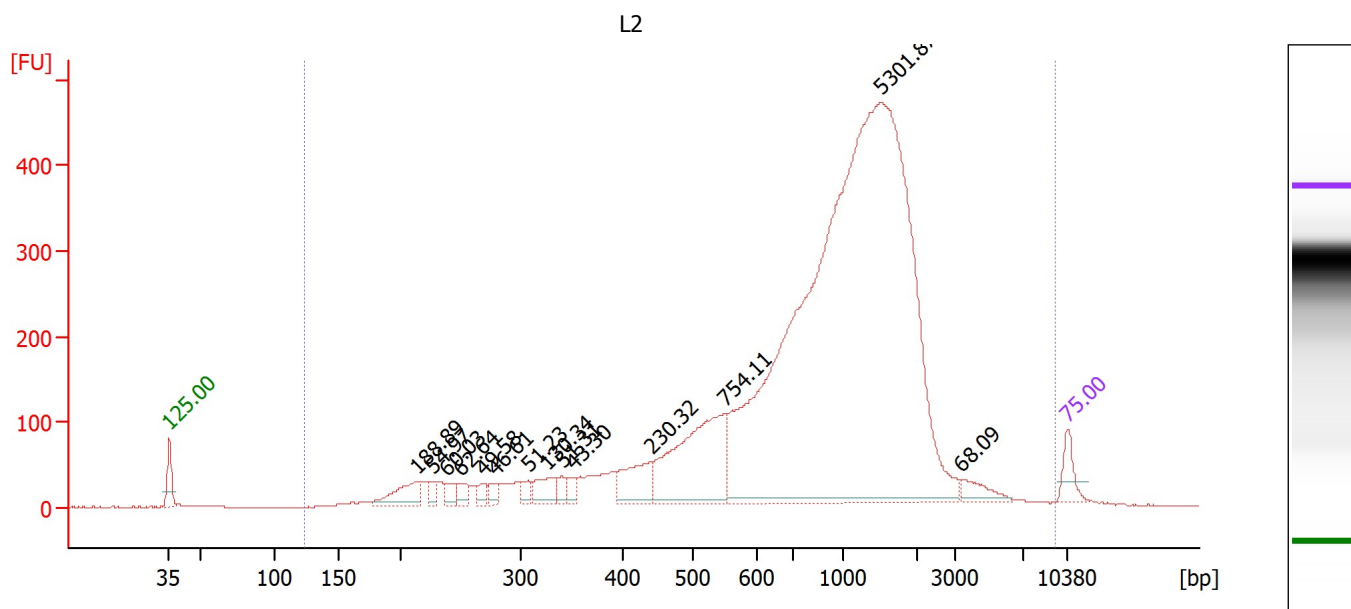Electropherogram Summary Continued ...**Overall Results for sample 10 : L2**

Number of peaks found: 14 Corr. Area 1: 6 623,3
 Noise: 0,5


Peak table for sample 10 : L2

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	35	125,00	5 411,3	Lower Marker
2	214	188,89	1 338,3	
3	227	54,97	367,5	
4	238	60,03	381,5	
5	250	62,64	379,5	
6	268	49,58	280,1	
7	278	46,61	254,2	
8	307	51,23	253,1	
9	326	130,34	606,0	
10	341	51,31	228,2	
11	352	43,30	186,6	
12	440	230,32	792,9	
13	548	754,11	2 083,9	
14	1 496	5 301,87	5 371,4	
15	3 388	68,09	30,4	
16	10 380	75,00	10,9	Upper Marker

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...gh Sensitivity DNA Assay_DE13805677_2019-06-20_09-10-48.xad

Created: 20/06/2019 09:10:48
 Modified: 20/06/2019 10:26:04

Electropherogram Summary Continued ...

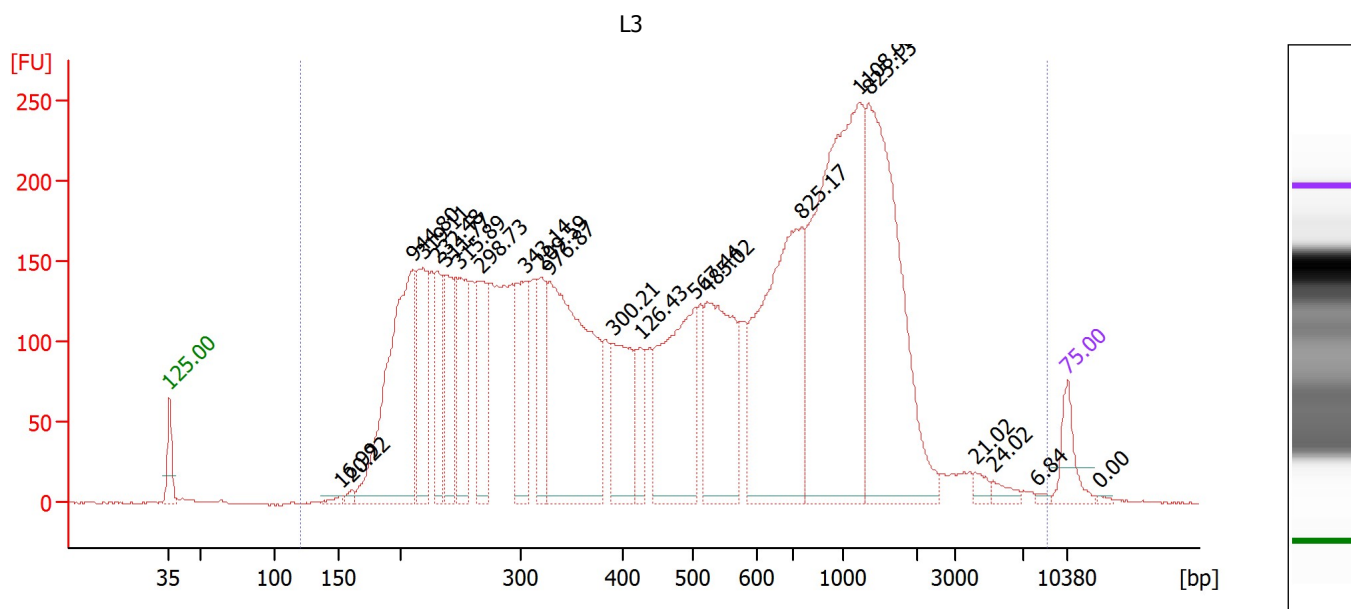

Overall Results for sample 11 : L3


Number of peaks found: 22 Corr. Area 1: 7 816,5
 Noise: 0,4

Peak table for sample 11 : L3

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	35	125,00	5 411,3	Lower Marker
2	152	16,99	169,1	
3	161	20,22	190,2	
4	211	944,80	6 791,1	
5	219	319,11	2 209,8	
6	231	232,48	1 527,9	
7	237	311,77	1 989,2	
8	249	315,89	1 920,5	
9	266	298,73	1 699,8	
10	304	343,14	1 708,1	
11	320	209,59	993,1	
12	327	976,87	4 520,1	
13	391	300,21	1 163,6	
14	425	126,43	450,5	
15	502	567,44	1 714,3	
16	522	485,02	1 407,5	
17	748	825,17	1 672,5	
18	1 205	1 108,96	1 394,8	
19	1 327	825,13	941,9	
20	4 217	21,02	7,6	
21	5 240	24,02	6,9	
22	8 078	6,84	1,3	
23	10 380	75,00	10,9	Upper Marker
24	12 932	0,00	0,0	

Assay Class: High Sensitivity DNA Assay
Data Path: C:\...gh Sensitivity DNA Assay_DE13805677_2019-06-20_09-10-48.xad

Created: 20/06/2019 09:10:48
Modified: 20/06/2019 10:26:04

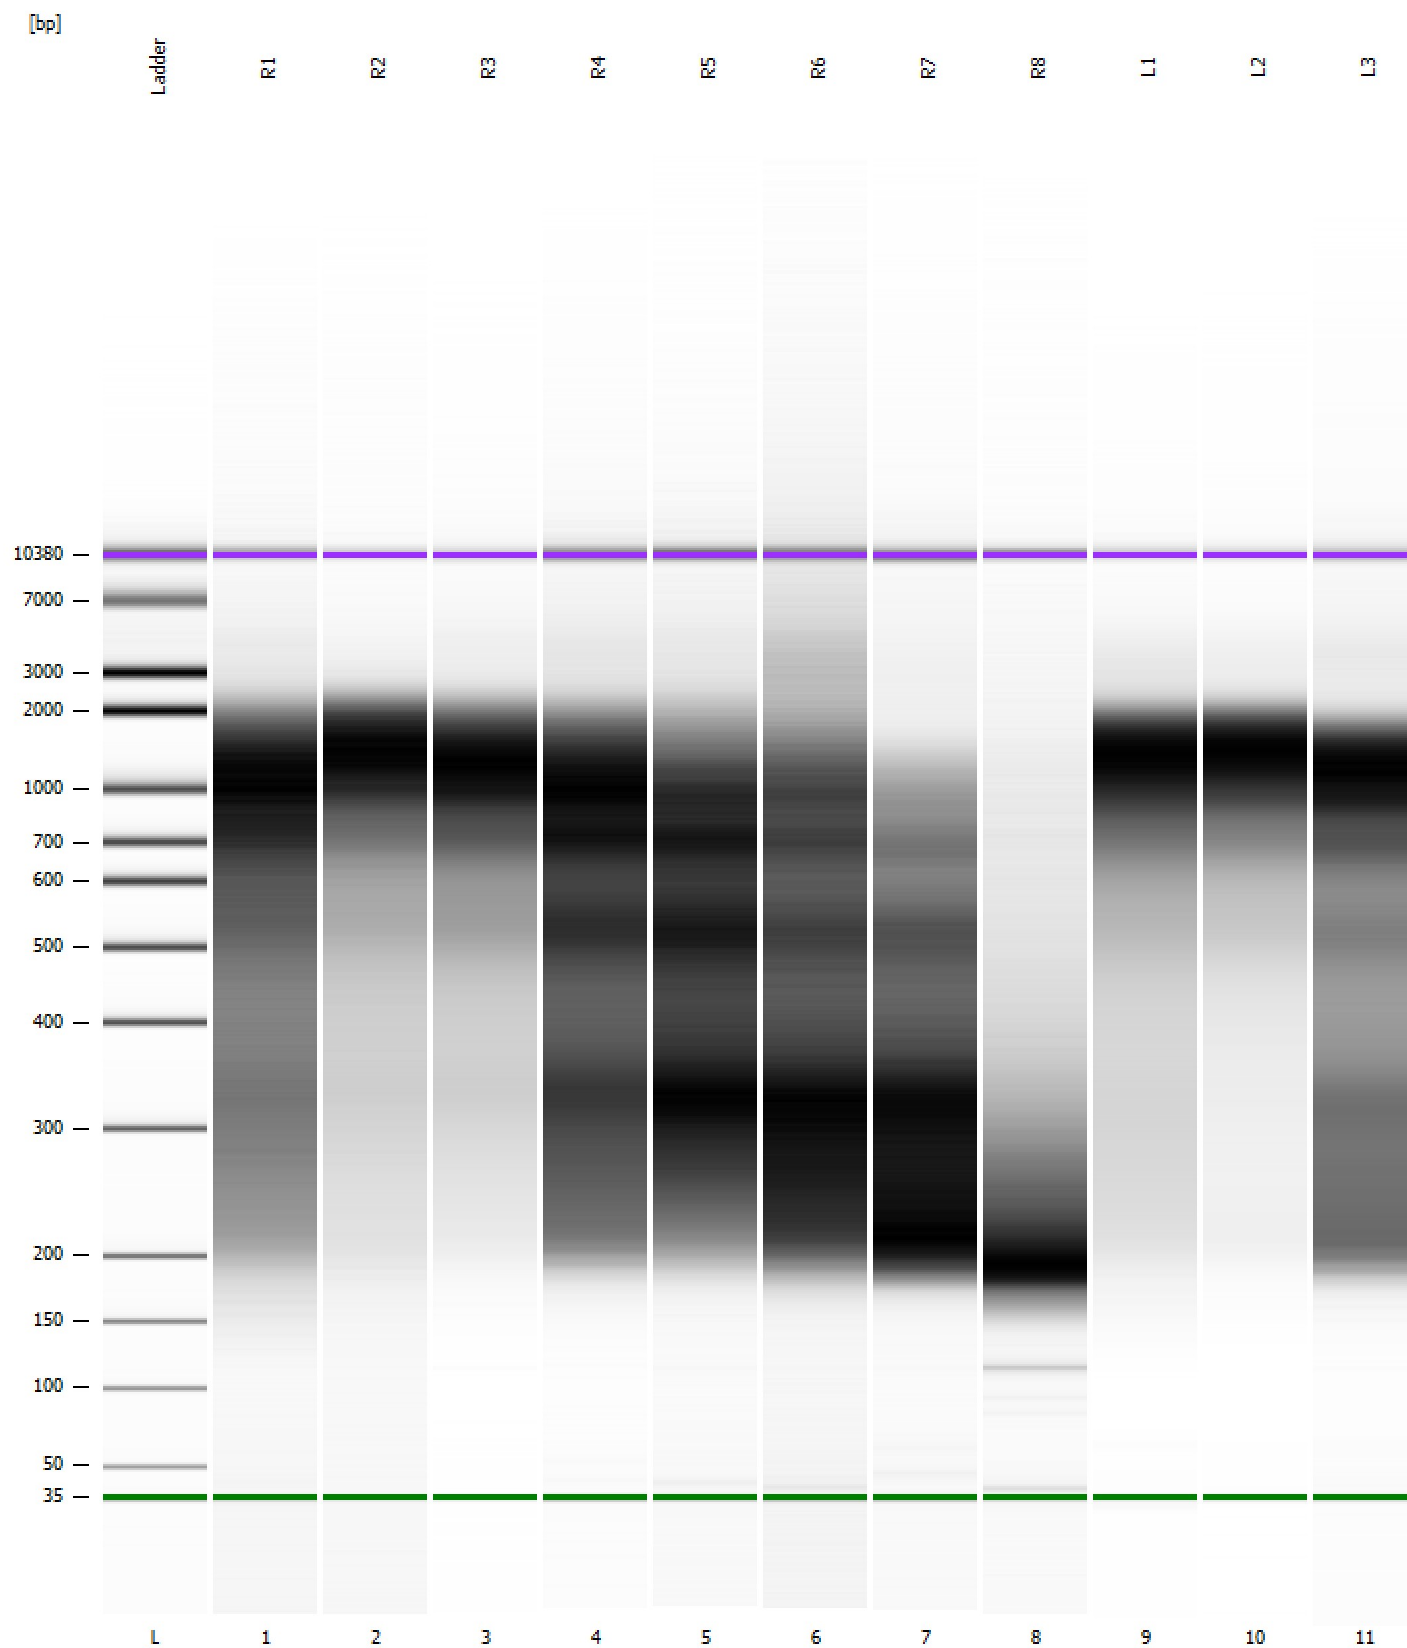Gel Image

Assay Class: High Sensitivity DNA Assay Created: 20/06/2019 09:10:48
 Data Path: C:\...gh Sensitivity DNA Assay_DE13805677_2019-06-20_09-10-48.xad Modified: 20/06/2019 10:26:04

Run Logbook

Description	Number	Source	Category	Sub Category	Time	Time Zone	User	Host
Run ended on port 3 (Number of wells acquired: 12)		Instrument	Run		20/06/2019 09:52:06	(GMT +02:00) Paris, Madrid	cnrs	cnrs-PC
Run started on port 3 (File: C:\Program Files (x86)\Agilent\2100 bioanalyzer\2100 expert\data\jfa\NGS_jfa\NGS2019\juin_2019\2019-06-20\CG_Ro_1_High Sensitivity DNA Assay_DE13805677_2019-06-20_09-10-48.xad)		Instrument	Run		20/06/2019 09:10:53	(GMT +02:00) Paris, Madrid	cnrs	cnrs-PC
Product Number : G2939A		Instrument	Run		20/06/2019 09:10:53	(GMT +02:00) Paris, Madrid	cnrs	cnrs-PC
Name :		Instrument	Run		20/06/2019 09:10:53	(GMT +02:00) Paris, Madrid	cnrs	cnrs-PC
Vendor : Agilent Technologies		Instrument	Run		20/06/2019 09:10:53	(GMT +02:00) Paris, Madrid	cnrs	cnrs-PC
Serial# : DE13805677		Instrument	Run		20/06/2019 09:10:53	(GMT +02:00) Paris, Madrid	cnrs	cnrs-PC
Firmware : C.01.069		Instrument	Run		20/06/2019 09:10:53	(GMT +02:00) Paris, Madrid	cnrs	cnrs-PC
Cartridge : Electrode		Instrument	Run		20/06/2019 09:10:53	(GMT +02:00) Paris, Madrid	cnrs	cnrs-PC