


Assay Class: High Sensitivity DNA Assay  
Data Path: C:\...gh Sensitivity DNA Assay\_DE13805677\_2019-06-20\_10-12-12.xad

Created: 20/06/2019 10:12:12  
Modified: 20/06/2019 11:17:47

### Electrophoresis File Run Summary

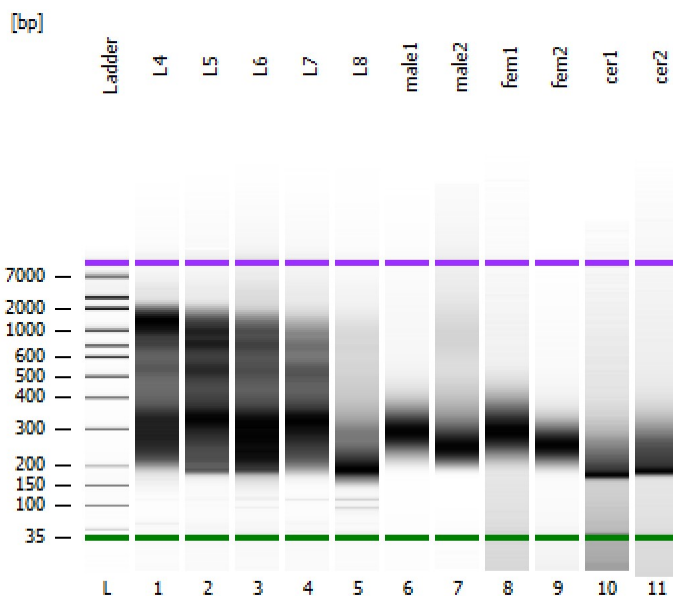

#### Instrument Information:

Instrument Name: DE13805677  
Serial#: DE13805677

Firmware: C.01.069  
Type: G2939A

#### Assay Information:

Assay Origin Path: C:\Program Files (x86)\Agilent\2100 bioanalyzer\2100 expert\assays\dsDNA\High Sensitivity DNA.xsy

Assay Class: High Sensitivity DNA Assay

Version: 1.03


Assay Comments: Copyright © 2003-2010 Agilent Technologies

#### Chip Information:

Chip Lot #:

Reagent Kit Lot #:

Chip Comments:

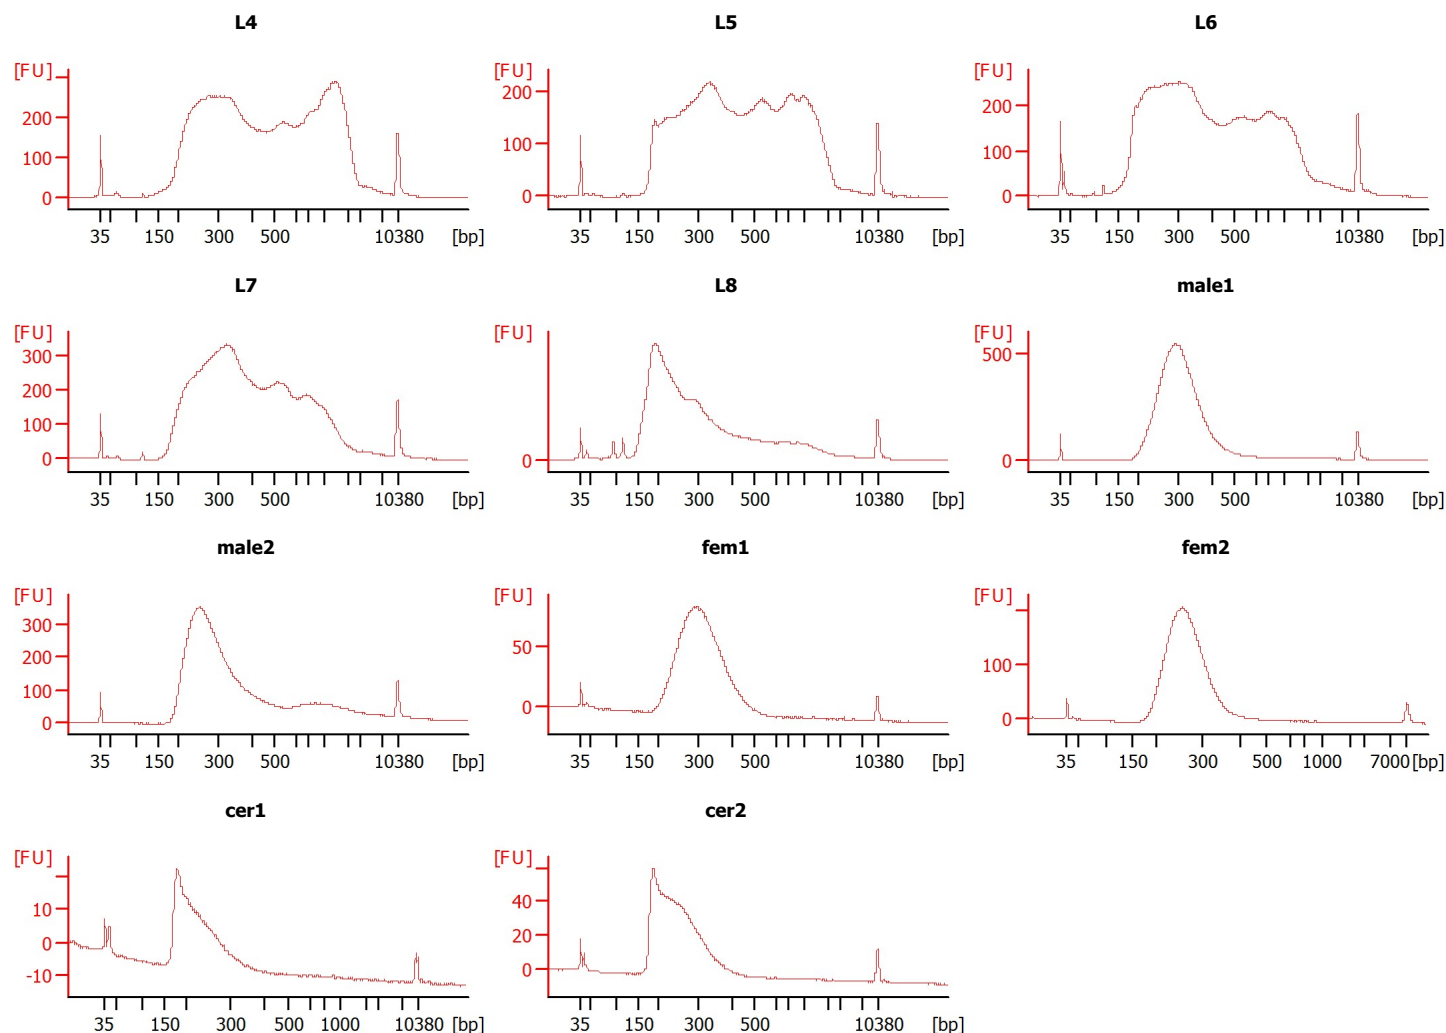

Assay Class: High Sensitivity DNA Assay  
Data Path: C:\...gh Sensitivity DNA Assay\_DE13805677\_2019-06-20\_10-12-12.xad

Created: 20/06/2019 10:12:12  
Modified: 20/06/2019 11:17:47

**Electrophoresis File Run Summary (Chip Summary)**

| Sample Name | Sample Comment | Rest. Digest             | Status            | Observation | Result Label | Result Color |
|-------------|----------------|--------------------------|-------------------|-------------|--------------|--------------|
| L4          |                | <input type="checkbox"/> | ✓                 |             |              |              |
| L5          |                | <input type="checkbox"/> | ✓                 |             |              |              |
| L6          |                | <input type="checkbox"/> | ✓                 |             |              |              |
| L7          |                | <input type="checkbox"/> | ✓                 |             |              |              |
| L8          |                | <input type="checkbox"/> | ✓                 |             |              |              |
| male1       |                | <input type="checkbox"/> | ✓                 |             |              |              |
| male2       |                | <input type="checkbox"/> | ✓                 |             |              |              |
| fem1        |                | <input type="checkbox"/> | ✓                 |             |              |              |
| fem2        |                | <input type="checkbox"/> | ✓                 |             |              |              |
| cer1        |                | <input type="checkbox"/> | ✓                 |             |              |              |
| cer2        |                | <input type="checkbox"/> | ✓                 |             |              |              |
| Ladder      |                | <input type="checkbox"/> | ✓                 |             |              |              |
| Chip Lot #  |                |                          | Reagent Kit Lot # |             |              |              |

Chip Comments :

Assay Class: High Sensitivity DNA Assay  
Data Path: C:\...gh Sensitivity DNA Assay\_DE13805677\_2019-06-20\_10-12-12.xad

Created: 20/06/2019 10:12:12  
Modified: 20/06/2019 11:17:47

## Electrophoresis Assay Details

### General Analysis Settings

Number of Available Sample and Ladder Wells (Max.) : 12  
Minimum Visible Range [s] : 32  
Maximum Visible Range [s] : 138  
Start Analysis Time Range [s] : 33  
End Analysis Time Range [s] : 137,5  
Ladder Concentration [pg/μl] : 1950  
Uses Standard Area for Ladder Fragments  
Lower Marker Concentration [pg/μl] : 125  
Upper Marker Concentration [pg/μl] : 75  
Used Upper Marker for Quantitation  
Standard Curve Fit is Point to Point  
Show Data Aligned to Lower and Upper Marker

### Integrator Settings

Integration Start Time [s] : 33,05  
Integration End Time [s] : 137  
Slope Threshold : 0,8  
Height Threshold [FU] : 5  
Area Threshold : 0,1  
Width Threshold [s] : 0,6  
Baseline Plateau [s] : 0,5


### Filter Settings

Filter Width [s] : 0,5  
Polynomial Order : 4

### Ladder

| Ladder Peak | Size  | Area |
|-------------|-------|------|
| 1           | 35    | 160  |
| 2           | 50    | 210  |
| 3           | 100   | 208  |
| 4           | 150   | 221  |
| 5           | 200   | 242  |
| 6           | 300   | 270  |
| 7           | 400   | 305  |
| 8           | 500   | 306  |
| 9           | 600   | 336  |
| 10          | 700   | 321  |
| 11          | 1000  | 366  |
| 12          | 2000  | 413  |
| 13          | 3000  | 411  |
| 14          | 7000  | 400  |
| 15          | 10380 | 214  |

Created: 20/06/2019 10:12:12  
Modified: 20/06/2019 11:17:47

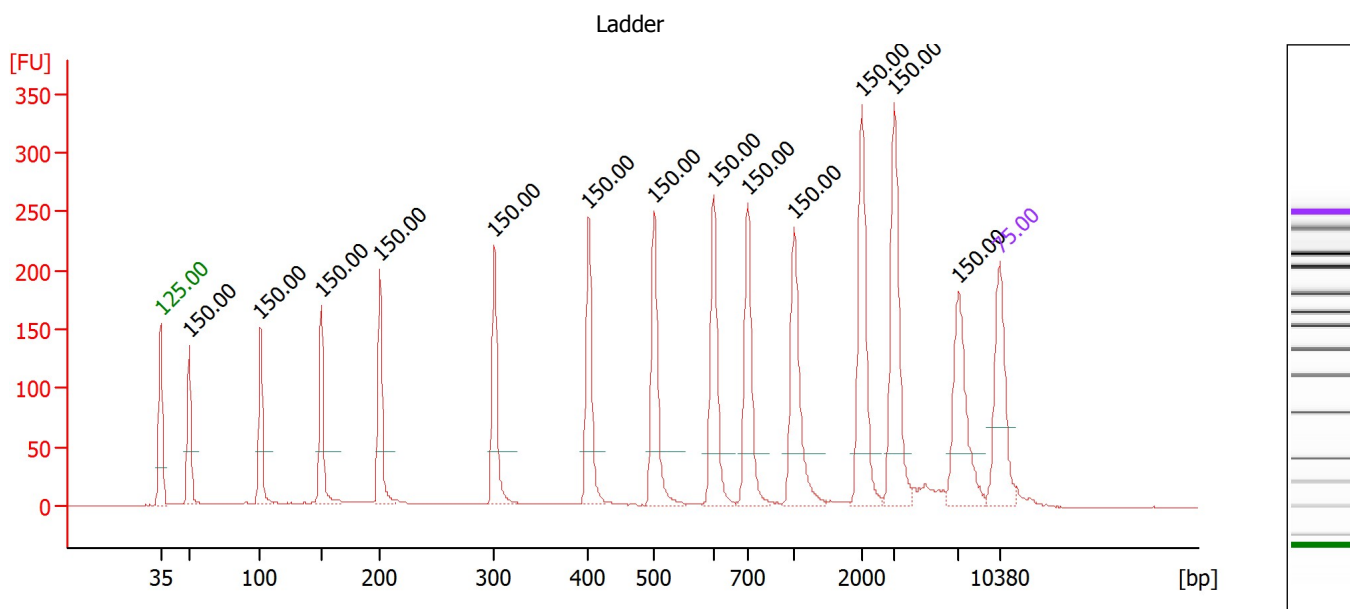


Noise: 0,4

| Peak |   | Size [bp] | Conc. [pg/μl] | Molarity [pmol/l] | Observations |
|------|---|-----------|---------------|-------------------|--------------|
| 1    | ◀ | 35        | 125,00        | 5 411,3           | Lower Marker |
| 2    | █ | 50        | 150,00        | 4 545,5           | Ladder Peak  |
| 3    | █ | 100       | 150,00        | 2 272,7           | Ladder Peak  |
| 4    | █ | 150       | 150,00        | 1 515,2           | Ladder Peak  |
| 5    | █ | 200       | 150,00        | 1 136,4           | Ladder Peak  |
| 6    | █ | 300       | 150,00        | 757,6             | Ladder Peak  |
| 7    | █ | 400       | 150,00        | 568,2             | Ladder Peak  |
| 8    | █ | 500       | 150,00        | 454,5             | Ladder Peak  |
| 9    | █ | 600       | 150,00        | 378,8             | Ladder Peak  |
| 10   | █ | 700       | 150,00        | 324,7             | Ladder Peak  |
| 11   | █ | 1 000     | 150,00        | 227,3             | Ladder Peak  |
| 12   | █ | 2 000     | 150,00        | 113,6             | Ladder Peak  |
| 13   | █ | 3 000     | 150,00        | 75,8              | Ladder Peak  |
| 14   | █ | 7 000     | 150,00        | 32,5              | Ladder Peak  |
| 15   | ▶ | 10 380    | 75,00         | 10,9              | Upper Marker |

Assay Class: High Sensitivity DNA Assay  
 Data Path: C:\...gh Sensitivity DNA Assay\_DE13805677\_2019-06-20\_10-12-12.xad

Created: 20/06/2019 10:12:12  
 Modified: 20/06/2019 11:17:47

### Electropherogram Summary Continued ...

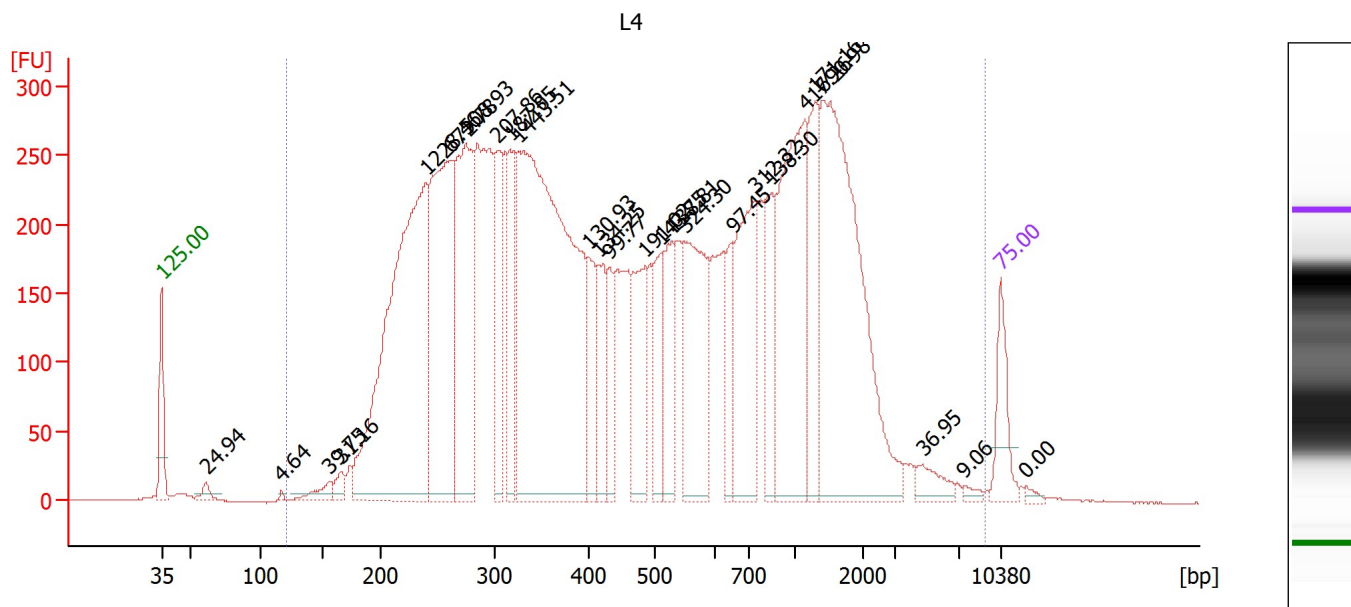

### Overall Results for sample 1 : L4

Number of peaks found: 26      Corr. Area 1: 11 980,6  
 Noise: 0,6

### Peak table for sample 1 : L4

| Peak | Size [bp] | Conc. [pg/μl] | Molarity [pmol/l] | Observations |
|------|-----------|---------------|-------------------|--------------|
| 1    | 35        | 125,00        | 5 411,3           | Lower Marker |
| 2    | 61        | 24,94         | 621,2             |              |
| 3    | 116       | 4,64          | 60,3              |              |
| 4    | 155       | 39,75         | 387,4             |              |
| 5    | 166       | 31,16         | 284,3             |              |
| 6    | 239       | 1 228,46      | 7 782,4           |              |
| 7    | 261       | 672,78        | 3 910,2           |              |
| 8    | 274       | 508,93        | 2 814,0           |              |
| 9    | 302       | 207,86        | 1 042,6           |              |
| 10   | 315       | 187,05        | 899,1             |              |
| 11   | 324       | 1 443,51      | 6 751,3           |              |
| 12   | 399       | 130,93        | 497,2             |              |
| 13   | 414       | 134,25        | 491,7             |              |
| 14   | 430       | 99,77         | 351,8             |              |
| 15   | 485       | 191,02        | 596,7             |              |
| 16   | 510       | 143,75        | 427,0             |              |
| 17   | 528       | 138,81        | 398,5             |              |
| 18   | 548       | 324,30        | 895,9             |              |
| 19   | 653       | 97,45         | 226,0             |              |
| 20   | 735       | 312,32        | 643,9             |              |
| 21   | 845       | 138,30        | 248,0             |              |
| 22   | 1 149     | 417,26        | 550,1             |              |
| 23   | 1 288     | 171,16        | 201,3             |              |
| 24   | 1 401     | 690,98        | 747,2             |              |
| 25   | 4 665     | 36,95         | 12,0              |              |
| 26   | 7 348     | 9,06          | 1,9               |              |

Assay Class: High Sensitivity DNA Assay  
Data Path: C:\...gh Sensitivity DNA Assay\_DE13805677\_2019-06-20\_10-12-12.xad

Created: 20/06/2019 10:12:12  
Modified: 20/06/2019 11:17:47


**Electropherogram Summary Continued ...****... Peak table for sample 1 : L4**

| Peak | Size [bp] | Conc. [pg/μl] | Molarity [pmol/l] | Observations |
|------|-----------|---------------|-------------------|--------------|
| 27   | 10 380    | 75,00         | 10,9              | Upper Marker |
| 28   | 12 401    | 0,00          | 0,0               |              |

Assay Class: High Sensitivity DNA Assay  
 Data Path: C:\...gh Sensitivity DNA Assay\_DE13805677\_2019-06-20\_10-12-12.xad

Created: 20/06/2019 10:12:12  
 Modified: 20/06/2019 11:17:47

### Electropherogram Summary Continued ...

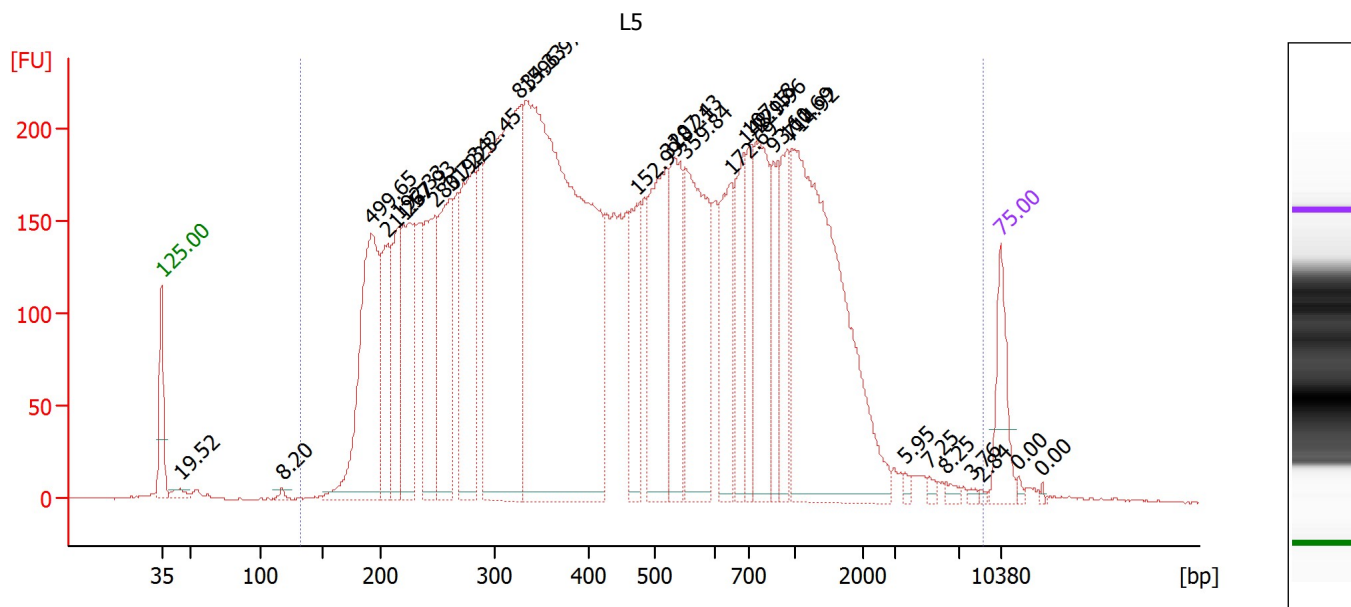

### Overall Results for sample 2 : L5

Number of peaks found: 29      Corr. Area 1: 9 572,7  
 Noise: 0,5

### Peak table for sample 2 : L5

| Peak | Size [bp] | Conc. [pg/μl] | Molarity [pmol/l] | Observations |
|------|-----------|---------------|-------------------|--------------|
| 1    | 35        | 125,00        | 5 411,3           | Lower Marker |
| 2    | 45        | 19,52         | 659,3             |              |
| 3    | 117       | 8,20          | 106,3             |              |
| 4    | 192       | 499,65        | 3 947,3           |              |
| 5    | 205       | 211,57        | 1 560,1           |              |
| 6    | 215       | 192,33        | 1 354,0           |              |
| 7    | 225       | 267,93        | 1 804,5           |              |
| 8    | 247       | 280,72        | 1 721,8           |              |
| 9    | 261       | 319,23        | 1 854,1           |              |
| 10   | 281       | 342,45        | 1 843,9           |              |
| 11   | 325       | 834,33        | 3 891,4           |              |
| 12   | 332       | 1 596,97      | 7 280,3           |              |
| 13   | 471       | 152,99        | 491,9             |              |
| 14   | 519       | 318,21        | 929,8             |              |
| 15   | 532       | 207,43        | 590,4             |              |
| 16   | 550       | 359,84        | 991,1             |              |
| 17   | 646       | 172,69        | 405,1             |              |
| 18   | 686       | 148,15        | 327,3             |              |
| 19   | 707       | 107,18        | 229,6             |              |
| 20   | 764       | 229,96        | 455,9             |              |
| 21   | 859       | 93,60         | 165,1             |              |
| 22   | 950       | 111,69        | 178,1             |              |
| 23   | 977       | 714,92        | 1 108,8           |              |
| 24   | 3 599     | 5,95          | 2,5               |              |
| 25   | 5 138     | 7,25          | 2,1               |              |
| 26   | 6 091     | 8,25          | 2,1               |              |

Assay Class: High Sensitivity DNA Assay  
Data Path: C:\...gh Sensitivity DNA Assay\_DE13805677\_2019-06-20\_10-12-12.xad

Created: 20/06/2019 10:12:12  
Modified: 20/06/2019 11:17:47


**Electropherogram Summary Continued ...****... Peak table for sample 2 : L5**

| Peak | Size [bp]                                                                                | Conc. [pg/μl] | Molarity [pmol/l] | Observations |
|------|------------------------------------------------------------------------------------------|---------------|-------------------|--------------|
| 27   | 7 924                                                                                    | 3,76          | 0,7               |              |
| 28   | 8 791                                                                                    | 2,84          | 0,5               |              |
| 29   |  10 380 | 75,00         | 10,9              | Upper Marker |
| 30   | 11 777                                                                                   | 0,00          | 0,0               |              |
| 31   | 13 751                                                                                   | 0,00          | 0,0               |              |



Assay Class: High Sensitivity DNA Assay  
 Data Path: C:\...gh Sensitivity DNA Assay\_DE13805677\_2019-06-20\_10-12-12.xad

Created: 20/06/2019 10:12:12  
 Modified: 20/06/2019 11:17:47

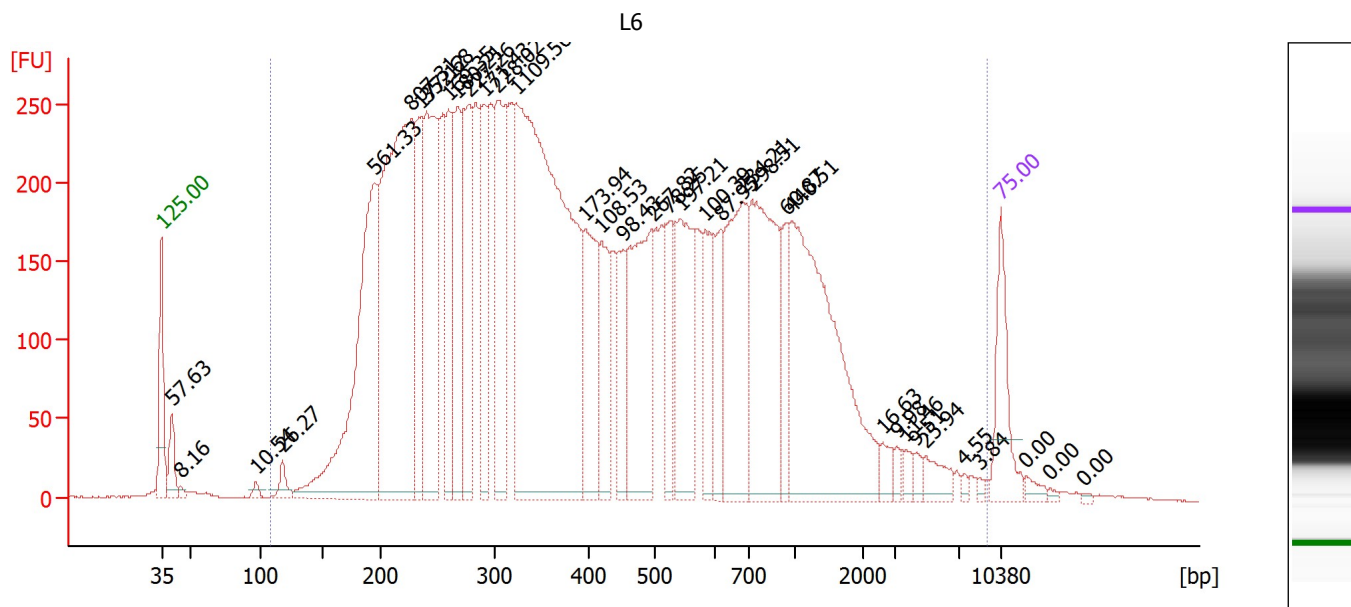**Electropherogram Summary Continued ...****Overall Results for sample 3 : L6**

Number of peaks found: 36  
 Noise: 0,5  
 Corr. Area 1: 11 465,4

**Peak table for sample 3 : L6**

| Peak | Size [bp] | Conc. [pg/μl] | Molarity [pmol/l] | Observations |
|------|-----------|---------------|-------------------|--------------|
| 1    | 35        | 125,00        | 5 411,3           | Lower Marker |
| 2    | 40        | 57,63         | 2 167,6           |              |
| 3    | 45        | 8,16          | 275,0             |              |
| 4    | 96        | 10,54         | 165,8             |              |
| 5    | 117       | 26,27         | 338,9             |              |
| 6    | 195       | 561,33        | 4 370,9           |              |
| 7    | 227       | 807,31        | 5 398,2           |              |
| 8    | 235       | 177,12        | 1 140,0           |              |
| 9    | 240       | 352,68        | 2 230,8           |              |
| 10   | 259       | 169,35        | 989,8             |              |
| 11   | 266       | 180,21        | 1 024,6           |              |
| 12   | 277       | 227,26        | 1 243,8           |              |
| 13   | 291       | 171,43        | 893,1             |              |
| 14   | 301       | 228,02        | 1 146,1           |              |
| 15   | 322       | 1 109,56      | 5 226,4           |              |
| 16   | 396       | 173,94        | 666,2             |              |
| 17   | 418       | 108,53        | 393,4             |              |
| 18   | 450       | 98,43         | 331,1             |              |
| 19   | 495       | 267,82        | 820,4             |              |
| 20   | 523       | 78,25         | 226,7             |              |
| 21   | 542       | 197,21        | 551,5             |              |
| 22   | 584       | 100,39        | 260,6             |              |
| 23   | 615       | 87,95         | 216,6             |              |
| 24   | 682       | 234,21        | 520,4             |              |
| 25   | 722       | 298,51        | 626,6             |              |
| 26   | 941       | 60,87         | 98,1              |              |

Assay Class: High Sensitivity DNA Assay  
Data Path: C:\...gh Sensitivity DNA Assay\_DE13805677\_2019-06-20\_10-12-12.xad

Created: 20/06/2019 10:12:12  
Modified: 20/06/2019 11:17:47


**Electropherogram Summary Continued ...****... Peak table for sample 3 : L6**

| Peak | Size [bp]                                                                                | Conc. [pg/μl] | Molarity [pmol/l] | Observations |
|------|------------------------------------------------------------------------------------------|---------------|-------------------|--------------|
| 27   | 975                                                                                      | 440,51        | 684,5             |              |
| 28   | 2 611                                                                                    | 16,63         | 9,7               |              |
| 29   | 3 059                                                                                    | 9,98          | 4,9               |              |
| 30   | 3 614                                                                                    | 11,46         | 4,8               |              |
| 31   | 4 206                                                                                    | 9,51          | 3,4               |              |
| 32   | 4 872                                                                                    | 25,94         | 8,1               |              |
| 33   | 7 364                                                                                    | 4,55          | 0,9               |              |
| 34   | 8 580                                                                                    | 3,84          | 0,7               |              |
| 35   |  10 380 | 75,00         | 10,9              | Upper Marker |
| 36   | 12 423                                                                                   | 0,00          | 0,0               |              |
| 37   | 14 417                                                                                   | 0,00          | 0,0               |              |
| 38   | 17 189                                                                                   | 0,00          | 0,0               |              |

Assay Class: High Sensitivity DNA Assay  
 Data Path: C:\...gh Sensitivity DNA Assay\_DE13805677\_2019-06-20\_10-12-12.xad

Created: 20/06/2019 10:12:12  
 Modified: 20/06/2019 11:17:47

### Electropherogram Summary Continued ...

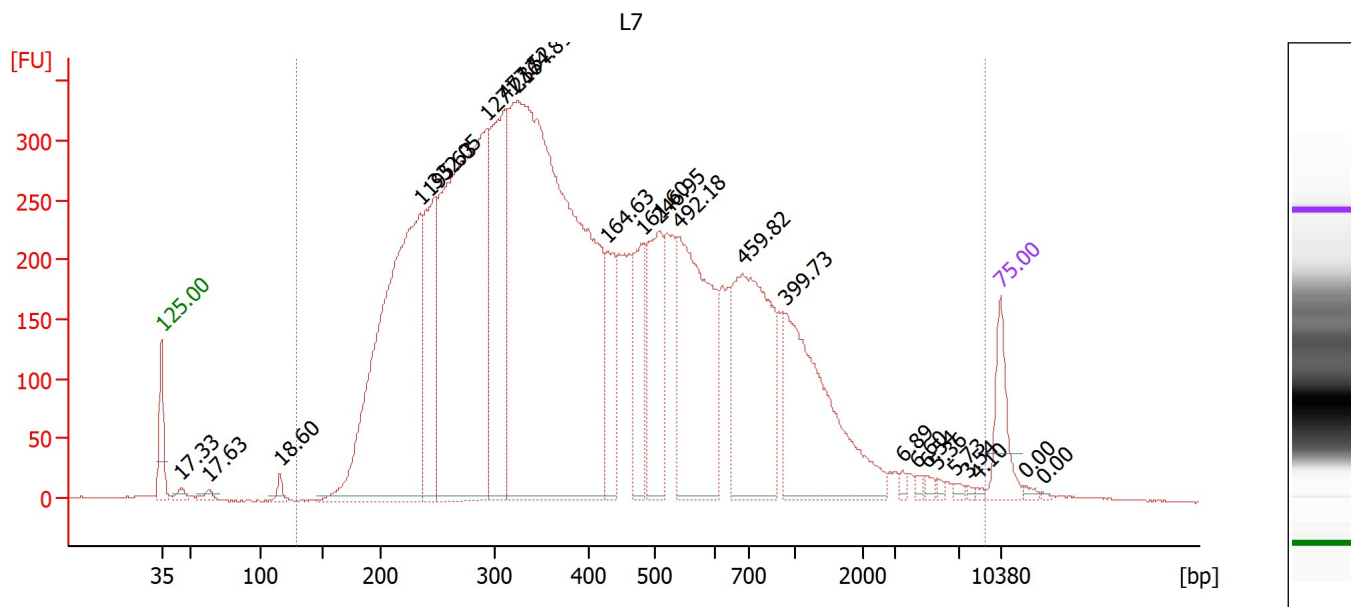

### Overall Results for sample 4 : L7

Number of peaks found: 23      Corr. Area 1: 12 232,8  
 Noise: 0,5


### Peak table for sample 4 : L7

| Peak | Size [bp] | Conc. [pg/μl] | Molarity [pmol/l] | Observations |
|------|-----------|---------------|-------------------|--------------|
| 1    | 35        | 125,00        | 5 411,3           | Lower Marker |
| 2    | 45        | 17,33         | 579,1             |              |
| 3    | 64        | 17,63         | 420,5             |              |
| 4    | 115       | 18,60         | 244,4             |              |
| 5    | 234       | 1 195,63      | 7 740,2           |              |
| 6    | 247       | 332,05        | 2 036,1           |              |
| 7    | 292       | 1 271,37      | 6 597,0           |              |
| 8    | 311       | 477,52        | 2 329,3           |              |
| 9    | 323       | 2 164,89      | 10 144,2          |              |
| 10   | 427       | 164,63        | 584,3             |              |
| 11   | 481       | 161,60        | 508,7             |              |
| 12   | 506       | 246,95        | 740,2             |              |
| 13   | 540       | 492,18        | 1 381,9           |              |
| 14   | 681       | 459,82        | 1 022,7           |              |
| 15   | 937       | 399,73        | 646,1             |              |
| 16   | 3 418     | 6,89          | 3,1               |              |
| 17   | 4 388     | 6,60          | 2,3               |              |
| 18   | 4 910     | 6,54          | 2,0               |              |
| 19   | 5 581     | 5,36          | 1,5               |              |
| 20   | 6 737     | 5,73          | 1,3               |              |
| 21   | 7 586     | 3,54          | 0,7               |              |
| 22   | 8 419     | 4,10          | 0,7               |              |
| 23   | 10 380    | 75,00         | 10,9              | Upper Marker |
| 24   | 12 292    | 0,00          | 0,0               |              |
| 25   | 13 811    | 0,00          | 0,0               |              |

Assay Class: High Sensitivity DNA Assay  
 Data Path: C:\...gh Sensitivity DNA Assay\_DE13805677\_2019-06-20\_10-12-12.xad

Created: 20/06/2019 10:12:12  
 Modified: 20/06/2019 11:17:47

### Electropherogram Summary Continued ...

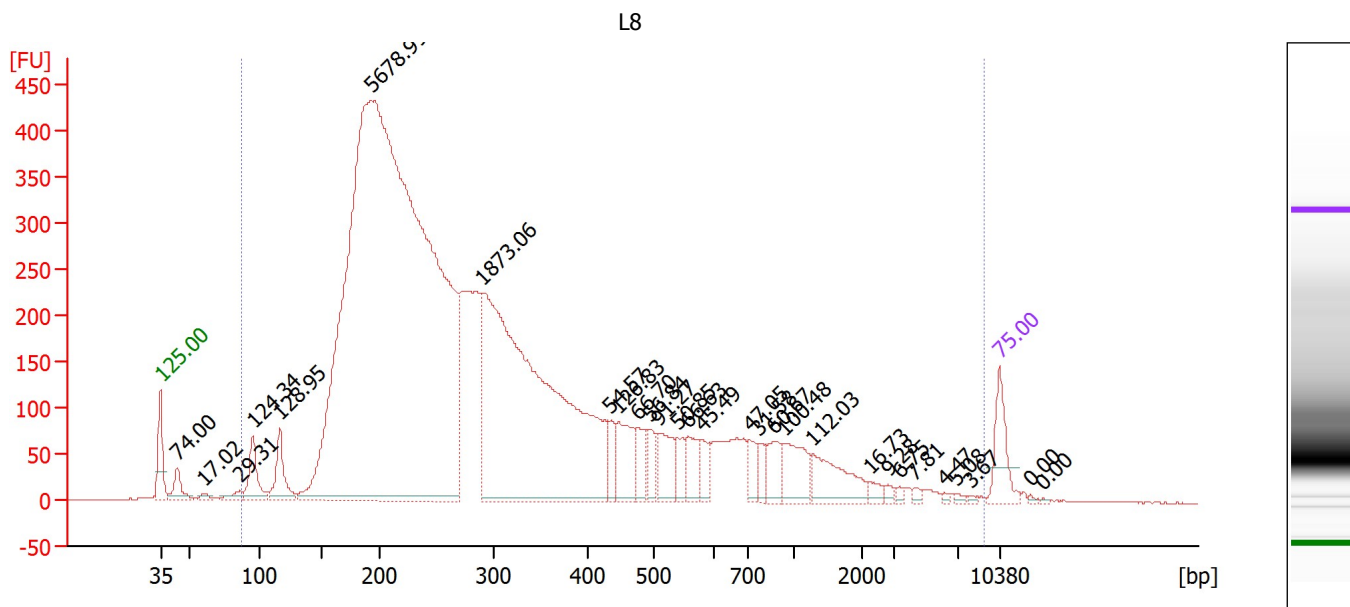

### Overall Results for sample 5 : L8

Number of peaks found: 29      Corr. Area 1: 10 541,0  
 Noise: 0,4

### Peak table for sample 5 : L8

| Peak | Size [bp] | Conc. [pg/μl] | Molarity [pmol/l] | Observations |
|------|-----------|---------------|-------------------|--------------|
| 1    | 35        | 125,00        | 5 411,3           | Lower Marker |
| 2    | 44        | 74,00         | 2 557,6           |              |
| 3    | 60        | 17,02         | 427,0             |              |
| 4    | 86        | 29,31         | 517,2             |              |
| 5    | 95        | 124,34        | 1 987,9           |              |
| 6    | 116       | 128,95        | 1 683,4           |              |
| 7    | 193       | 5 678,99      | 44 624,4          |              |
| 8    | 290       | 1 873,06      | 9 802,9           |              |
| 9    | 433       | 54,57         | 190,9             |              |
| 10   | 445       | 126,83        | 431,8             |              |
| 11   | 475       | 66,70         | 212,6             |              |
| 12   | 494       | 56,84         | 174,5             |              |
| 13   | 507       | 91,27         | 272,7             |              |
| 14   | 538       | 50,85         | 143,1             |              |
| 15   | 558       | 66,63         | 181,0             |              |
| 16   | 581       | 45,49         | 118,6             |              |
| 17   | 708       | 47,05         | 100,7             |              |
| 18   | 770       | 31,58         | 62,1              |              |
| 19   | 868       | 60,67         | 105,9             |              |
| 20   | 934       | 100,48        | 163,0             |              |
| 21   | 1 269     | 112,03        | 133,8             |              |
| 22   | 2 221     | 16,73         | 11,4              |              |
| 23   | 2 794     | 9,28          | 5,0               |              |
| 24   | 3 294     | 6,75          | 3,1               |              |
| 25   | 4 234     | 7,81          | 2,8               |              |
| 26   | 6 076     | 4,47          | 1,1               |              |

Assay Class: High Sensitivity DNA Assay  
Data Path: C:\...gh Sensitivity DNA Assay\_DE13805677\_2019-06-20\_10-12-12.xad

Created: 20/06/2019 10:12:12  
Modified: 20/06/2019 11:17:47


**Electropherogram Summary Continued ...****... Peak table for sample 5 : L8**

| Peak | Size [bp]                                                                                | Conc. [pg/μl] | Molarity [pmol/l] | Observations |
|------|------------------------------------------------------------------------------------------|---------------|-------------------|--------------|
| 27   | 6 790                                                                                    | 5,08          | 1,1               |              |
| 28   | 7 959                                                                                    | 3,67          | 0,7               |              |
| 29   |  10 380 | 75,00         | 10,9              | Upper Marker |
| 30   | 12 850                                                                                   | 0,00          | 0,0               |              |
| 31   | 13 838                                                                                   | 0,00          | 0,0               |              |

Assay Class: High Sensitivity DNA Assay  
 Data Path: C:\...gh Sensitivity DNA Assay\_DE13805677\_2019-06-20\_10-12-12.xad

Created: 20/06/2019 10:12:12  
 Modified: 20/06/2019 11:17:47

### Electropherogram Summary Continued ...

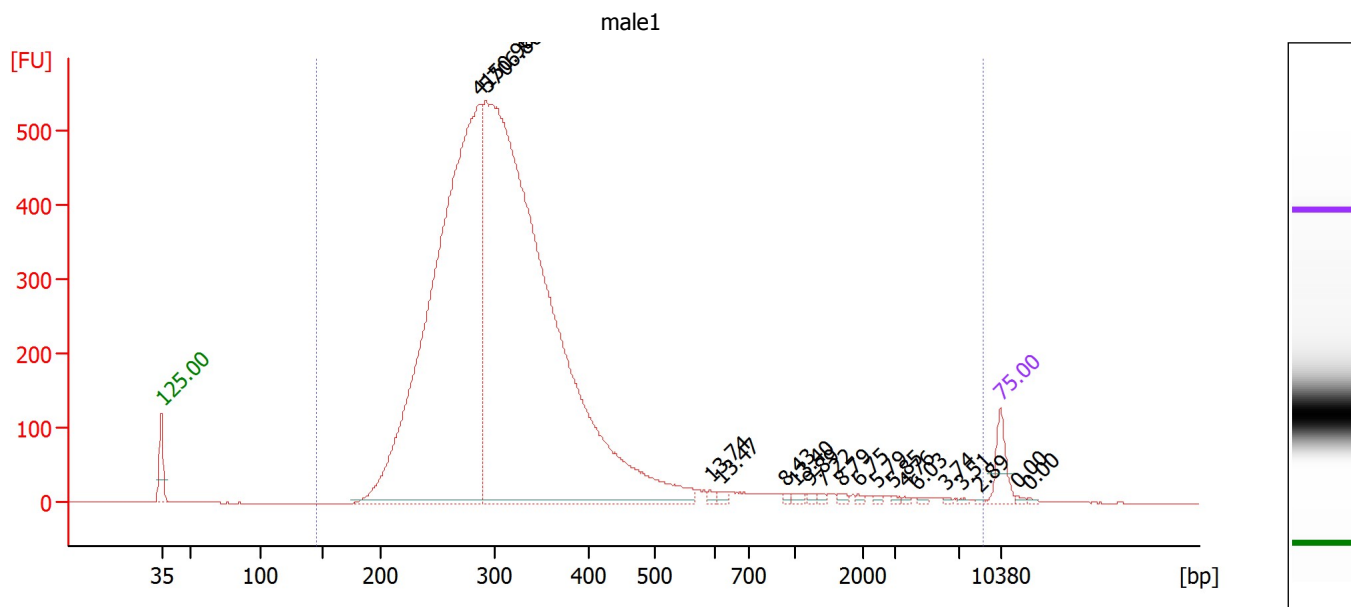

### Overall Results for sample 6 : male1

Number of peaks found: 19      Corr. Area 1: 9 173,5  
 Noise: 0,4


### Peak table for sample 6 : male1

| Peak | Size [bp] | Conc. [pg/μl] | Molarity [pmol/l] | Observations |
|------|-----------|---------------|-------------------|--------------|
| 1    | 35        | 125,00        | 5 411,3           | Lower Marker |
| 2    | 286       | 4 150,96      | 22 024,4          |              |
| 3    | 292       | 5 706,80      | 29 622,5          |              |
| 4    | 593       | 13,74         | 35,1              |              |
| 5    | 616       | 13,47         | 33,1              |              |
| 6    | 934       | 8,43          | 13,7              |              |
| 7    | 1 001     | 13,40         | 20,3              |              |
| 8    | 1 216     | 9,89          | 12,3              |              |
| 9    | 1 404     | 7,22          | 7,8               |              |
| 10   | 1 681     | 8,79          | 7,9               |              |
| 11   | 1 931     | 6,75          | 5,3               |              |
| 12   | 2 432     | 5,79          | 3,6               |              |
| 13   | 2 951     | 5,85          | 3,0               |              |
| 14   | 3 578     | 4,76          | 2,0               |              |
| 15   | 4 332     | 6,03          | 2,1               |              |
| 16   | 6 141     | 3,74          | 0,9               |              |
| 17   | 7 110     | 3,51          | 0,7               |              |
| 18   | 8 547     | 2,89          | 0,5               |              |
| 19   | 10 380    | 75,00         | 10,9              | Upper Marker |
| 20   | 11 668    | 0,00          | 0,0               |              |
| 21   | 12 758    | 0,00          | 0,0               |              |

Assay Class: High Sensitivity DNA Assay  
 Data Path: C:\...gh Sensitivity DNA Assay\_DE13805677\_2019-06-20\_10-12-12.xad

Created: 20/06/2019 10:12:12  
 Modified: 20/06/2019 11:17:47

### Electropherogram Summary Continued ...

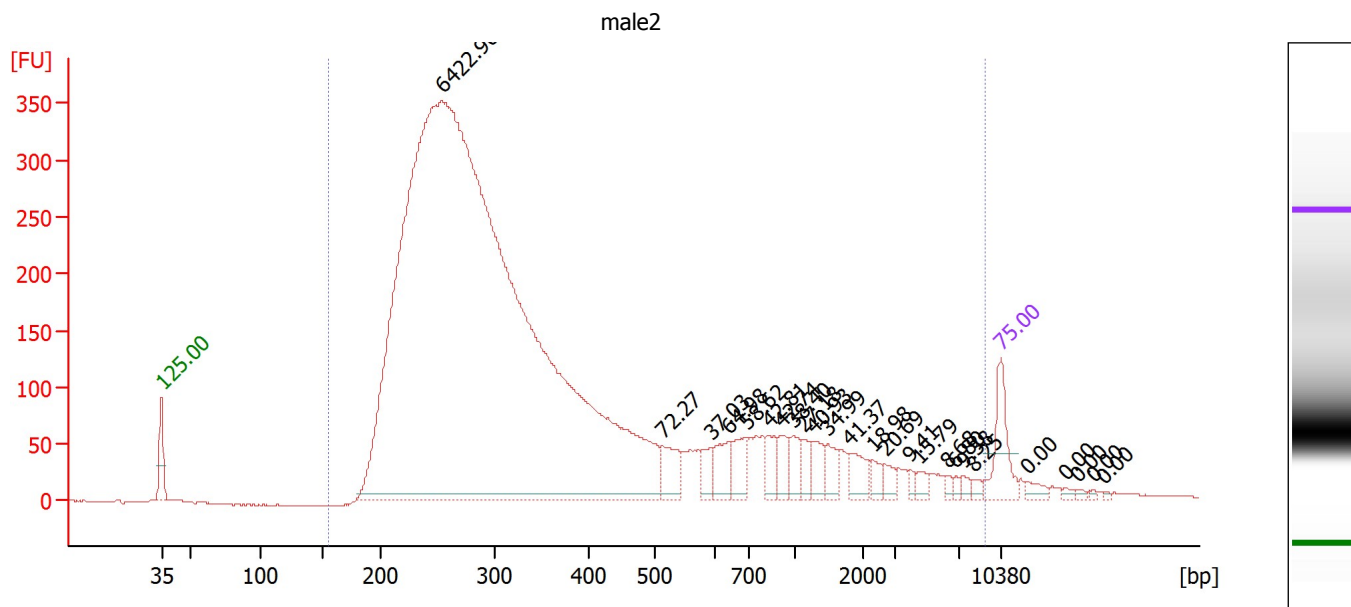

### Overall Results for sample 7 : male2

Number of peaks found: 25      Corr. Area 1: 7 810,6  
 Noise: 0,7

### Peak table for sample 7 : male2

| Peak | Size [bp] | Conc. [pg/μl] | Molarity [pmol/l] | Observations |
|------|-----------|---------------|-------------------|--------------|
| 1    | 35        | 125,00        | 5 411,3           | Lower Marker |
| 2    | 253       | 6 422,90      | 38 466,6          |              |
| 3    | 511       | 72,27         | 214,3             |              |
| 4    | 592       | 37,03         | 94,8              |              |
| 5    | 640       | 64,98         | 153,9             |              |
| 6    | 692       | 58,62         | 128,3             |              |
| 7    | 827       | 42,81         | 78,4              |              |
| 8    | 913       | 42,74         | 70,9              |              |
| 9    | 988       | 38,40         | 58,9              |              |
| 10   | 1 113     | 27,18         | 37,0              |              |
| 11   | 1 261     | 40,93         | 49,2              |              |
| 12   | 1 482     | 34,99         | 35,8              |              |
| 13   | 1 802     | 41,37         | 34,8              |              |
| 14   | 2 304     | 18,98         | 12,5              |              |
| 15   | 2 678     | 20,69         | 11,7              |              |
| 16   | 3 866     | 9,41          | 3,7               |              |
| 17   | 4 419     | 15,79         | 5,4               |              |
| 18   | 6 217     | 8,68          | 2,1               |              |
| 19   | 6 770     | 6,80          | 1,5               |              |
| 20   | 7 335     | 9,38          | 1,9               |              |
| 21   | 8 153     | 8,25          | 1,5               |              |
| 22   | 10 380    | 75,00         | 10,9              | Upper Marker |
| 23   | 12 562    | 0,00          | 0,0               |              |
| 24   | 15 607    | 0,00          | 0,0               |              |
| 25   | 16 698    | 0,00          | 0,0               |              |
| 26   | 17 926    | 0,00          | 0,0               |              |

Assay Class: High Sensitivity DNA Assay  
Data Path: C:\...gh Sensitivity DNA Assay\_DE13805677\_2019-06-20\_10-12-12.xad

Created: 20/06/2019 10:12:12  
Modified: 20/06/2019 11:17:47

**Electropherogram Summary Continued ...**

... Peak table for sample 7 : male2


| Peak | Size [bp] | Conc. [pg/μl] | Molarity [pmol/l] | Observations |
|------|-----------|---------------|-------------------|--------------|
| 27   | 18 835    | 0,00          | 0,0               |              |



Assay Class: High Sensitivity DNA Assay  
 Data Path: C:\...gh Sensitivity DNA Assay\_DE13805677\_2019-06-20\_10-12-12.xad

Created: 20/06/2019 10:12:12  
 Modified: 20/06/2019 11:17:47

### Electropherogram Summary Continued ...

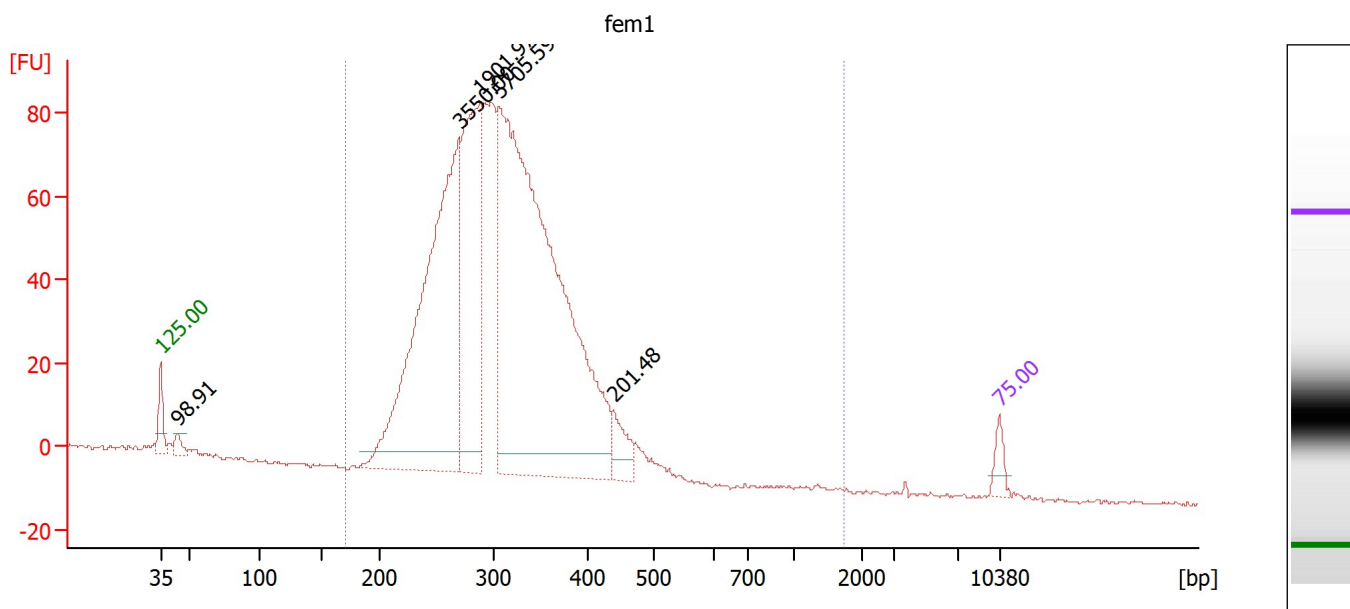

### Overall Results for sample 8 : fem1

Number of peaks found: 5      Corr. Area 1: 1 514,3  
 Noise: 0,4


### Peak table for sample 8 : fem1

| Peak | Size [bp] | Conc. [pg/μl] | Molarity [pmol/l] | Observations |
|------|-----------|---------------|-------------------|--------------|
| 1    | 35        | 125,00        | 5 411,3           | Lower Marker |
| 2    | 44        | 98,91         | 3 423,4           |              |
| 3    | 269       | 3 550,00      | 20 018,6          |              |
| 4    | 287       | 1 901,97      | 10 041,9          |              |
| 5    | 305       | 5 705,59      | 28 389,7          |              |
| 6    | 437       | 201,48        | 698,0             | Upper Marker |
| 7    | 10 380    | 75,00         | 10,9              |              |

Assay Class: High Sensitivity DNA Assay  
 Data Path: C:\...gh Sensitivity DNA Assay\_DE13805677\_2019-06-20\_10-12-12.xad

Created: 20/06/2019 10:12:12  
 Modified: 20/06/2019 11:17:47

### Electropherogram Summary Continued ...

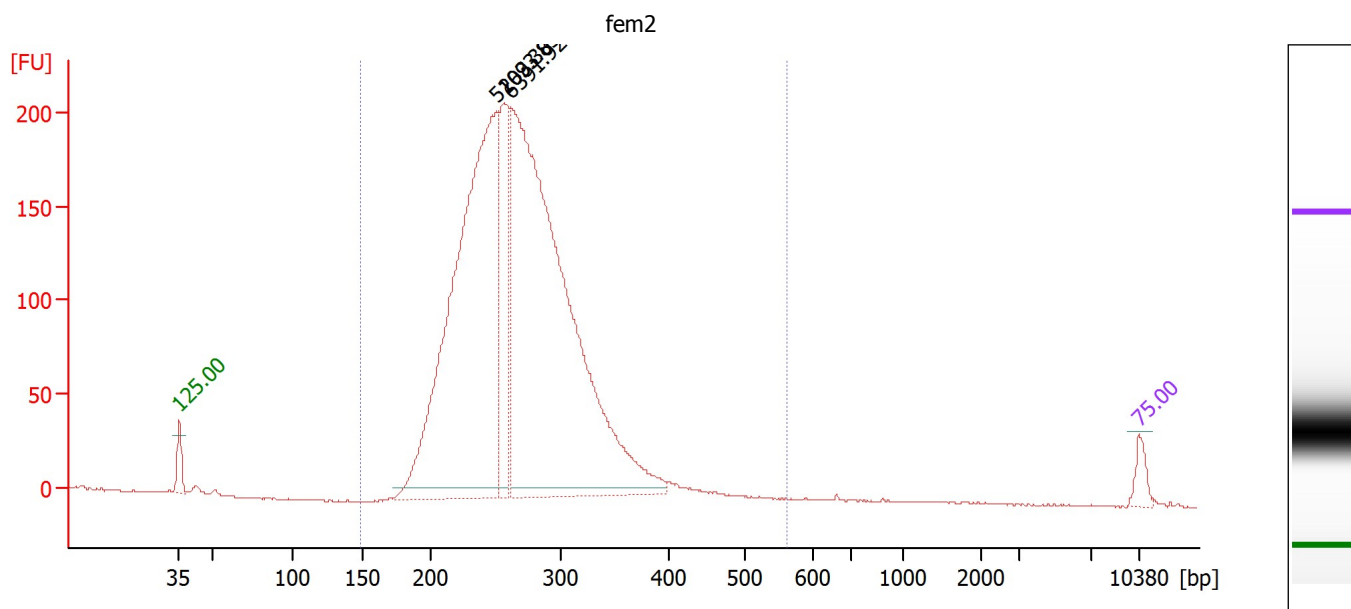

### Overall Results for sample 9 : fem2

Number of peaks found: 3      Corr. Area 1: 3 340,2  
 Noise: 0,3


### Peak table for sample 9 : fem2

| Peak | Size [bp] | Conc. [pg/μl] | Molarity [pmol/l] | Observations |
|------|-----------|---------------|-------------------|--------------|
| 1    | 35        | 125,00        | 5 411,3           | Lower Marker |
| 2    | 251       | 5 203,30      | 31 455,6          |              |
| 3    | 257       | 1 093,85      | 6 455,5           |              |
| 4    | 262       | 6 391,92      | 37 018,3          |              |
| 5    | 10 380    | 75,00         | 10,9              | Upper Marker |

Assay Class: High Sensitivity DNA Assay  
 Data Path: C:\...gh Sensitivity DNA Assay\_DE13805677\_2019-06-20\_10-12-12.xad

Created: 20/06/2019 10:12:12  
 Modified: 20/06/2019 11:17:47

### Electropherogram Summary Continued ...

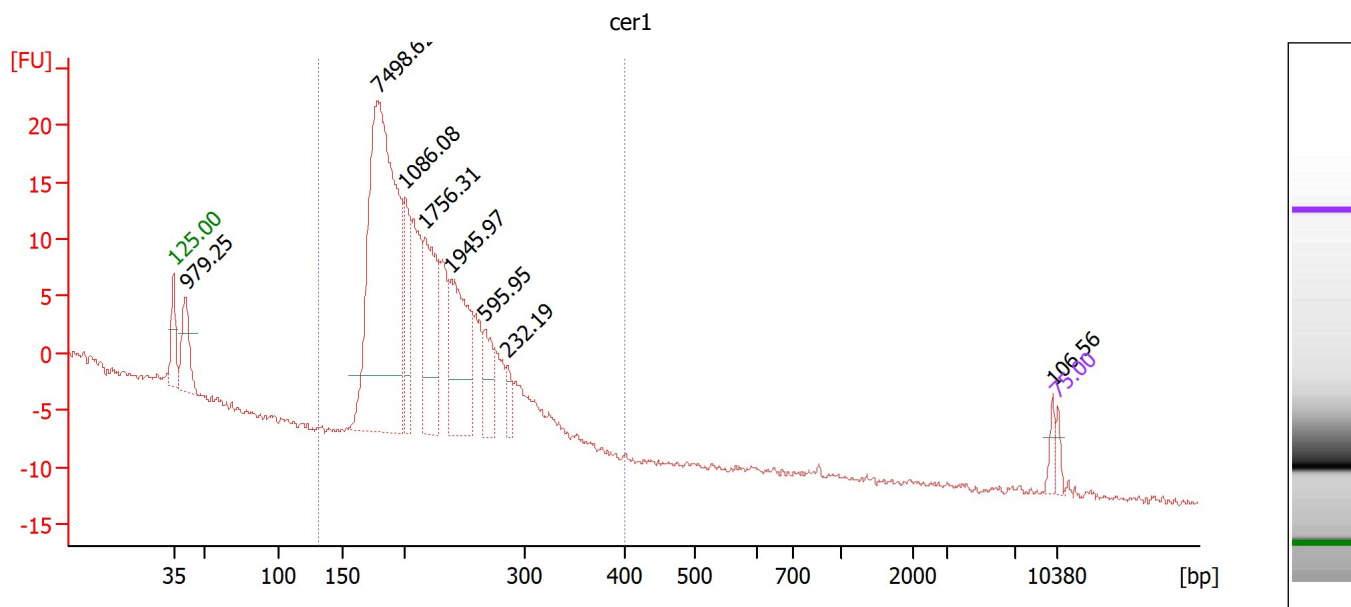

### Overall Results for sample 10 : cer1


Number of peaks found: 8      Corr. Area 1: 276,8  
 Noise: 0,2

### Peak table for sample 10 : cer1

| Peak | Size [bp] | Conc. [pg/μl] | Molarity [pmol/l] | Observations |
|------|-----------|---------------|-------------------|--------------|
| 1    | 35        | 125,00        | 5 411,3           | Lower Marker |
| 2    | 41        | 979,25        | 36 106,0          |              |
| 3    | 178       | 7 498,63      | 63 657,8          |              |
| 4    | 201       | 1 086,08      | 8 204,6           |              |
| 5    | 217       | 1 756,31      | 12 268,5          |              |
| 6    | 238       | 1 945,97      | 12 383,4          |              |
| 7    | 267       | 595,95        | 3 384,4           |              |
| 8    | 285       | 232,19        | 1 234,8           |              |
| 9    | 9 965     | 106,56        | 16,2              | Upper Marker |
| 10   | 10 380    | 75,00         | 10,9              |              |

Assay Class: High Sensitivity DNA Assay  
 Data Path: C:\...gh Sensitivity DNA Assay\_DE13805677\_2019-06-20\_10-12-12.xad

Created: 20/06/2019 10:12:12  
 Modified: 20/06/2019 11:17:47

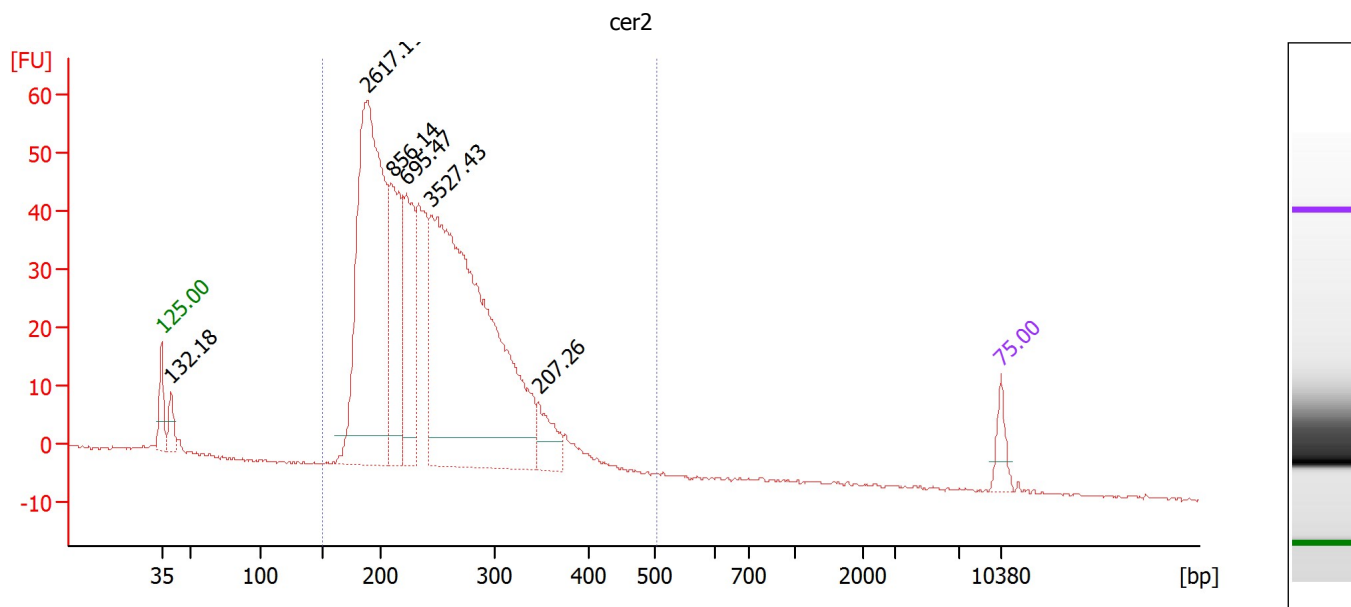**Electropherogram Summary Continued ...****Overall Results for sample 11 : cer2**


Number of peaks found: 6      Corr. Area 1: 929,2  
 Noise: 0,2

**Peak table for sample 11 : cer2**

| Peak | Size [bp] | Conc. [pg/μl] | Molarity [pmol/l] | Observations |
|------|-----------|---------------|-------------------|--------------|
| 1    | 35        | 125,00        | 5 411,3           | Lower Marker |
| 2    | 40        | 132,18        | 5 007,3           |              |
| 3    | 188       | 2 617,11      | 21 053,6          |              |
| 4    | 209       | 856,14        | 6 193,1           |              |
| 5    | 222       | 695,47        | 4 736,5           |              |
| 6    | 244       | 3 527,43      | 21 920,5          |              |
| 7    | 345       | 207,26        | 909,9             |              |
| 8    | 10 380    | 75,00         | 10,9              | Upper Marker |

Assay Class: High Sensitivity DNA Assay  
Data Path: C:\...gh Sensitivity DNA Assay\_DE13805677\_2019-06-20\_10-12-12.xad

Created: 20/06/2019 10:12:12  
Modified: 20/06/2019 11:17:47

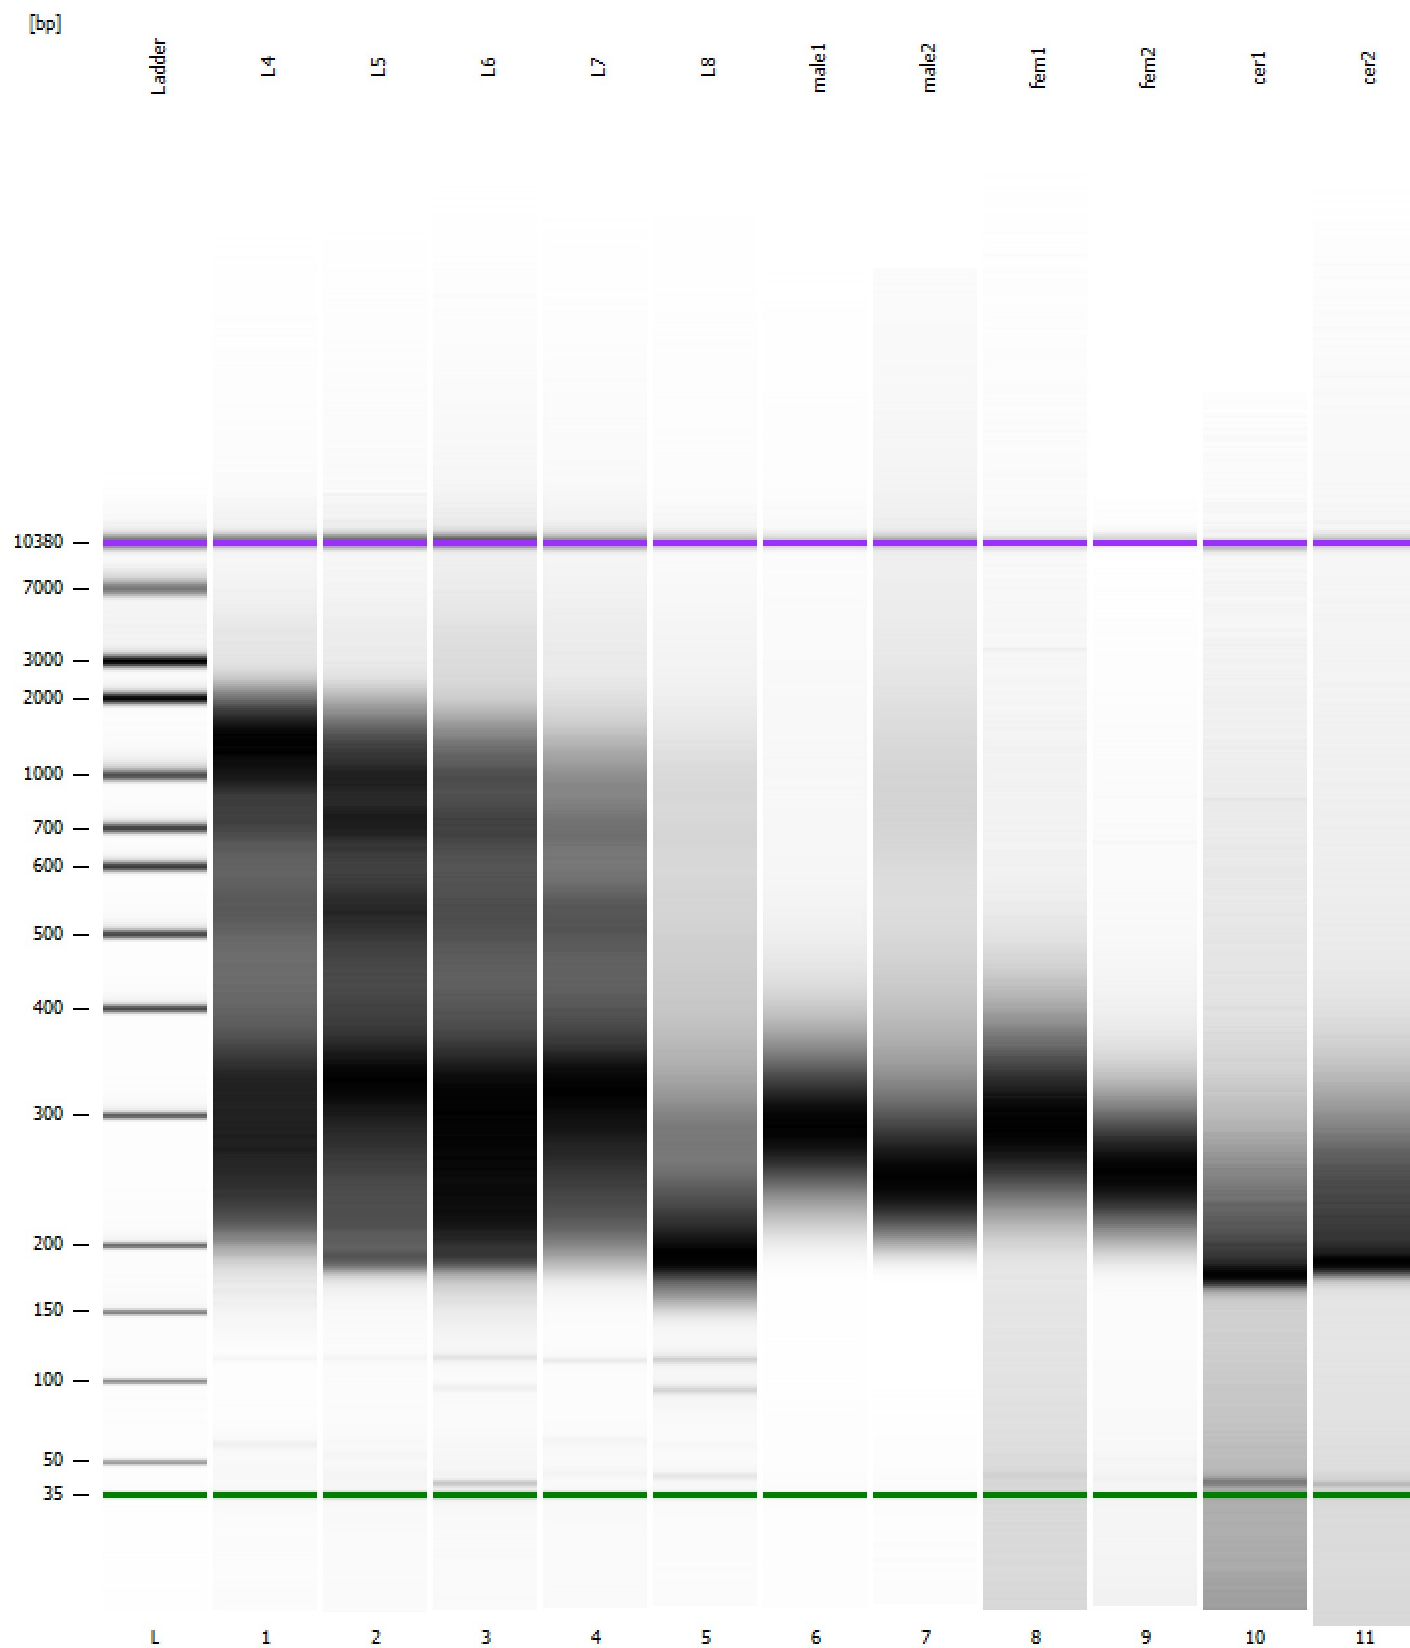**Gel Image**

Assay Class: High Sensitivity DNA Assay Created: 20/06/2019 10:12:12  
 Data Path: C:\...gh Sensitivity DNA Assay\_DE13805677\_2019-06-20\_10-12-12.xad Modified: 20/06/2019 11:17:47

**Run Logbook**

| Description                                                                                                                                                                                                   | Number | Source     | Category | Sub Category | Time                | Time Zone                  | User | Host    |
|---------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|--------|------------|----------|--------------|---------------------|----------------------------|------|---------|
| Run ended on port 3 (Number of wells acquired: 12)                                                                                                                                                            |        | Instrument | Run      |              | 20/06/2019 10:52:38 | (GMT +02:00) Paris, Madrid | cnrs | cnrs-PC |
| Run started on port 3 (File: C:\Program Files (x86)\Agilent\2100 bioanalyzer\2100 expert\data\jfa\NGS_jfa\NGS2019\juin_2019\2019-06-20\CG_Ro_2_High Sensitivity DNA Assay_DE13805677_2019-06-20_10-12-12.xad) |        | Instrument | Run      |              | 20/06/2019 10:12:17 | (GMT +02:00) Paris, Madrid | cnrs | cnrs-PC |
| Product Number : G2939A                                                                                                                                                                                       |        | Instrument | Run      |              | 20/06/2019 10:12:17 | (GMT +02:00) Paris, Madrid | cnrs | cnrs-PC |
| Name :                                                                                                                                                                                                        |        | Instrument | Run      |              | 20/06/2019 10:12:17 | (GMT +02:00) Paris, Madrid | cnrs | cnrs-PC |
| Vendor : Agilent Technologies                                                                                                                                                                                 |        | Instrument | Run      |              | 20/06/2019 10:12:17 | (GMT +02:00) Paris, Madrid | cnrs | cnrs-PC |
| Serial# : DE13805677                                                                                                                                                                                          |        | Instrument | Run      |              | 20/06/2019 10:12:17 | (GMT +02:00) Paris, Madrid | cnrs | cnrs-PC |
| Firmware : C.01.069                                                                                                                                                                                           |        | Instrument | Run      |              | 20/06/2019 10:12:17 | (GMT +02:00) Paris, Madrid | cnrs | cnrs-PC |
| Cartridge : Electrode                                                                                                                                                                                         |        | Instrument | Run      |              | 20/06/2019 10:12:17 | (GMT +02:00) Paris, Madrid | cnrs | cnrs-PC |