RECORDING QUALITY CHECK · RESEARCH USE

S004R01

61.0 seconds · 64 sensors · 160 samples/second · 60 Hz electrical check

9.1/100 Not usable

Do not use the full recording as-is. Inspect it and decide whether any part can be recovered.

Why this result?


- flat: flagged in 1 of 31 time windows
- noisy: flagged in 30 of 31 time windows
- line: flagged in 24 of 31 time windows
- blink: flagged in 12 of 31 time windows
- muscle: flagged in 10 of 31 time windows
- At least 20% of channel-time is flat/noisy or 50% of time has artifact flags

What needs attention?

Check	Flagged windows	Sensors	Suggested action
Flat sensors Little or no changing signal	1 / 31	All 64 sensors	Check sensor contact; exclude affected sensors.
Noisy sensors Unusually large or erratic signal	30 / 31	Af7, Af8, Fp1, Fp2, Ft8, P7	Inspect contact and affected sensors.
Electrical interference A strong repeating mains-frequency signal	24 / 31	30 sensors: F2, F4, Fc4, Fc6; full list in JSON	Check grounding and power sources.
Possible eye blinks Large slow changes at forehead sensors	12 / 31	Fp1, Fp2, Fpz	Inspect marked times before analysis.
Possible muscle tension Extra fast activity in the signal	10 / 31	Af3, Af8, Fpz	Inspect marked times for tension or movement.

When did it happen?

Left to right: start to end (61.0 s). Rust blocks flag a time window; pale blocks cross no threshold.

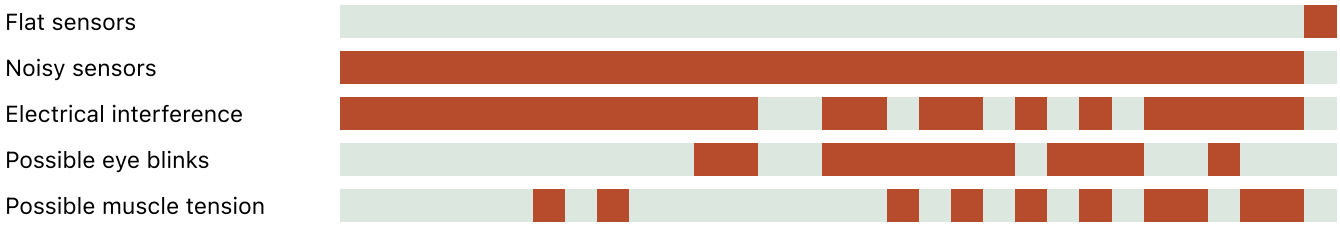

Not a diagnostic tool. These rules flag suspicious signals, not confirmed causes or illness. Forehead sensors stand in for eye sensors; fast brain activity can resemble muscle tension. The score is the percentage of unflagged channel-time multiplied by the percentage of time without interference flags. It is not a probability of correctness. All sensors, times, values and thresholds are in the accompanying JSON. Original data are unchanged.