
Somfit Automatic Report

Somfit Check SLEEP 1st®

PATIENT DETAILS				STUDY DETAILS			
Name	N/A	ID		Study Date	Night 1		
Age	26	BMI	kg/m^2	Start/End Time	22:23:10	–	06:34:09

GRAPHIC SUMMARY

DISCLAIMER: This data in this report has been automatically generated with no manual review. It is not intended for clinical interpretation purposes. Clinical interpretation can only be performed by a suitably qualified sleep medicine practitioner.

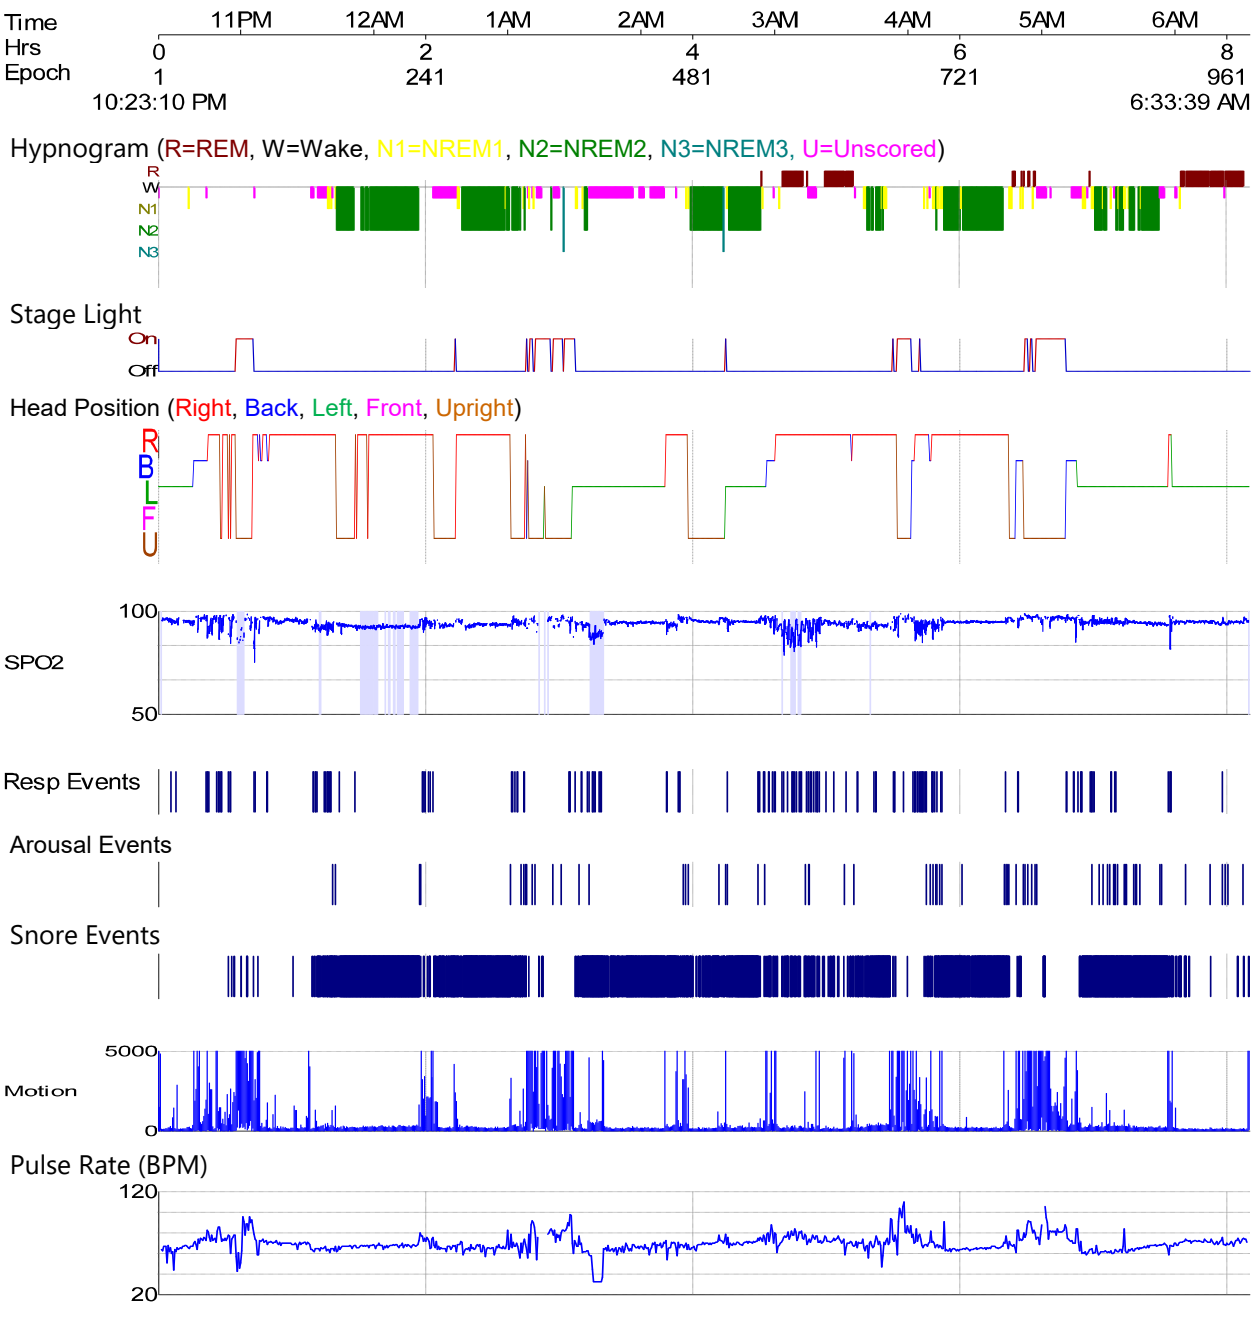

Note: periods of baseline drift are indicated by pale blue background shading on the SpO_2 graph. This time period is included for detection of respiratory events metrics (pAHI, ODI) but excluded for SpO_2 metrics calculations.

DISCLAIMER: This data in this report has been automatically generated with no manual review. It is not intended for clinical interpretation purposes. Clinical interpretation can only be performed by a suitably qualified sleep medicine practitioner.

Somfit Automatic Report

Somfit Check SLEEP 1st®

SLEEP STAGING SUMMARY

	Time	% of Sleep
N1 sleep	28.5 min	12.6 %
N2 sleep	141.0 min	62.5 %
N3 sleep	1.0 min	0.4 %
REM sleep	55.0 min	24.4 %
NREM sleep	170.5 min	75.6 %

	Time	
Sleep (TST)	225.5 min	
Wake	189.5 min	(SOL + WASO)
Sleep efficiency	51.3 %	


SLEEP TIME STATISTICS

	Time
Total Recording Time (TRT)	8:10:59 hh:mm:ss
Time Available for Sleep	7:19:30 hh:mm:ss
Total Sleep Time (TST)	3:45:30 hh:mm:ss
SpO_2 Artifact Time (during TST)	0:10:36 hh:mm:ss
Monitoring Time (MT)	6:31:28 hh:mm:ss
Sleep Onset Latency (SOL)	13.5 min
REM latency	257.5 min
Wake after sleep onset (WASO)*	176.0 min

**includes wake between sleep offset and lights on time*

STUDY TIMES

Reference hypnogram only – not actual patient hypnogram

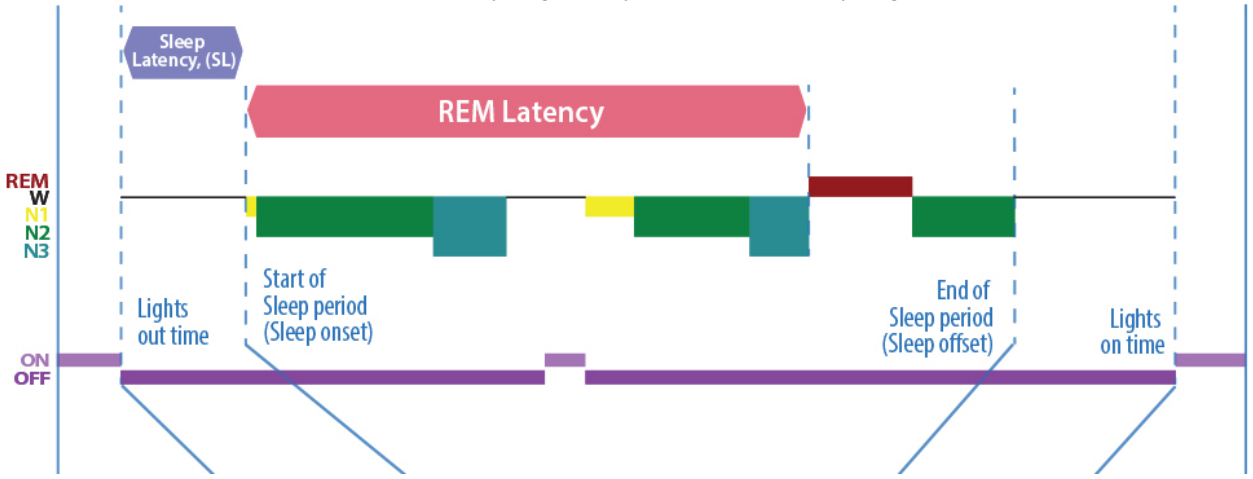

Start recording	Lights out	Sleep onset	Sleep offset	Lights on	End Recording
22:23:10	22:23:10	22:36:40	06:31:09	6:33:39	06:34:09

Sleep availability time	7:54:30
Time available for sleep	7:19:30
Total recording time (TRT)	8:10:59


DISCLAIMER: This data in this report has been automatically generated with no manual review. It is not intended for clinical interpretation purposes. Clinical interpretation can only be performed by a suitably qualified sleep medicine practitioner.

RESPIRATORY EVENTS (BY STAGING AND POSITION)

	REM	NREM	Total	Head Supine	Head Non-Supine
Qty Respiratory Events	16	28	44	0	44
Sleep Duration (TST)	55.0 min	170.5 min	225.5 min	2 min	224 min
pAHI (≥3%)	17.5 /hr	9.9 /hr	**11.7 /hr**	0.0 /hr	11.8 /hr
Monitoring Time (MT)			391.5 min	17 min	374 min
REI			23.1 /hr	59.6 /hr	21.5 /hr
ODI (≥3%)	16.4 /hr	8.8 /hr	10.6 /hr	0.0 /hr	10.7 /hr
ODI (≥4%)	13.1 /hr	3.9 /hr	6.1 /hr		
Arousals Index	7.6 /hr	6.3 /hr	6.7 /hr	30.0 /hr	6.4 /hr
Snore Index	123.3 /hr	1026.2 /hr	805.9 /hr	90 /hr	812 /hr
Longest Resp. Event			72 sec		

Note: Respiratory events (RE) are identified using peripheral arterial tone, oxygen desaturation and changes in heart rate derived from oximetry. pAHI is defined as the number of valid respiratory events during TST divided by the TST. REI is defined as the number of valid respiratory events during MT divided by the MT.

pAHI GRAPH

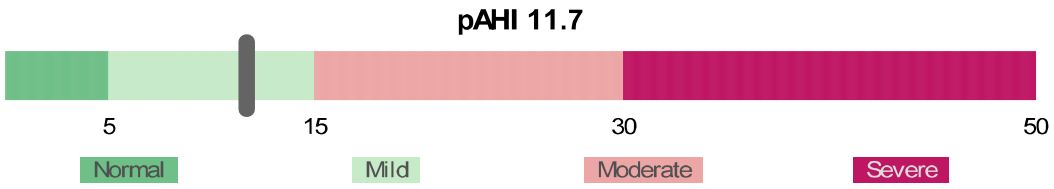

Reference values for AHI are in accordance with AASM guidelines.

OXYGEN SATURATION SUMMARY

	SpO_2	SpO_2 Time	Duration*	Sleep %*
Start (awake)	96 %	<90%	3.4 min	1.7 %
Average during sleep*	94 %	<88%	2.0 min	1.0 %
Minimum during sleep*	79 %	<85%	1.1 min	0.5 %
Largest desaturation	14 %	<80%	0.1 min	0.0 %

* Valid SpO2 measurement time is 200.3 minutes, determined by Total Sleep Time (TST) less any periods of baseline drift during TST.

VITAL SIGNS (FROM PPG)

	Average	Highest	Lowest
Pulse Rate (during Sleep)	68 BPM	87 BPM	52 BPM

DISCLAIMER: This data in this report has been automatically generated with no manual review. It is not intended for clinical interpretation purposes. Clinical interpretation can only be performed by a suitably qualified sleep medicine practitioner.



Somfit Automatic Report

Somfit Check SLEEP 1st®

STUDY QUALITY

	Start	+3Hrs	+6hrs	Rating
EEG Impedance – Right	332 kΩ	45 kΩ	40 kΩ	Query
EEG Impedance – Left	147 kΩ	46 kΩ	41 kΩ	Adequate
		%	%	Rating
Somfit Data Lost			1.0 %	Good
Unscorable Sleep Staging			16.0 %	Adequate
Total SpO_2 Artifact			16.0 %	Adequate
– Motion		15.0 %		
– Off		1.0 %		
– Low SNR		0.0 %		
– Low PI		0.0 %		
% Time of Baseline Drift			6.0 %	Good
Start Battery Level			100 %	Good
Battery Discharge Rate			4 %/hr	Good

DEVICE INFORMATION

Somfit Device	Somfit N/A
Somfit Service	Somfit Diagnostic
Somfit Firmware Version	116
Somfit App Version	5.2.0 (138)
Somfit Study Processing Version	SomfitBatch 2.1.0.106
Bluetooth Address	N/A
Bluetooth Connection Time	Night 1 22:23:10
App Start Date/Time	Night 1 22:23:10
App End Date/Time	Night 1 (+1 d) 06:34:15
Average Device Temperature	29.0 °C

PHONE INFORMATION

Phone Model	iPhone16
Phone OS	26.6.1
Phone Start Battery Level	85%
Phone End Battery Level	100.0%

DISCLAIMER: This data in this report has been automatically generated with no manual review. It is not intended for clinical interpretation purposes. Clinical interpretation can only be performed by a suitably qualified sleep medicine practitioner.


Somfit Automatic Report

Somfit Check SLEEP 1st®

PATIENT DETAILS				STUDY DETAILS			
Name	N/A	ID		Study Date	Night 7		
Age	26	BMI	kg/m^2	Start/End Time	23:06:47	–	06:47:36

GRAPHIC SUMMARY

DISCLAIMER: This data in this report has been automatically generated with no manual review. It is not intended for clinical interpretation purposes. Clinical interpretation can only be performed by a suitably qualified sleep medicine practitioner.

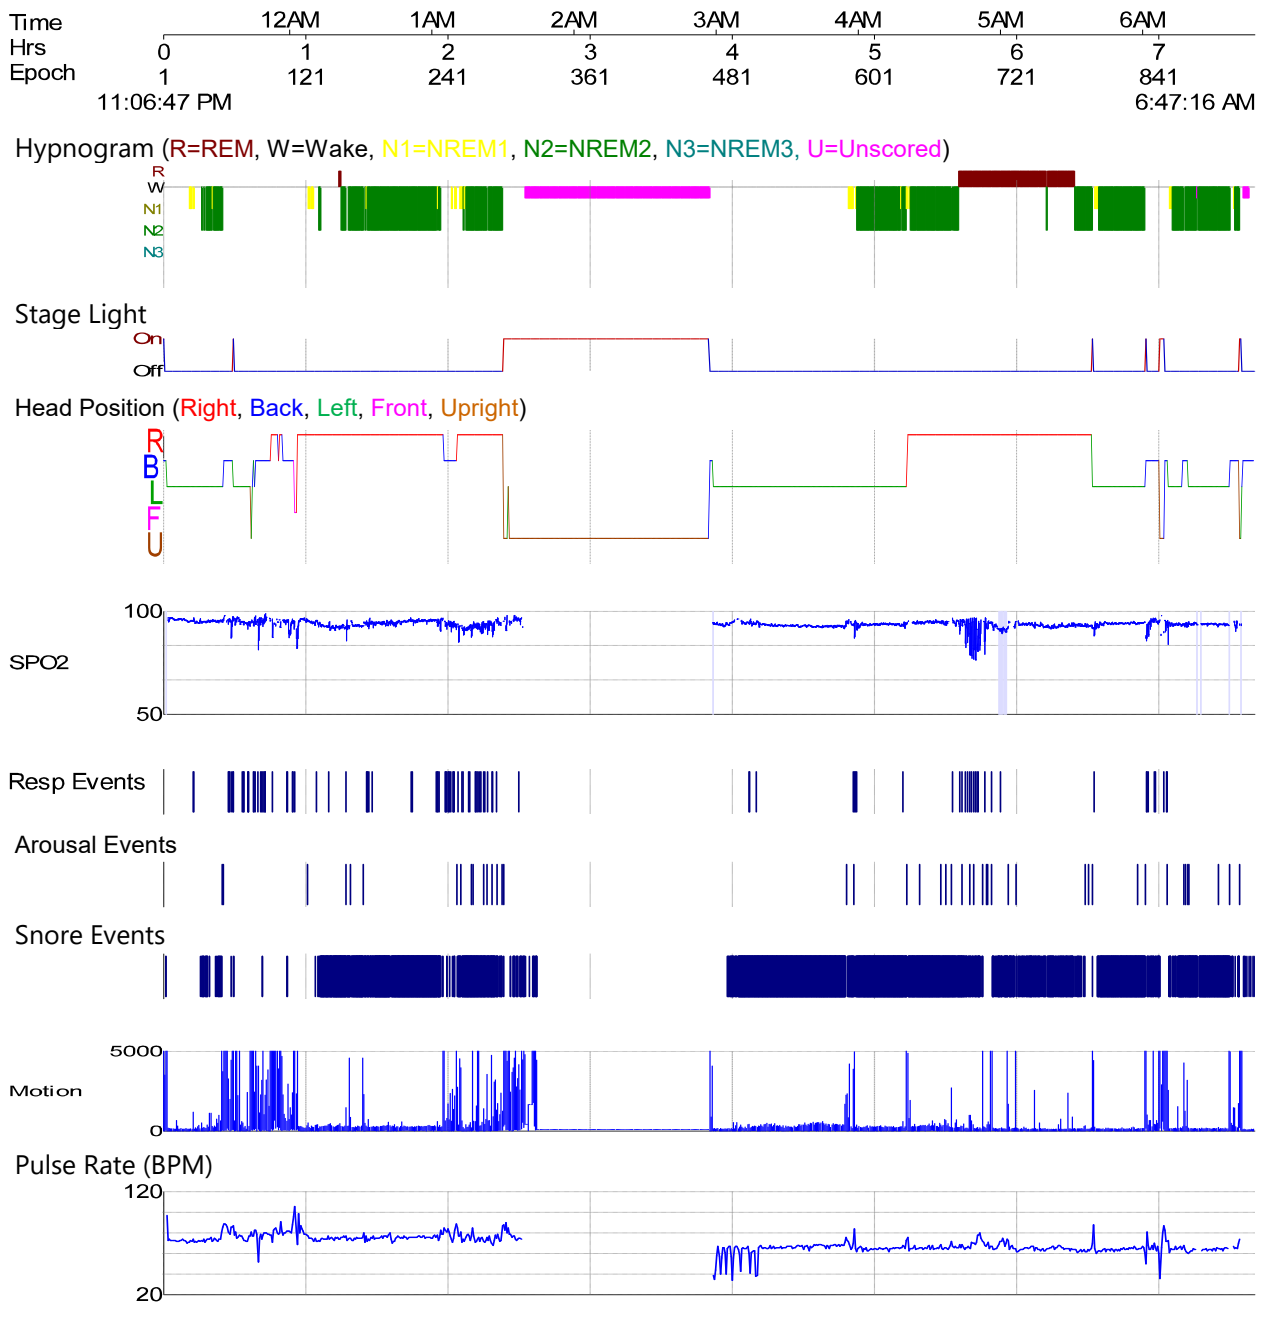

Note: periods of baseline drift are indicated by pale blue background shading on the SpO_2 graph. This time period is included for detection of respiratory events metrics (pAHI, ODI) but excluded for SpO_2 metrics calculations.

DISCLAIMER: This data in this report has been automatically generated with no manual review. It is not intended for clinical interpretation purposes. Clinical interpretation can only be performed by a suitably qualified sleep medicine practitioner.

Somfit Automatic Report

Somfit Check SLEEP 1st®

SLEEP STAGING SUMMARY

	Time	% of Sleep
N1 sleep	15.0 min	6.8 %
N2 sleep	157.0 min	70.9 %
N3 sleep	0.0 min	0.0 %
REM sleep	49.5 min	22.3 %
NREM sleep	172.0 min	77.7 %

	Time	
Sleep (TST)	221.5 min	
Wake	157.5 min	(SOL + WASO)
Sleep efficiency	60.1 %	


SLEEP TIME STATISTICS

	Time
Total Recording Time (TRT)	7:40:49 hh:mm:ss
Time Available for Sleep	6:08:30 hh:mm:ss
Total Sleep Time (TST)	3:41:30 hh:mm:ss
SpO_2 Artifact Time (during TST)	0:13:09 hh:mm:ss
Monitoring Time (MT)	5:29:57 hh:mm:ss
Sleep Onset Latency (SOL)	10.5 min
REM latency	63.0 min
Wake after sleep onset (WASO)*	147.0 min

**includes wake between sleep offset and lights on time*

STUDY TIMES

Reference hypnogram only – not actual patient hypnogram

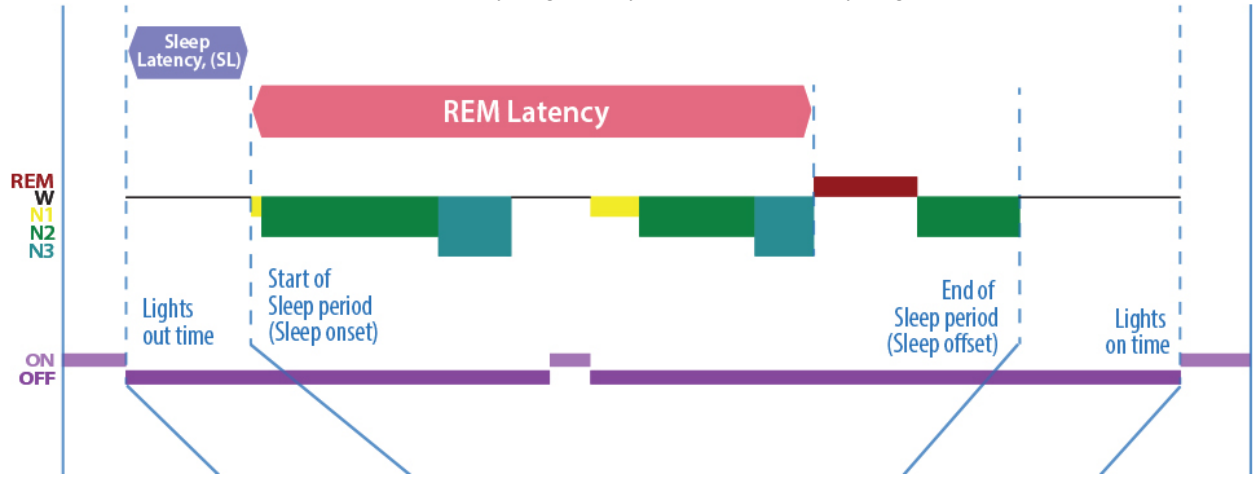

Start recording	Lights out	Sleep onset	Sleep offset	Lights on	End Recording
23:06:47	23:07:17	23:17:47	06:40:46	6:47:16	06:47:36

Sleep availability time	7:23:00
Time available for sleep	6:08:30
Total recording time (TRT)	7:40:49


DISCLAIMER: This data in this report has been automatically generated with no manual review. It is not intended for clinical interpretation purposes. Clinical interpretation can only be performed by a suitably qualified sleep medicine practitioner.

RESPIRATORY EVENTS (BY STAGING AND POSITION)

	REM	NREM	Total	Head Supine	Head Non-Supine
Qty Respiratory Events	13	31	44	0	44
Sleep Duration (TST)	49.5 min	172.0 min	221.5 min	6 min	216 min
pAHI (≥3%)	15.8 /hr	10.8 /hr	**11.9 /hr**	0.0 /hr	12.2 /hr
Monitoring Time (MT)			329.9 min	28 min	302 min
REI			17.8 /hr	72.0 /hr	12.7 /hr
ODI (≥3%)	17.0 /hr	10.1 /hr	11.6 /hr	32.7 /hr	11.1 /hr
ODI (≥4%)	14.5 /hr	5.2 /hr	7.3 /hr		
Arousals Index	10.9 /hr	8.4 /hr	8.9 /hr	21.8 /hr	8.6 /hr
Snore Index	587.9 /hr	1057.7 /hr	952.7 /hr	524 /hr	964 /hr
Longest Resp. Event			82 sec		

Note: Respiratory events (RE) are identified using peripheral arterial tone, oxygen desaturation and changes in heart rate derived from oximetry. pAHI is defined as the number of valid respiratory events during TST divided by the TST. REI is defined as the number of valid respiratory events during MT divided by the MT.

pAHI GRAPH

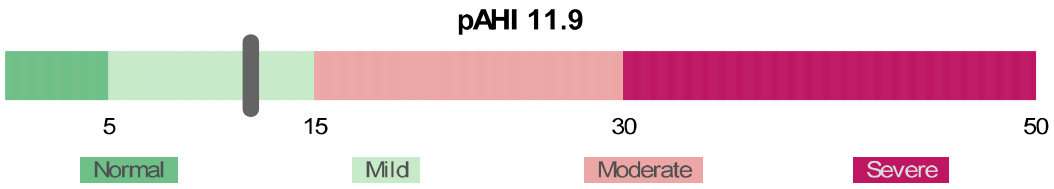

Reference values for AHI are in accordance with AASM guidelines.

OXYGEN SATURATION SUMMARY

	SpO_2	SpO_2 Time	Duration*	Sleep %*
Start (awake)	96 %	<90%	5.2 min	2.5 %
Average during sleep*	94 %	<88%	3.5 min	1.7 %
Minimum during sleep*	76 %	<85%	2.4 min	1.2 %
Largest desaturation	21 %	<80%	0.7 min	0.3 %

* Valid SpO2 measurement time is 205.6 minutes, determined by Total Sleep Time (TST) less any periods of baseline drift during TST.

VITAL SIGNS (FROM PPG)

	Average	Highest	Lowest
Pulse Rate (during Sleep)	69 BPM	86 BPM	57 BPM

DISCLAIMER: This data in this report has been automatically generated with no manual review. It is not intended for clinical interpretation purposes. Clinical interpretation can only be performed by a suitably qualified sleep medicine practitioner.



Somfit Automatic Report

Somfit Check SLEEP 1st®

STUDY QUALITY

	Start	+3Hrs	+6hrs	Rating
EEG Impedance – Right	101 kΩ	66 kΩ	60 kΩ	Adequate
EEG Impedance – Left	81 kΩ	52 kΩ	46 kΩ	Good
		%	%	Rating
Somfit Data Lost			17.0 %	Adequate
Unscorable Sleep Staging			18.0 %	Adequate
Total SpO_2 Artifact			27.0 %	Query
– Motion		8.0 %		
– Off		19.0 %		
– Low SNR		0.0 %		
– Low PI		0.0 %		
% Time of Baseline Drift			1.0 %	Good
Start Battery Level			100 %	Good
Battery Discharge Rate			3 %/hr	Good

DEVICE INFORMATION

Somfit Device	Somfit N/A
Somfit Service	Somfit Diagnostic
Somfit Firmware Version	116
Somfit App Version	5.2.0 (138)
Somfit Study Processing Version	SomfitBatch 2.1.0.106
Bluetooth Address	N/A
Bluetooth Connection Time	Night 7 23:06:47
App Start Date/Time	Night 7 23:06:47
App End Date/Time	Night 7 (+1 d) 06:47:36
Average Device Temperature	31.0 °C

PHONE INFORMATION

Phone Model	iPhone16
Phone OS	26.6.1
Phone Start Battery Level	45%
Phone End Battery Level	100.0%

DISCLAIMER: This data in this report has been automatically generated with no manual review. It is not intended for clinical interpretation purposes. Clinical interpretation can only be performed by a suitably qualified sleep medicine practitioner.


Somfit Automatic Report

Somfit Check SLEEP 1st®

PATIENT DETAILS				STUDY DETAILS			
Name	N/A	ID		Study Date	Night 9		
Age	26	BMI	kg/m^2	Start/End Time	21:59:55	–	05:51:19

GRAPHIC SUMMARY

DISCLAIMER: This data in this report has been automatically generated with no manual review. It is not intended for clinical interpretation purposes. Clinical interpretation can only be performed by a suitably qualified sleep medicine practitioner.

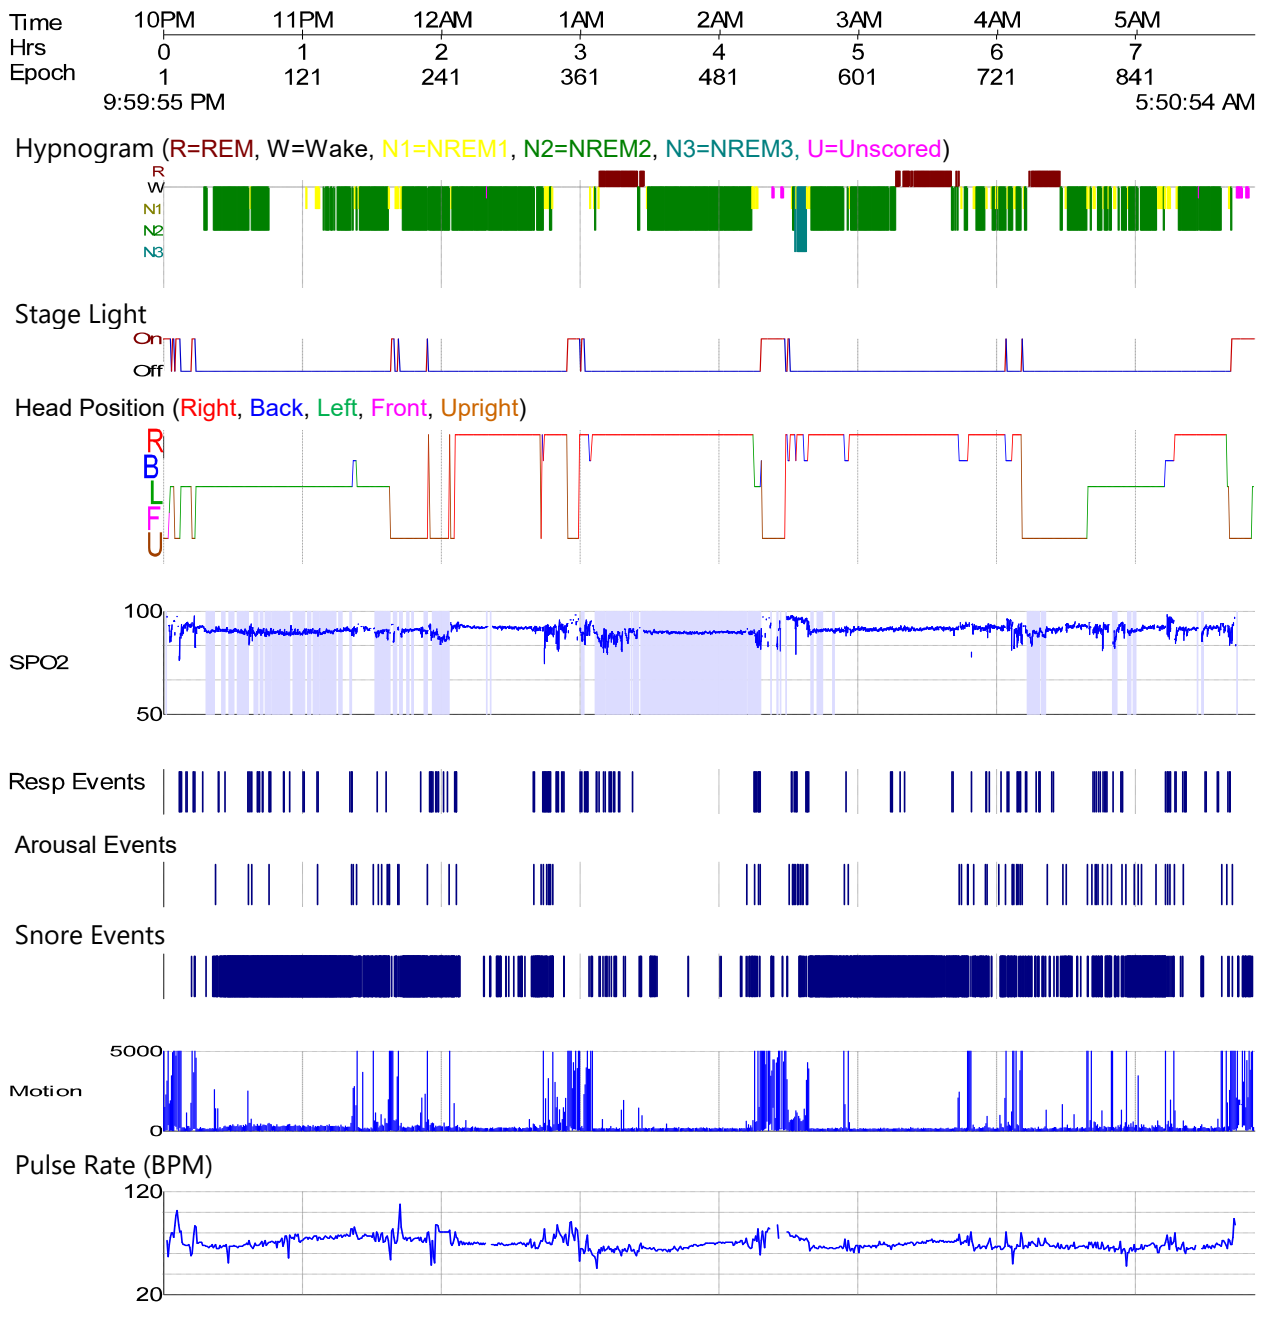

Note: periods of baseline drift are indicated by pale blue background shading on the SpO_2 graph. This time period is included for detection of respiratory events metrics (pAHI, ODI) but excluded for SpO_2 metrics calculations.

DISCLAIMER: This data in this report has been automatically generated with no manual review. It is not intended for clinical interpretation purposes. Clinical interpretation can only be performed by a suitably qualified sleep medicine practitioner.

Somfit Automatic Report

Somfit Check SLEEP 1st®

SLEEP STAGING SUMMARY

	Time	% of Sleep
N1 sleep	34.0 min	9.9 %
N2 sleep	252.0 min	73.0 %
N3 sleep	4.5 min	1.3 %
REM sleep	54.5 min	15.8 %
NREM sleep	290.5 min	84.2 %

	Time	
Sleep (TST)	345.0 min	
Wake	109.5 min	(SOL + WASO)
Sleep efficiency	80.0 %	


SLEEP TIME STATISTICS

	Time
Total Recording Time (TRT)	7:51:24 hh:mm:ss
Time Available for Sleep	7:11:00 hh:mm:ss
Total Sleep Time (TST)	5:45:00 hh:mm:ss
SpO_2 Artifact Time (during TST)	0:26:06 hh:mm:ss
Monitoring Time (MT)	6:32:33 hh:mm:ss
Sleep Onset Latency (SOL)	14.0 min
REM latency	170.5 min
Wake after sleep onset (WASO)*	95.5 min

**includes wake between sleep offset and lights on time*

STUDY TIMES

Reference hypnogram only – not actual patient hypnogram

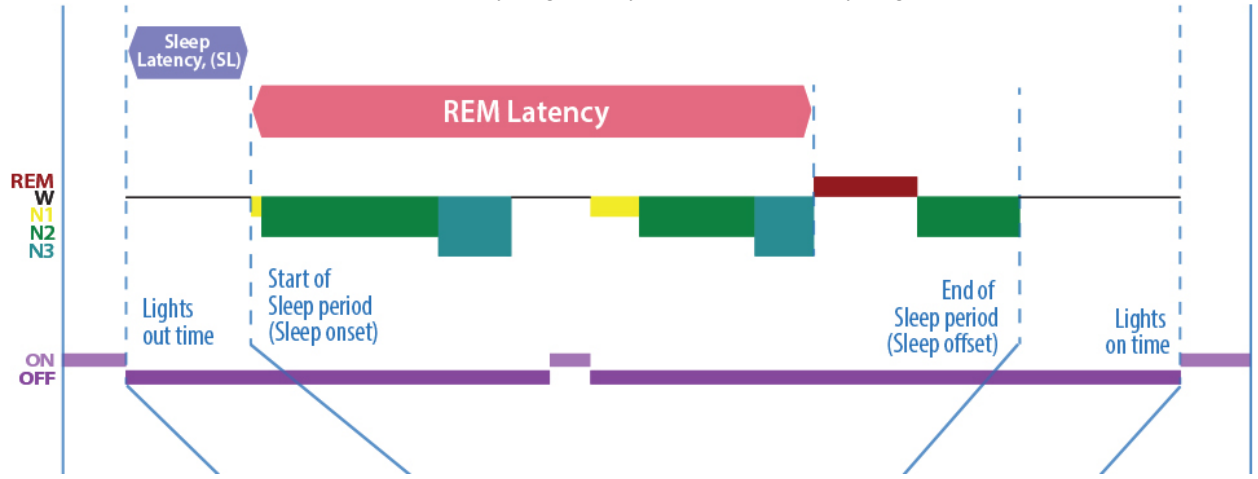

Start recording	Lights out	Sleep onset	Sleep offset	Lights on	End Recording
21:59:55	22:03:25	22:17:25	05:40:54	5:40:54	05:51:19

Sleep availability time	7:23:30
Time available for sleep	7:11:00
Total recording time (TRT)	7:51:24


DISCLAIMER: This data in this report has been automatically generated with no manual review. It is not intended for clinical interpretation purposes. Clinical interpretation can only be performed by a suitably qualified sleep medicine practitioner.

RESPIRATORY EVENTS (BY STAGING AND POSITION)

	REM	NREM	Total	Head Supine	Head Non-Supine
Qty Respiratory Events	18	98	116	11	105
Sleep Duration (TST)	54.5 min	290.5 min	345.0 min	10 min	335 min
pAHI (≥3%)	19.8 /hr	20.2 /hr	**20.2 /hr**	66.0 /hr	18.8 /hr
Monitoring Time (MT)			392.6 min	15 min	377 min
REI			25.5 /hr	63.4 /hr	24.0 /hr
ODI (≥3%)	18.7 /hr	15.9 /hr	16.3 /hr	54.0 /hr	15.2 /hr
ODI (≥4%)	13.2 /hr	11.4 /hr	11.7 /hr		
Arousals Index	2.2 /hr	12.4 /hr	10.8 /hr	60.0 /hr	9.3 /hr
Snore Index	475.6 /hr	575.2 /hr	559.5 /hr	450 /hr	563 /hr
Longest Resp. Event			67 sec		

Note: Respiratory events (RE) are identified using peripheral arterial tone, oxygen desaturation and changes in heart rate derived from oximetry. pAHI is defined as the number of valid respiratory events during TST divided by the TST. REI is defined as the number of valid respiratory events during MT divided by the MT.

pAHI GRAPH

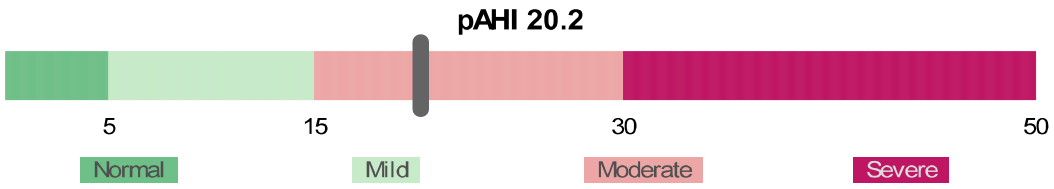

Reference values for AHI are in accordance with AASM guidelines.

OXYGEN SATURATION SUMMARY

	SpO_2	SpO_2 Time	Duration*	Sleep %*
Start (awake)	91 %	<90%	17.3 min	8.1 %
Average during sleep*	91 %	<88%	4.0 min	1.9 %
Minimum during sleep*	76 %	<85%	1.0 min	0.5 %
Largest desaturation	18 %	<80%	0.1 min	0.0 %

* Valid SpO2 measurement time is 213.7 minutes, determined by Total Sleep Time (TST) less any periods of baseline drift during TST.

VITAL SIGNS (FROM PPG)

	Average	Highest	Lowest
Pulse Rate (during Sleep)	69 BPM	83 BPM	57 BPM

DISCLAIMER: This data in this report has been automatically generated with no manual review. It is not intended for clinical interpretation purposes. Clinical interpretation can only be performed by a suitably qualified sleep medicine practitioner.



Somfit Automatic Report

Somfit Check SLEEP 1st®

STUDY QUALITY

	Start	+3Hrs	+6hrs	Rating
EEG Impedance – Right	83 kΩ	33 kΩ	37 kΩ	Good
EEG Impedance – Left	80 kΩ	35 kΩ	39 kΩ	Good
		%	%	Rating
Somfit Data Lost			1.0 %	Good
Unscorable Sleep Staging			1.0 %	Good
Total SpO_2 Artifact			13.0 %	Adequate
– Motion		11.0 %		
– Off		2.0 %		
– Low SNR		0.0 %		
– Low PI		0.0 %		
% Time of Baseline Drift			31.0 %	Adequate
Start Battery Level			100 %	Good
Battery Discharge Rate			4 %/hr	Good

DEVICE INFORMATION

Somfit Device	Somfit N/A
Somfit Service	Somfit Diagnostic
Somfit Firmware Version	116
Somfit App Version	5.2.0 (138)
Somfit Study Processing Version	SomfitBatch 2.1.0.106
Bluetooth Address	N/A
Bluetooth Connection Time	Night 9 21:59:55
App Start Date/Time	Night 9 21:59:55
App End Date/Time	Night 9 (+1 d) 05:51:35
Average Device Temperature	29.0 °C

PHONE INFORMATION

Phone Model	iPhone16
Phone OS	26.6.1
Phone Start Battery Level	95%
Phone End Battery Level	100.0%

DISCLAIMER: This data in this report has been automatically generated with no manual review. It is not intended for clinical interpretation purposes. Clinical interpretation can only be performed by a suitably qualified sleep medicine practitioner.