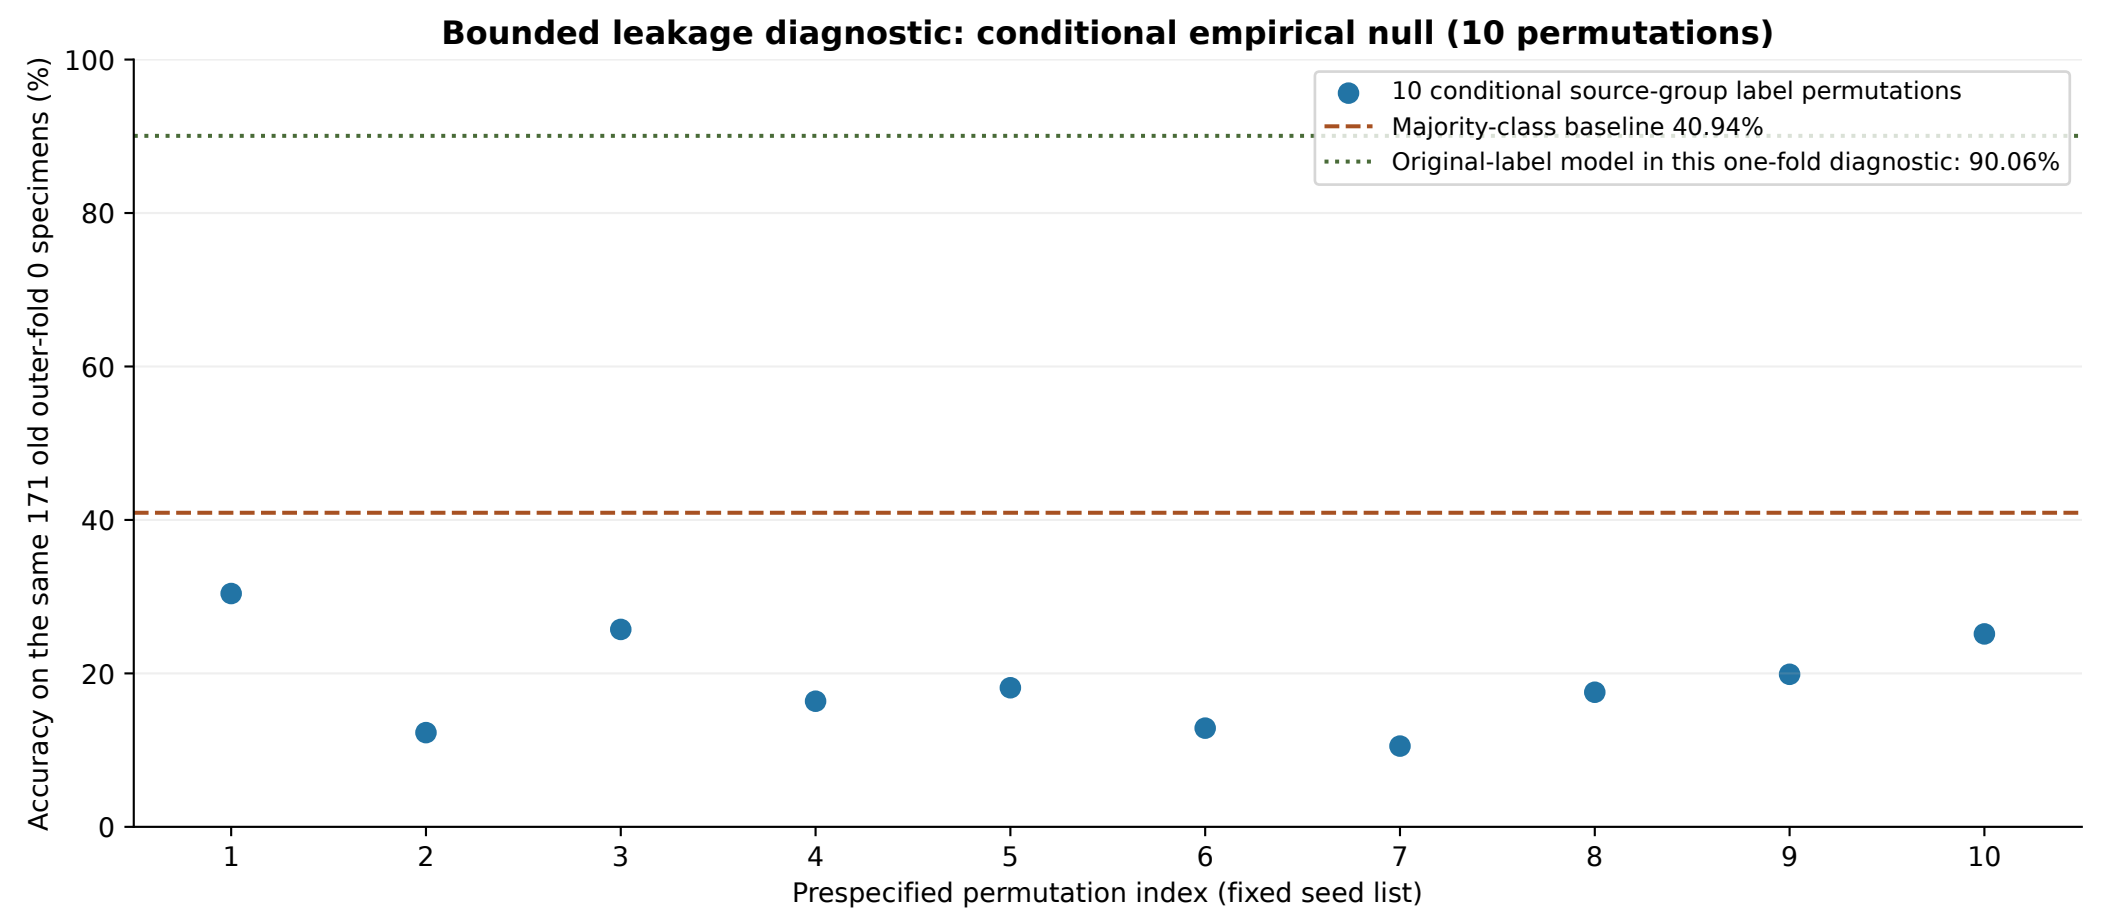

Each permutation reruns source-only MC-UVE and inner SVM selection. The same 171 query specimens are reused.
Plus-one resolution is 1/11; not a 1/7 acceptance rule or a biological/cross-batch significance certificate.