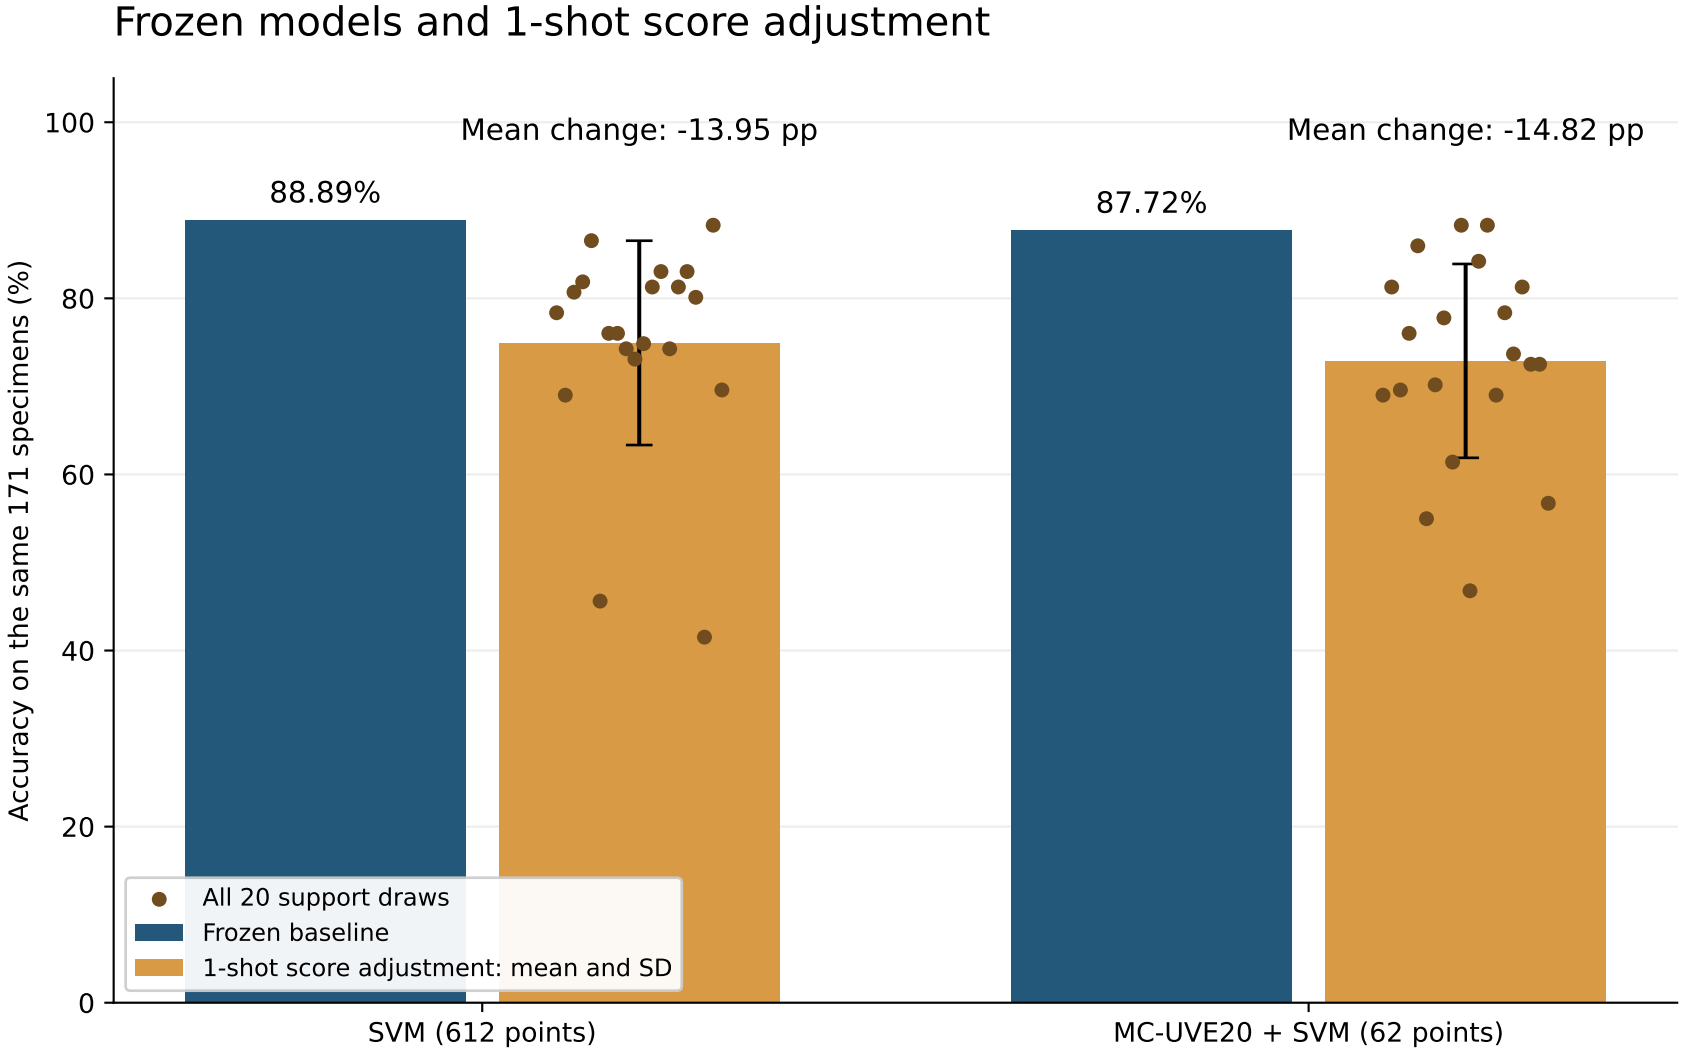

Retrospective within-batch split; 7 support specimens per draw.
ZY02 has 1 query specimen. Draw SD is not an independent-batch confidence interval.