
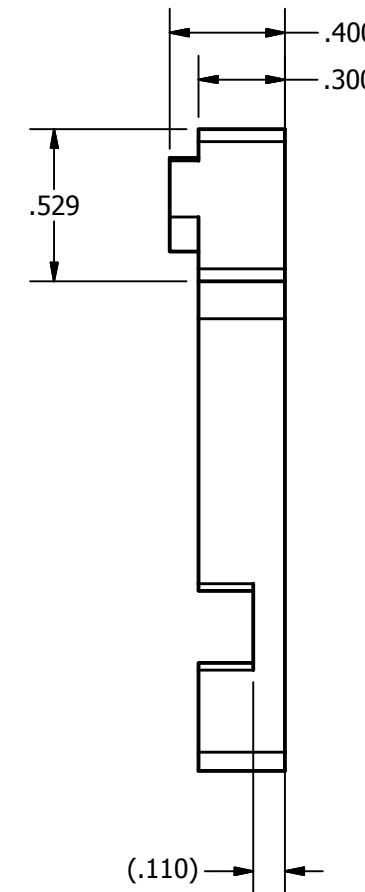
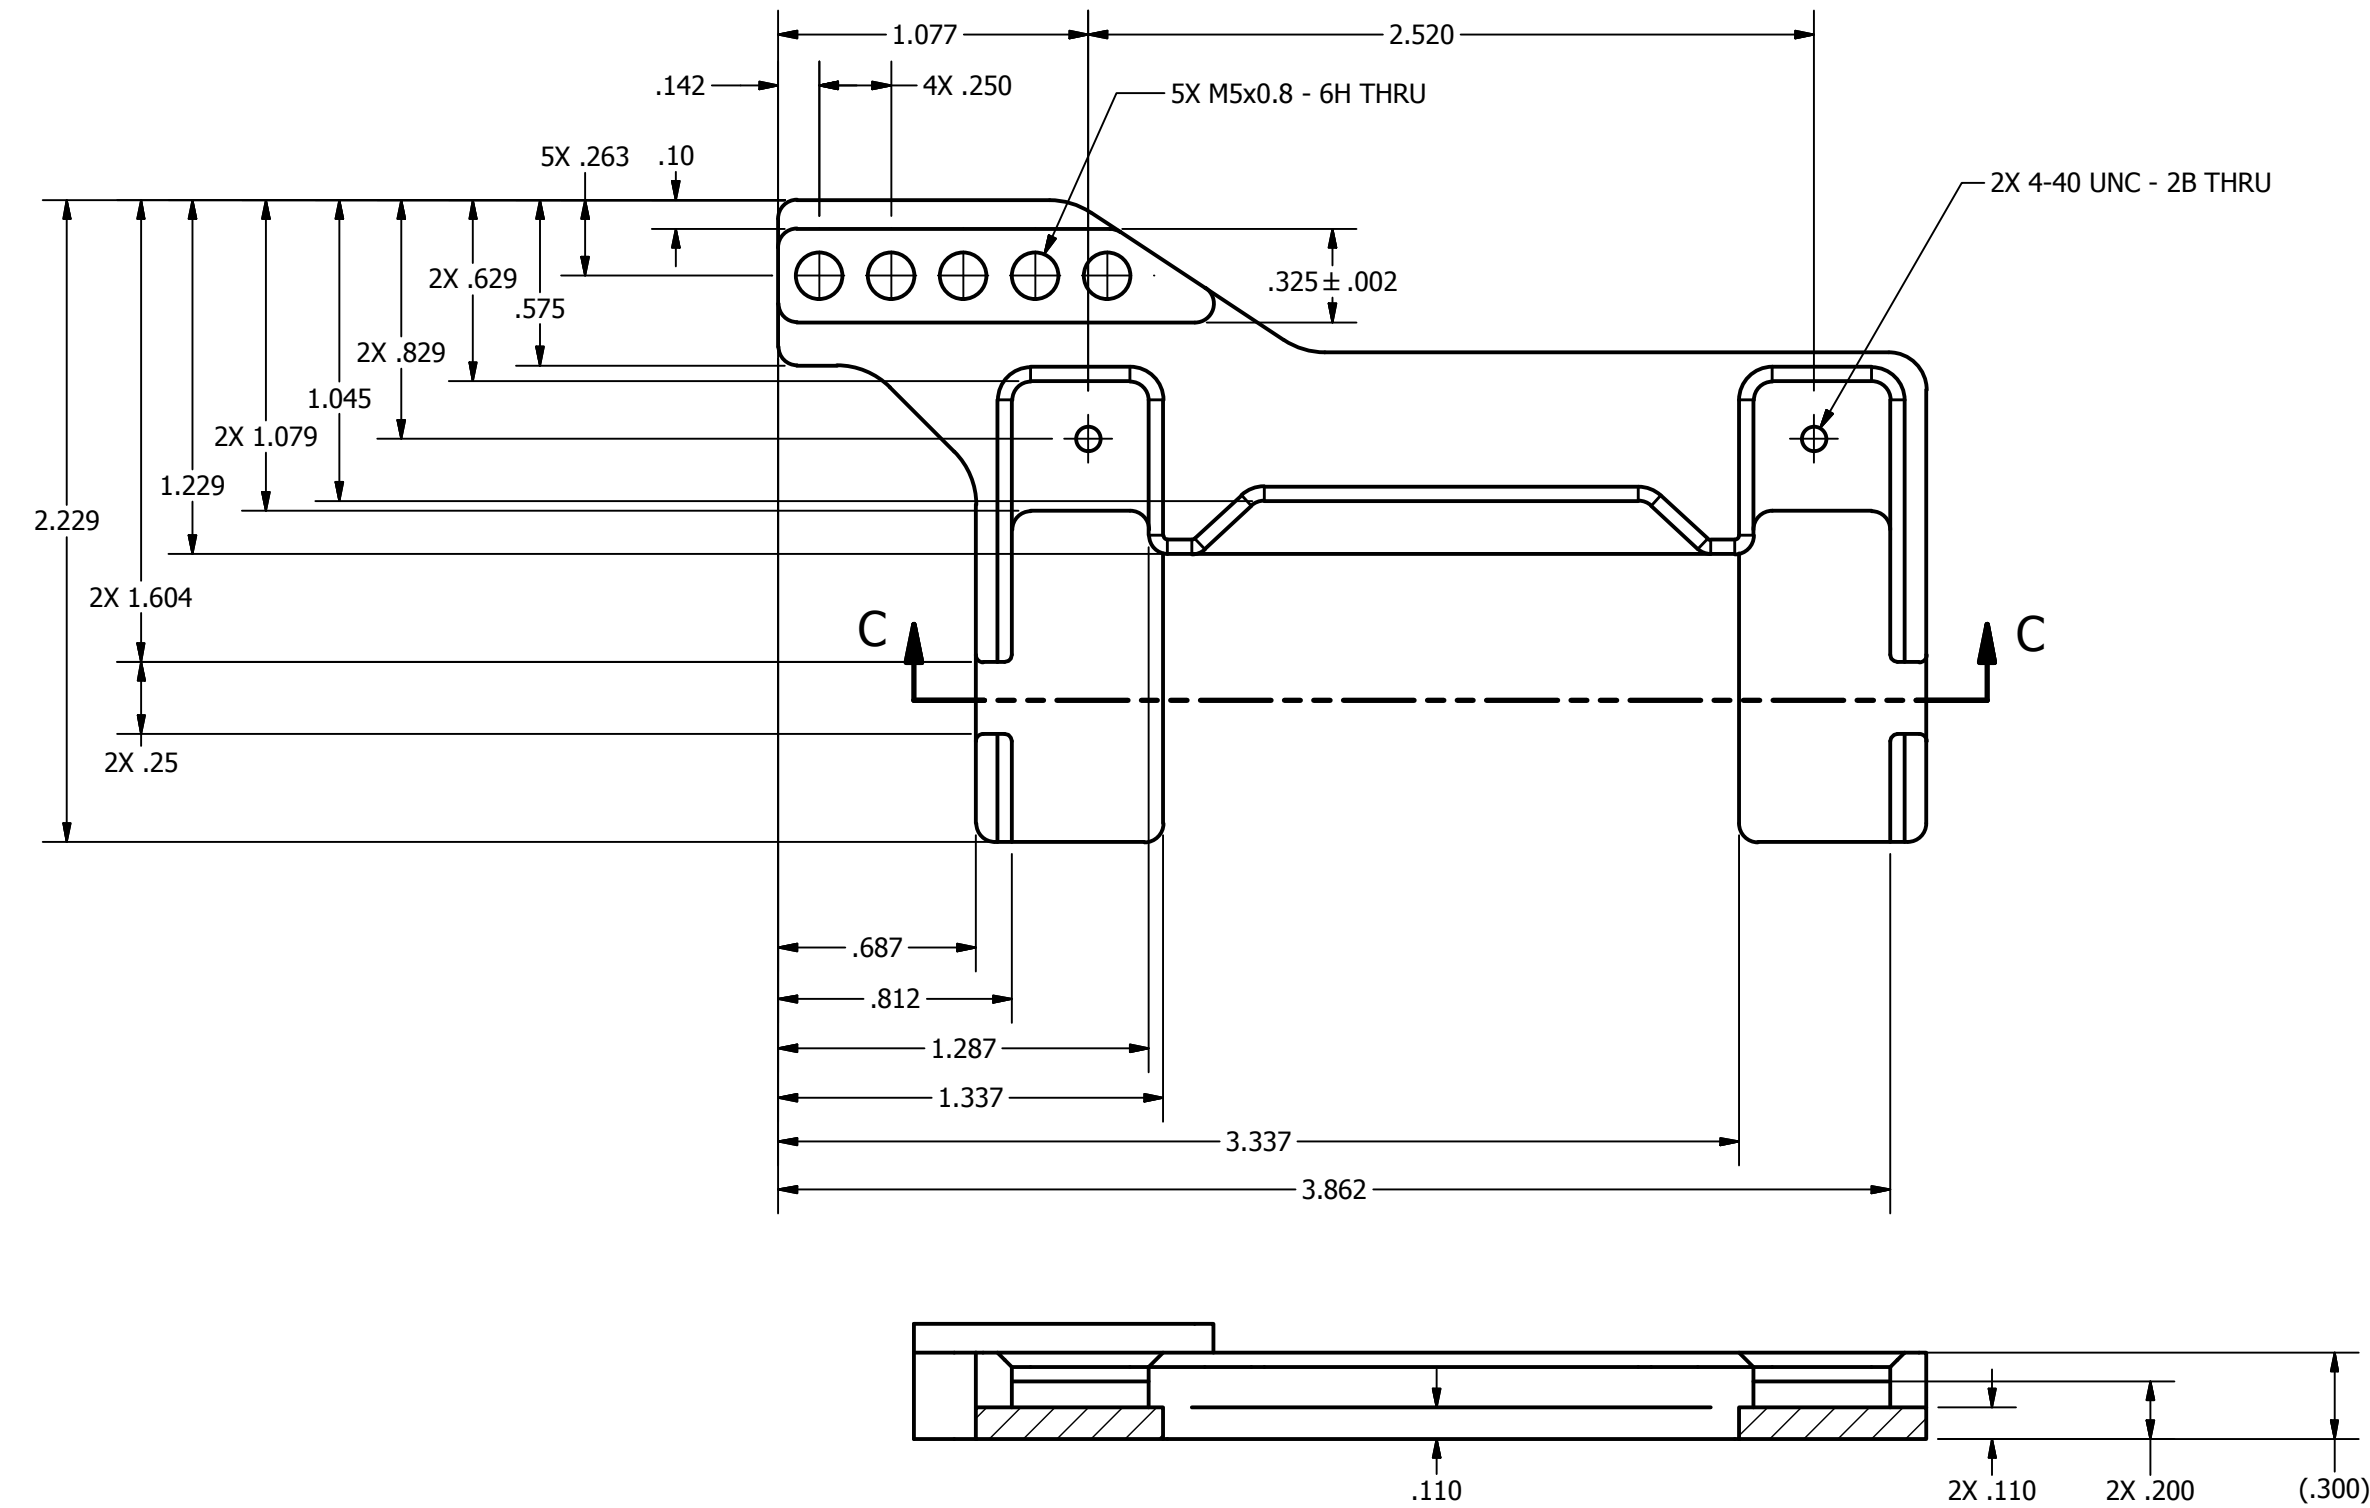


1. MATERIAL: **ALUMINUM, 6061-T651**
2. SPECIAL FINISH: **NONE**
3. SURFACE ROUGHNESS (UNLESS SPECIFIED OTHERWISE): **63 Ra** (AVERAGE MICRO-INCHES)
4. INTERPRET DIMENSIONS AND TOLERANCES PER ASME Y14.5M-1994
5. DEBURR AND BREAK ALL SHARP EDGES, MAX 0.010" (UNLESS SPECIFIED OTHERWISE)
6. PARTS ARE TO BE CLEAN AND FREE OF OIL, GREASE, AND OTHER CONTAMINANTS
7. DIMENSIONS INCLUDE ANODIZING, ELECTROPLATING, AND CHEMICALLY APPLIED FINISHES IF APPLICABLE

1. THIS DRAWING SHOWS CRITICAL DIMENSIONS THAT OTHERWISE CAN'T BE INTERPRETED FROM THE CORRESPONDING 3D MODEL. ALL OTHER GEOMETRY SHALL BE DETERMINED FROM THE CORRESPONDING 3D MODEL.

2. ALL GEOMETRY AND SURFACE PROFILES SHALL BE HELD TO WITHIN $\pm 0.005"$ OF THE PROVIDED 3D MODEL UNLESS SPECIFIED OTHERWISE.

1. CLARIZEN PROJECT NUMBER: **P-201804**
2. REQUESTING LAB/DEPT: **SVOBODA (LAB)**
3. REQUESTING SCIENTIST: **SOFRONIEW, NICK**
4. DESIGN DEPARTMENT: **HHMI: JRC - ID&F**

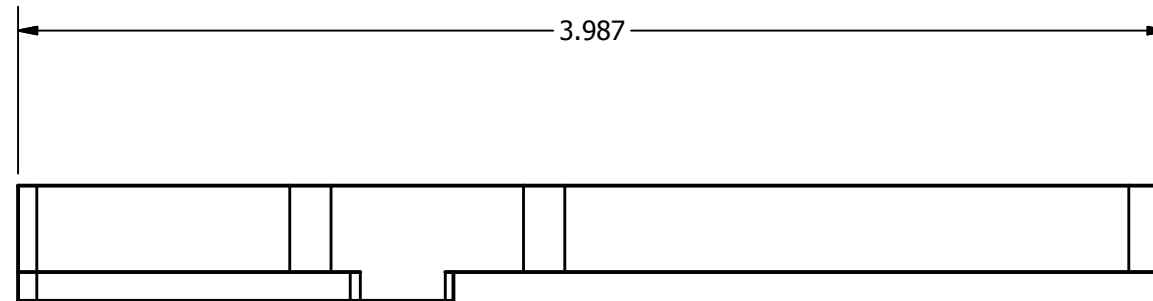

NOTICE:
INFORMATION CONTAINED IN THIS DOCUMENT OR ANY REPRODUCTION THEREOF, IS PROPRIETARY INFORMATION AND PROPERTY OF HOWARD HUGHES MEDICAL INSTITUTE. IT SHALL NOT BE DISCLOSED, COPIED, DUPLICATED OR USED FOR MANUFACTURE, PRODUCTION OR PROCUREMENT, WITHOUT THE EXPRESS WRITTEN PERMISSION OF HOWARD HUGHES MEDICAL INSTITUTE.

 Howard Hughes Medical Institute		 	
MBS INLINE SLIDE HOLDER.ipt			
SIZE C	PART NUMBER J005316	REV -	SHEET 1 OF 1