



REVISION HISTORY				
ZONE	REV	DESCRIPTION	DATE	APPROVED
	-	INITIAL RELEASE	2018/11/15	HHMI\\arnoldj



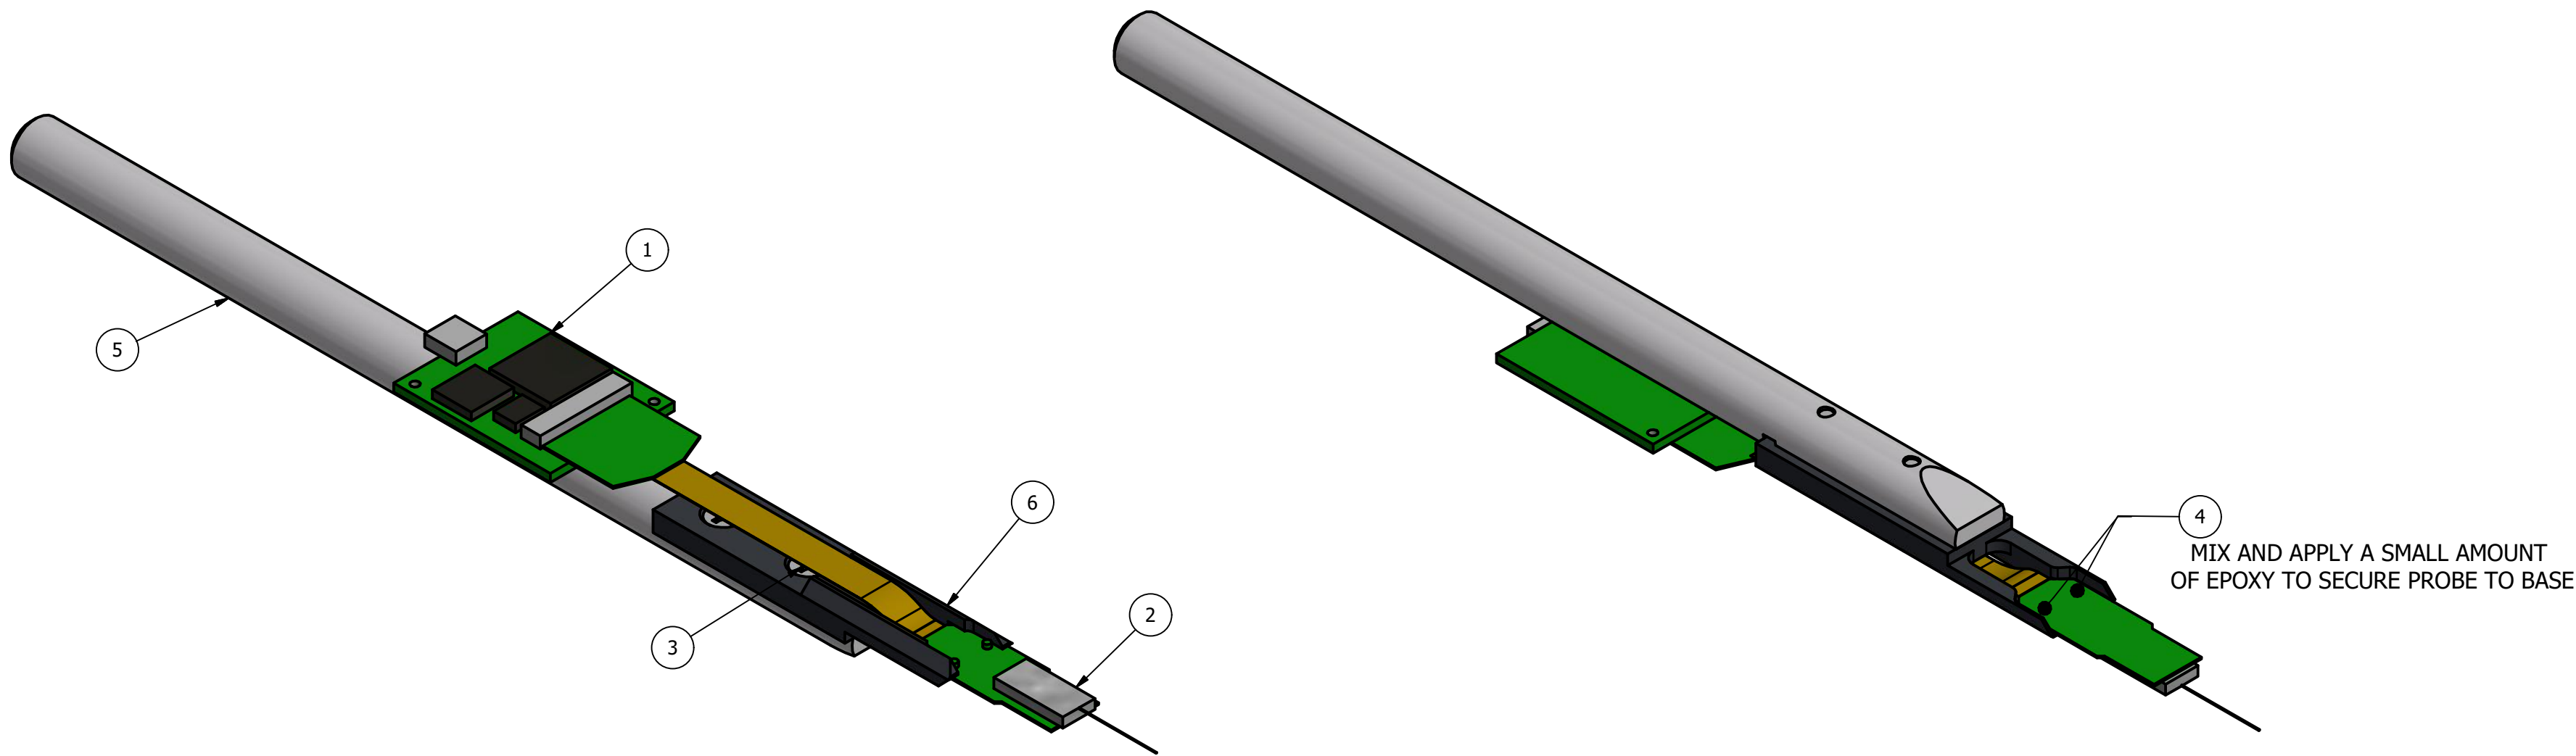

1	1	NEUROPIXEL HEADSTAGE PCB	-	IMEC
2	1	NEUROPIXEL 3A PROBE	-	IMEC
3	2	SCREW, FHP, M2 x 6, SS	92010A003	MCMASTER
4	A/R	LOCTITE EPOXY 5 MINUTE INSTANT MIX	1365868	HENKEL
5	1	PTR RECORDING POST 1/4" DIA EXTENDED	J007626	HHMI: JRC - ID&F
6	1	NEUROPIXEL 3A PROBE BASE	J007803	HHMI: JRC - ID&F
ITEM	QTY	DESCRIPTION	PART NUMBER	VENDOR
PARTS LIST				

NOTICE:
INFORMATION CONTAINED IN THIS DOCUMENT OR ANY REPRODUCTION THEREOF, IS PROPRIETARY INFORMATION AND PROPERTY OF HOWARD HUGHES MEDICAL INSTITUTE. IT SHALL NOT BE DISCLOSED, COPIED, DUPLICATED OR USED FOR MANUFACTURE, PRODUCTION OR PROCUREMENT, WITHOUT THE EXPRESS WRITTEN PERMISSION OF HOWARD HUGHES MEDICAL INSTITUTE.

(UNLESS SPECIFIED OTHERWISE)
PRIMARY UNITS: INCHES
[SECONDARY UNITS]: MILLIMETERS
PRIMARY TOLERANCES:
X.X ± 0.020
X.XX ± 0.010
X.XXX ± 0.005
X.XXXX ± 0.0005
ANGULAR ± 0.5 DEG
- DO NOT SCALE DRAWING -
THIRD ANGLE PROJECTION:



Howard Hughes
Medical Institute



Research Campus

NEUROPIXEL 3A PROBE AND ROD
HOLDER.iam