

Howard Hughes Medical Institute

Sheet: /power/
File: power.kicad_sch


Title: cluster-pcb

Size: A4 Date: 2024-09-13




KiCad E.D.A. kicad 7.0.11

Rev: 1.2

Id: 3/14

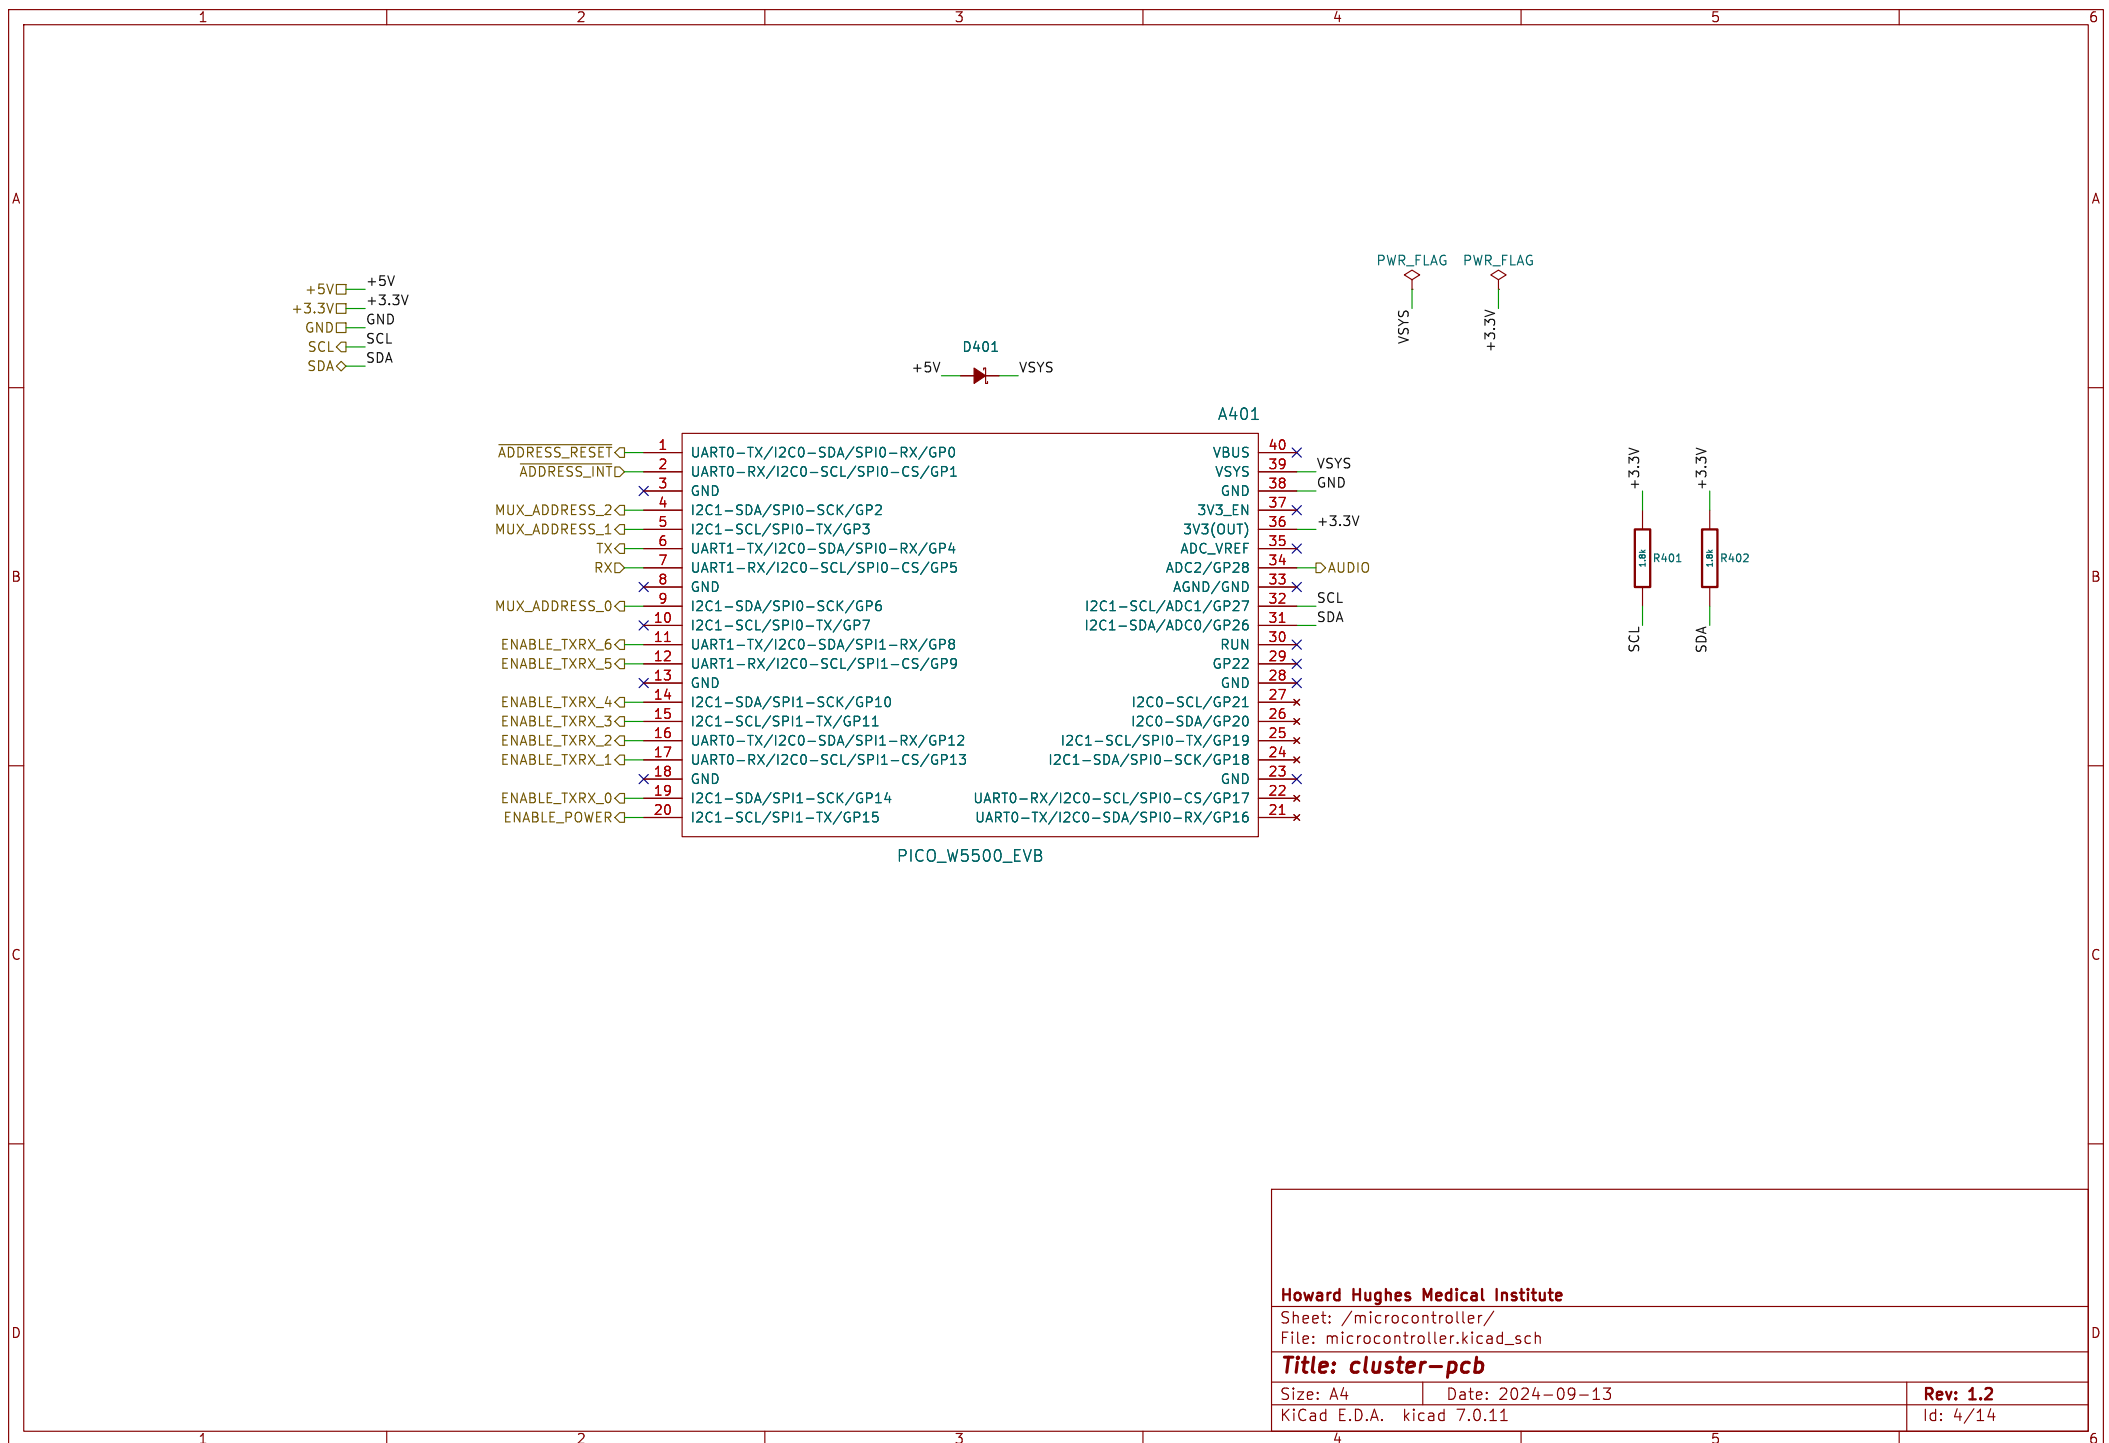

VAA □ VAA
+5V □ +5V
+3.3V □ +3.3V
GND □ GND

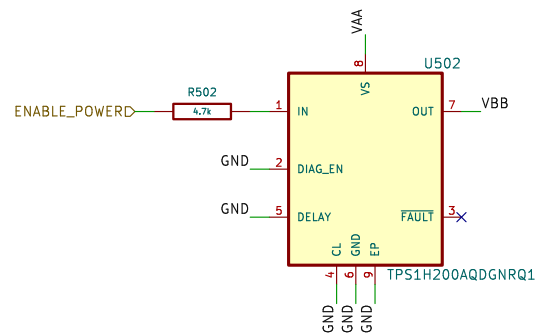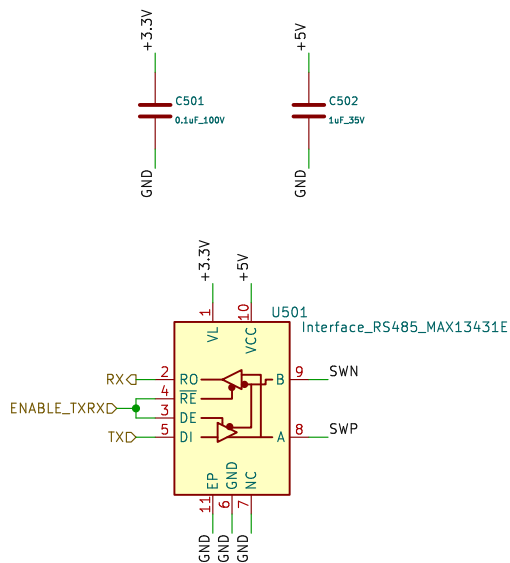

Howard Hughes Medical Institute

Sheet: /prism-0/
File: prism.kicad_sch

Title: cluster-pcb



Size: A4 Date: 2024-09-13

KiCad E.D.A. kicad 7.0.11

Rev: 1.2

Id: 5/14

VAA □ VAA
+5V □ +5V
+3.3V □ +3.3V
GND □ GND

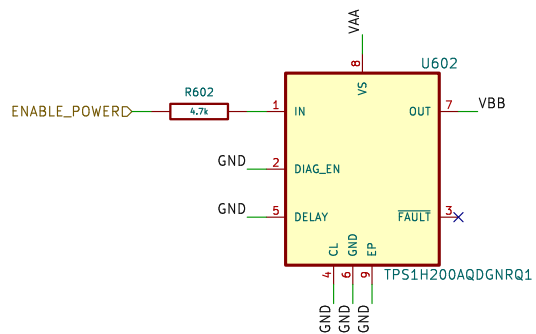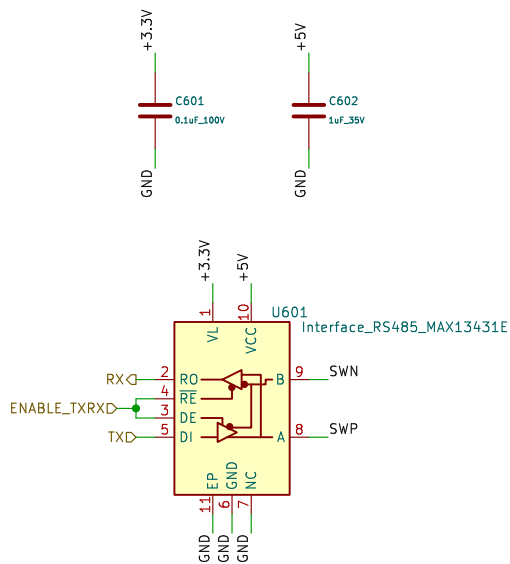

Howard Hughes Medical Institute

Sheet: /prism-1/
File: prism.kicad_sch

Title: cluster-pcb




Size: A4 Date: 2024-09-13

KiCad E.D.A. kicad 7.0.11

Rev: 1.2

Id: 6/14

VAA□—VAA
+5V□—+5V
+3.3V□—+3.3V
GND□—GND

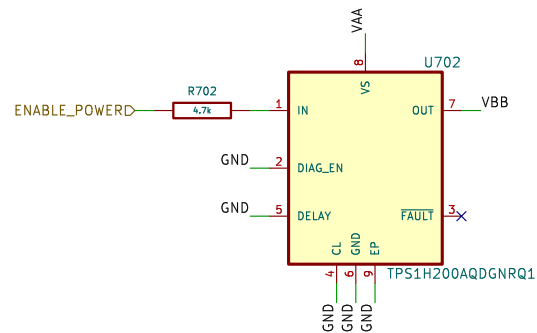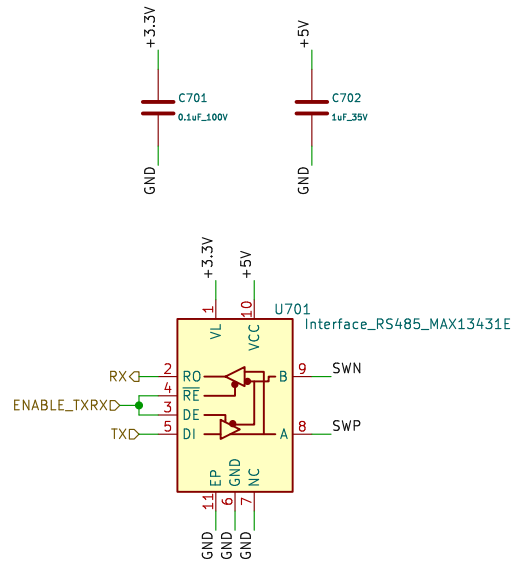

Howard Hughes Medical Institute

Sheet: /prism-2/

File: prism.kicad_sch

Title: cluster-pcb




Size: A4 Date: 2024-09-13

KiCad E.D.A. kicad 7.0.11

Rev: 1.2

Id: 7/14

VAA □ VAA
+5V □ +5V
+3.3V □ +3.3V
GND □ GND

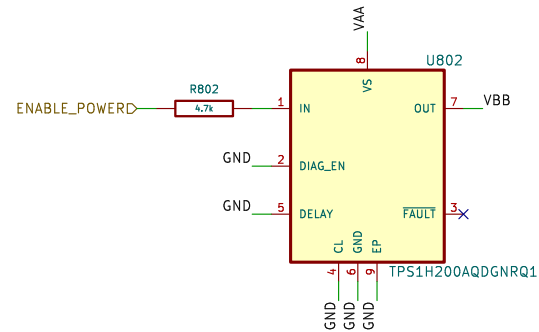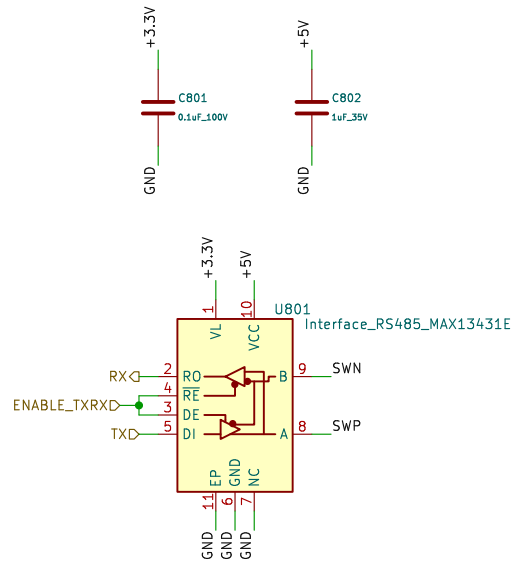

Howard Hughes Medical Institute

Sheet: /prism-3/
File: prism.kicad_sch


Title: cluster-pcb

Size: A4 Date: 2024-09-13

KiCad E.D.A. kicad 7.0.11




Rev: 1.2

Id: 8/14

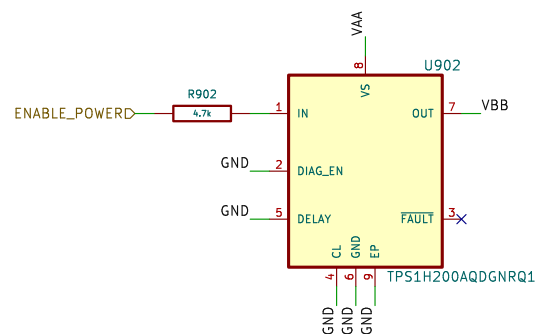

Id: 9/14

VAA□—VAA
+5V□—+5V
+3.3V□—+3.3V
GND□—GND

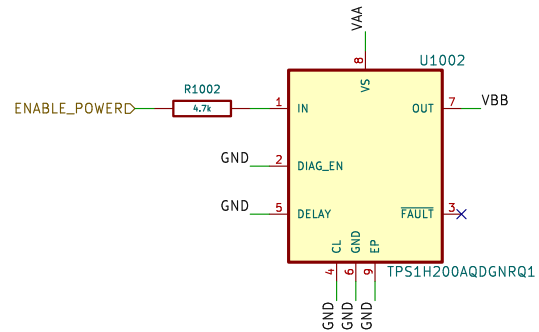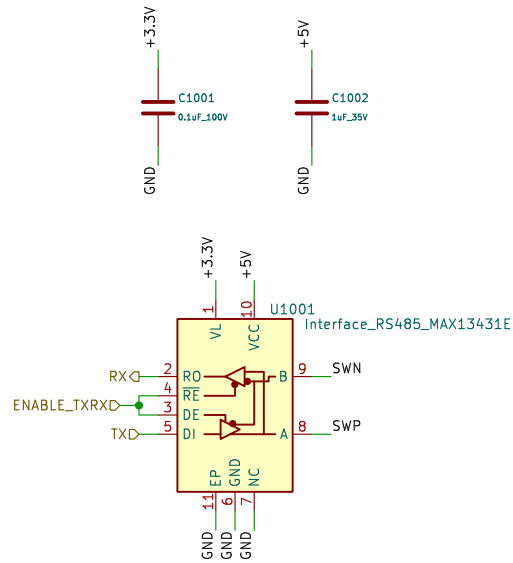

Howard Hughes Medical Institute

Sheet: /prism-4/

File: prism.kicad_sch

Title: cluster-pcb





Size: A4 Date: 2024-09-13

KiCad E.D.A. kicad 7.0.11

Rev: 1.2

Id: 10/14

VAA□—VAA
+5V□—+5V
+3.3V□—+3.3V
GND□—GND

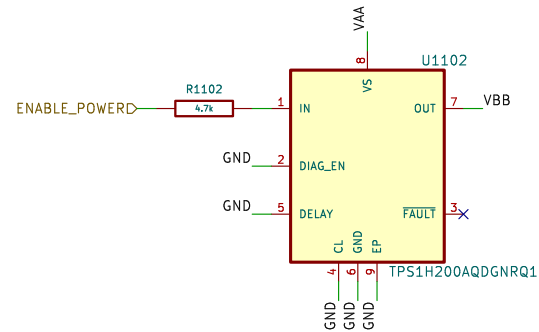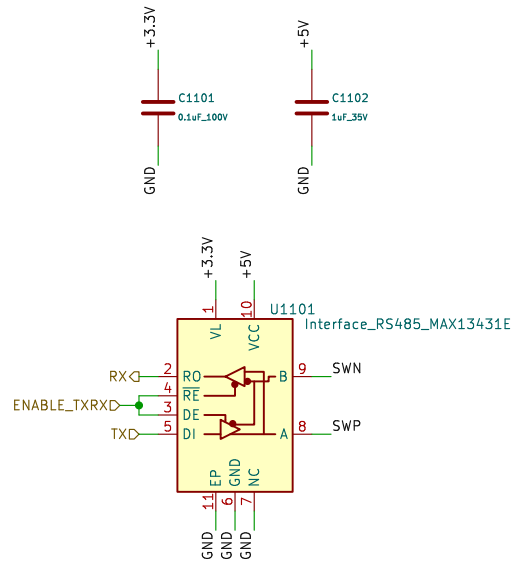

Howard Hughes Medical Institute

Sheet: /prism-6/

File: prism.kicad_sch

Title: cluster-pcb

Size: A4 Date: 2024-09-13


KiCad E.D.A. kicad 7.0.11

Rev: 1.2

Id: 11/14

Id: 12/14

Id: 13/14

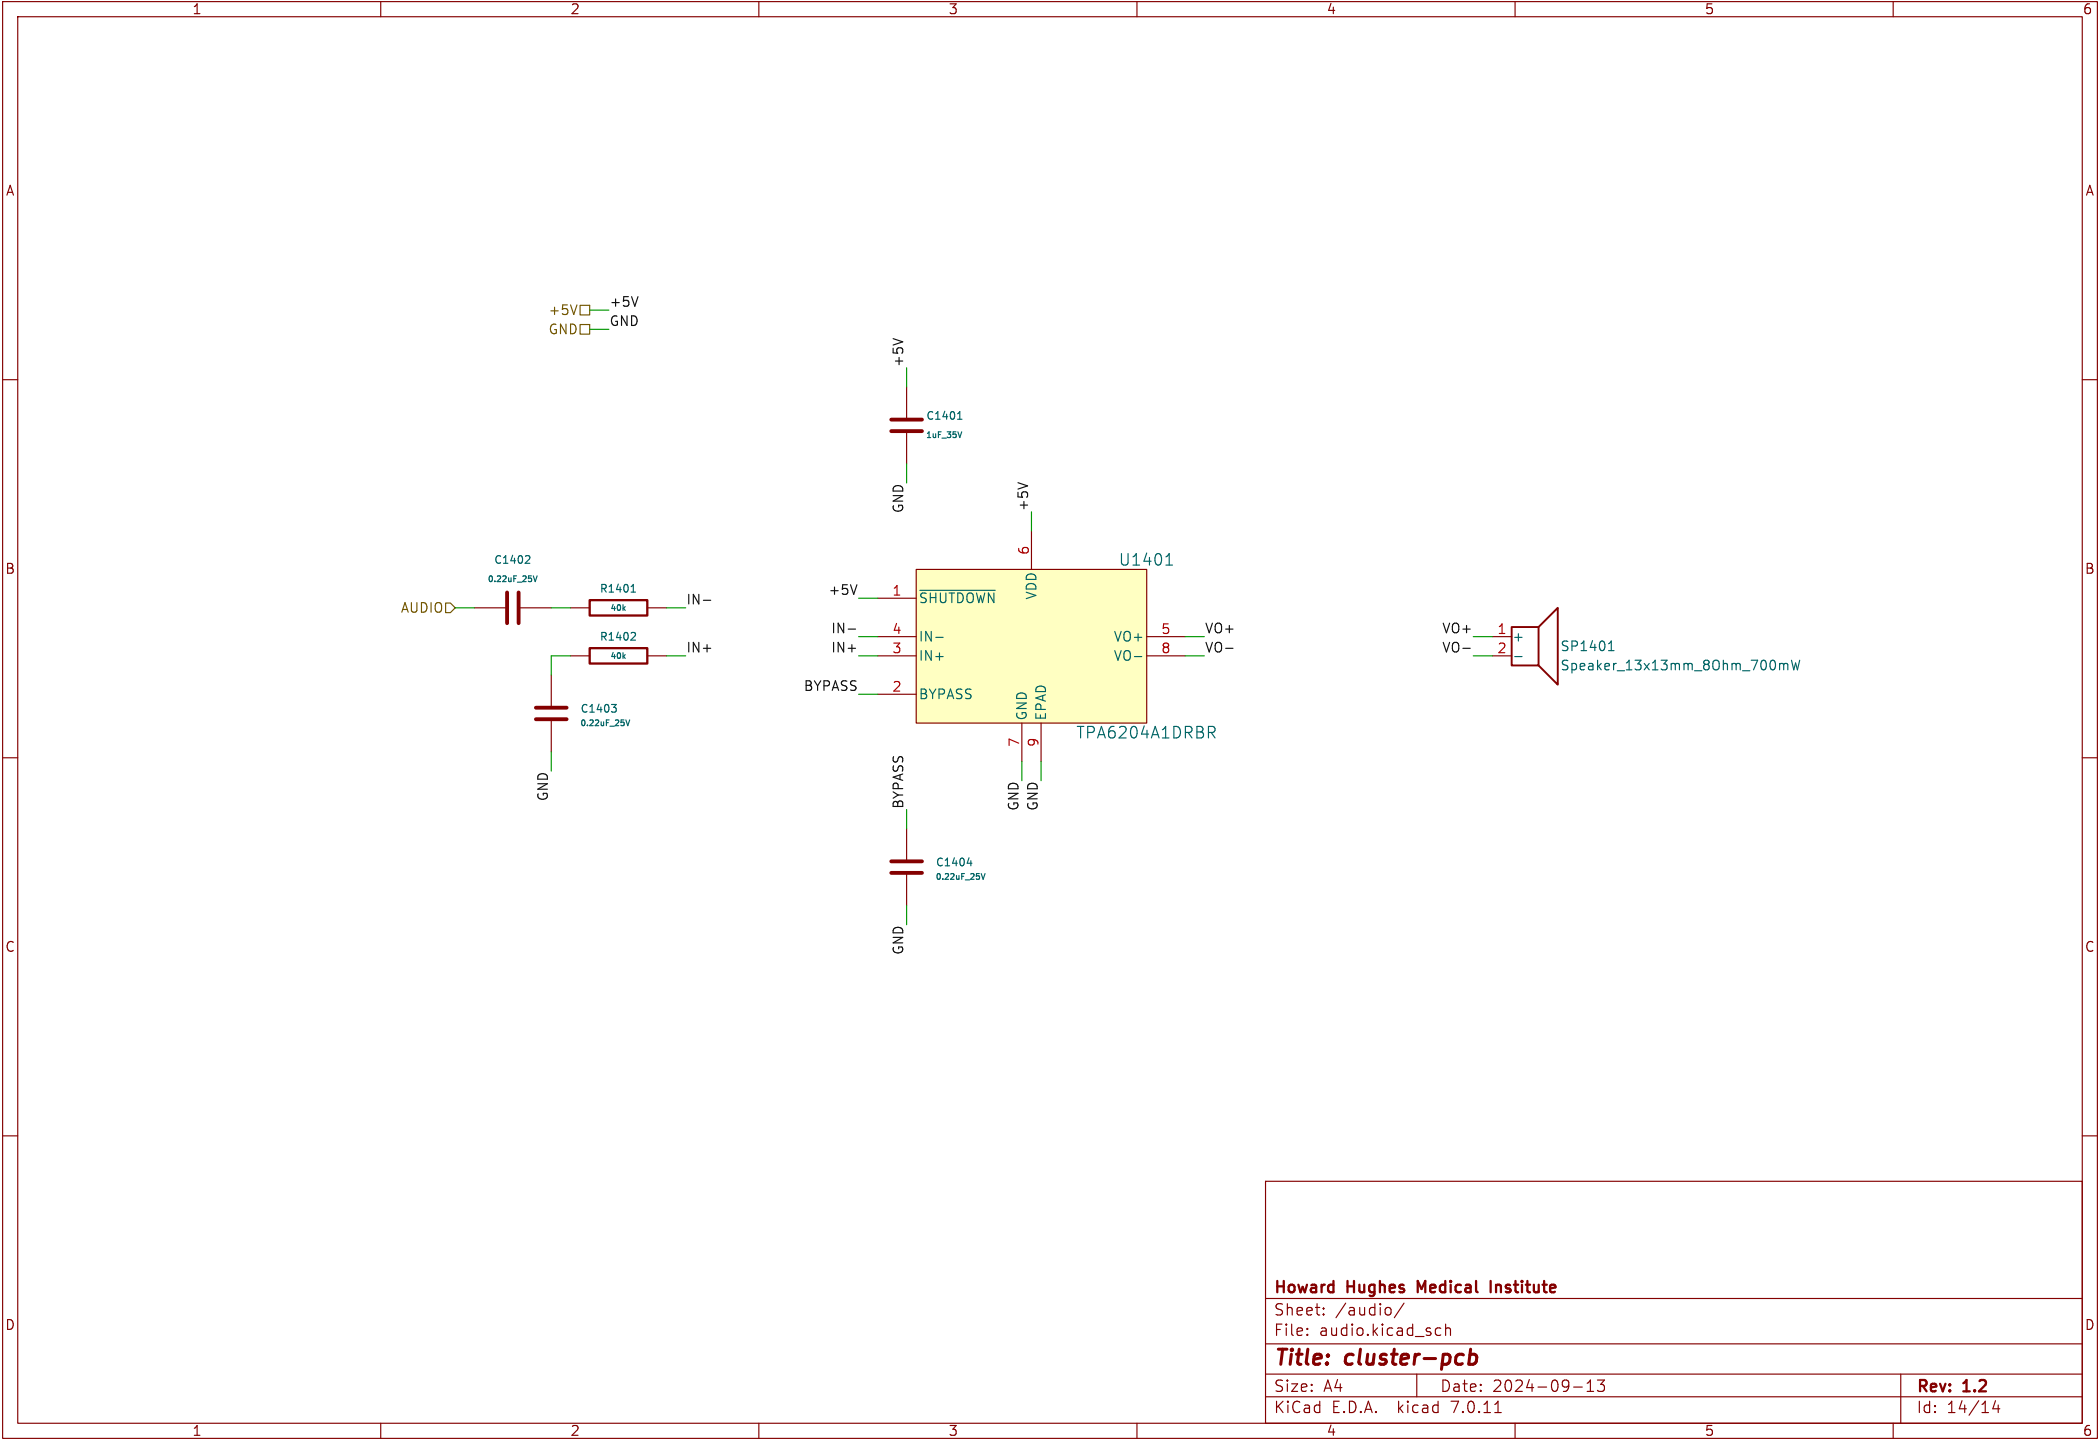

Howard Hughes Medical Institute

Sheet: /audio/
File: audio.kicad_sch

Title: cluster-pcb

Size: A4 Date: 2024-09-13

KiCad E.D.A. kicad 7.0.11

Rev: 1.2

Id: 14/14