

Howard Hughes Medical Institute

Sheet: /
File: cluster-pcb.kicad_sch


Title: cluster-pcb


Size: A4 Date: 2024-10-22


KiCad E.D.A. kicad 7.0.11

Rev: 2.1

Id: 1/13

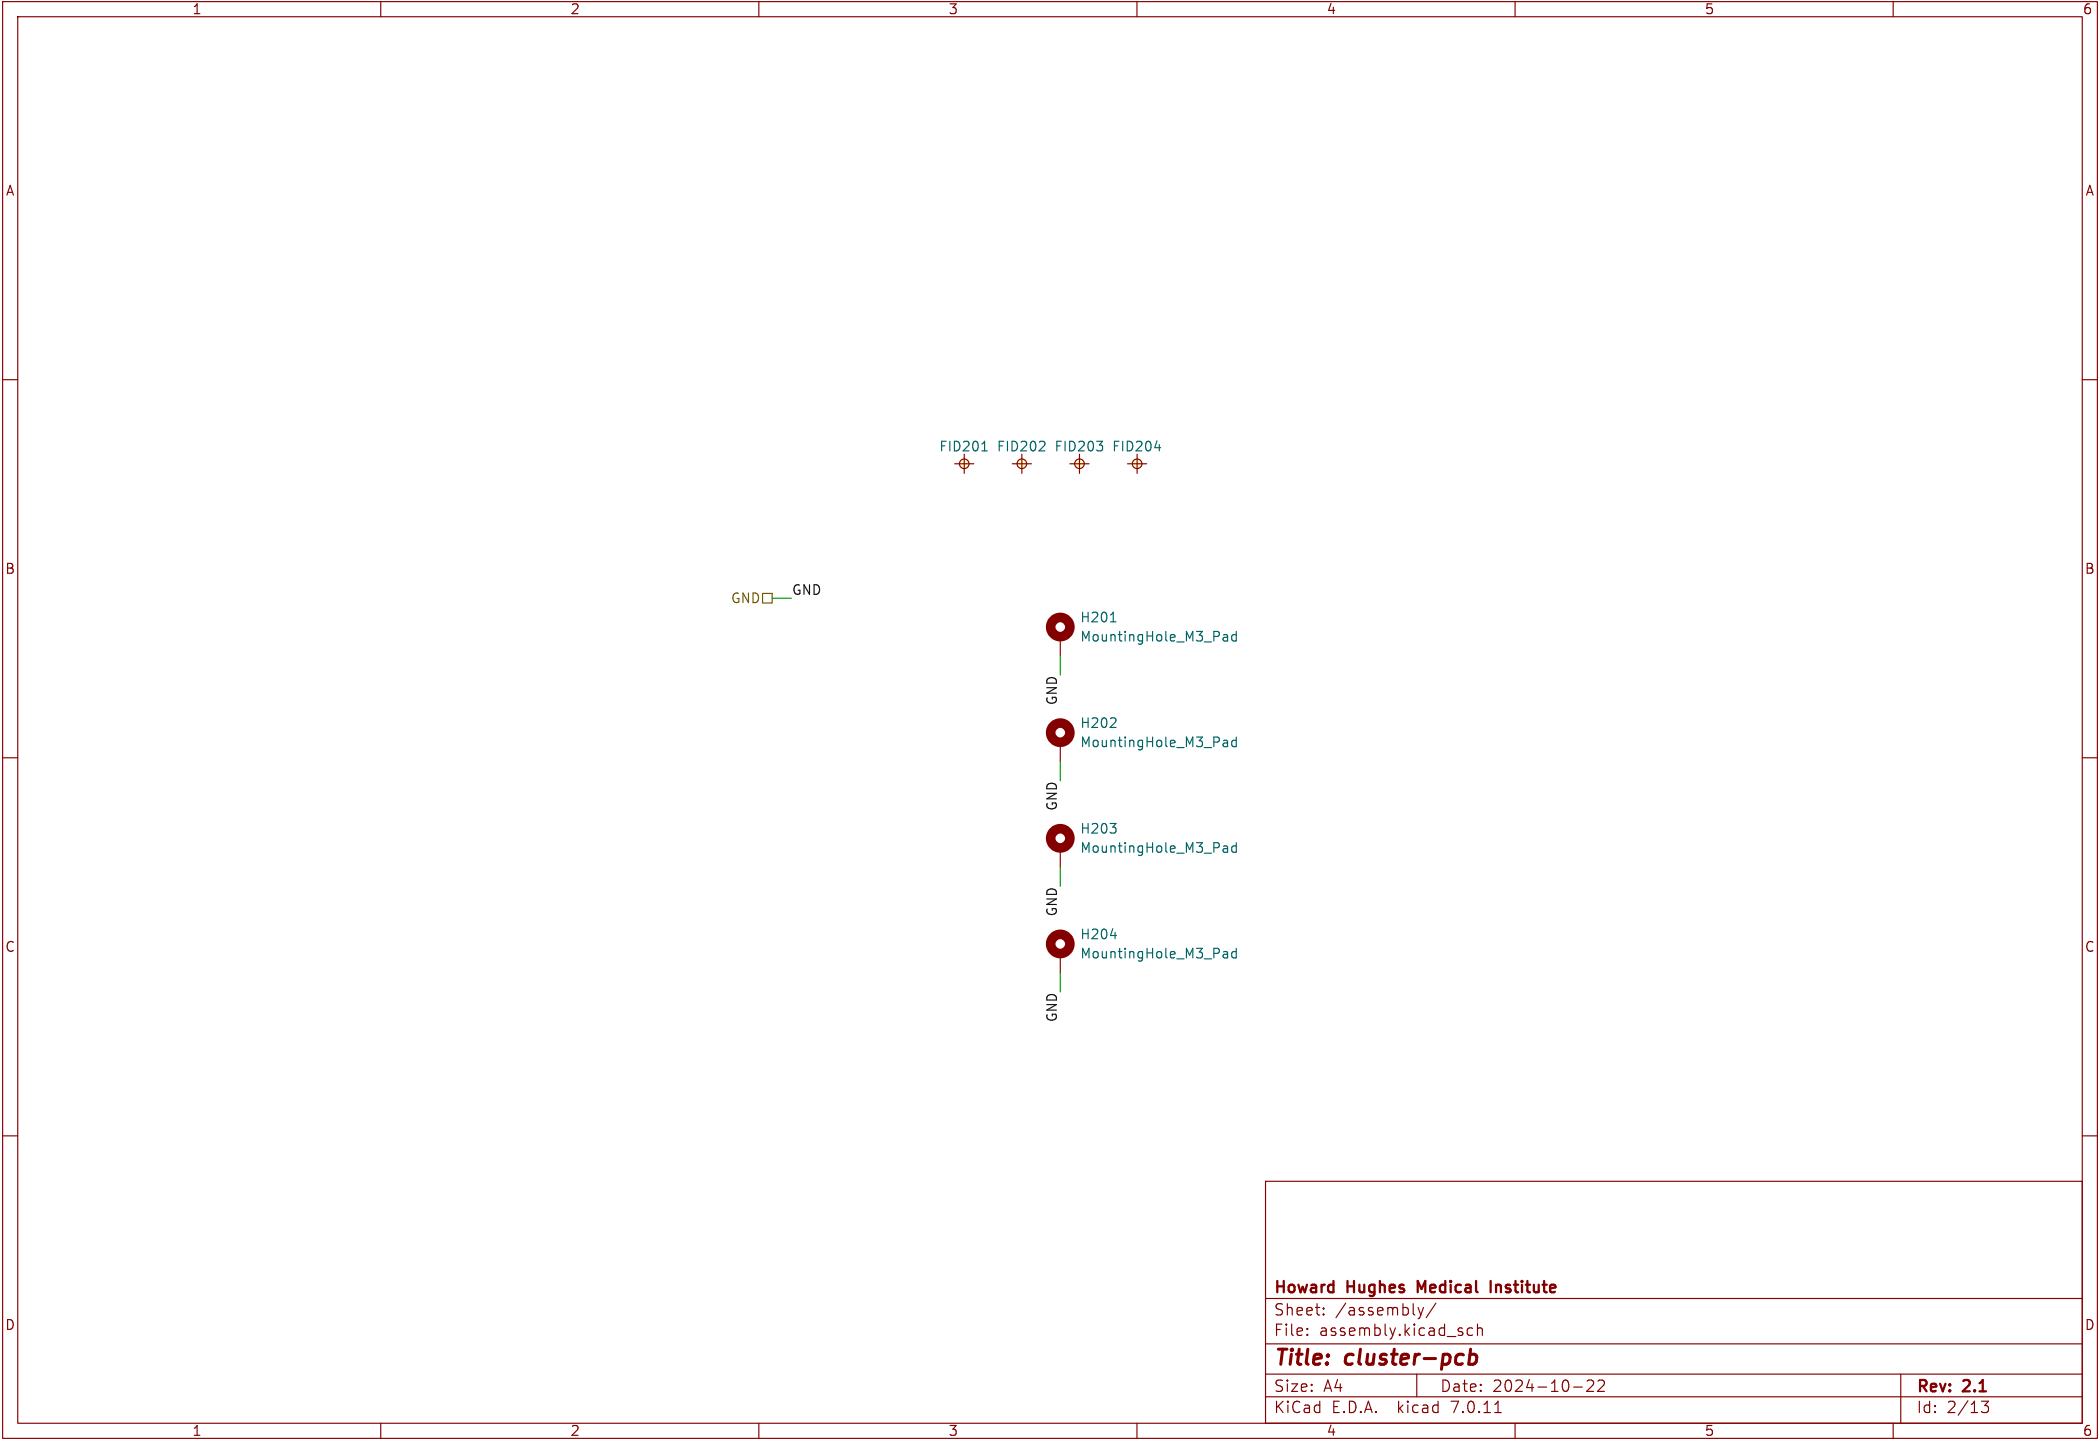

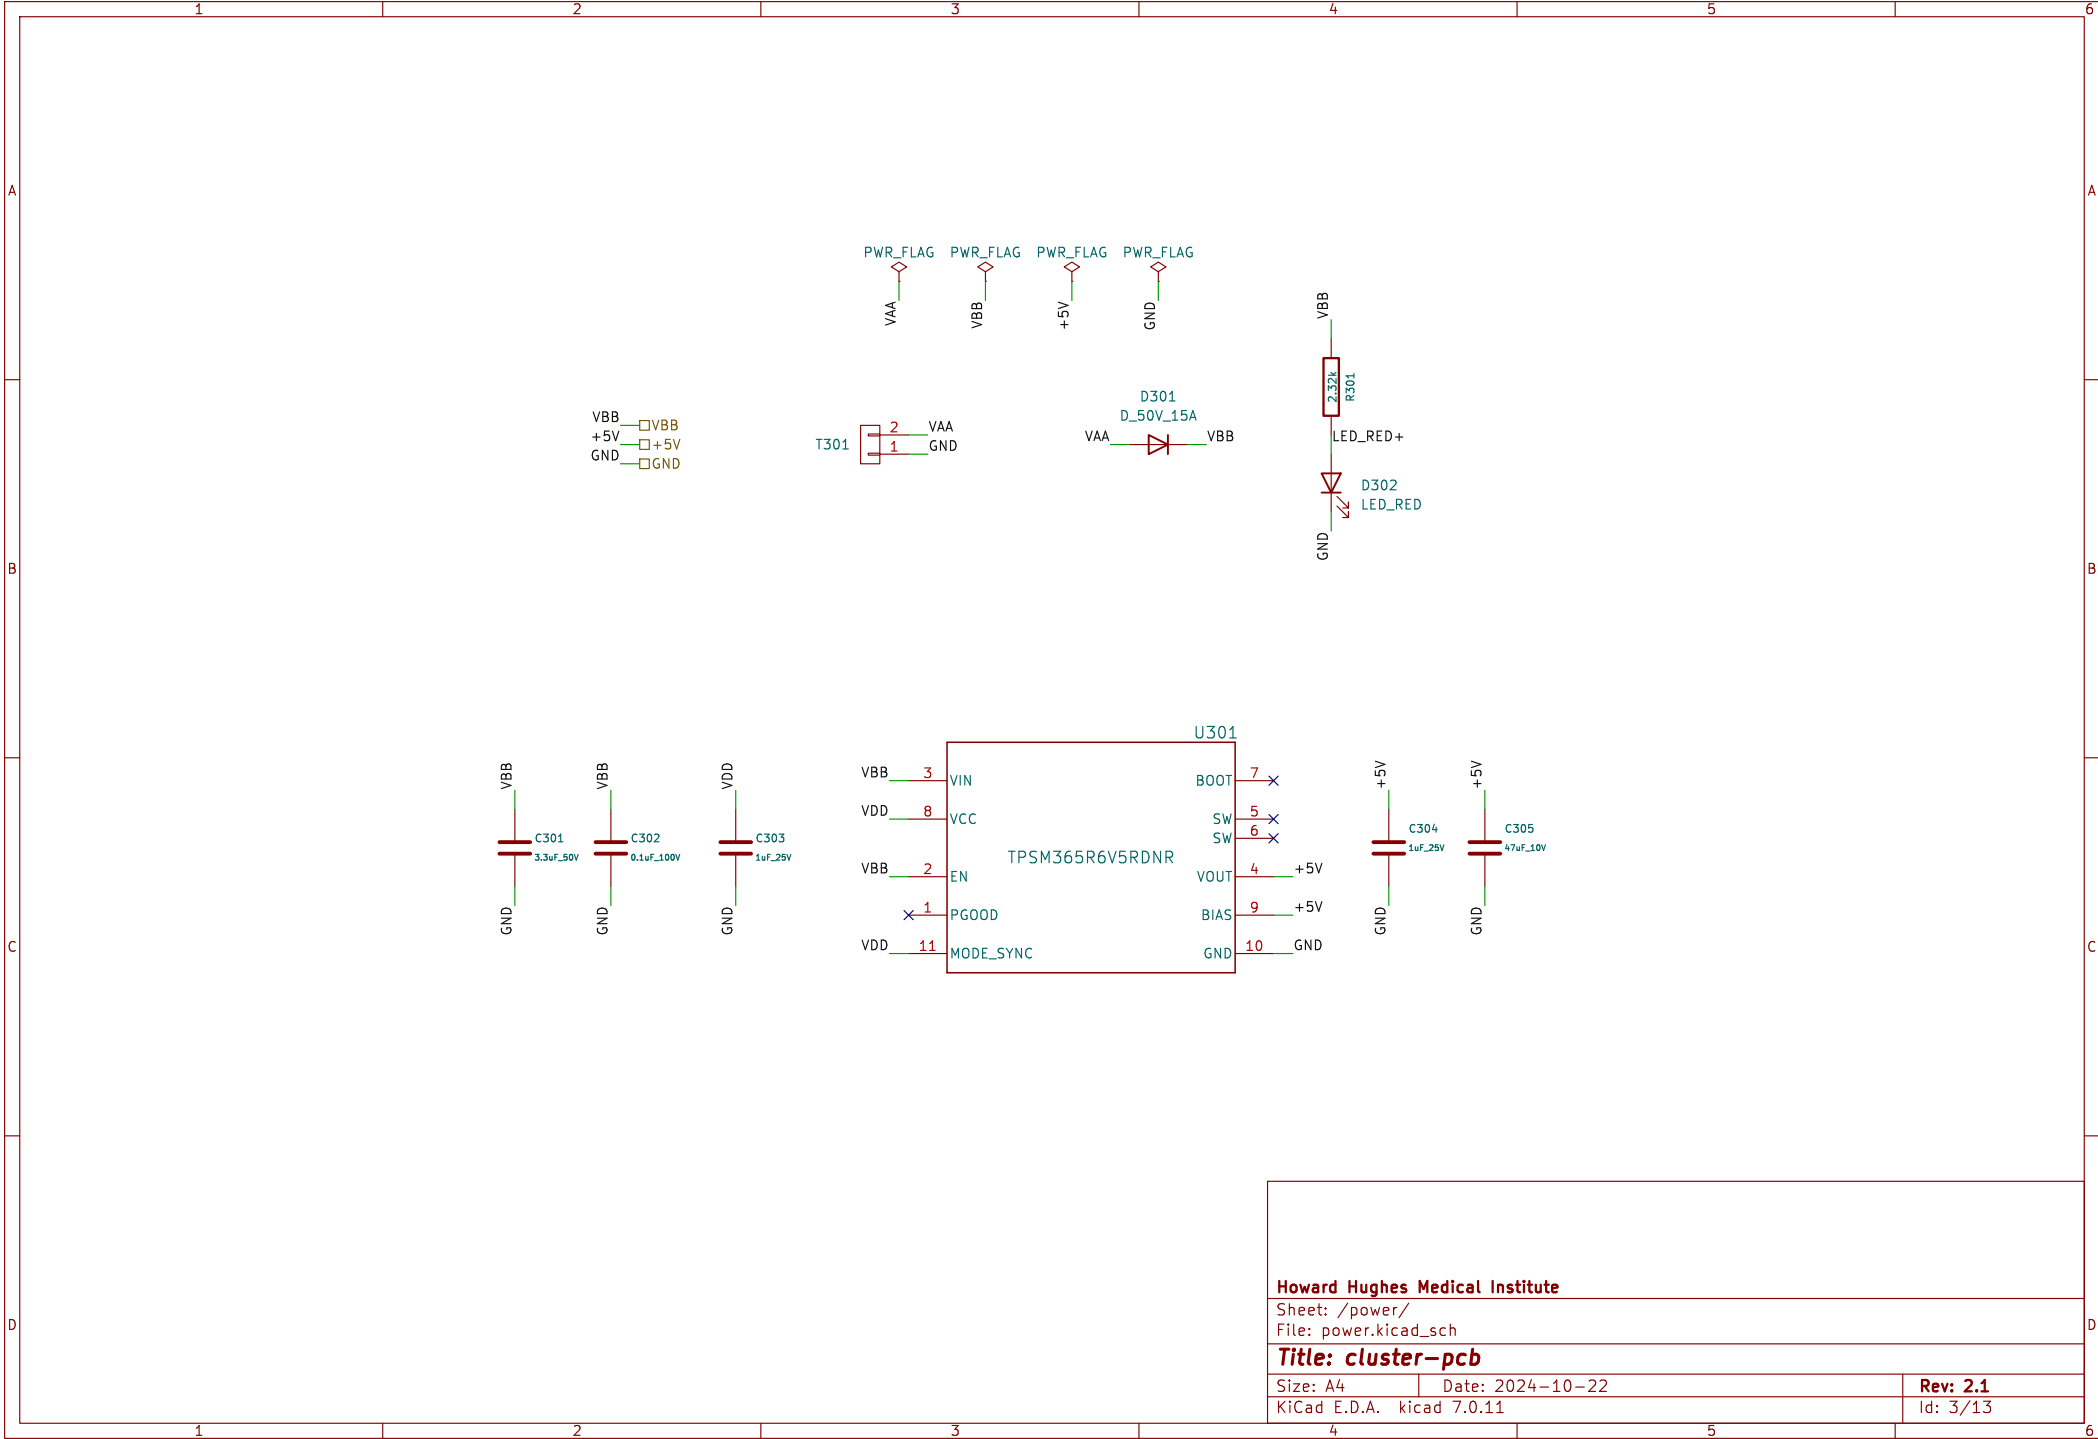

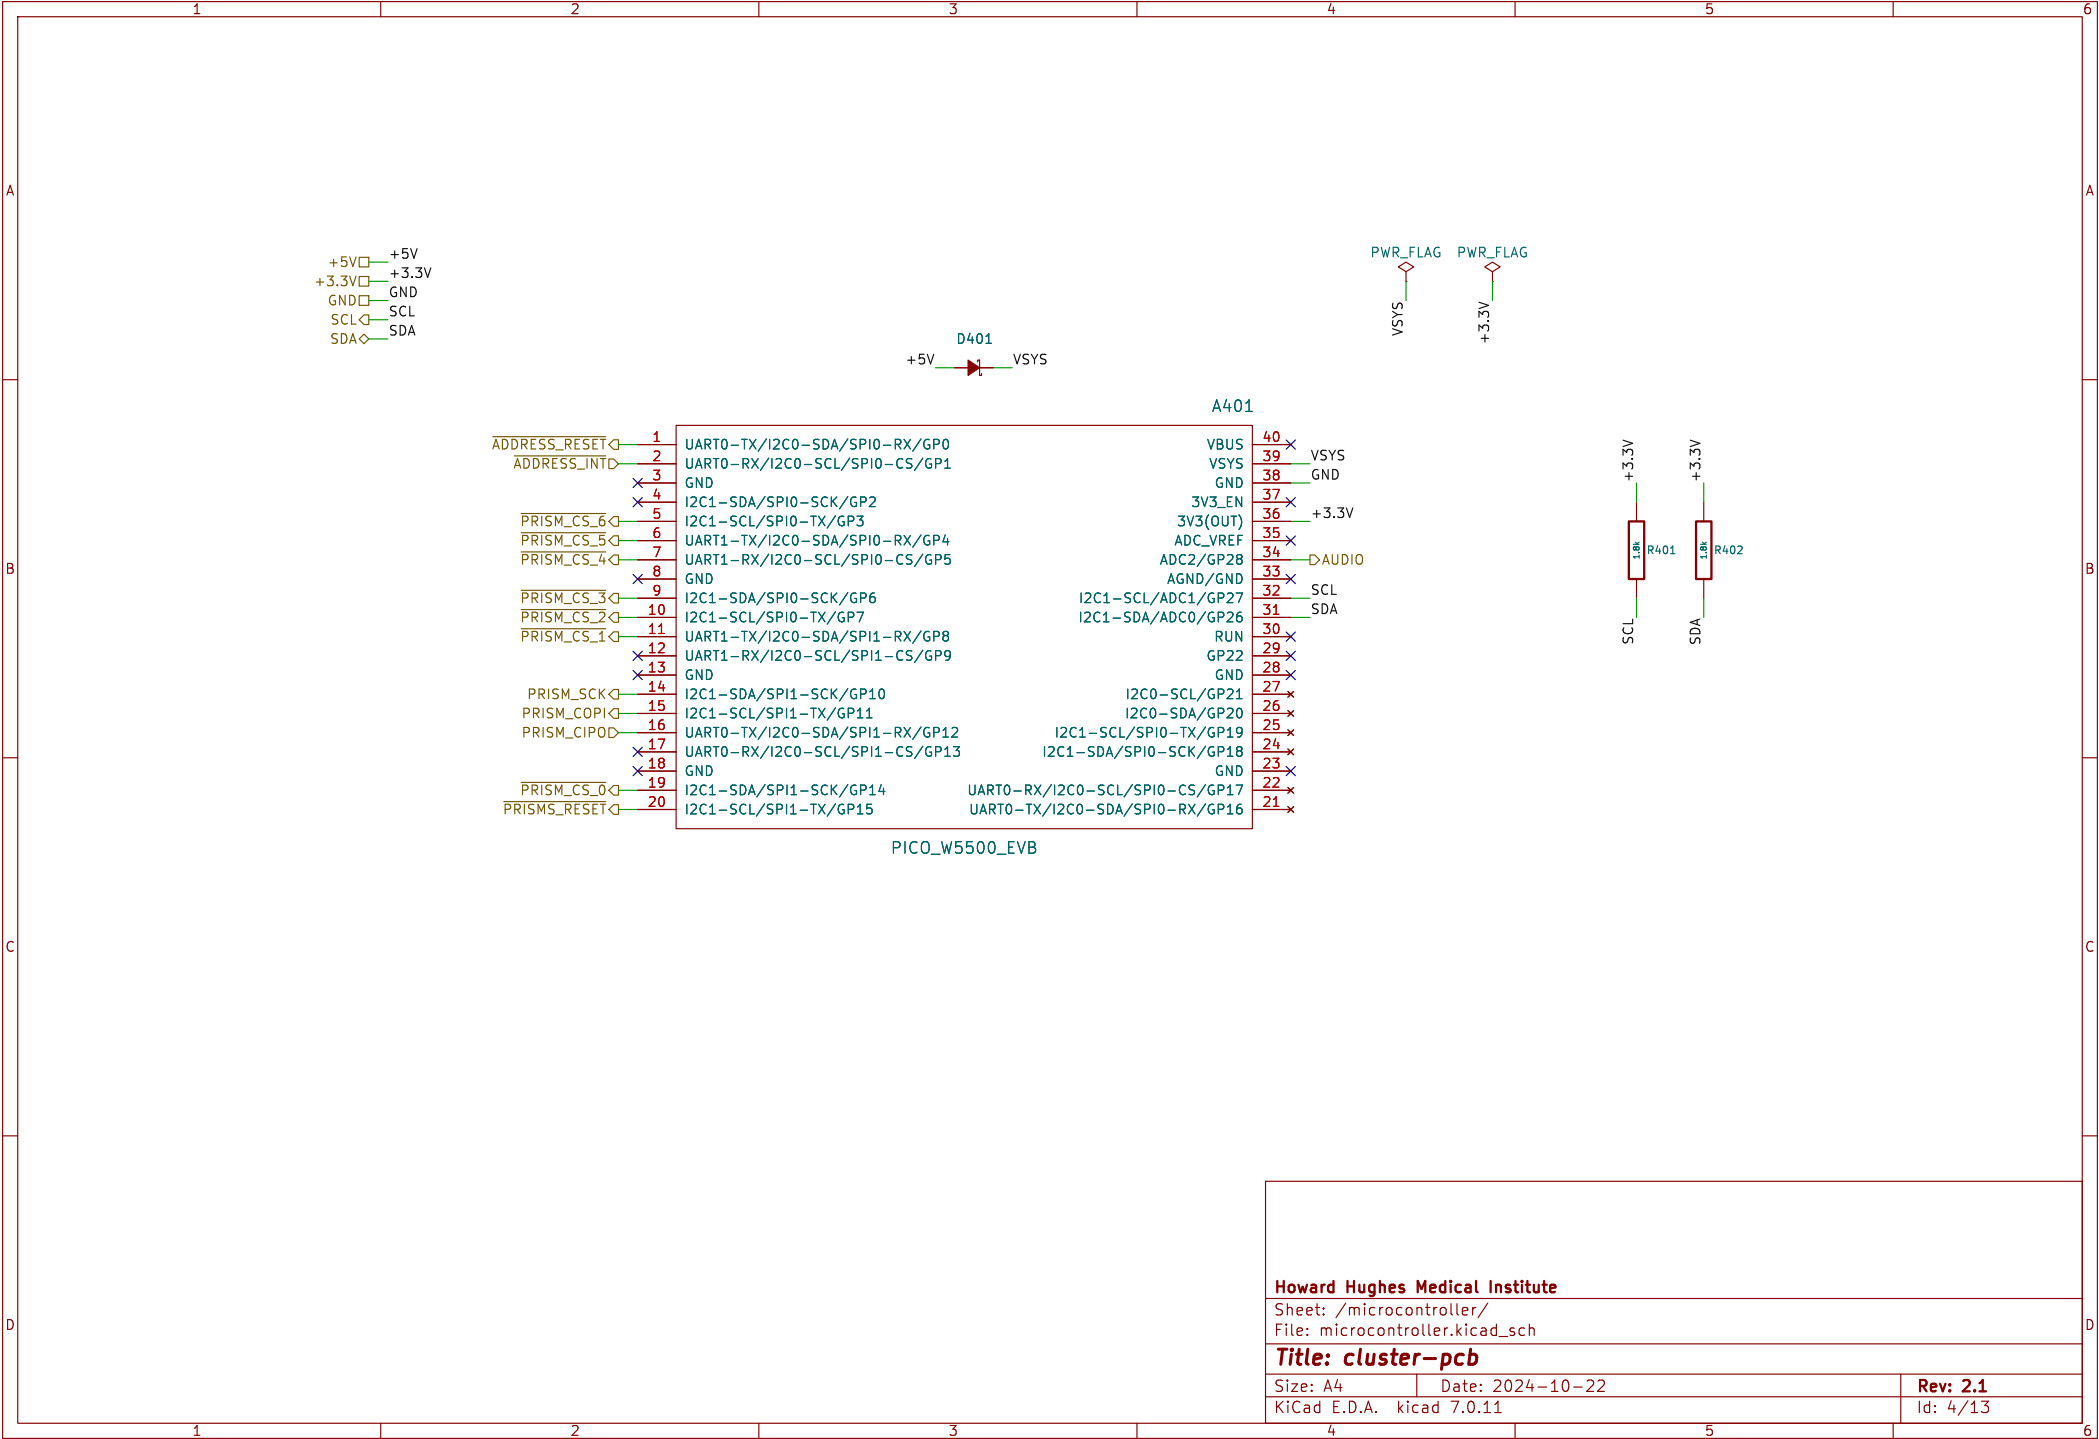

Howard Hughes Medical Institute

Sheet: /microcontroller/
File: microcontroller.kicad_sch


Title: cluster-pcb

Size: A4 Date: 2024-10-22

KiCad E.D.A. kicad 7.0.11

Rev: 2.1

Id: 4/13

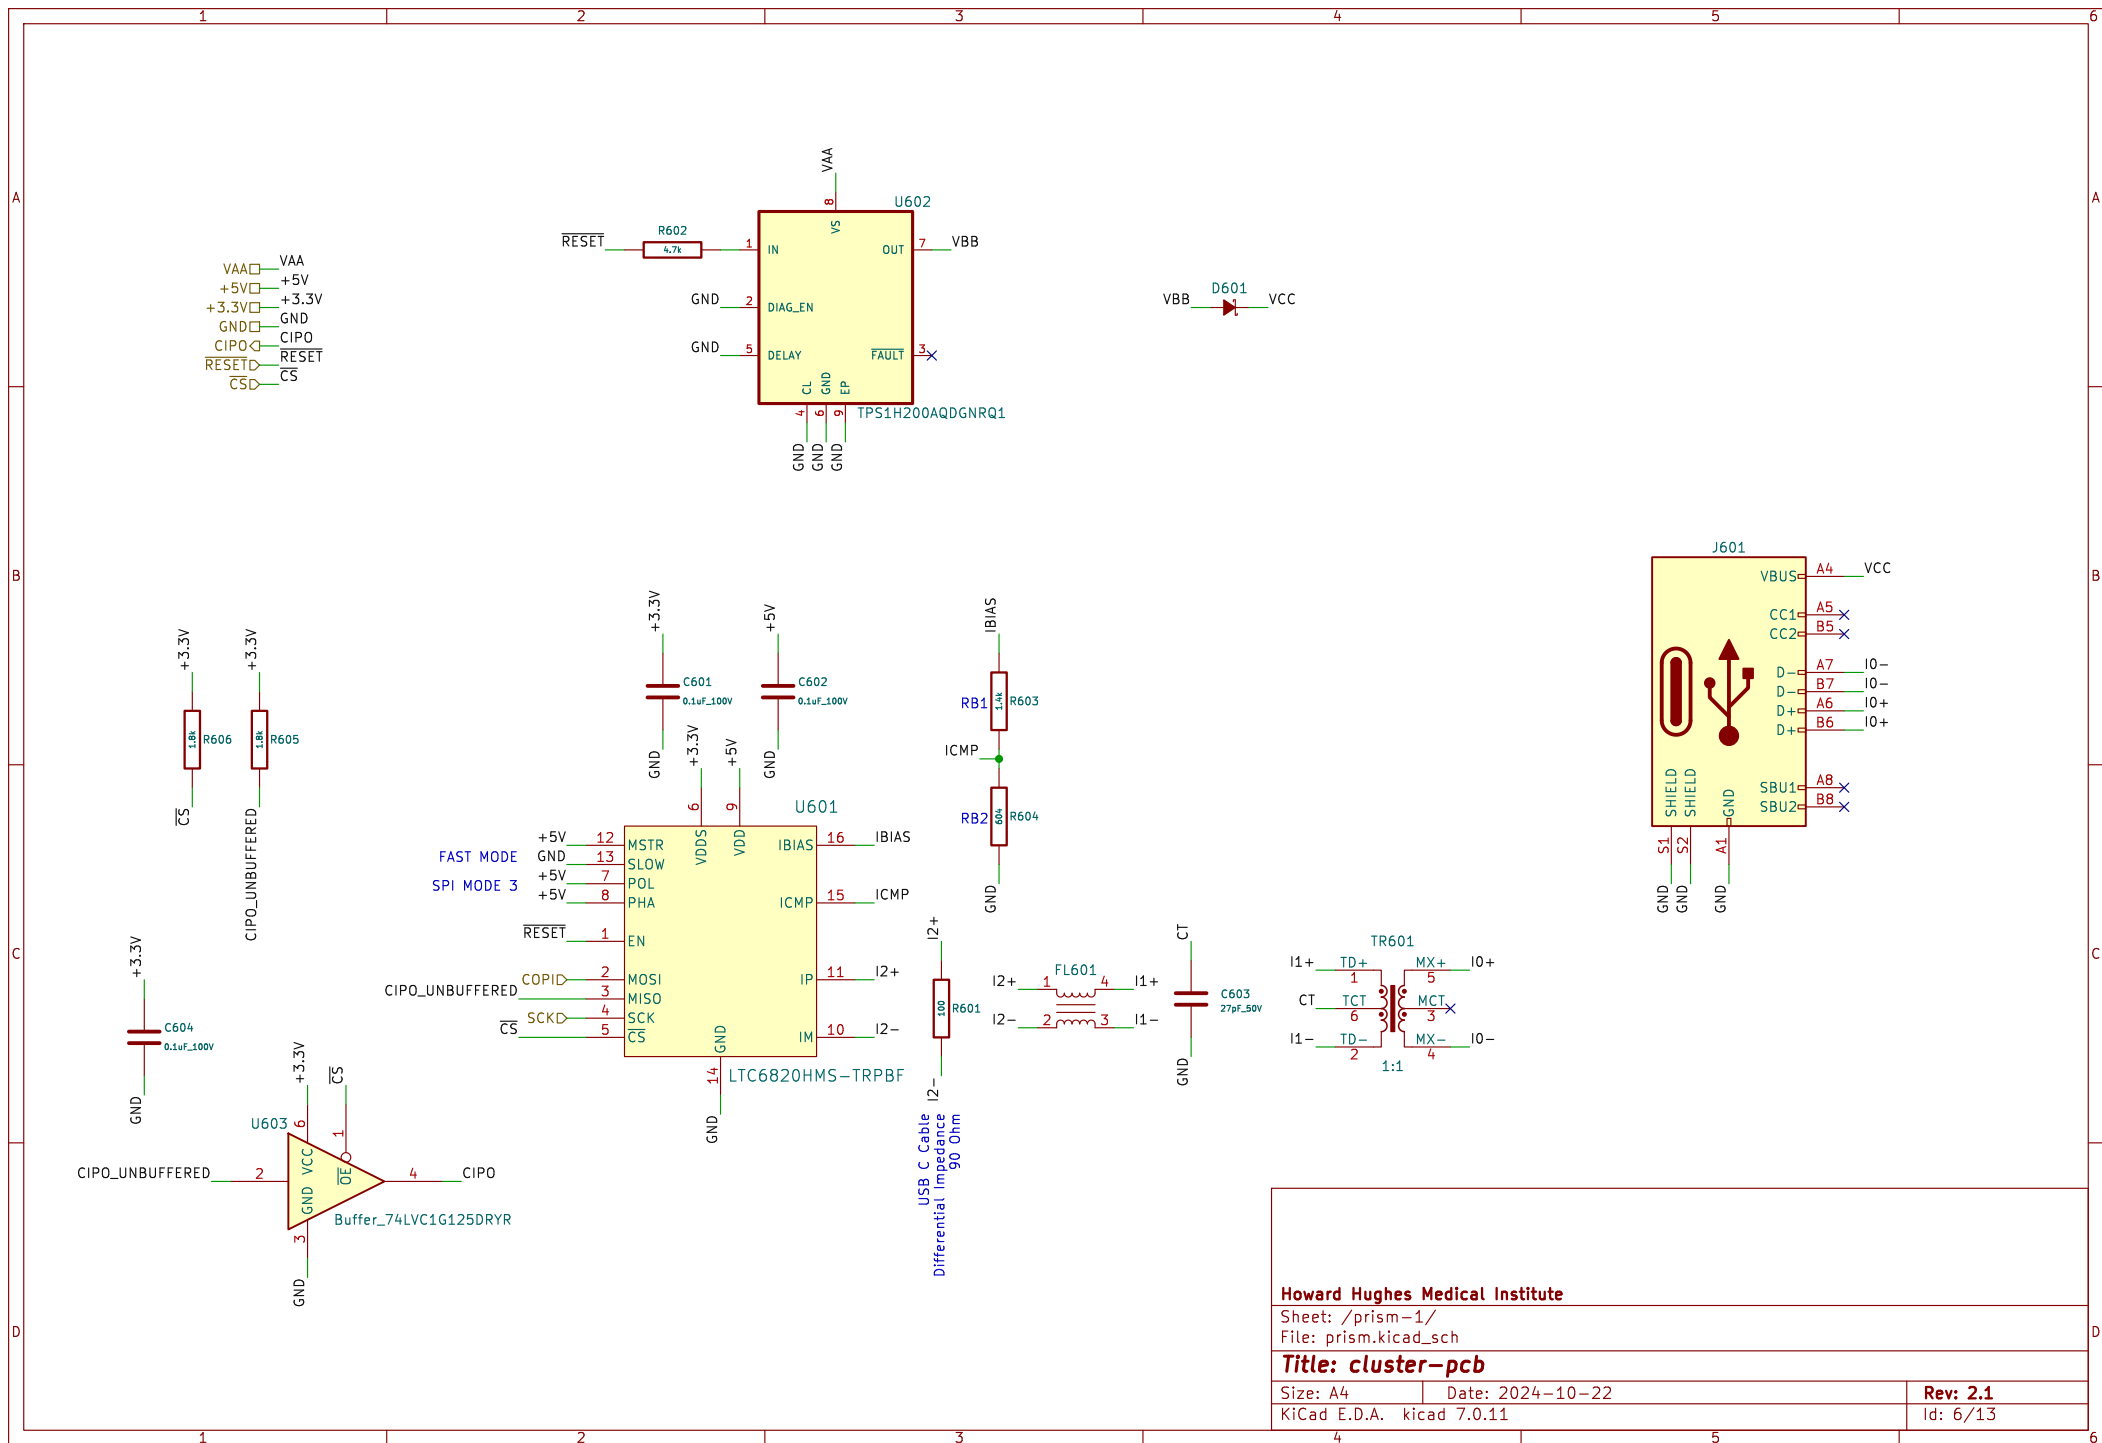

Howard Hughes Medical Institute

Sheet: /prism-1/

File: prism.kicad_sch


Title: cluster-pcb

Size: A4 Date: 2024-10-22

KiCad E.D.A. kicad 7.0.11

Rev: 2.1

Id: 6/13

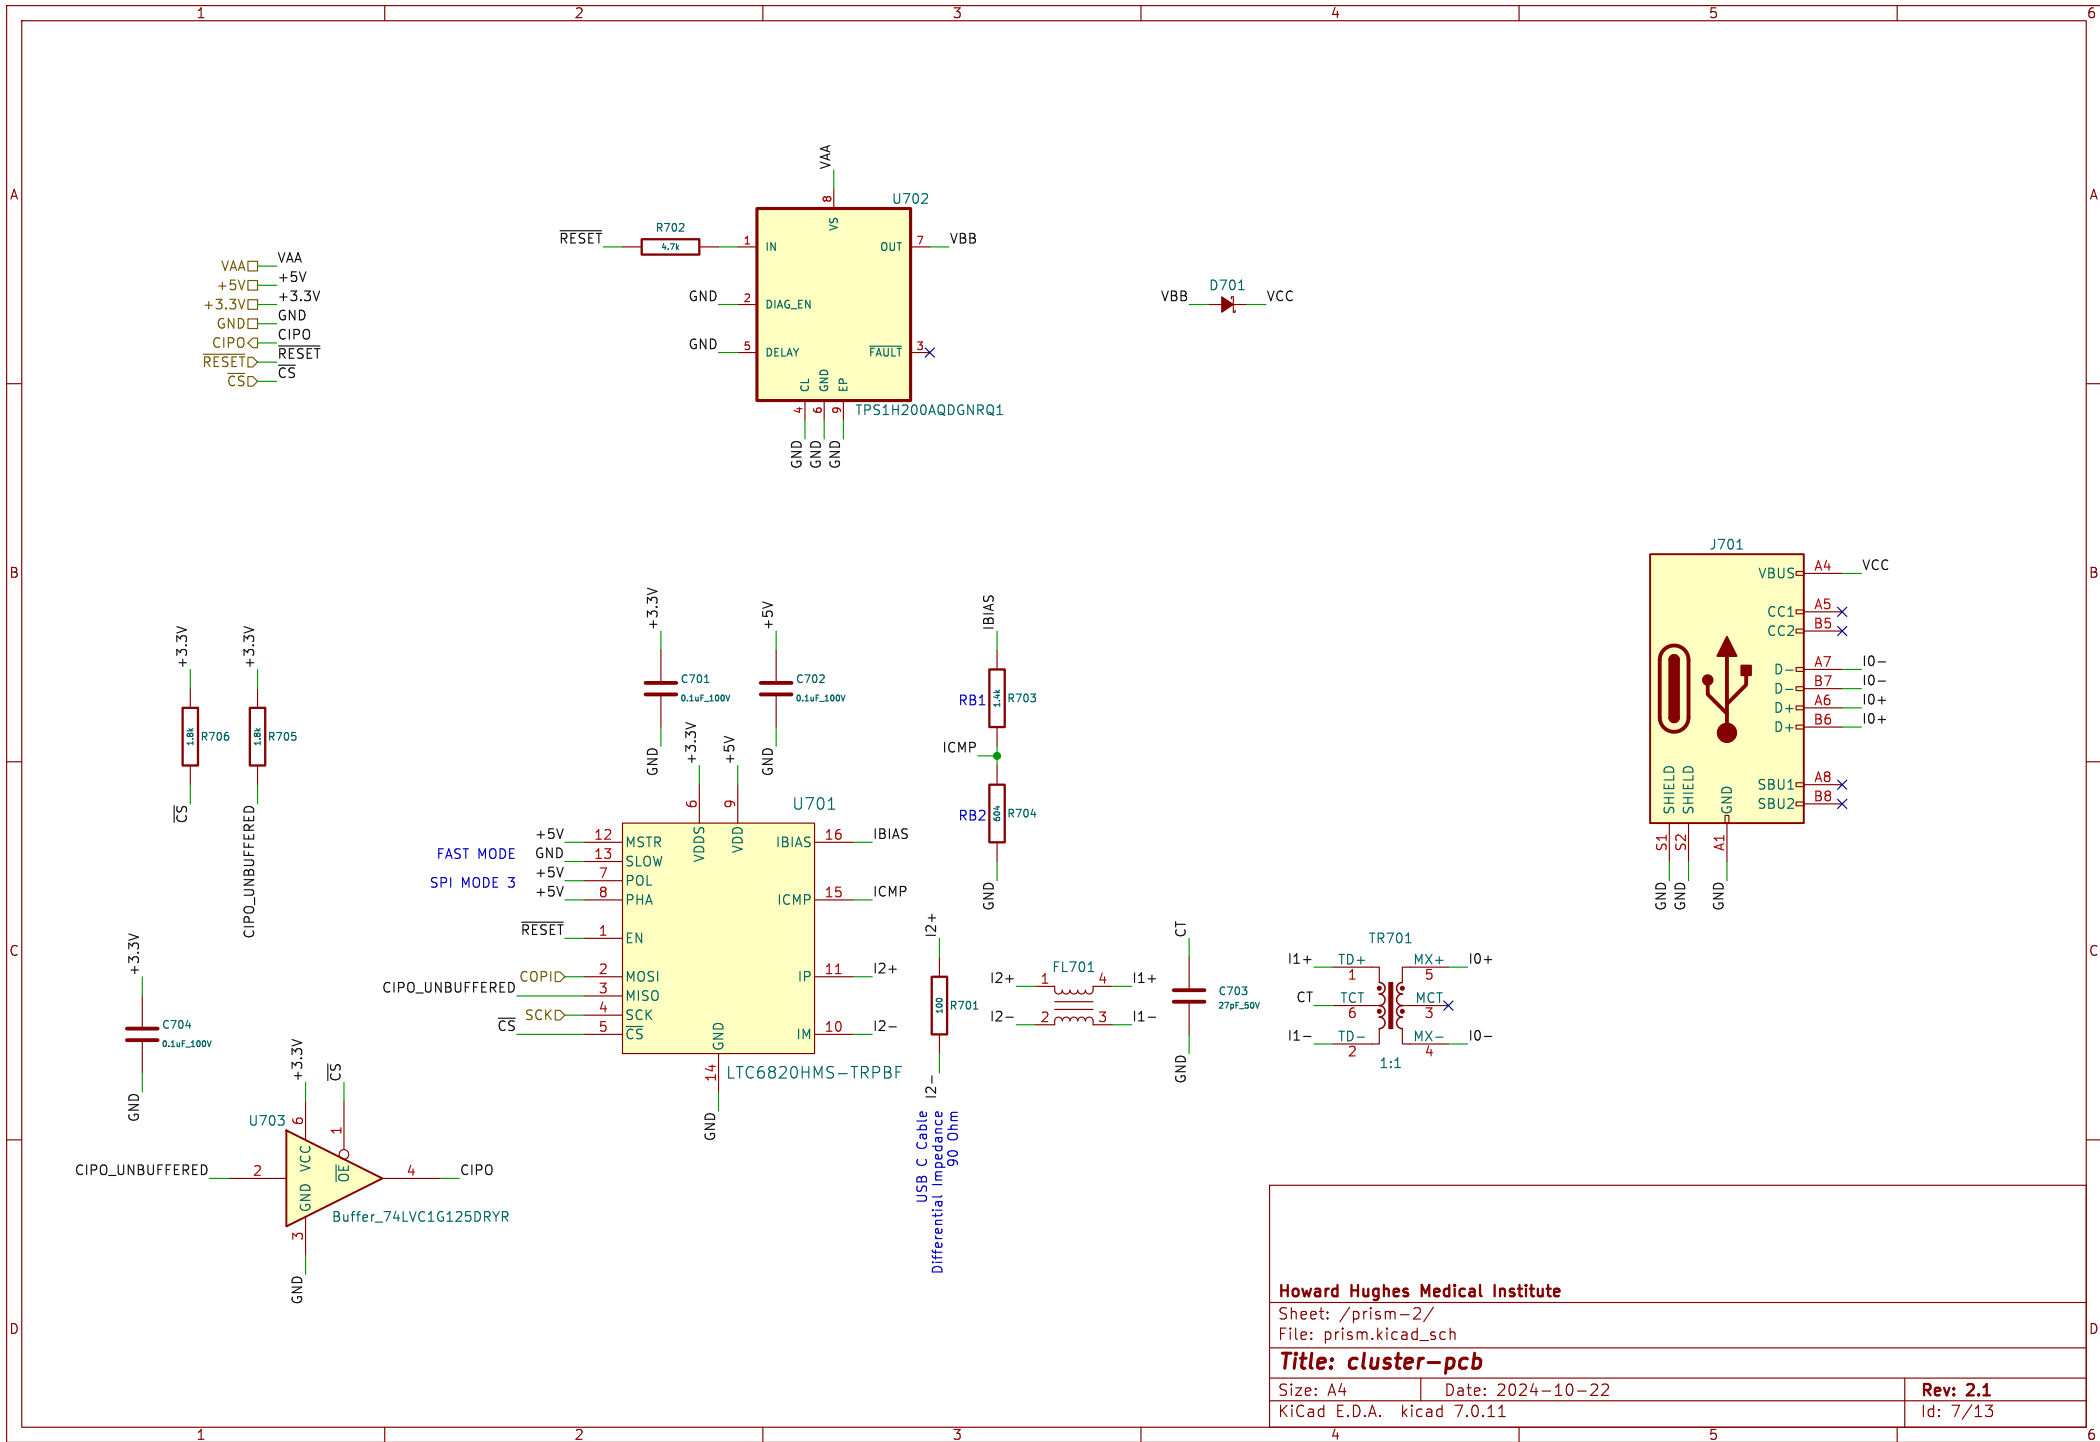

Howard Hughes Medical Institute

Sheet: /prism-2/

File: prism.kicad_sch

Title: cluster-pcb


Size: A4

Date: 2024-10-22

KiCad E.D.A. kicad 7.0.11

Rev: 2.1

Id: 7/13

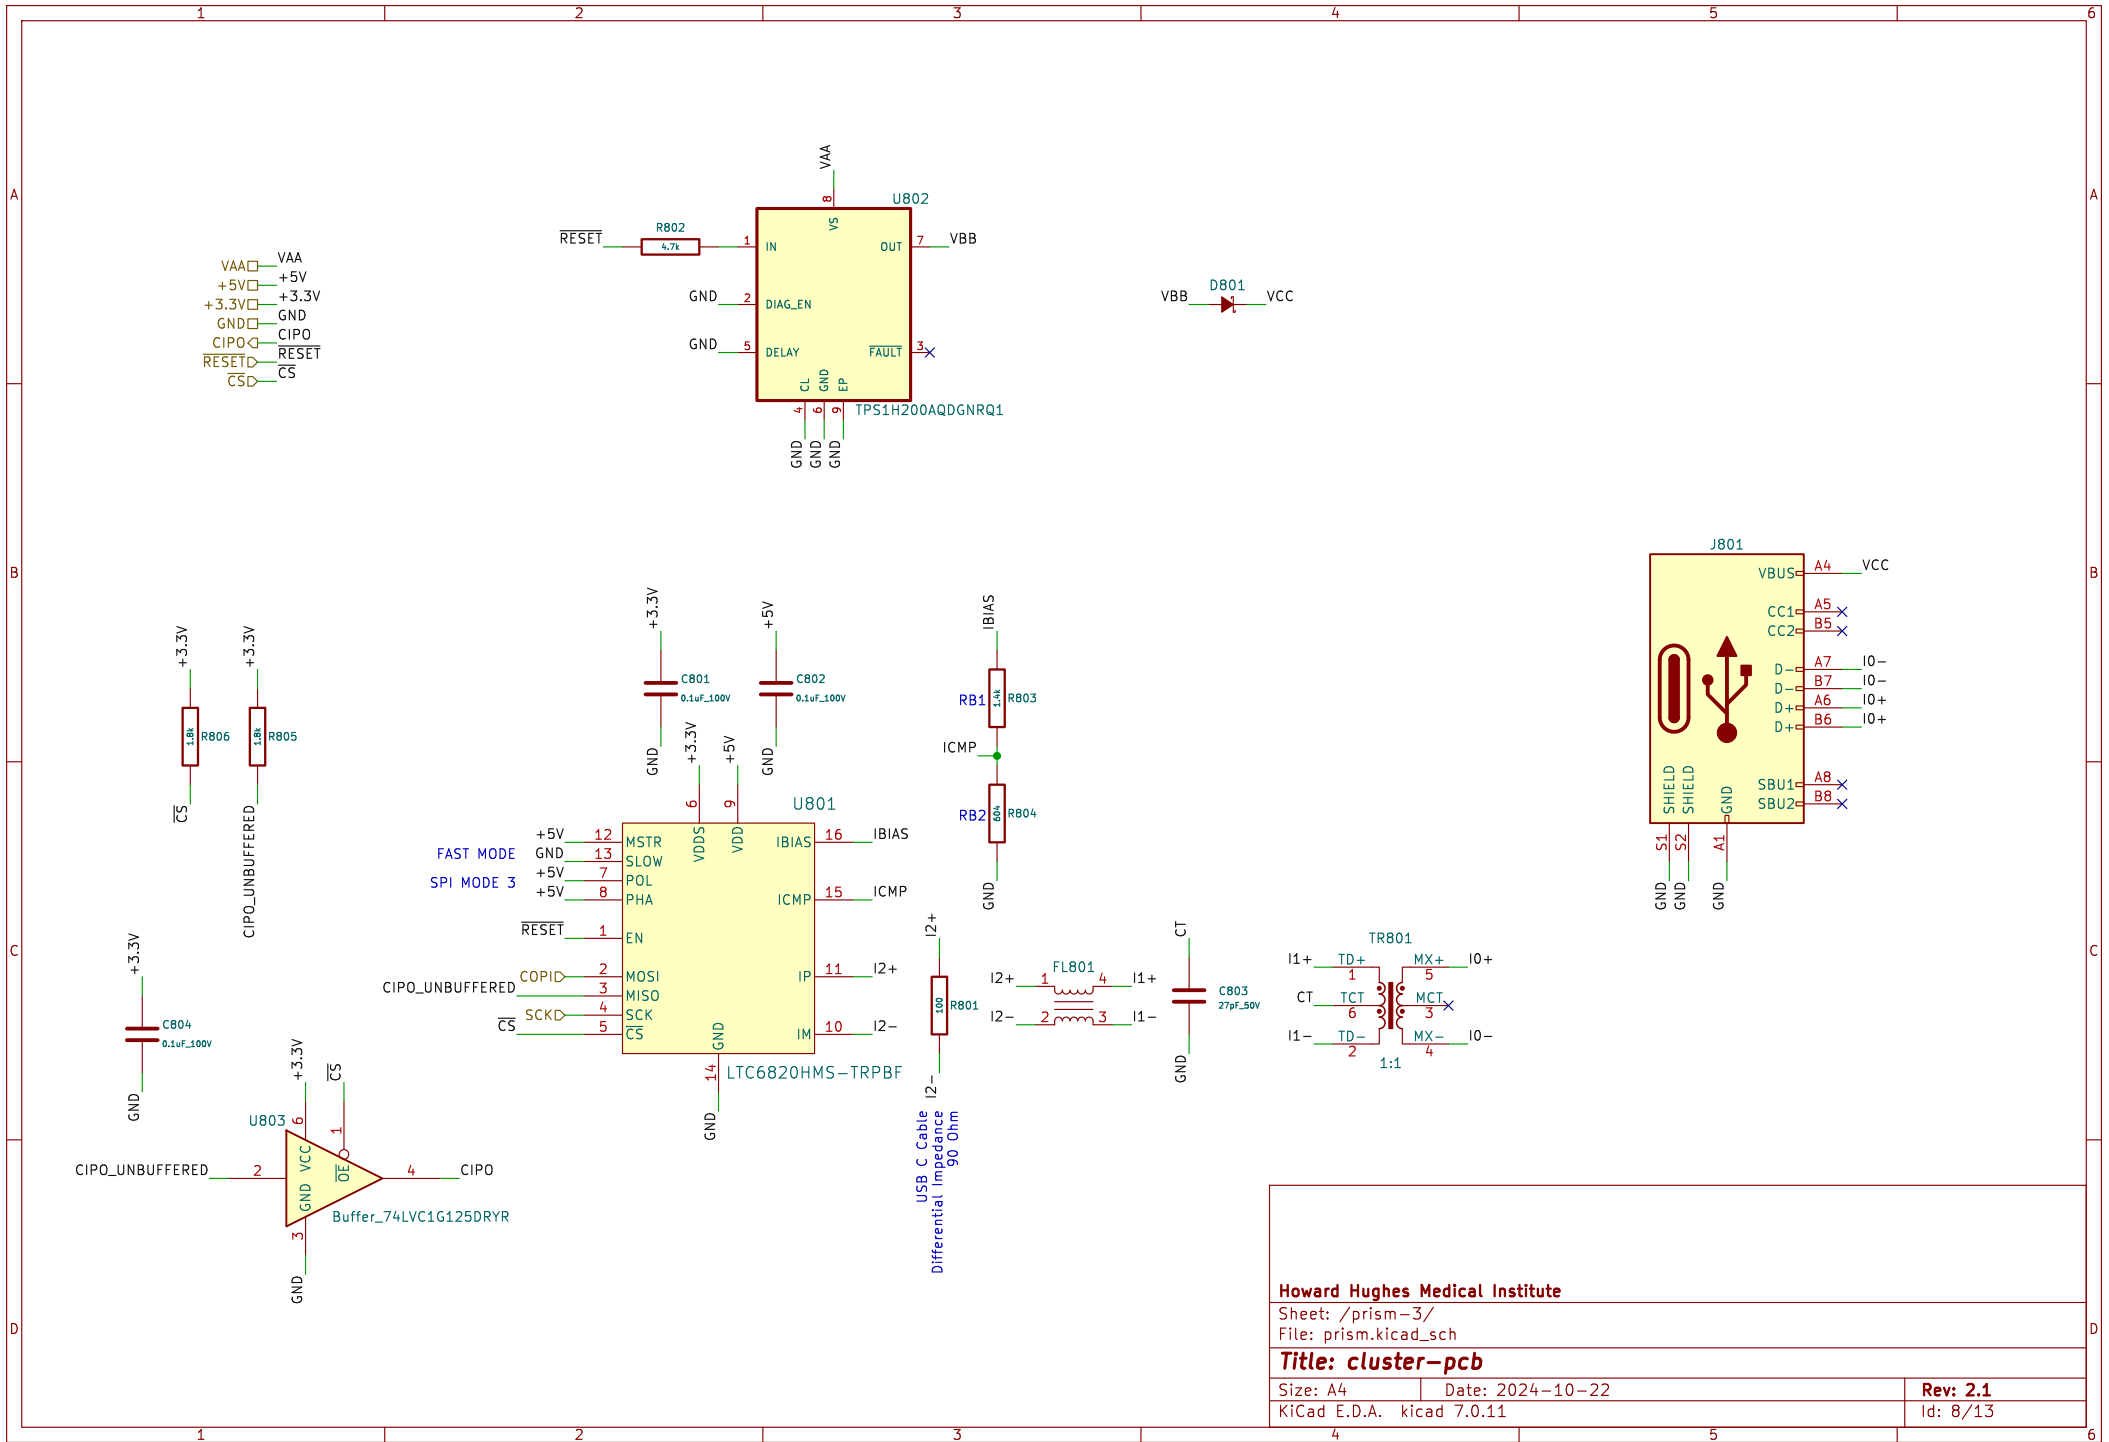

Howard Hughes Medical Institute







Sheet: /prism-3/
File: prism.kicad_sch

Title: cluster-pcb

Size: A4 Date: 2024-10-22
KiCad E.D.A. kicad 7.0.11

Rev: 2.1
Id: 8/13

VAA □ VAA
+5V □ +5V
+3.3V □ +3.3V
GND □ GND
CIPO □ CIPO
RESET □ RESET
CS □ CS

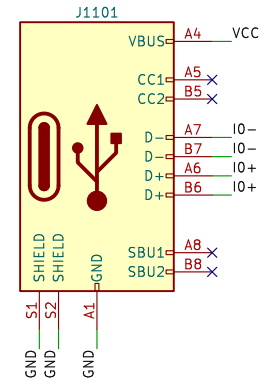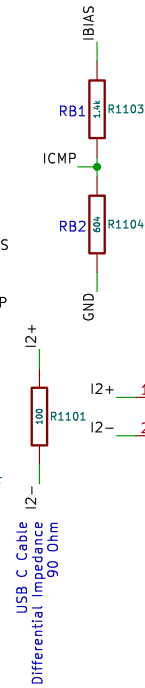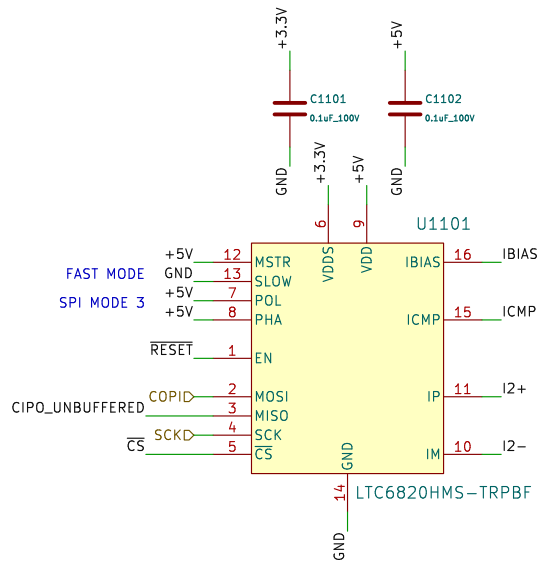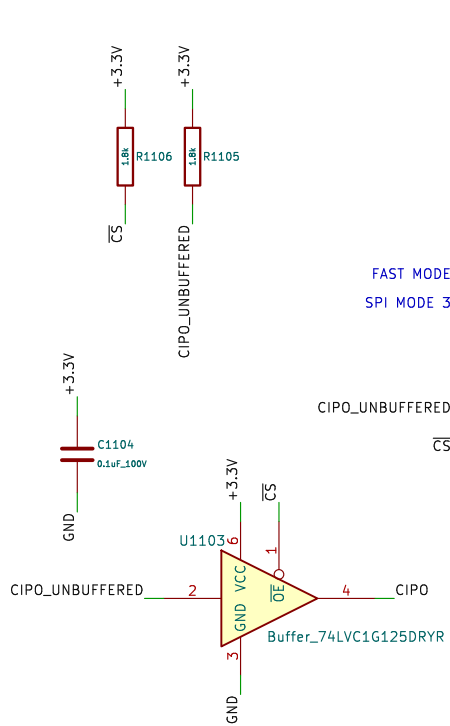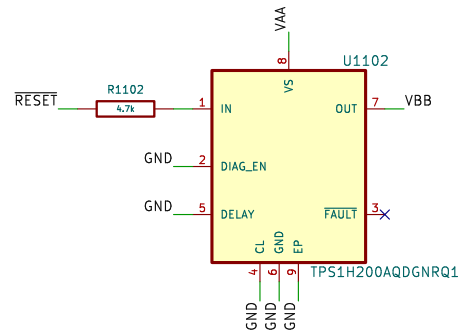

Howard Hughes Medical Institute

Sheet: /prism-6/
File: prism.kicad_sch


Title: cluster-pcb

Size: A4 Date: 2024-10-22

KiCad E.D.A. kicad 7.0.11

Rev: 2.1

Id: 11/13

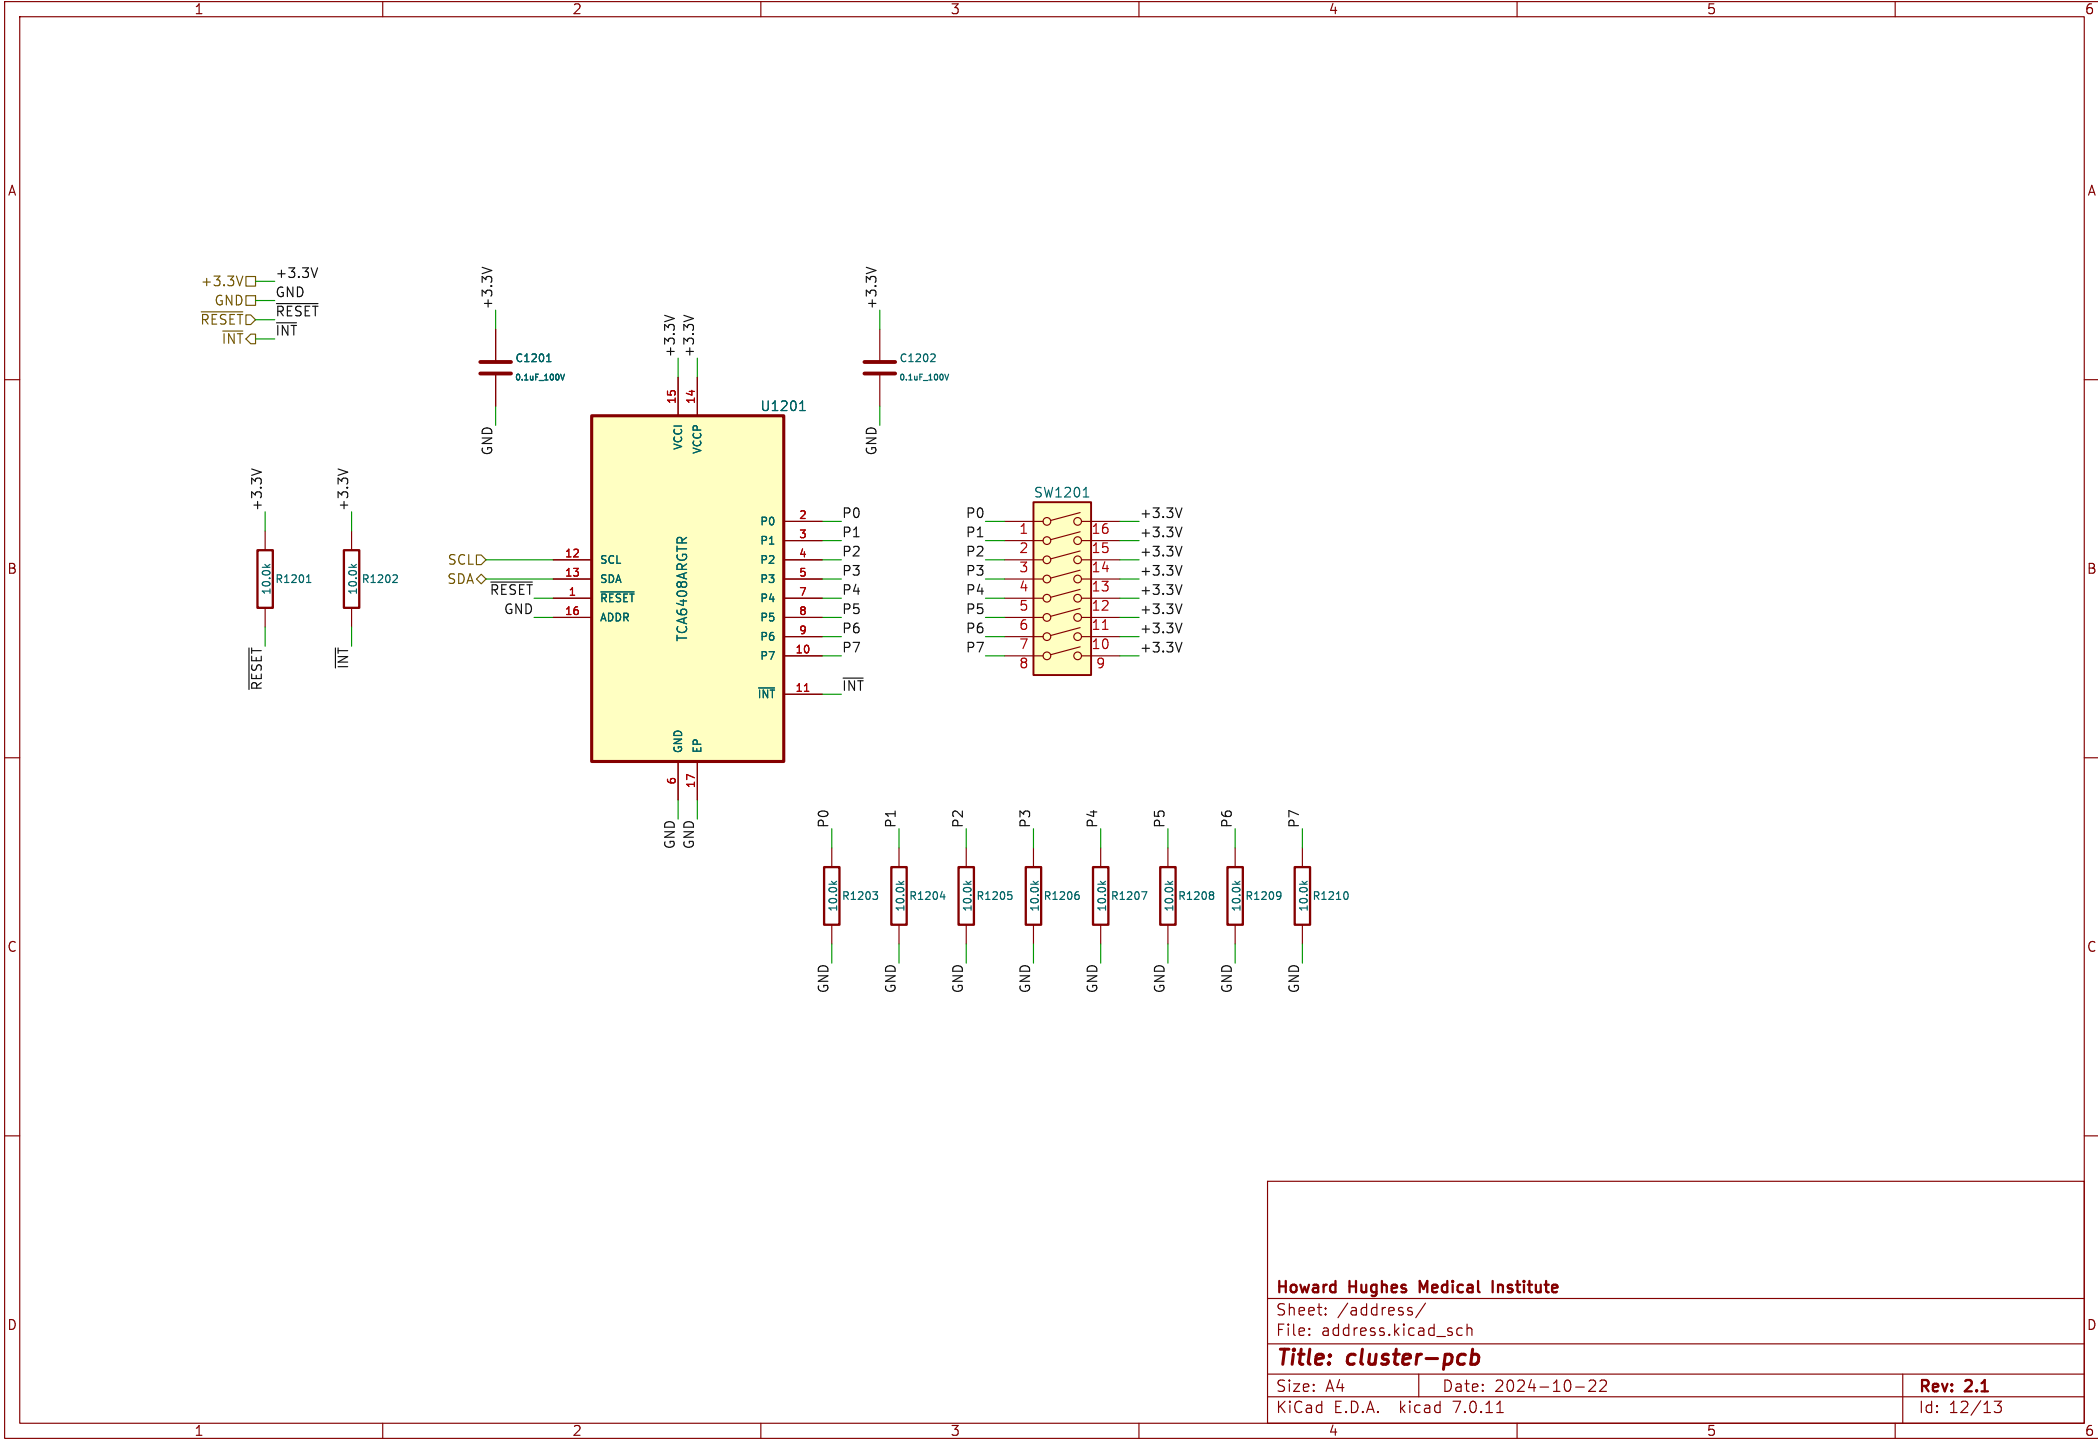

Howard Hughes Medical Institute

Sheet: /address/
File: address.kicad_sch


Title: cluster-pcb

Size: A4 Date: 2024-10-22

KiCad E.D.A. kicad 7.0.11

Rev: 2.1

Id: 12/13

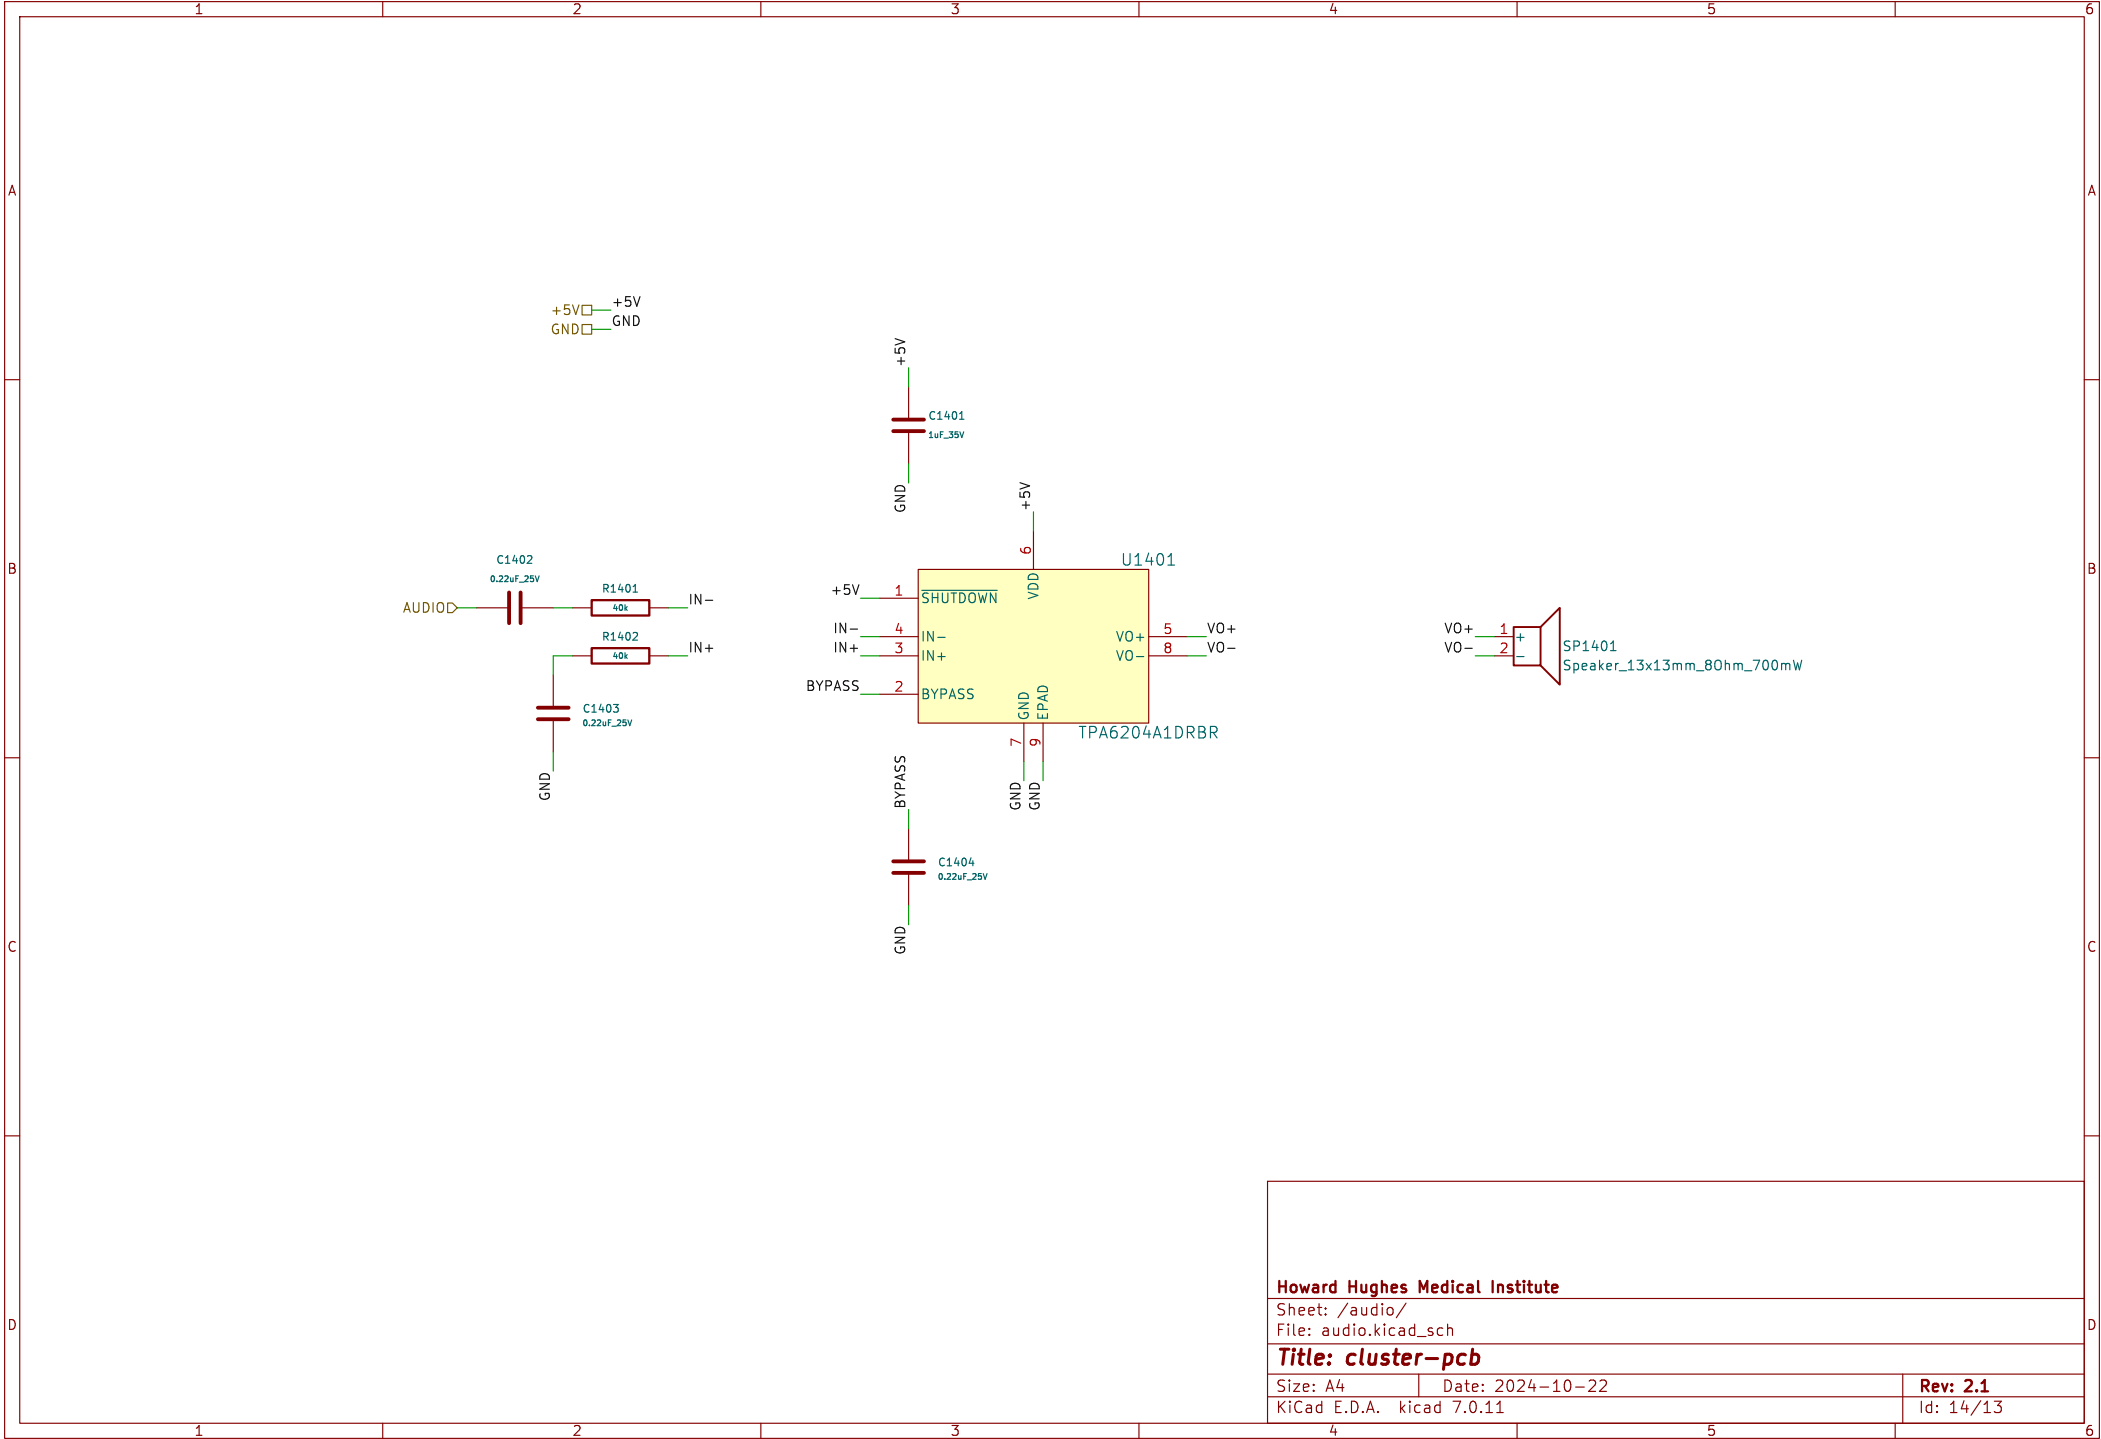

Howard Hughes Medical Institute

Sheet: /audio/
File: audio.kicad_sch

Title: cluster-pcb

Size: A4 Date: 2024-10-22

KiCad E.D.A. kicad 7.0.11

Rev: 2.1

Id: 14/13