

14-Day Glucose Report

Andrew · Type 1 · Dexcom G7 + Loop (closed-loop) · Jul 4 - Jul 18, 2026 · 14 days · 99% sensor active

Observational summary generated from Nightscout CGM data. **Not medical advice** — for discussion with the care team.

TIME IN RANGE

93.1%

● Goal >70%

MEAN GLUCOSE

110 mg/dL

—

GMI · EST. A1C

5.9%

● Goal <7%

VARIABILITY · CV



27%

● Goal ≤36%

TIME BELOW 54

0.8%

● Goal <1%

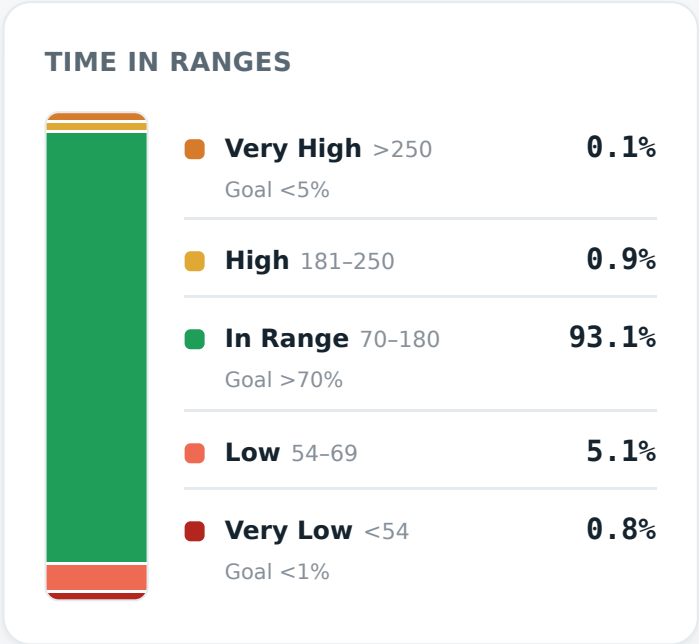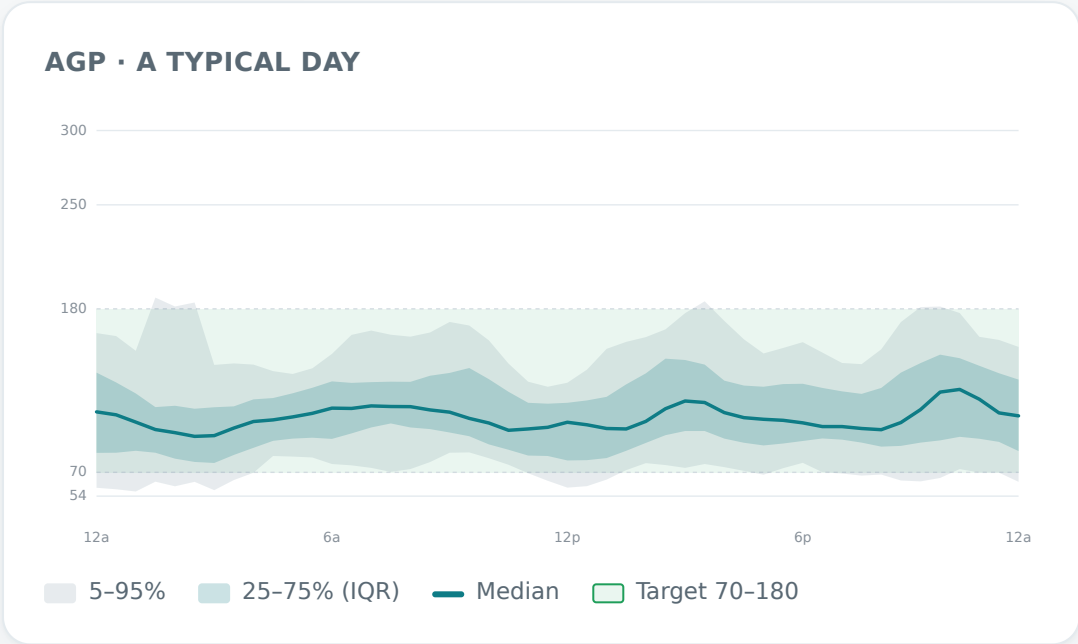

Excellent control. Every standard target is met — time-in-range 93.1% (goal >70%), GMI 5.9%, and time above 180 under 1%. The below-range readings are dominated by G7 nighttime compression lows (sensor pressure, self-recovering); excluding those, true time-in-range is ~95%.

Metrics. 4,002 readings over 14 days, 99% sensor-active. GMI (Glucose Management Indicator) estimates lab A1c from mean glucose. CV = coefficient of variation (glucose stability). Ranges follow the international consensus (Battelino 2019). Times are local (UTC−7). Overnight lows are largely sensor compression artifact, not hypoglycemia — see the report notes.