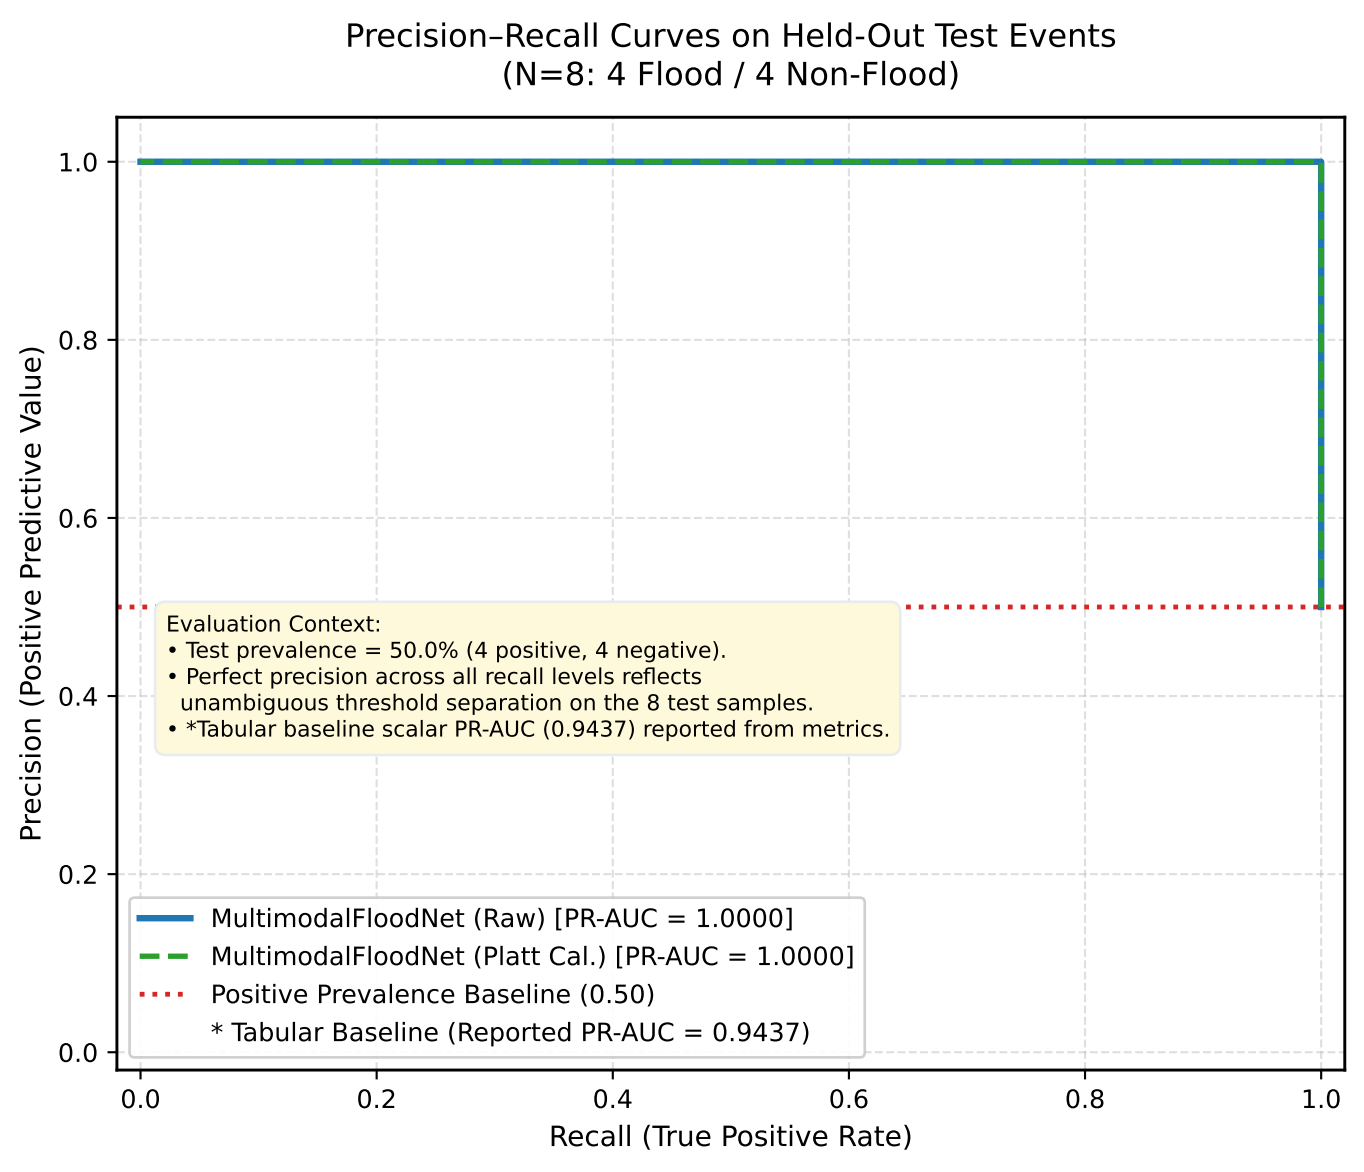
Precision–Recall Curves on Held-Out Test Events
(N=8: 4 Flood / 4 Non-Flood)
Precision (Positive Predictive Value)
Recall (True Positive Rate)
1.0
0.8
0.6
0.4
0.2
0.0
0.0
0.2
0.4
0.6
0.8
1.0
Evaluation Context:
• Test prevalence = 50.0% (4 positive, 4 negative).
• Perfect precision across all recall levels reflects
unambiguous threshold separation on the 8 test samples.
• *Tabular baseline scalar PR-AUC (0.9437) reported from metrics.
MultimodalFloodNet (Raw) [PR-AUC = 1.0000]
MultimodalFloodNet (Platt Cal.) [PR-AUC = 1.0000]
Positive Prevalence Baseline (0.50)
* Tabular Baseline (Reported PR-AUC = 0.9437)