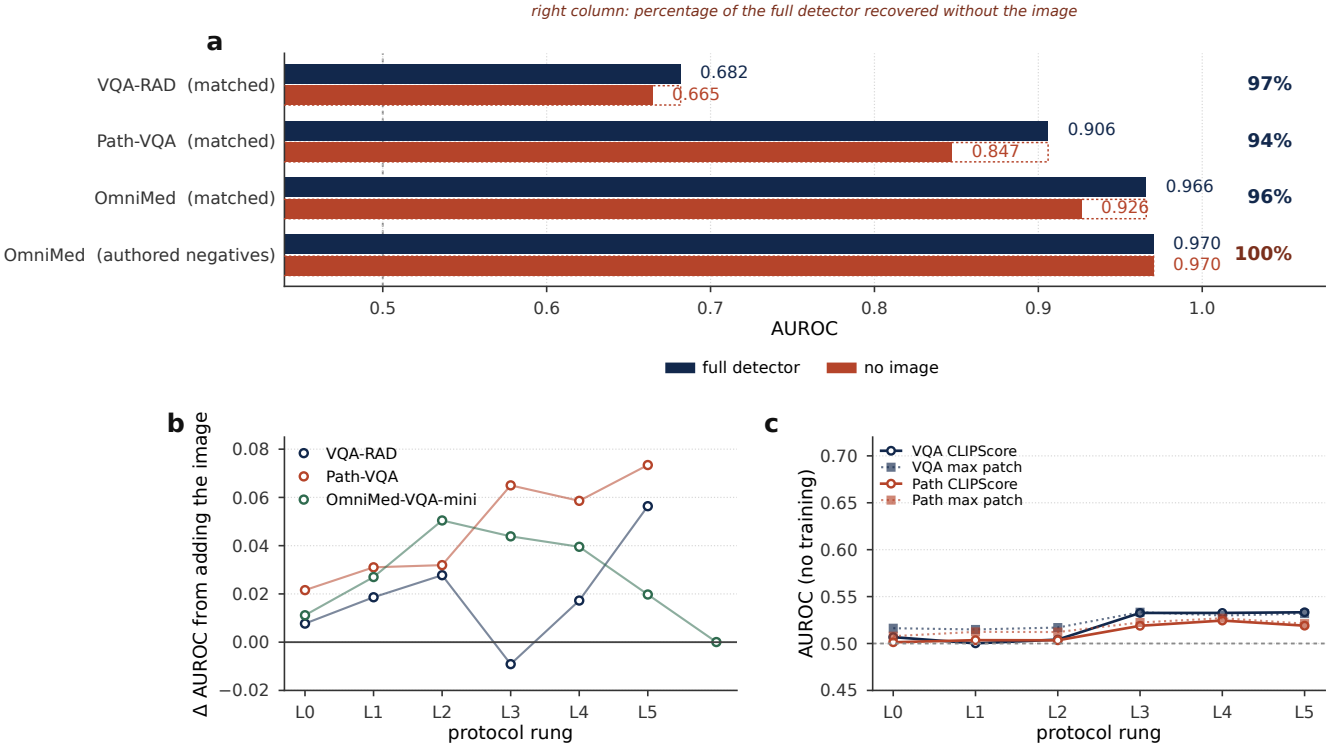
right column: percentage of the full detector recovered without the image
a
VQA-RAD (matched)
Path-VQA (matched)
OmniMed (matched)
OmniMed (authored negatives)
0.682
0.665
97%
0.906
0.847
94%
0.966
0.926
96%
0.970
0.970
100%
0.5
0.6
0.7
0.8
0.9
1.0
AUROC
full detector
no image
b
Δ AUROC from adding the image
0.08
0.06
0.04
0.02
0.00
−0.02
VQA-RAD
Path-VQA
OmniMed-VQA-mini
L0
L1
L2
L3
L4
L5
protocol rung
c
AUROC (no training)
0.70
0.65
0.60
0.55
0.50
0.45
VQA CLIPScore
VQA max patch
Path CLIPScore
Path max patch
L0
L1
L2
L3
L4
L5
protocol rung