


Supplementary Fig. S1. Coverage and variance calibration across the 180-cell simulation grid (regime-map DGP; shared-instrument channel, $\rho_{MY} = 0$)

A Coverage: strength-dependent regime



B Variance calibration

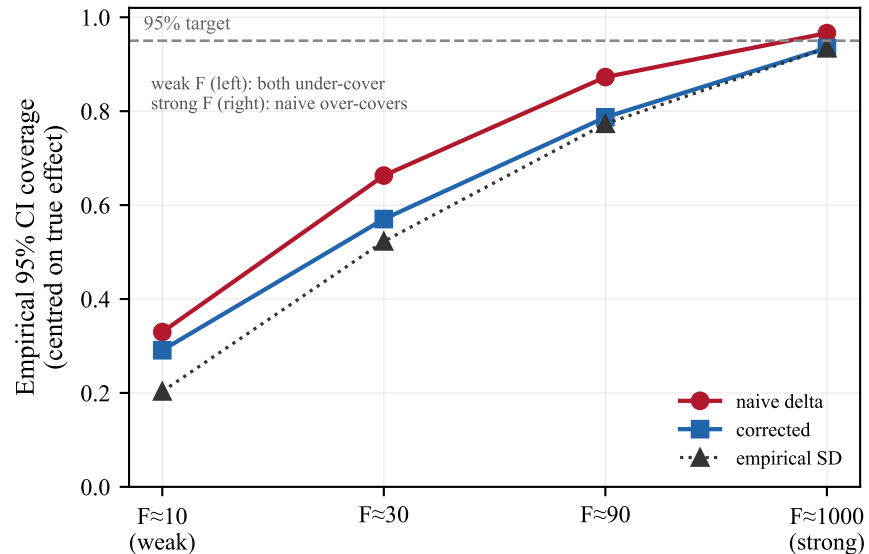