

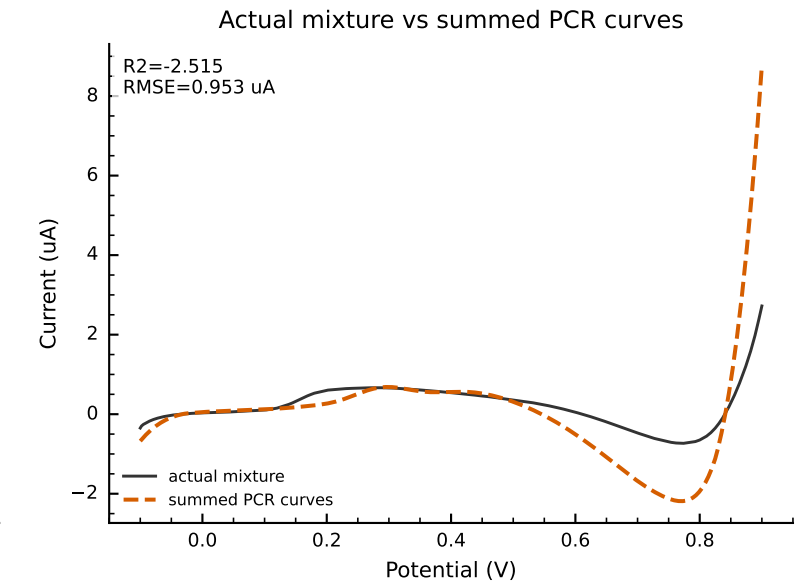
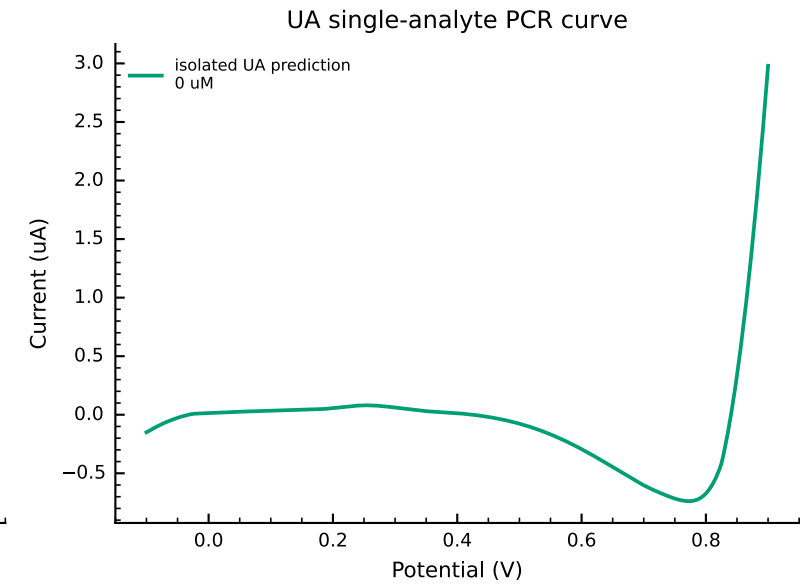
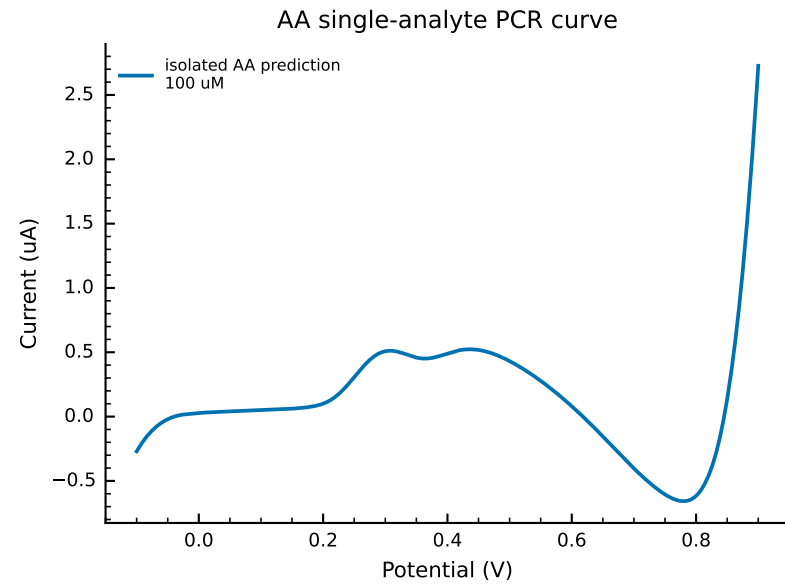
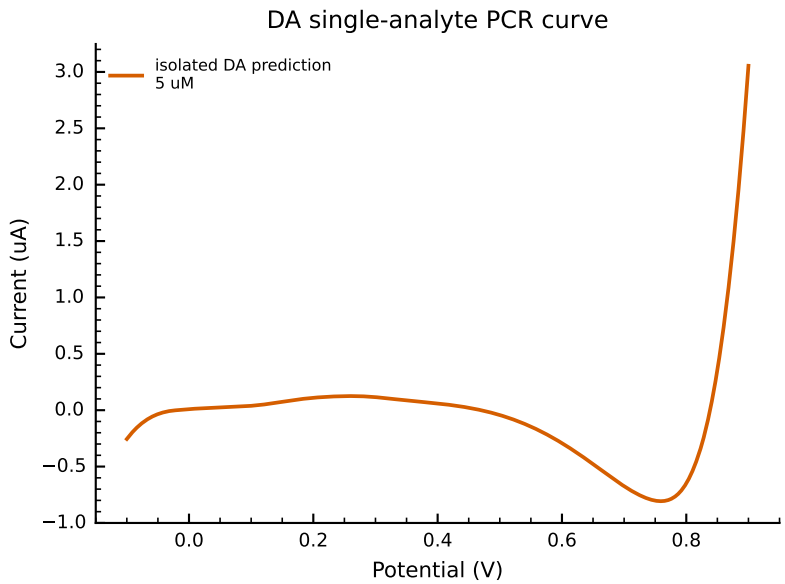
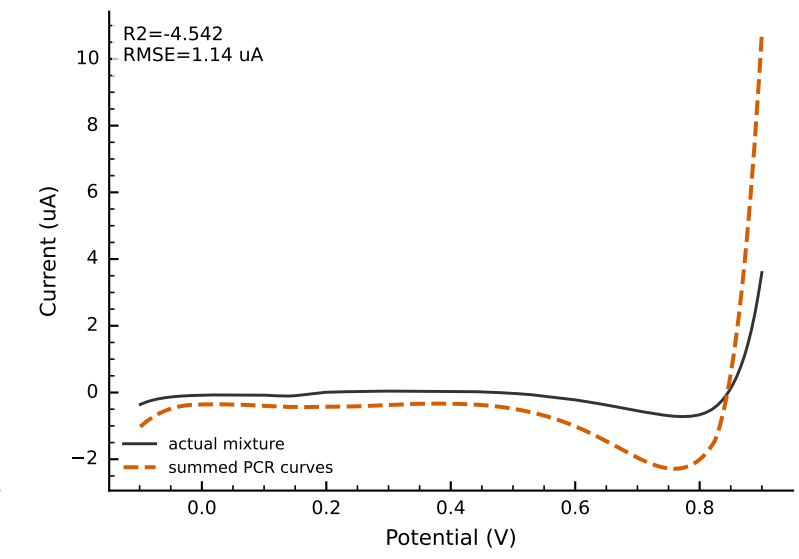
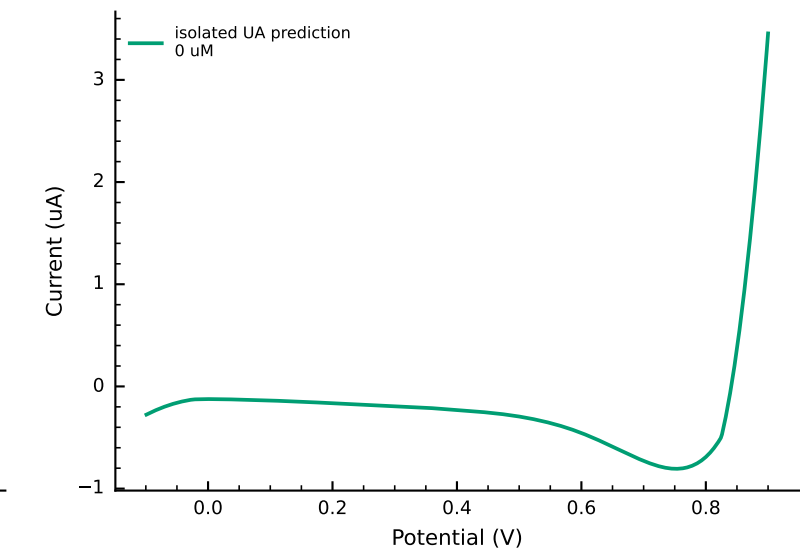






CV normal
Anodic

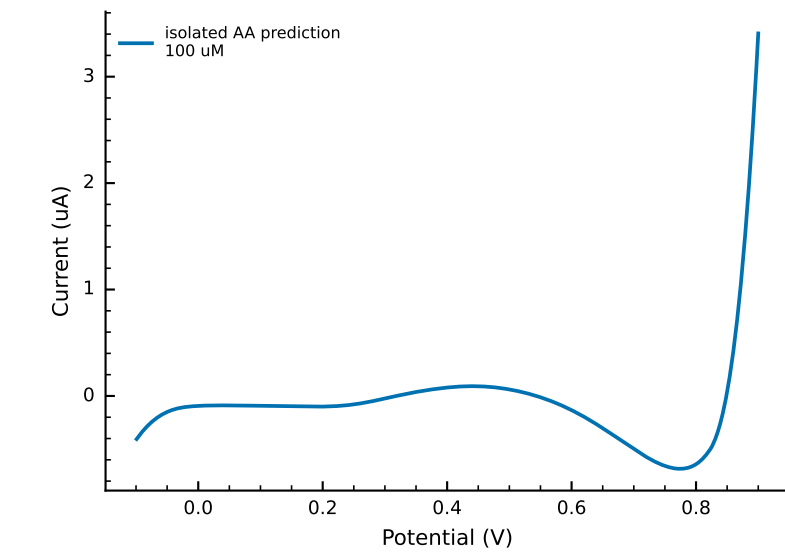





CV normal
Cathodic

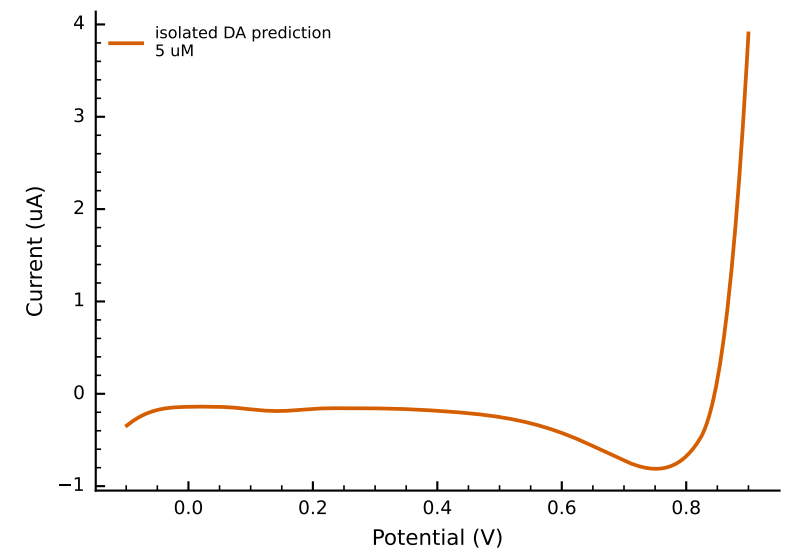





CV QC
Anodic

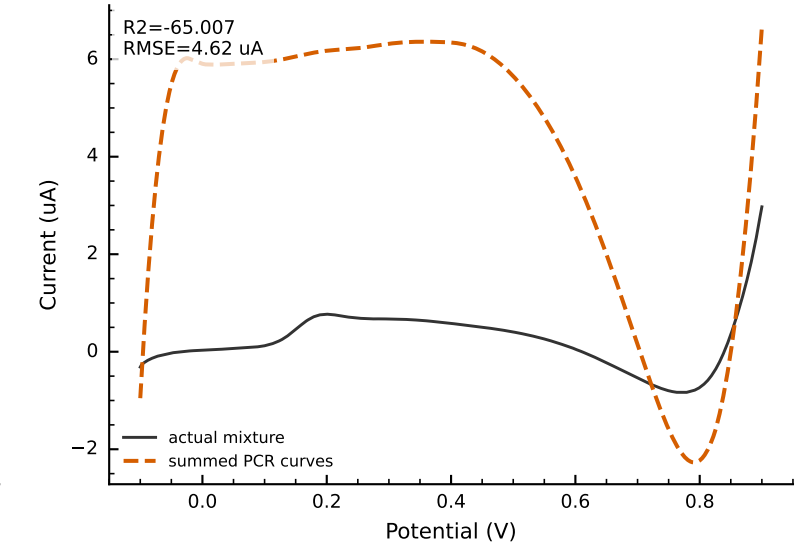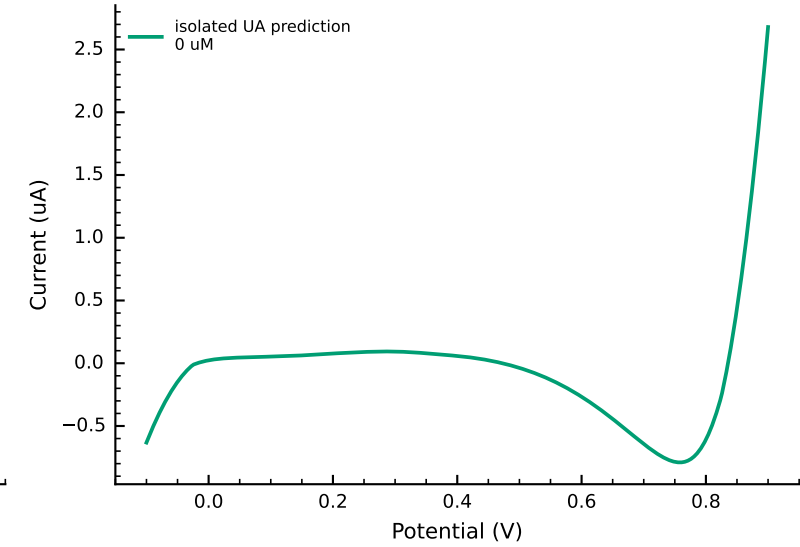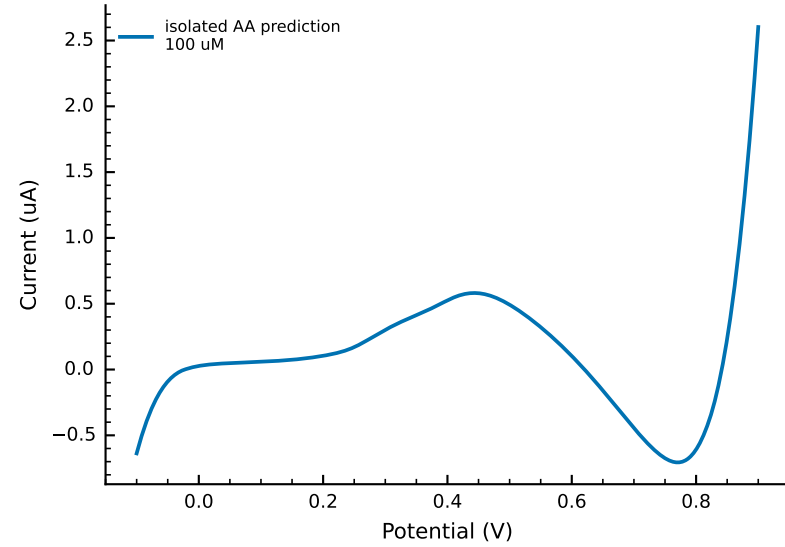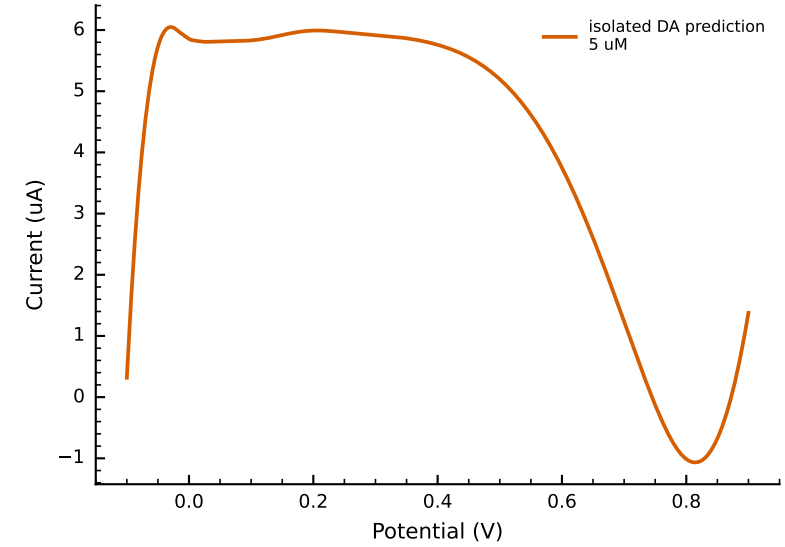





CV QC
Cathodic

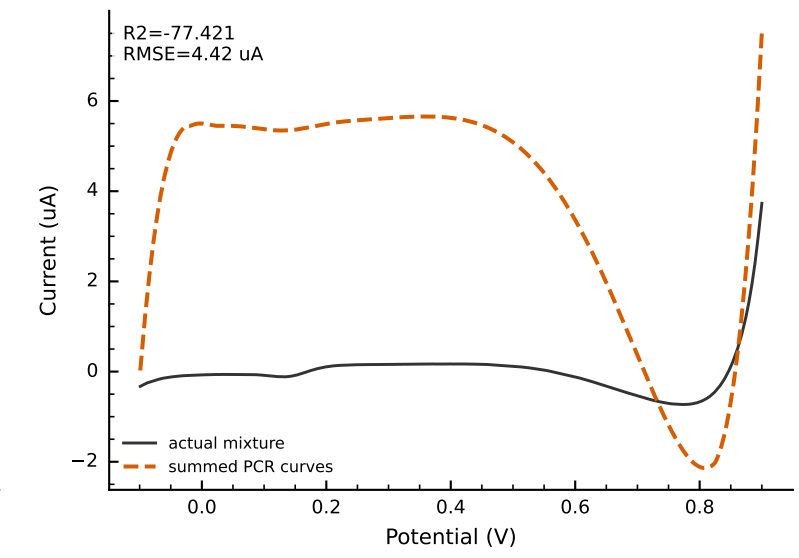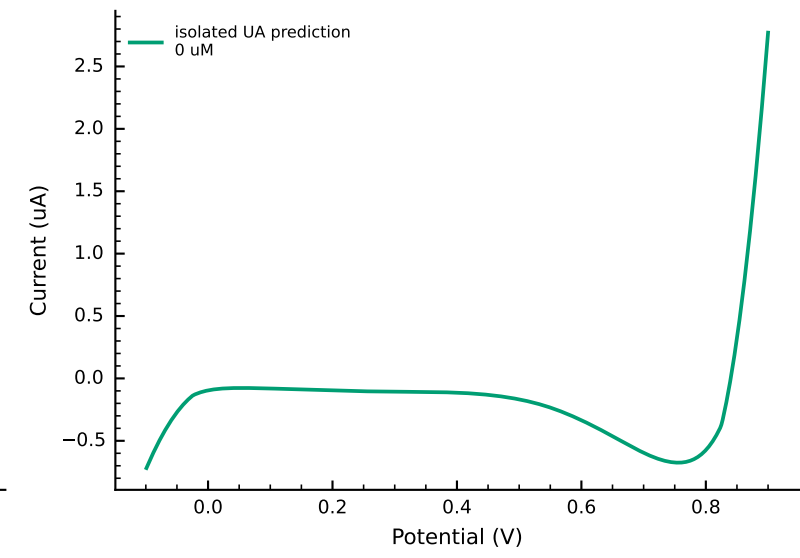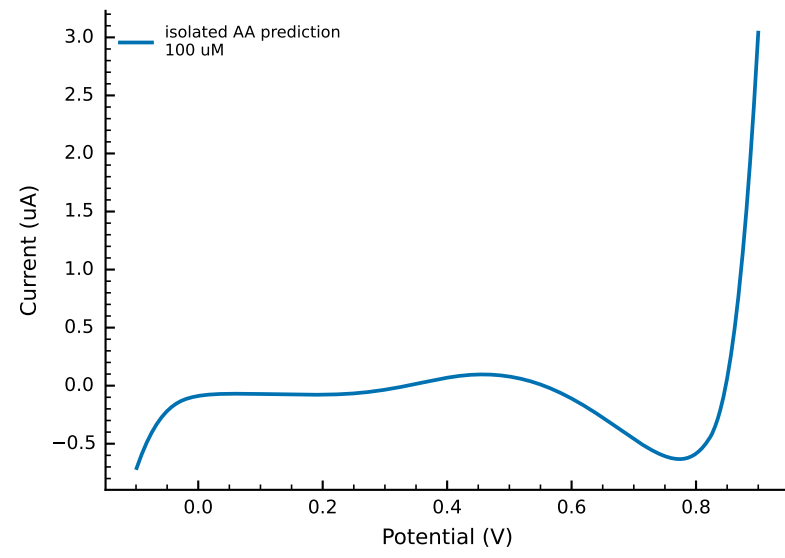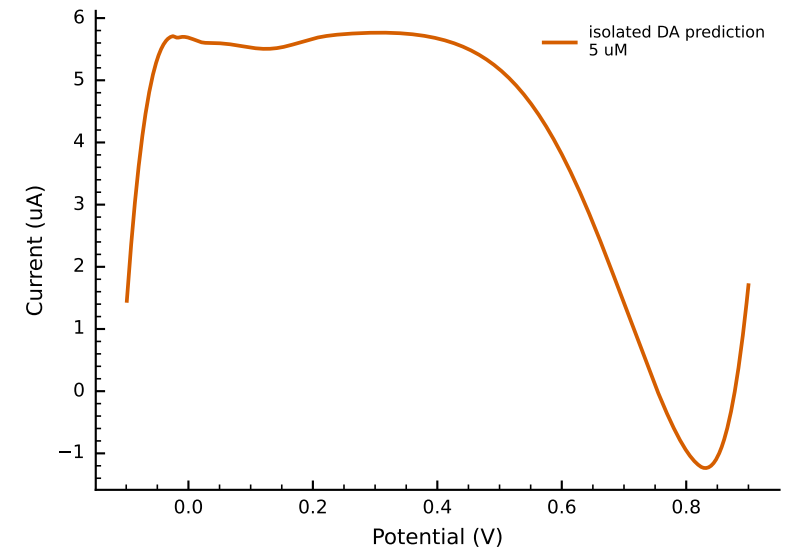





CV Normal
Anodic

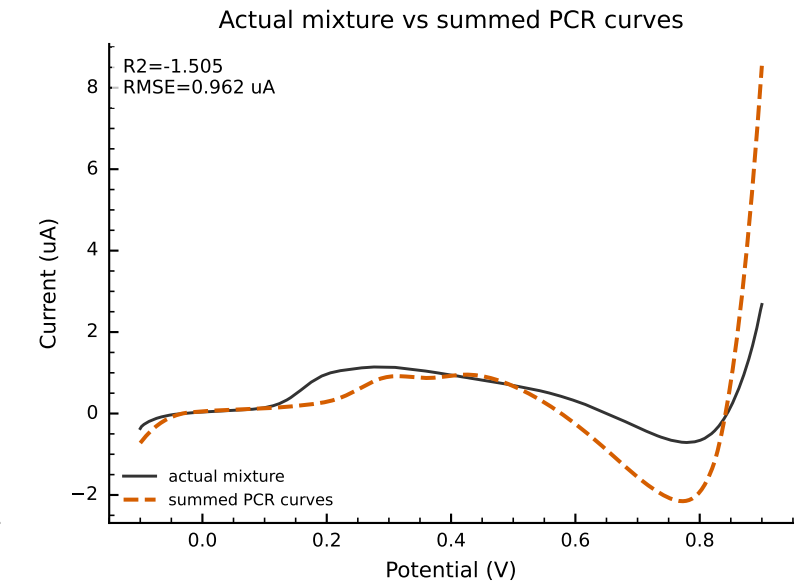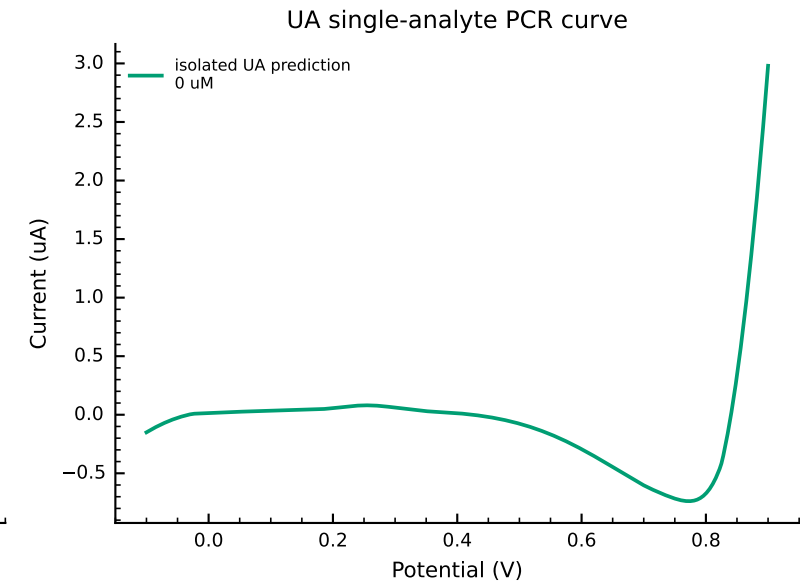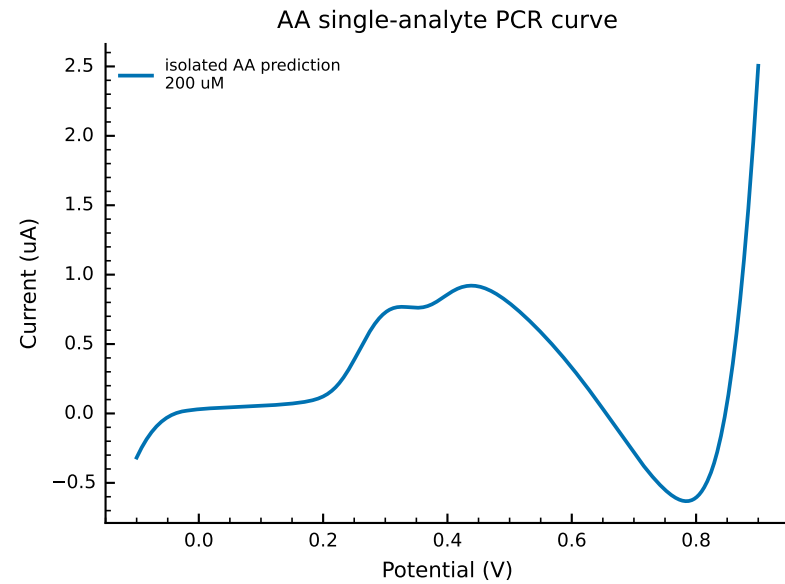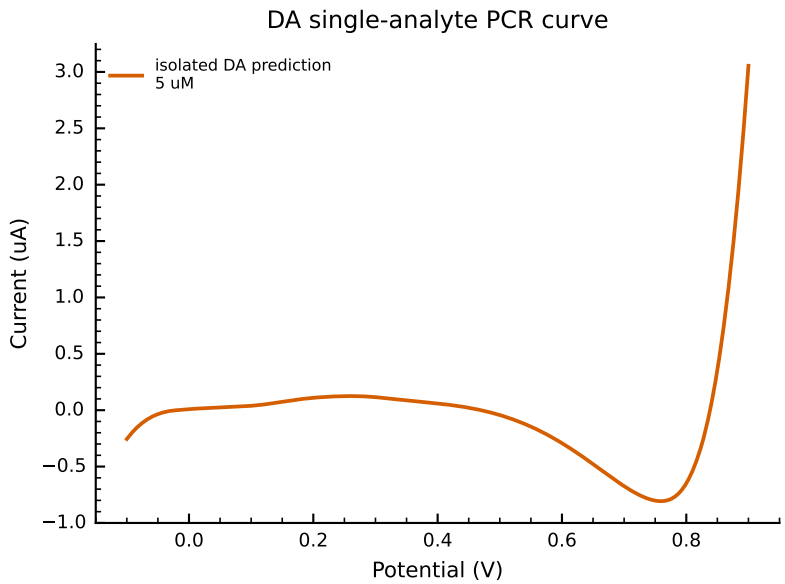





CV Normal
Cathodic

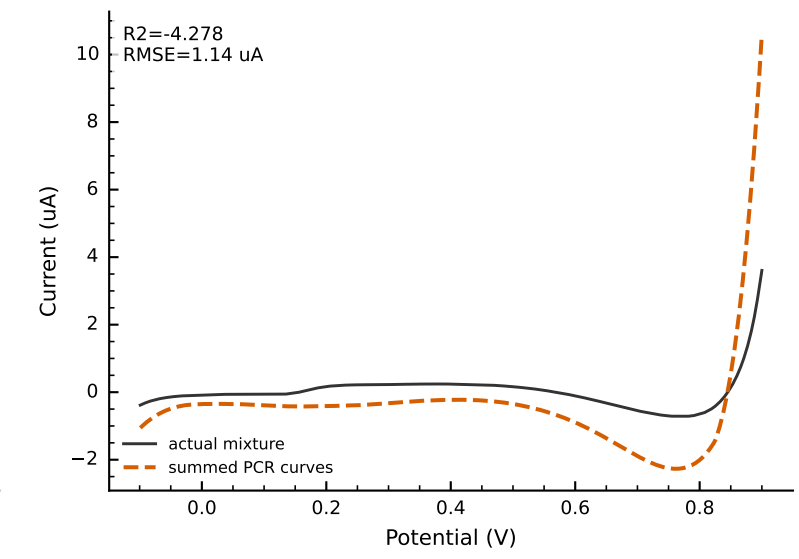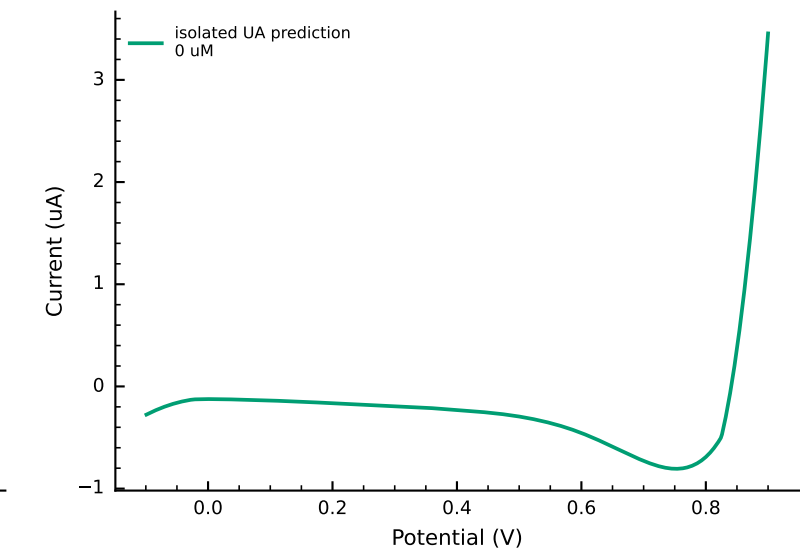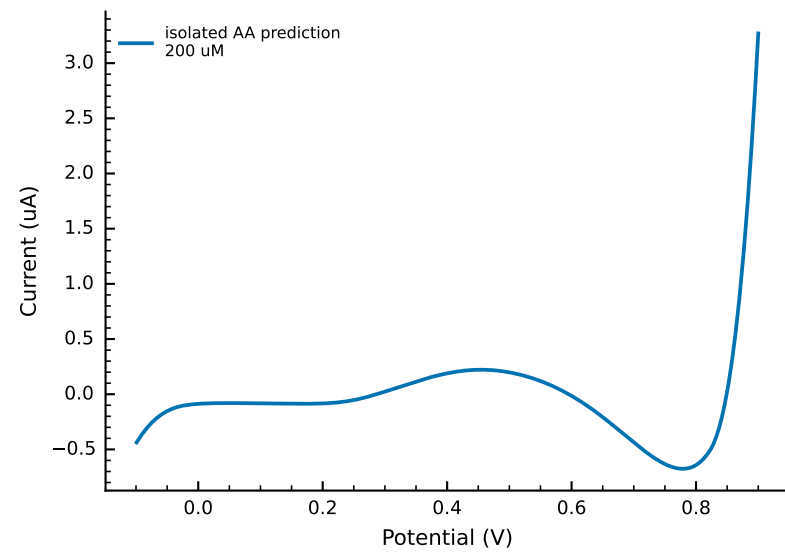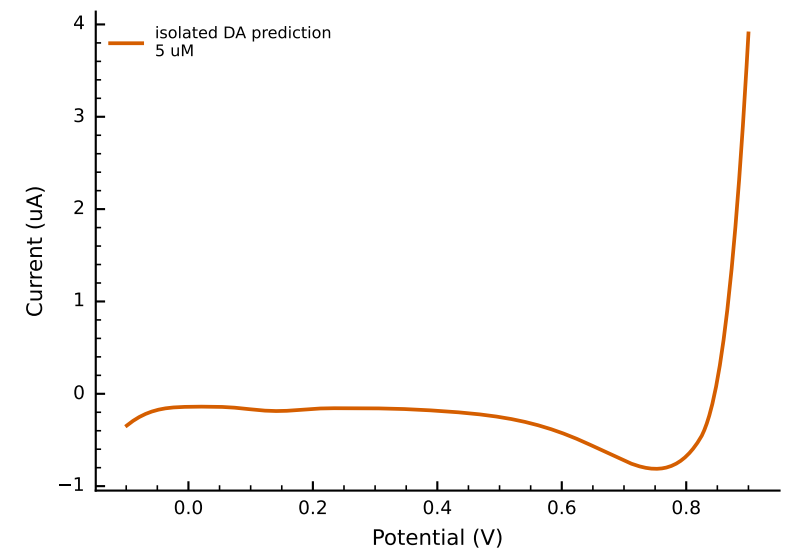





CV QC
Anodic

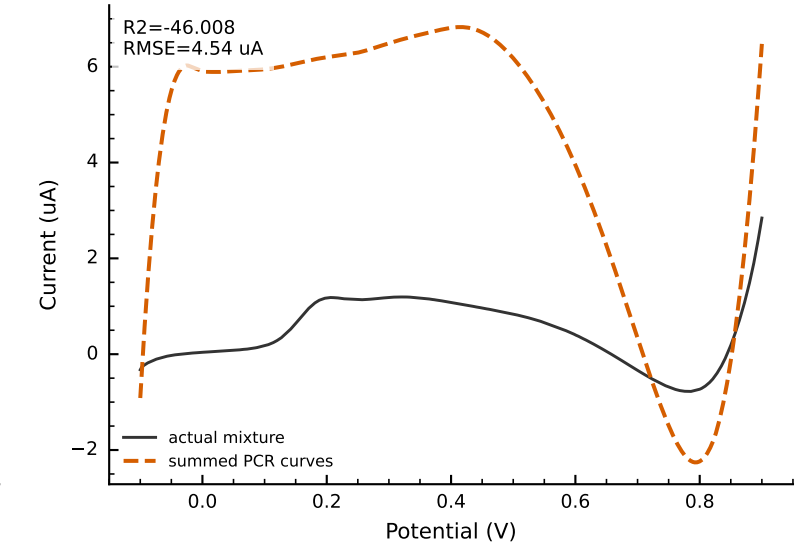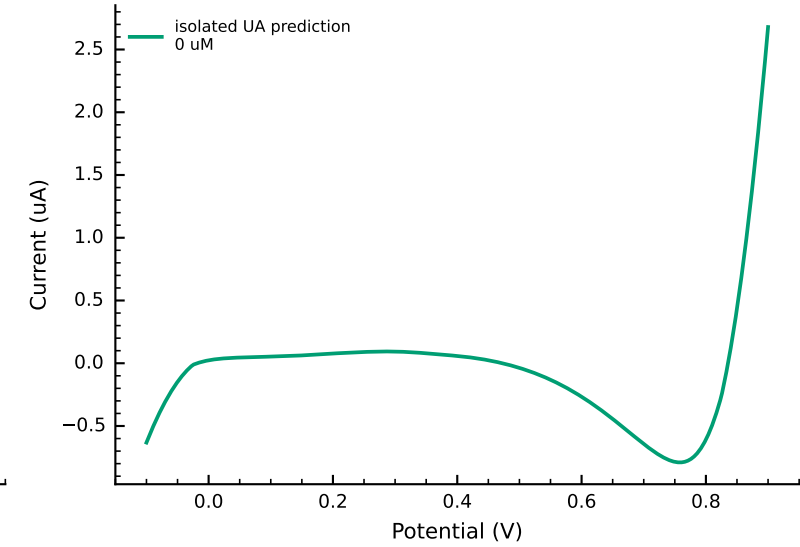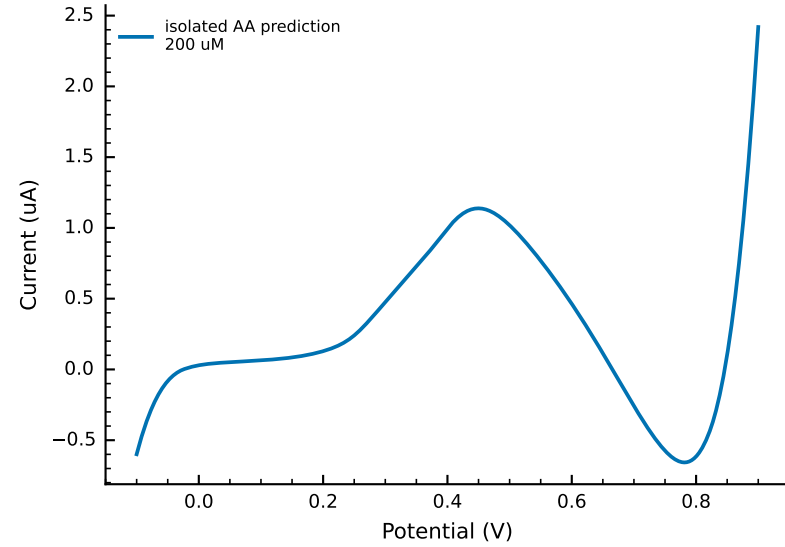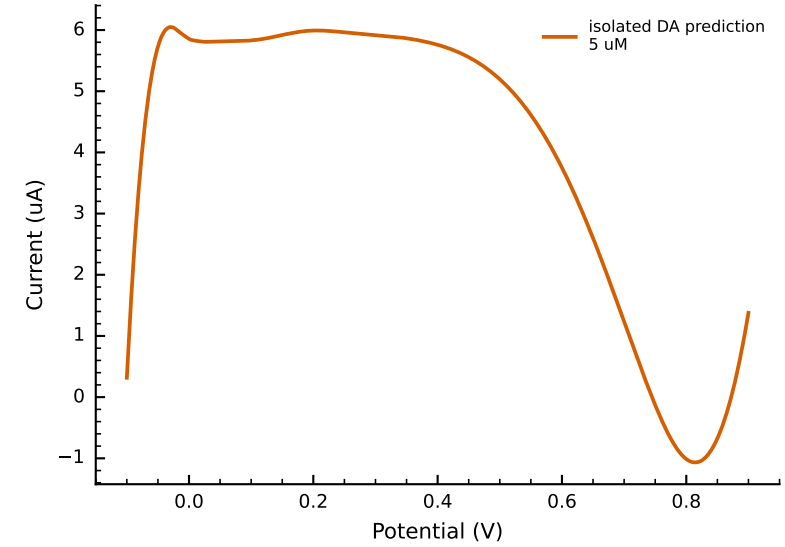





CV QC
Cathodic

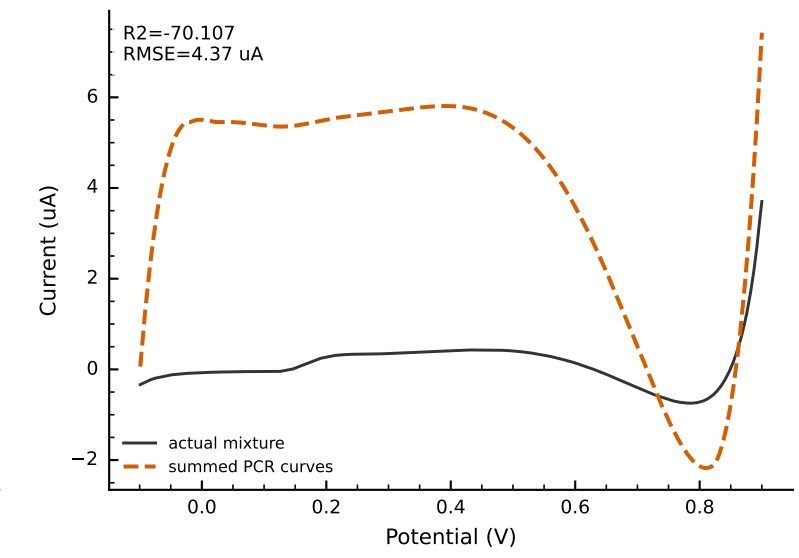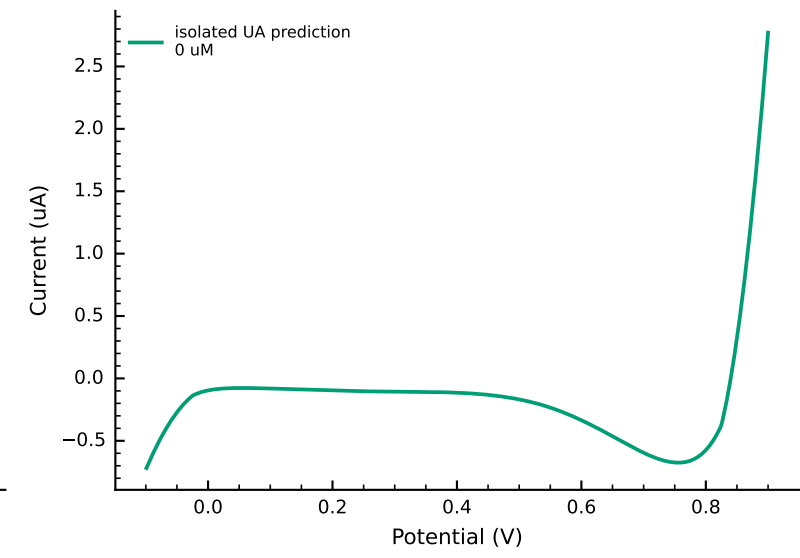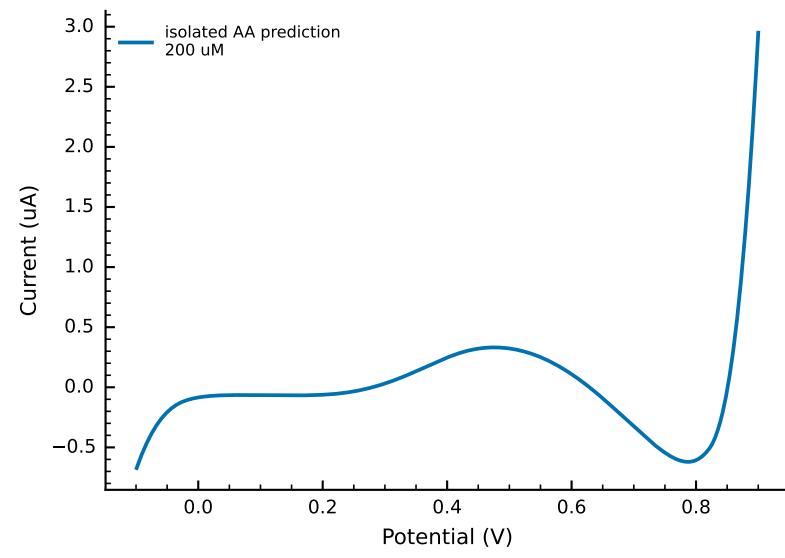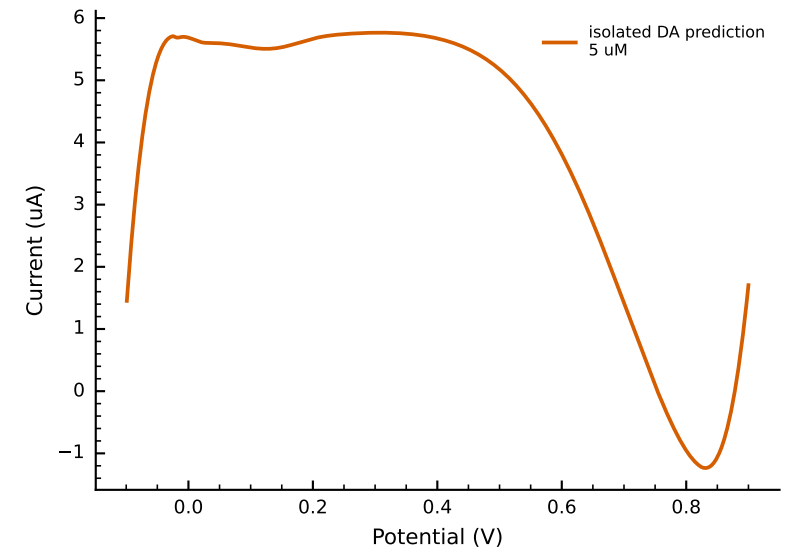





CV normal
Anodic

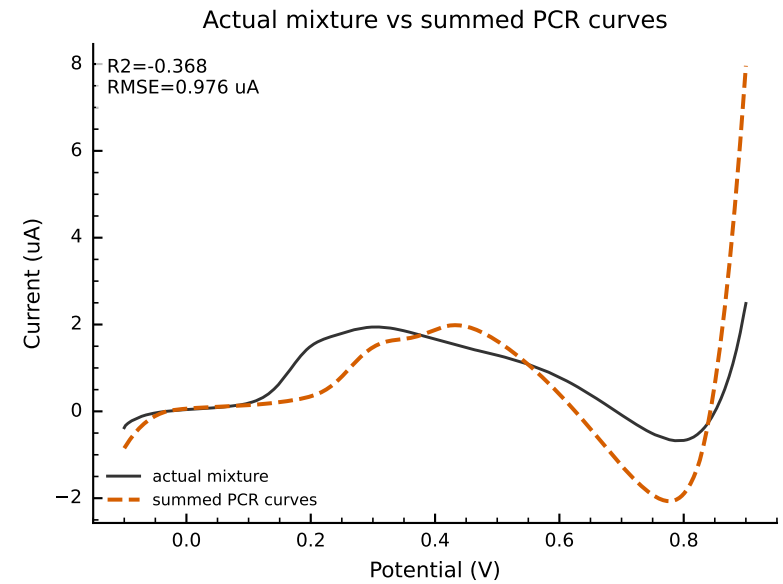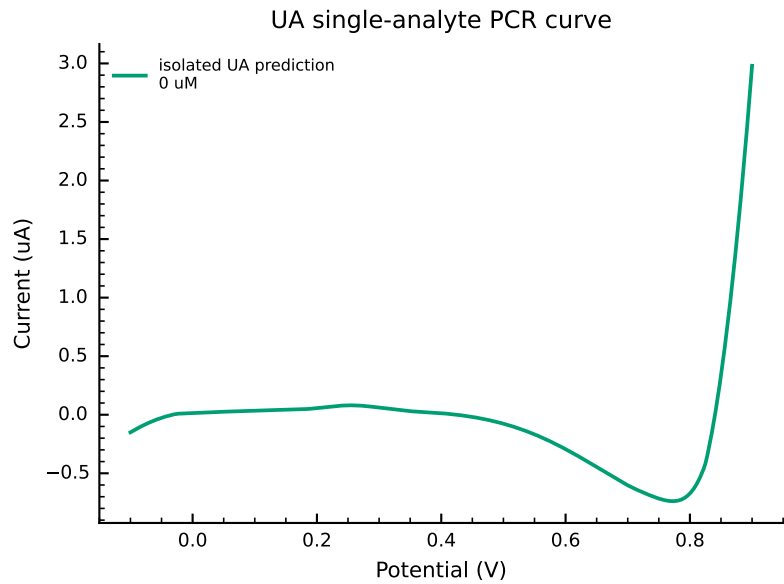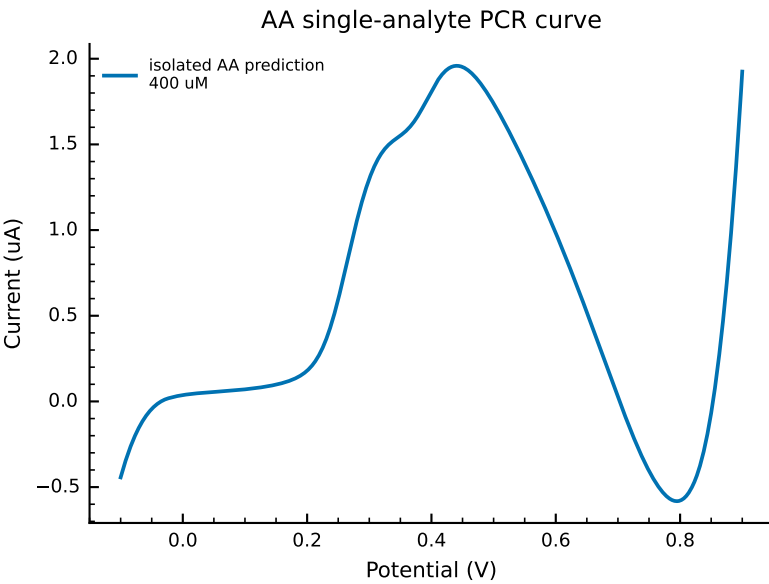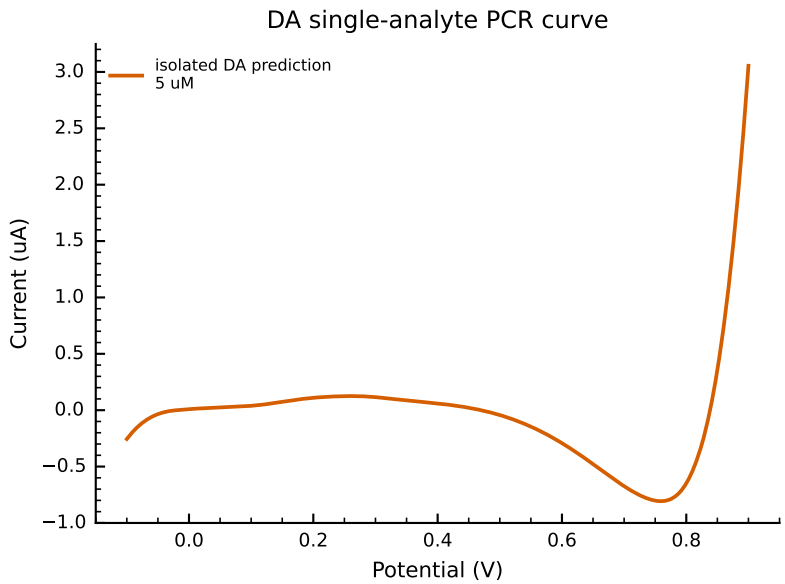

CV normal
Cathodic

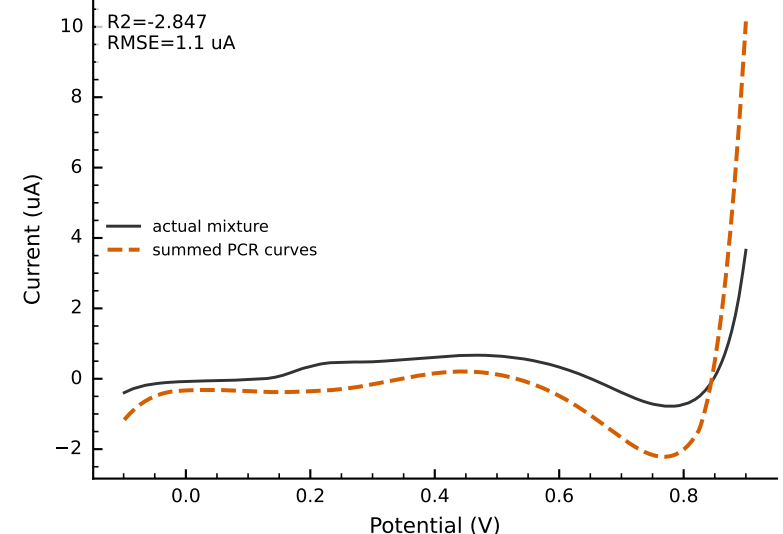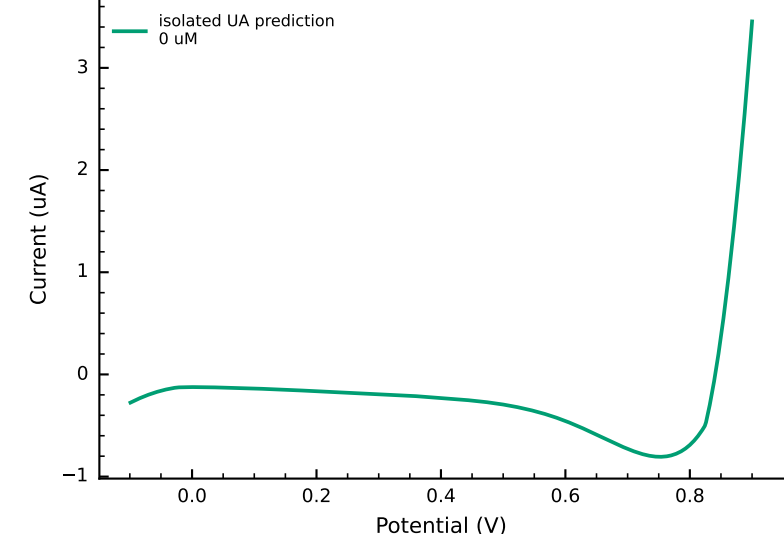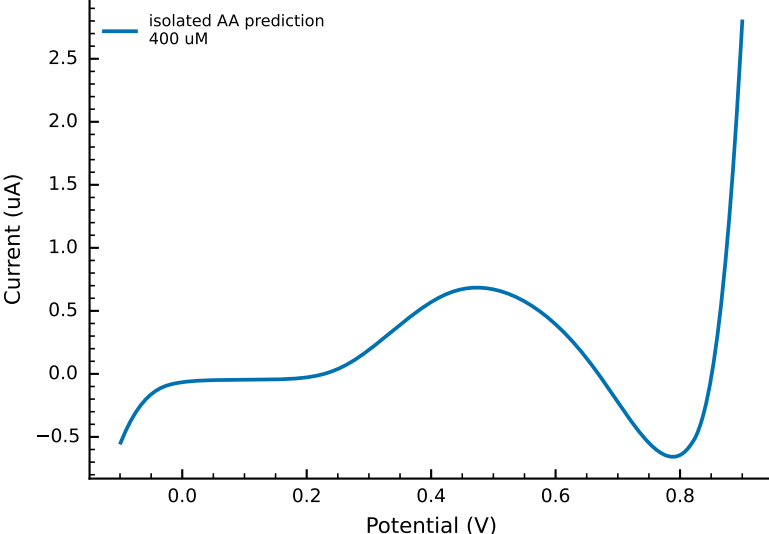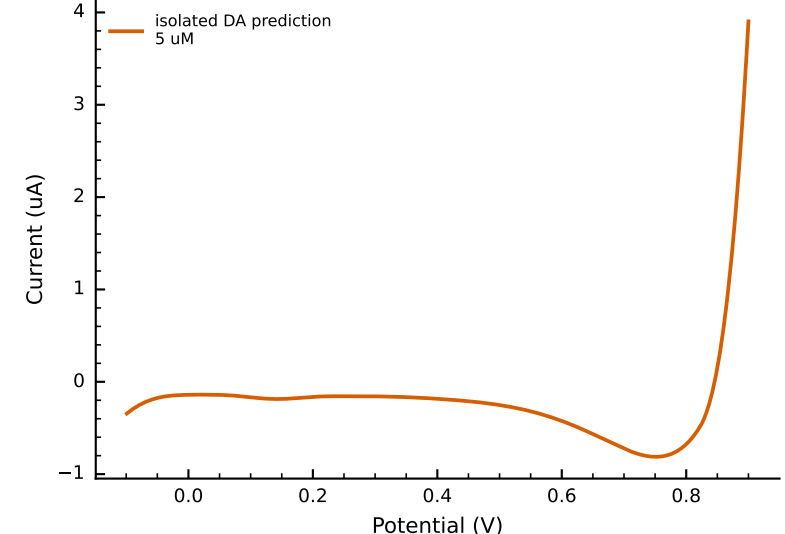

CV QC
Anodic

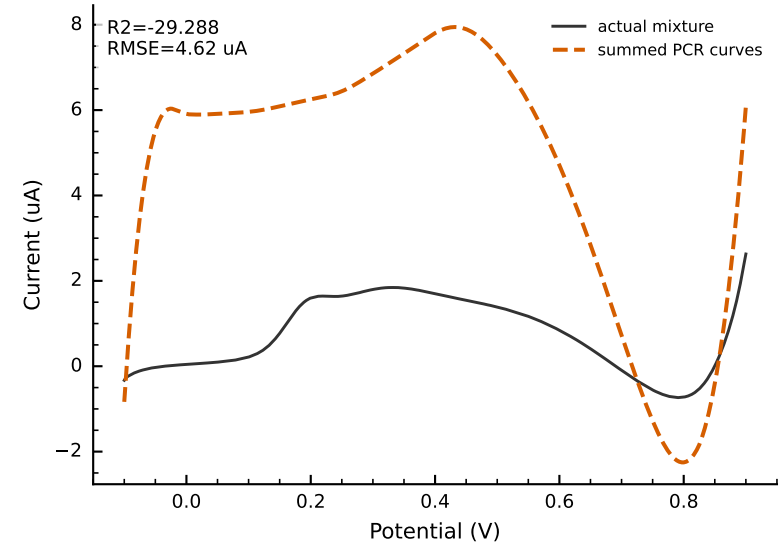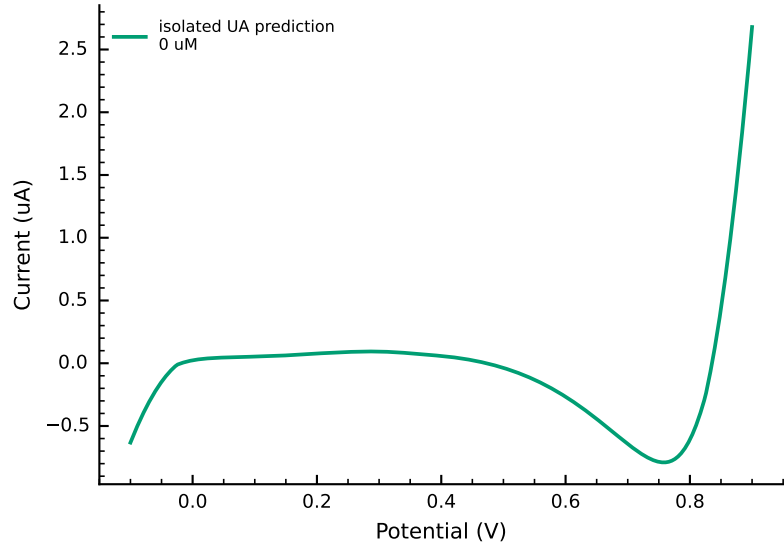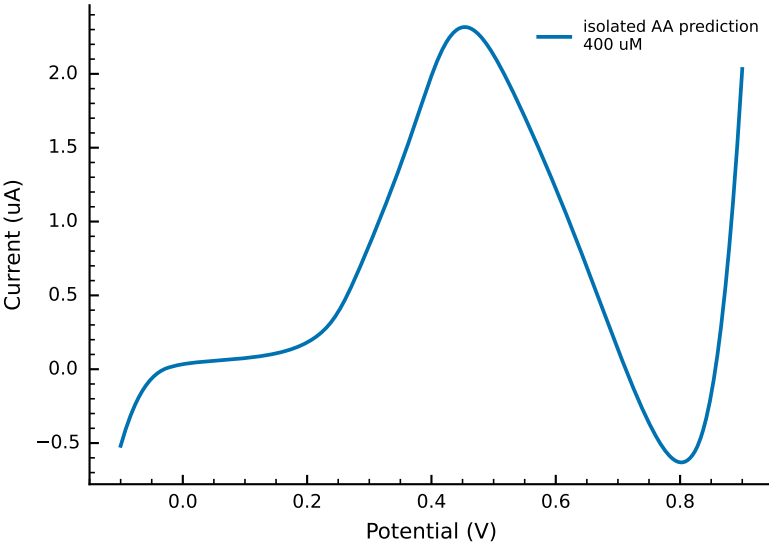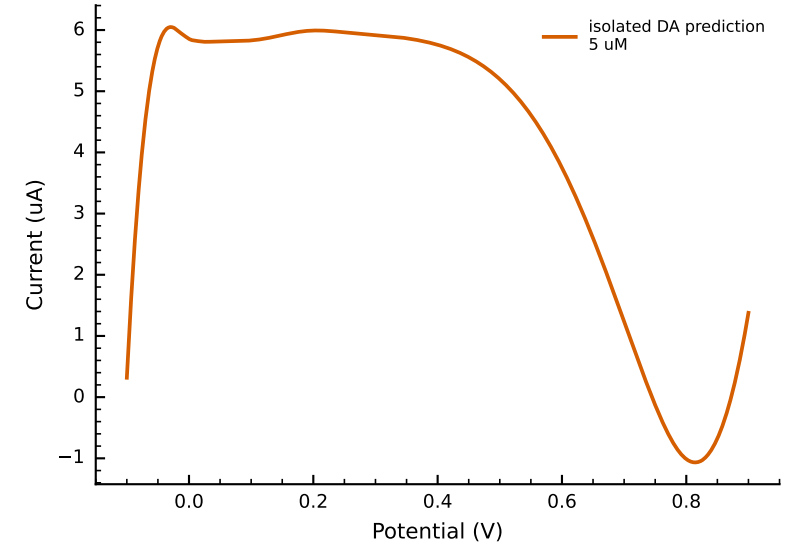

CV QC
Cathodic

