


Paired SCC increase relative to baseline

Each point subtracts the matched baseline draw from the wildfire-feedback draw; x-axis truncated at \$500/tCO₂.

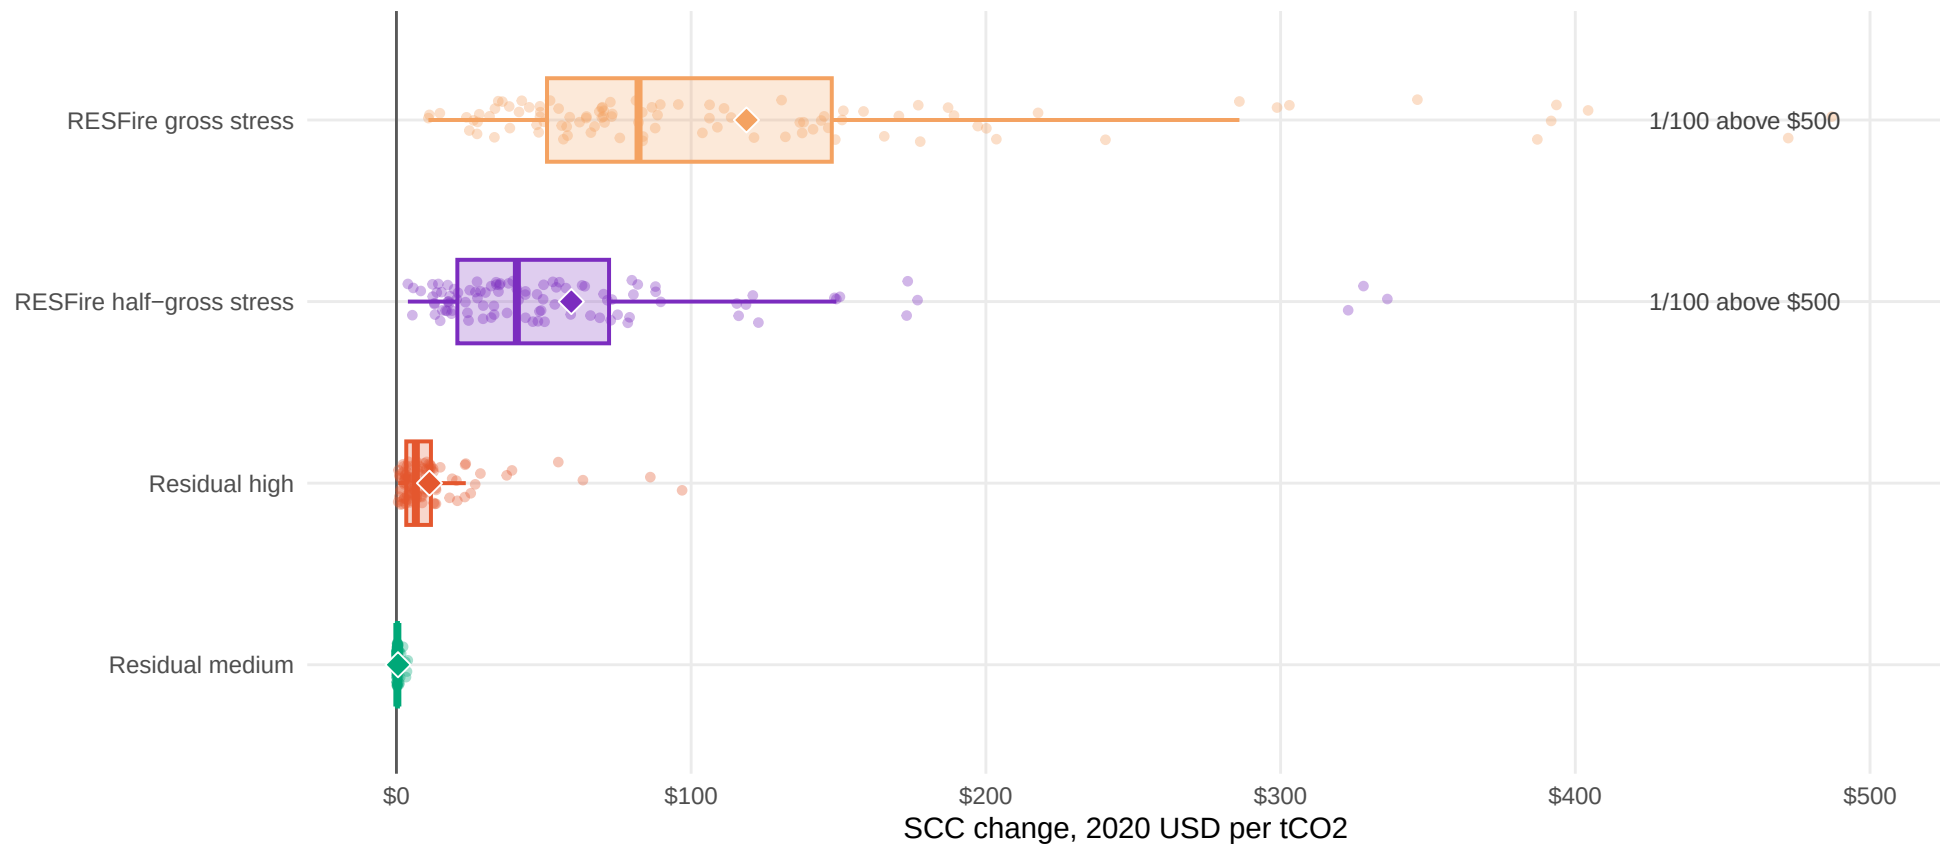

Paired draws hold RFF-SP, FAIR, and discounting samples fixed within trial.