

T0130

Seite 1 von 6
Page 1 de 6
Pagina 1 din 6
Seiten 1 pages
pages

KALIBRIER – ZERTIFIKAT CERTIFICAT D'ÉTALONNAGE CERTIFICATE OF CALIBRATION

Instrument
Instrument
Instrument

Digital Oscilloscope

Hersteller
Fabricant
Manufacturer

AGILENT

Typ
Type
Model

DSOX1204G

Serien- / Inventar-Nr.
No. de série- / inventaire
Serial- / Inv. No.

CN64277307

Kunde
Client
Customer

COMPUTER CONTROLS, 8112 Otelfingen

Auftragsnummer
No. de la commande
Order No.

n/a

Bemerkungen
Remarques
Remarks

n/a

Datum der Kalibrierung
Date de l'étalonnage
Date of calibration


28. April 2026

ELCAL AG bestätigt hiermit, dass genanntes Gerät im firmeneigenen Kalibrationslabor kalibriert wurde. Es erfüllte oder übertraf zu diesem Zeitpunkt alle im Manual aufgeführten Spezifikationen.


Die Kalibration wurde in Übereinstimmung mit unserem ISO 17025:2017 konformen Qualitätssicherungshandbuch mit Hilfe von Instrumenten ausgeführt, die um ein mehrfaches genauer sind als der Prüfling. Alle als Referenz verwendeten Normale werden periodisch von amtlichen Stellen überprüft.

Dietikon, 29. April 2026

Kalibriert durch:

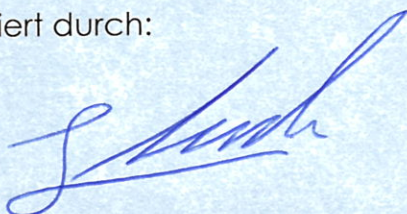

Technischer Leiter:

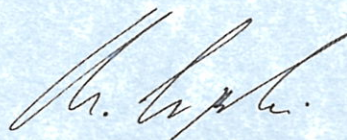

Testreport
422854

Unit under Test : AGILENT DSOX1204G Digital Oscilloscope
Serial No : CN64277307
Customer : COMPUTER CONTROLS, 8112 Otelfingen
Inventory No :
Date : 28.04.2026
Operator : L. Pascale

TRACEABILITY INFORMATION

Instruments used:	Serial No:	Inventory No:	Cal Due Date:
Fluke PM6681	SM798703	LAB-401	13.08.2026
Fluke 9500B	252367200	LAB-389	13.08.2026
Fluke 9530	261467745	LAB-392	13.08.2026
Fluke 9530	112460139	LAB-387	13.08.2026
Fluke 9530	197464419	LAB-372	13.08.2026
Fluke 9530	197464418	LAB-371	13.08.2026
Agilent 3458A/01/02/H01	MY45052511	LAB-431	26.07.2026
Fluke Hart 2626-S	A79867	LAB-432A	17.07.2026

All listed result are direct traceable to the Swiss Federal Office of Metrology, as far as listed in the uncertainty table of the SCS Certificate.

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k=2$, which for a normal distribution corresponds to a coverage probability of approx 95%.

SUMMARY OF LAST RECORDED CAL DATA

This certificate records the calibration status.
Points where %Tol exceeds the adjustment threshold are marked with a "M".
Points where %Tol exceeds the specification limit are marked with a "F".

Number of Test Marginal: 0
Number of Test Failed: 0

Testreport
422854

Unit under Test : AGILENT DSOX1204G Digital Oscilloscope
Serial No : CN64277307
Customer : COMPUTER CONTROLS, 8112 Otelfingen
Inventory No :
Date : 28.04.2026
Operator : L. Pascale

TEST	RANGE	UUT INDICATED	SYSTEM ACTUAL	MODIFIER	ERROR	ERROR (%TOL)	M F
------	-------	---------------	---------------	----------	-------	--------------	-----

Actual Ambient Temp. 22.7 ±0.5°C / Humidity 35.1%

Marginal limit 95% of UUT Tol.

Keysight DSOX 1204G: Oscilloscope C/L Ver.

All Tests refer to UUT 360 Days Specifications as per
Keysight InfiniiVision 1200 X-Series Service Guide
Manual Part Number N2137-97014, Edition February 2020

Programmed UUT Identification:

Manufacturer: KEYSIGHT TECHNOLOGIES
Model: DSOX1204G
Serial No.: CN64277307
Firmware Rev.: 02.12.2021071625
Bandwidth: 70MHz

DC Vertical Gain Accuracy Test:

Channel 1:

1	10	69.915V	70.0000V	-0.121 %	4
2	5	34.849V	35.0000V	-0.430 %	13
3	2	14.016V	14.0000V	0.113 %	3
4	1	7.0090V	7.00000V	0.128 %	4
5	0.5	3.4880V	3.50000V	-0.343 %	10
6	0.2	1.3937V	1.40000V	-0.450 %	13
7	100	699.35mV	700.000mV	-0.093 %	3
8	50	350.78mV	350.000mV	0.223 %	7
9	20	139.619mV	140.0000mV	-0.272 %	8
10	10	69.783mV	70.0000mV	-0.310 %	9
11	5	34.941mV	35.0000mV	-0.167 %	4
12	2	13.9902mV	14.00000mV	-0.070 %	2
13	1	6.9584mV	7.00000mV	-0.594 %	13
14	0.5	3.4993mV	3.50000mV	-0.019 %	0

Channel 2:

15	10	70.021V	70.0000V	0.030 %	1
16	5	34.968V	35.0000V	-0.093 %	3
17	2	14.036V	14.0000V	0.260 %	8
18	1	7.0410V	7.00000V	0.586 %	17
19	0.5	3.5066V	3.50000V	0.190 %	6
20	0.2	1.3977V	1.40000V	-0.163 %	5
21	100	700.86mV	700.000mV	0.123 %	4
22	50	351.55mV	350.000mV	0.443 %	13
23	20	140.311mV	140.0000mV	0.222 %	6
24	10	70.196mV	70.0000mV	0.280 %	8
25	5	35.122mV	35.0000mV	0.348 %	8
26	2	14.0734mV	14.00000mV	0.525 %	12
27	1	6.9817mV	7.00000mV	-0.262 %	6
28	0.5	3.5038mV	3.50000mV	0.107 %	1

Testreport
422854

Unit under Test : AGILENT DSOX1204G Digital Oscilloscope
Serial No : CN64277307
Customer : COMPUTER CONTROLS, 8112 Otelfingen
Inventory No :
Date : 28.04.2026
Operator : L. Pascale

TEST	RANGE	UUT INDICATED	SYSTEM ACTUAL	MODIFIER	ERROR	ERROR (%TOL)	M F
Channel 3:							
29	10	69.886V	70.0000V		-0.162 %	5	
30	5	34.825V	35.0000V		-0.501 %	15	
31	2	14.016V	14.0000V		0.115 %	3	
32	1	7.0130V	7.00000V		0.186 %	5	
33	0.5	3.4974V	3.50000V		-0.073 %	2	
34	0.2	1.3948V	1.40000V		-0.369 %	11	
35	100	698.20mV	700.000mV		-0.257 %	7	
36	50	350.45mV	350.000mV		0.128 %	4	
37	20	139.651mV	140.0000mV		-0.249 %	7	
38	10	70.009mV	70.0000mV		0.012 %	0	
39	5	34.985mV	35.0000mV		-0.044 %	1	
40	2	14.0112mV	14.00000mV		0.080 %	2	
41	1	6.9844mV	7.00000mV		-0.223 %	5	
42	0.5	3.4997mV	3.50000mV		-91.4 ppm	0	
Channel 4:							
43	10	70.055V	70.0000V		0.079 %	2	
44	5	34.908V	35.0000V		-0.263 %	8	
45	2	14.038V	14.0000V		0.275 %	8	
46	1	7.0236V	7.00000V		0.337 %	10	
47	0.5	3.5113V	3.50000V		0.324 %	9	
48	0.2	1.3975V	1.40000V		-0.180 %	5	
49	100	700.17mV	700.000mV		0.024 %	1	
50	50	351.81mV	350.000mV		0.517 %	15	
51	20	140.074mV	140.0000mV		0.053 %	2	
52	10	70.156mV	70.0000mV		0.223 %	6	
53	5	35.125mV	35.0000mV		0.358 %	8	
54	2	14.0597mV	14.00000mV		0.426 %	9	
55	1	7.0127mV	7.00000mV		0.182 %	4	
56	0.5	3.5135mV	3.50000mV		0.386 %	4	

Bandwidth Test:

Relative to 1MHz, 200mV/Div Range @ 1.2Vpp Signal

Channel 1:

Measurement Uncertainty: ± 0.6 dB

57 Amplitude Deviation @70MHz: -1.91dB > -3dB

Pass

Channel 2:

Measurement Uncertainty: ± 0.6 dB

58 Amplitude Deviation @70MHz: -1.87dB > -3dB

Pass

Channel 3:

Measurement Uncertainty: ± 0.6 dB

59 Amplitude Deviation @70MHz: -1.91dB > -3dB

Pass

Channel 4:

Measurement Uncertainty: ± 0.6 dB

60 Amplitude Deviation @70MHz: -1.92dB > -3dB

Pass

Testreport
422854

Unit under Test : AGILENT DSOX1204G Digital Oscilloscope
Serial No : CN64277307
Customer : COMPUTER CONTROLS, 8112 Otelfingen
Inventory No :
Date : 28.04.2026
Operator : L. Pascale

TEST	UUT RANGE INDICATED	SYSTEM ACTUAL	MODIFIER	ERROR	ERROR (%TOL)	M F
Time Base Accuracy Test:						

Last Time Scale Calibration: 2026-4-28						
61	1.000ms	1.0000ms		-10.6 ppm	21	
Internal Trigger Sensitivity Test:						

10mV/Div Range						
Channel 1:						
62	@10MHz 6mVpp				Pass	
63	@70MHz 9mVpp				Pass	
Channel 2:						
64	@10MHz 6mVpp				Pass	
65	@70MHz 9mVpp				Pass	
Channel 3:						
66	@10MHz 6mVpp				Pass	
67	@70MHz 9mVpp				Pass	
Channel 4:						
68	@10MHz 6mVpp				Pass	
69	@70MHz 9mVpp				Pass	

Testreport
422854

Unit under Test : AGILENT DSOX1204G Digital Oscilloscope
Serial No : CN64277307
Customer : COMPUTER CONTROLS, 8112 Otelfingen
Inventory No :
Date : 28.04.2026
Operator : L. Pascale

TEST	UUT RANGE INDICATED	SYSTEM ACTUAL	MODIFIER	ERROR ERROR	ERROR (%TOL)	M F
All Tests refer to UUT typical Specifications as per Datasheet 5991-1103EN, Aug 14						
Wavegen Option Verification: -----						
All Test Performed with following Settings, unless otherwise specified: Function: Sine Impedance: 50Ohm						
Channel 1: -----						
70	Frequency Accuracy 10.000MHz	10.0000MHz		-2.99 ppm		6
71	Amplitude Accuracy: 1.000V	0.9930V		-0.705 %		47
Amplitude Flatness: Relative to 1kHz						
72	0.000dB	0.00dB	@10kHz	0.0000dB		0
73	0.000dB	0.03dB	@100kHz	0.0344dB		7
74	0.000dB	0.09dB	@1MHz	0.0856dB		17
75	0.000dB	0.10dB	@10MHz	0.1030dB		21
76	0.000dB	0.45dB	@20MHz	0.4547dB		91
Square Wave & Pulse Test:						
77	Rise Time < 19ns: 16.7ns					Pass
78	Fall Time < 19ns: 18ns					Pass
79	Overshoot < 2%: 1%					Pass

End of Keysight DSOX 1204G: Oscilloscope C/L Ver.